

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008962.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 13:12
 Operator : DD\AJ
 Sample : L1626-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-GF-02-051-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 24 14:22:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	499.6E6	203.1E6	228.476	210.734
Target Compounds							
2) T	3,5-DICHL...	0.000	6.115	0	139.6E6	N.D.	95.654
5) T	DICAMBA	7.373	0.000	137.5E6	0	16.927	N.D. #
7) T	MCPA	7.742	7.408	56949136	-3515038	7.080	N.D. #
11) T	2,4,5-TP ...	0.000	8.796	0	48773417	N.D.	9.004
12) T	2,4,5-T	9.455	0.000	107.9E6	0	10.090	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008962.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 13:12
Operator : DD\AJ
Sample : L1626-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 24 14:22:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

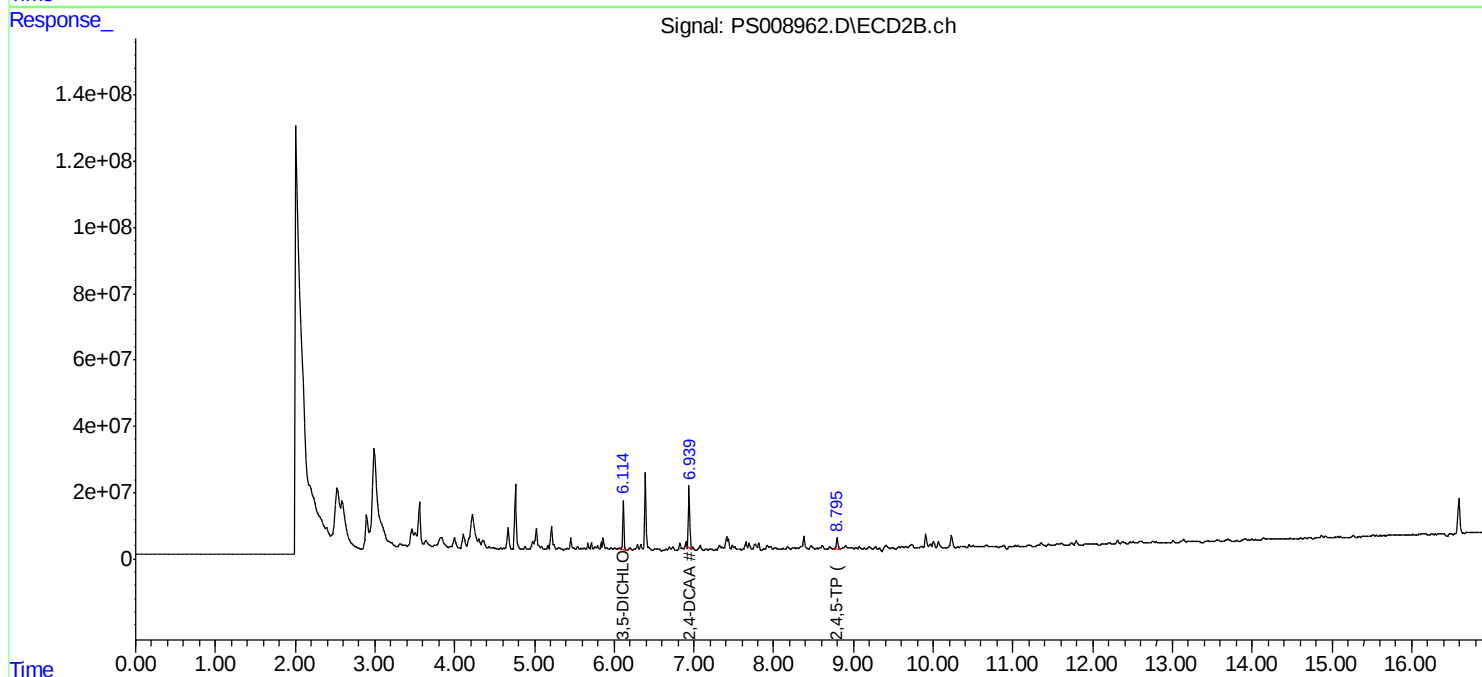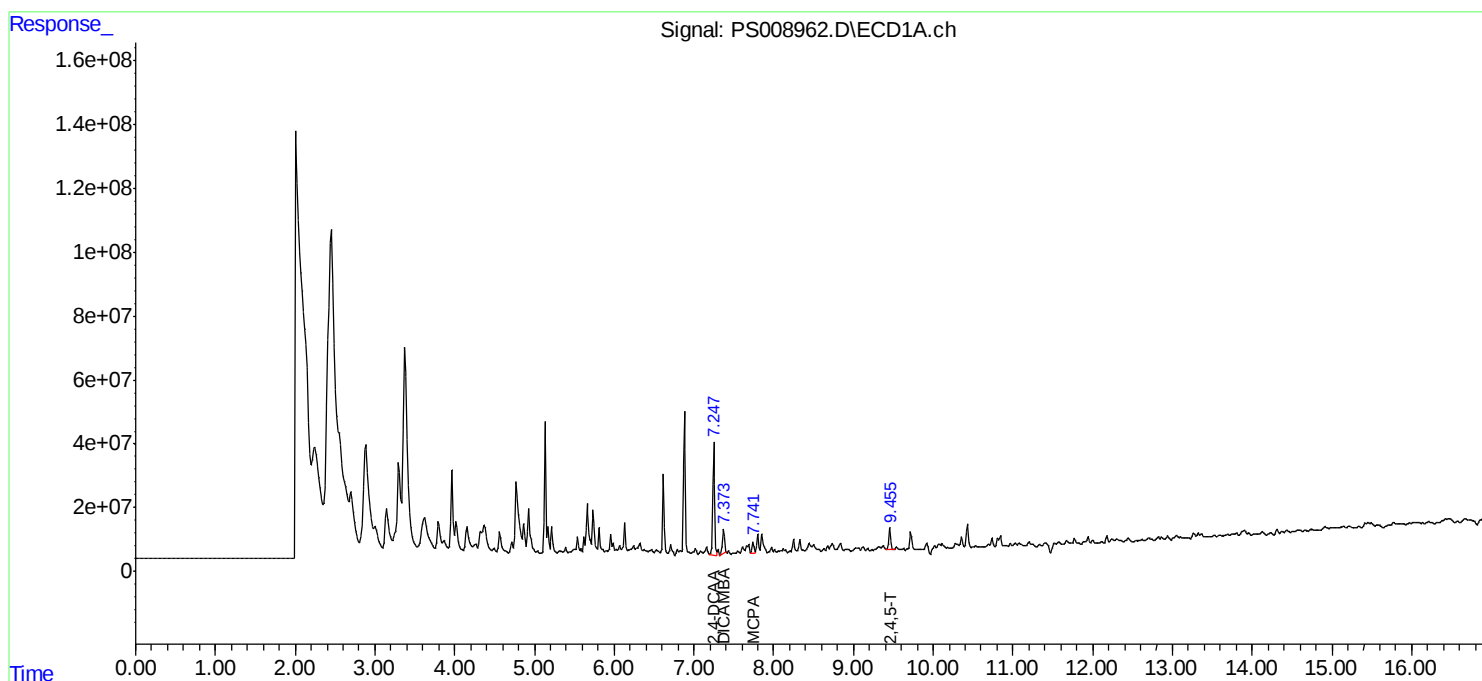


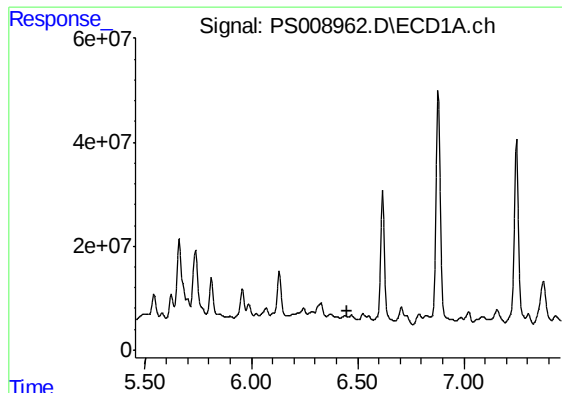

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-B

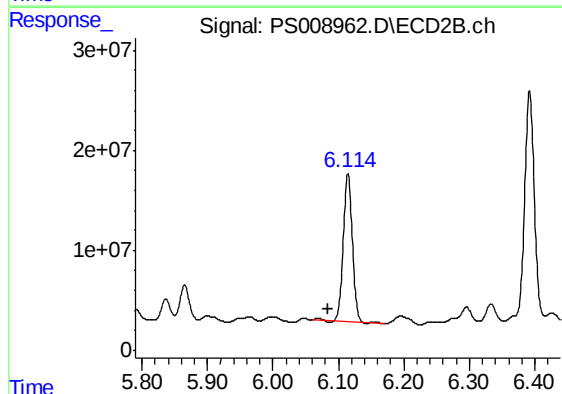


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 139585509
Conc: 95.65 ng/ml

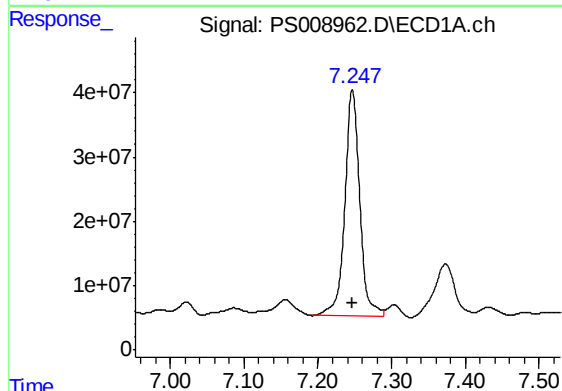


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 499584533
Conc: 228.48 ng/ml

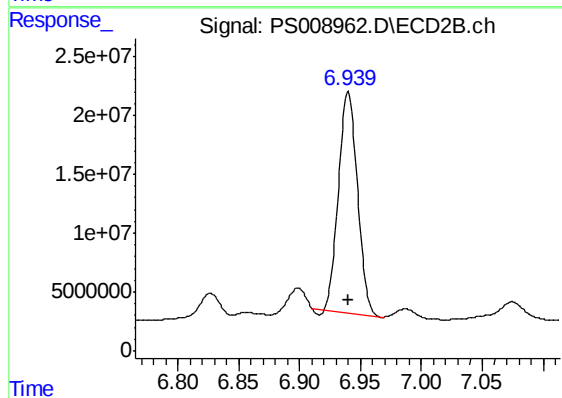

#4 2,4-DCAA


R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 203053508
Conc: 210.73 ng/ml

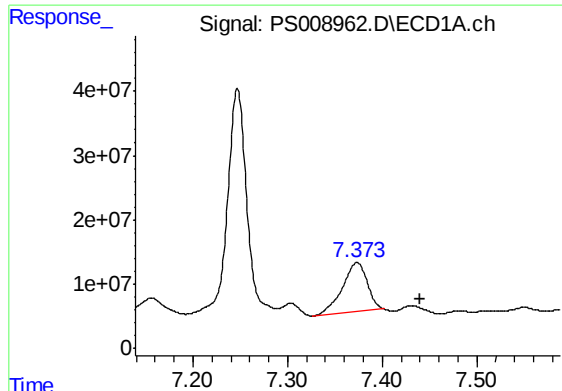

#5 DICAMBA


R.T.: 7.373 min
Delta R.T.: -0.067 min
Response: 137510348
Conc: 16.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-B

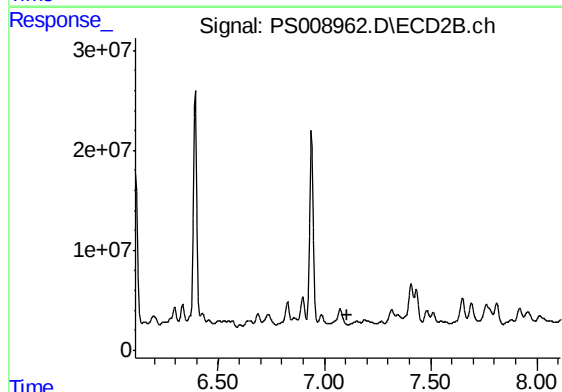


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.111 min
Response: 0
Conc: N.D.

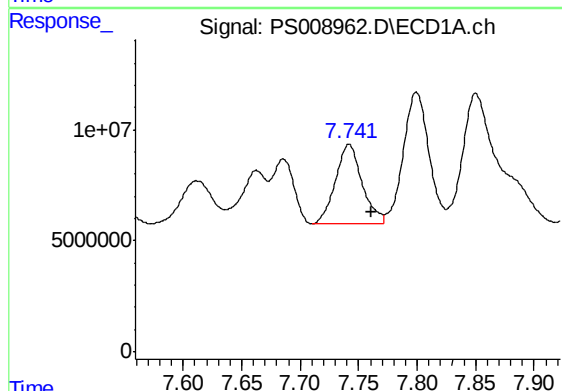


#7 MCPA

R.T.: 7.742 min
Delta R.T.: -0.019 min
Response: 56949136
Conc: 7.08 ug/ml

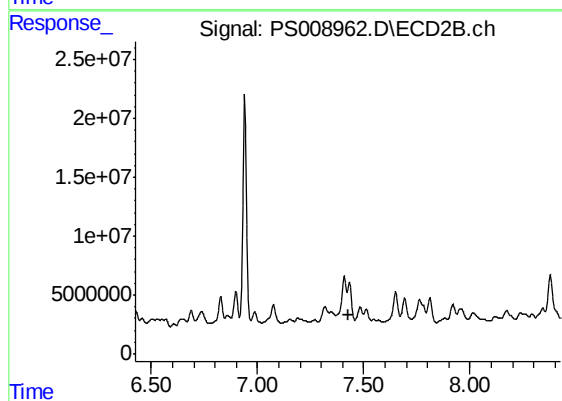

#7 MCPA


R.T.: 7.408 min
Delta R.T.: -0.017 min
Response: -3515038
Conc: N.D.

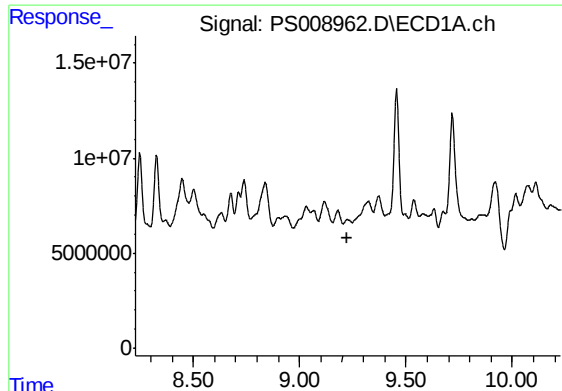

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-GF-02-051-B

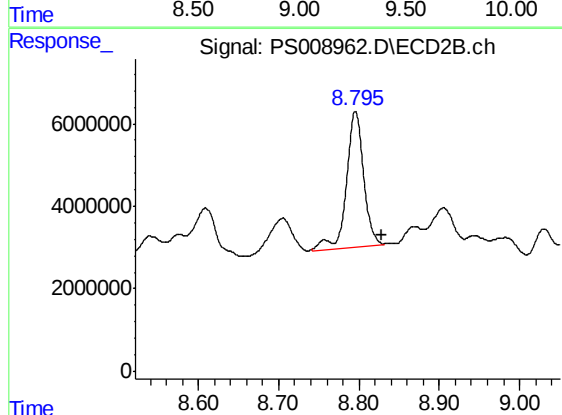


#11 2,4,5-TP (SILVEX)

R.T.: 8.796 min
Delta R.T.: -0.032 min
Response: 48773417
Conc: 9.00 ng/ml

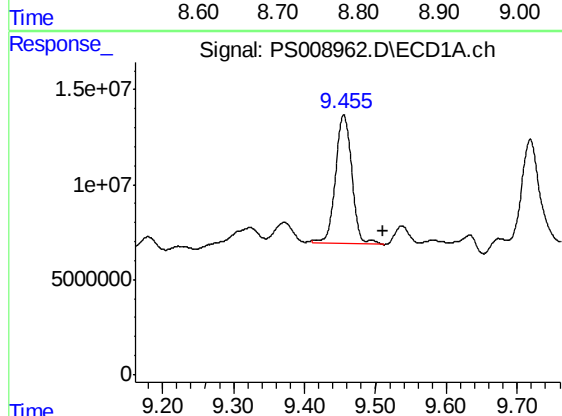

#12 2,4,5-T

R.T.: 9.455 min
Delta R.T.: -0.056 min
Response: 107878641
Conc: 10.09 ng/ml

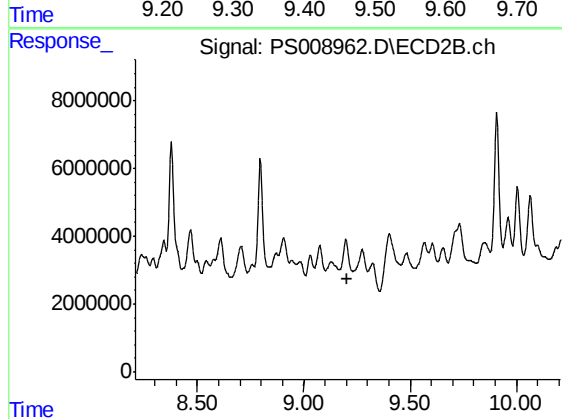

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.