

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008965.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 17:18
 Operator : DD\AJ
 Sample : PB127024BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB127024BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 03:57:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	1021.0E6	502.5E6	466.959	521.539
Target Compounds							
1) T	Dalapon	0.000	2.592	0	140.1E6	N.D.	95.808
2) T	3,5-DICHL...	0.000	6.114	0	58602103	N.D.	40.158
7) T	MCPA	7.800	7.408	69341690	40061459	8.620	9.055
12) T	2,4,5-T	0.000	9.259	0	92188110	N.D.	17.031
15) T	Picloram	11.044	11.031	572.7E6	322.0E6	41.832	44.310
16) T	DCPA	0.000	11.031	0	322.0E6	N.D.	46.533



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008965.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 17:18
Operator : DD\AJ
Sample : PB127024BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB127024BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 03:57:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

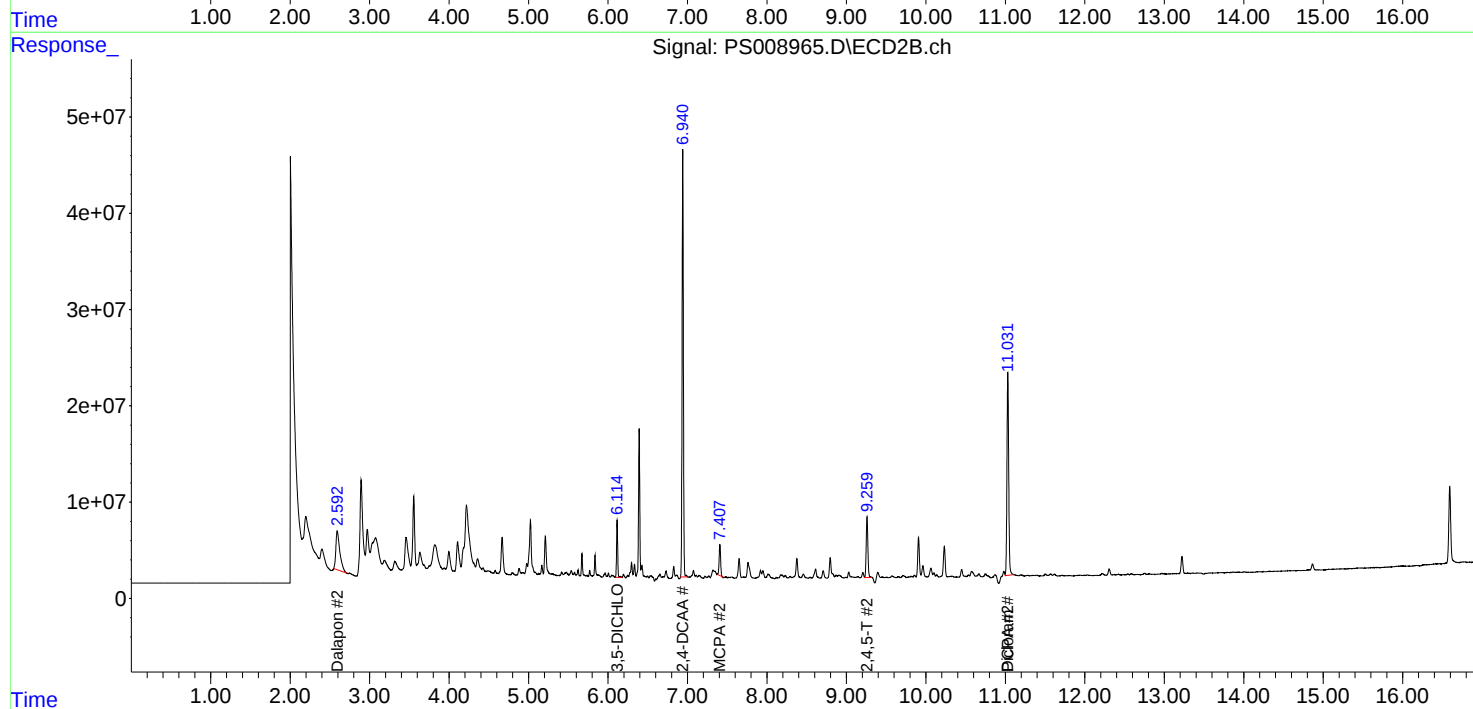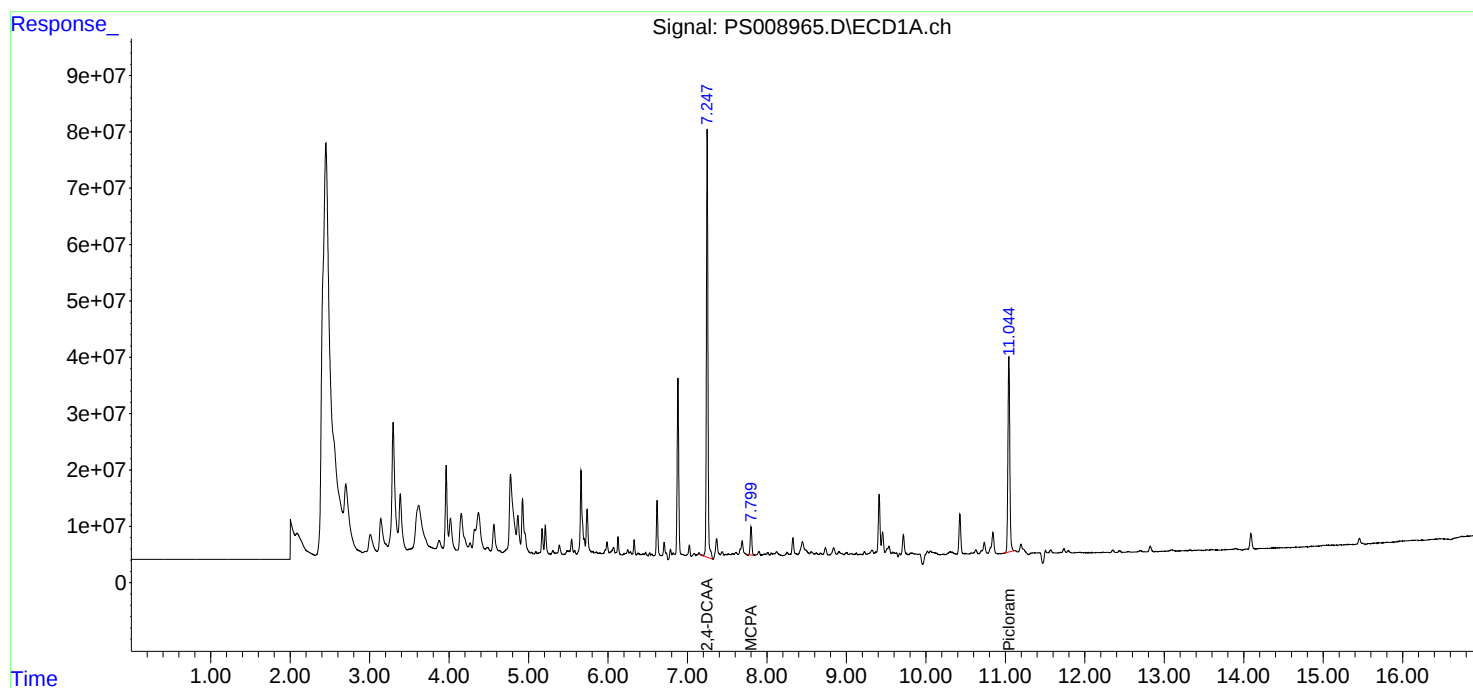


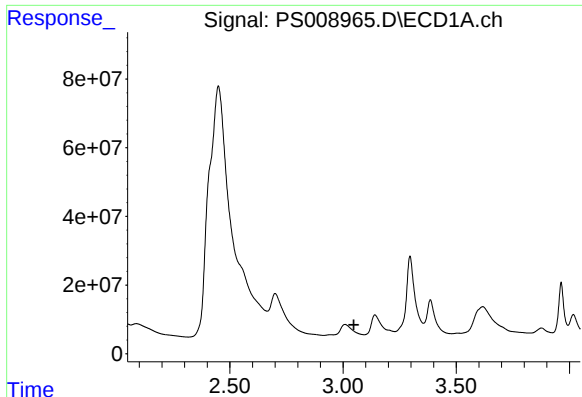

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127024BL

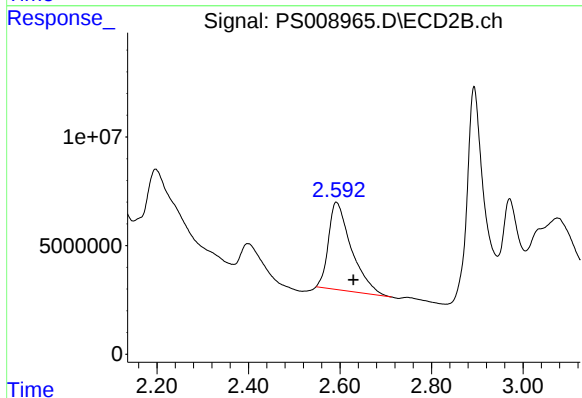


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 140092546
Conc: 95.81 ng/ml

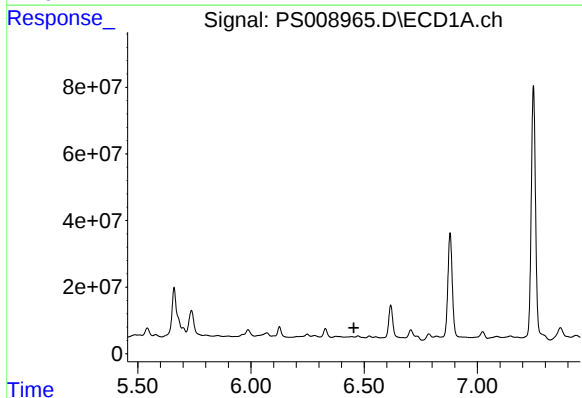


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

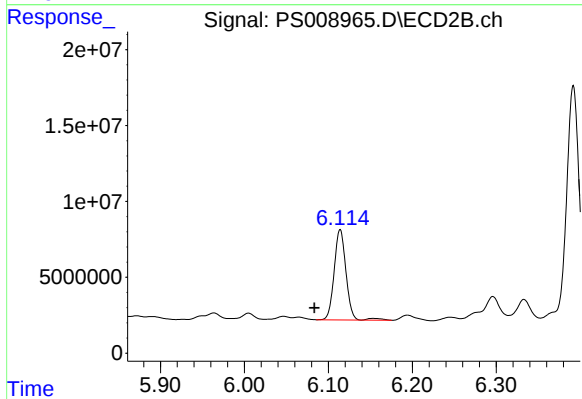

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 58602103
Conc: 40.16 ng/ml

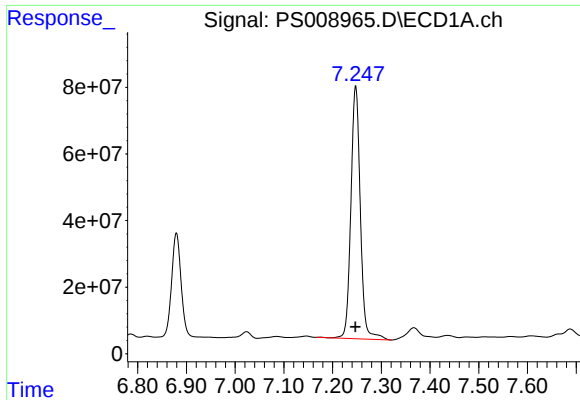

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 1021048584
Conc: 466.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127024BL

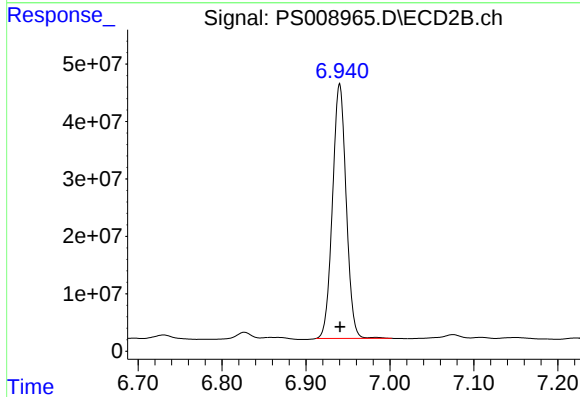


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 502531994
Conc: 521.54 ng/ml

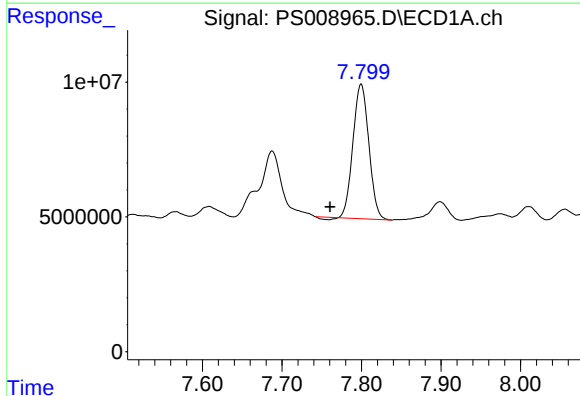


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 69341690
Conc: 8.62 ug/ml

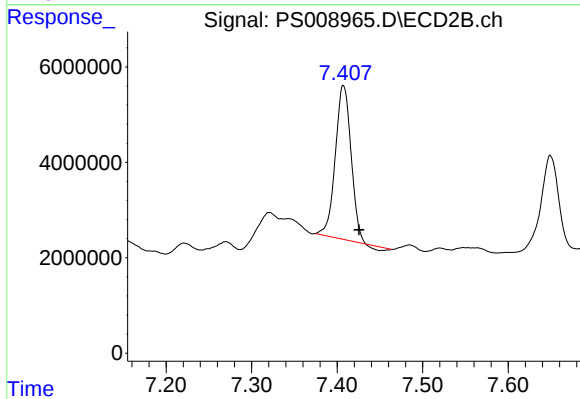

#7 MCPA


R.T.: 7.408 min
Delta R.T.: -0.018 min
Response: 40061459
Conc: 9.05 ug/ml

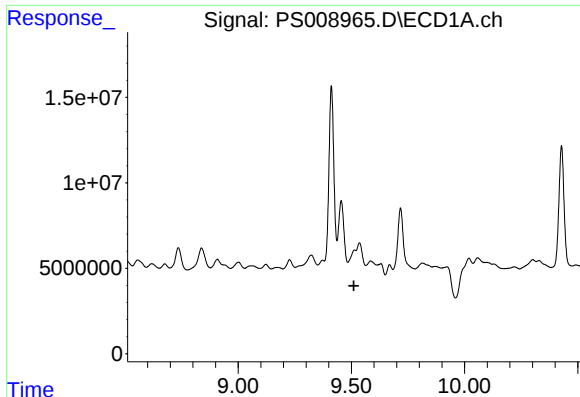

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127024BL

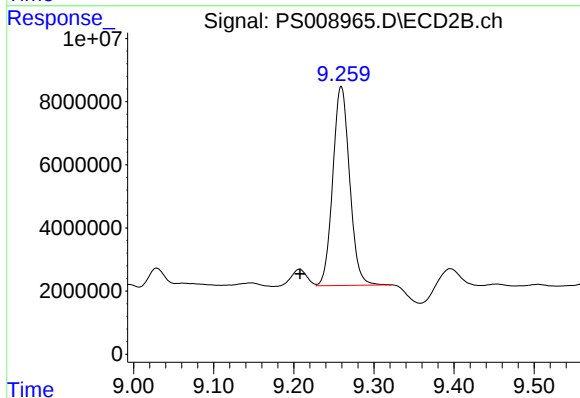


#12 2,4,5-T

R.T.: 9.259 min
Delta R.T.: 0.052 min
Response: 92188110
Conc: 17.03 ng/ml

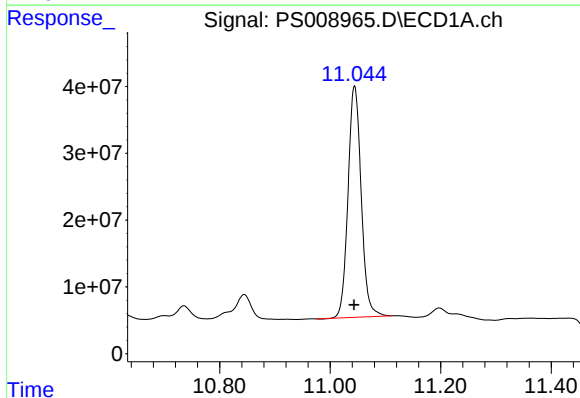


#15 Picloram

R.T.: 11.044 min
Delta R.T.: 0.001 min
Response: 572718495
Conc: 41.83 ng/ml

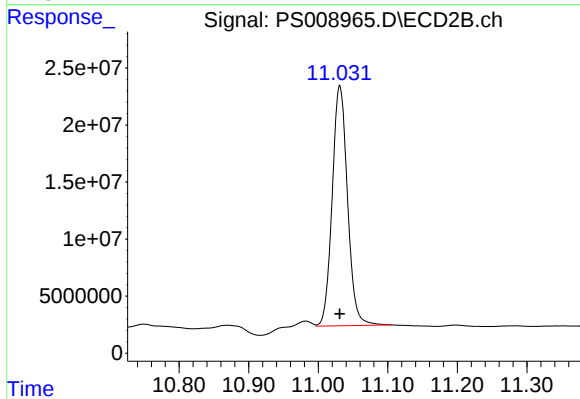

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 321980678
Conc: 44.31 ng/ml

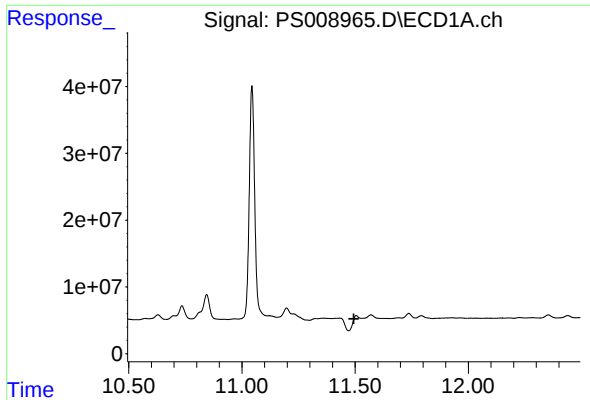

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127024BL

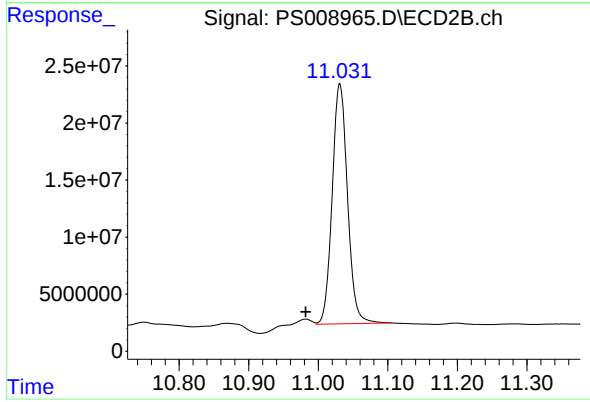

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.049 min
Response: 321980678
Conc: 46.53 ng/ml