

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 19:36
 Operator : DD\AJ
 Sample : L1635-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 03:59:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	716.4E6	320.7E6	327.620	332.876
Target Compounds							
1) T	Dalapon	0.000	2.591	0	173.3E6	N.D.	118.516
2) T	3,5-DICHL...	0.000	6.114	0	143.8E6	N.D.	98.573
7) T	MCPA	7.799	7.407	176.0E6	82772594	21.880	18.709
8) T	DICHLORPROP	0.000	7.760	0	74762914	N.D.	74.619
11) T	2,4,5-TP ...	0.000	8.795	0	60248891	N.D.	11.122
12) T	2,4,5-T	9.455	0.000	89010125	0	8.325	N.D. #
14) T	DINOSEB	0.000	10.065	0	99991003	N.D.	25.288
16) T	DCPA	11.509	0.000	146.8E6	0	10.686	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 19:36
Operator : DD\AJ
Sample : L1635-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 03:59:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

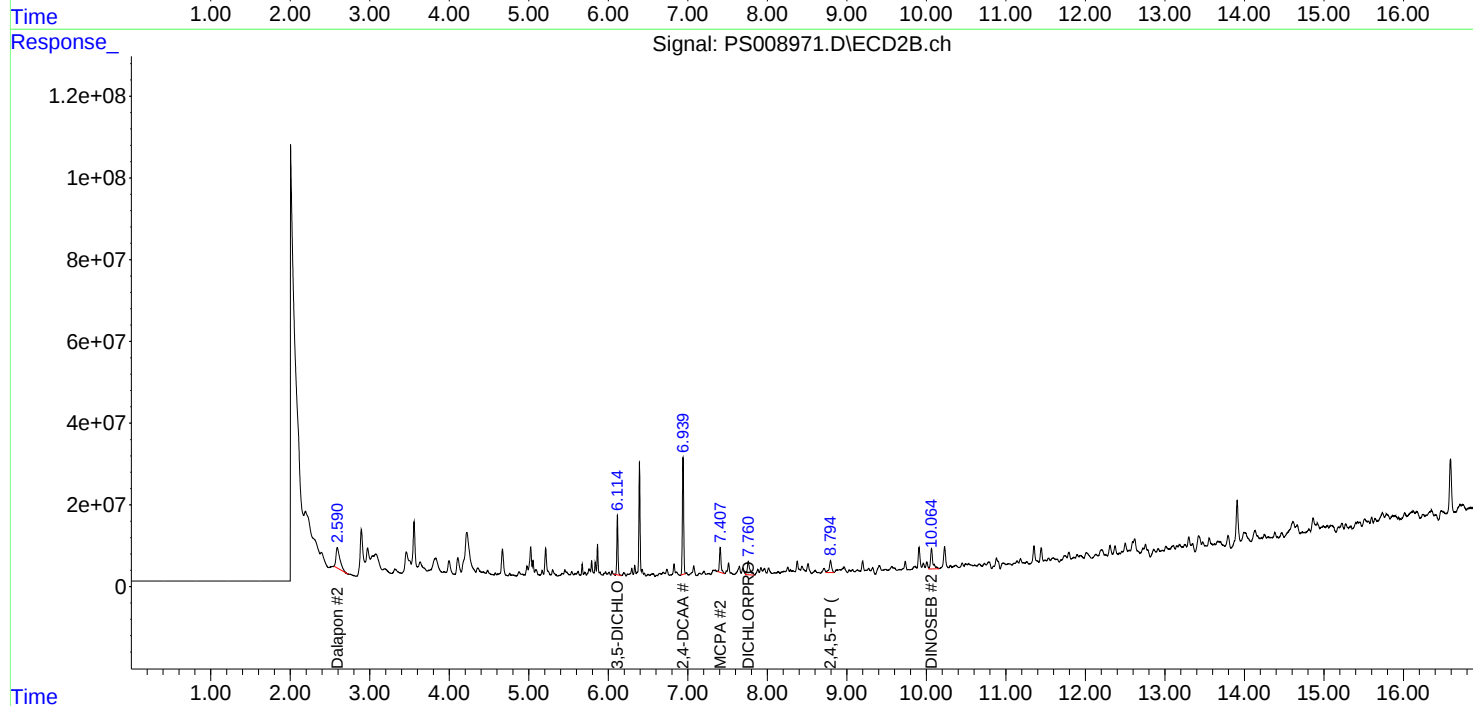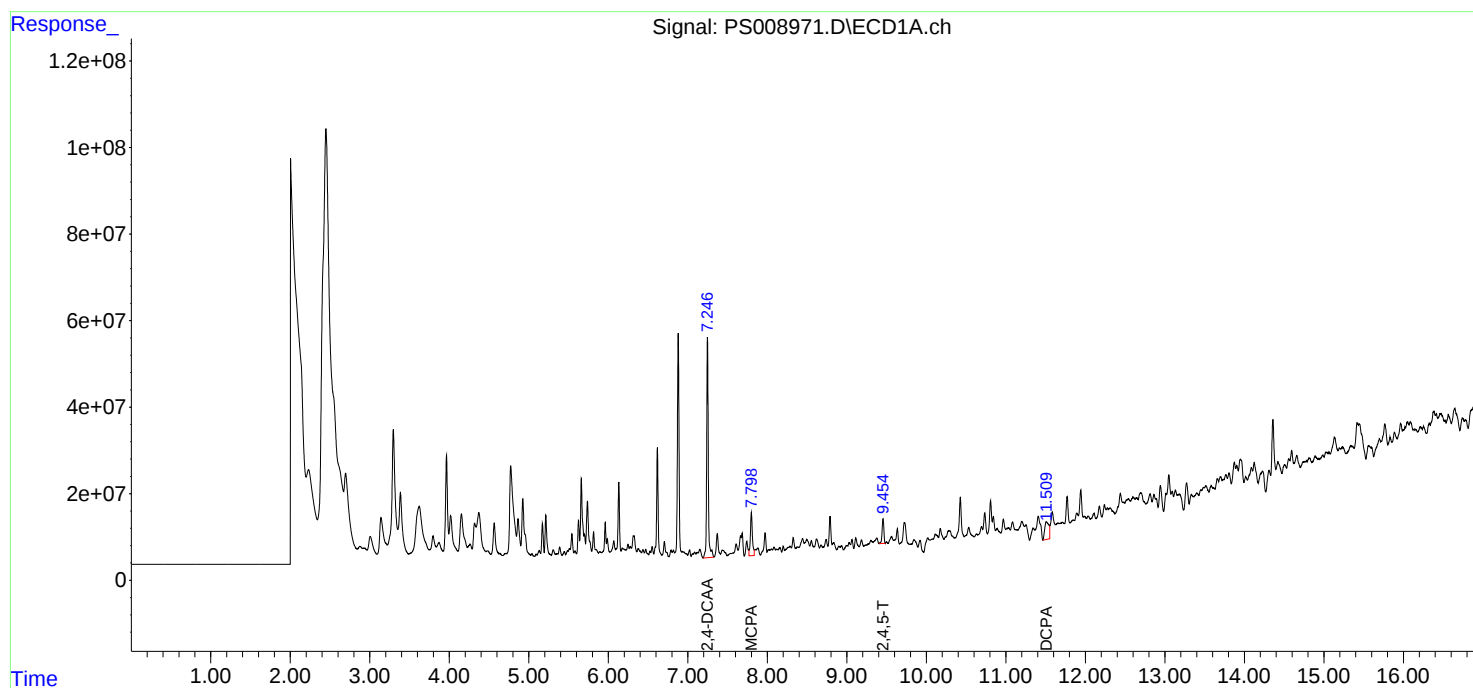


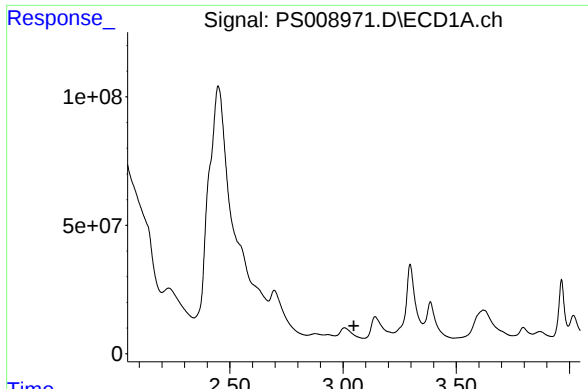

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

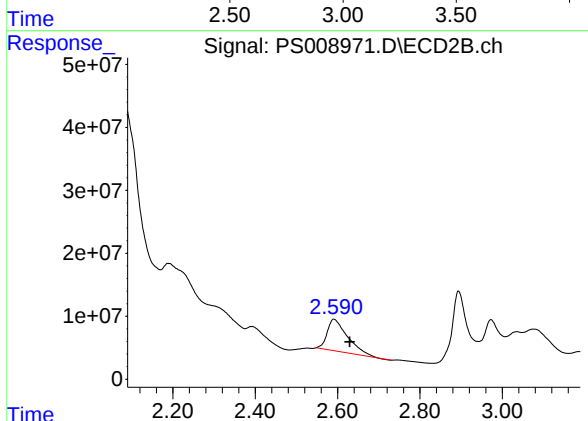


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 173296185
Conc: 118.52 ng/ml

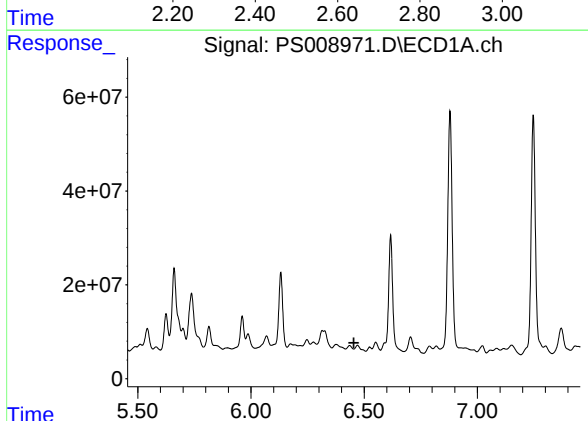


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

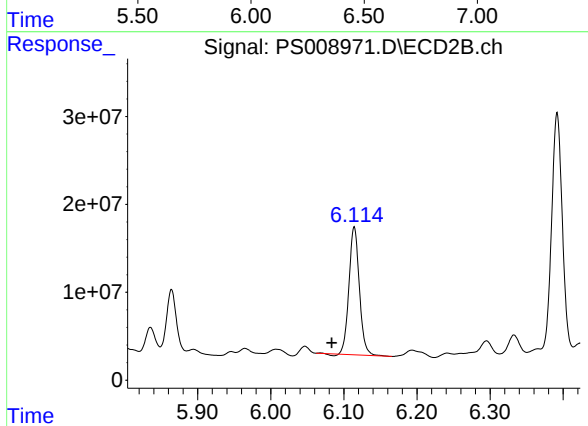

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 143844638
Conc: 98.57 ng/ml

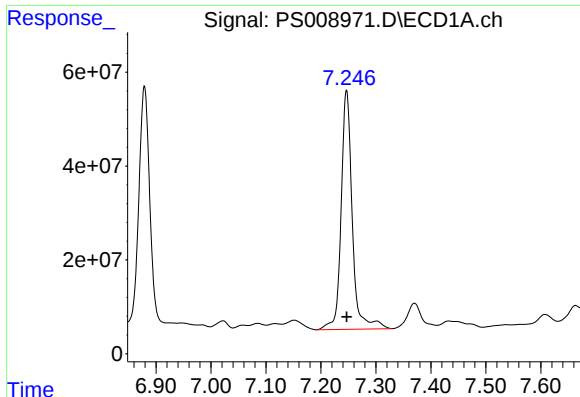

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 716371742
Conc: 327.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

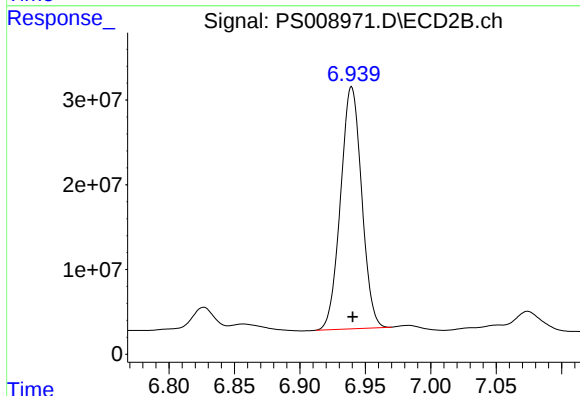


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 320744525
Conc: 332.88 ng/ml

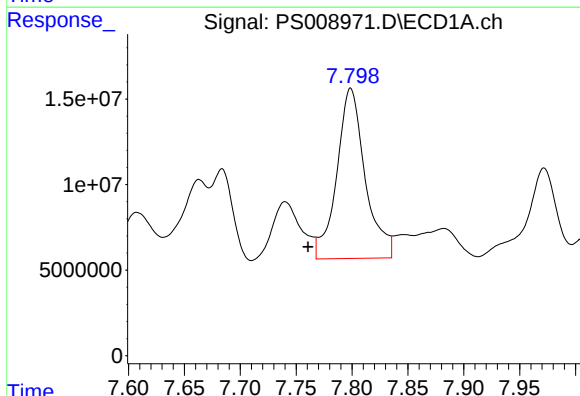


#7 MCPA

R.T.: 7.799 min
Delta R.T.: 0.038 min
Response: 176000767
Conc: 21.88 ug/ml

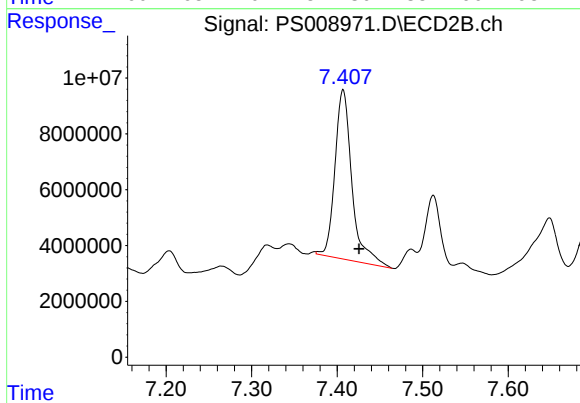

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 82772594
Conc: 18.71 ug/ml

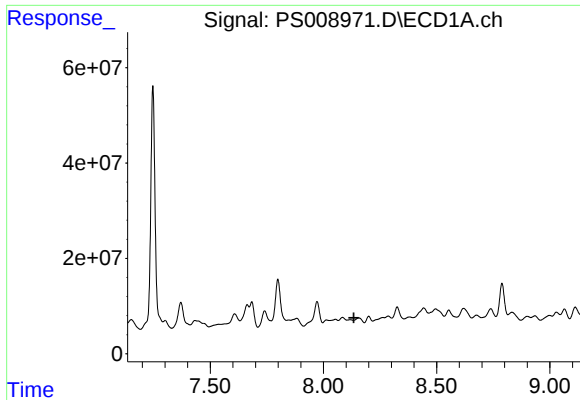

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

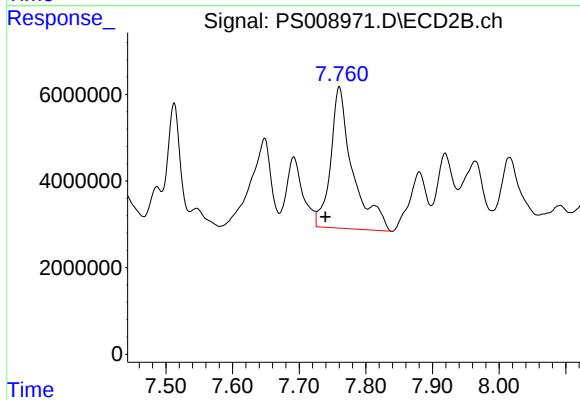


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 74762914
Conc: 74.62 ng/ml

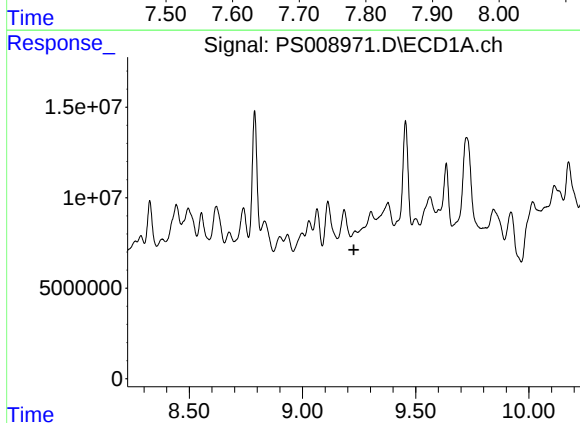


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

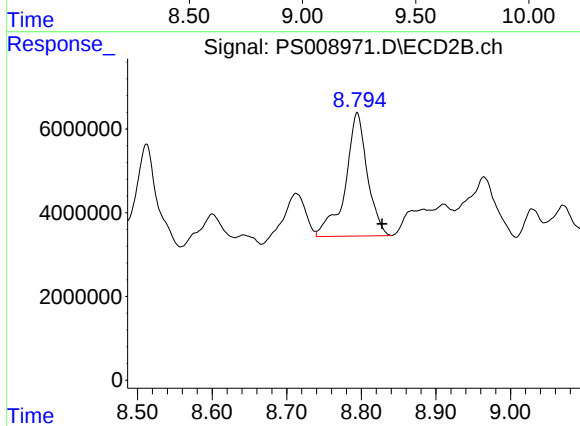

#11 2,4,5-TP (SILVEX)


R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 60248891
Conc: 11.12 ng/ml

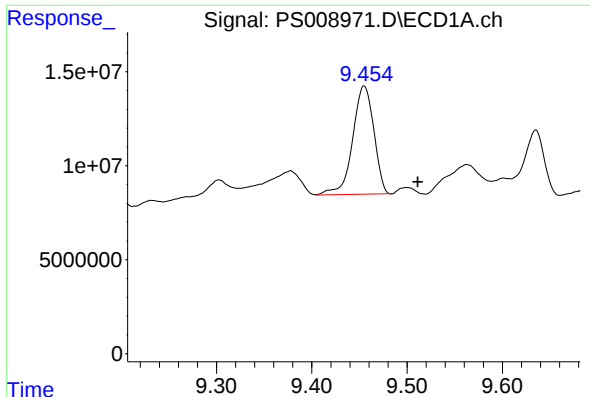

#12 2,4,5-T


R.T.: 9.455 min
Delta R.T.: -0.056 min
Response: 89010125
Conc: 8.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

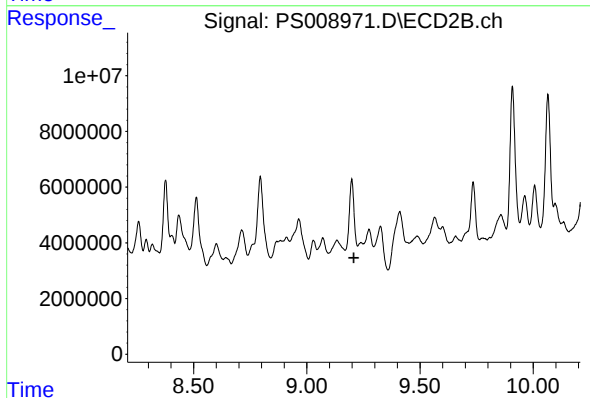


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

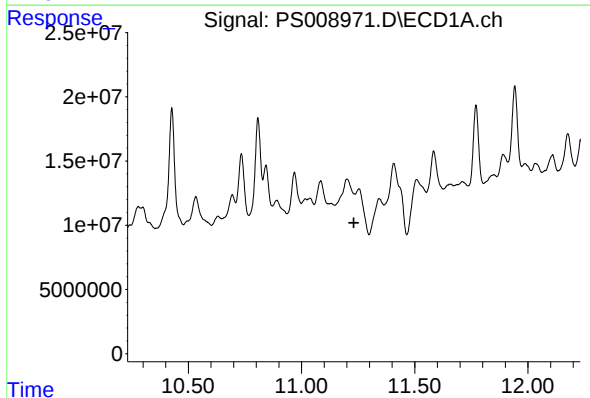


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

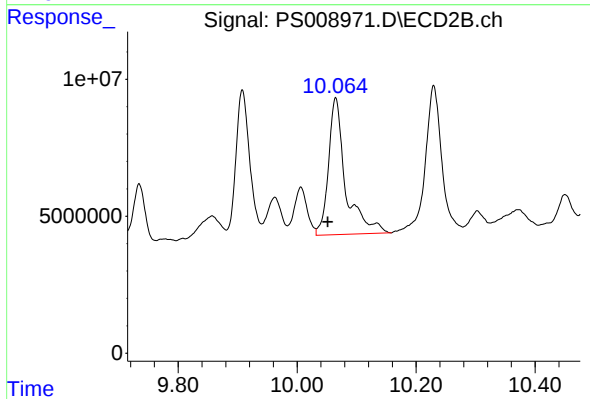

#14 DINOSEB


R.T.: 10.065 min
Delta R.T.: 0.013 min
Response: 99991003
Conc: 25.29 ng/ml

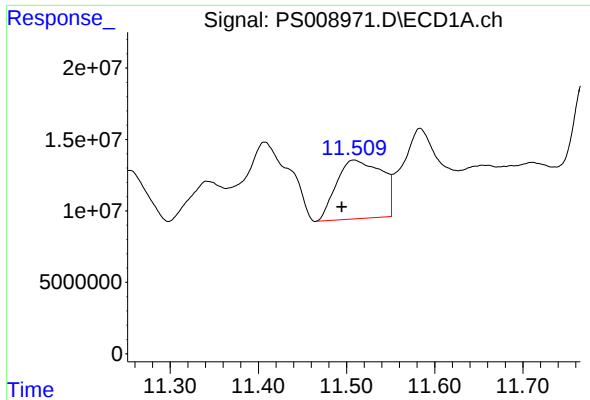

#16 DCPA

R.T.: 11.509 min
Delta R.T.: 0.014 min
Response: 146836735
Conc: 10.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

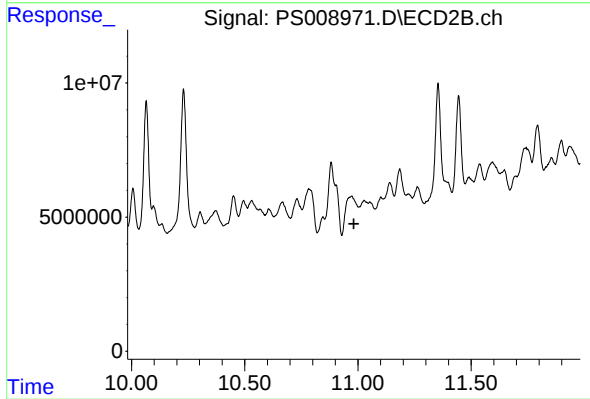

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.982 min
Response: 0
Conc: N.D.