

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 20:22
 Operator : DD\AJ
 Sample : L1635-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DUNR-TS004-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 03:59:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	661.2E6	312.5E6	302.404	324.366
Target Compounds							
1) T	Dalapon	0.000	2.591	0	149.5E6	N.D.	102.274
2) T	3,5-DICHL...	0.000	6.115	0	138.5E6	N.D.	94.923
7) T	MCPA	7.740	7.408	119.5E6	143.7E6	14.853	32.483 #
8) T	DICHLORPROP	0.000	7.761	0	81822653	N.D.	81.665
12) T	2,4,5-T	9.455	0.000	171.7E6	0	16.063	N.D. #
13) T	2,4-DB	10.017	0.000	60598863	0	41.994	N.D. #
14) T	DINOSEB	0.000	10.066	0	69713899	N.D.	17.631
16) T	DCPA	11.505	0.000	140.3E6	0	10.213	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 20:22
Operator : DD\AJ
Sample : L1635-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
DUNR-TS004-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 03:59:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

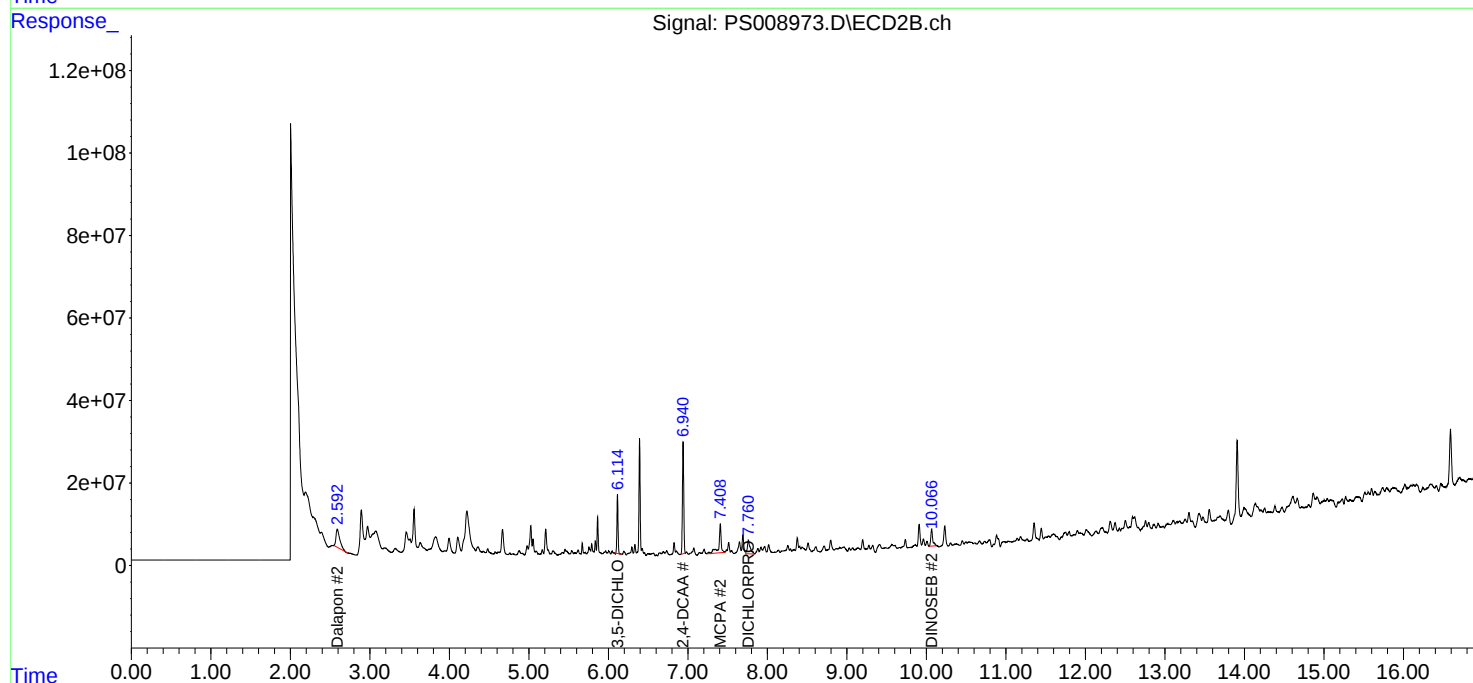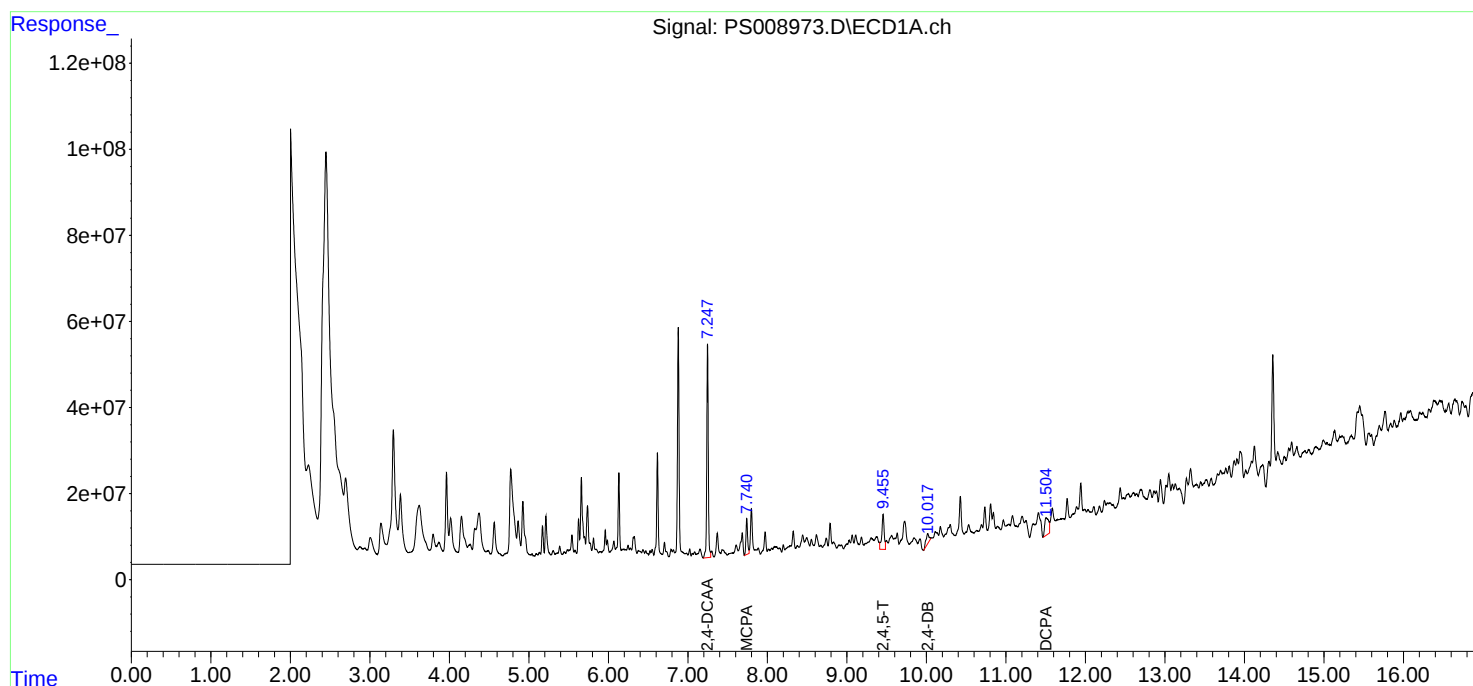


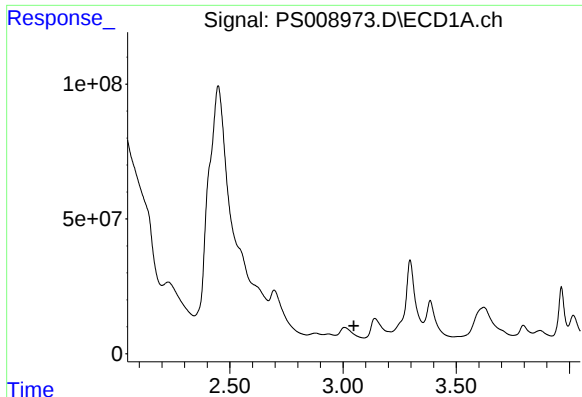

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUNR-TS004-01

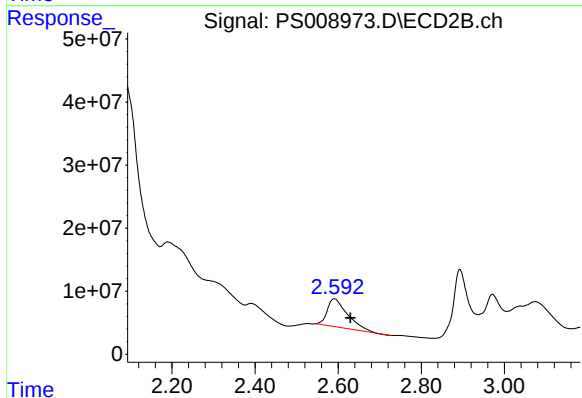


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 149547034
Conc: 102.27 ng/ml

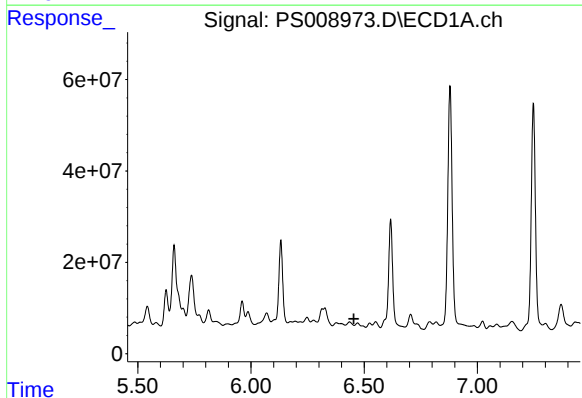


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

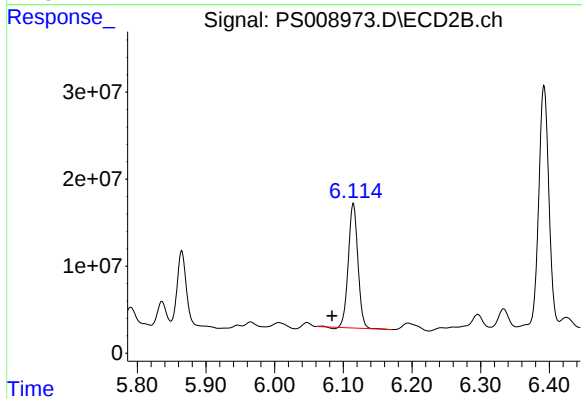

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 138518908
Conc: 94.92 ng/ml

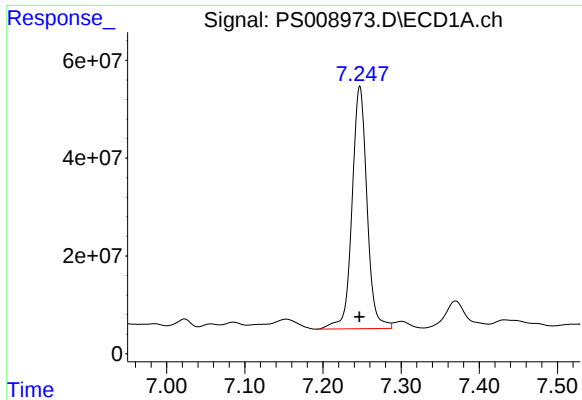

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 661234850
Conc: 302.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS004-01

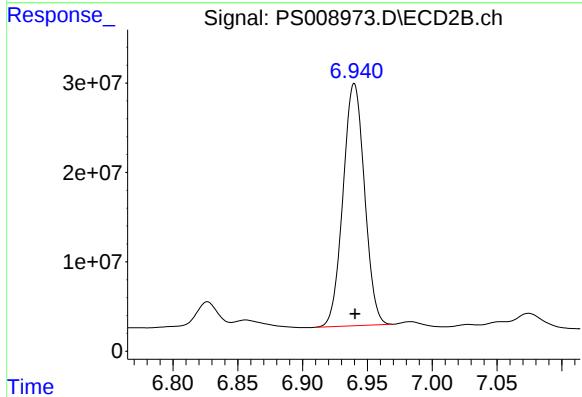


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 312544295
Conc: 324.37 ng/ml

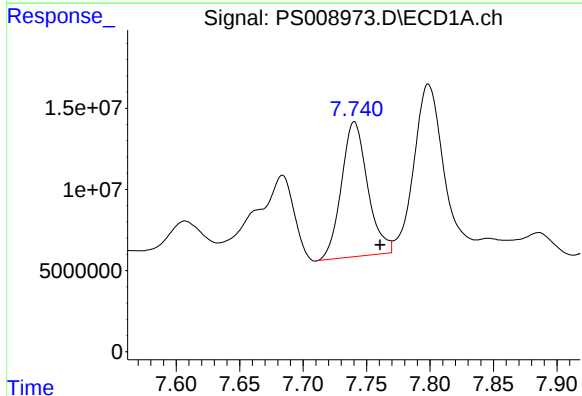


#7 MCPA

R.T.: 7.740 min
Delta R.T.: -0.020 min
Response: 119477137
Conc: 14.85 ug/ml

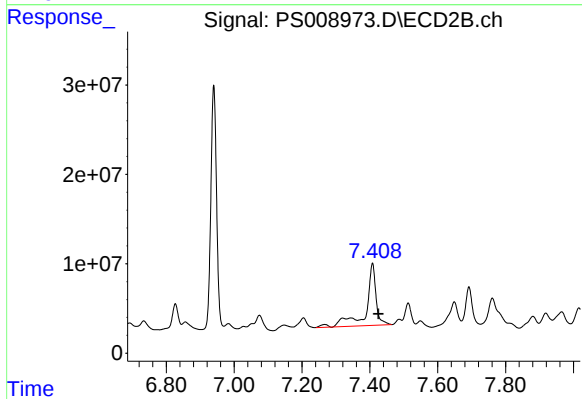

#7 MCPA


R.T.: 7.408 min
Delta R.T.: -0.018 min
Response: 143711755
Conc: 32.48 ug/ml

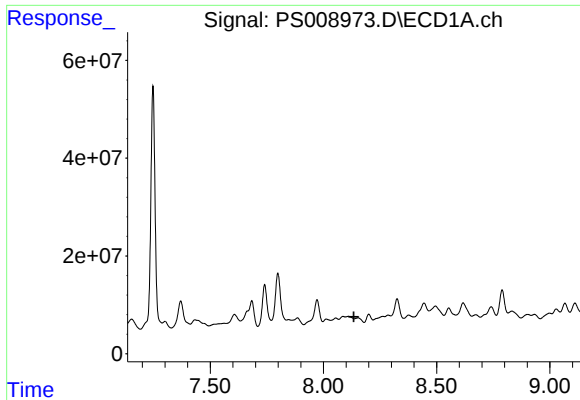

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUNR-TS004-01

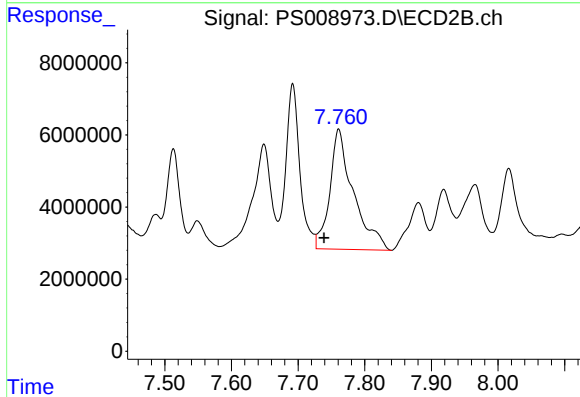


#8 DICHLORPROP

R.T.: 7.761 min
Delta R.T.: 0.022 min
Response: 81822653
Conc: 81.66 ng/ml

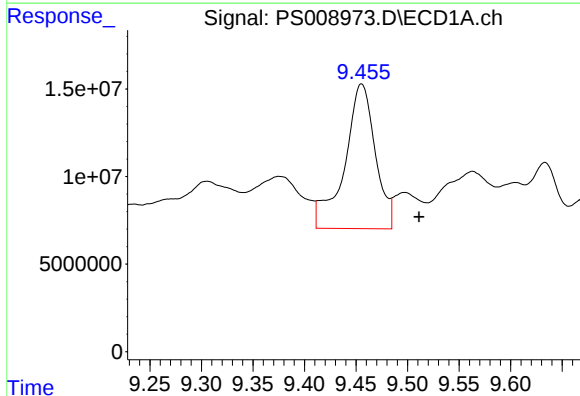


#12 2,4,5-T

R.T.: 9.455 min
Delta R.T.: -0.056 min
Response: 171744746
Conc: 16.06 ng/ml

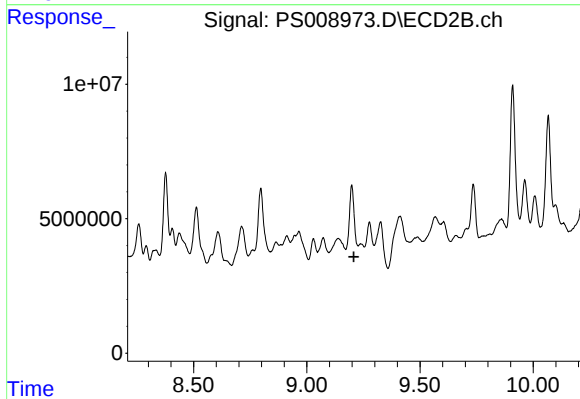

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

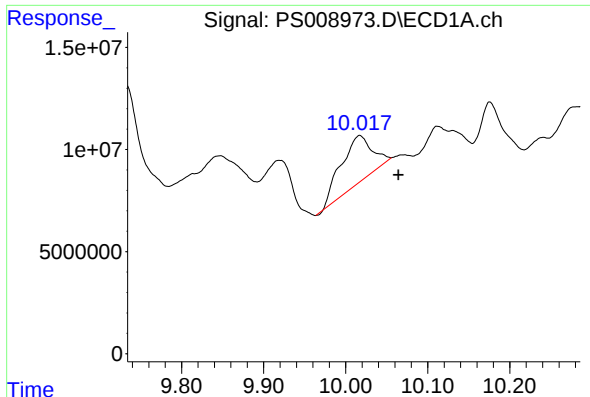

#13 2,4-DB


R.T.: 10.017 min
Delta R.T.: -0.047 min
Response: 60598863
Conc: 41.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS004-01

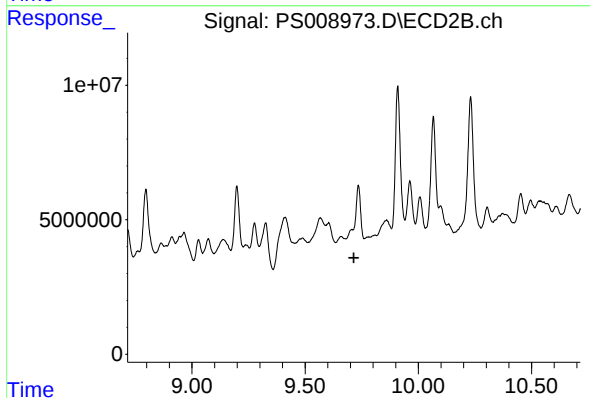


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.715 min
Response: 0
Conc: N.D.

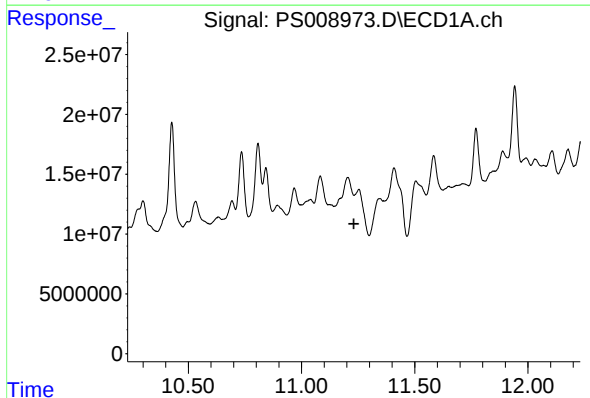


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

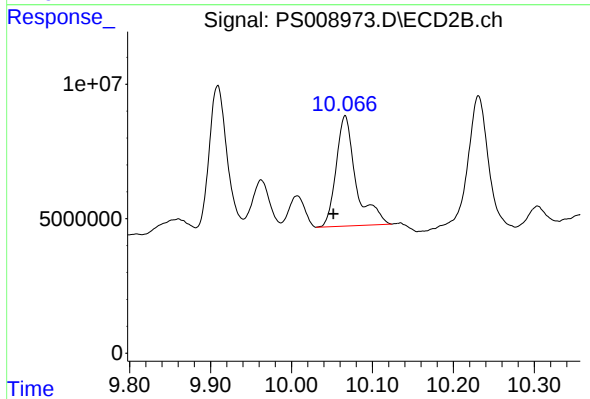

#14 DINOSEB


R.T.: 10.066 min
Delta R.T.: 0.015 min
Response: 69713899
Conc: 17.63 ng/ml

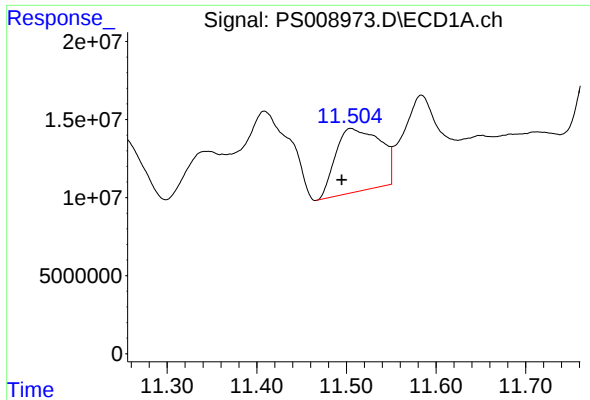

#16 DCPA

R.T.: 11.505 min
Delta R.T.: 0.011 min
Response: 140341009
Conc: 10.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS004-01

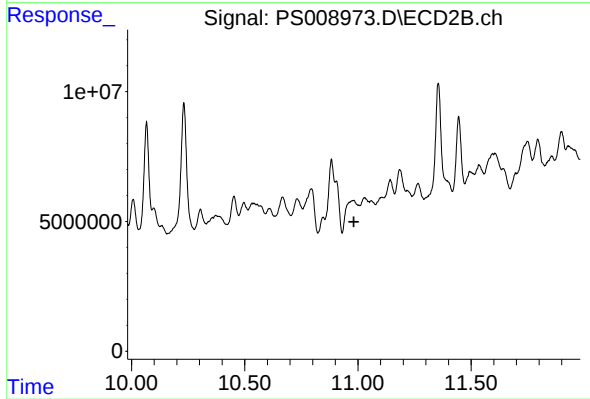

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.982 min
Response: 0
Conc: N.D.