

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 22:39
 Operator : DD\AJ
 Sample : L1635-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DUNR-TS006-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:00:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	586.4E6	300.4E6	268.188	311.739
Target Compounds							
1) T	Dalapon	0.000	2.591	0	164.8E6	N.D.	112.730
2) T	3,5-DICHL...	0.000	6.114	0	174.1E6	N.D.	119.305
7) T	MCPA	7.739	7.407	123.2E6	147.9E6	15.313	33.428 #
8) T	DICHLORPROP	0.000	7.760	0	82749997	N.D.	82.590
10) T	Pentachlo...	8.675	0.000	53002146	0	1.826	N.D. #
12) T	2,4,5-T	9.455	9.201	94584746	52592612	8.846	9.716
14) T	DINOSEB	0.000	10.064	0	148.2E6	N.D.	37.470
15) T	Picloram	11.043	11.030	755.3E6	349.2E6	55.165	48.060
16) T	DCPA	11.499	11.030	144.8E6	349.2E6	10.536	50.471 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 22:39
Operator : DD\AJ
Sample : L1635-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DUNR-TS006-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:00:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

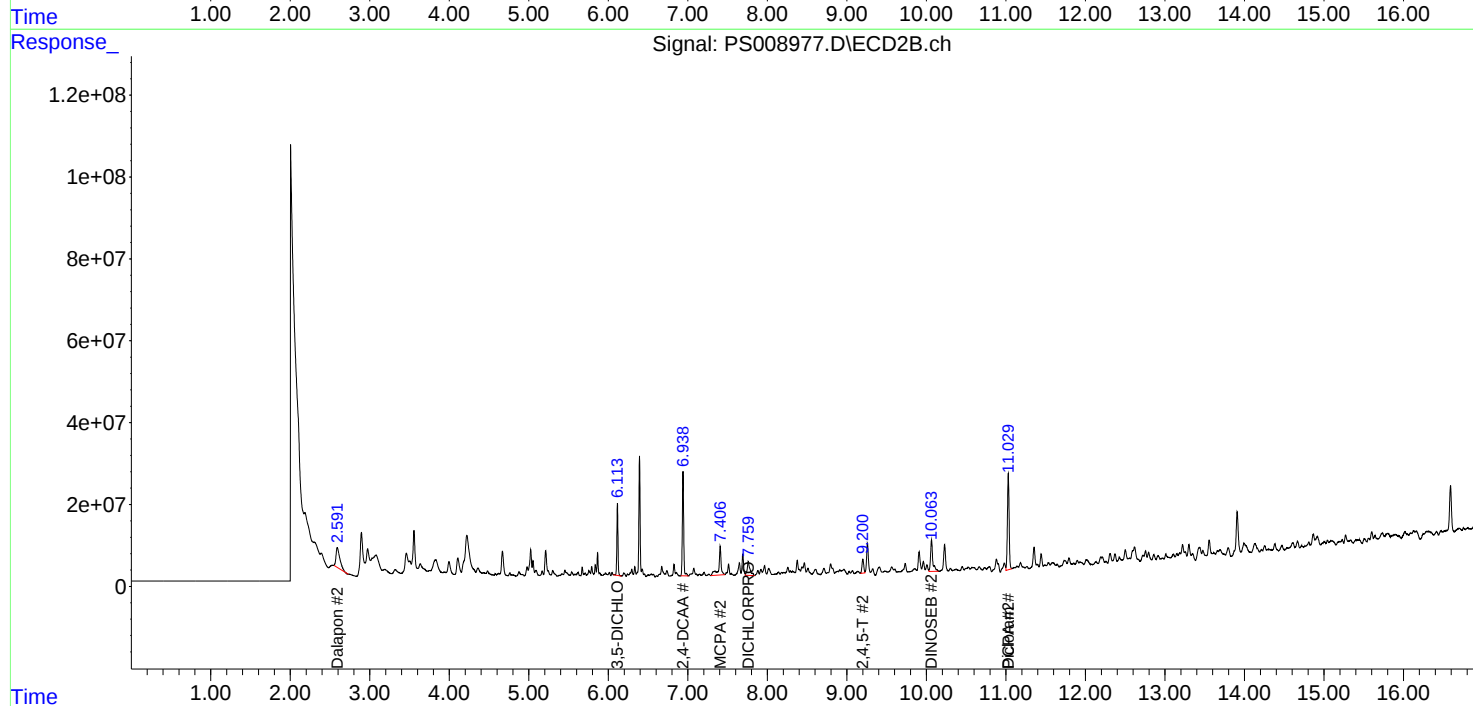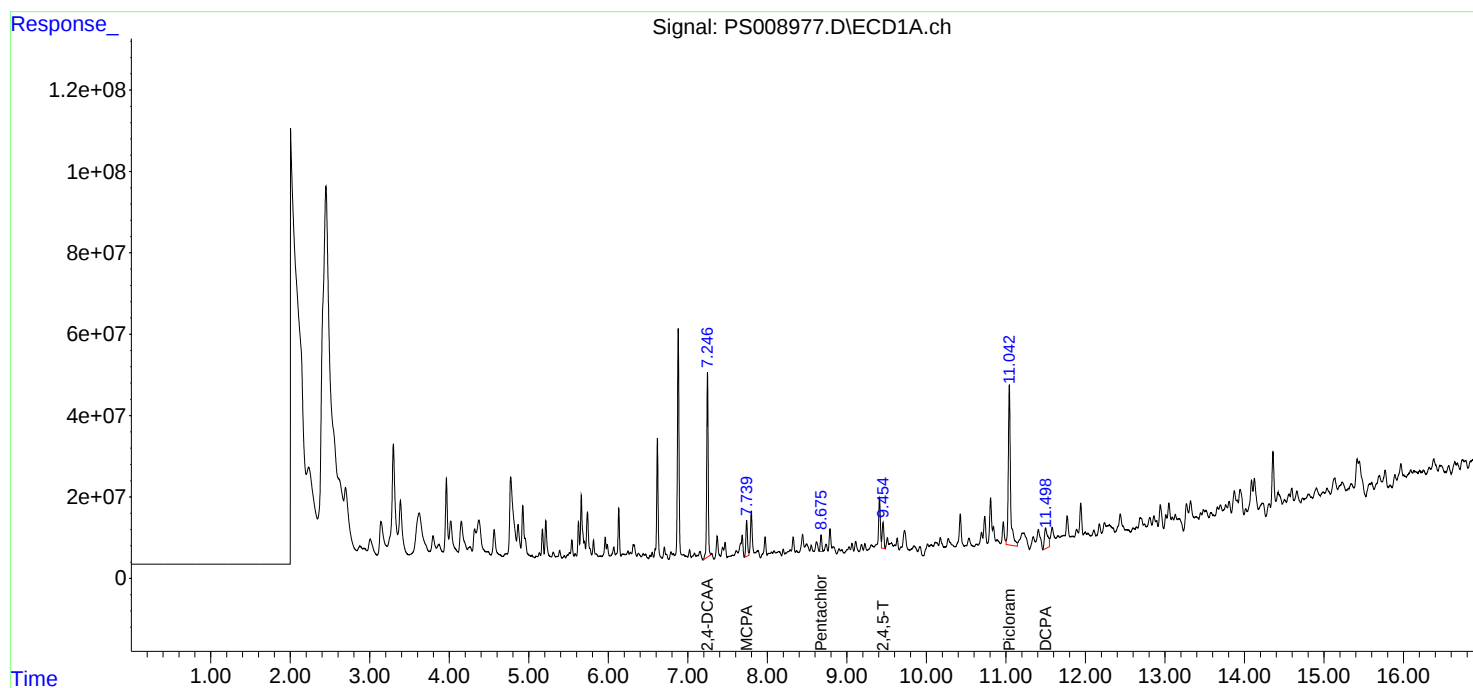


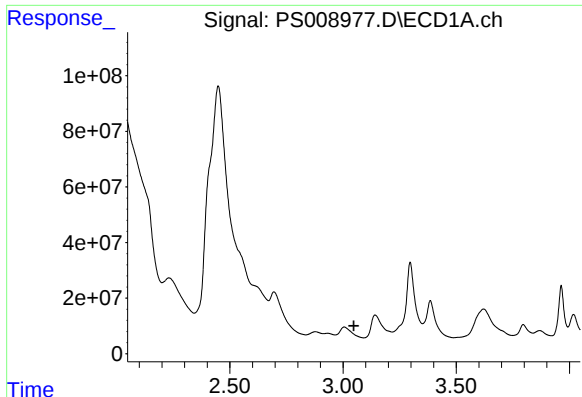

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUNR-TS006-01

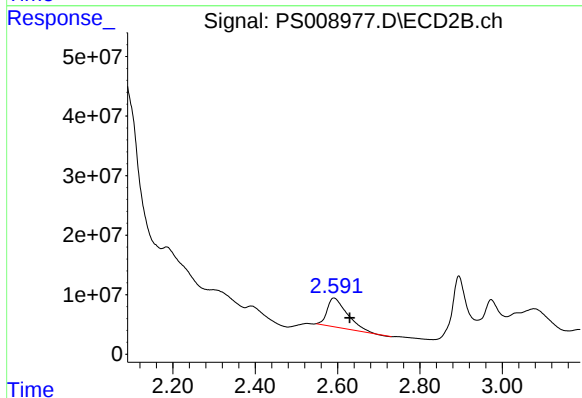


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 164835970
Conc: 112.73 ng/ml

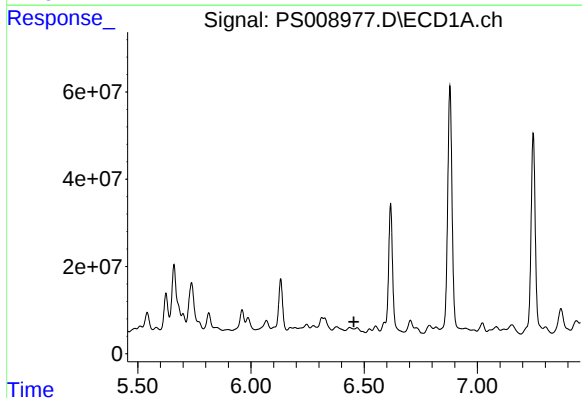


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

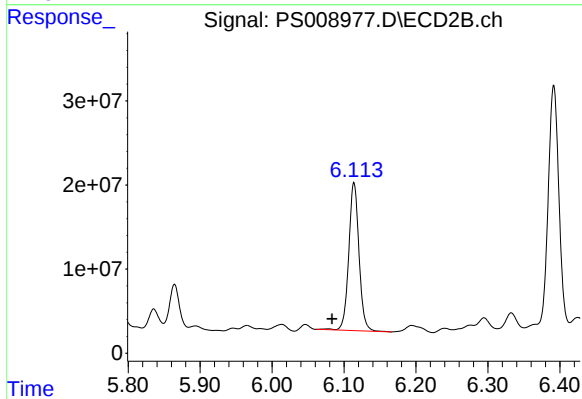

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 174098166
Conc: 119.30 ng/ml

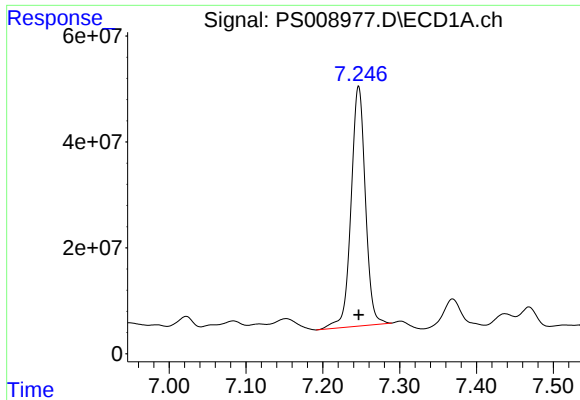

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 586418456
Conc: 268.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS006-01

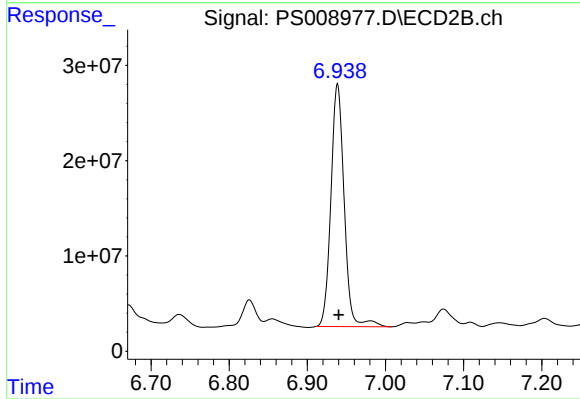


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 300377530
Conc: 311.74 ng/ml

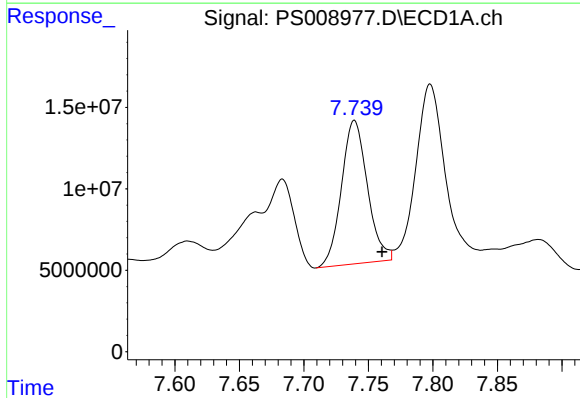


#7 MCPA

R.T.: 7.739 min
Delta R.T.: -0.021 min
Response: 123180578
Conc: 15.31 ug/ml

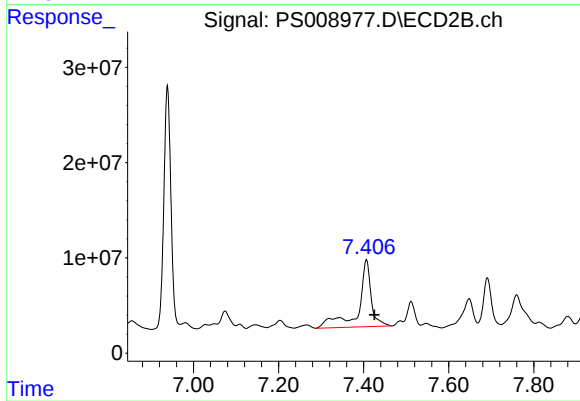

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 147892169
Conc: 33.43 ug/ml

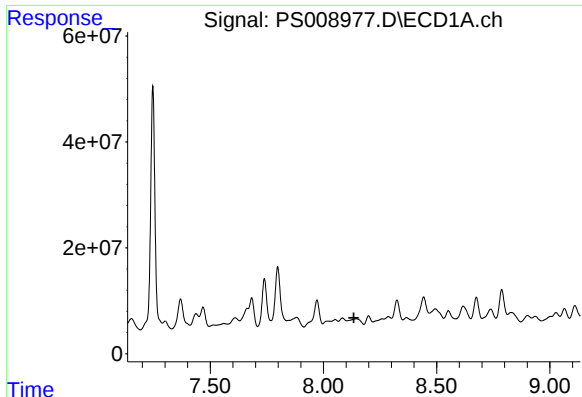

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUNR-TS006-01

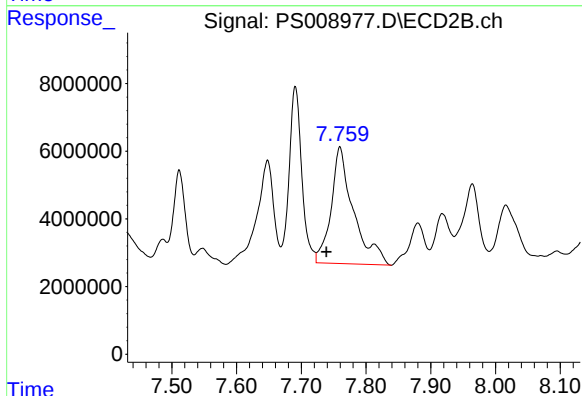


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 82749997
Conc: 82.59 ng/ml

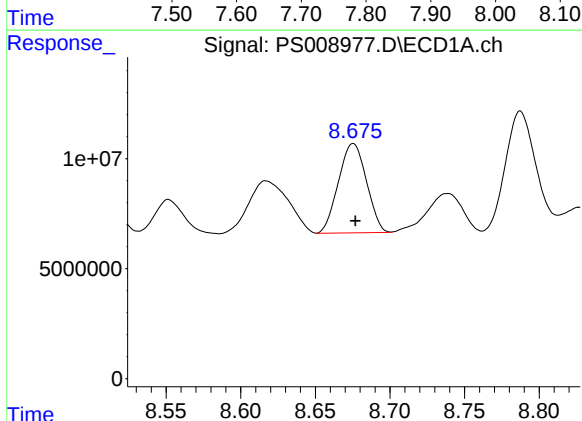


#10 Pentachlorophenol

R.T.: 8.675 min
Delta R.T.: -0.002 min
Response: 53002146
Conc: 1.83 ng/ml

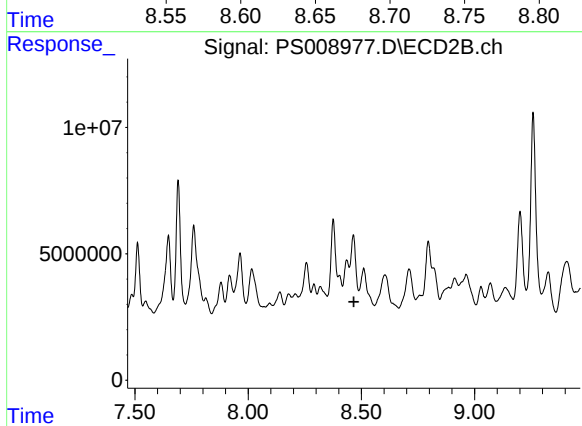

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.467 min
Response: 0
Conc: N.D.

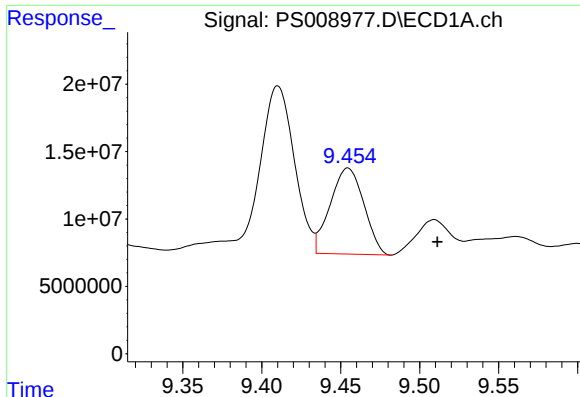

#12 2,4,5-T


R.T.: 9.455 min
Delta R.T.: -0.057 min
Response: 94584746
Conc: 8.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS006-01

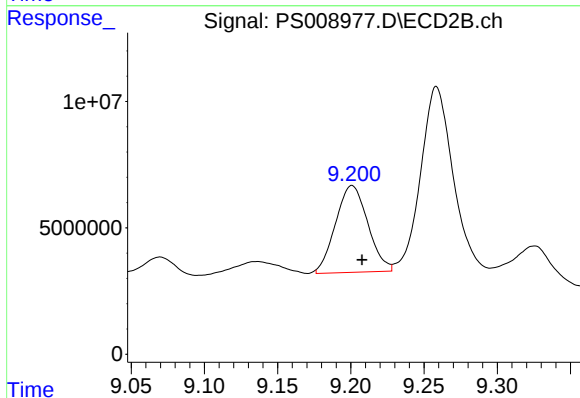


#12 2,4,5-T

R.T.: 9.201 min
Delta R.T.: -0.007 min
Response: 52592612
Conc: 9.72 ng/ml

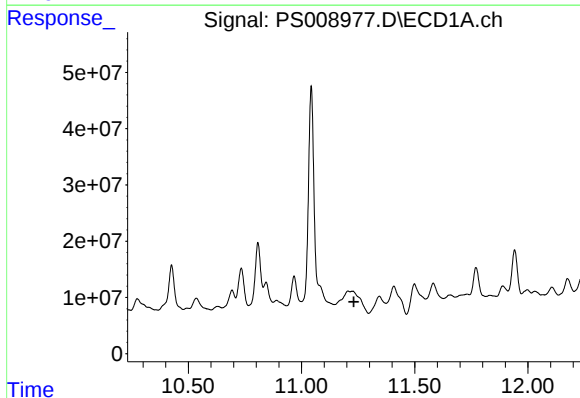


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

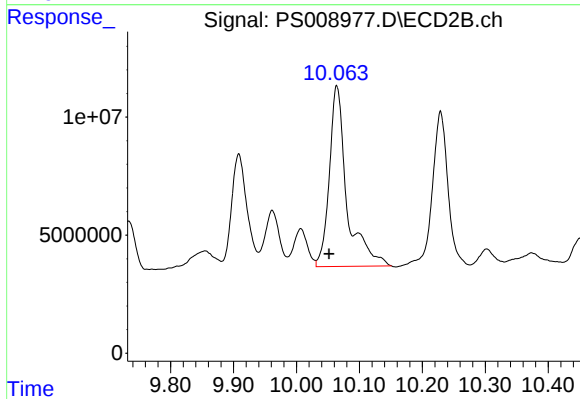

#14 DINOSEB


R.T.: 10.064 min
Delta R.T.: 0.013 min
Response: 148157176
Conc: 37.47 ng/ml

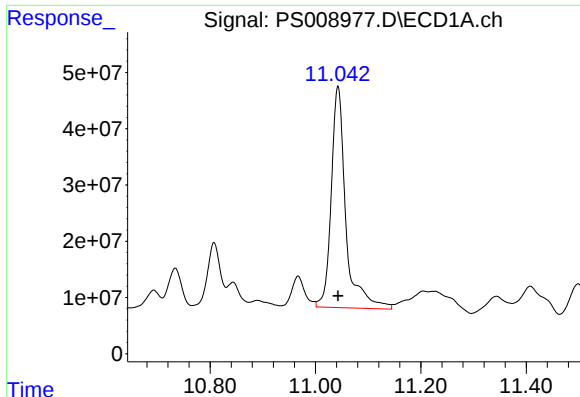

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 755261802
Conc: 55.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS006-01

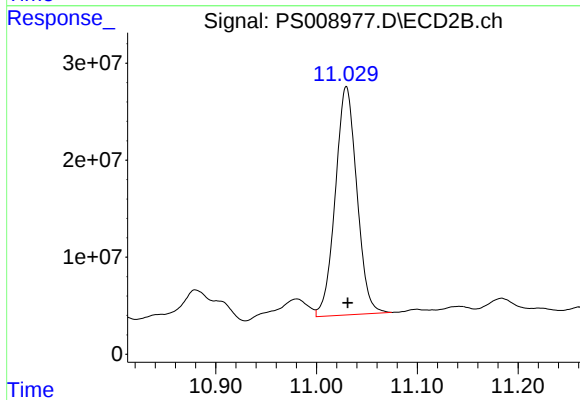


#15 Picloram

R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 349227631
Conc: 48.06 ng/ml

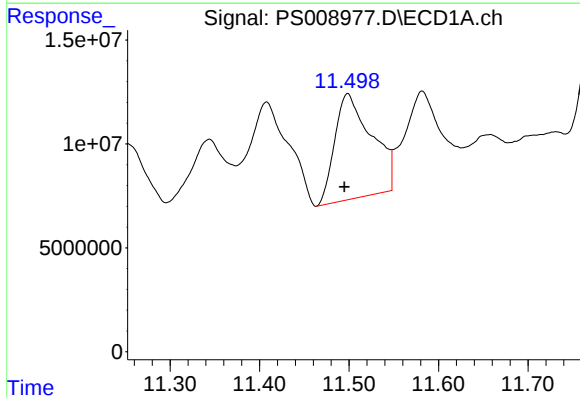

#16 DCPA

R.T.: 11.499 min
Delta R.T.: 0.004 min
Response: 144776477
Conc: 10.54 ng/ml

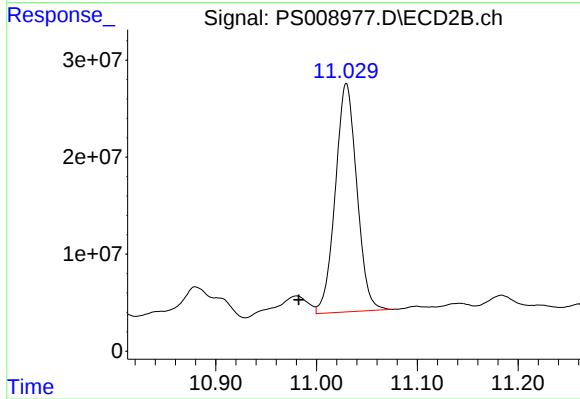

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.047 min
Response: 349227631
Conc: 50.47 ng/ml