

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008978.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 23:02
 Operator : DD\AJ
 Sample : L1635-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 DUNR-TS007-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:00:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	550.5E6	262.0E6	251.740	271.871
Target Compounds							
1) T	Dalapon	0.000	2.592	0	128.6E6	N.D.	87.956
2) T	3,5-DICHL...	0.000	6.114	0	144.1E6	N.D.	98.728
7) T	MCPA	7.741	7.407	260.0E6	120.5E6	32.323	27.229
8) T	DICHLORPROP	0.000	7.760	0	67827902	N.D.	67.697
11) T	2,4,5-TP ...	0.000	8.789	0	77998603	N.D.	14.399
12) T	2,4,5-T	9.454	0.000	140.5E6	0	13.136	N.D. #
14) T	DINOSEB	0.000	10.063	0	114.1E6	N.D.	28.865
16) T	DCPA	11.508	0.000	154.5E6	0	11.241	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008978.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 23:02
Operator : DD\AJ
Sample : L1635-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
DUNR-TS007-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:00:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

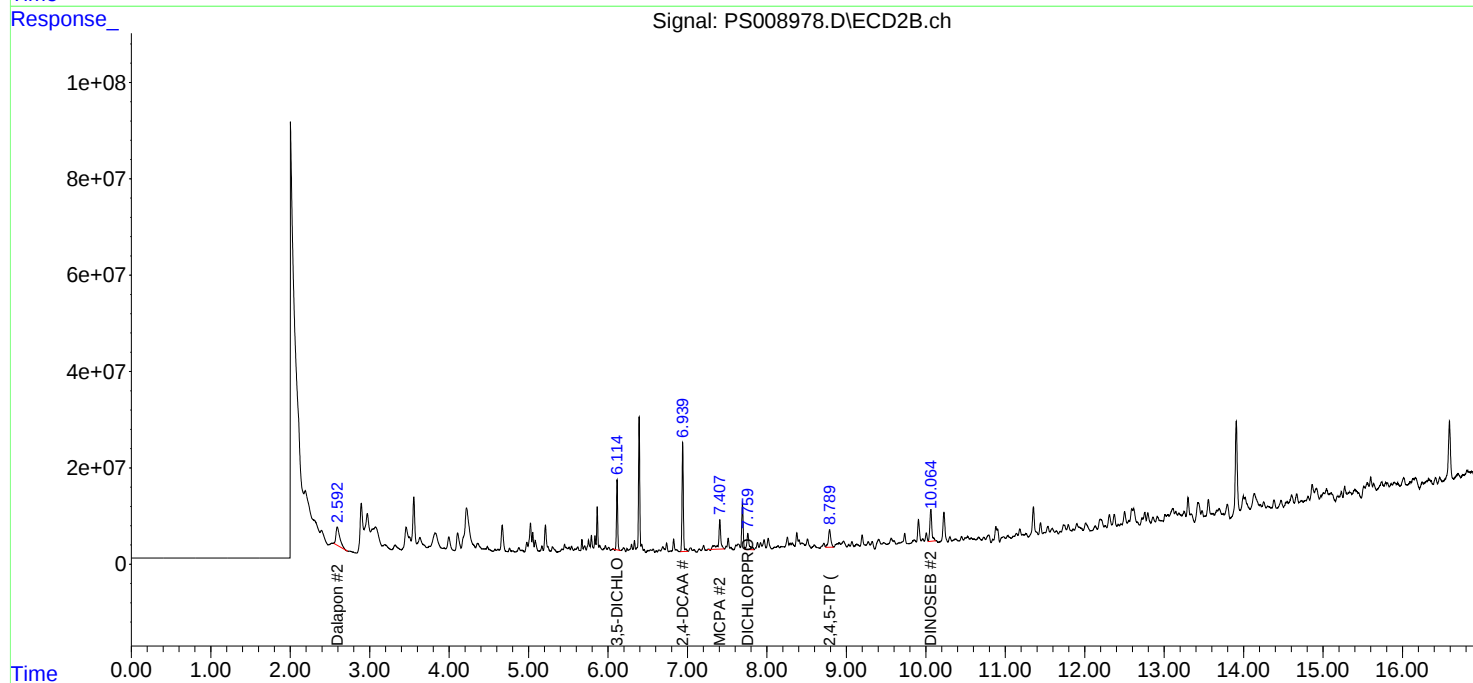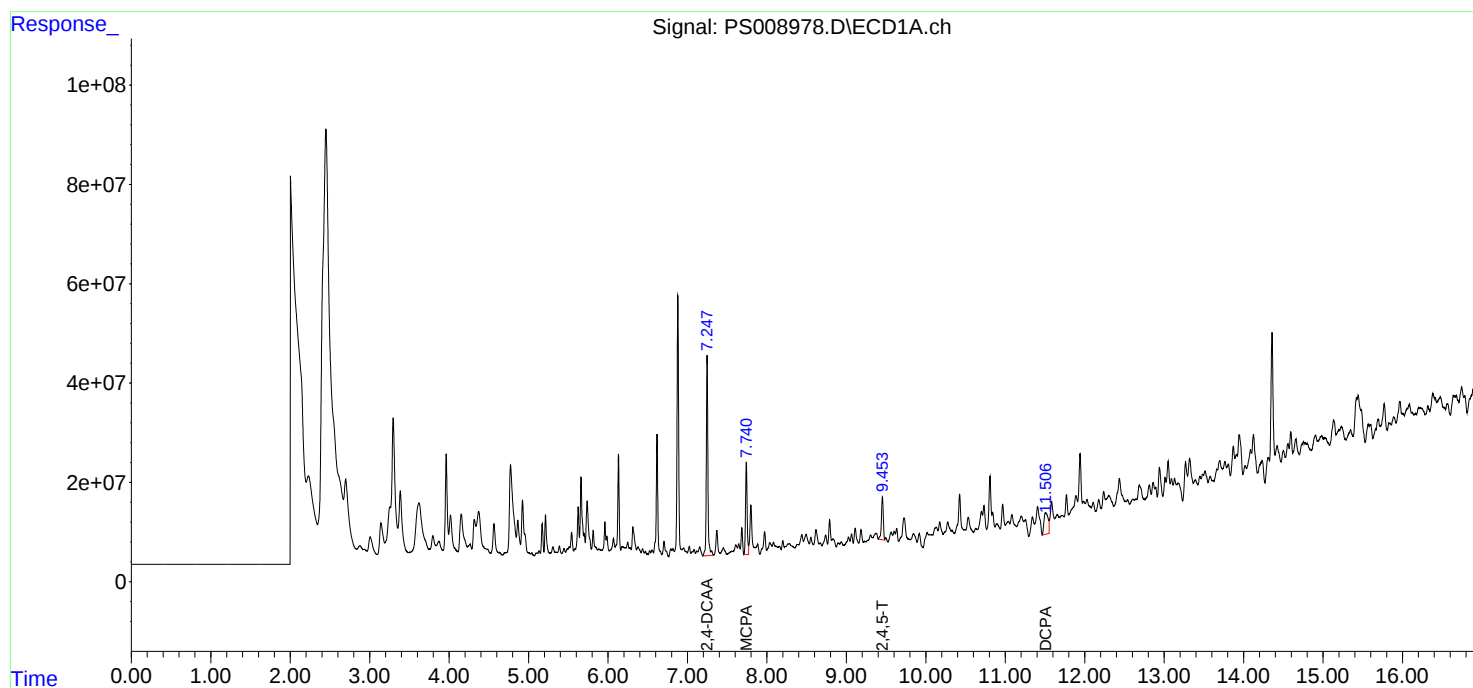


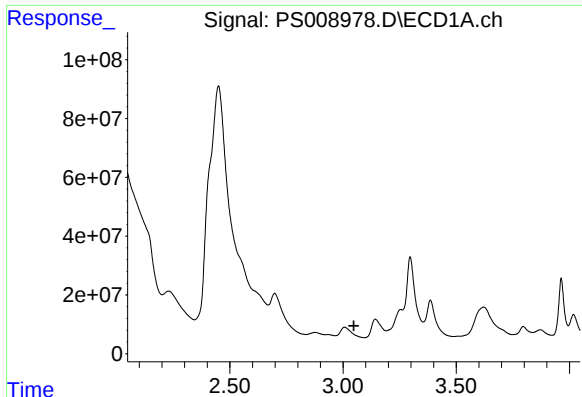

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUNR-TS007-01

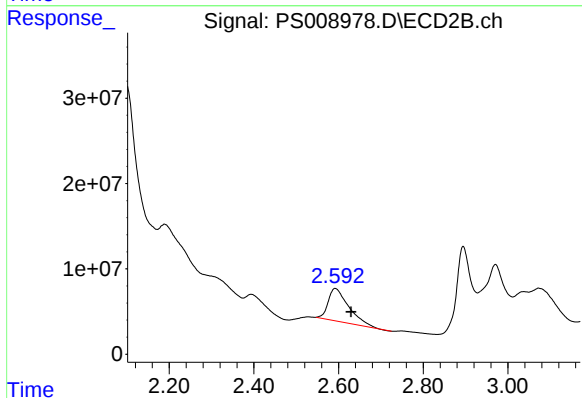


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 128611656
Conc: 87.96 ng/ml

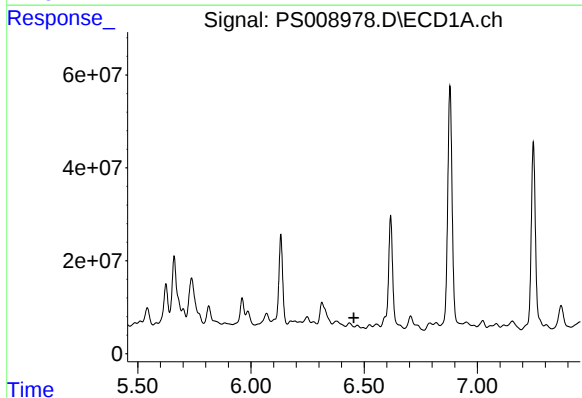


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

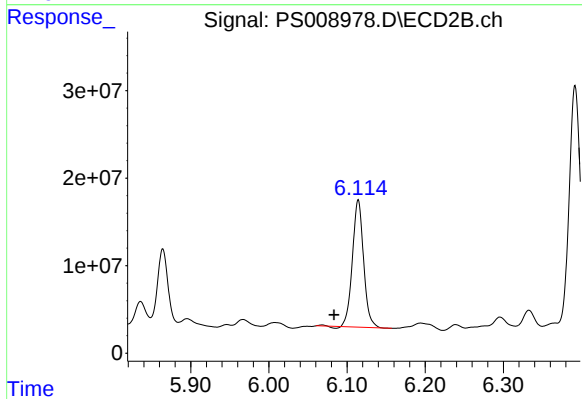

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 144070299
Conc: 98.73 ng/ml

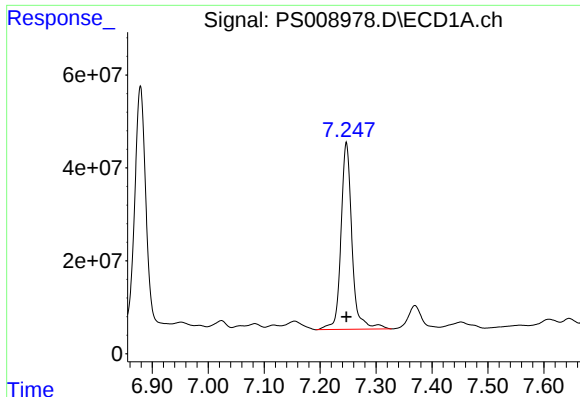

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 550452730
Conc: 251.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS007-01

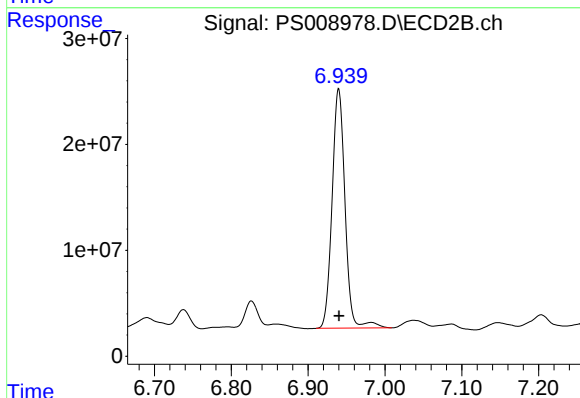


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 261962412
Conc: 271.87 ng/ml

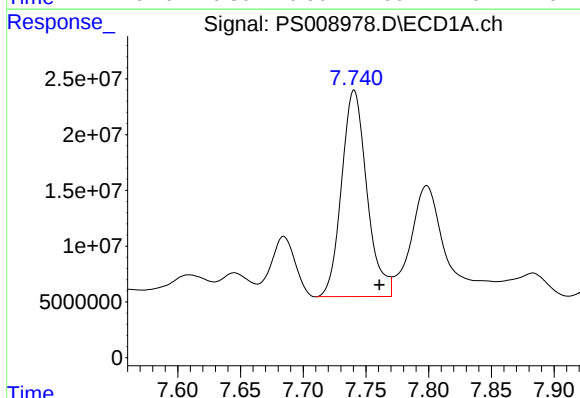


#7 MCPA

R.T.: 7.741 min
Delta R.T.: -0.020 min
Response: 260006871
Conc: 32.32 ug/ml

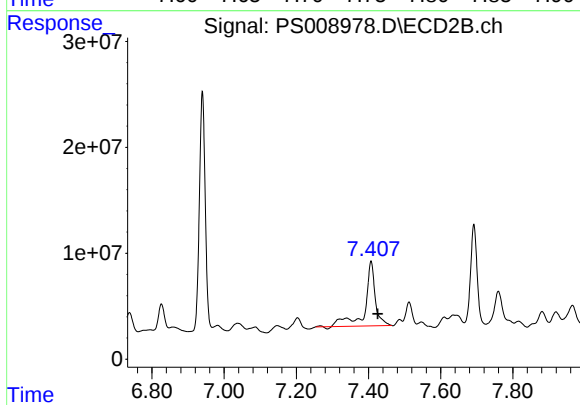

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 120469001
Conc: 27.23 ug/ml

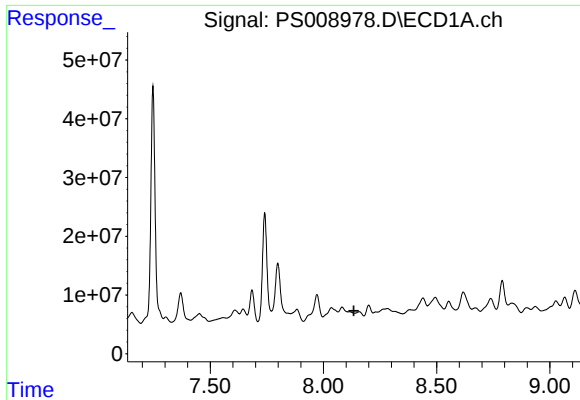

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
DUNR-TS007-01

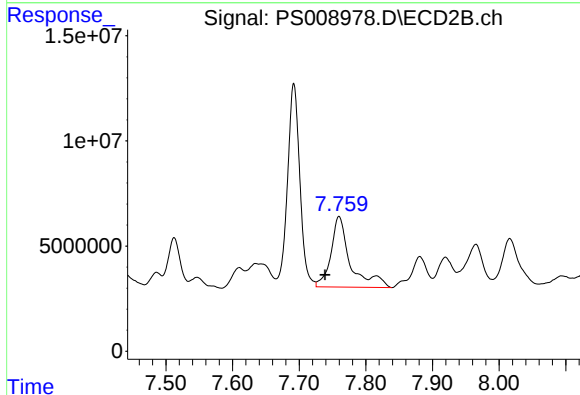


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 67827902
Conc: 67.70 ng/ml

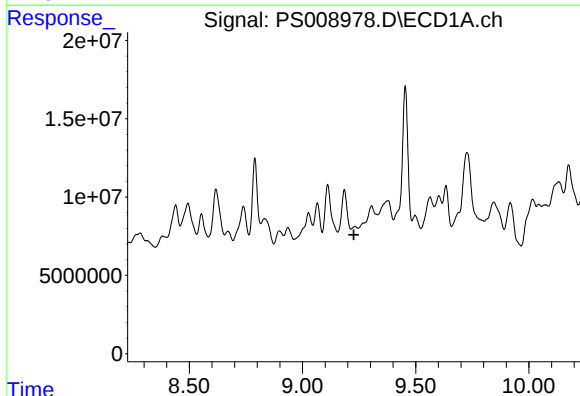


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

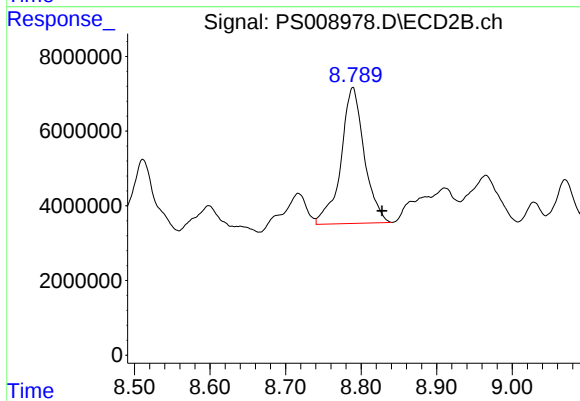

#11 2,4,5-TP (SILVEX)


R.T.: 8.789 min
Delta R.T.: -0.039 min
Response: 77998603
Conc: 14.40 ng/ml

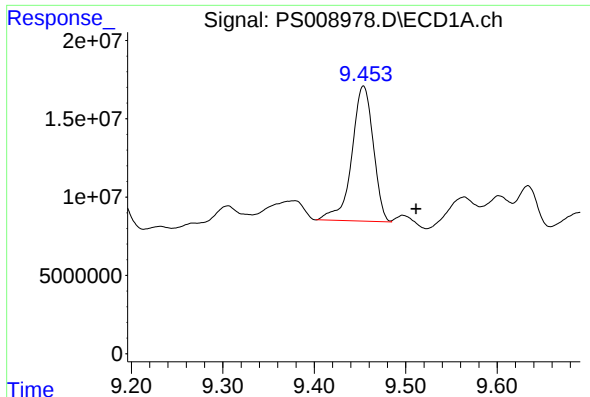

#12 2,4,5-T


R.T.: 9.454 min
Delta R.T.: -0.057 min
Response: 140451258
Conc: 13.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS007-01

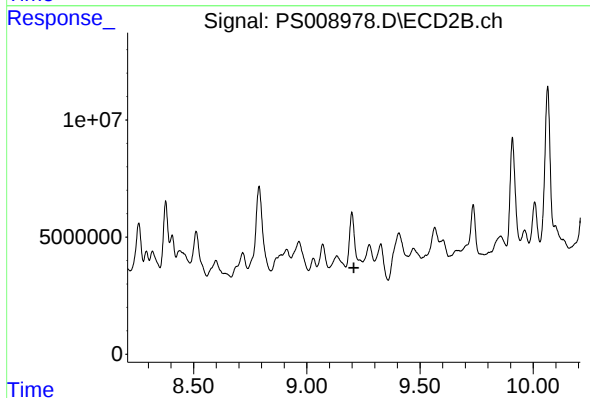


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

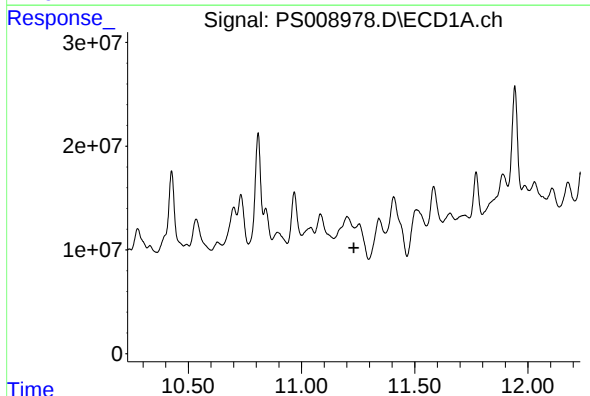


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

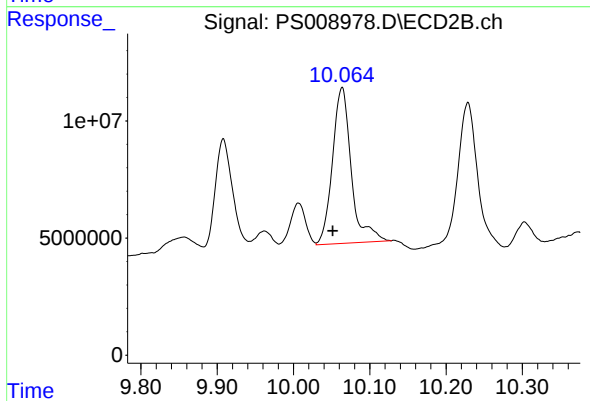

#14 DINOSEB


R.T.: 10.063 min
Delta R.T.: 0.012 min
Response: 114135776
Conc: 28.87 ng/ml

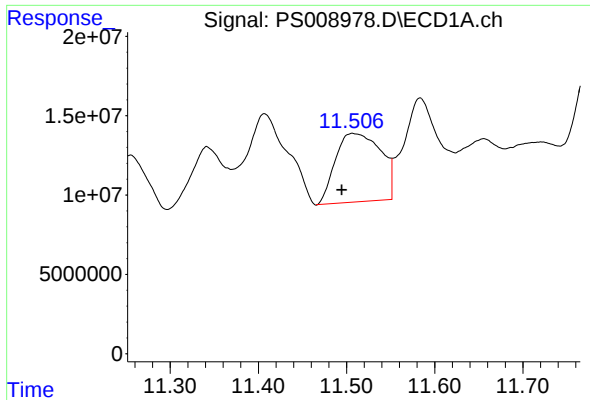

#16 DCPA

R.T.: 11.508 min
Delta R.T.: 0.013 min
Response: 154454681
Conc: 11.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
DUNR-TS007-01

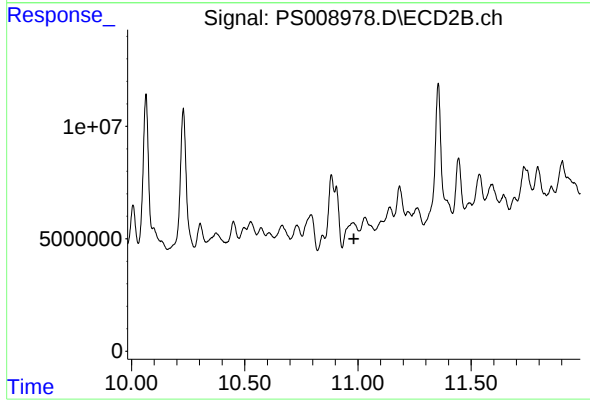

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.982 min
Response: 0
Conc: N.D.