

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2020 23:25
 Operator : DD\AJ
 Sample : L1635-11
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LIED-TS001-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:00:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	574.0E6	253.7E6	262.517	263.336
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	108.1E6	N.D.	74.057
5) T	DICAMBA	7.374	0.000	124.0E6	0	15.264	N.D. #
7) T	MCPA	7.740	7.407	119.4E6	101.8E6	14.841	23.014 #
8) T	DICHLORPROP	0.000	7.691	0	54650097	N.D.	54.545
12) T	2,4,5-T	9.456	0.000	79585466	0	7.443	N.D. #
14) T	DINOSEB	0.000	10.066	0	65008619	N.D.	16.441
16) T	DCPA	11.518	0.000	122.3E6	0	8.902	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2020 23:25
Operator : DD\AJ
Sample : L1635-11
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
LIED-TS001-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:00:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

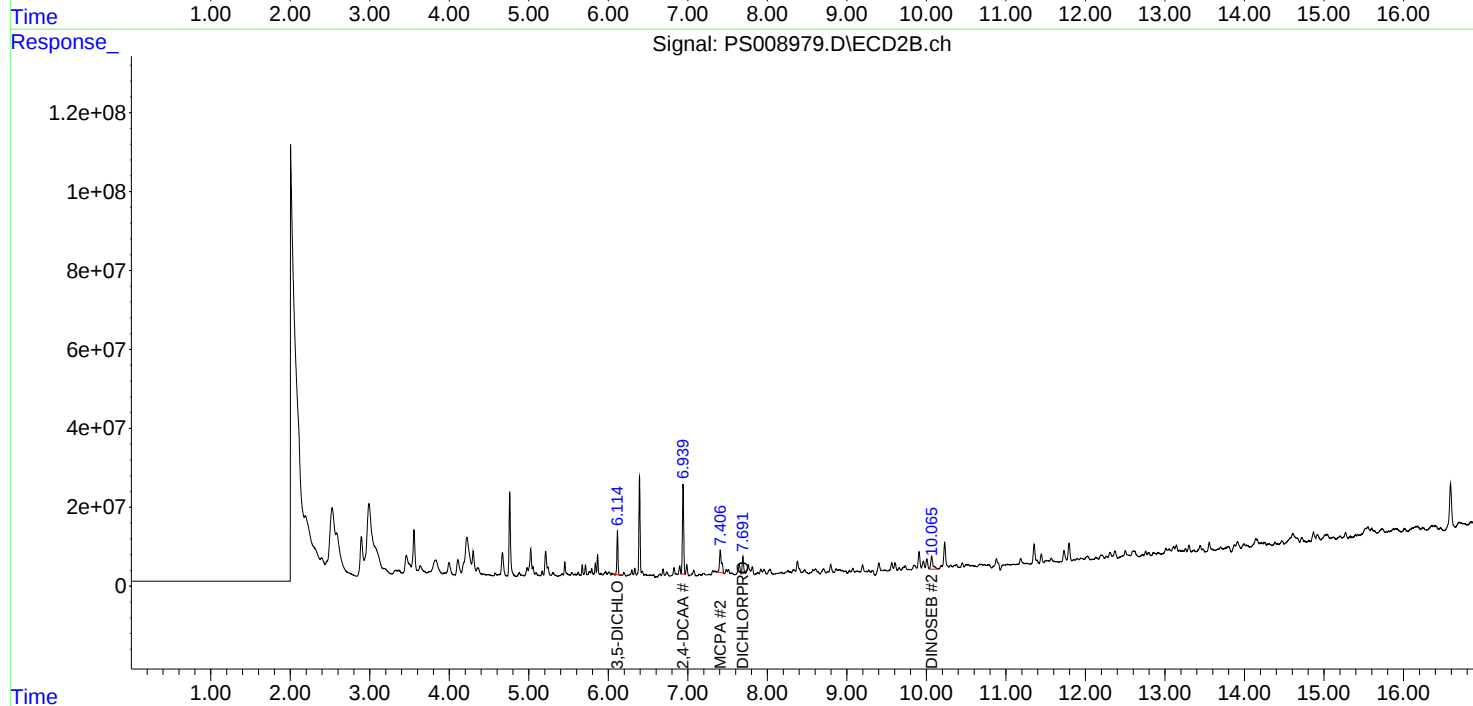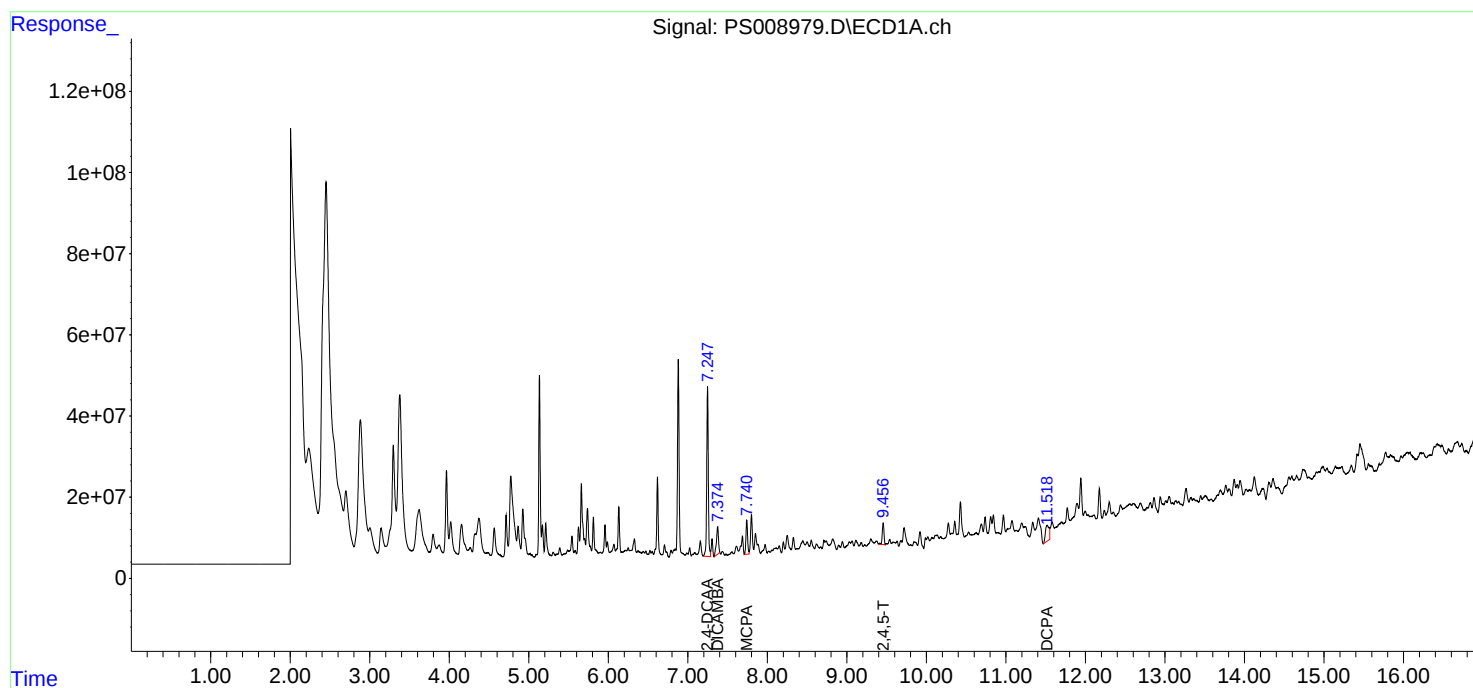


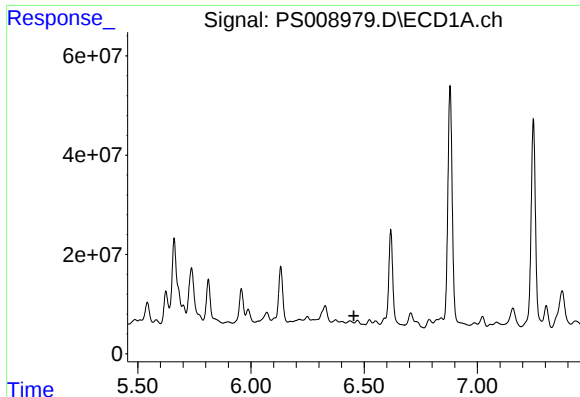

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS001-01

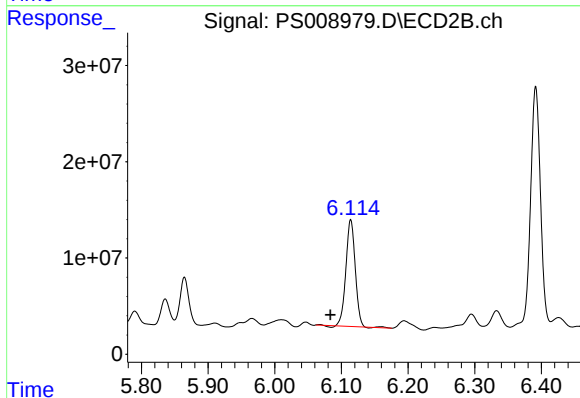


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 108068695
Conc: 74.06 ng/ml

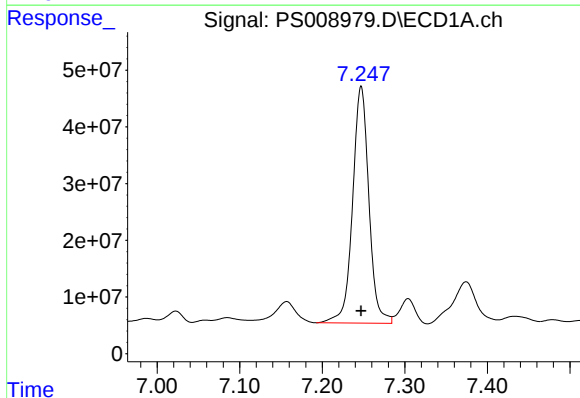


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 574017283
Conc: 262.52 ng/ml

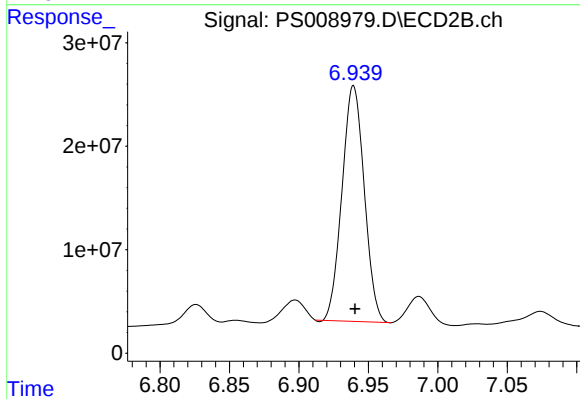

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 253739309
Conc: 263.34 ng/ml

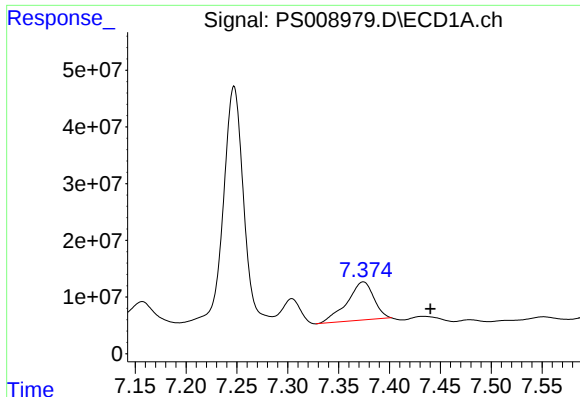

#5 DICAMBA


R.T.: 7.374 min
Delta R.T.: -0.066 min
Response: 124001910
Conc: 15.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
LIED-TS001-01

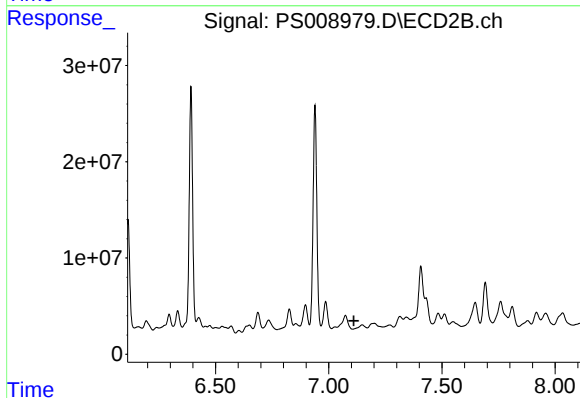


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.111 min
Response: 0
Conc: N.D.

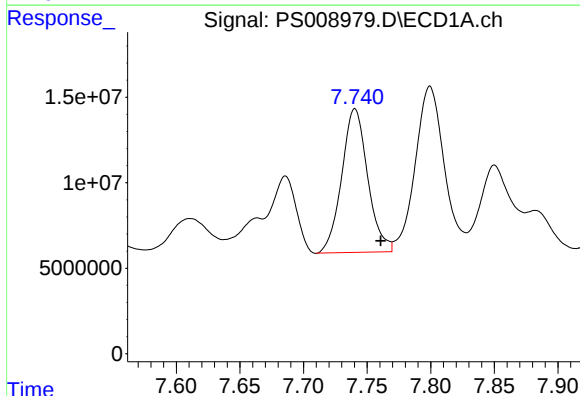


#7 MCPA

R.T.: 7.740 min
Delta R.T.: -0.020 min
Response: 119382705
Conc: 14.84 ug/ml

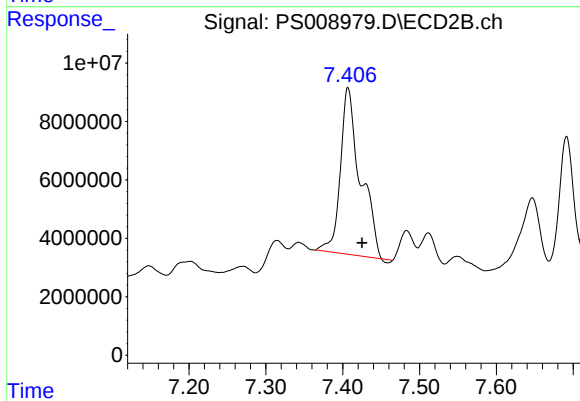

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 101818203
Conc: 23.01 ug/ml

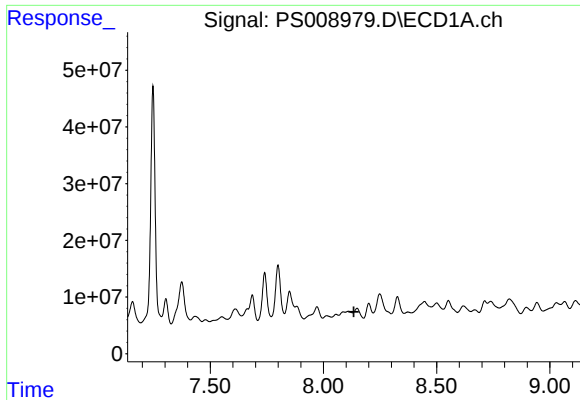

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS001-01

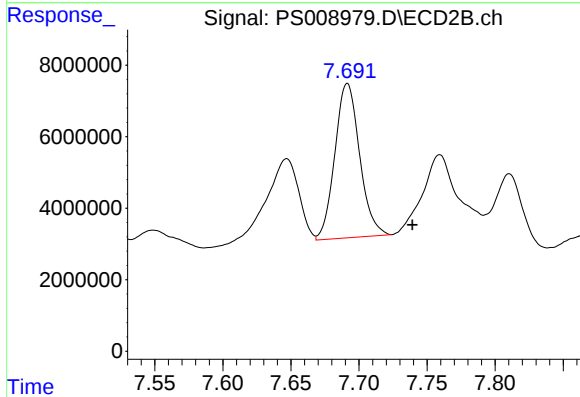


#8 DICHLORPROP

R.T.: 7.691 min
Delta R.T.: -0.048 min
Response: 54650097
Conc: 54.54 ng/ml

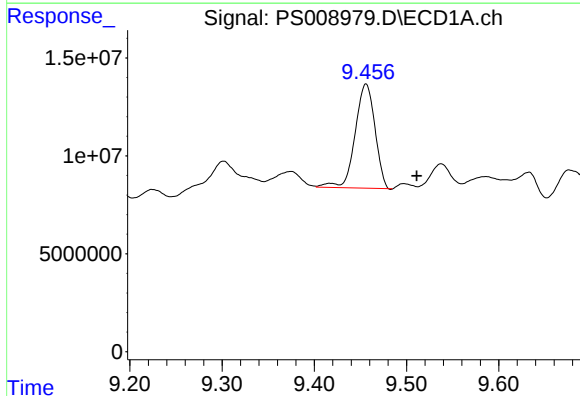


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.055 min
Response: 79585466
Conc: 7.44 ng/ml

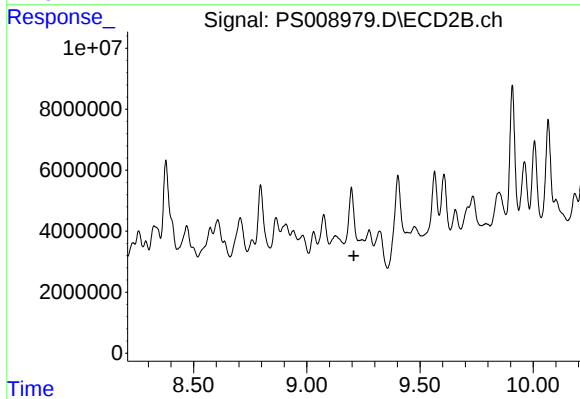

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

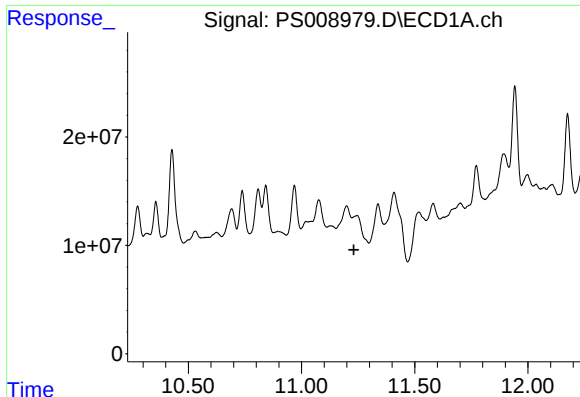

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS001-01

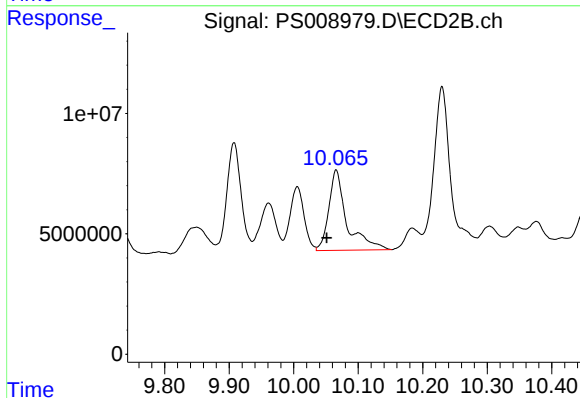


#14 DINOSEB

R.T.: 10.066 min
Delta R.T.: 0.014 min
Response: 65008619
Conc: 16.44 ng/ml

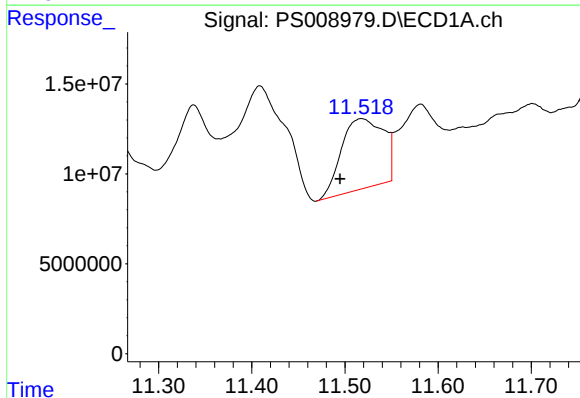

#16 DCPA

R.T.: 11.518 min
Delta R.T.: 0.023 min
Response: 122316521
Conc: 8.90 ng/ml

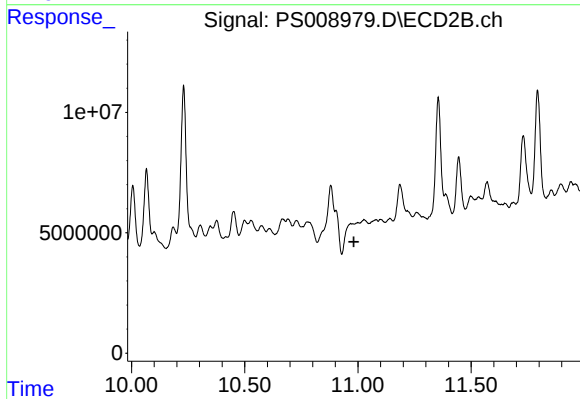

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.982 min
Response: 0
Conc: N.D.