

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 00:33
 Operator : DD\AJ
 Sample : L1635-14
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:01:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	689.6E6	314.8E6	315.385	326.747
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	146.4E6	N.D.	100.291
5) T	DICAMBA	7.372	0.000	99597575	0	12.260	N.D. #
7) T	MCPA	7.740	7.407	55038988	106.5E6	6.842	24.071 #
11) T	2,4,5-TP ...	0.000	8.790	0	67304364	N.D.	12.425
12) T	2,4,5-T	9.454	0.000	106.1E6	0	9.922	N.D. #
14) T	DINOSEB	0.000	10.061	0	64083949	N.D.	16.207
16) T	DCPA	11.511	0.000	109.6E6	0	7.980	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 00:33
Operator : DD\AJ
Sample : L1635-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:01:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

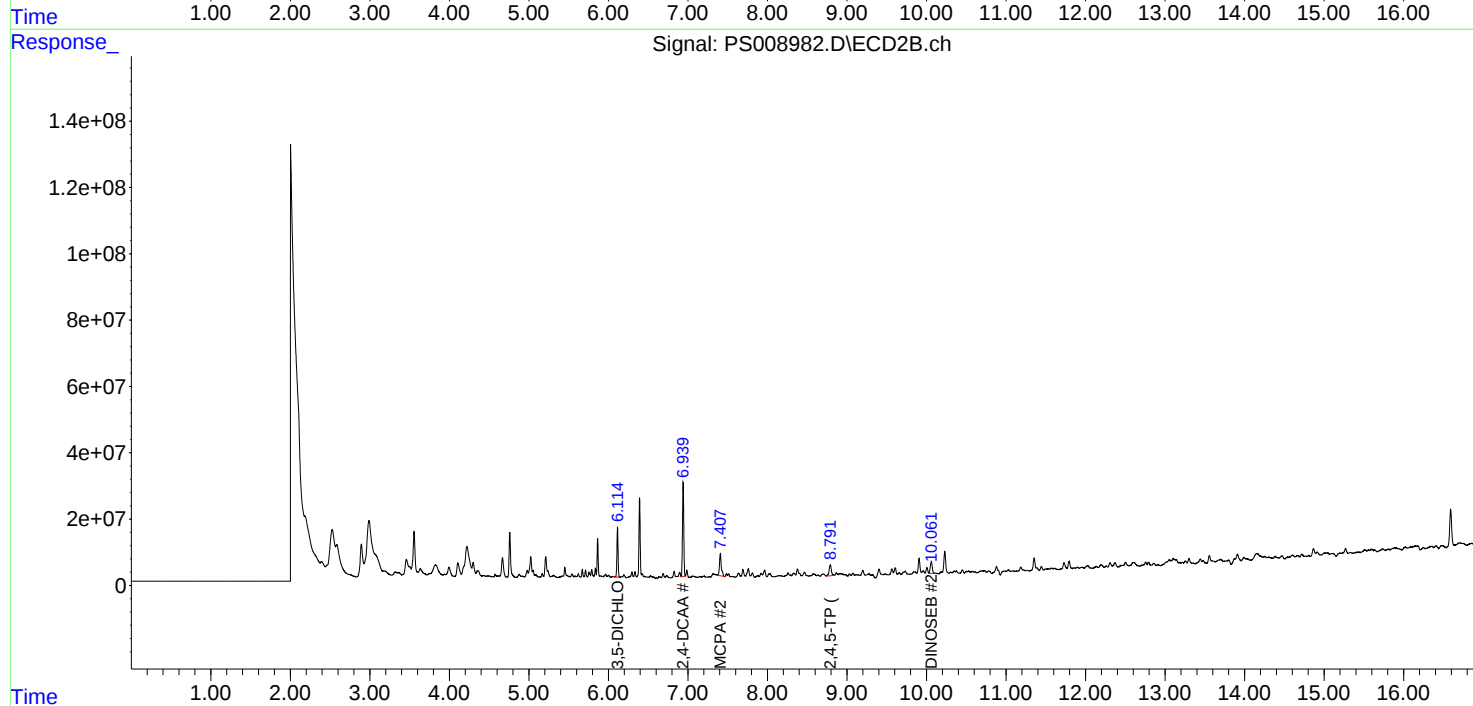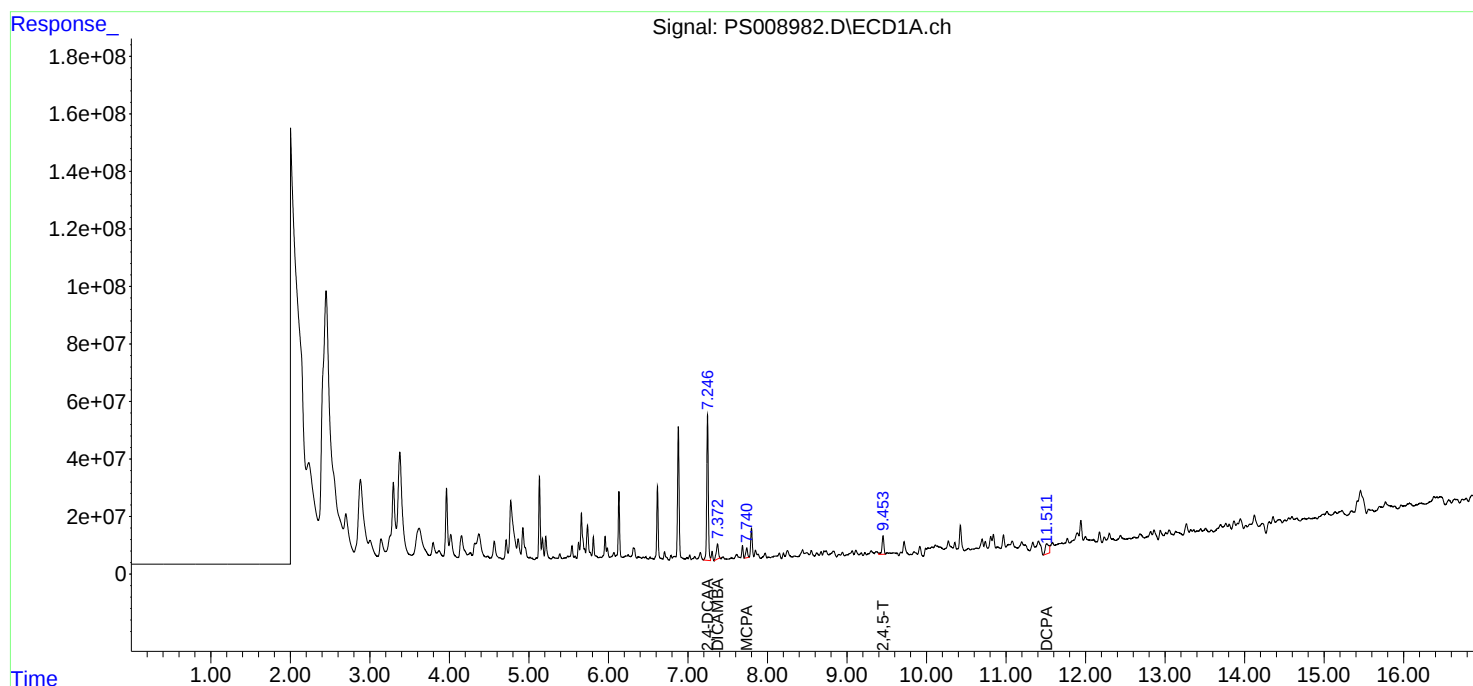


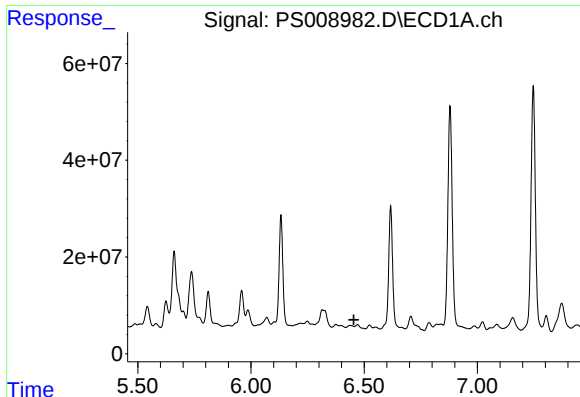

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

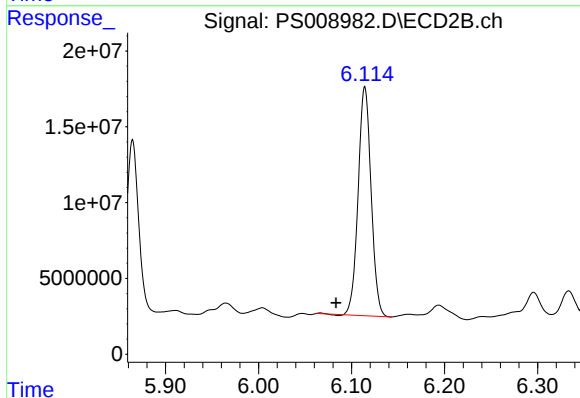


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 146351796
Conc: 100.29 ng/ml

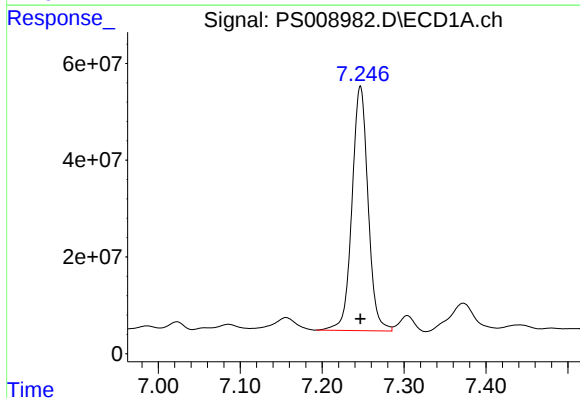


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 689618664
Conc: 315.39 ng/ml

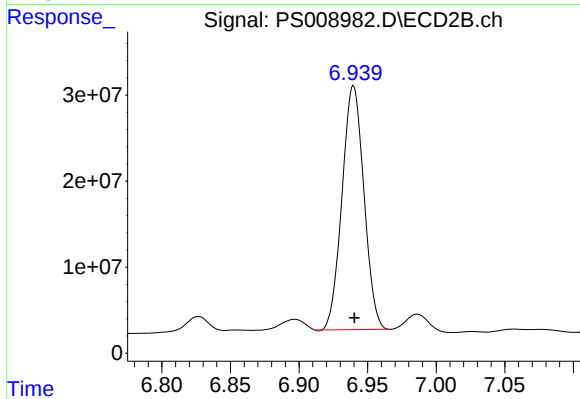

#4 2,4-DCAA


R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 314838846
Conc: 326.75 ng/ml

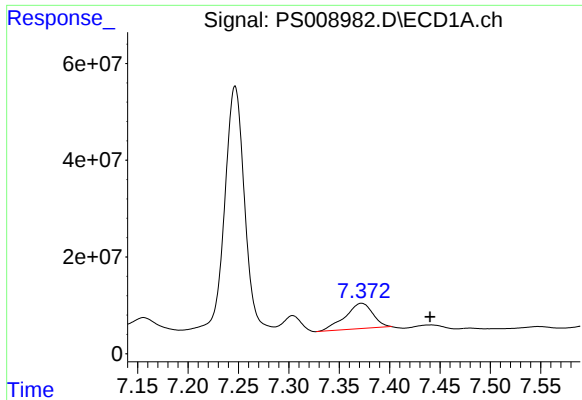

#5 DICAMBA


R.T.: 7.372 min
Delta R.T.: -0.068 min
Response: 99597575
Conc: 12.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

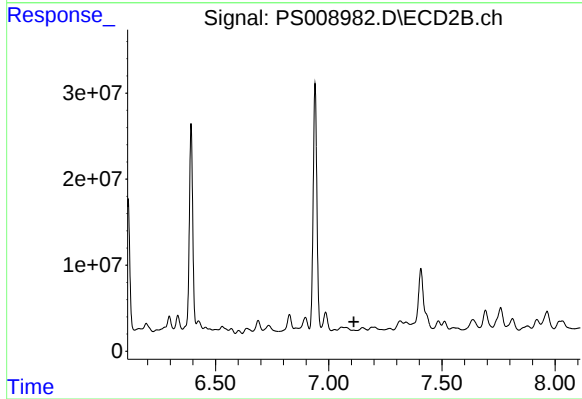


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.111 min
Response: 0
Conc: N.D.

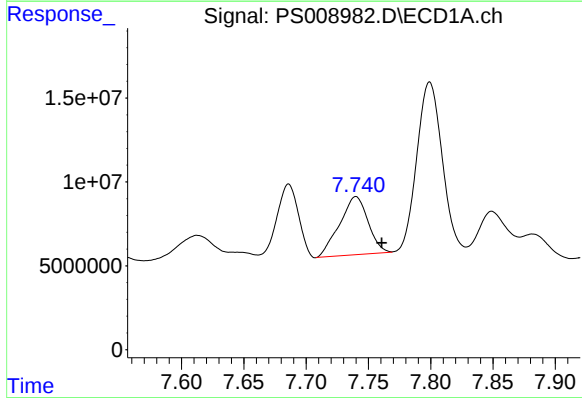


#7 MCPA

R.T.: 7.740 min
Delta R.T.: -0.021 min
Response: 55038988
Conc: 6.84 ug/ml

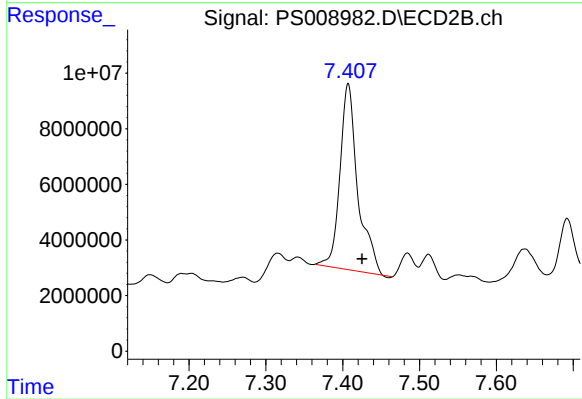

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 106496192
Conc: 24.07 ug/ml

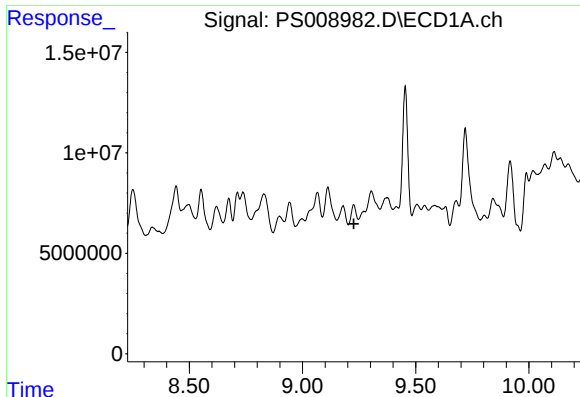

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

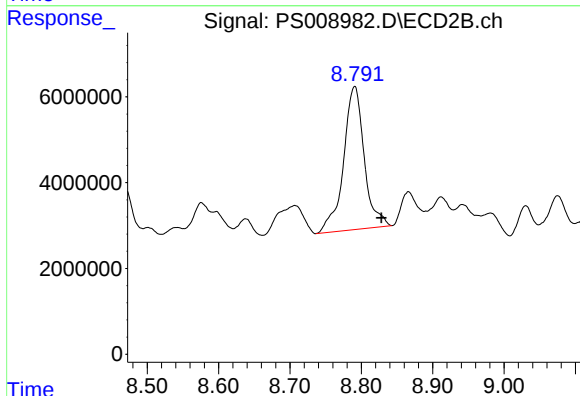


#11 2,4,5-TP (SILVEX)

R.T.: 8.790 min
Delta R.T.: -0.038 min
Response: 67304364
Conc: 12.42 ng/ml

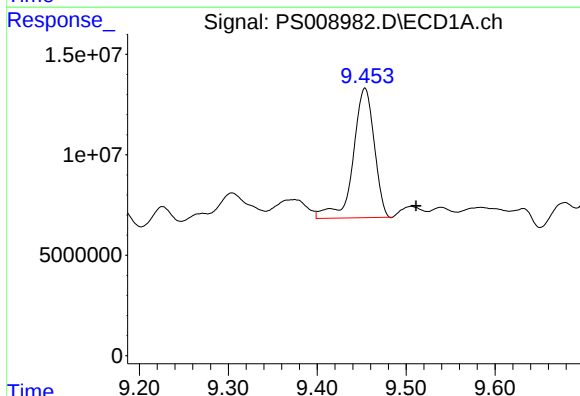


#12 2,4,5-T

R.T.: 9.454 min
Delta R.T.: -0.058 min
Response: 106090909
Conc: 9.92 ng/ml

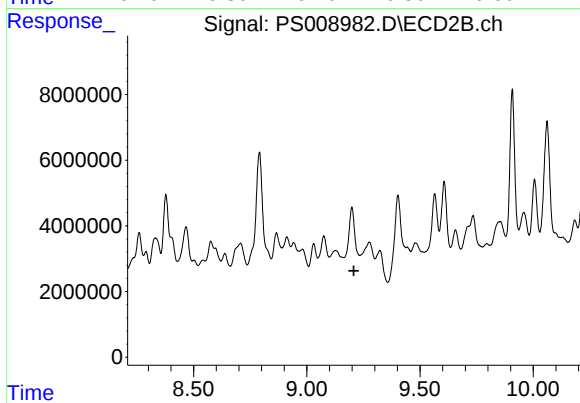

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

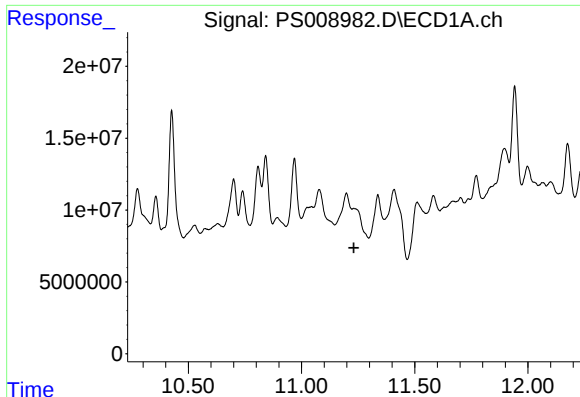

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

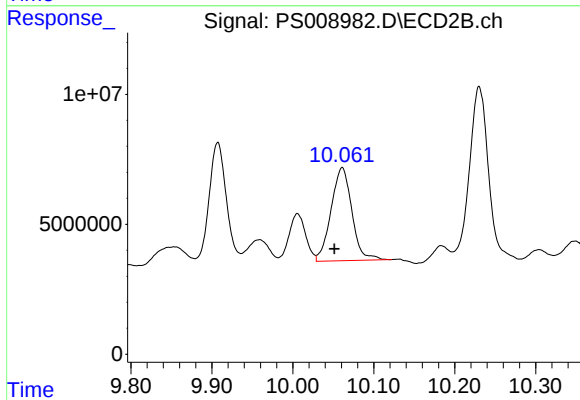


#14 DINOSEB

R.T.: 10.061 min
Delta R.T.: 0.009 min
Response: 64083949
Conc: 16.21 ng/ml

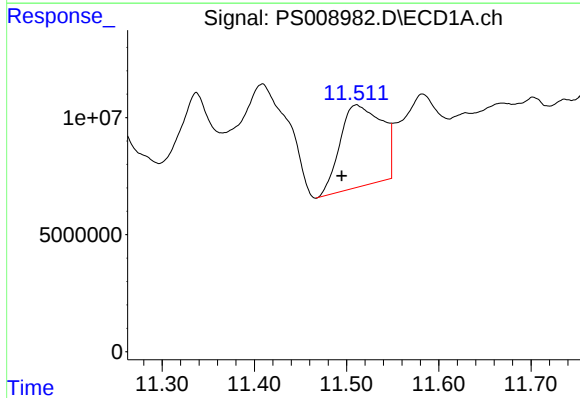

#16 DCPA

R.T.: 11.511 min
Delta R.T.: 0.016 min
Response: 109649775
Conc: 7.98 ng/ml

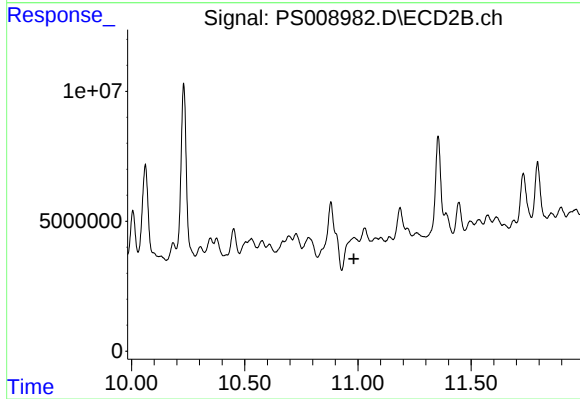

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.982 min
Response: 0
Conc: N.D.