

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS022420\  
 Data File : PS008983.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Feb 2020 00:56  
 Operator : DD\AJ  
 Sample : L1635-15  
 Misc :  
 ALS Vial : 25 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 25 04:01:56 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022020.M  
 Quant Title : 8080.M  
 QLast Update : Thu Feb 20 11:30:26 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|--------------|--------|--------|----------|----------|---------|----------|
| -----                       |              |        |        |          |          |         |          |
| System Monitoring Compounds |              |        |        |          |          |         |          |
| 4) S                        | 2,4-DCAA     | 7.247  | 6.939  | 752.6E6  | 333.3E6  | 344.190 | 345.930  |
| Target Compounds            |              |        |        |          |          |         |          |
| 2) T                        | 3,5-DICHL... | 0.000  | 6.114  | 0        | 148.6E6  | N.D.    | 101.828  |
| 5) T                        | DICAMBA      | 7.375  | 0.000  | 152.0E6  | 0        | 18.710  | N.D. #   |
| 7) T                        | MCPA         | 7.741  | 7.407  | 76265706 | 128.8E6  | 9.481   | 29.103 # |
| 11) T                       | 2,4,5-TP ... | 0.000  | 8.790  | 0        | 73500706 | N.D.    | 13.569   |
| 12) T                       | 2,4,5-T      | 9.453  | 0.000  | 152.8E6  | 0        | 14.287  | N.D. #   |
| 14) T                       | DINOSEB      | 0.000  | 10.062 | 0        | 71591903 | N.D.    | 18.106   |
| 15) T                       | Picloram     | 11.075 | 0.000  | 77738161 | 0        | 5.678   | N.D. #   |
| 16) T                       | DCPA         | 11.510 | 0.000  | 129.3E6  | 0        | 9.412   | N.D. #   |
| -----                       |              |        |        |          |          |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS022420\  
Data File : PS008983.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Feb 2020 00:56  
Operator : DD\AJ  
Sample : L1635-15  
Misc :  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 25 04:01:56 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022020.M  
Quant Title : 8080.M  
QLast Update : Thu Feb 20 11:30:26 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

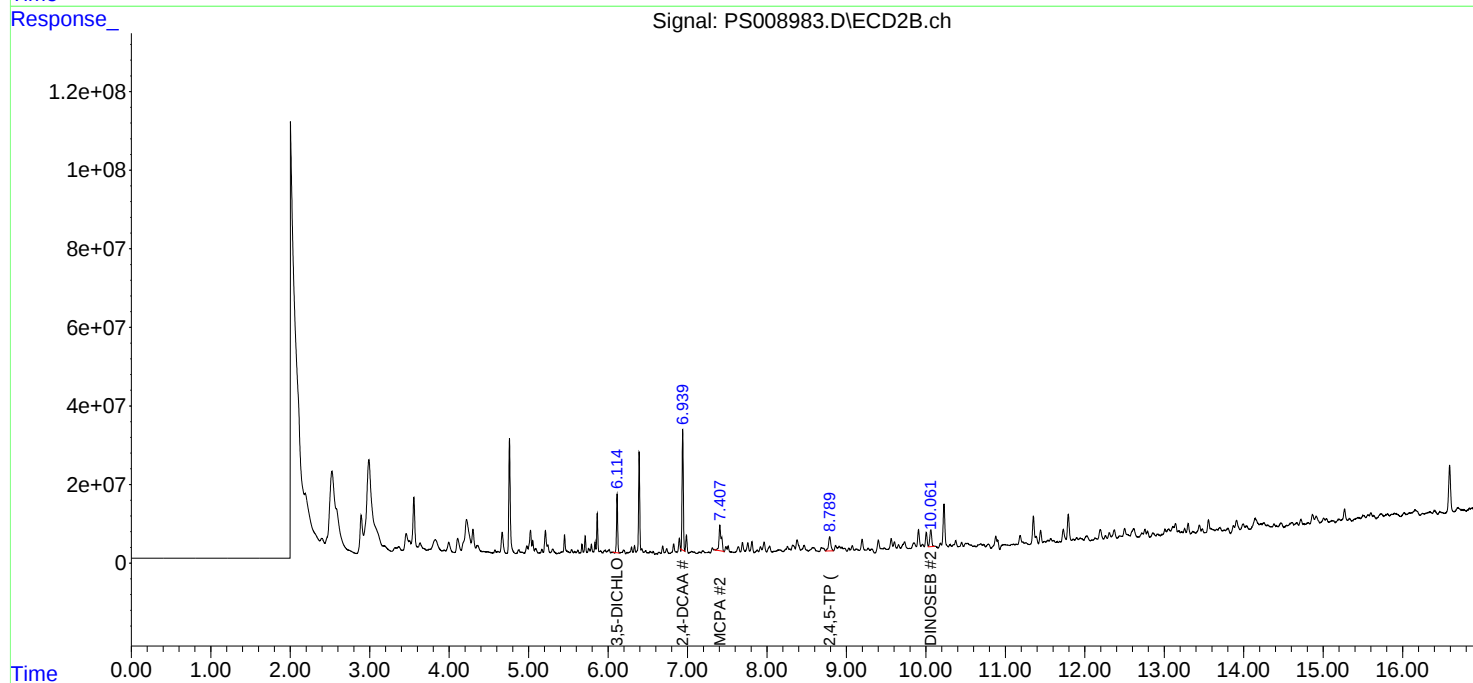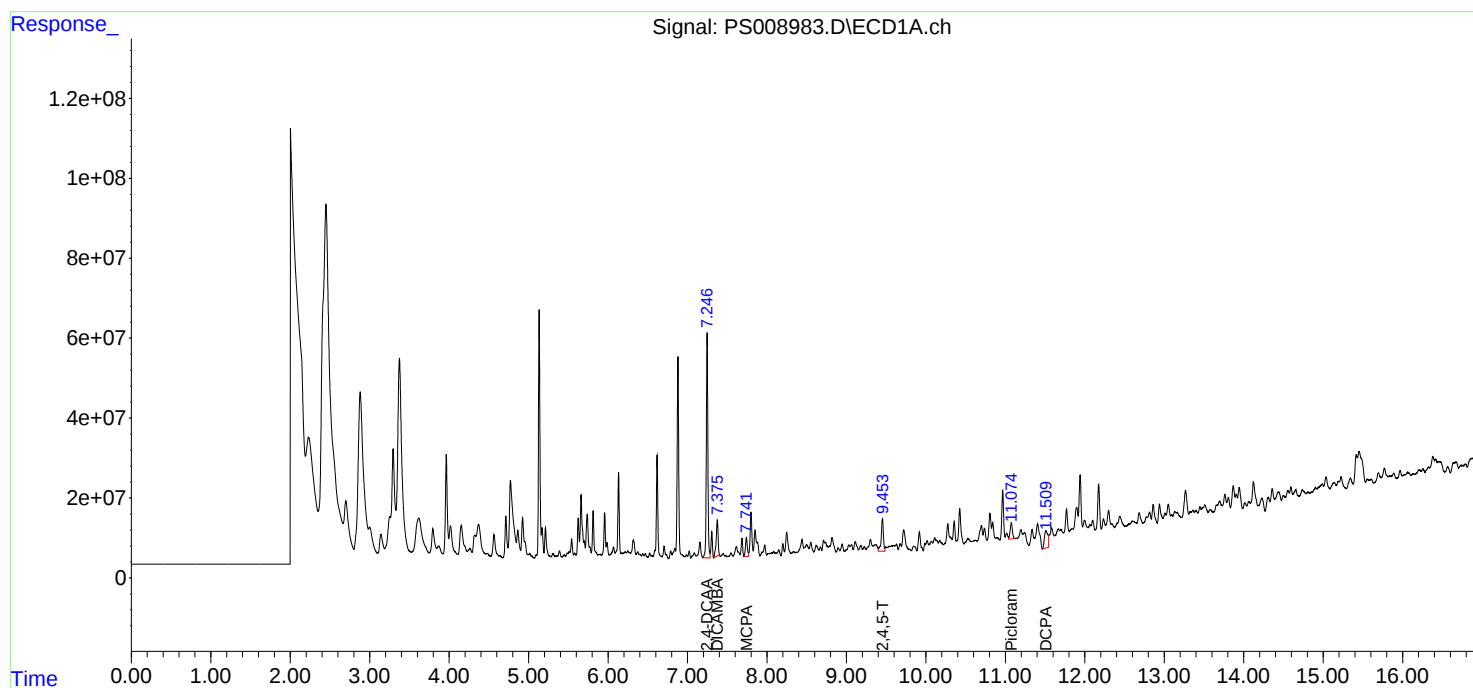


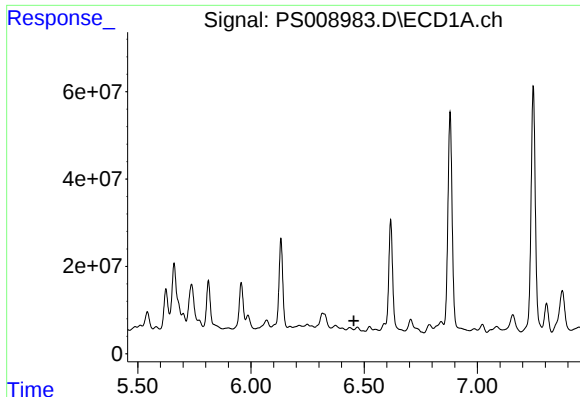

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min  
Exp R.T.: 6.455 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

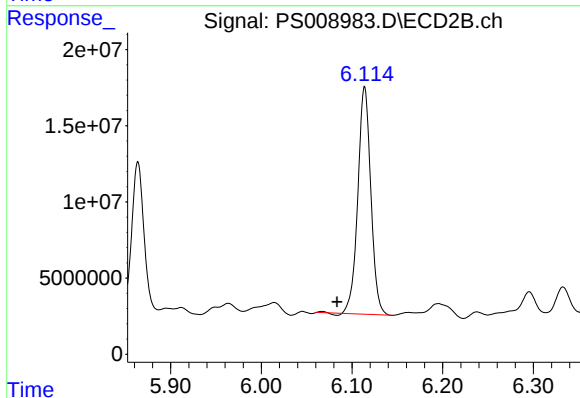


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min  
Delta R.T.: 0.031 min  
Response: 148595299  
Conc: 101.83 ng/ml

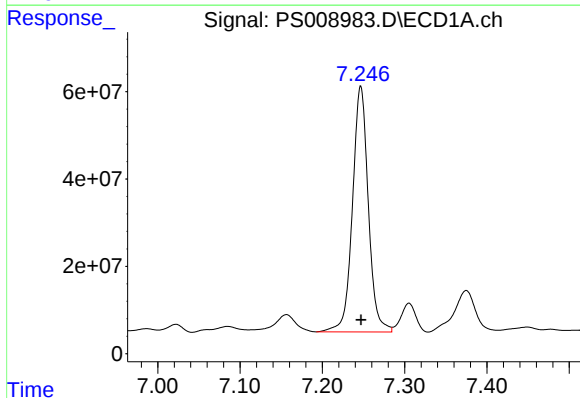


#4 2,4-DCAA

R.T.: 7.247 min  
Delta R.T.: 0.000 min  
Response: 752603668  
Conc: 344.19 ng/ml

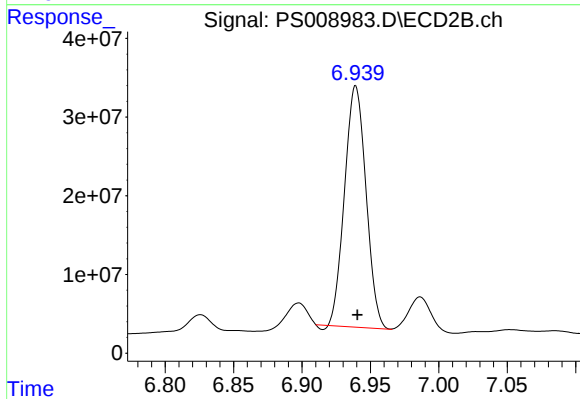

#4 2,4-DCAA


R.T.: 6.939 min  
Delta R.T.: -0.001 min  
Response: 333322535  
Conc: 345.93 ng/ml

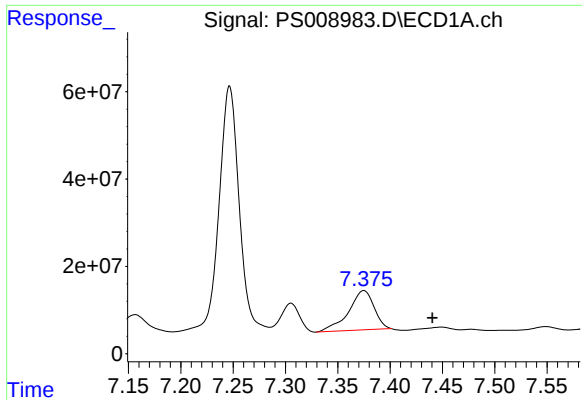

#5 DICAMBA


R.T.: 7.375 min  
Delta R.T.: -0.066 min  
Response: 151999432  
Conc: 18.71 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

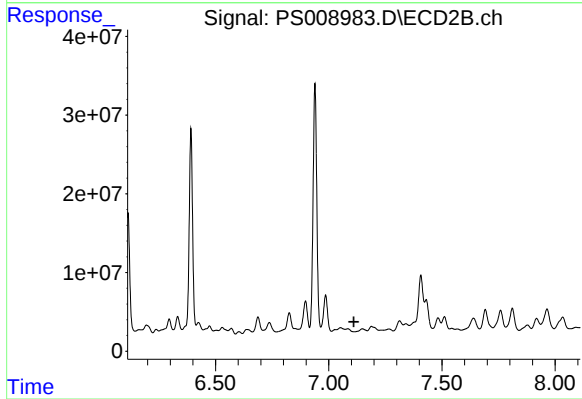


#5 DICAMBA

R.T.: 0.000 min  
Exp R.T. : 7.111 min  
Response: 0  
Conc: N.D.

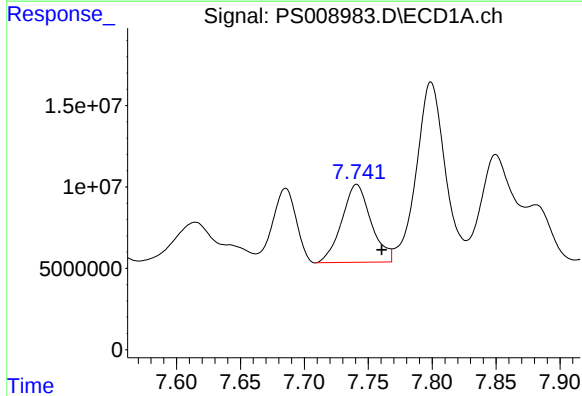


#7 MCPA

R.T.: 7.741 min  
Delta R.T.: -0.020 min  
Response: 76265706  
Conc: 9.48 ug/ml

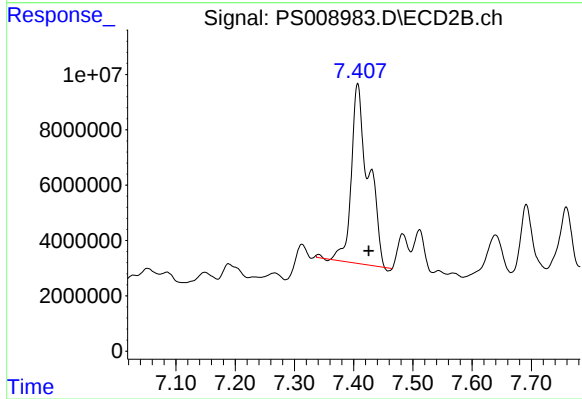

#7 MCPA


R.T.: 7.407 min  
Delta R.T.: -0.019 min  
Response: 128759040  
Conc: 29.10 ug/ml

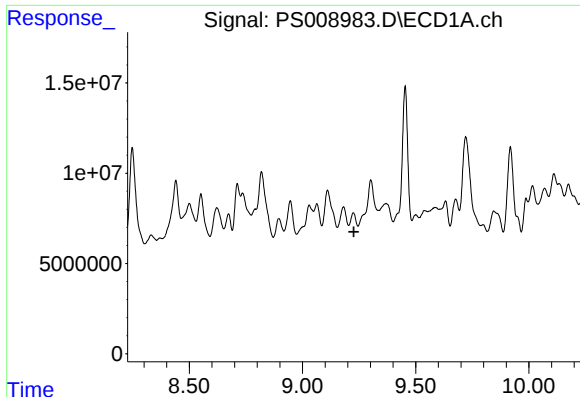

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min  
Exp R.T.: 9.227 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

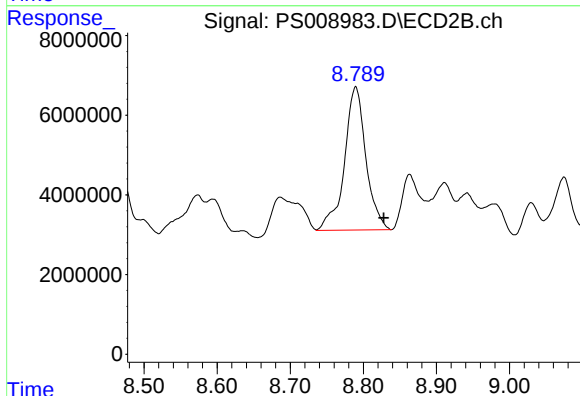


#11 2,4,5-TP (SILVEX)

R.T.: 8.790 min  
Delta R.T.: -0.038 min  
Response: 73500706  
Conc: 13.57 ng/ml

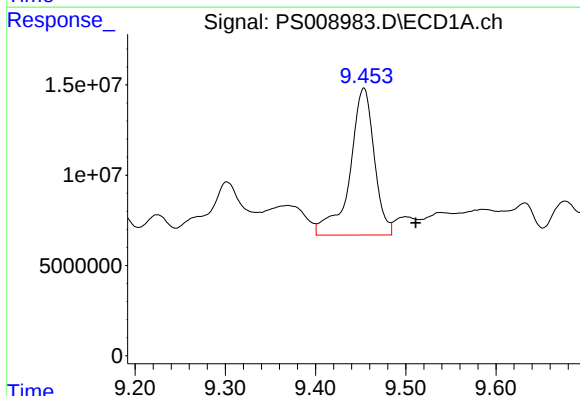


#12 2,4,5-T

R.T.: 9.453 min  
Delta R.T.: -0.058 min  
Response: 152757687  
Conc: 14.29 ng/ml

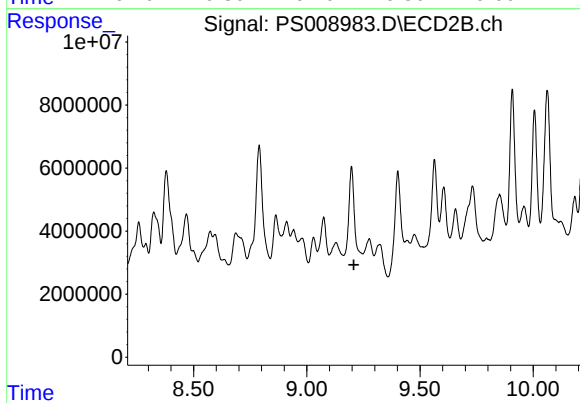

#12 2,4,5-T


R.T.: 0.000 min  
Exp R.T.: 9.208 min  
Response: 0  
Conc: N.D.

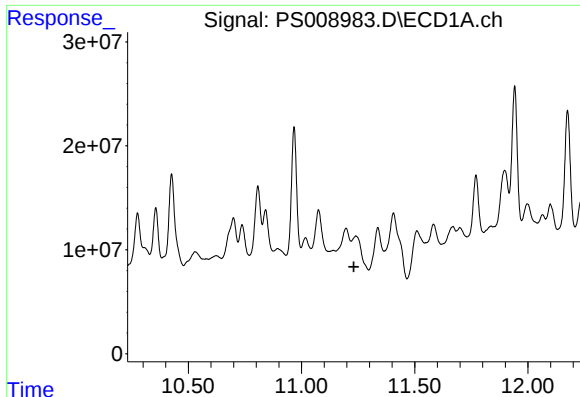

#14 DINOSEB


R.T.: 0.000 min  
Exp R.T.: 11.231 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

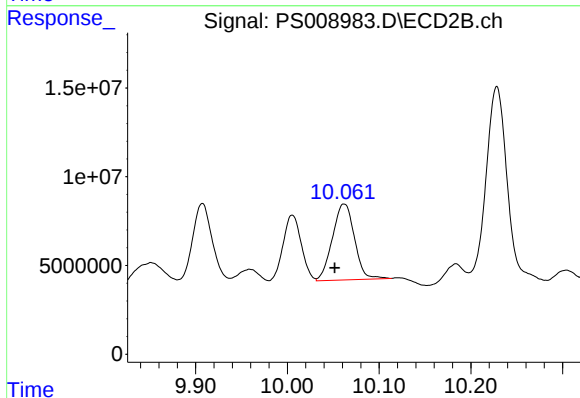


#14 DINOSEB

R.T.: 10.062 min  
Delta R.T.: 0.010 min  
Response: 71591903  
Conc: 18.11 ng/ml

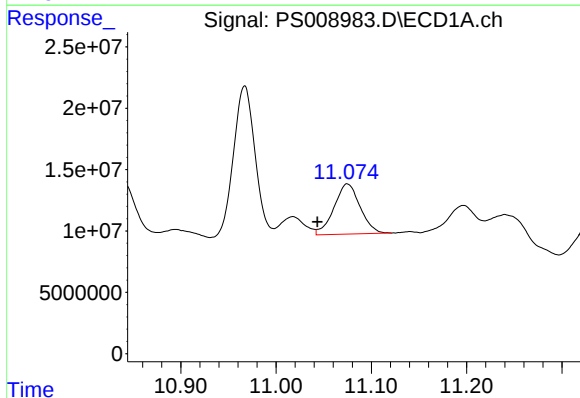


#15 Picloram

R.T.: 11.075 min  
Delta R.T.: 0.032 min  
Response: 77738161  
Conc: 5.68 ng/ml

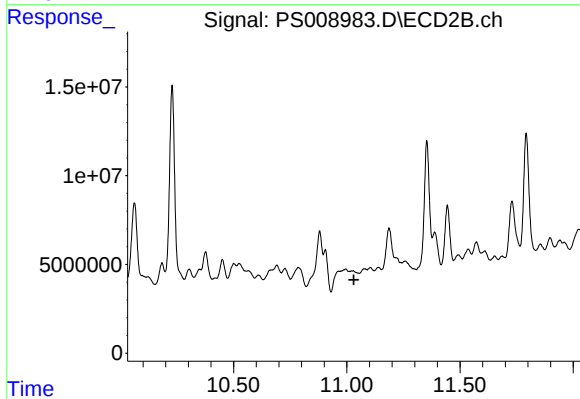

#15 Picloram


R.T.: 0.000 min  
Exp R.T.: 11.031 min  
Response: 0  
Conc: N.D.

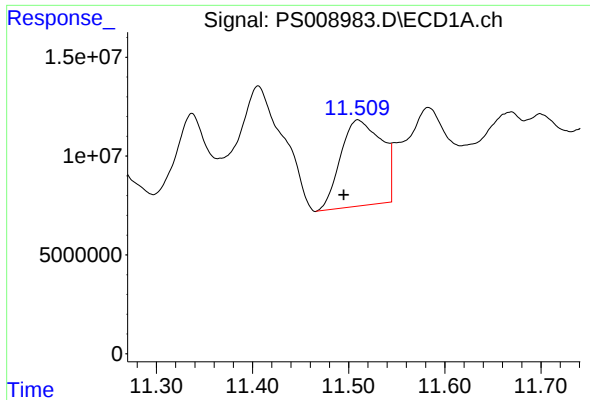

#16 DCPA

R.T.: 11.510 min  
Delta R.T.: 0.015 min  
Response: 129332362  
Conc: 9.41 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

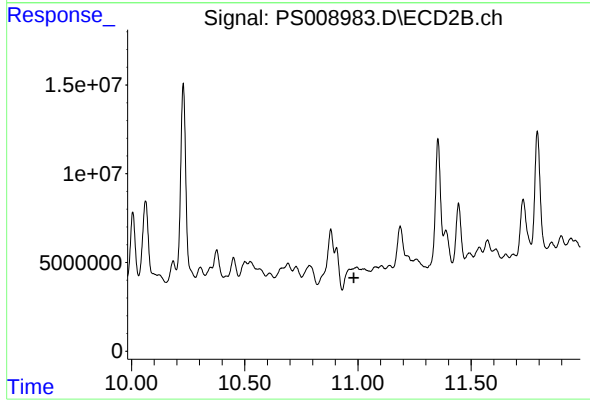

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 10.982 min  
Response: 0  
Conc: N.D.