

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 00:56
 Operator : DD\AJ
 Sample : L1635-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LIED-TS002-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:01:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	752.6E6	333.3E6	344.190	345.930
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	148.6E6	N.D.	101.828
5) T	DICAMBA	7.375	0.000	152.0E6	0	18.710	N.D. #
7) T	MCPA	7.741	7.407	76265706	128.8E6	9.481	29.103 #
11) T	2,4,5-TP ...	0.000	8.790	0	73500706	N.D.	13.569
12) T	2,4,5-T	9.453	0.000	152.8E6	0	14.287	N.D. #
14) T	DINOSEB	0.000	10.062	0	71591903	N.D.	18.106
15) T	Picloram	11.075	0.000	77738161	0	5.678	N.D. #
16) T	DCPA	11.510	0.000	129.3E6	0	9.412	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 00:56
Operator : DD\AJ
Sample : L1635-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
LIED-TS002-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:01:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

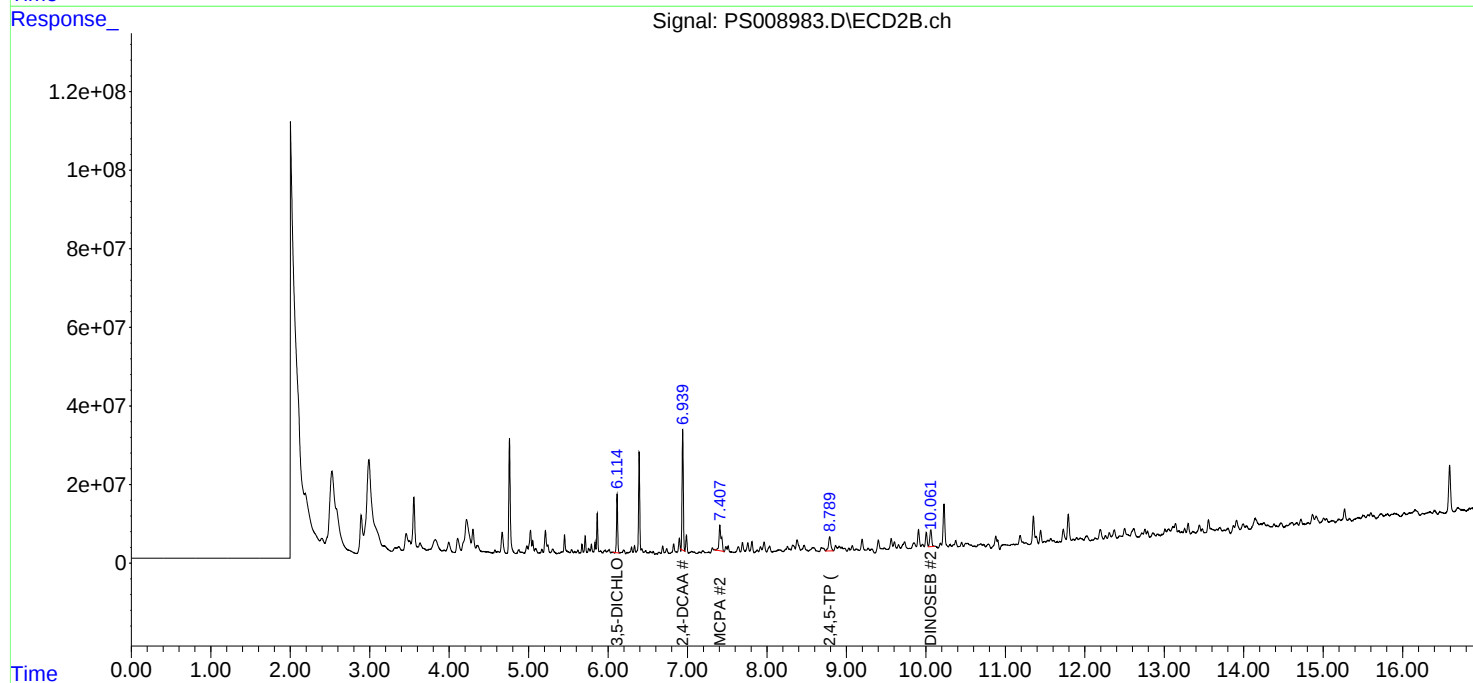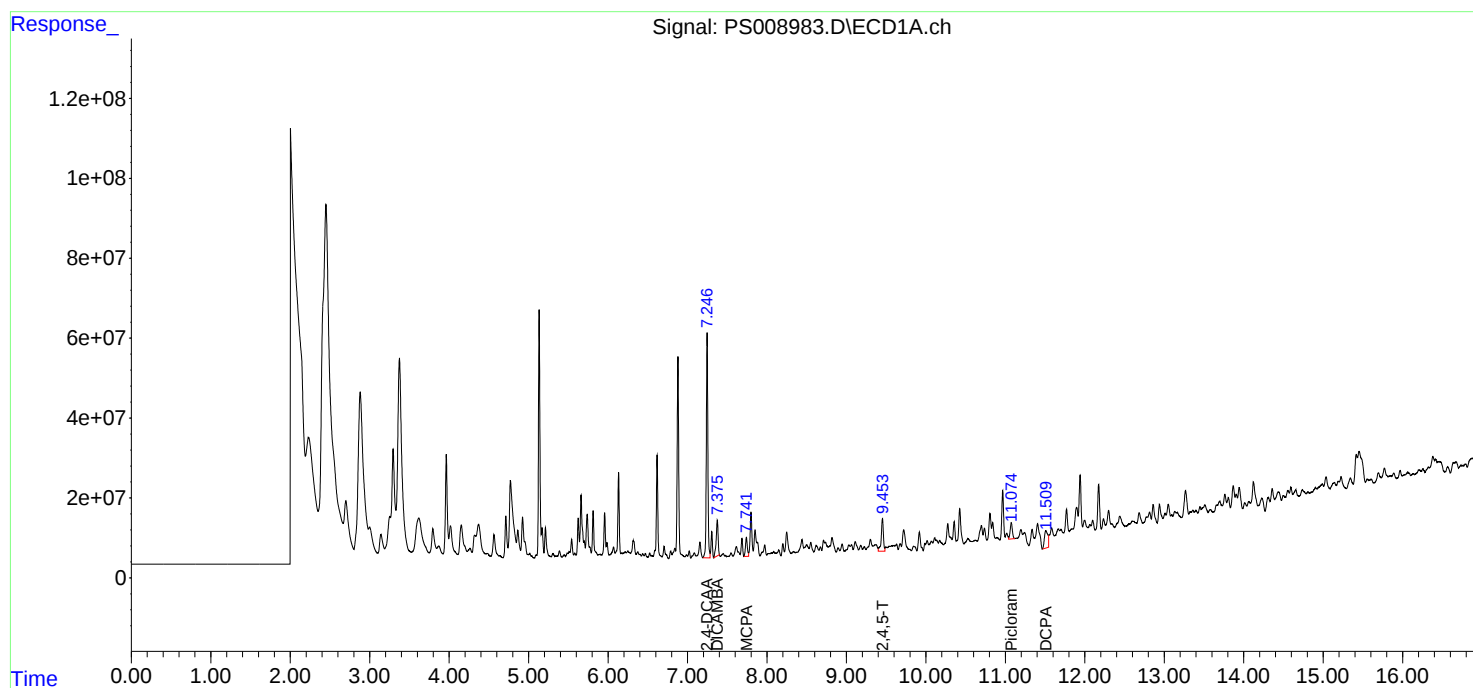


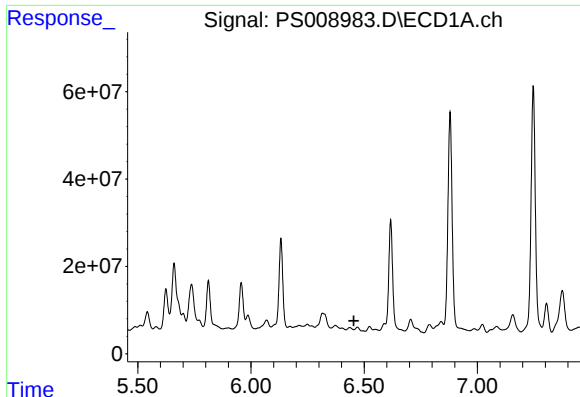

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS002-01

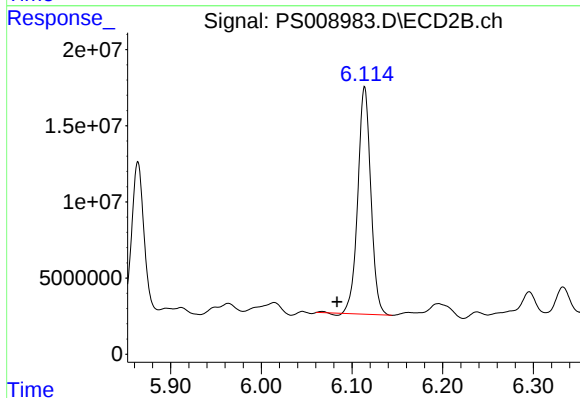


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 148595299
Conc: 101.83 ng/ml

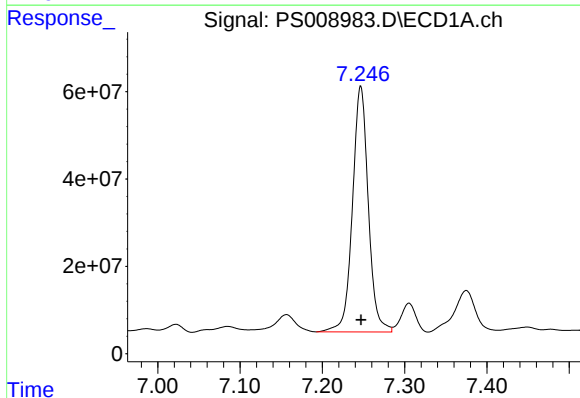


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 752603668
Conc: 344.19 ng/ml

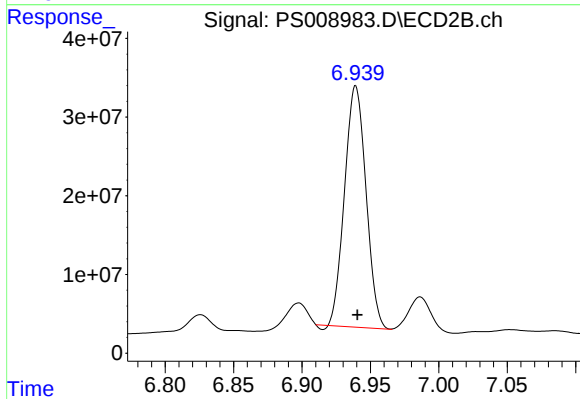

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 333322535
Conc: 345.93 ng/ml

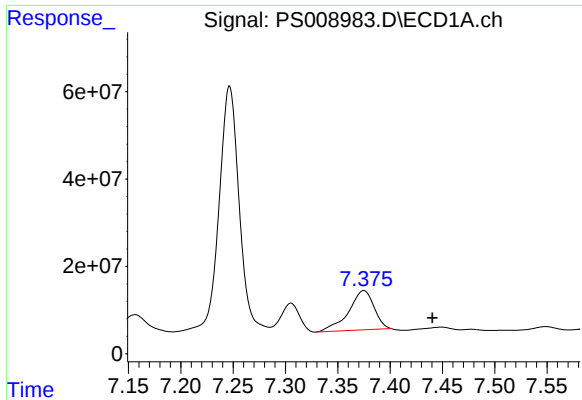

#5 DICAMBA


R.T.: 7.375 min
Delta R.T.: -0.066 min
Response: 151999432
Conc: 18.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
LIED-TS002-01

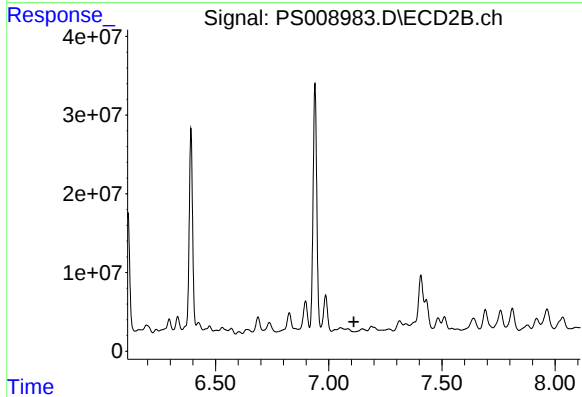


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.111 min
Response: 0
Conc: N.D.

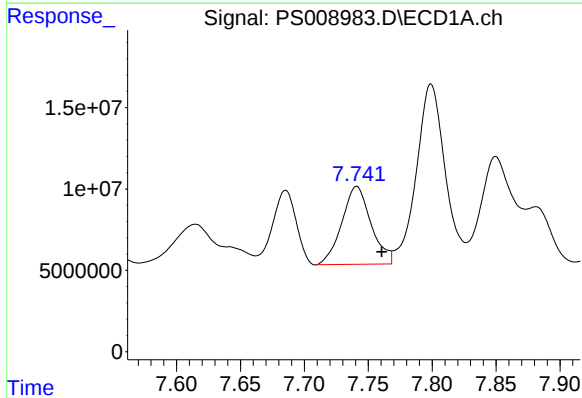


#7 MCPA

R.T.: 7.741 min
Delta R.T.: -0.020 min
Response: 76265706
Conc: 9.48 ug/ml

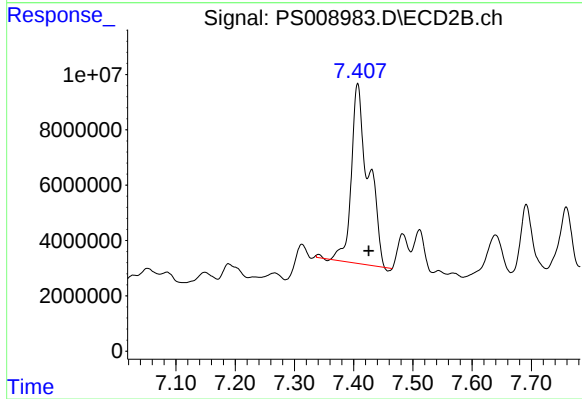

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 128759040
Conc: 29.10 ug/ml

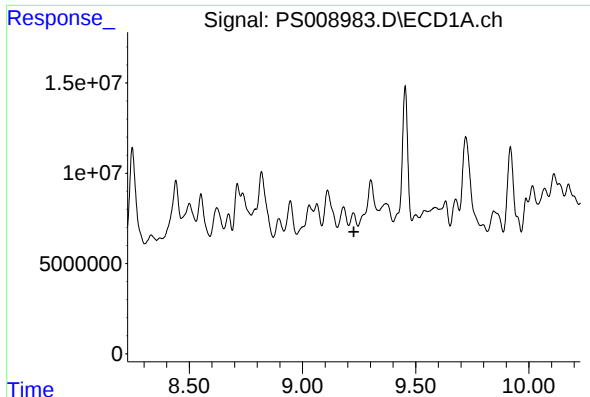

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS002-01

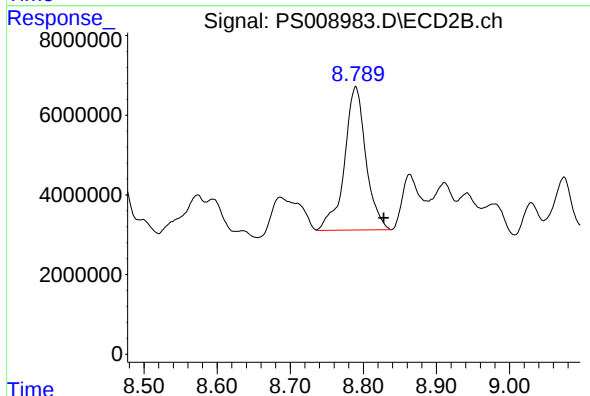


#11 2,4,5-TP (SILVEX)

R.T.: 8.790 min
Delta R.T.: -0.038 min
Response: 73500706
Conc: 13.57 ng/ml

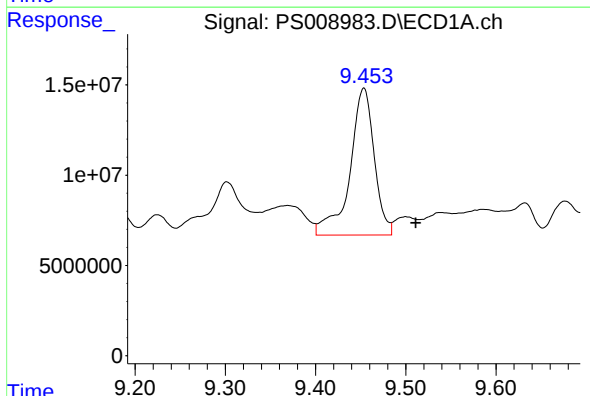


#12 2,4,5-T

R.T.: 9.453 min
Delta R.T.: -0.058 min
Response: 152757687
Conc: 14.29 ng/ml

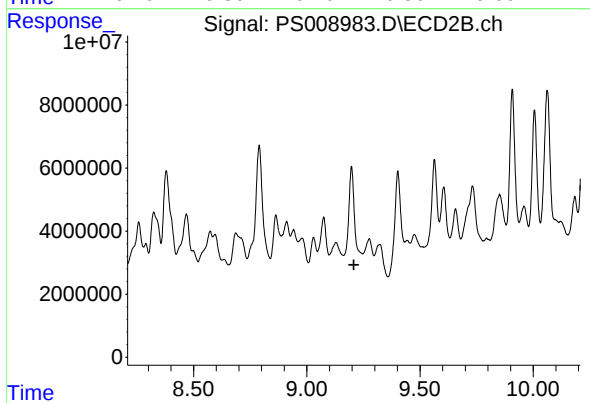

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

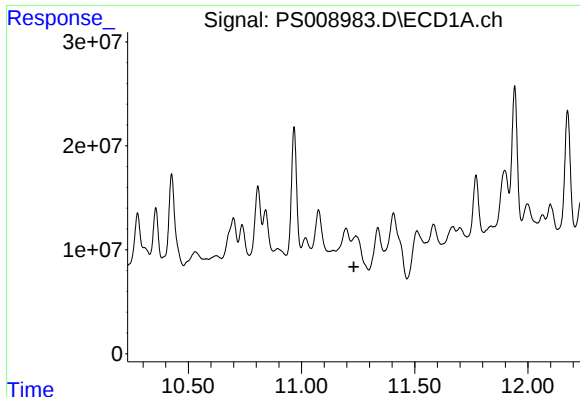

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS002-01

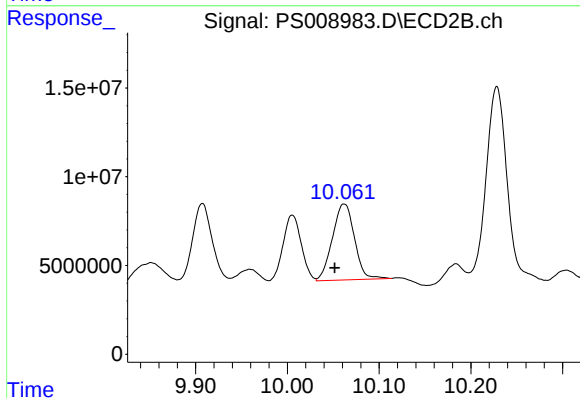


#14 DINOSEB

R.T.: 10.062 min
Delta R.T.: 0.010 min
Response: 71591903
Conc: 18.11 ng/ml

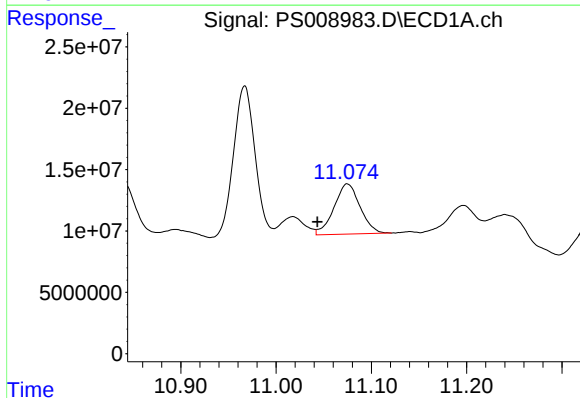


#15 Picloram

R.T.: 11.075 min
Delta R.T.: 0.032 min
Response: 77738161
Conc: 5.68 ng/ml

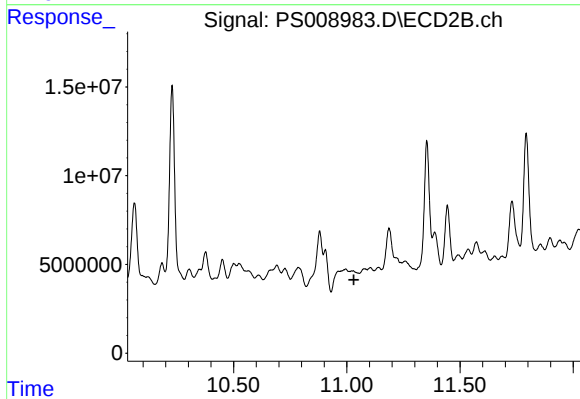

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.031 min
Response: 0
Conc: N.D.

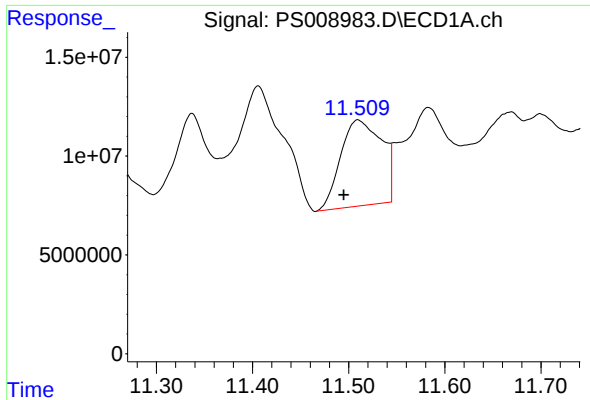

#16 DCPA

R.T.: 11.510 min
Delta R.T.: 0.015 min
Response: 129332362
Conc: 9.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
LIED-TS002-01

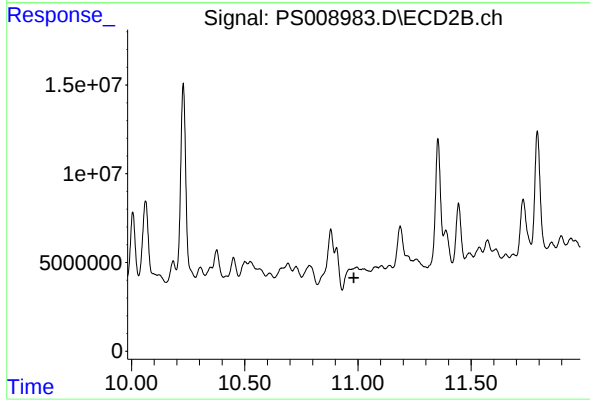

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.982 min
Response: 0
Conc: N.D.