

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 02:05
 Operator : DD\AJ
 Sample : L1635-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:02:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.939	395.5E6	149.9E6	180.862	155.584
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	128.2E6	N.D.	87.835
5) T	DICAMBA	7.374	0.000	132.9E6	0	16.354	N.D. #
7) T	MCPA	7.798	7.430	281.6E6	63757785	35.009	14.411 #
8) T	DICHLORPROP	0.000	7.758	0	62735088	N.D.	62.614
10) T	Pentachlo...	8.711	0.000	114.1E6	0	3.932	N.D. #
11) T	2,4,5-TP ...	0.000	8.783	0	77747783	N.D.	14.353
12) T	2,4,5-T	9.453	0.000	165.1E6	0	15.438	N.D. #
13) T	2,4-DB	10.068	0.000	103.6E6	0	71.774	N.D. #
14) T	DINOSEB	0.000	10.005	0	115.3E6	N.D.	29.159
16) T	DCPA	11.509	0.000	151.8E6	0	11.045	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 02:05
Operator : DD\AJ
Sample : L1635-18
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:02:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

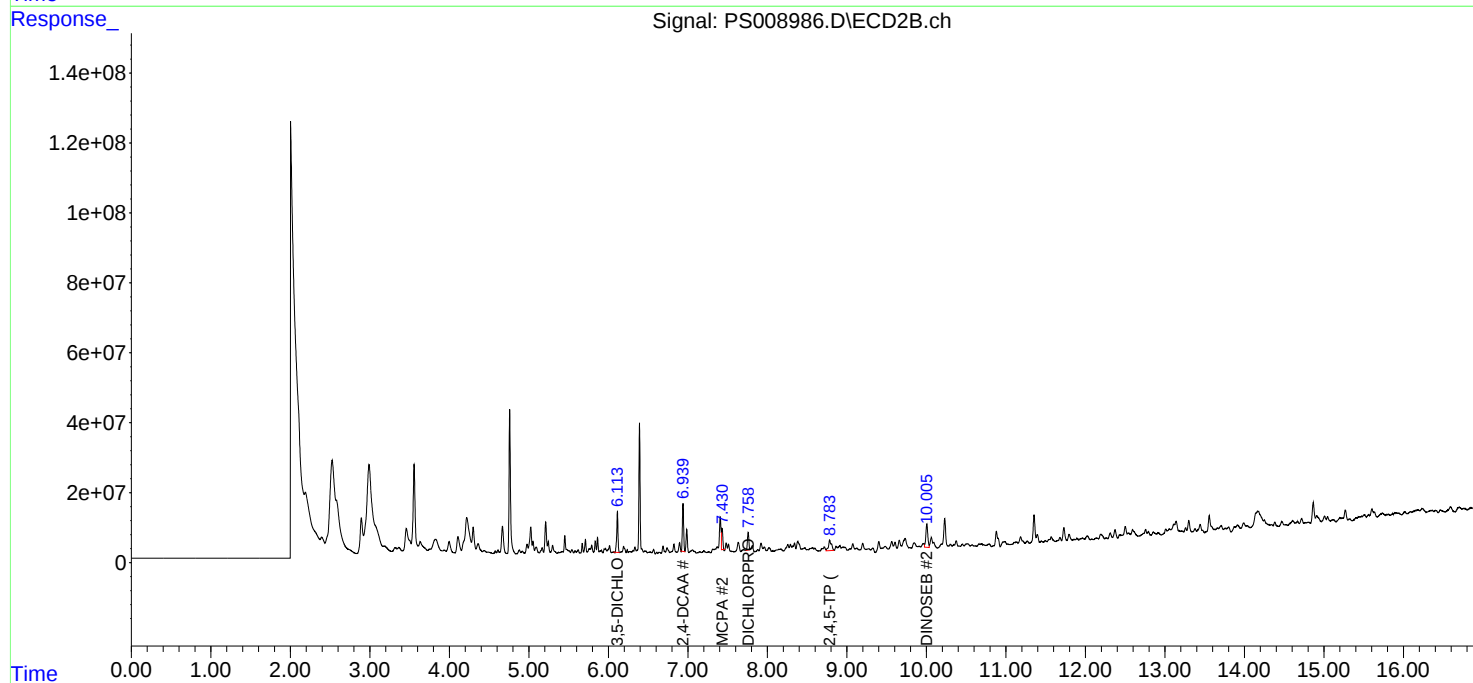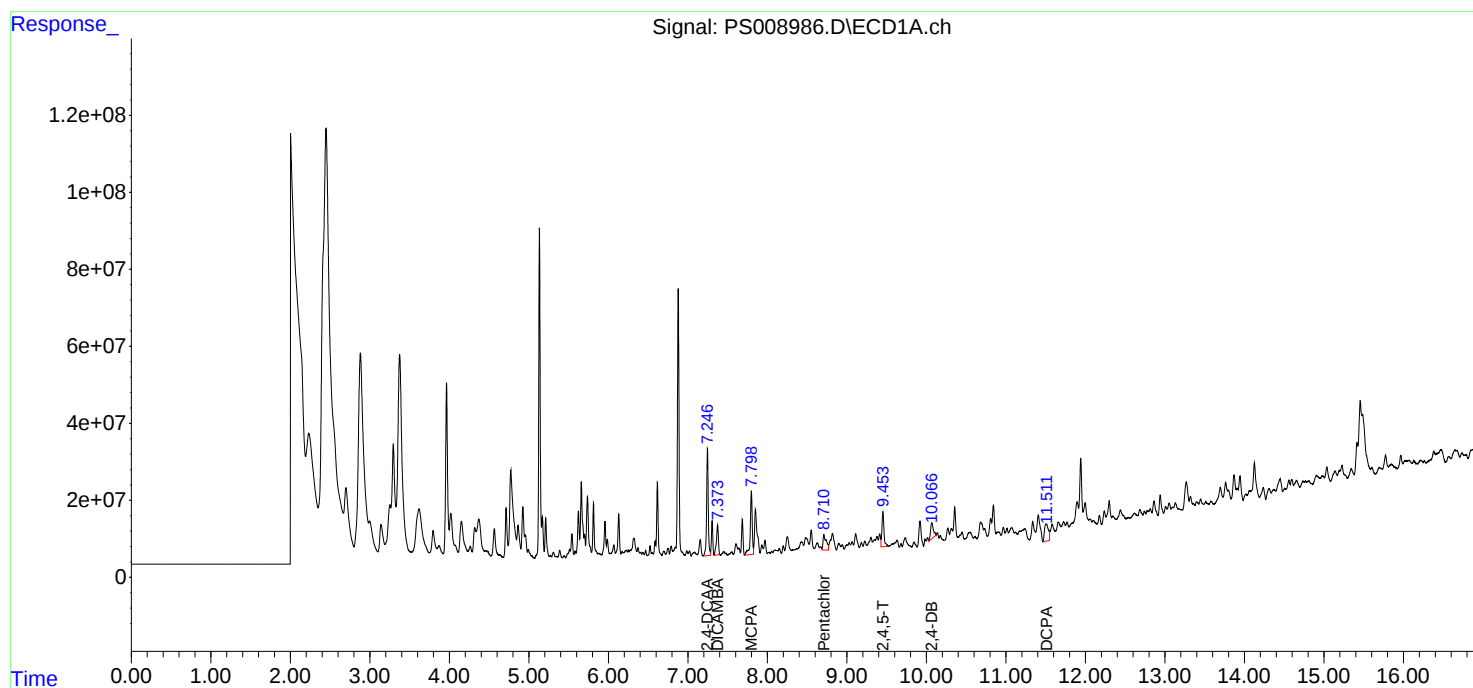


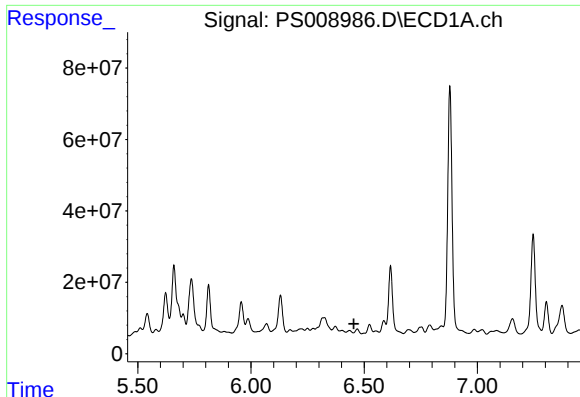

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

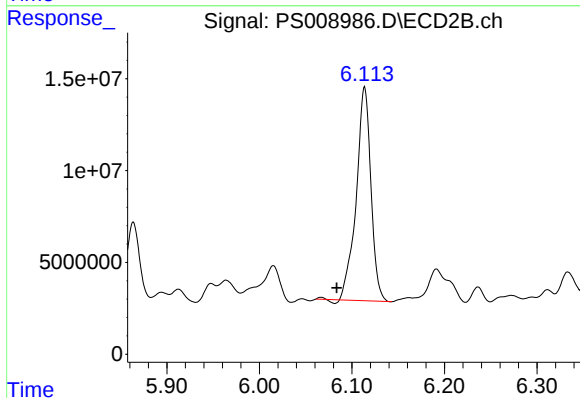


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 128174943
Conc: 87.83 ng/ml

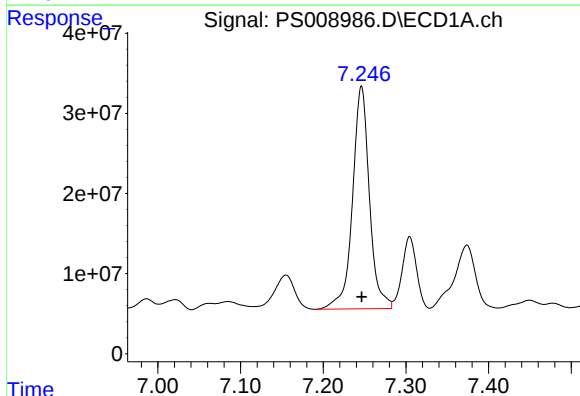


#4 2,4-DCAA

R.T.: 7.246 min
Delta R.T.: 0.000 min
Response: 395470995
Conc: 180.86 ng/ml

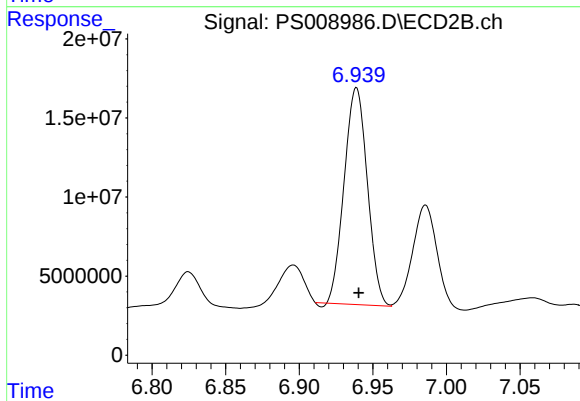

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 149914258
Conc: 155.58 ng/ml

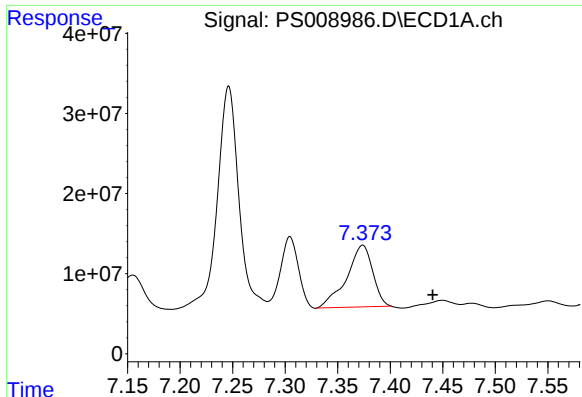

#5 DICAMBA


R.T.: 7.374 min
Delta R.T.: -0.067 min
Response: 132859411
Conc: 16.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

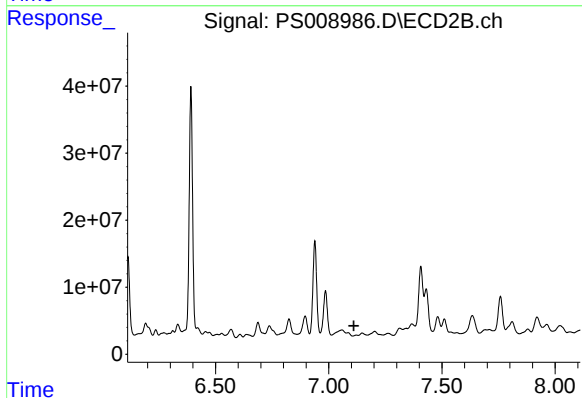


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.111 min
Response: 0
Conc: N.D.

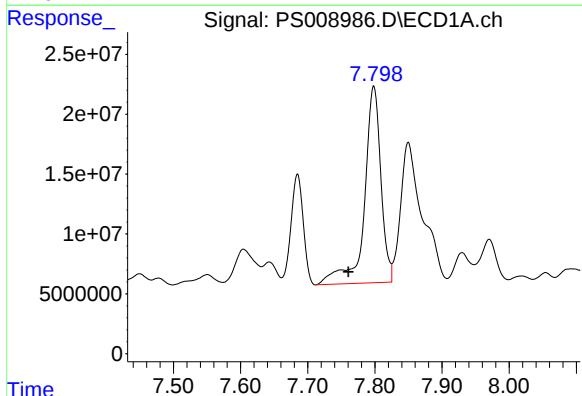


#7 MCPA

R.T.: 7.798 min
Delta R.T.: 0.038 min
Response: 281614282
Conc: 35.01 ug/ml

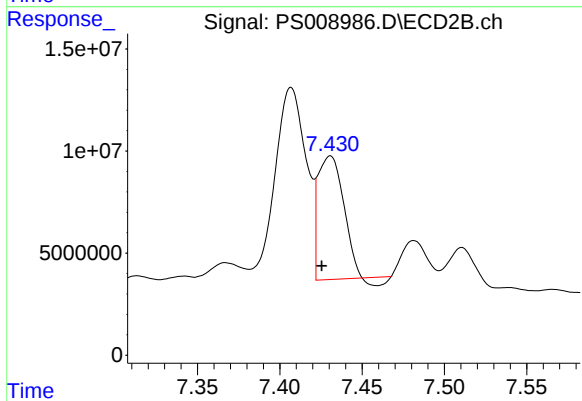

#7 MCPA


R.T.: 7.430 min
Delta R.T.: 0.005 min
Response: 63757785
Conc: 14.41 ug/ml

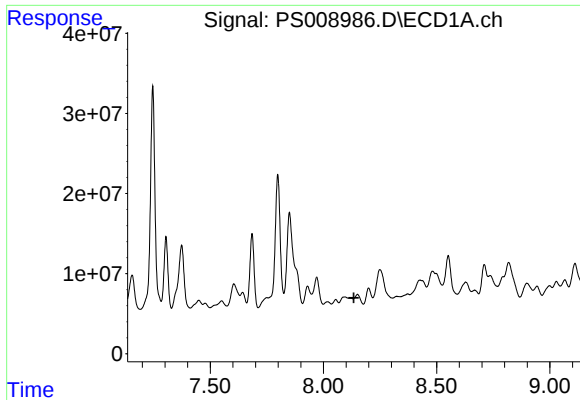

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

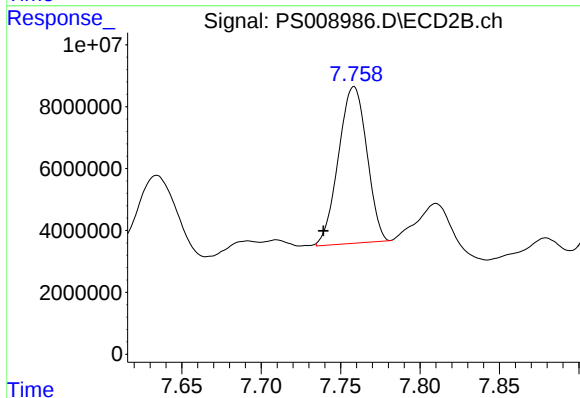


#8 DICHLORPROP

R.T.: 7.758 min
Delta R.T.: 0.019 min
Response: 62735088
Conc: 62.61 ng/ml

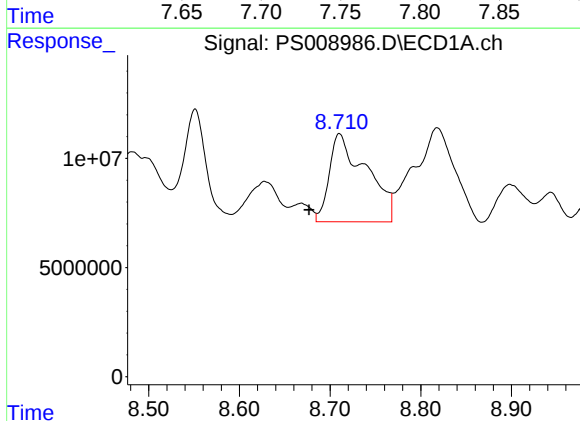


#10 Pentachlorophenol

R.T.: 8.711 min
Delta R.T.: 0.034 min
Response: 114106451
Conc: 3.93 ng/ml

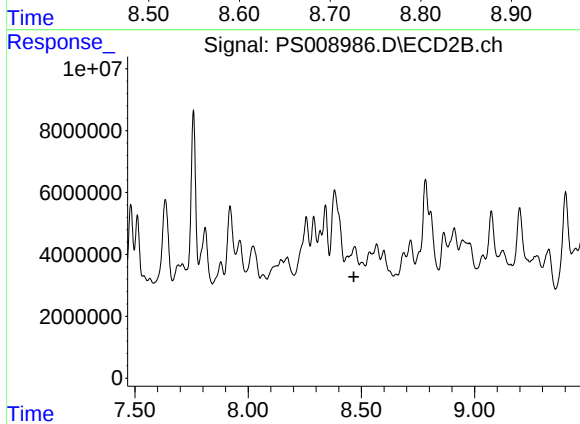

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.467 min
Response: 0
Conc: N.D.

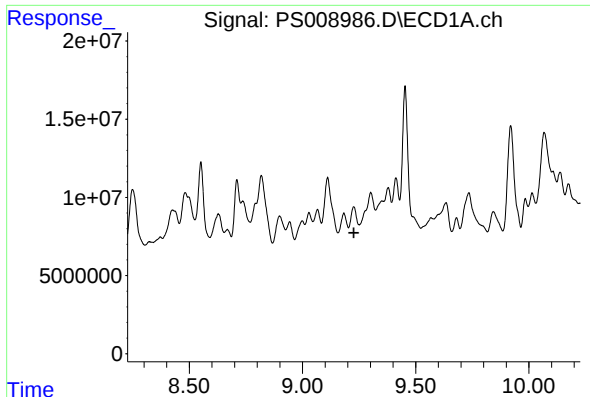

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

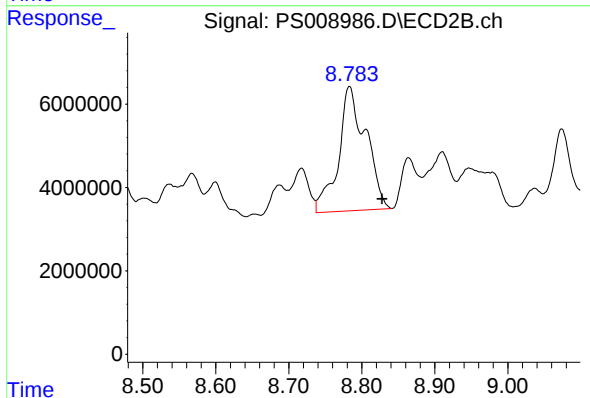


#11 2,4,5-TP (SILVEX)

R.T.: 8.783 min
Delta R.T.: -0.045 min
Response: 77747783
Conc: 14.35 ng/ml

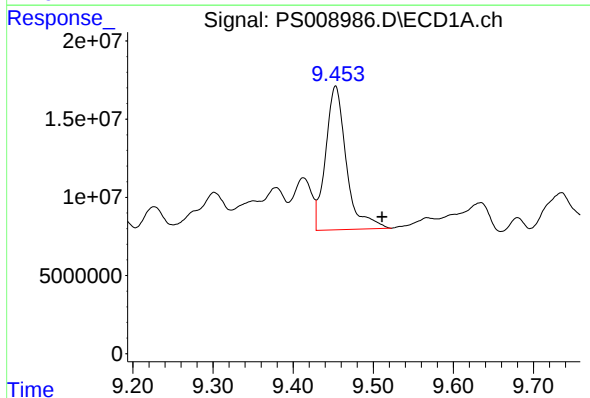


#12 2,4,5-T

R.T.: 9.453 min
Delta R.T.: -0.058 min
Response: 165069091
Conc: 15.44 ng/ml

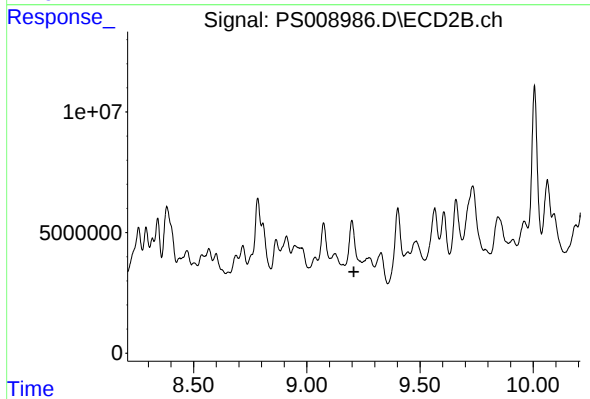

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

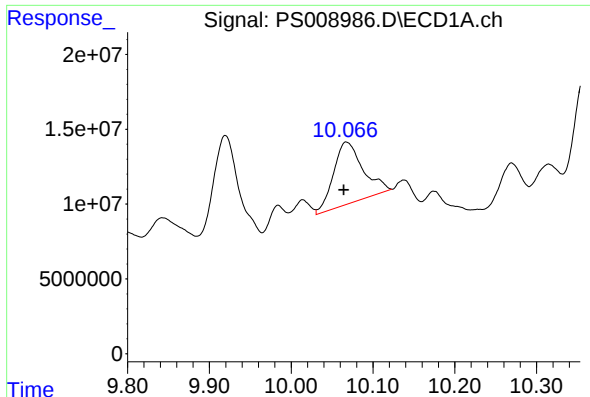

#13 2,4-DB


R.T.: 10.068 min
Delta R.T.: 0.003 min
Response: 103572352
Conc: 71.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

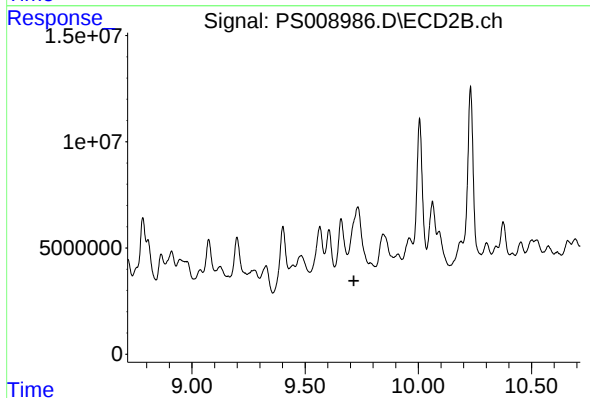


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.715 min
Response: 0
Conc: N.D.

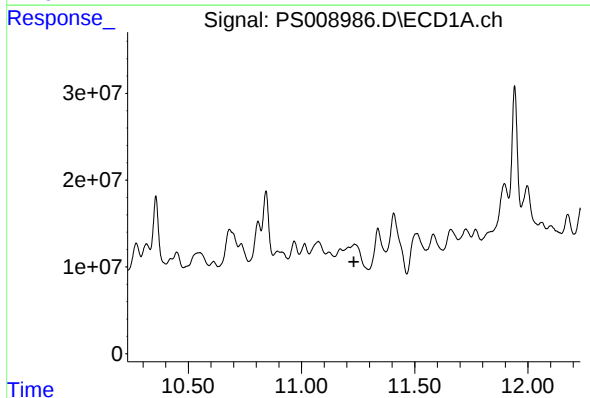


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

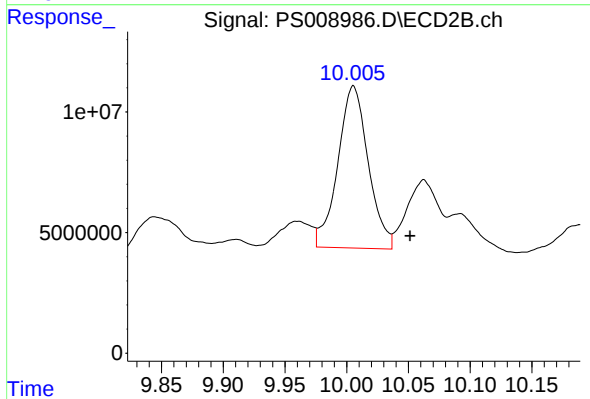

#14 DINOSEB


R.T.: 10.005 min
Delta R.T.: -0.046 min
Response: 115294809
Conc: 29.16 ng/ml

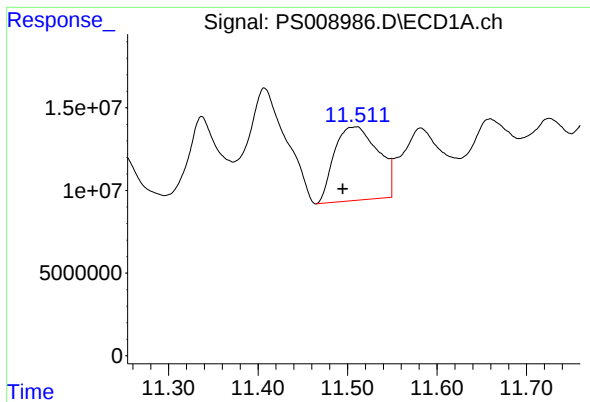

#16 DCPA

R.T.: 11.509 min
Delta R.T.: 0.014 min
Response: 151761349
Conc: 11.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

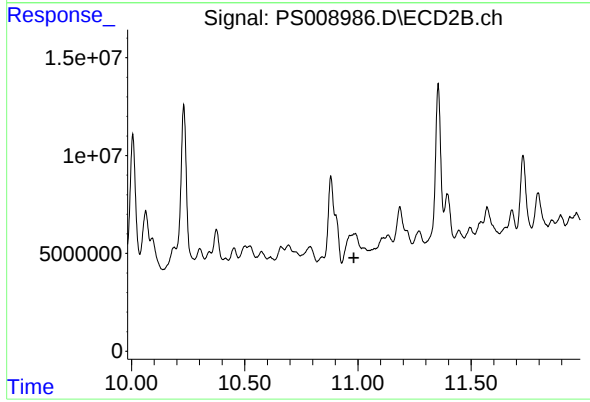

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.982 min
Response: 0
Conc: N.D.