

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 03:59
 Operator : DD\AJ
 Sample : L1635-19
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LIED-TS006-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 04:40:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	675.9E6	307.0E6	309.113	318.582
Target Compounds							
2) T	3,5-DICHL...	0.000	6.115	0	151.0E6	N.D.	103.471
7) T	MCPA	7.799	7.407	242.4E6	197.2E6	30.132	44.565 #
8) T	DICHLORPROP	0.000	7.760	0	119.7E6	N.D.	119.465
11) T	2,4,5-TP ...	0.000	8.783	0	42697770	N.D.	7.882
12) T	2,4,5-T	9.453	9.259	134.7E6	103.0E6	12.599	19.027 #
14) T	DINOSEB	0.000	10.059	0	56585148	N.D.	14.311
15) T	Picloram	11.044	11.031	638.4E6	326.3E6	46.631	44.904
16) T	DCPA	11.503	11.031	77799365	326.3E6	5.662	47.157 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 03:59
Operator : DD\AJ
Sample : L1635-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
LIED-TS006-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 04:40:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

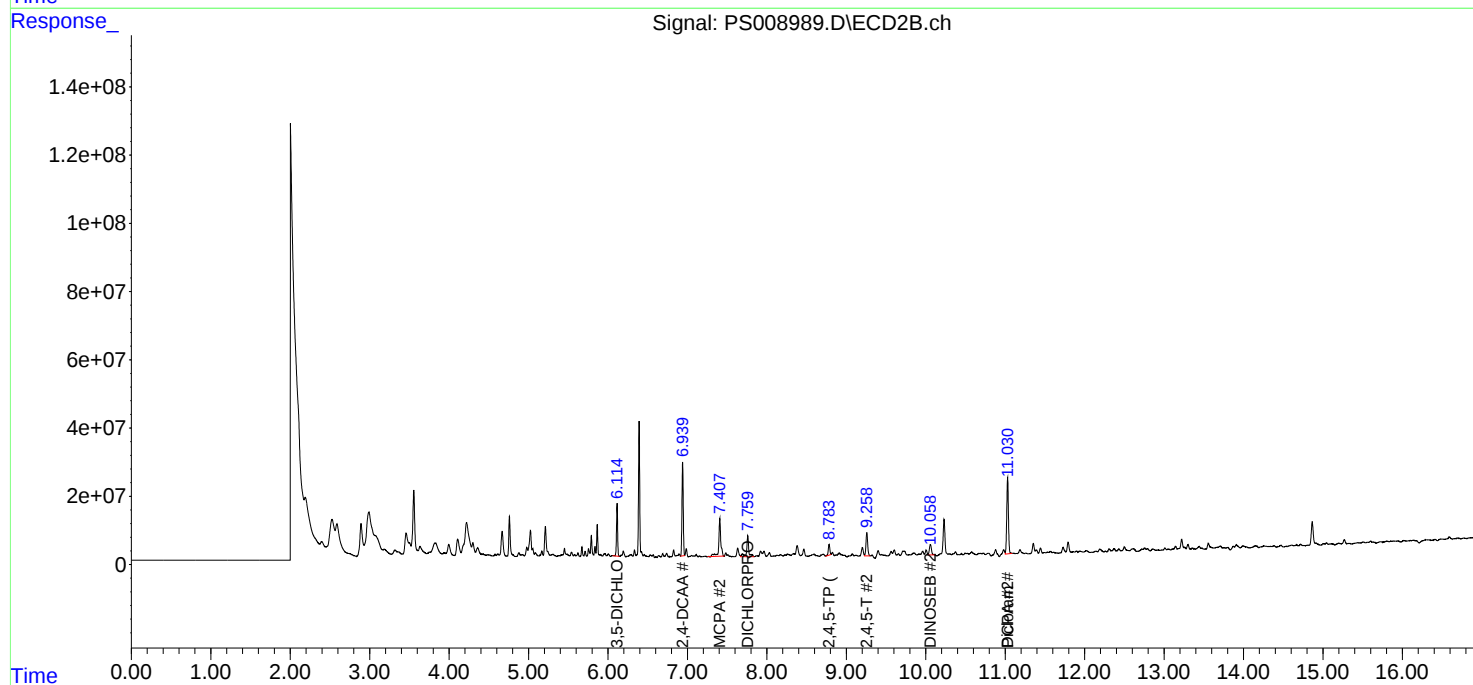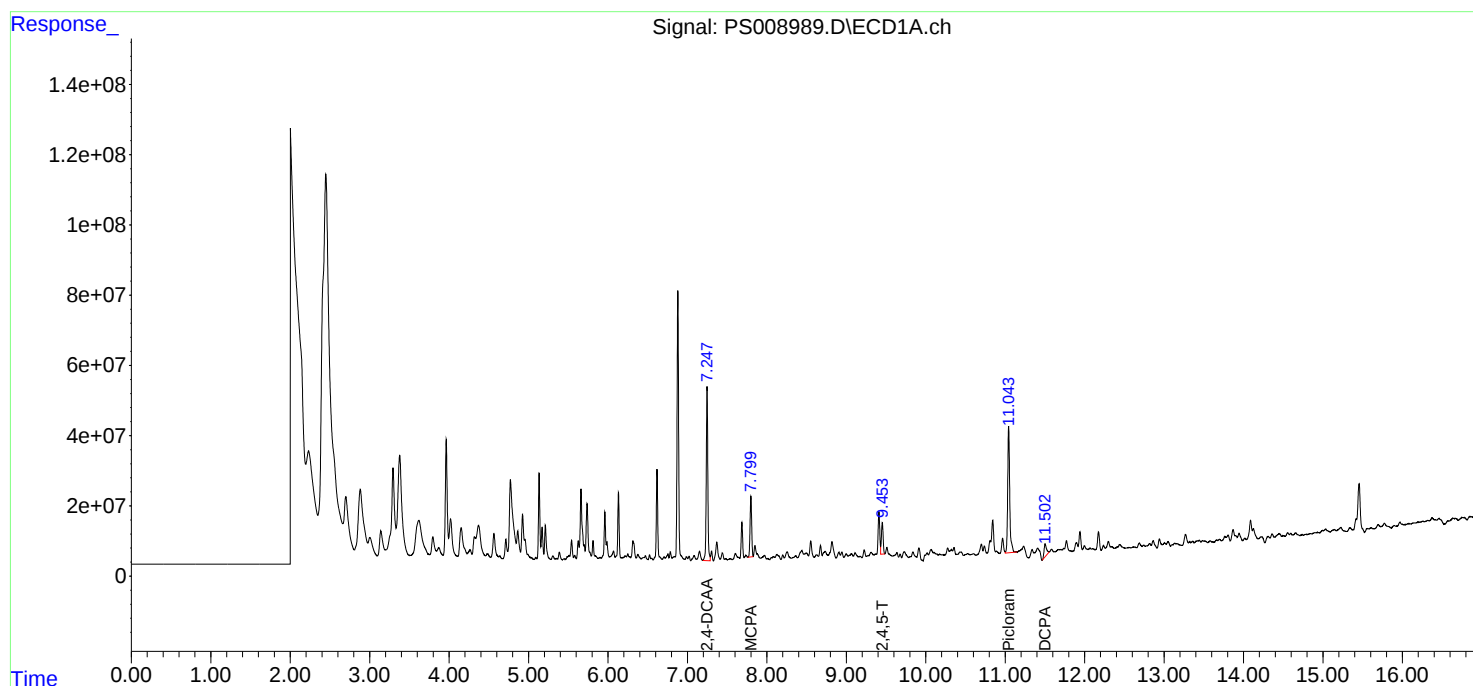


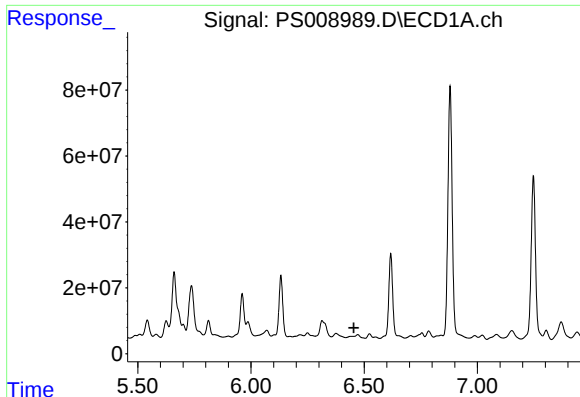

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS006-01

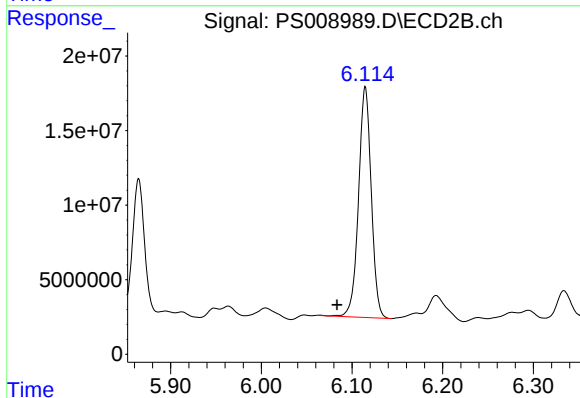


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 150992183
Conc: 103.47 ng/ml

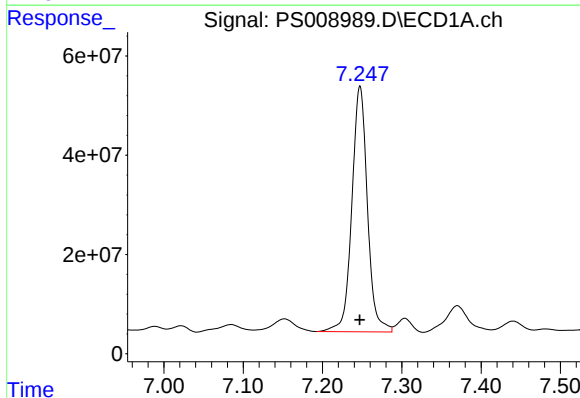


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 675904659
Conc: 309.11 ng/ml

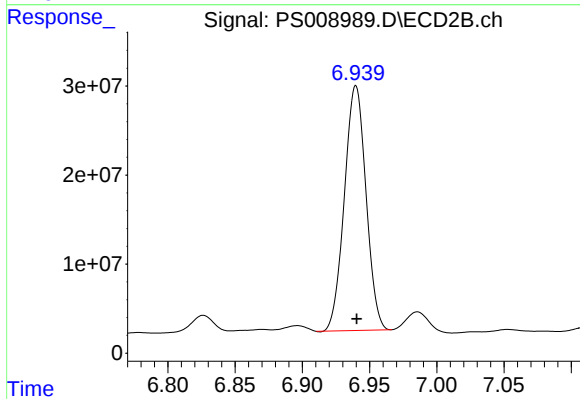

#4 2,4-DCAA


R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 306971772
Conc: 318.58 ng/ml

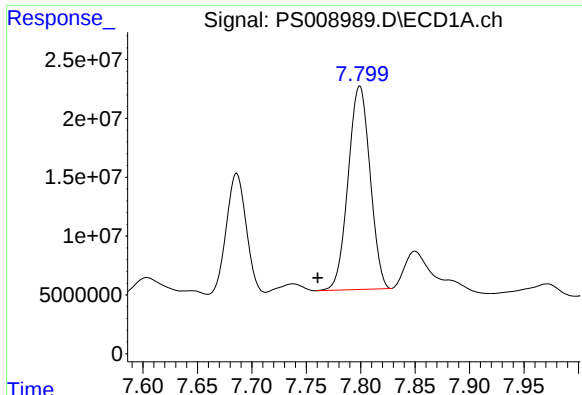

#7 MCPA


R.T.: 7.799 min
Delta R.T.: 0.038 min
Response: 242379327
Conc: 30.13 ug/ml

Instrument :
ECD_S
ClientSampleId :
LIED-TS006-01

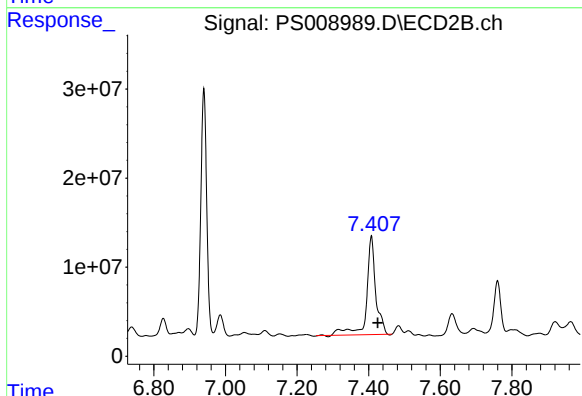


#7 MCPA

R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 197166417
Conc: 44.57 ug/ml

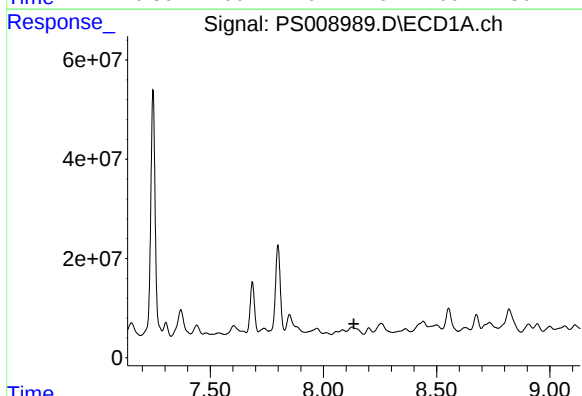


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

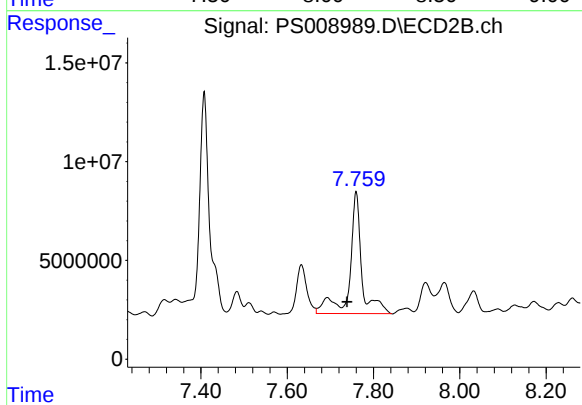

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 119696103
Conc: 119.47 ng/ml

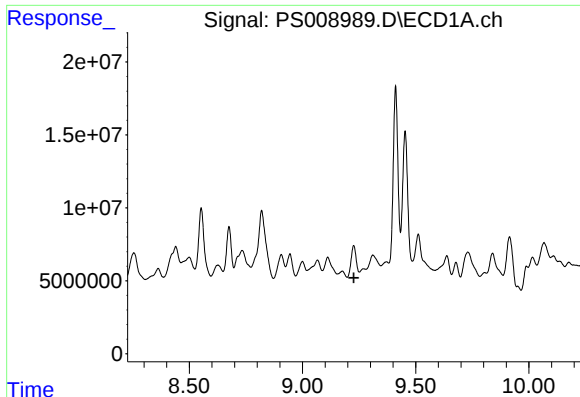

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS006-01

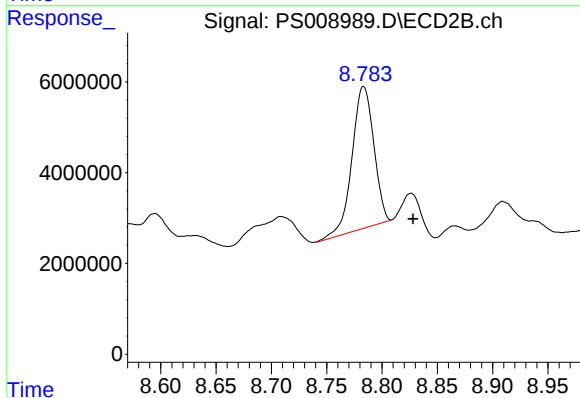


#11 2,4,5-TP (SILVEX)

R.T.: 8.783 min
Delta R.T.: -0.045 min
Response: 42697770
Conc: 7.88 ng/ml

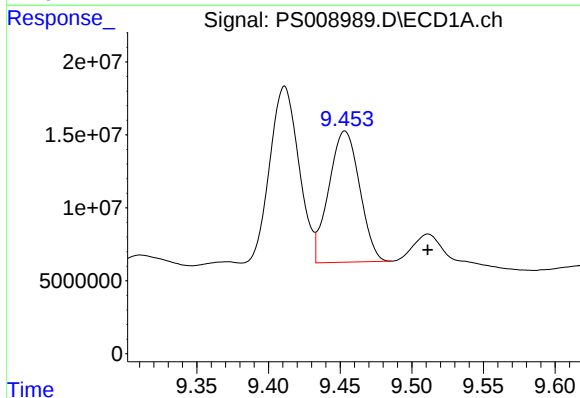


#12 2,4,5-T

R.T.: 9.453 min
Delta R.T.: -0.058 min
Response: 134710207
Conc: 12.60 ng/ml

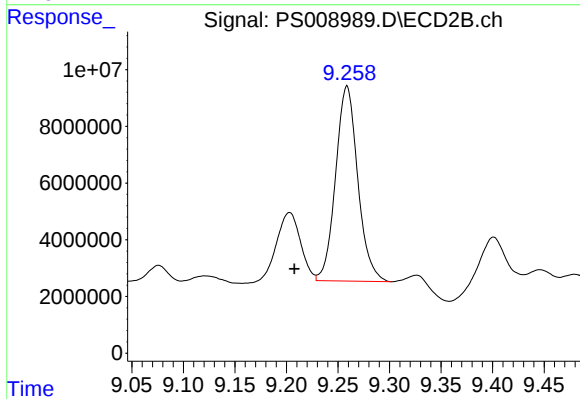

#12 2,4,5-T


R.T.: 9.259 min
Delta R.T.: 0.051 min
Response: 102995880
Conc: 19.03 ng/ml

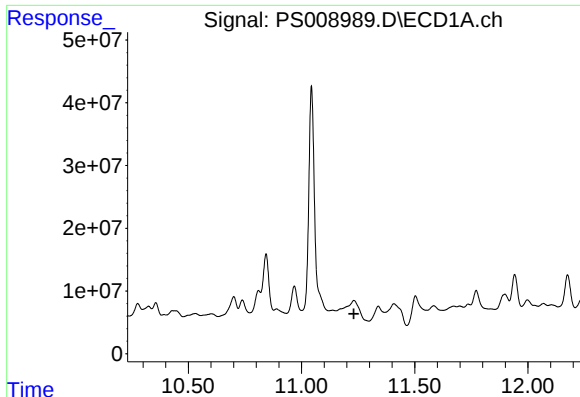

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
LIED-TS006-01

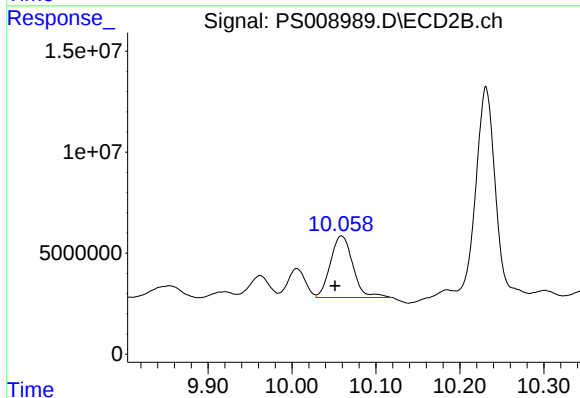


#14 DINOSEB

R.T.: 10.059 min
Delta R.T.: 0.008 min
Response: 56585148
Conc: 14.31 ng/ml

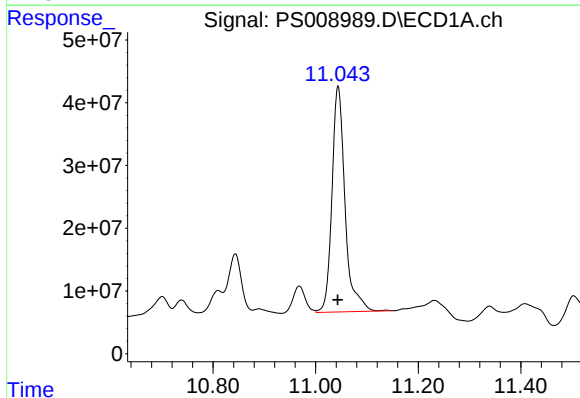


#15 Picloram

R.T.: 11.044 min
Delta R.T.: 0.000 min
Response: 638426563
Conc: 46.63 ng/ml

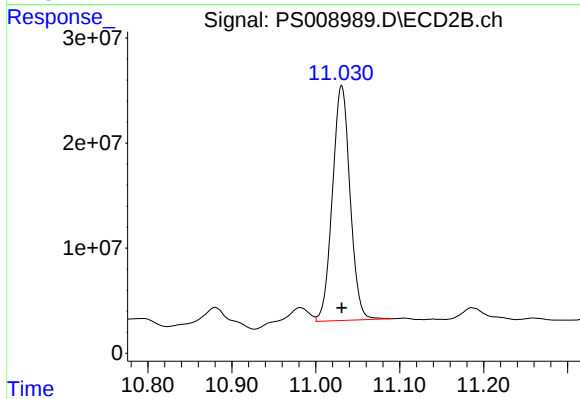

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 326299024
Conc: 44.90 ng/ml

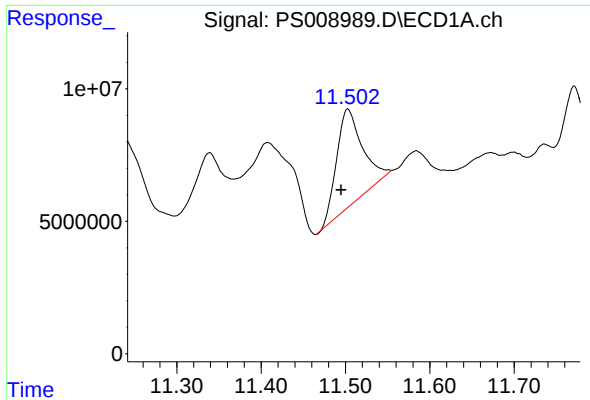

#16 DCPA

R.T.: 11.503 min
Delta R.T.: 0.008 min
Response: 77799365
Conc: 5.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
LIED-TS006-01

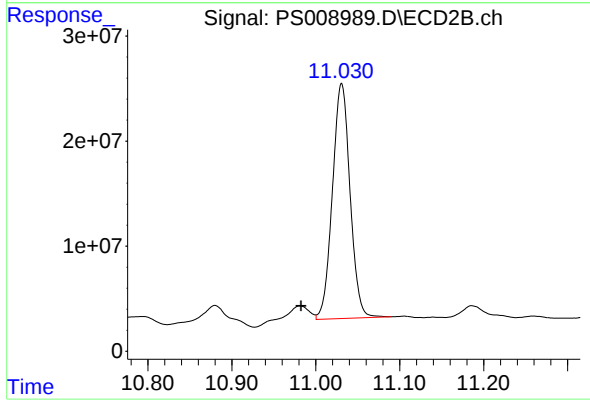

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.049 min
Response: 326299024
Conc: 47.16 ng/ml