

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
 Data File : PS008996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 10:19
 Operator : DD\AJ
 Sample : L1654-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-03-012-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:12:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.587	0	99305594	N.D. 67.914
2) T	3,5-DICHL...	0.000	6.114	0	95128650	N.D. 65.189
7) T	MCPA	7.802	7.407	246.0E6	138.5E6	30.579 31.307
8) T	DICHLORPROP	0.000	7.760	0	78002399	N.D. 77.852
9) T	2,4-D	0.000	8.018	0	23391968	N.D. 19.743
10) T	Pentachlo...	0.000	8.465	0	20455837	N.D. 1.440
11) T	2,4,5-TP ...	0.000	8.784	0	22266791	N.D. 4.111
12) T	2,4,5-T	9.457	9.207	89488459	28428220	8.370 5.252 #
13) T	2,4-DB	0.000	9.708	0	24062969	N.D. 34.256
14) T	DINOSEB	0.000	10.054	0	29569142	N.D. 7.478
15) T	Picloram	11.047	11.031	838.5E6	482.6E6	61.247 66.413
16) T	DCPA	11.501	10.981	66474734	24249187	4.838 3.505 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
Data File : PS008996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 10:19
Operator : DD\AJ
Sample : L1654-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:12:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

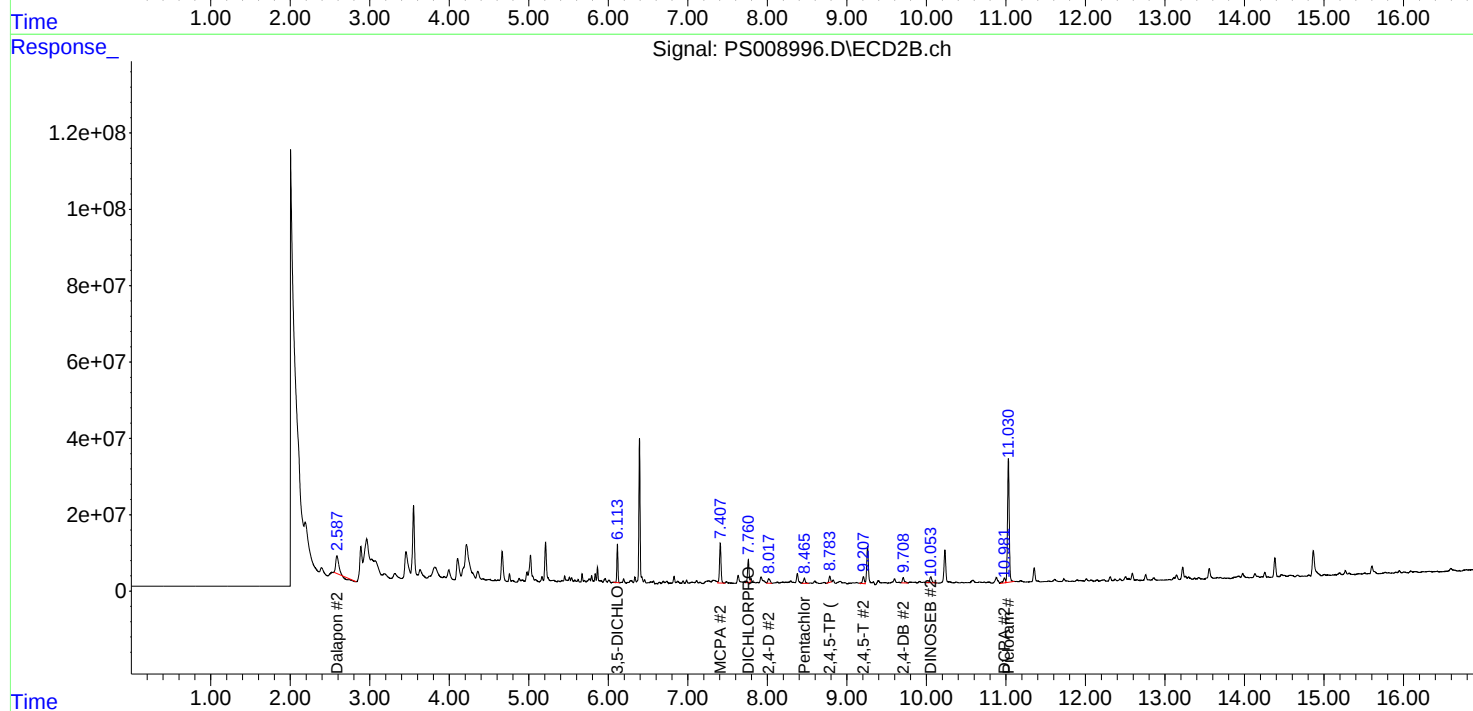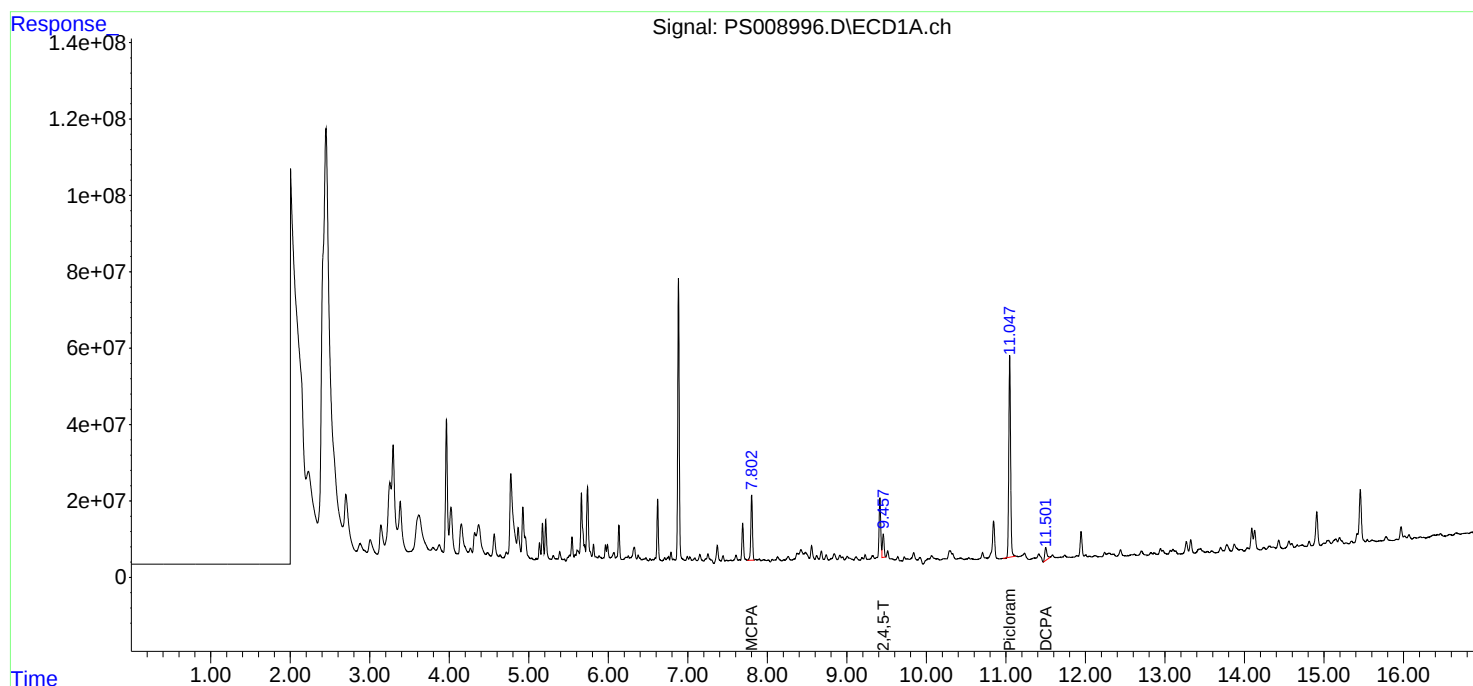


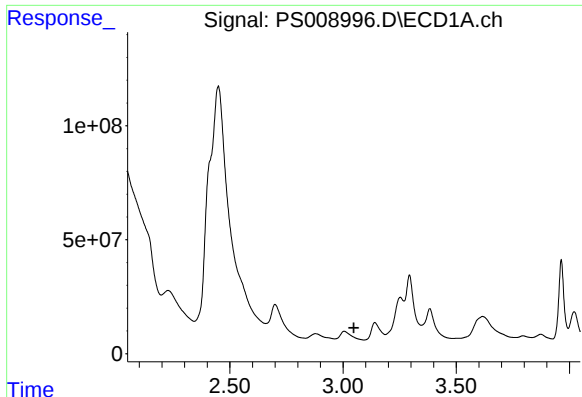

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

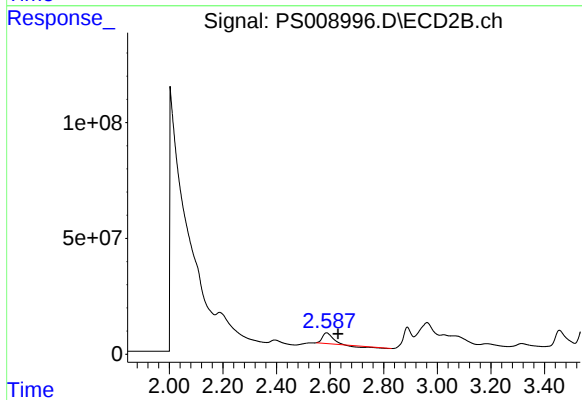


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.043 min
Response: 99305594
Conc: 67.91 ng/ml

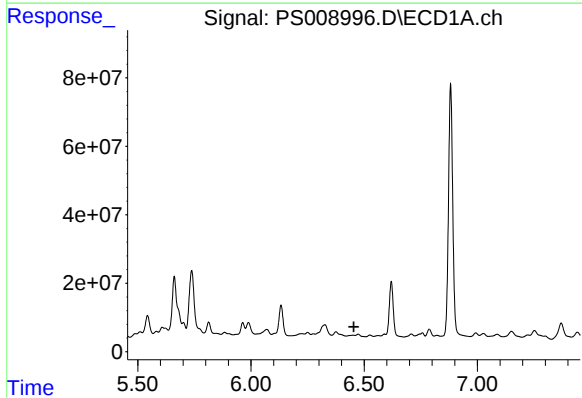


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

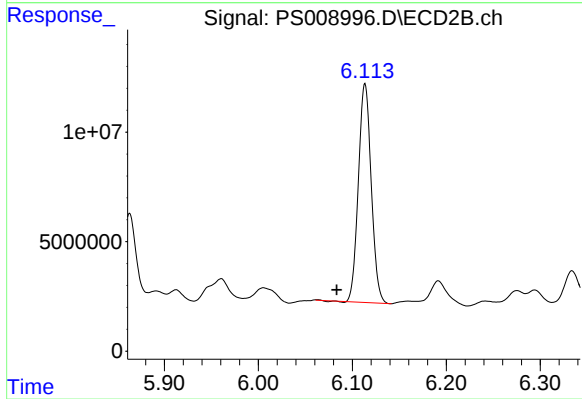

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 95128650
Conc: 65.19 ng/ml

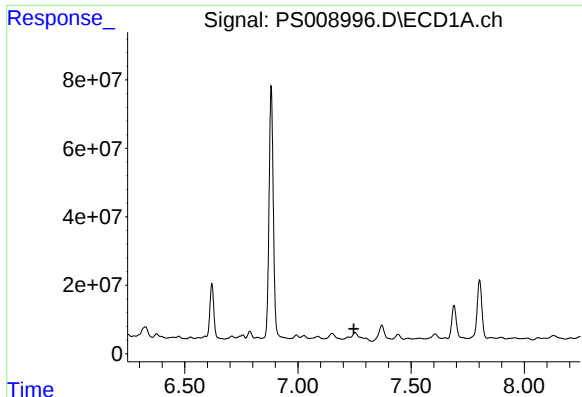

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.247 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

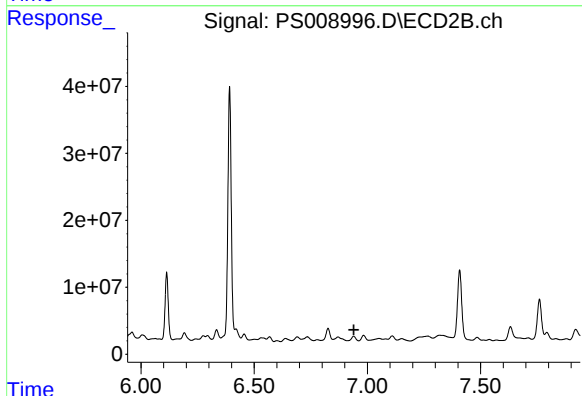


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.940 min
Response: 0
Conc: N.D.

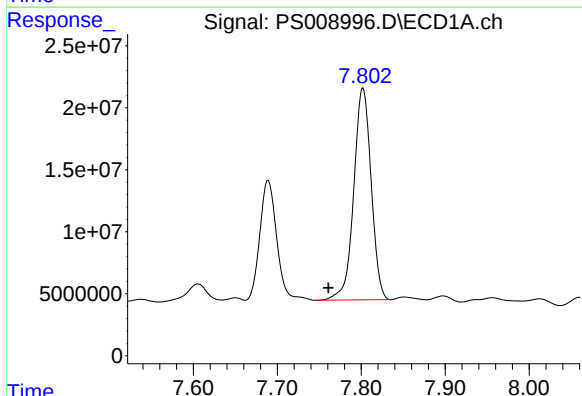


#7 MCPA

R.T.: 7.802 min
Delta R.T.: 0.041 min
Response: 245976885
Conc: 30.58 ug/ml

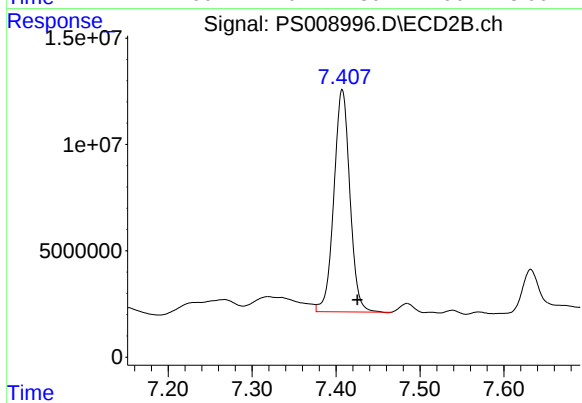

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 138511289
Conc: 31.31 ug/ml

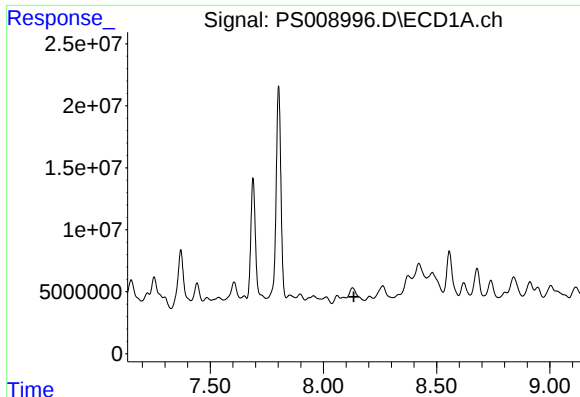

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

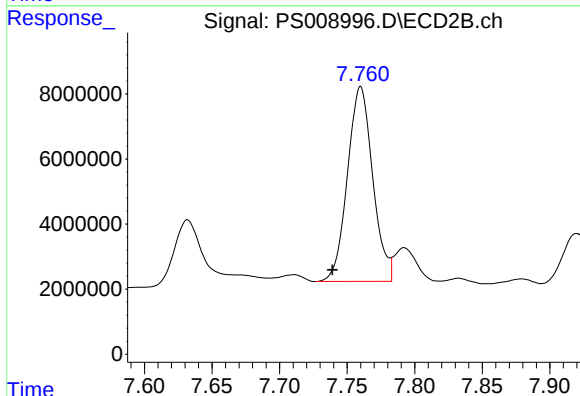


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 78002399
Conc: 77.85 ng/ml

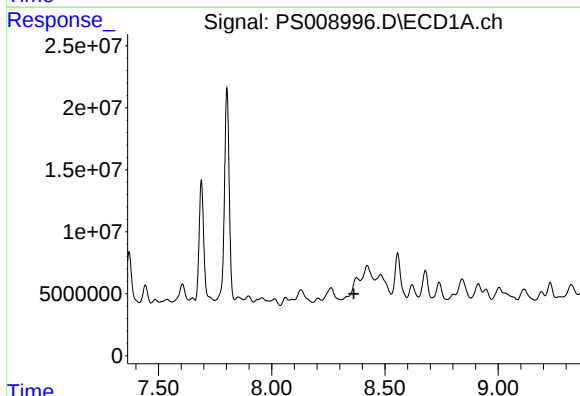


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

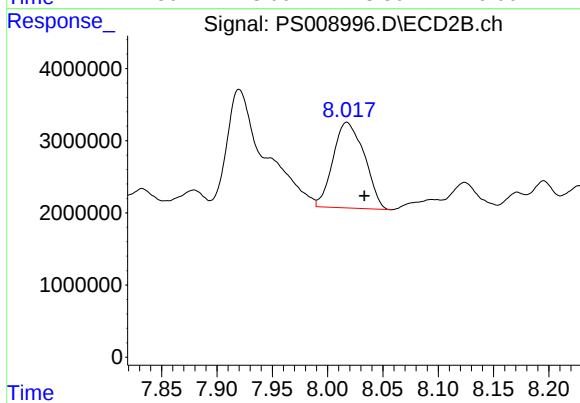

#9 2,4-D


R.T.: 8.018 min
Delta R.T.: -0.016 min
Response: 23391968
Conc: 19.74 ng/ml

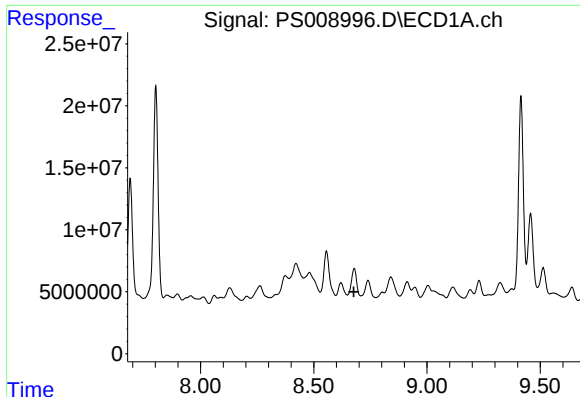

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

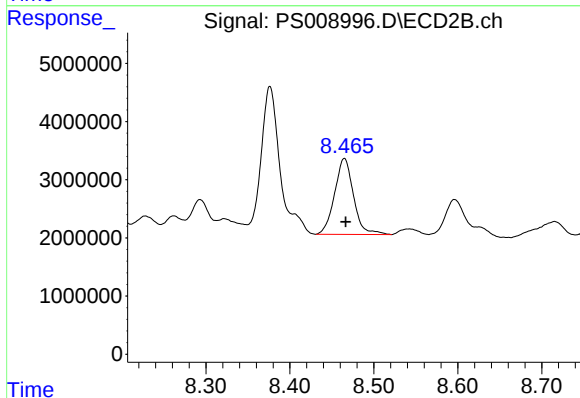


#10 Pentachlorophenol

R.T.: 8.465 min
Delta R.T.: -0.002 min
Response: 20455837
Conc: 1.44 ng/ml

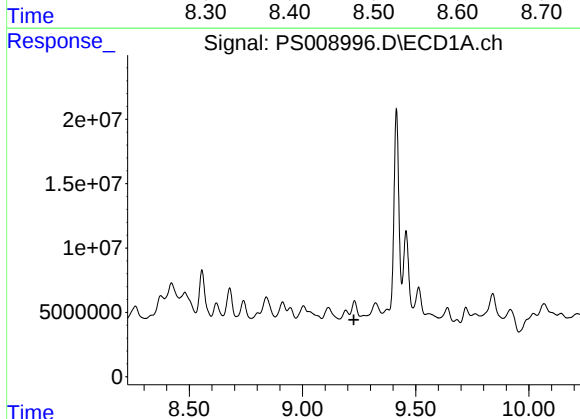


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

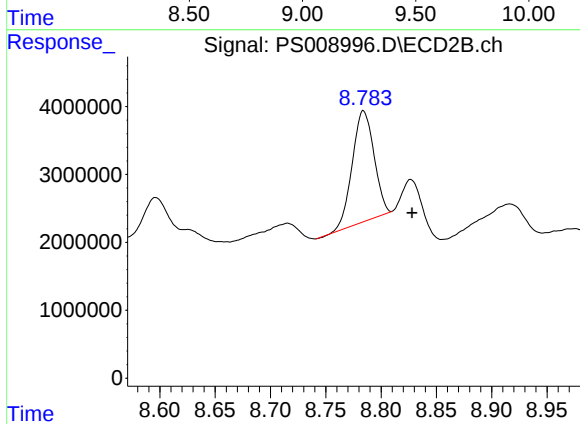

#11 2,4,5-TP (SILVEX)


R.T.: 8.784 min
Delta R.T.: -0.044 min
Response: 22266791
Conc: 4.11 ng/ml

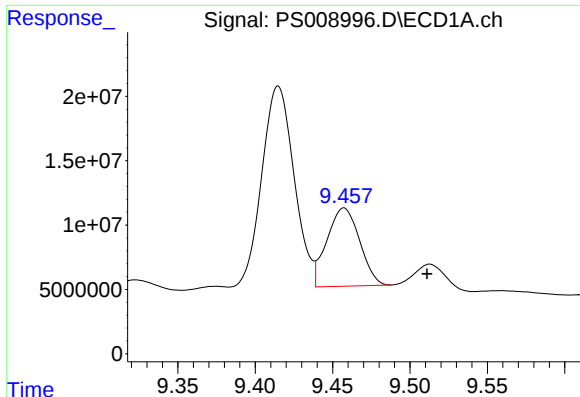

#12 2,4,5-T


R.T.: 9.457 min
Delta R.T.: -0.054 min
Response: 89488459
Conc: 8.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

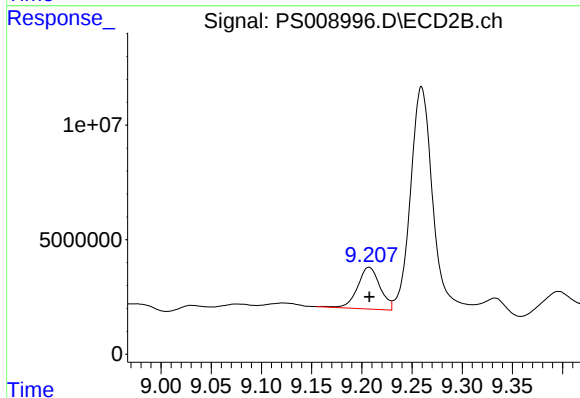


#12 2,4,5-T

R.T.: 9.207 min
Delta R.T.: 0.000 min
Response: 28428220
Conc: 5.25 ng/ml

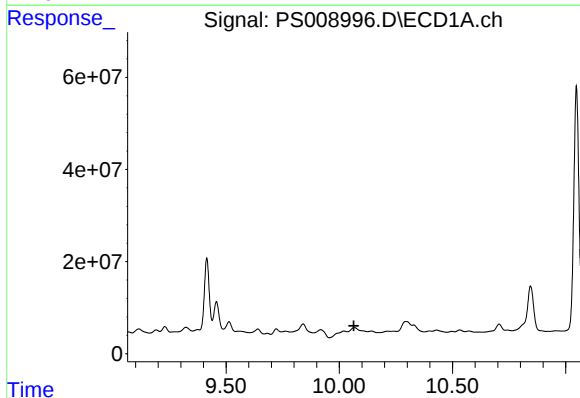


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

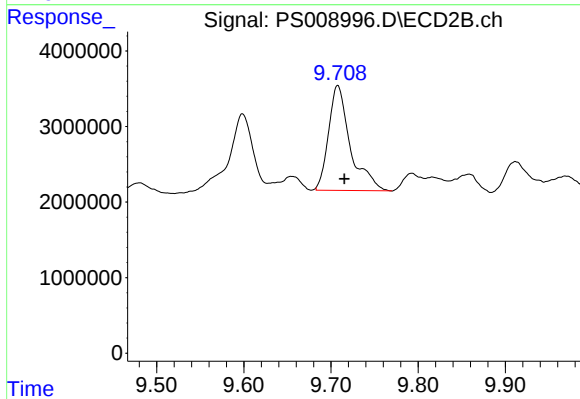

#13 2,4-DB


R.T.: 9.708 min
Delta R.T.: -0.007 min
Response: 24062969
Conc: 34.26 ng/ml

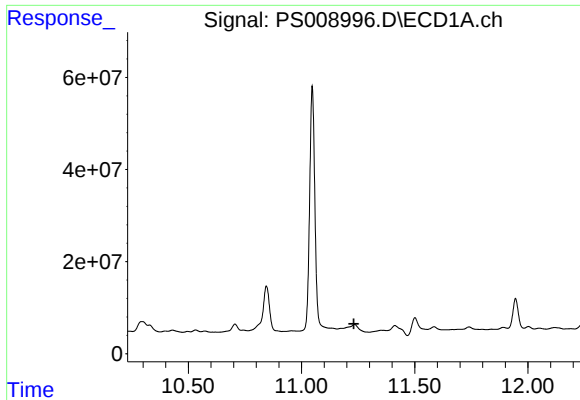

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

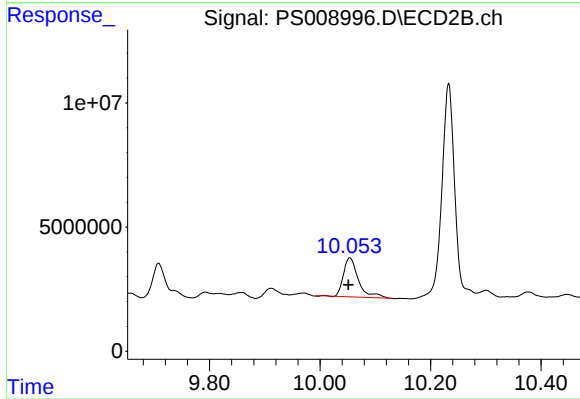


#14 DINOSEB

R.T.: 10.054 min
Delta R.T.: 0.002 min
Response: 29569142
Conc: 7.48 ng/ml

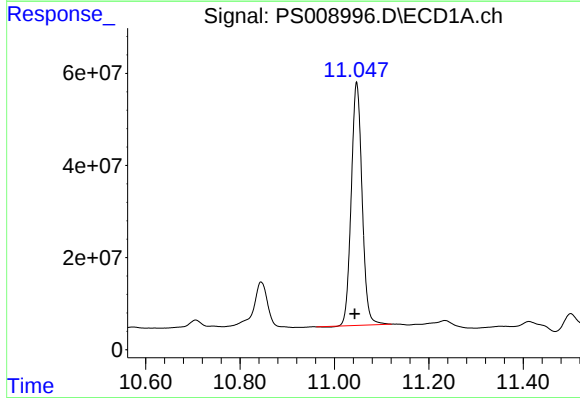


#15 Picloram

R.T.: 11.047 min
Delta R.T.: 0.004 min
Response: 838537131
Conc: 61.25 ng/ml

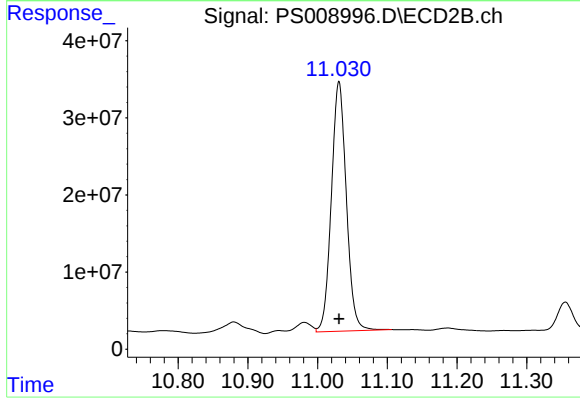

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 482589363
Conc: 66.41 ng/ml

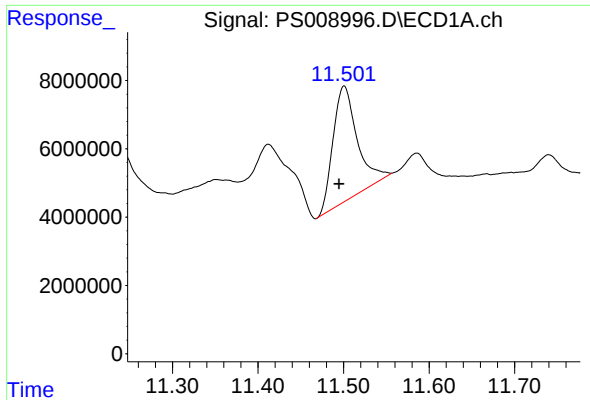

#16 DCPA

R.T.: 11.501 min
Delta R.T.: 0.006 min
Response: 66474734
Conc: 4.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-03-012-ABCD

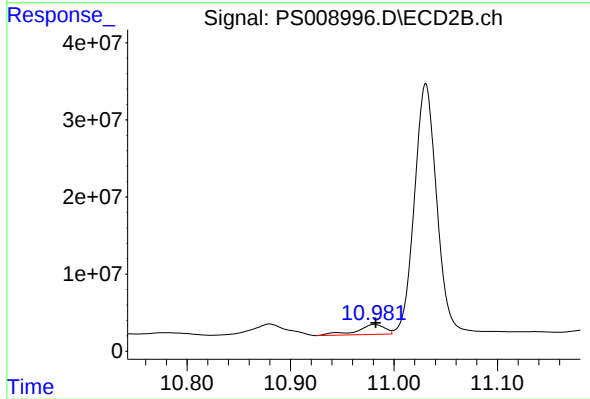

#16 DCPA

R.T.: 10.981 min
Delta R.T.: -0.001 min
Response: 24249187
Conc: 3.50 ng/ml