

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
 Data File : PS008997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 10:42
 Operator : DD\AJ
 Sample : L1655-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-BPM-01-AA1-BB1-AA1A-BB1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:12:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.984	0	8971905	N.D.	9.311
Target Compounds							
1) T	Dalapon	0.000	2.589	0	218.1E6	N.D.	149.181
2) T	3,5-DICHL...	0.000	6.114	0	107.0E6	N.D.	73.357
7) T	MCPA	7.799	7.407	234.5E6	126.9E6	29.151	28.694
8) T	DICHLORPROP	0.000	7.760	0	57806923	N.D.	57.695
11) T	2,4,5-TP ...	0.000	8.784	0	39913616	N.D.	7.368
12) T	2,4,5-T	9.454	0.000	158.7E6	0	14.846	N.D. #
14) T	DINOSEB	0.000	10.055	0	29238990	N.D.	7.395
15) T	Picloram	0.000	11.031	0	20845220	N.D.	2.869
16) T	DCPA	0.000	11.031	0	20845220	N.D.	3.013



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
Data File : PS008997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 10:42
Operator : DD\AJ
Sample : L1655-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:12:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

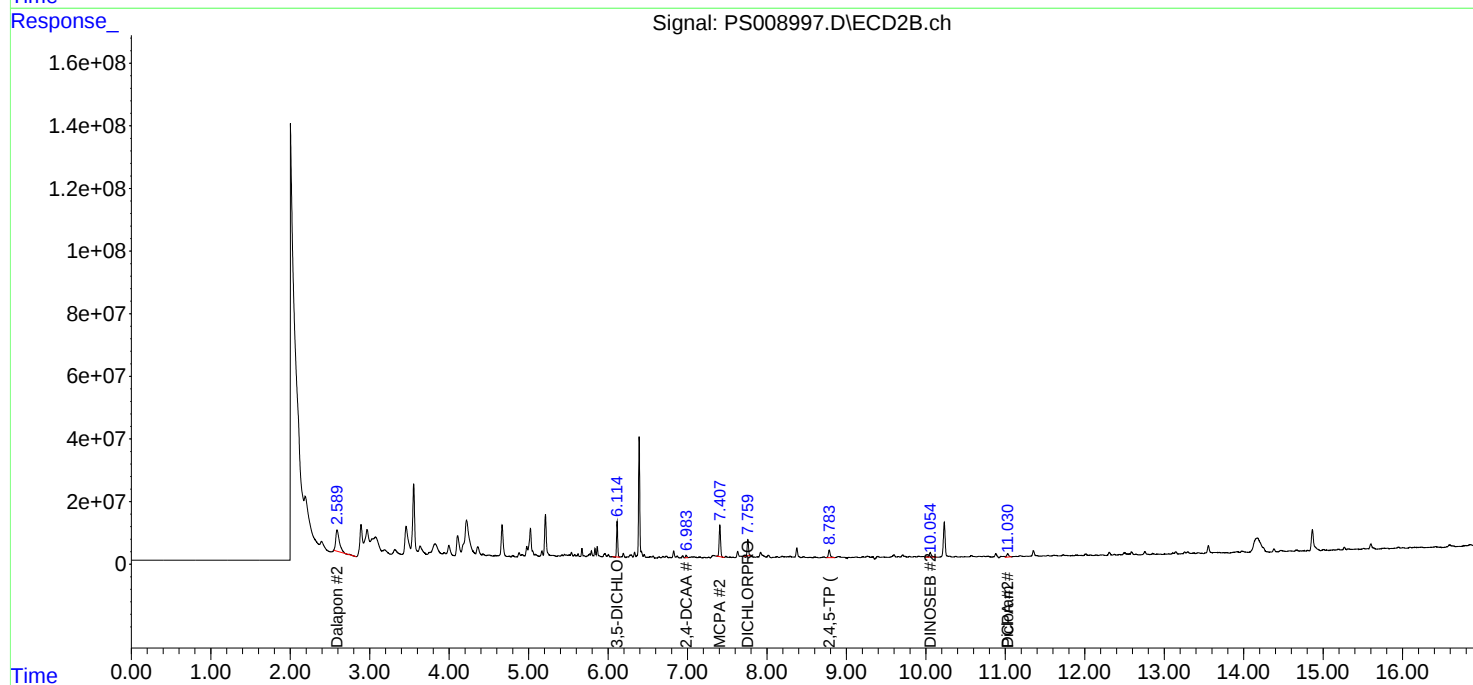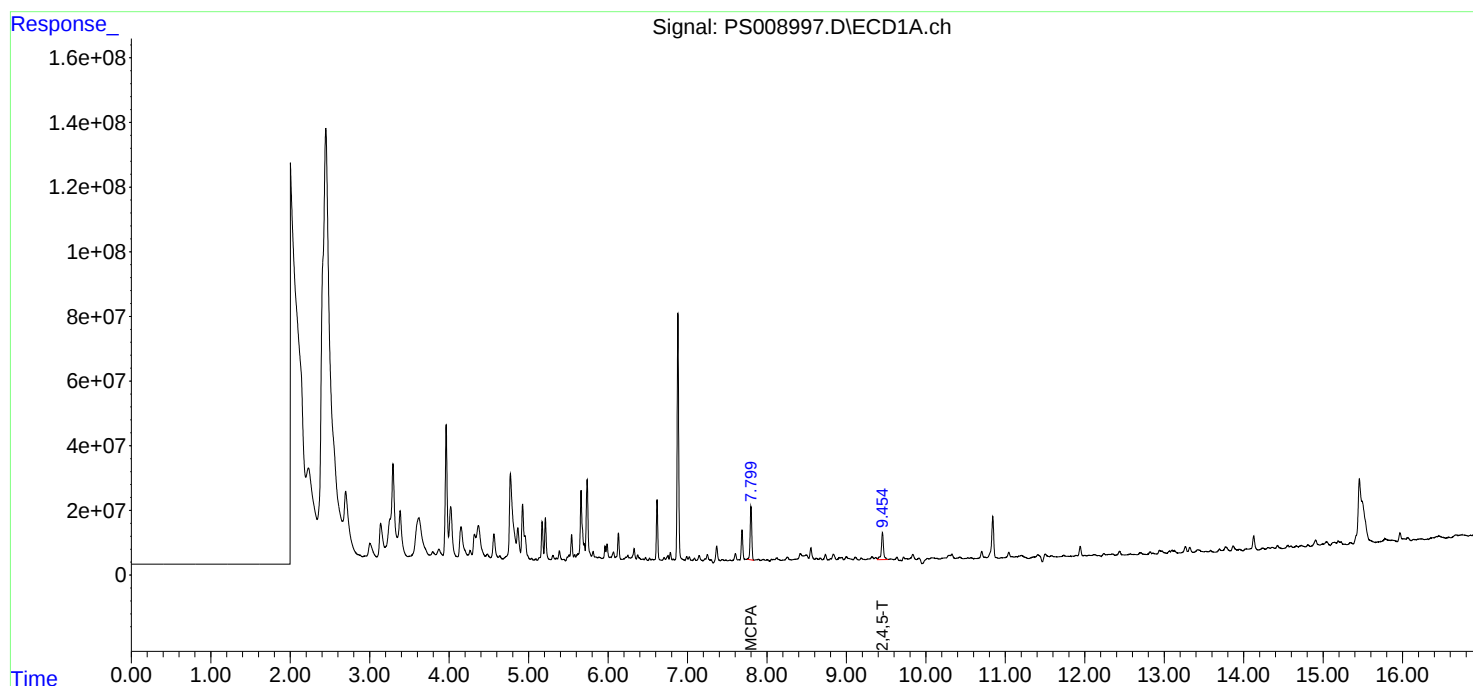


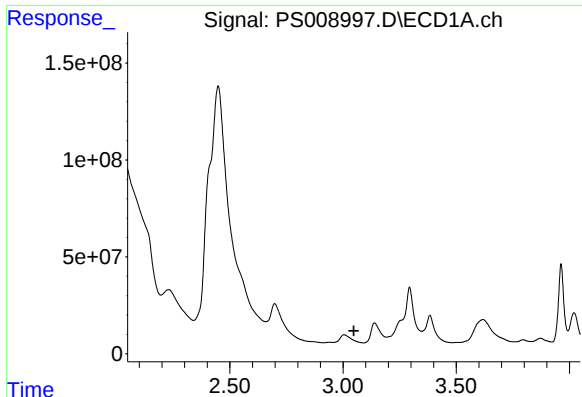

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

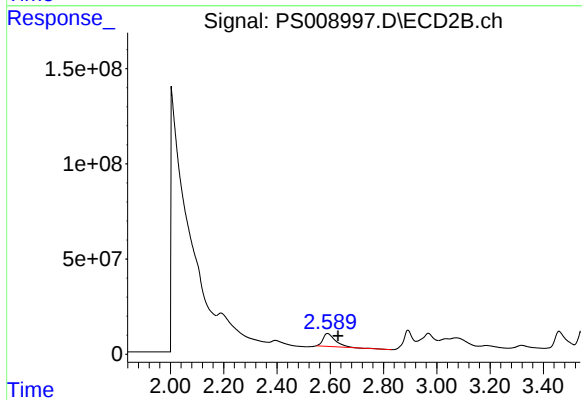


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.040 min
Response: 218135908
Conc: 149.18 ng/ml

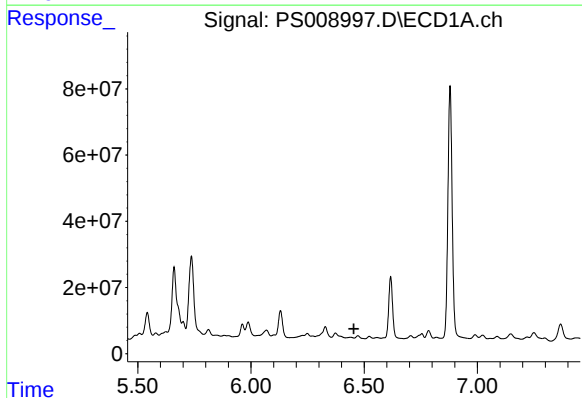


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

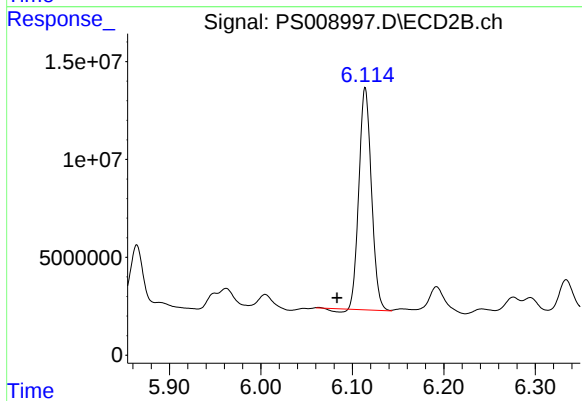

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 107047279
Conc: 73.36 ng/ml

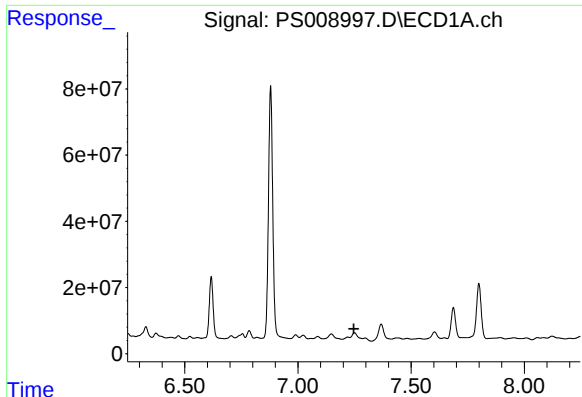

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.247 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

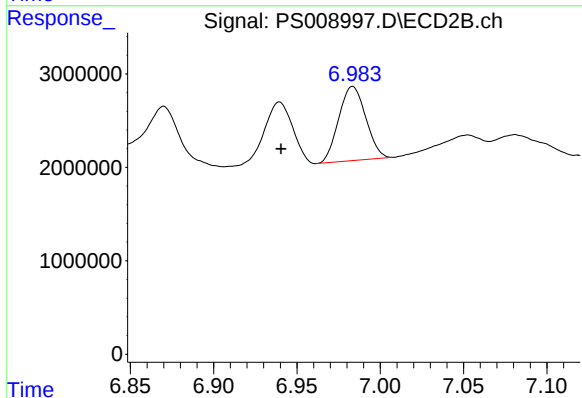


#4 2,4-DCAA

R.T.: 6.984 min
Delta R.T.: 0.043 min
Response: 8971905
Conc: 9.31 ng/ml

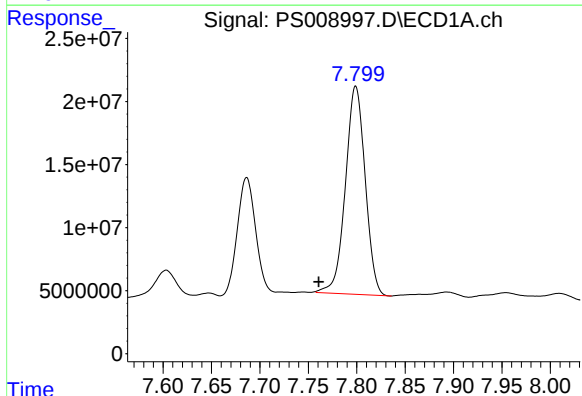


#7 MCPA

R.T.: 7.799 min
Delta R.T.: 0.038 min
Response: 234486343
Conc: 29.15 ug/ml

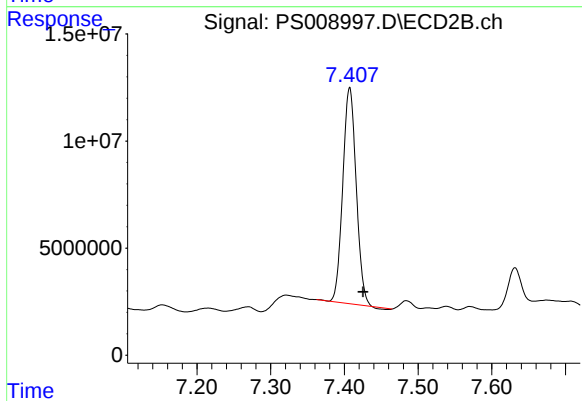

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 126949277
Conc: 28.69 ug/ml

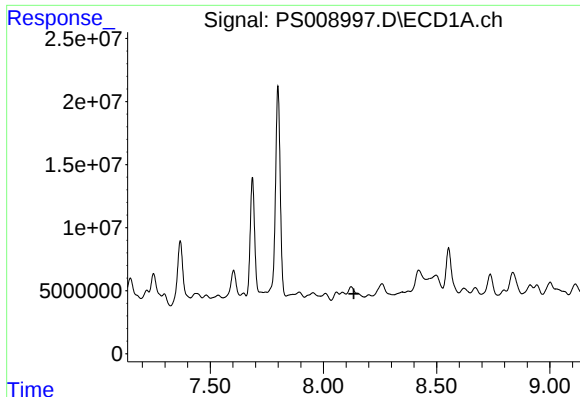

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

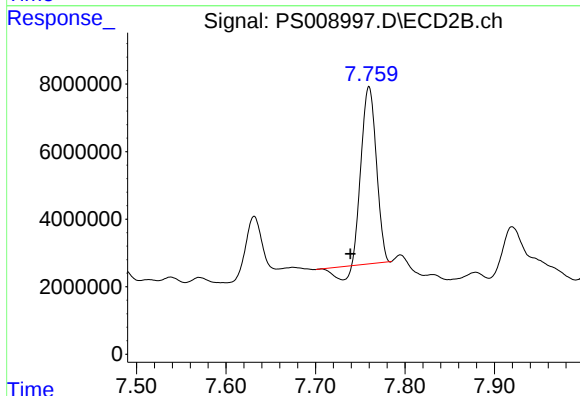


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 57806923
Conc: 57.70 ng/ml

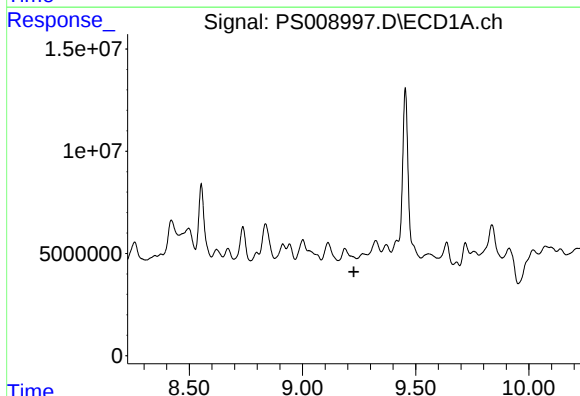


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

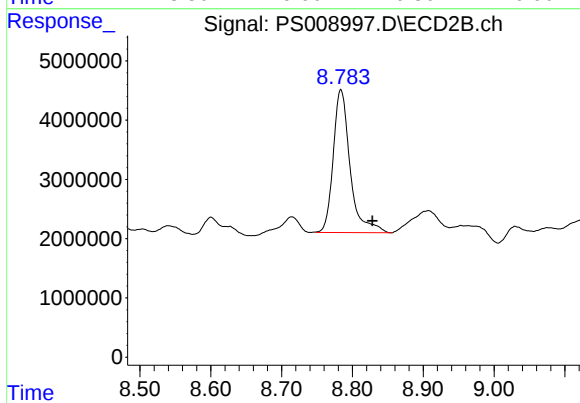

#11 2,4,5-TP (SILVEX)


R.T.: 8.784 min
Delta R.T.: -0.044 min
Response: 39913616
Conc: 7.37 ng/ml

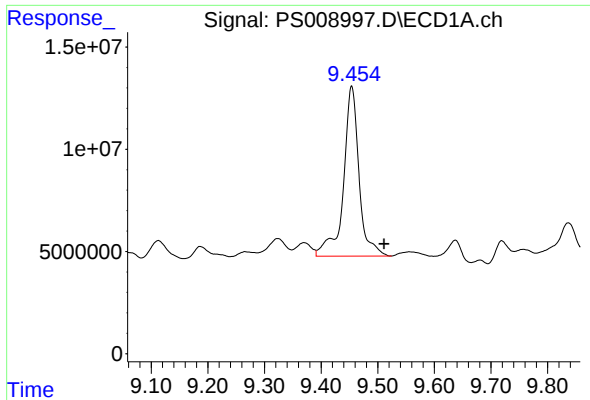

#12 2,4,5-T


R.T.: 9.454 min
Delta R.T.: -0.057 min
Response: 158733579
Conc: 14.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

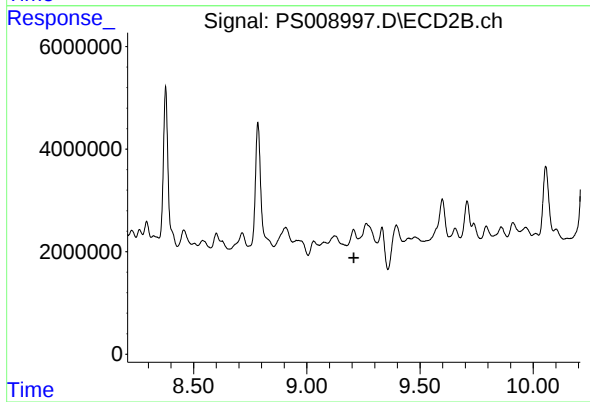


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

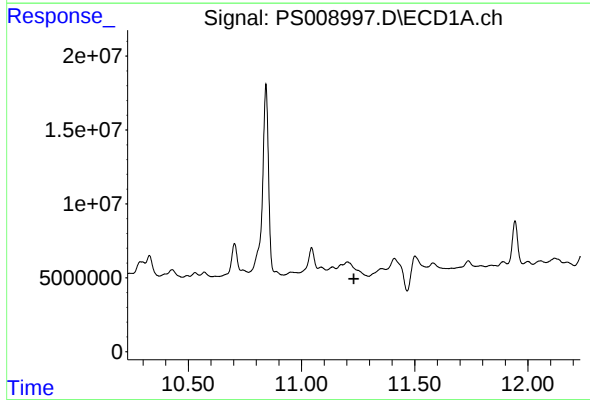


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

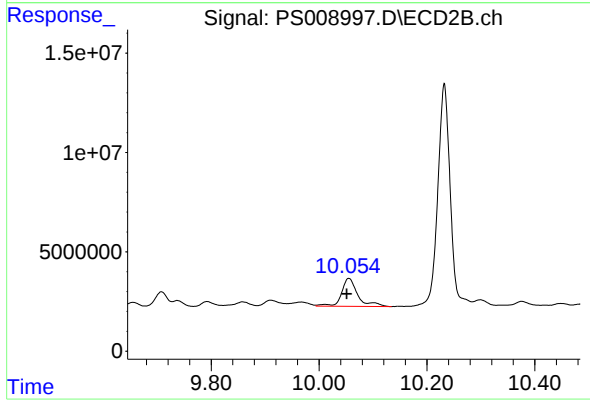

#14 DINOSEB


R.T.: 10.055 min
Delta R.T.: 0.004 min
Response: 29238990
Conc: 7.39 ng/ml

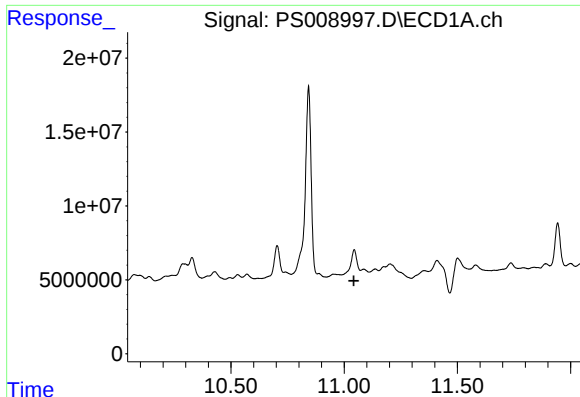

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
FK-BPM-01-AA1-BB1-AA1A-BB1A

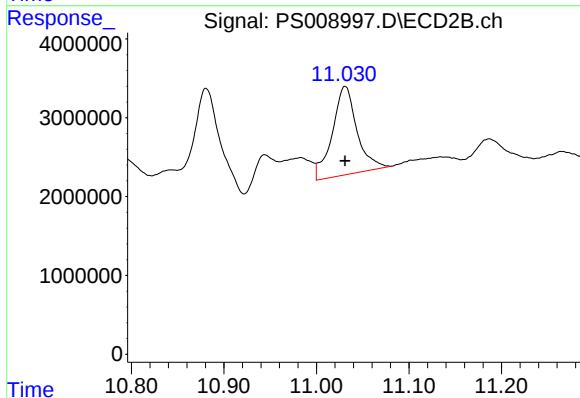


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 20845220
Conc: 2.87 ng/ml

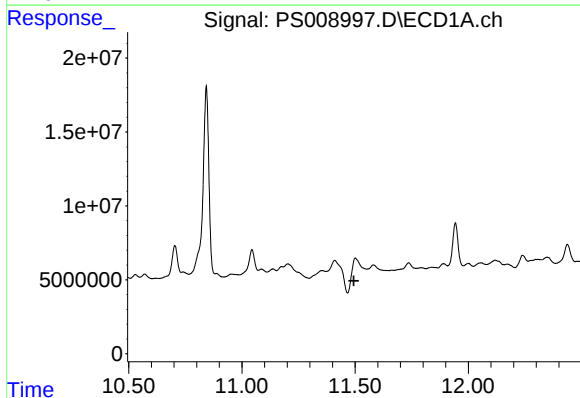

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

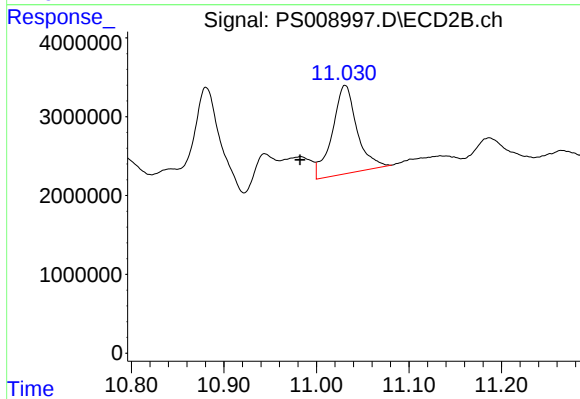

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.049 min
Response: 20845220
Conc: 3.01 ng/ml