

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
 Data File : PS008984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 01:19
 Operator : DD\AJ
 Sample : L1635-16
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LIED-TS003-01

Manual Integrations
 APPROVED

Sohil
 2/26/2020 12:24:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 13:24:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.247	6.939	657.0E6	285.4E6	300.463	296.226m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022420\
Data File : PS008984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 01:19
Operator : DD\AJ
Sample : L1635-16
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
LIED-TS003-01


Manual Integrations
APPROVED

Sohil
2/26/2020 12:24:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 13:24:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

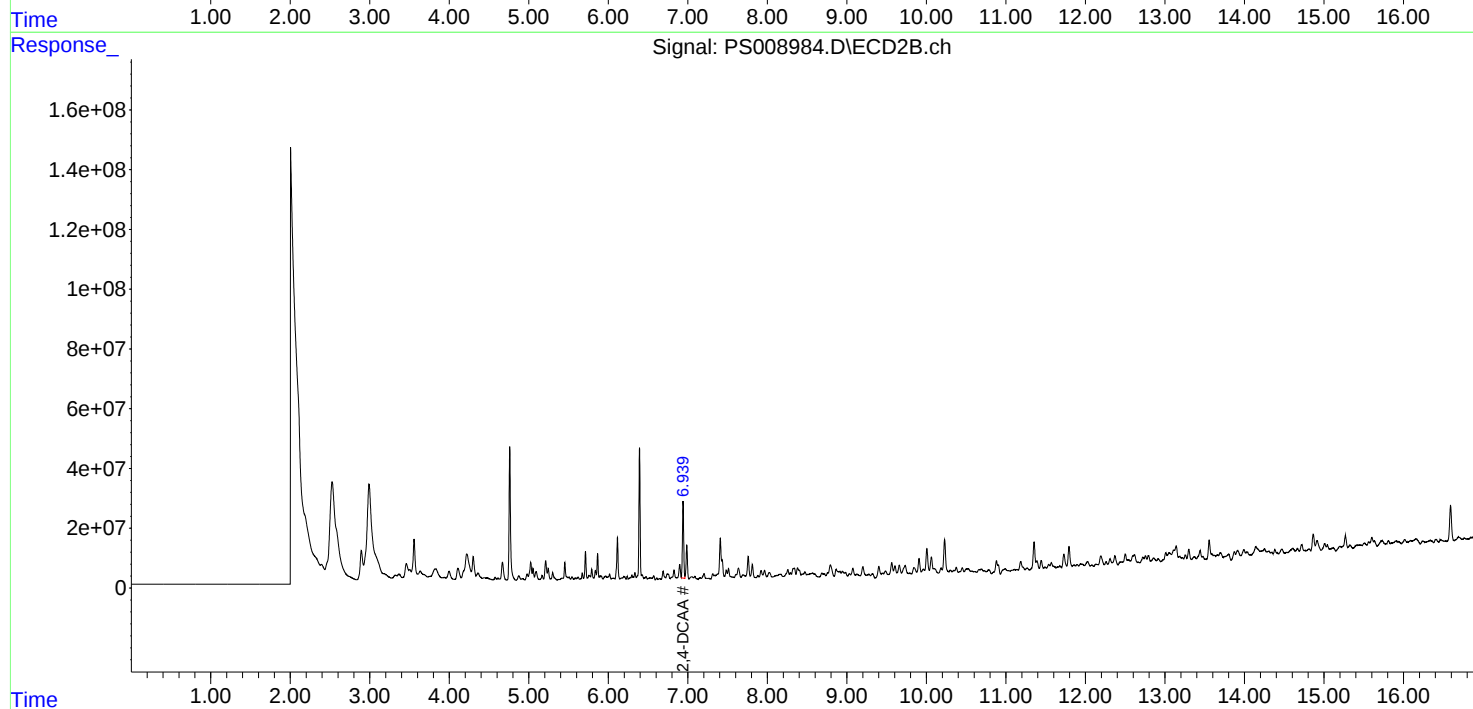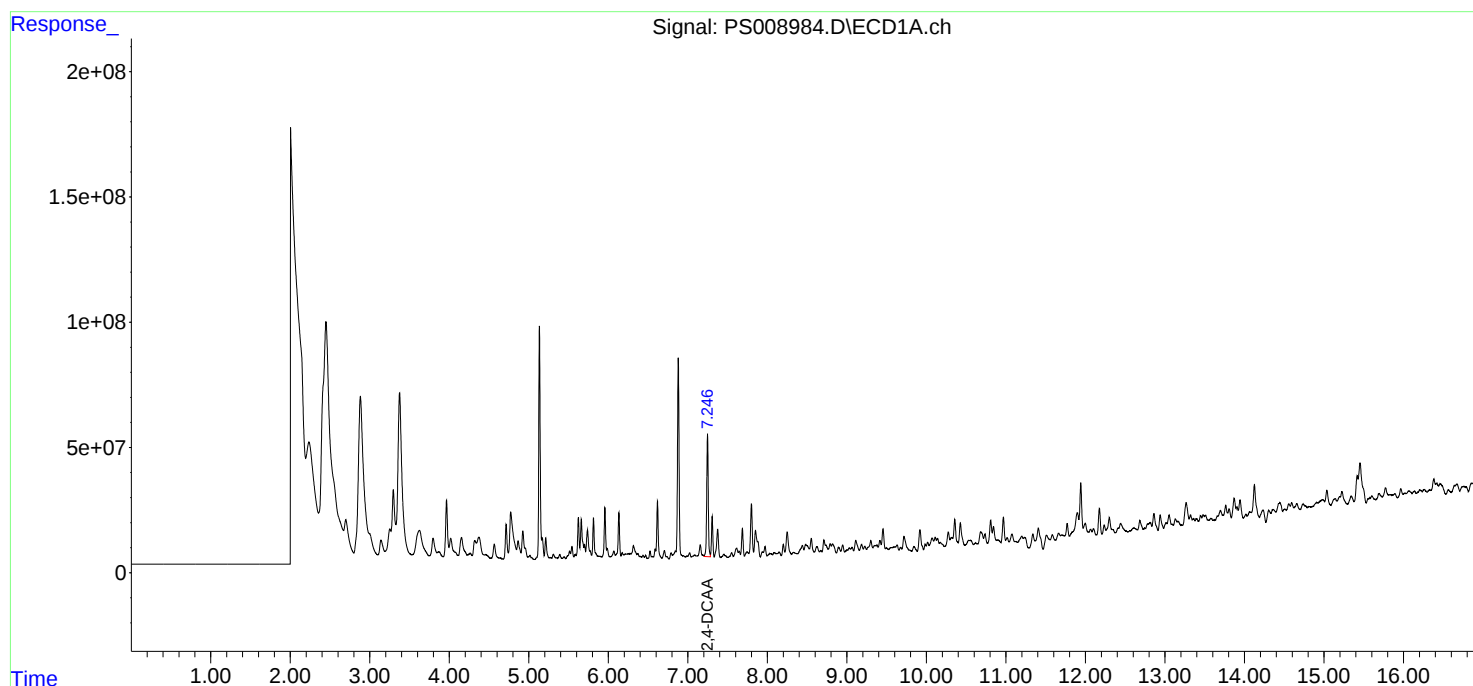

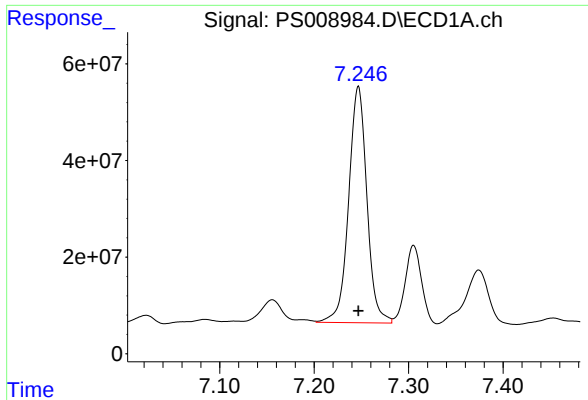


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 656989311
Conc: 300.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
LIED-TS003-01

Manual Integrations
APPROVED

Sohil
2/26/2020 12:24:20 PM

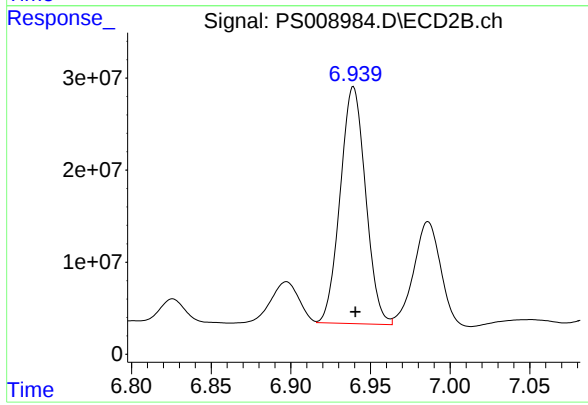

#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 285430343
Conc: 296.23 ng/ml m