

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022425\
 Data File : PS029271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2025 17:47
 Operator : AR\AJ
 Sample : Q1397-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 STOCK-PILE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/25/2025
 Supervised By :Ankita Jodhani 02/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 00:57:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.156	7.630	2039.3E6	262.0E6	494.914	278.669m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022425\
Data File : PS029271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2025 17:47
Operator : AR\AJ
Sample : Q1397-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
STOCK-PILE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/25/2025
Supervised By :Ankita Jodhani 02/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 00:57:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

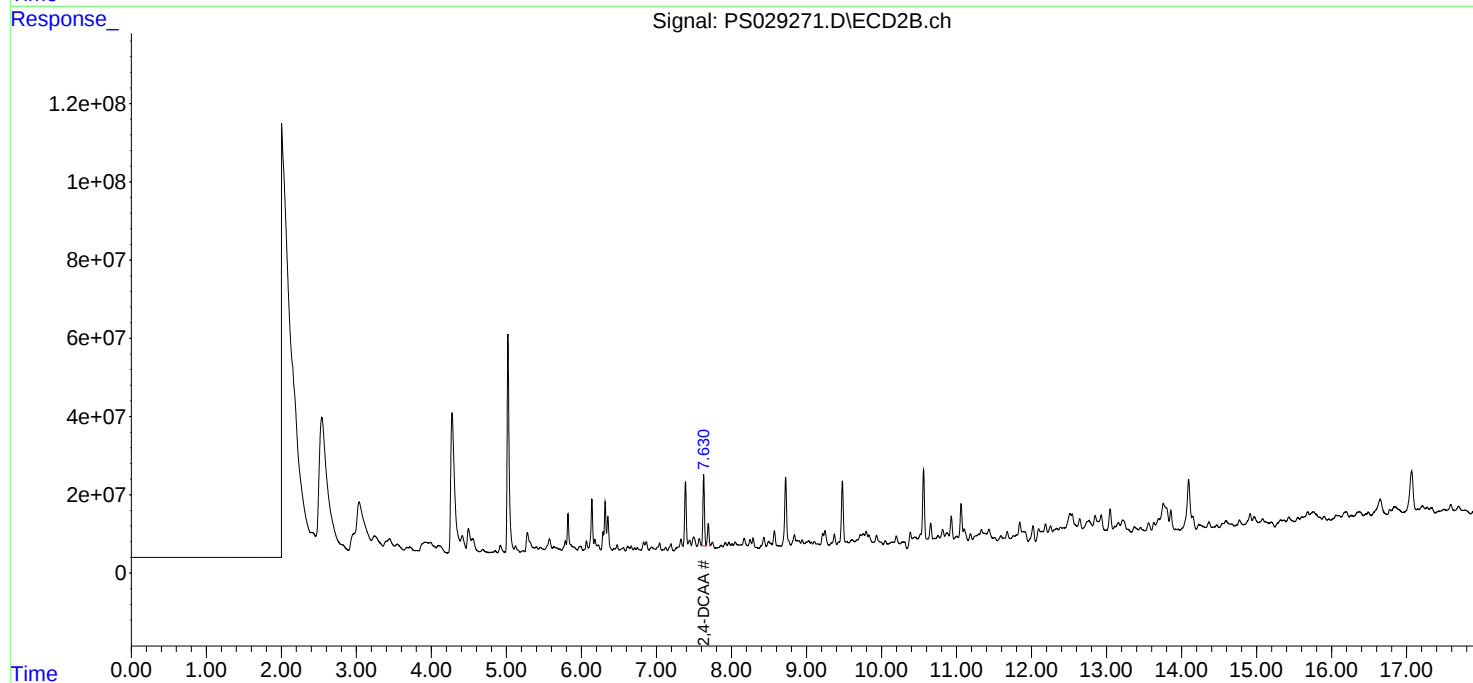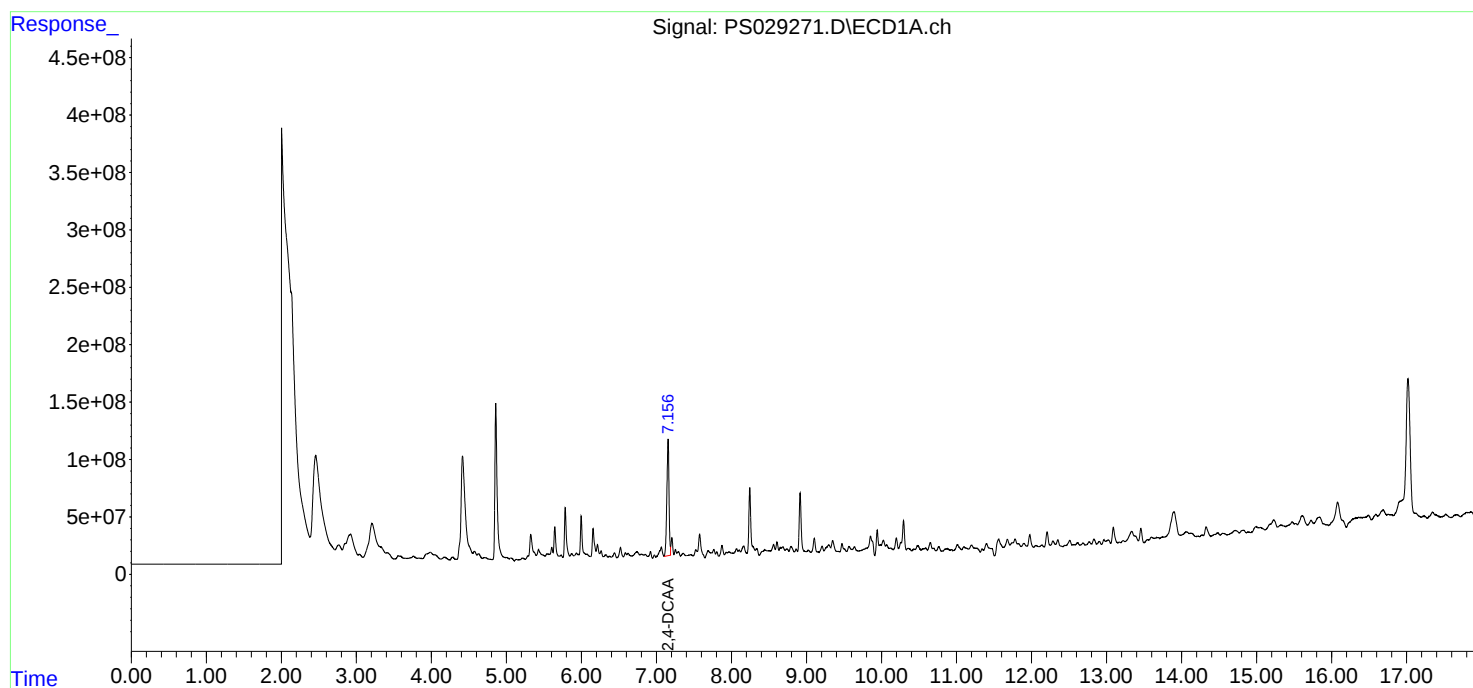

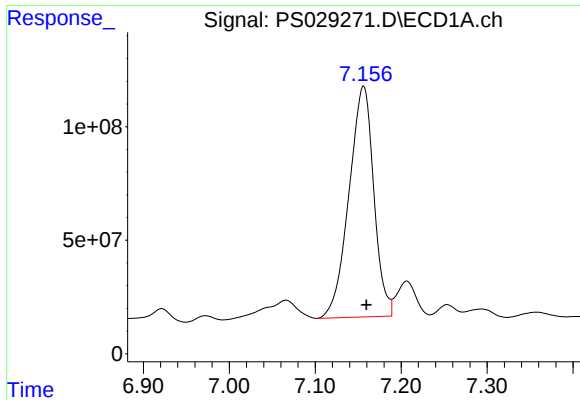

#4 2,4-DCAA

R.T.: 7.156 min
Delta R.T.: -0.004 min
Response: 2039329736
Conc: 494.91 ng/ml


Instrument :

ECD_S

ClientSampleId :
STOCK-PILE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/25/2025
Supervised By :Ankita Jodhani 02/25/2025

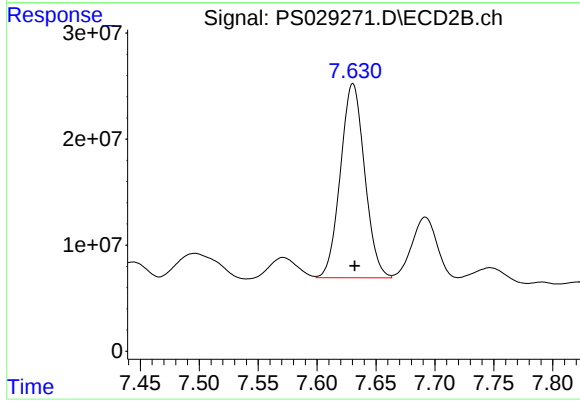

#4 2,4-DCAA

R.T.: 7.630 min
Delta R.T.: -0.002 min
Response: 262041265
Conc: 278.67 ng/ml m