

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022425\
 Data File : PS029274.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Feb 2025 18:59
 Operator : AR\AJ
 Sample : Q1397-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/25/2025
 Supervised By :Ankita Jodhani 02/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 00:58:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.155	7.629	4144.7E6	532.5E6	1005.864m	566.330m#

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022425\
Data File : PS029274.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Feb 2025 18:59
Operator : AR\AJ
Sample : Q1397-03
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP7


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/25/2025
Supervised By : Ankita Jodhani 02/25/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 00:58:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

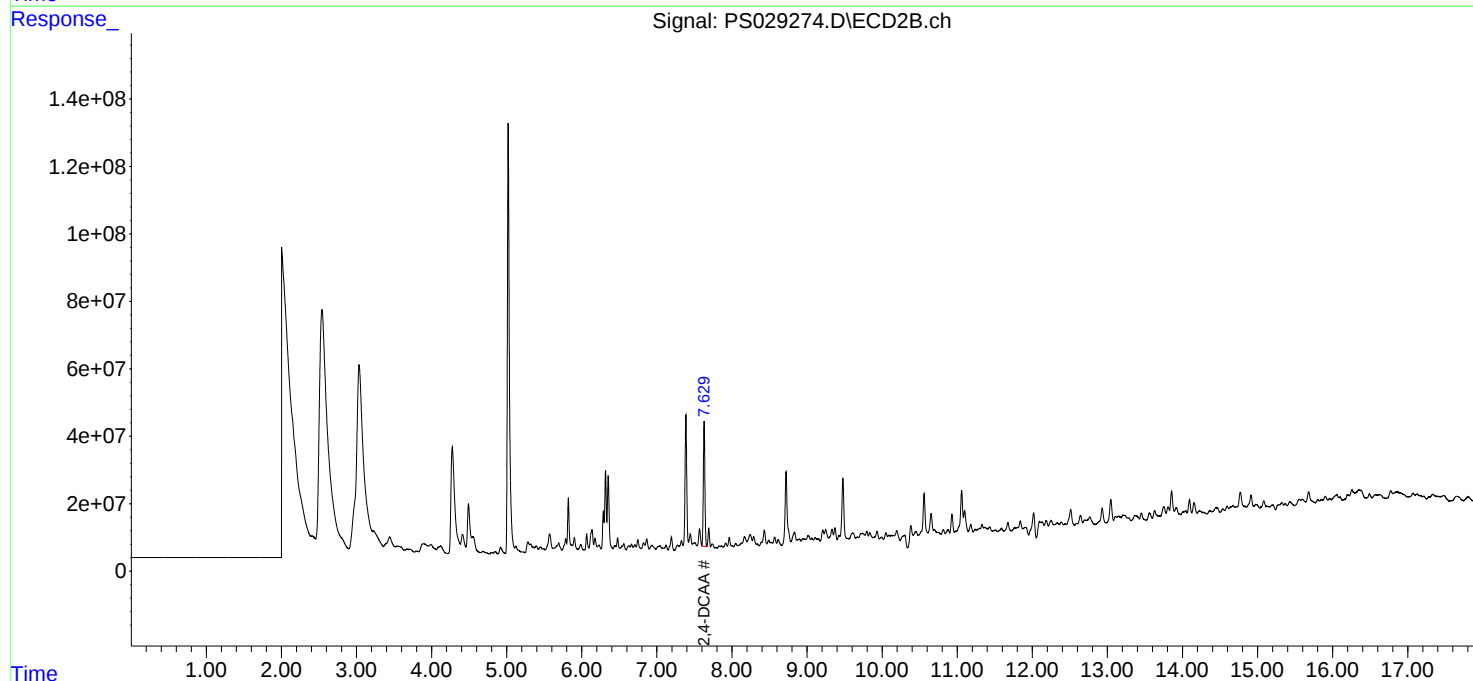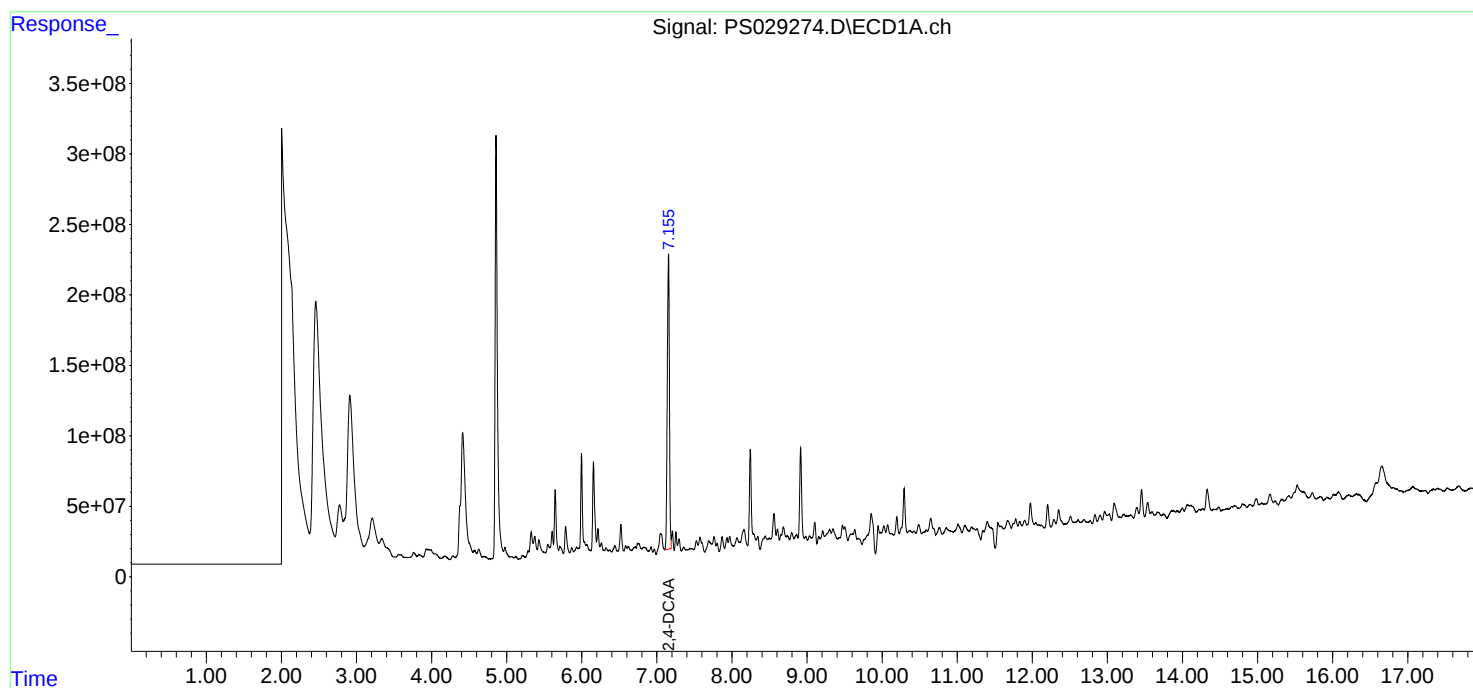

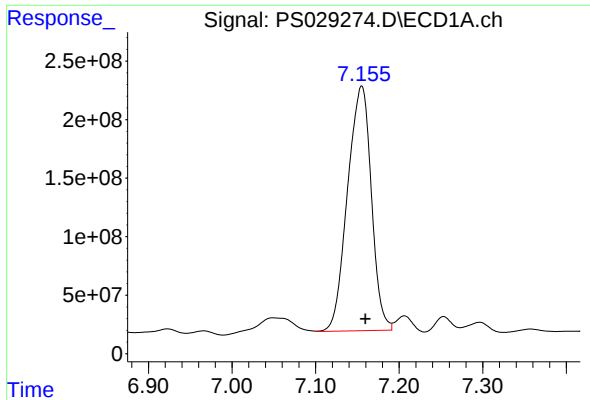


#4 2,4-DCAA

R.T.: 7.155 min
Delta R.T.: -0.005 min
Response: 4144739416
Conc: 1005.86 ng/m

Instrument :
ECD_S
ClientSampleId :
TP7

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/25/2025
Supervised By :Ankita Jodhani 02/25/2025

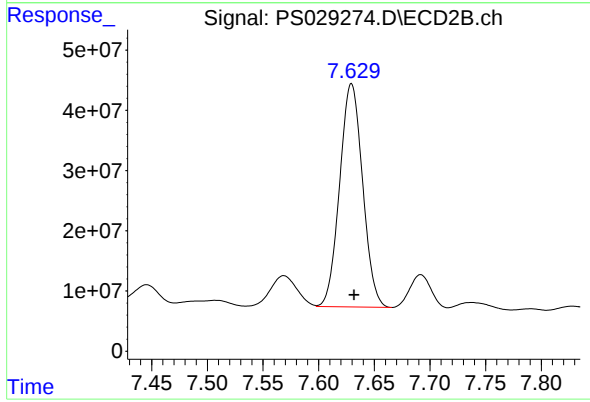

#4 2,4-DCAA

R.T.: 7.629 min
Delta R.T.: -0.003 min
Response: 532538485
Conc: 566.33 ng/ml m