

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022519\
 Data File : PS003326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 12:26
 Operator : EI\SJ
 Sample : K1334-06RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NB-07-022019-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 13:03:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.284	10.773	68857286	93026798	181.375	217.583
Target Compounds							
2) T	3,5-DICHL...	0.000	9.019	0	2016075	N.D.	3.577 #
6) T	MCCP	11.971	0.000	10952025	0	9.141	N.D. #
12) T	2,4,5-T	0.000	14.401	0	6406714	N.D.	3.348 #
15) T	Picloram	16.843	16.712	9427777	14852227	2.980	4.940 #
16) T	DCPA	0.000	16.635	0	2977641	N.D.	0.961 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022519\
Data File : PS003326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 12:26
Operator : EI\SJ
Sample : K1334-06RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
NB-07-022019-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 13:03:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

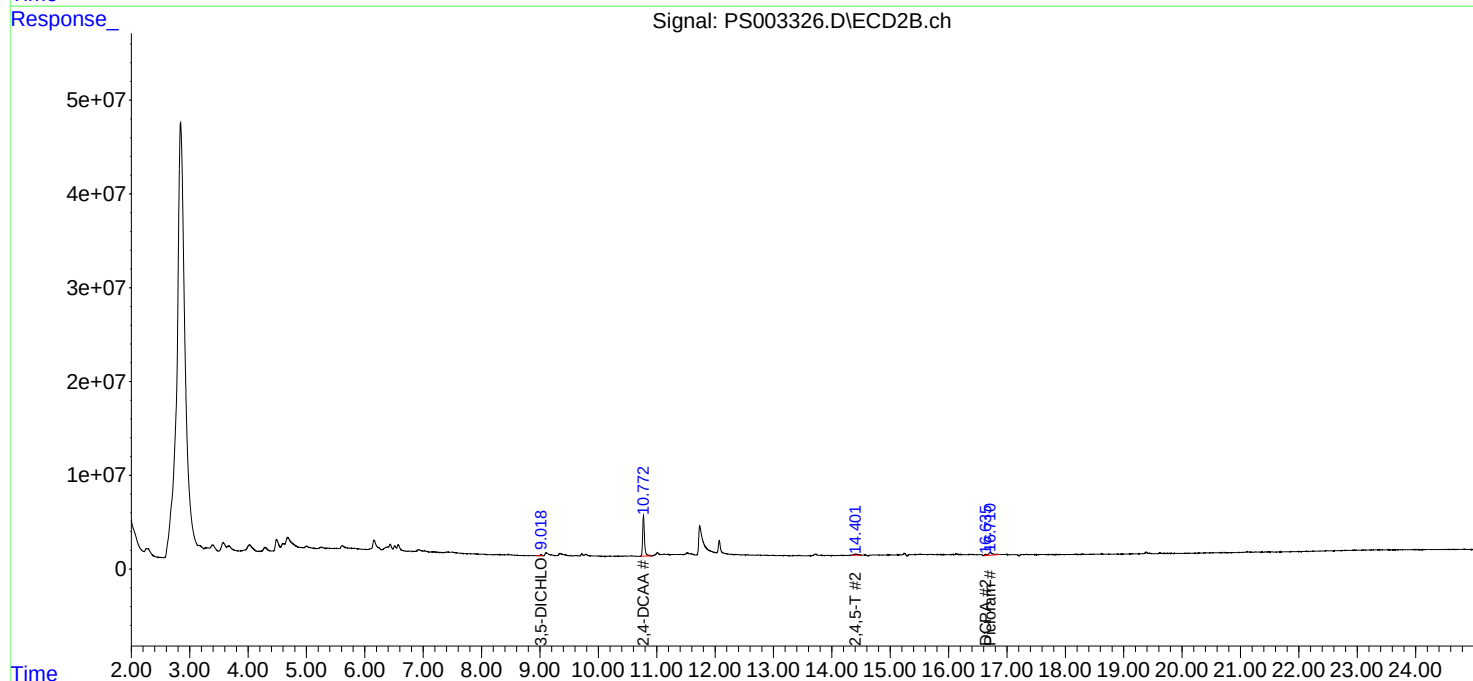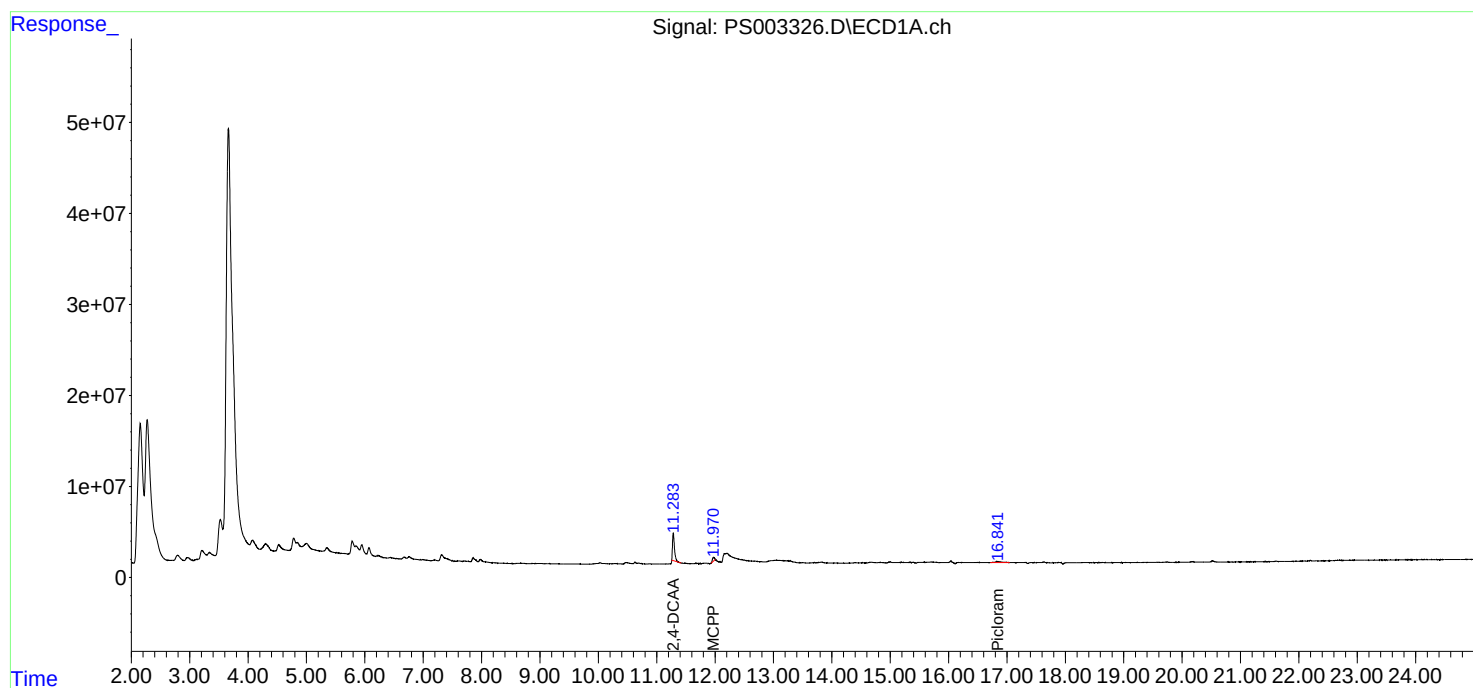


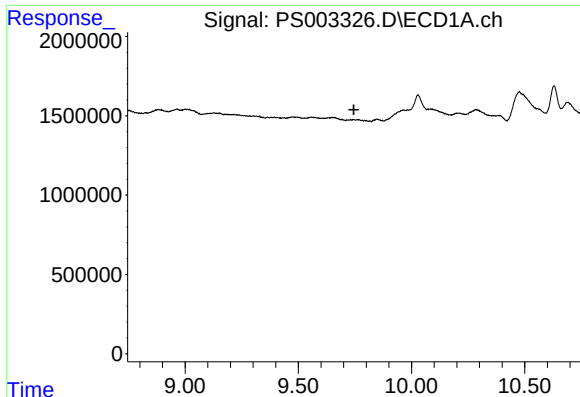

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-07-022019-A

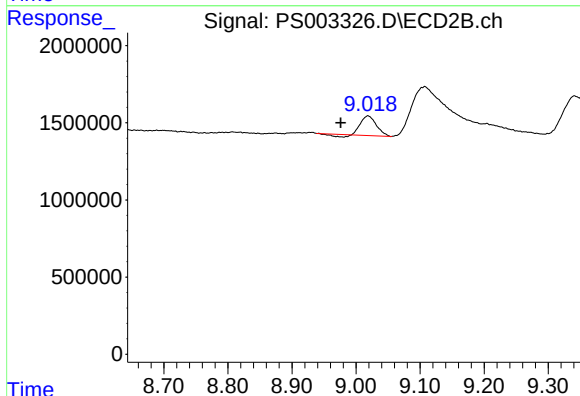


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.019 min
Delta R.T.: 0.042 min
Response: 2016075
Conc: 3.58 ng/ml

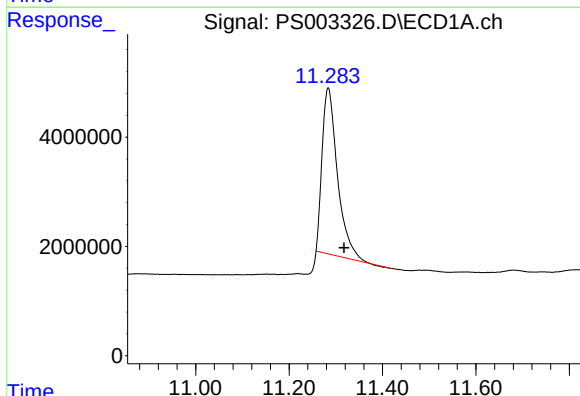


#4 2,4-DCAA

R.T.: 11.284 min
Delta R.T.: -0.034 min
Response: 68857286
Conc: 181.37 ng/ml

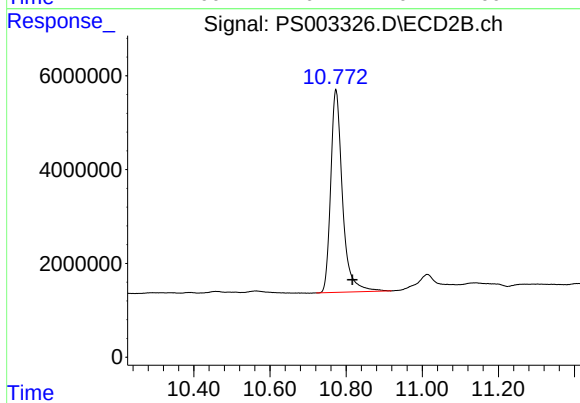

#4 2,4-DCAA


R.T.: 10.773 min
Delta R.T.: -0.043 min
Response: 93026798
Conc: 217.58 ng/ml

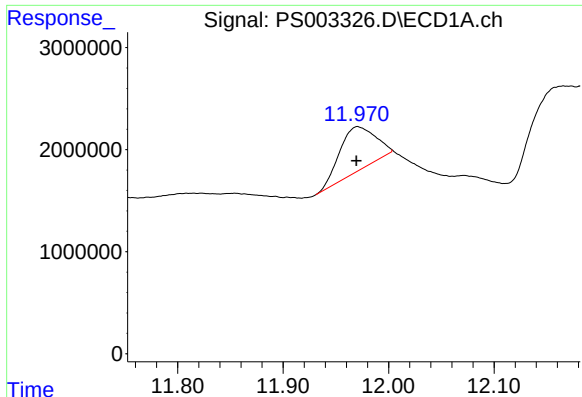

#6 MCP


R.T.: 11.971 min
Delta R.T.: 0.002 min
Response: 10952025
Conc: 9.14 ug/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-022019-A

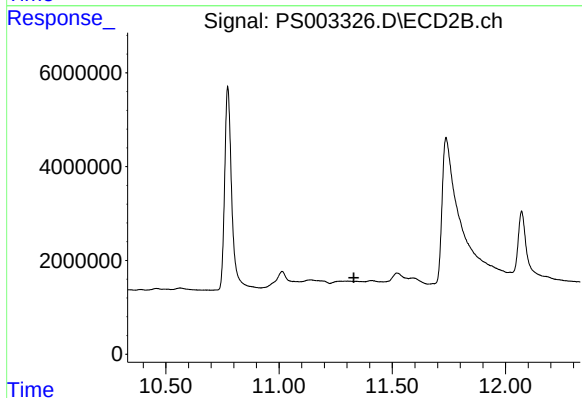


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.330 min
Response: 0
Conc: N.D.

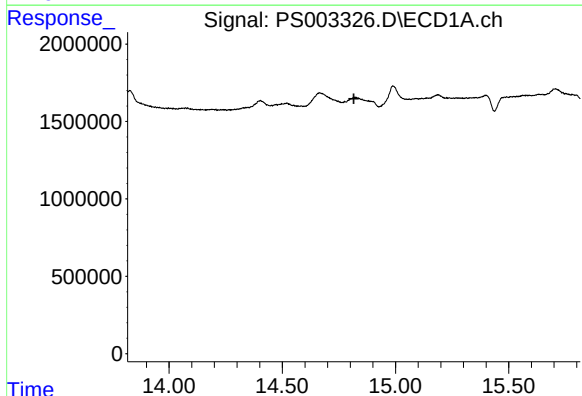


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

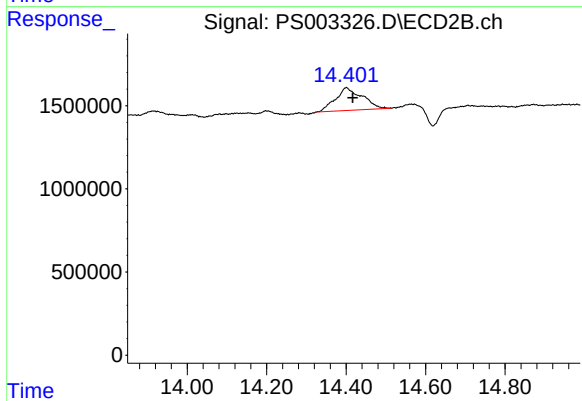

#12 2,4,5-T


R.T.: 14.401 min
Delta R.T.: -0.016 min
Response: 6406714
Conc: 3.35 ng/ml

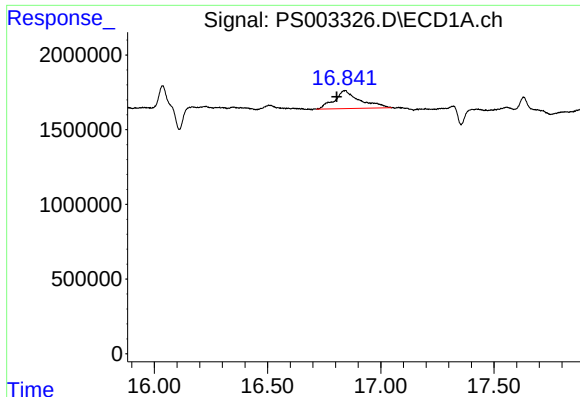

#15 Picloram


R.T.: 16.843 min
Delta R.T.: 0.038 min
Response: 9427777
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-07-022019-A

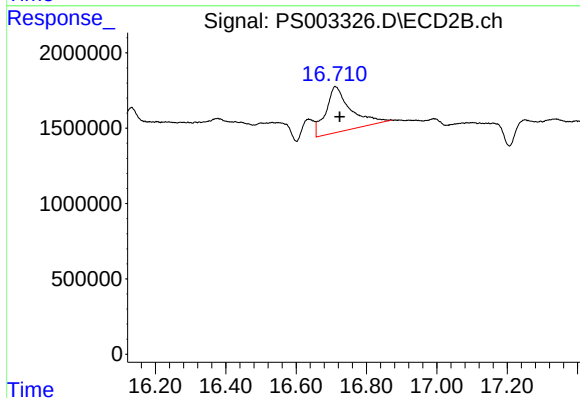


#15 Picloram

R.T.: 16.712 min
Delta R.T.: -0.013 min
Response: 14852227
Conc: 4.94 ng/ml

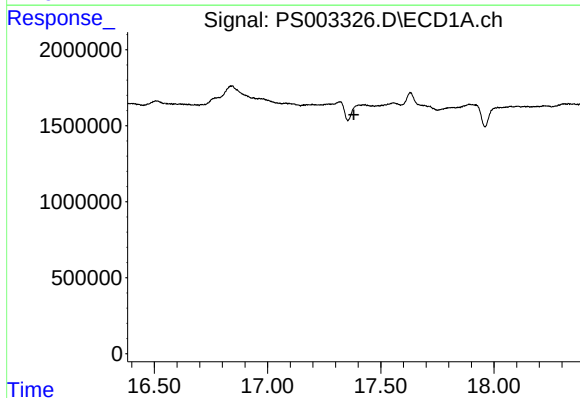

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

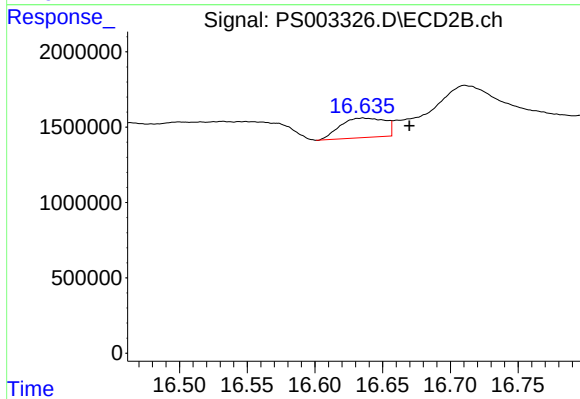

#16 DCPA

R.T.: 16.635 min
Delta R.T.: -0.034 min
Response: 2977641
Conc: 0.96 ng/ml