

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022519\
 Data File : PS003330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 18:58
 Operator : EI\SJ
 Sample : K1556-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:54:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.795	150.7E6	156.1E6	397.033	365.090
Target Compounds							
1) T	Dalapon	0.000	2.298	0	3400371	N.D.	6.345 #
7) T	MCPA	12.163	11.758	31113036	17303050	17.578	11.000 #
15) T	Picloram	0.000	16.737	0	6465746	N.D.	2.151 #
16) T	DCPA	0.000	16.737	0	6465746	N.D.	2.087 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022519\
Data File : PS003330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 18:58
Operator : EI\SJ
Sample : K1556-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:54:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

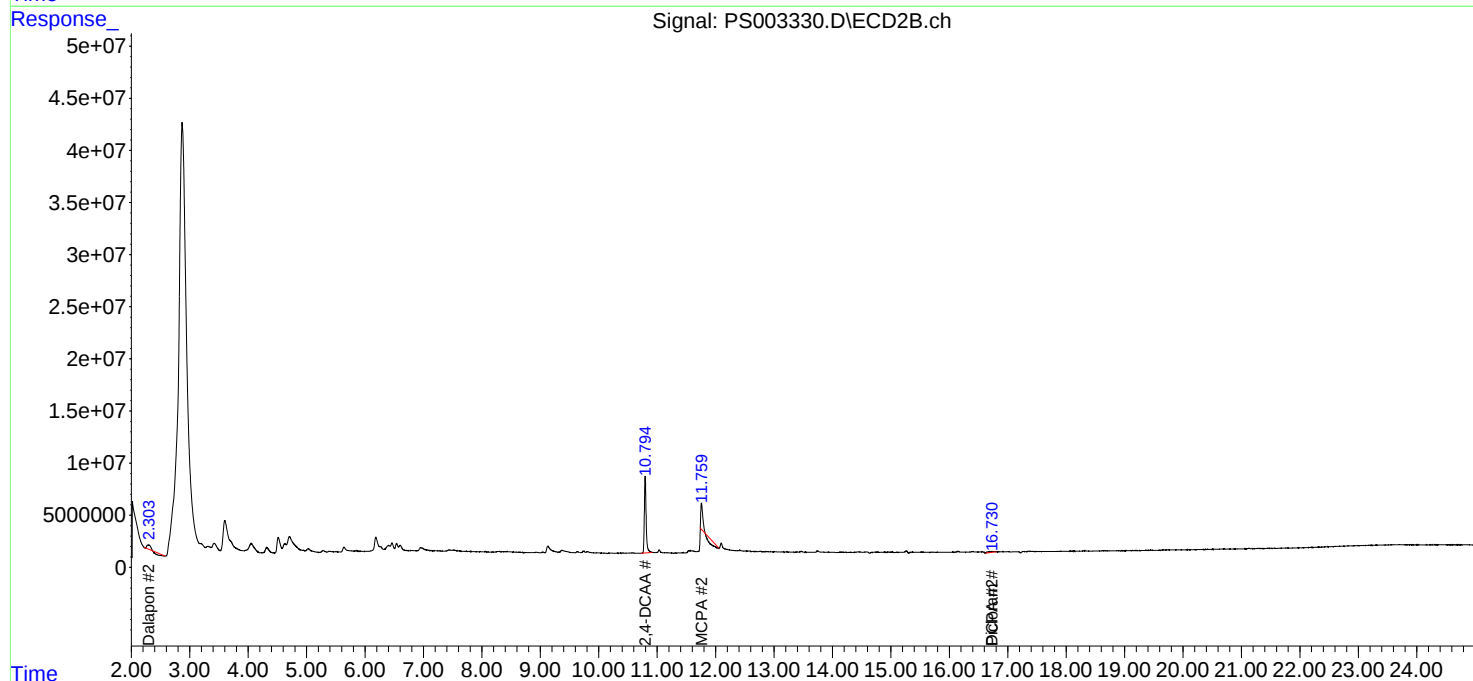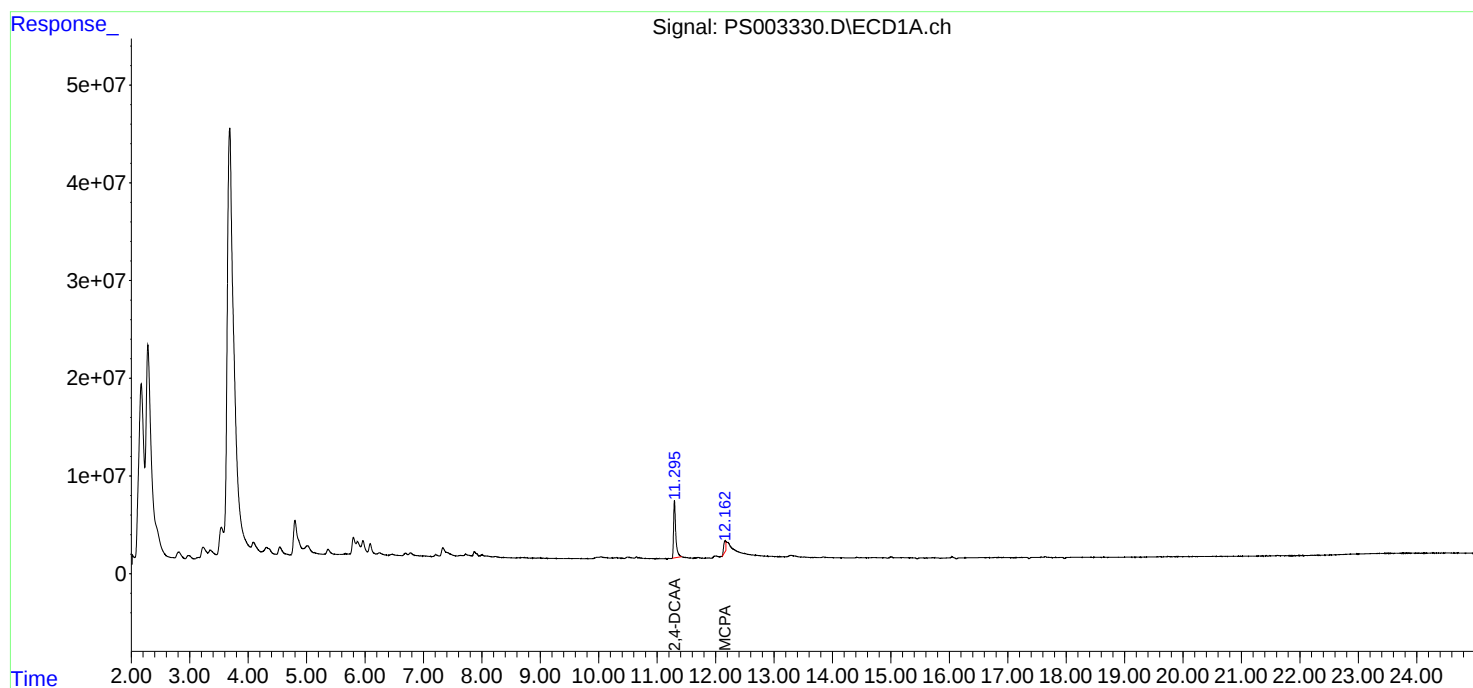


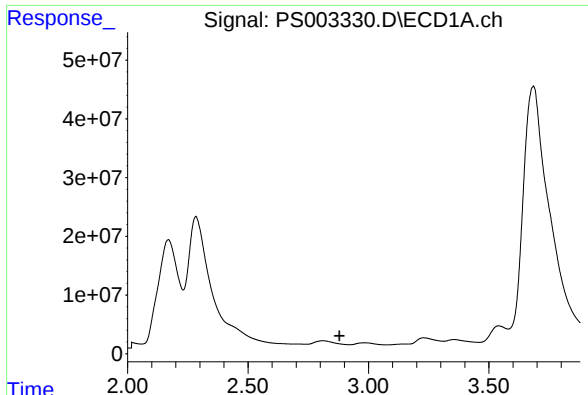

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP

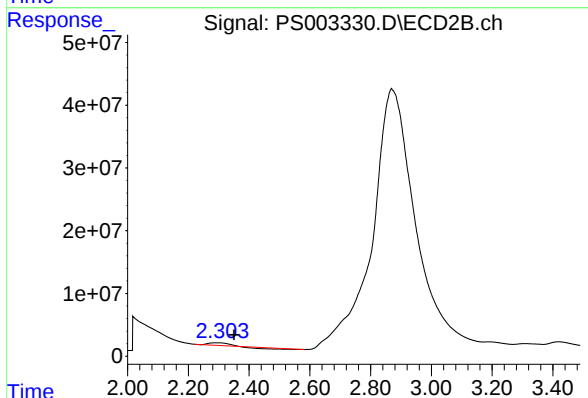


#1 Dalapon

R.T.: 2.298 min
Delta R.T.: -0.053 min
Response: 3400371
Conc: 6.34 ng/ml

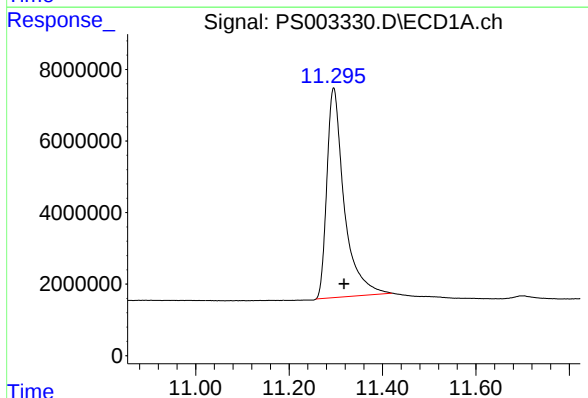


#4 2,4-DCAA

R.T.: 11.296 min
Delta R.T.: -0.022 min
Response: 150729810
Conc: 397.03 ng/ml

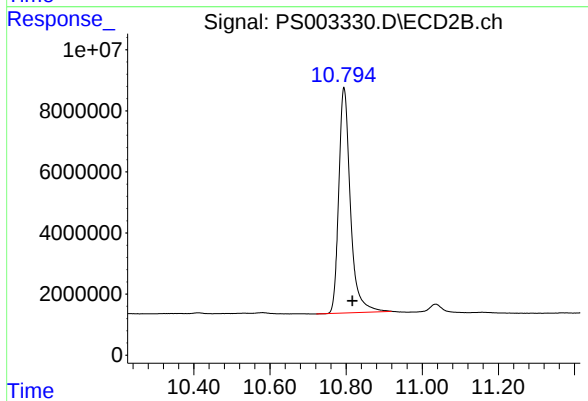

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: -0.022 min
Response: 156092519
Conc: 365.09 ng/ml

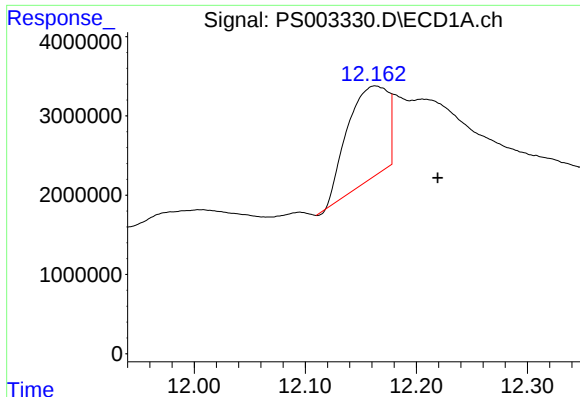

#7 MCPA


R.T.: 12.163 min
Delta R.T.: -0.056 min
Response: 31113036
Conc: 17.58 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP

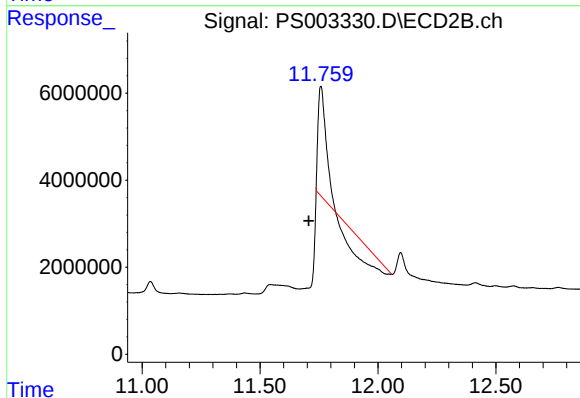


#7 MCPA

R.T.: 11.758 min
Delta R.T.: 0.052 min
Response: 17303050
Conc: 11.00 ug/ml

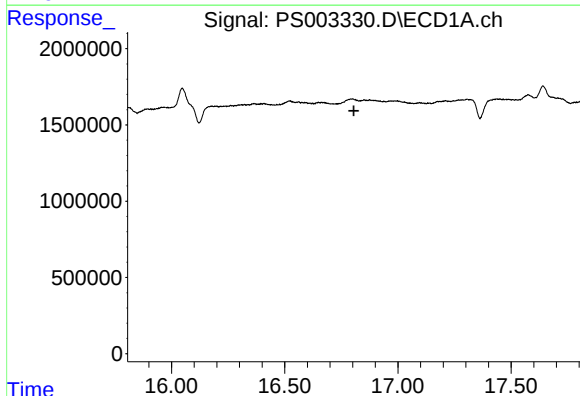


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

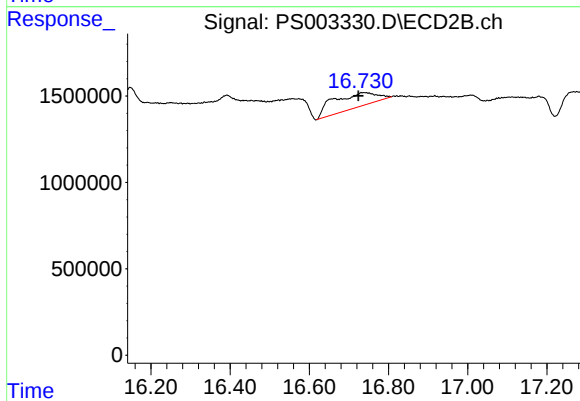

#15 Picloram


R.T.: 16.737 min
Delta R.T.: 0.013 min
Response: 6465746
Conc: 2.15 ng/ml

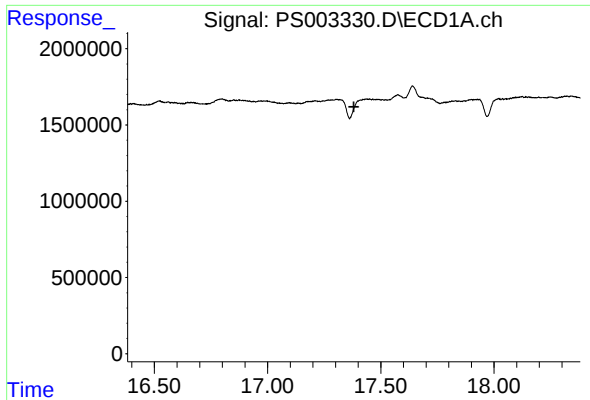

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP

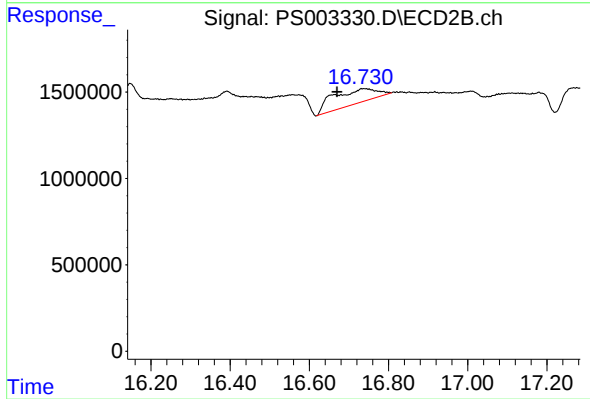

#16 DCPA

R.T.: 16.737 min
Delta R.T.: 0.067 min
Response: 6465746
Conc: 2.09 ng/ml