

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022519\
 Data File : PS003334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2019 21:02
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:55:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.785	0	330.7E6	N.D.	773.515 #
Target Compounds							
1) T	Dalapon	2.848	2.320	179.3E6	389.6E6	325.107	727.031 #
2) T	3,5-DICHL...	0.000	8.945	0	255.6E6	N.D.	453.487 #
3) T	4-Nitroph...	10.884	9.937	139.2E6	150.3E6	719.248	718.929
5) T	DICAMBA	0.000	11.064	0	621.3E6	N.D.	391.551 #
8) T	DICHLORPROP	0.000	12.190	0	280.9E6	N.D.	734.693 #
9) T	2,4-D	0.000	12.663	0	326.1E6	N.D.	650.322 #
10) T	Pentachlo...	0.000	13.195	0	1251.0E6	N.D.	202.405 #
11) T	2,4,5-TP ...	14.382	13.821	1922.5E6	1823.0E6	763.408	734.957
12) T	2,4,5-T	14.784	14.386	1840.1E6	1185.0E6	754.305	619.296
14) T	DINOSEB	16.993	15.460	1478.3E6	-293967440	785.799	N.D. #
15) T	Picloram	16.775	16.693	1894.0E6	1764.0E6	598.671	586.752
16) T	DCPA	0.000	16.693	0	1764.0E6	N.D.	569.479 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022519\
Data File : PS003334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2019 21:02
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:55:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

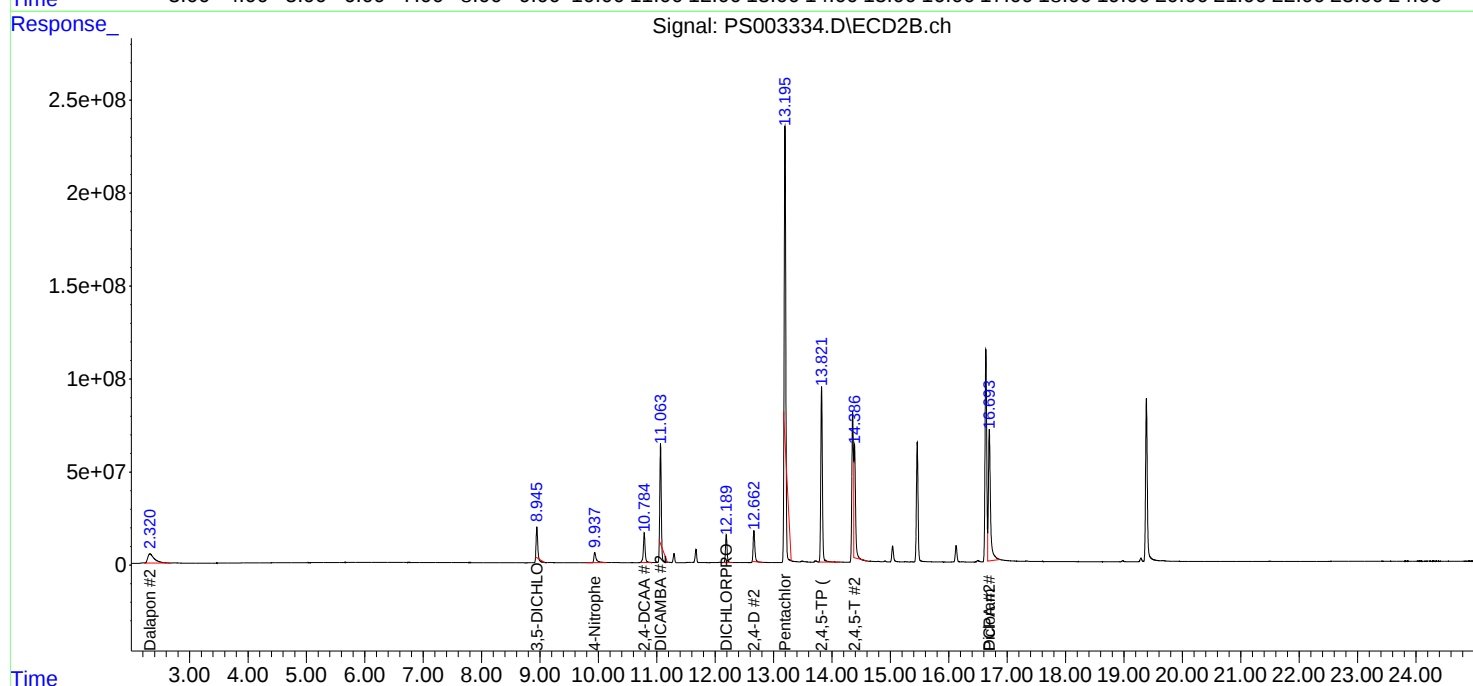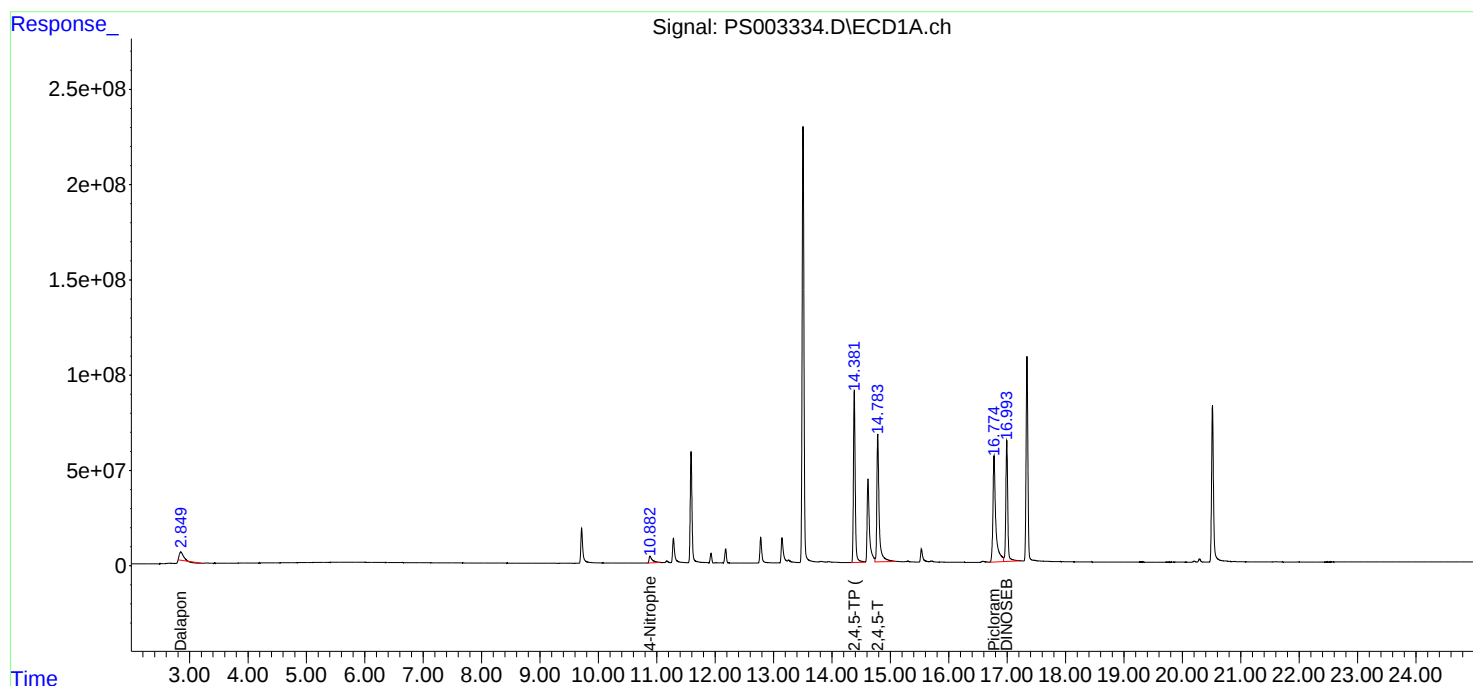


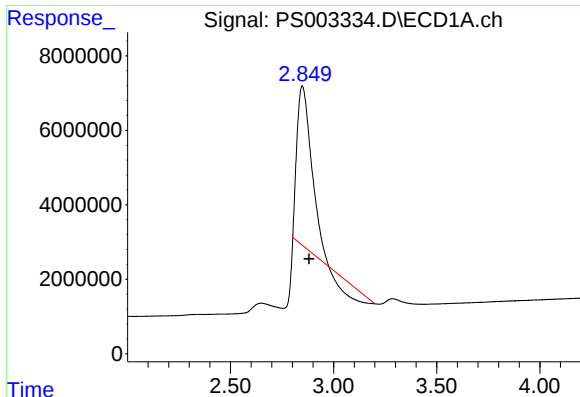

#1 Dalapon


R.T.: 2.848 min
Delta R.T.: -0.032 min
Response: 179344498
Conc: 325.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

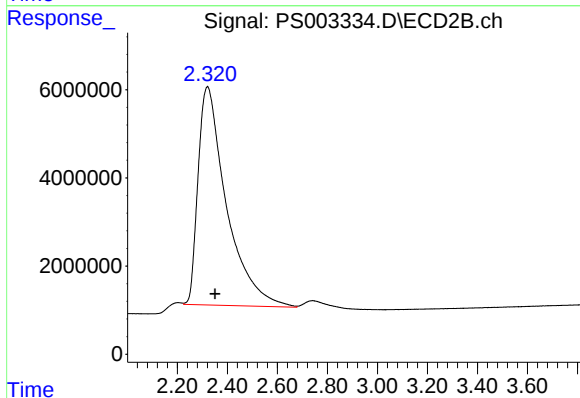


#1 Dalapon

R.T.: 2.320 min
Delta R.T.: -0.030 min
Response: 389631694
Conc: 727.03 ng/ml

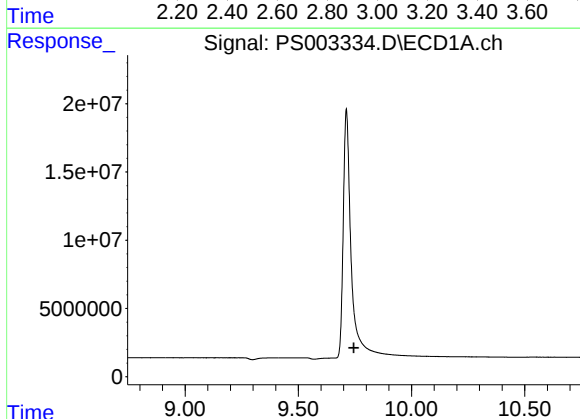


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

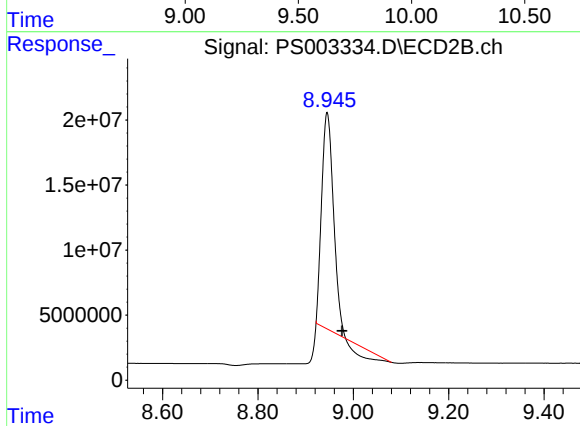

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: -0.031 min
Response: 255570793
Conc: 453.49 ng/ml

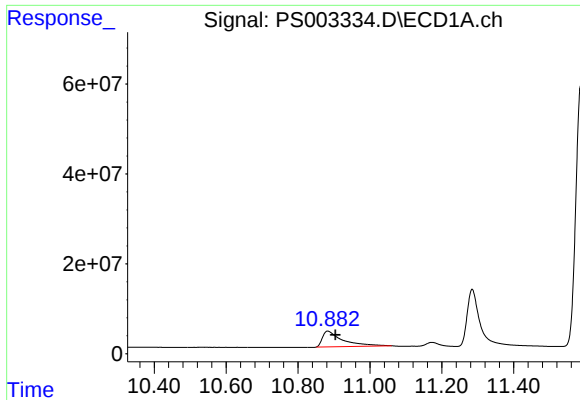

#3 4-Nitrophenol


R.T.: 10.884 min
Delta R.T.: -0.020 min
Response: 139202714
Conc: 719.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

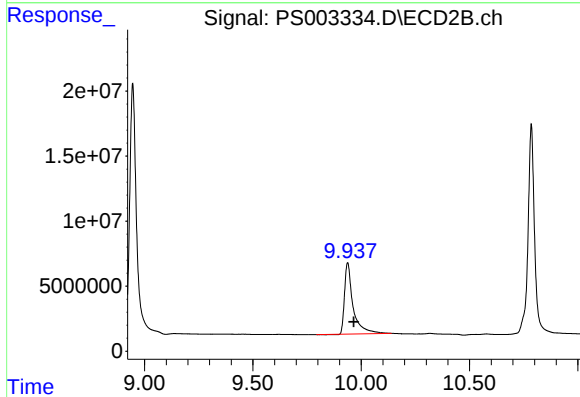


#3 4-Nitrophenol

R.T.: 9.937 min
Delta R.T.: -0.028 min
Response: 150272287
Conc: 718.93 ng/ml

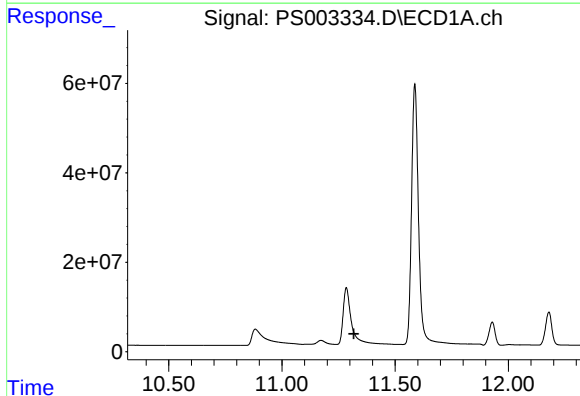


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.318 min
Response: 0
Conc: N.D.

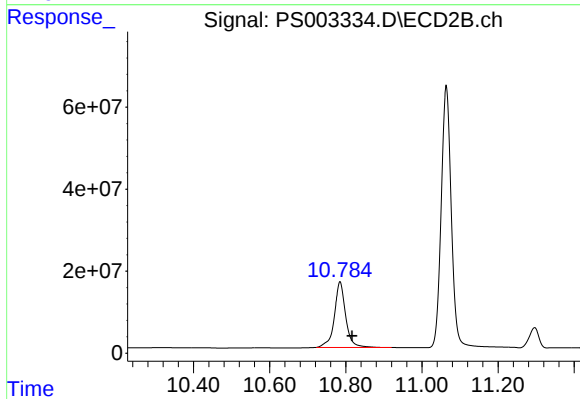

#4 2,4-DCAA


R.T.: 10.785 min
Delta R.T.: -0.032 min
Response: 330712991
Conc: 773.51 ng/ml

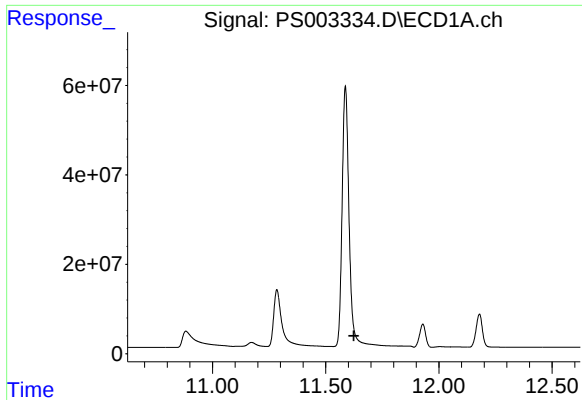

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.624 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

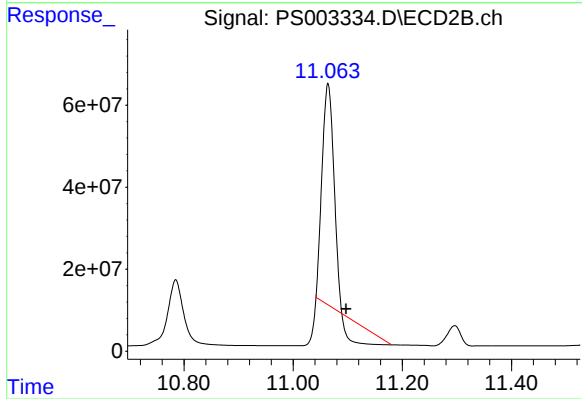


#5 DICAMBA

R.T.: 11.064 min
Delta R.T.: -0.033 min
Response: 621260148
Conc: 391.55 ng/ml

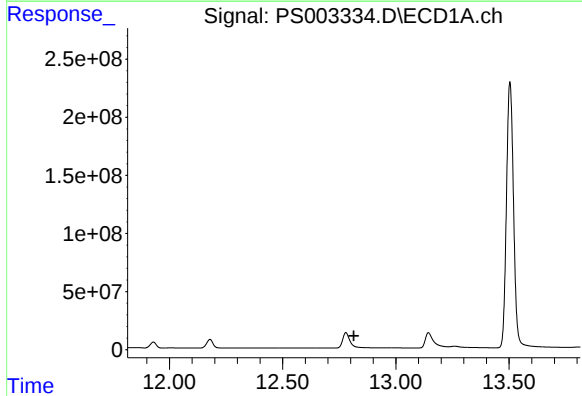


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

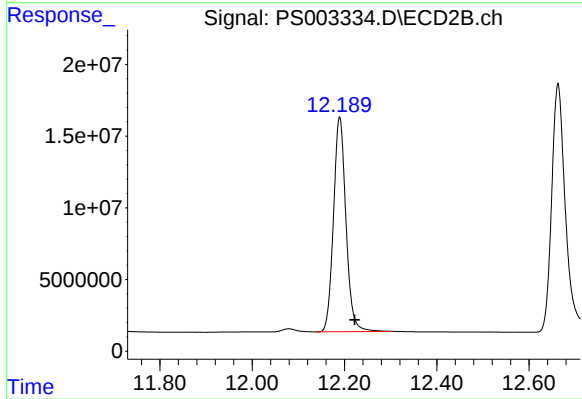

#8 DICHLORPROP


R.T.: 12.190 min
Delta R.T.: -0.033 min
Response: 280903426
Conc: 734.69 ng/ml

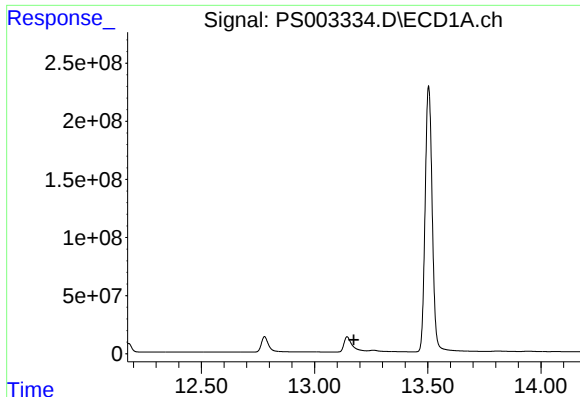

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

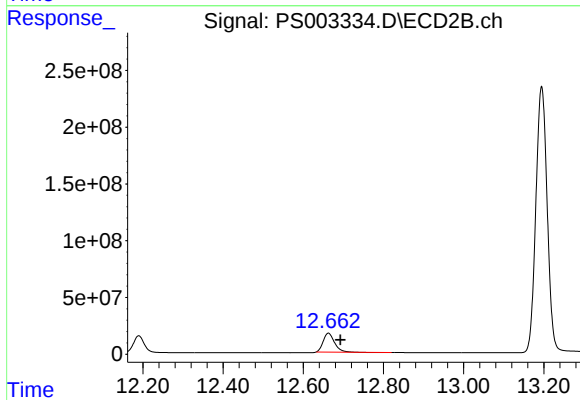


#9 2,4-D

R.T.: 12.663 min
Delta R.T.: -0.030 min
Response: 326062433
Conc: 650.32 ng/ml

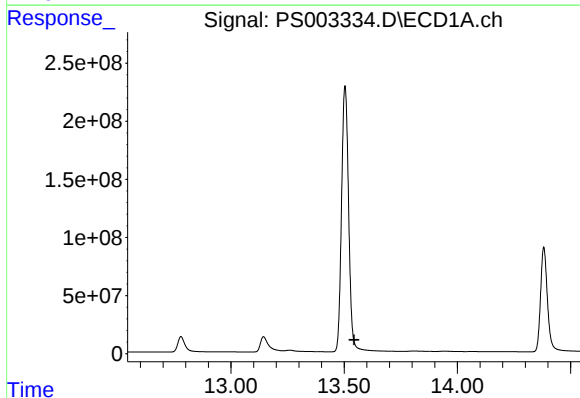


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.543 min
Response: 0
Conc: N.D.

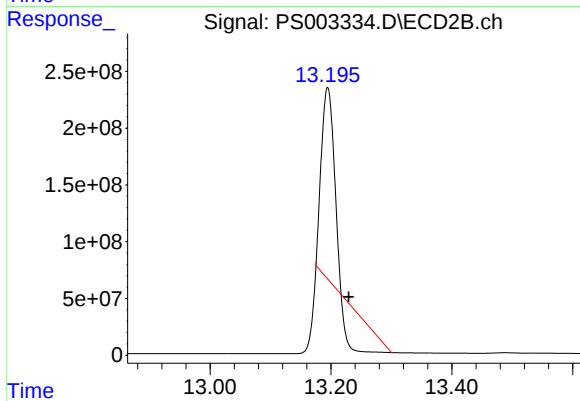

#10 Pentachlorophenol


R.T.: 13.195 min
Delta R.T.: -0.035 min
Response: 1250983461
Conc: 202.40 ng/ml

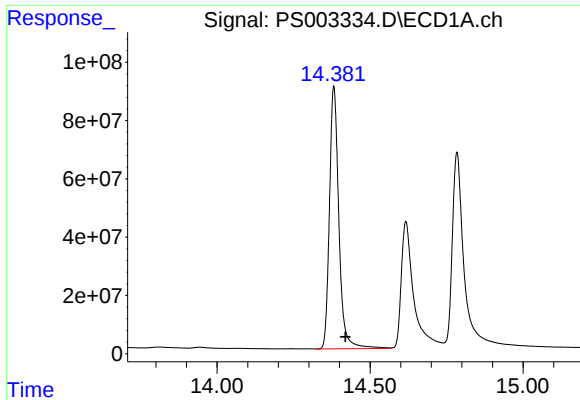

#11 2,4,5-TP (SILVEX)


R.T.: 14.382 min
Delta R.T.: -0.038 min
Response: 1922546168
Conc: 763.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

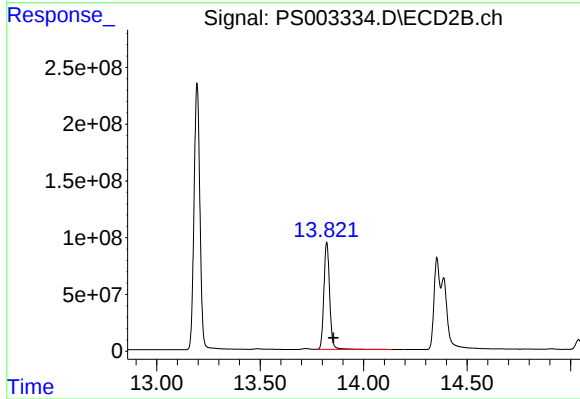


#11 2,4,5-TP (SILVEX)

R.T.: 13.821 min
Delta R.T.: -0.033 min
Response: 1822955006
Conc: 734.96 ng/ml

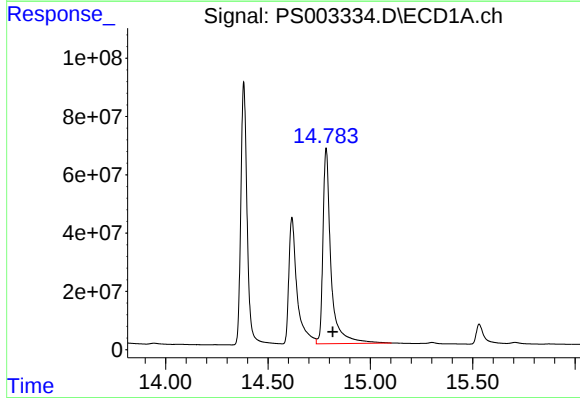


#12 2,4,5-T

R.T.: 14.784 min
Delta R.T.: -0.032 min
Response: 1840055791
Conc: 754.31 ng/ml

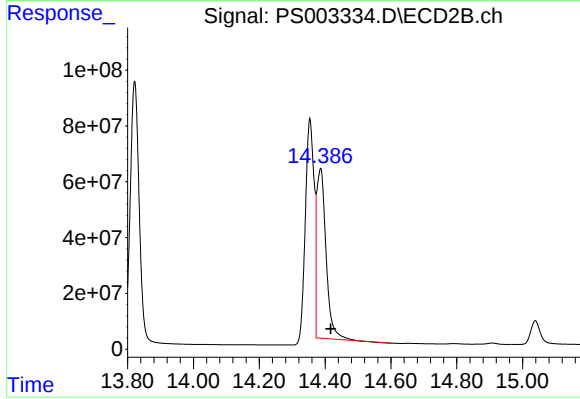

#12 2,4,5-T


R.T.: 14.386 min
Delta R.T.: -0.031 min
Response: 1185015313
Conc: 619.30 ng/ml

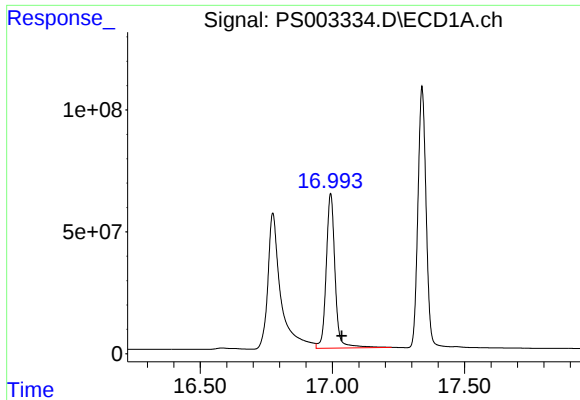

#14 DINOSEB


R.T.: 16.993 min
Delta R.T.: -0.042 min
Response: 1478345099
Conc: 785.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

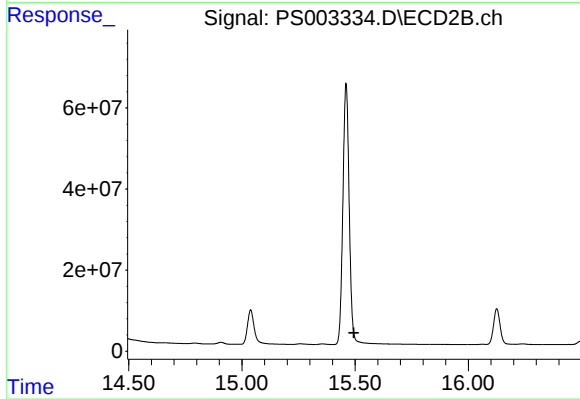


#14 DINOSEB

R.T.: 15.460 min
Delta R.T.: -0.035 min
Response: -293967440
Conc: N.D.

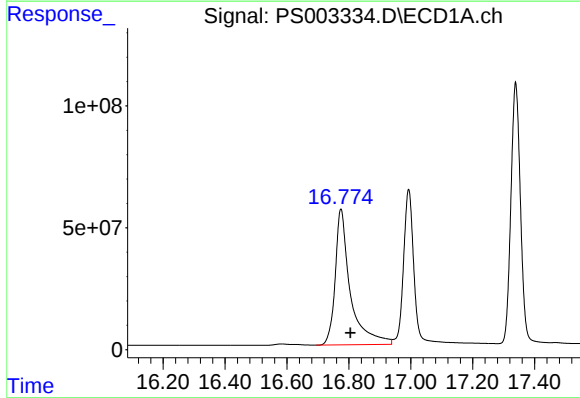


#15 Picloram

R.T.: 16.775 min
Delta R.T.: -0.031 min
Response: 1893975872
Conc: 598.67 ng/ml

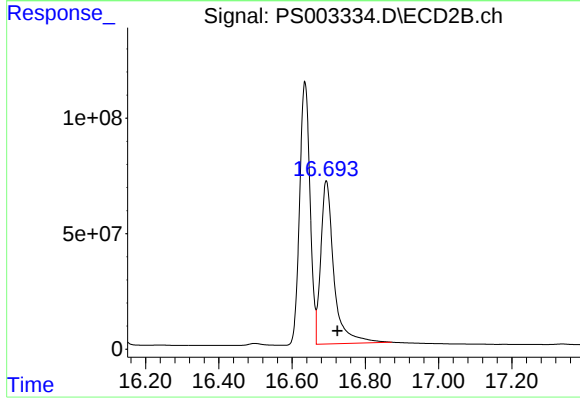

#15 Picloram


R.T.: 16.693 min
Delta R.T.: -0.031 min
Response: 1764013278
Conc: 586.75 ng/ml

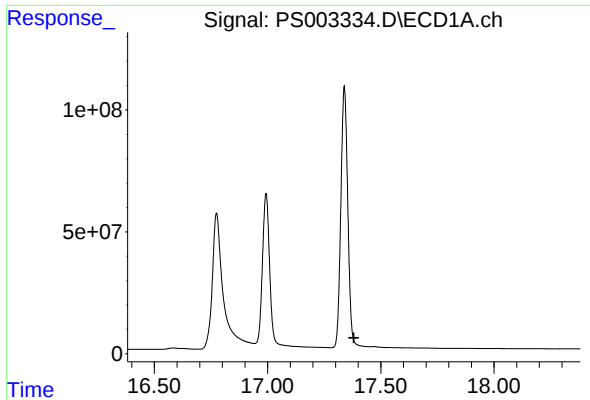

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

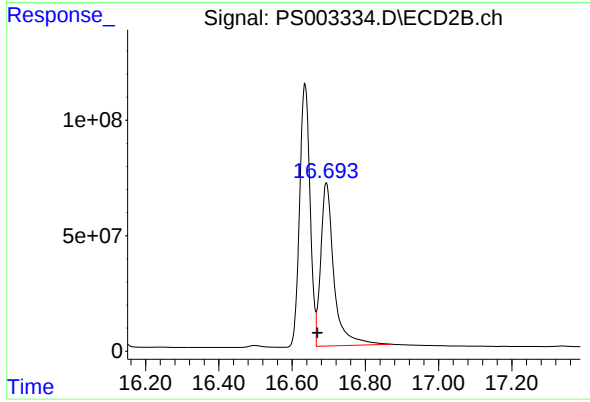

#16 DCPA

R.T.: 16.693 min
Delta R.T.: 0.024 min
Response: 1764013278
Conc: 569.48 ng/ml