

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
 Data File : PS008994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 09:23
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:20:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	919.8E6	479.6E6	420.655	497.705
Target Compounds							
12) T	2,4,5-T	0.000	9.259	0 42087858		N.D.	7.775
15) T	Picloram	11.044	11.031	156.3E6	91512021	11.413	12.594
16) T	DCPA	0.000	11.031	0 91512021		N.D.	13.226



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
Data File : PS008994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 09:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:20:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

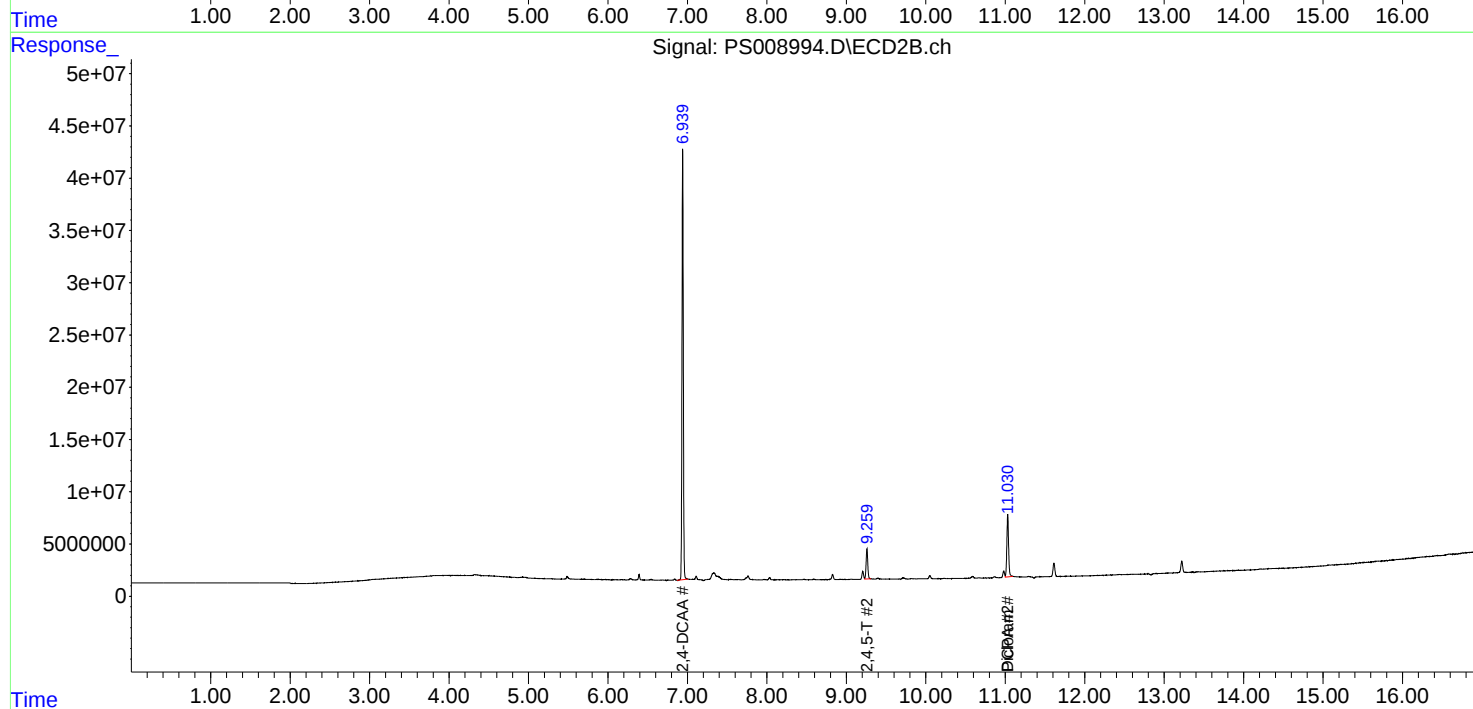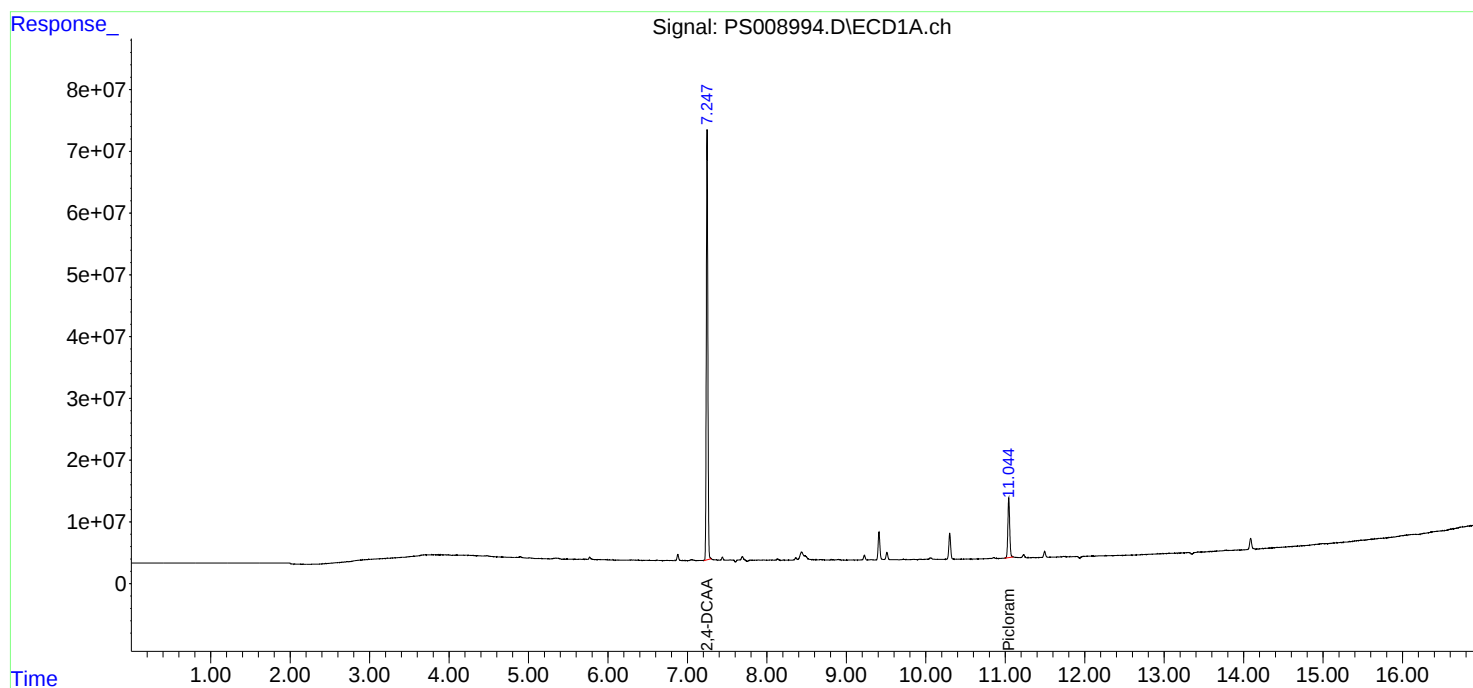


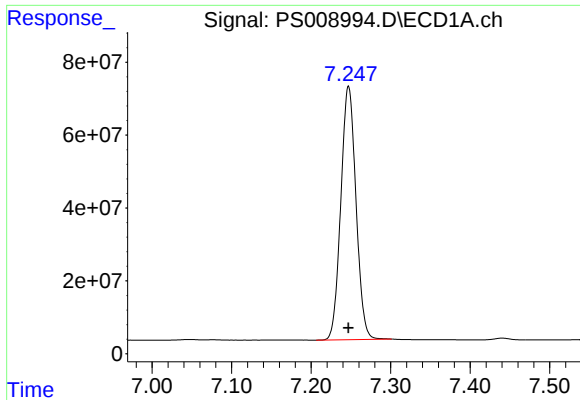

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 919800378
Conc: 420.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

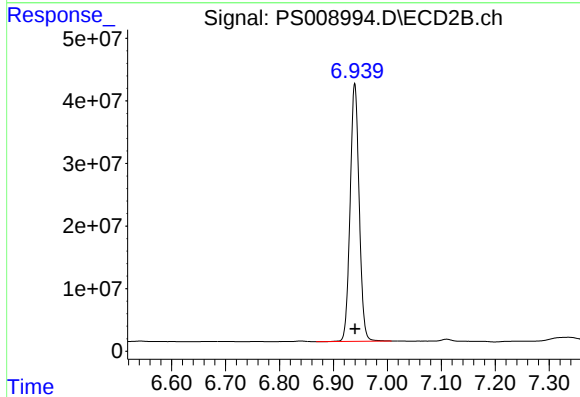


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 479566464
Conc: 497.71 ng/ml

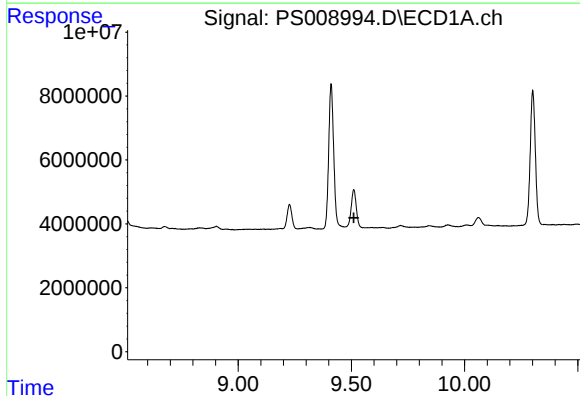


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

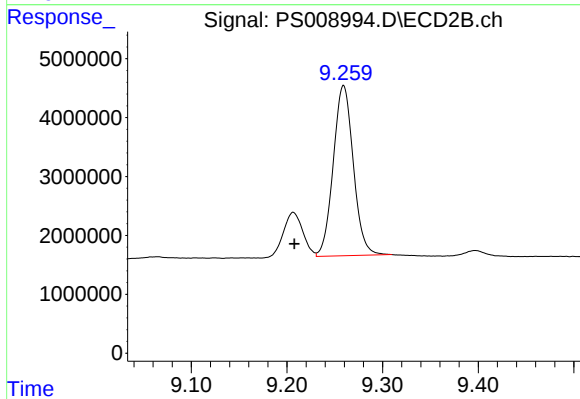

#12 2,4,5-T


R.T.: 9.259 min
Delta R.T.: 0.051 min
Response: 42087858
Conc: 7.78 ng/ml

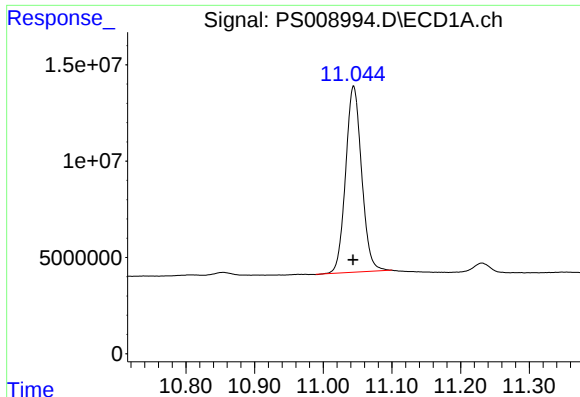

#15 Picloram


R.T.: 11.044 min
Delta R.T.: 0.001 min
Response: 156252270
Conc: 11.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

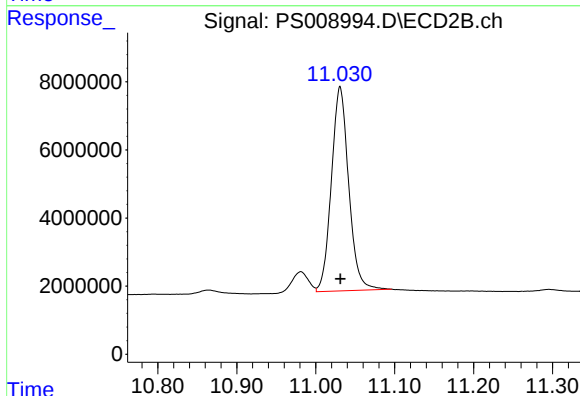


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 91512021
Conc: 12.59 ng/ml

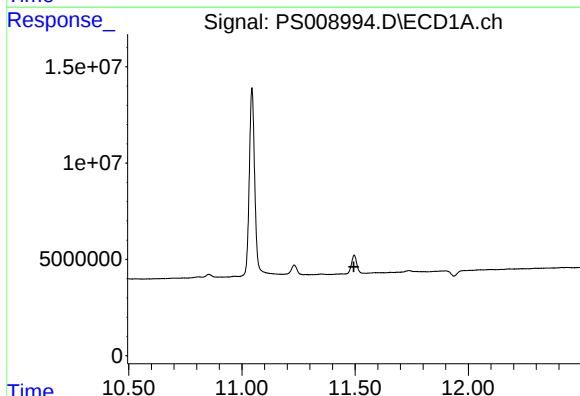

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

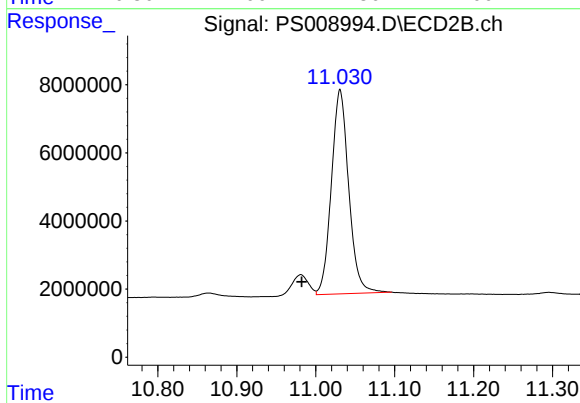

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.049 min
Response: 91512021
Conc: 13.23 ng/ml