

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
 Data File : PS009000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 17:10
 Operator : DD\AJ
 Sample : PB127074BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB127074BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:12:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	1033.8E6	517.6E6	472.795	537.175
Target Compounds							
1) T	Dalapon	0.000	2.591	0	256.7E6	N.D.	175.527
2) T	3,5-DICHL...	0.000	6.115	0	114.4E6	N.D.	78.412
5) T	DICAMBA	0.000	7.074	0	24327039	N.D.	5.877
7) T	MCPA	7.799	7.408	67257376	49142360	8.361	11.108 #
8) T	DICHLORPROP	0.000	7.761	0	29617002	N.D.	29.560
12) T	2,4,5-T	0.000	9.259	0	72681328	N.D.	13.427
15) T	Picloram	11.043	11.031	508.4E6	306.2E6	37.132	42.137
16) T	DCPA	0.000	10.981	0	18589721	N.D.	2.687



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
Data File : PS009000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 17:10
Operator : DD\AJ
Sample : PB127074BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB127074BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:12:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

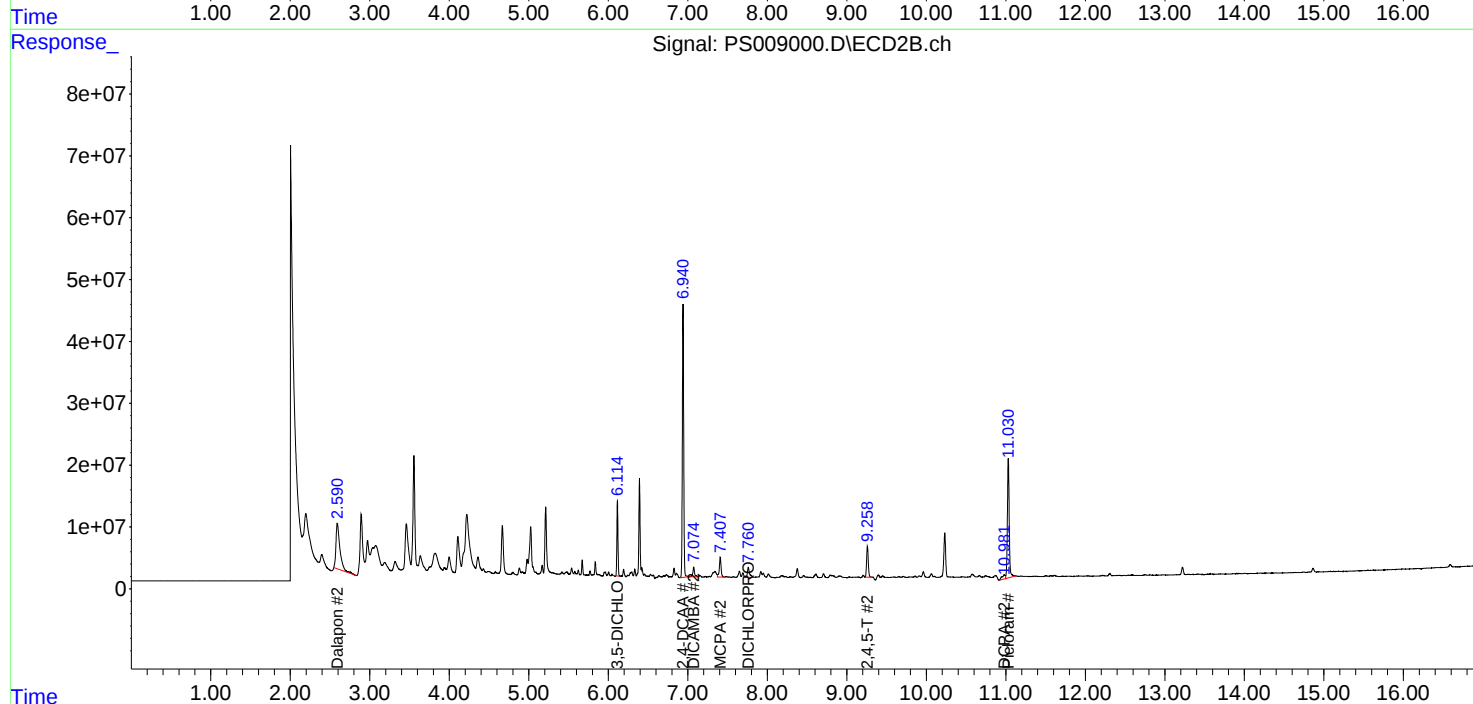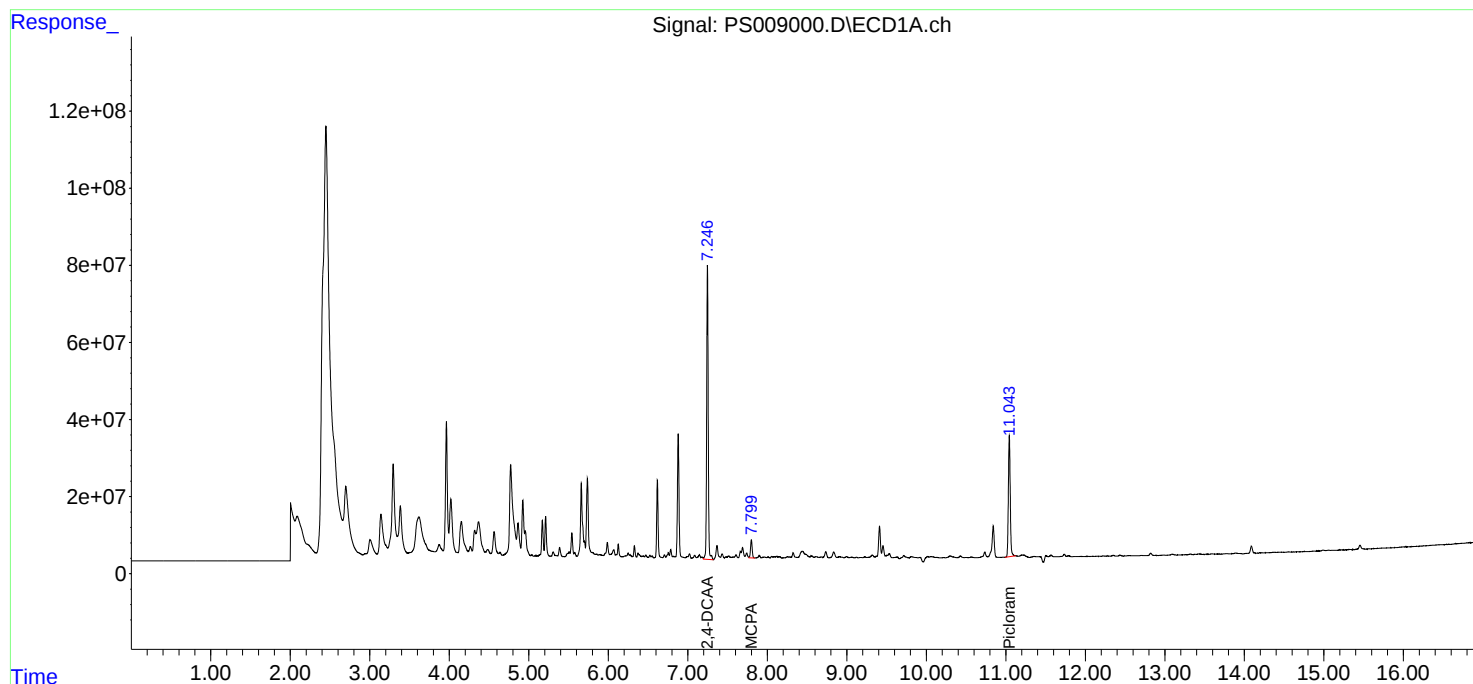


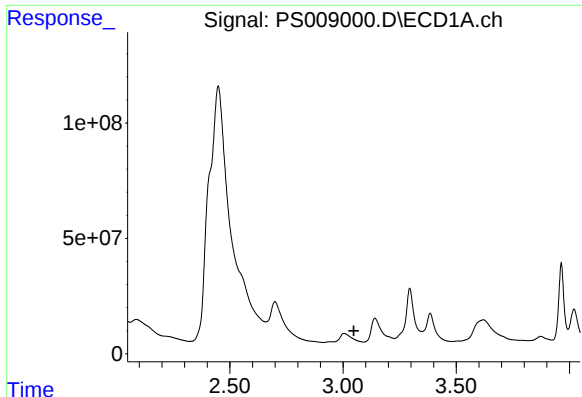

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127074BL

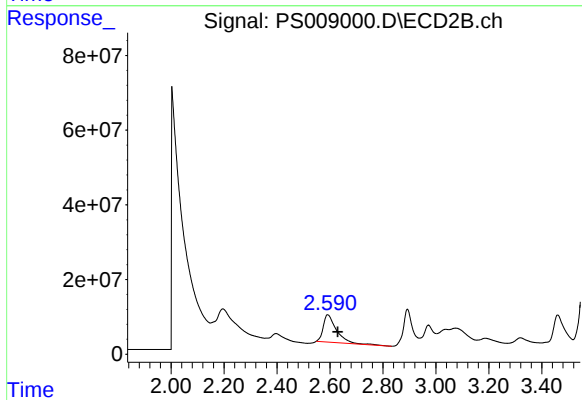


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 256659514
Conc: 175.53 ng/ml

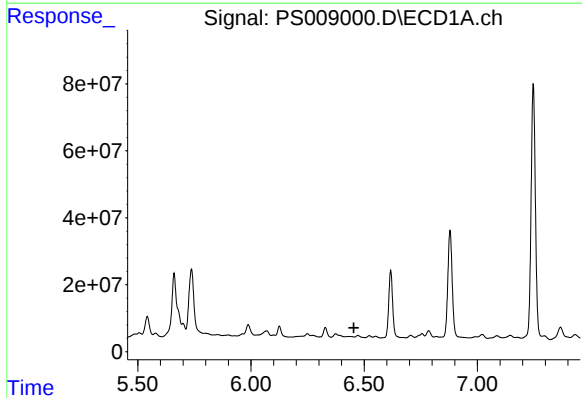


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

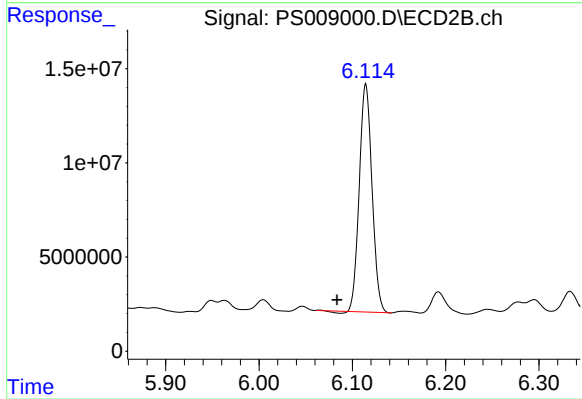

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 114425016
Conc: 78.41 ng/ml

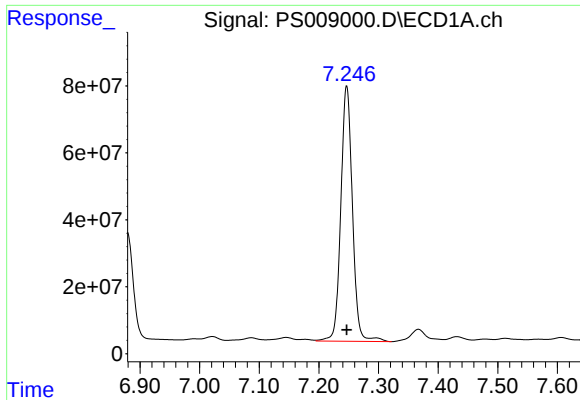

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 1033809354
Conc: 472.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127074BL

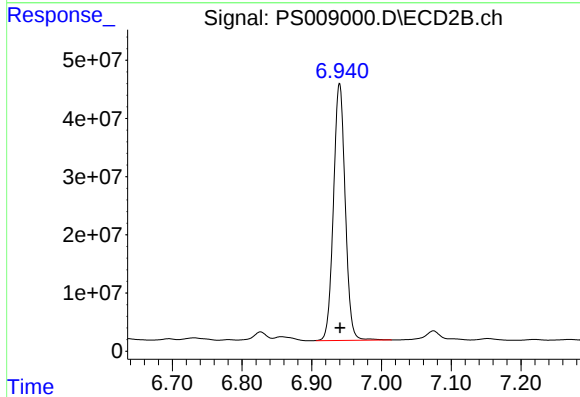


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 517597880
Conc: 537.17 ng/ml

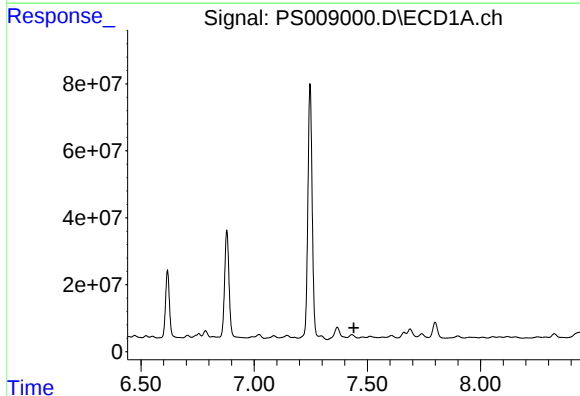


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

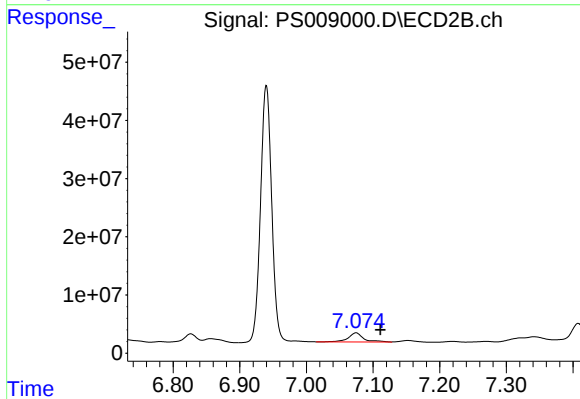

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 24327039
Conc: 5.88 ng/ml

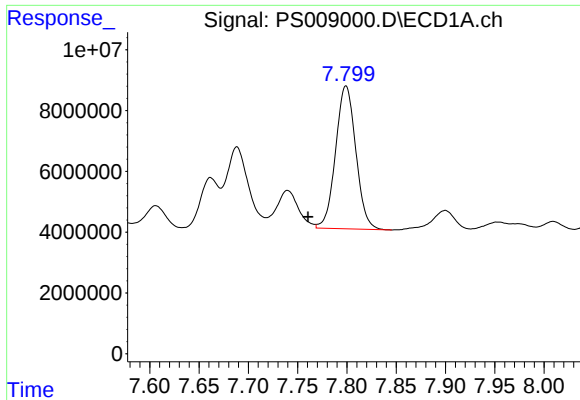

#7 MCPA


R.T.: 7.799 min
Delta R.T.: 0.038 min
Response: 67257376
Conc: 8.36 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB127074BL

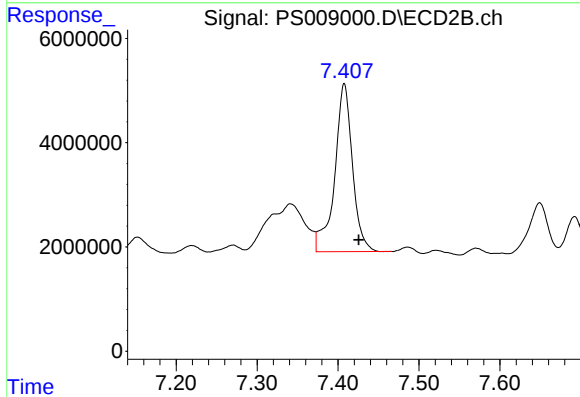


#7 MCPA

R.T.: 7.408 min
Delta R.T.: -0.018 min
Response: 49142360
Conc: 11.11 ug/ml

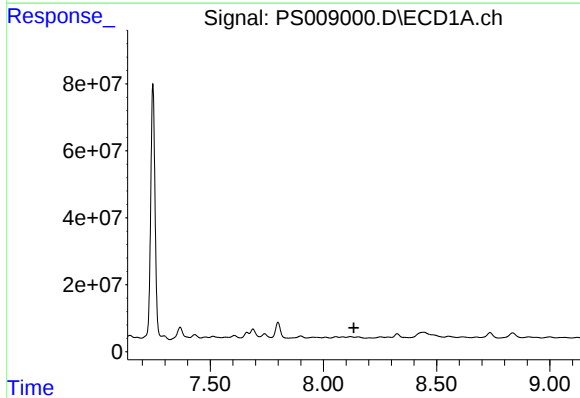


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

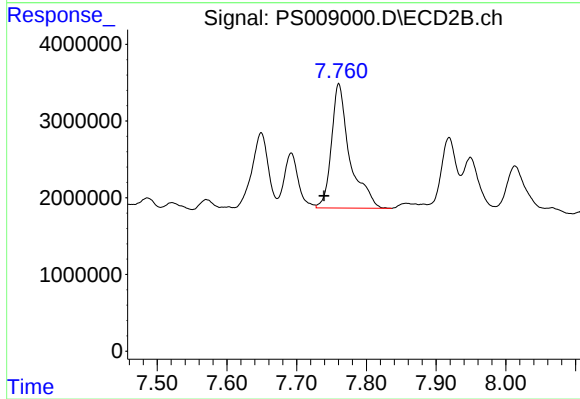

#8 DICHLORPROP


R.T.: 7.761 min
Delta R.T.: 0.022 min
Response: 29617002
Conc: 29.56 ng/ml

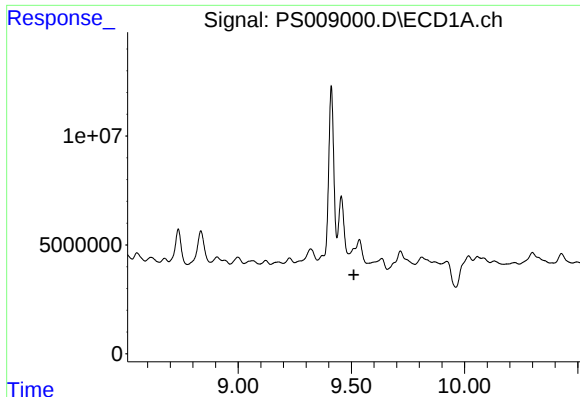

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127074BL

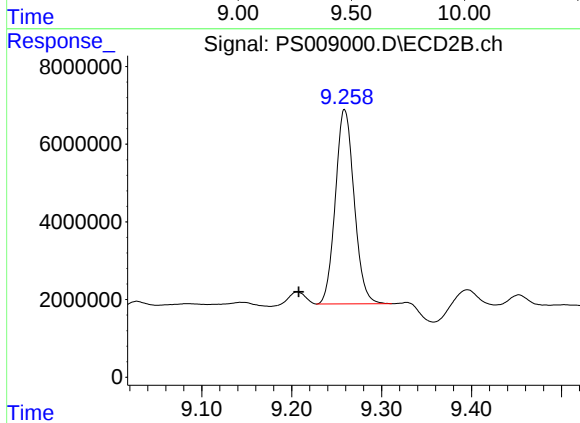


#12 2,4,5-T

R.T.: 9.259 min
Delta R.T.: 0.051 min
Response: 72681328
Conc: 13.43 ng/ml

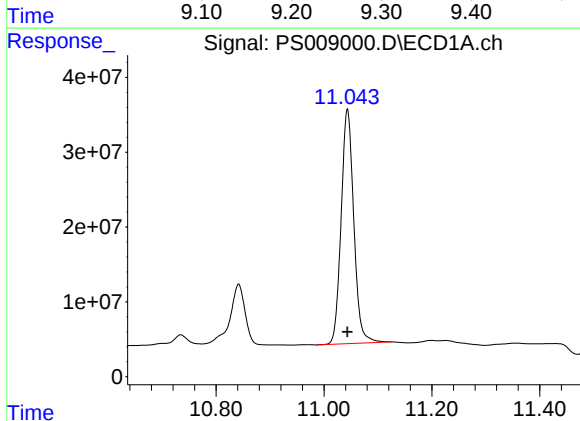


#15 Picloram

R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 508368479
Conc: 37.13 ng/ml

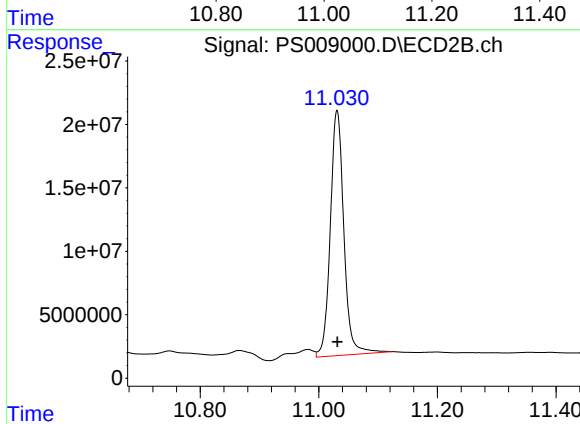

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 306190187
Conc: 42.14 ng/ml

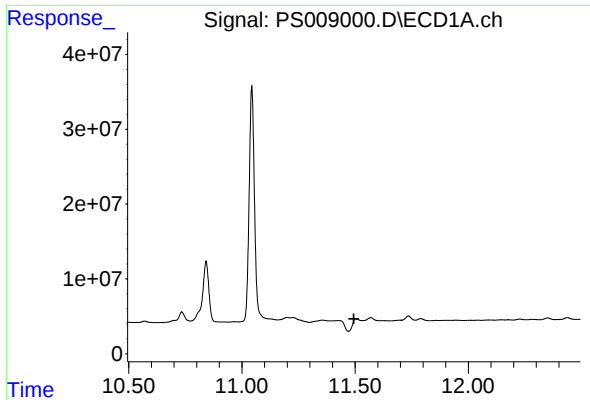

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127074BL

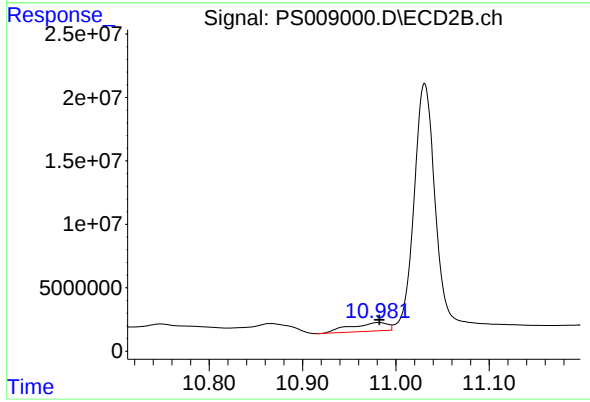

#16 DCPA

R.T.: 10.981 min
Delta R.T.: -0.001 min
Response: 18589721
Conc: 2.69 ng/ml