

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
 Data File : PS009002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 17:56
 Operator : DD\AJ
 Sample : PB127074TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB127074TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:13:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	723.9E6	393.8E6	331.057	408.697
Target Compounds							
1) T	Dalapon	0.000	2.592	0	300.3E6	N.D.	205.386
2) T	3,5-DICHL...	0.000	6.115	0	179.0E6	N.D.	122.659
5) T	DICAMBA	0.000	7.075	0	29830418	N.D.	7.207
7) T	MCPA	0.000	7.413	0	23664666	N.D.	5.349
8) T	DICHLORPROP	0.000	7.761	0	57102502	N.D.	56.992
10) T	Pentachlo...	0.000	8.464	0	18375057	N.D.	1.293
12) T	2,4,5-T	9.454	0.000	55153497	0	5.158	N.D. #
15) T	Picloram	0.000	11.031	0	15251205	N.D.	2.099
16) T	DCPA	0.000	11.031	0	15251205	N.D.	2.204



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
Data File : PS009002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 17:56
Operator : DD\AJ
Sample : PB127074TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB127074TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:13:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

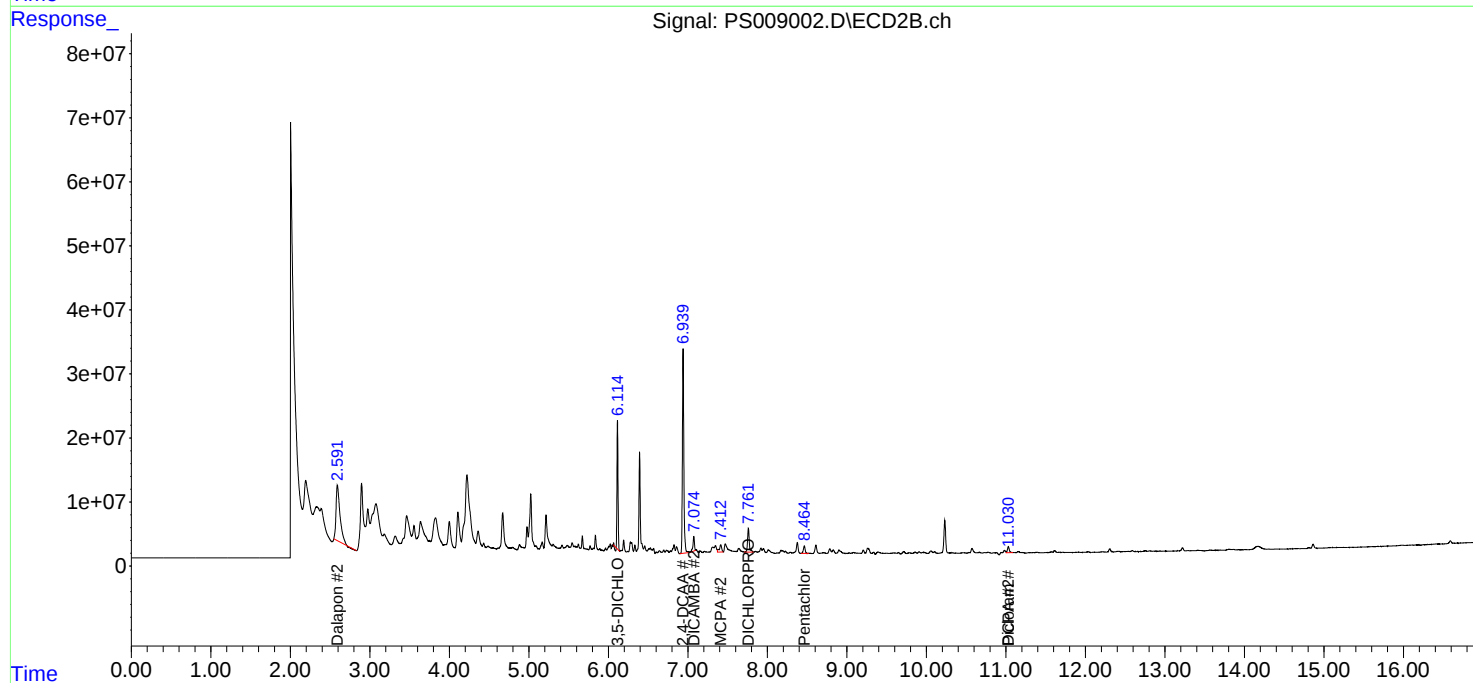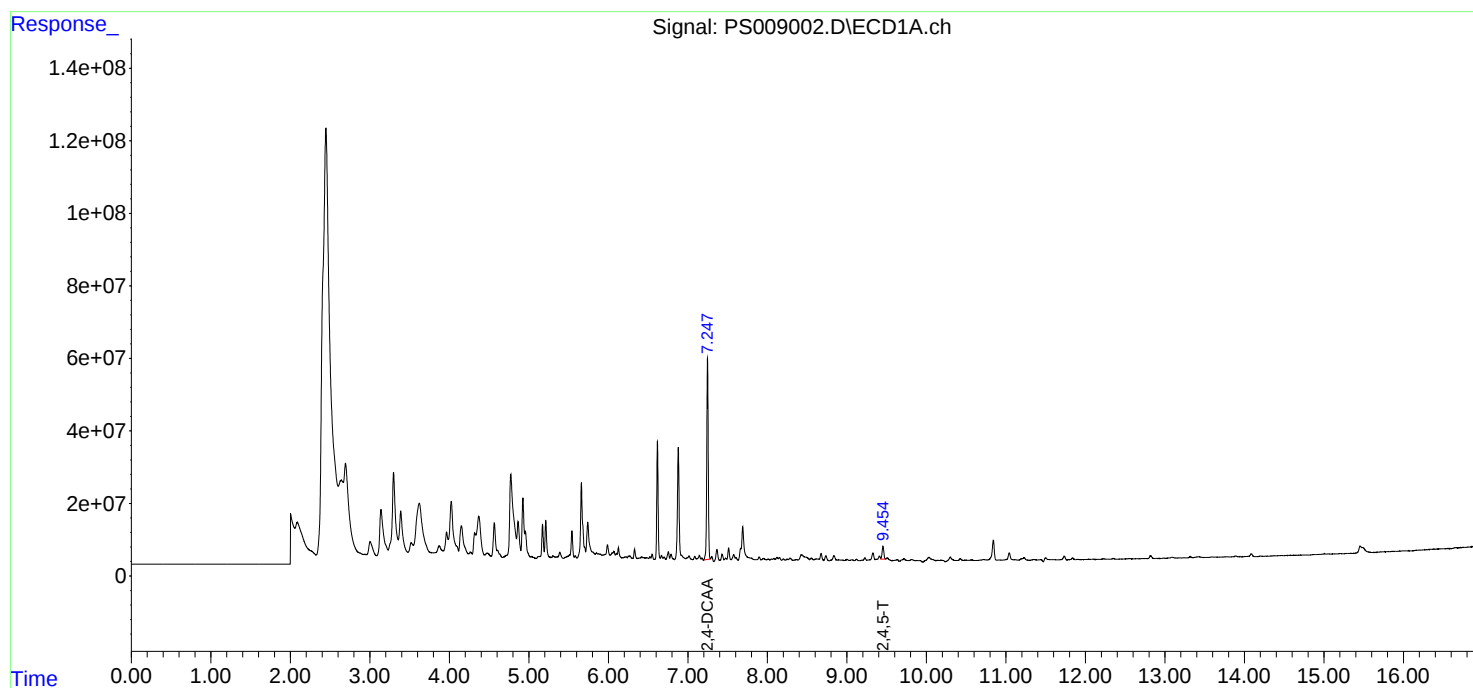


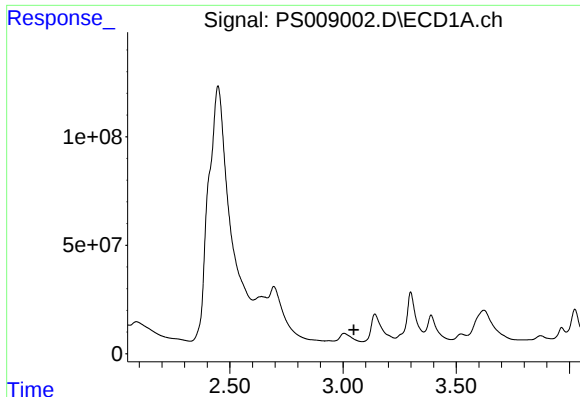

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127074TB

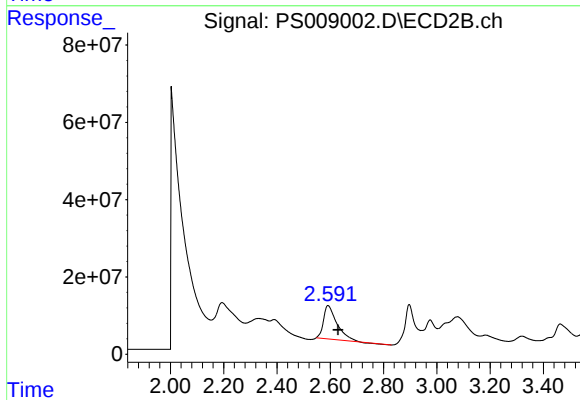


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 300319057
Conc: 205.39 ng/ml

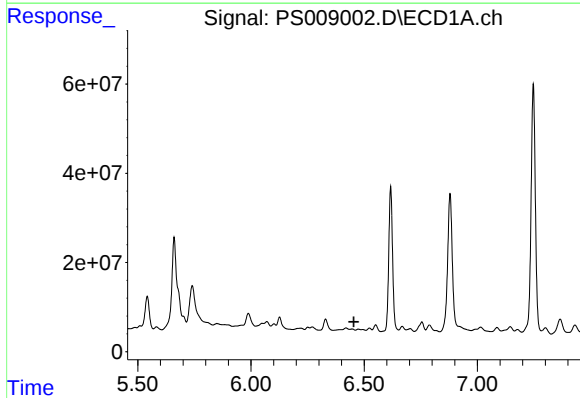


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

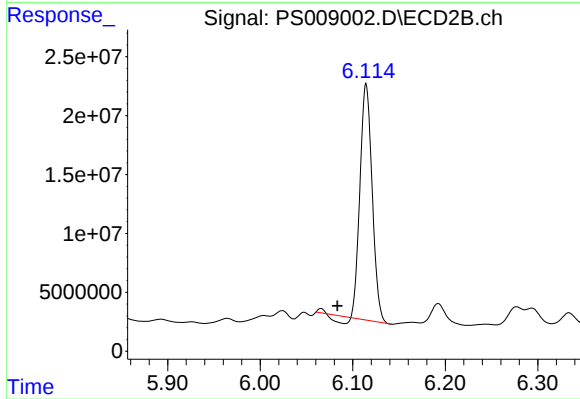

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 178993084
Conc: 122.66 ng/ml

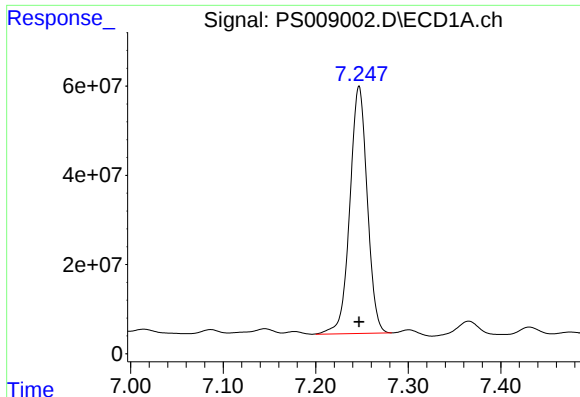

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 723886790
Conc: 331.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127074TB

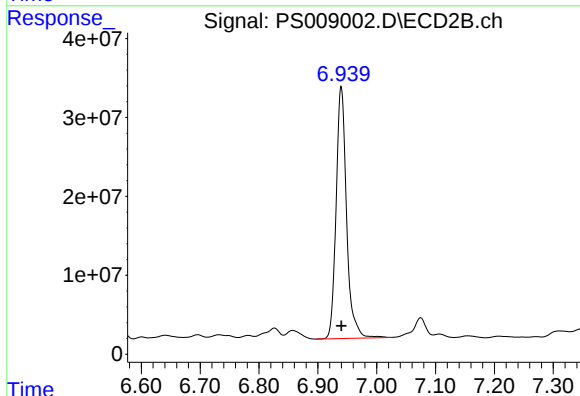


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 393802378
Conc: 408.70 ng/ml

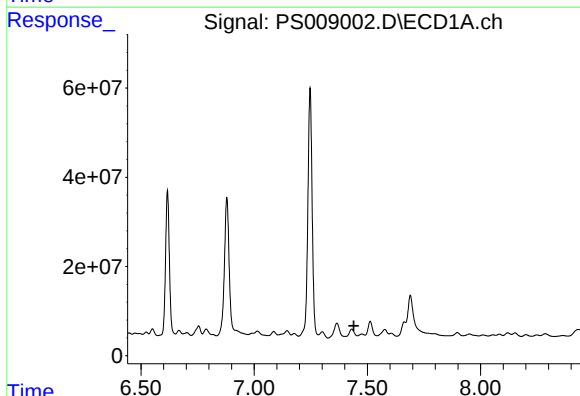


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

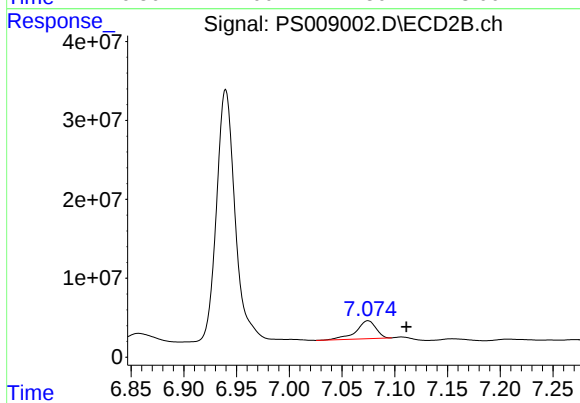

#5 DICAMBA


R.T.: 7.075 min
Delta R.T.: -0.037 min
Response: 29830418
Conc: 7.21 ng/ml

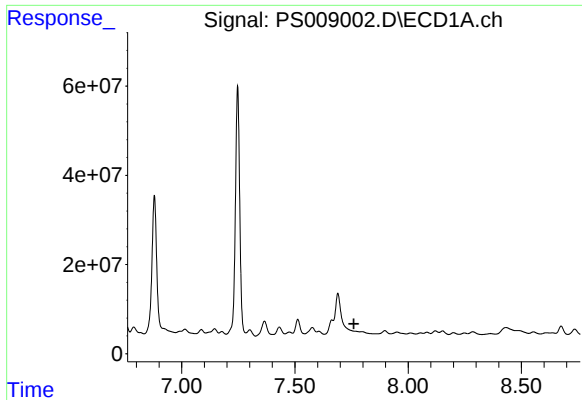

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.761 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127074TB

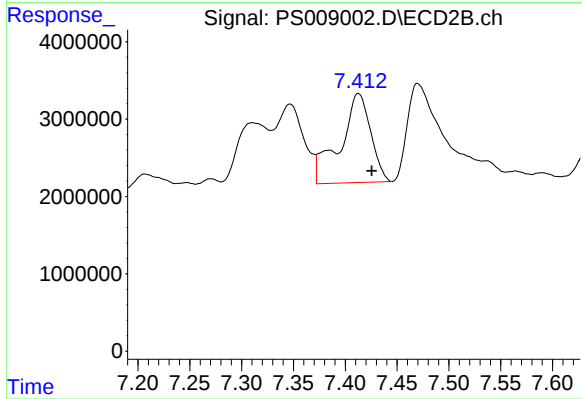


#7 MCPA

R.T.: 7.413 min
Delta R.T.: -0.013 min
Response: 23664666
Conc: 5.35 ug/ml

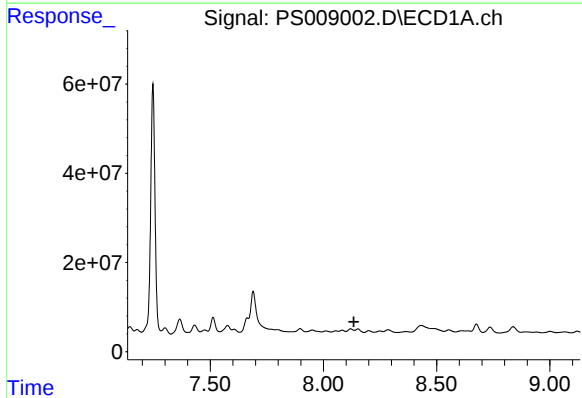


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

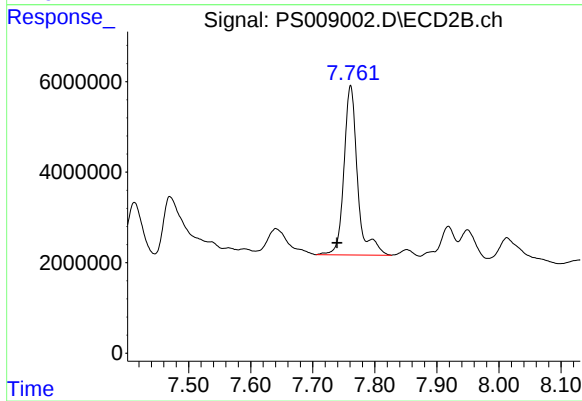

#8 DICHLORPROP


R.T.: 7.761 min
Delta R.T.: 0.022 min
Response: 57102502
Conc: 56.99 ng/ml

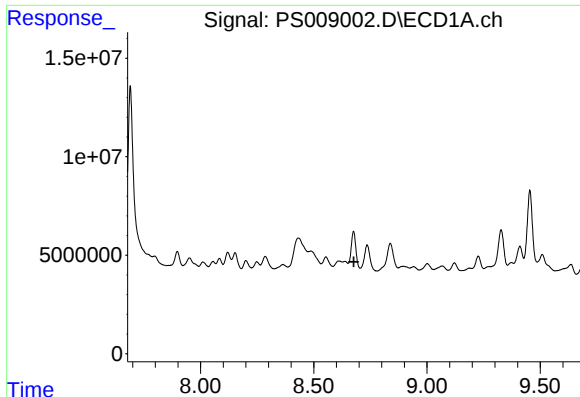

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127074TB

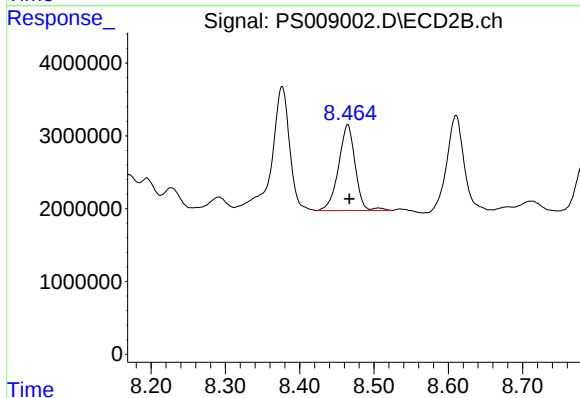


#10 Pentachlorophenol

R.T.: 8.464 min
Delta R.T.: -0.002 min
Response: 18375057
Conc: 1.29 ng/ml

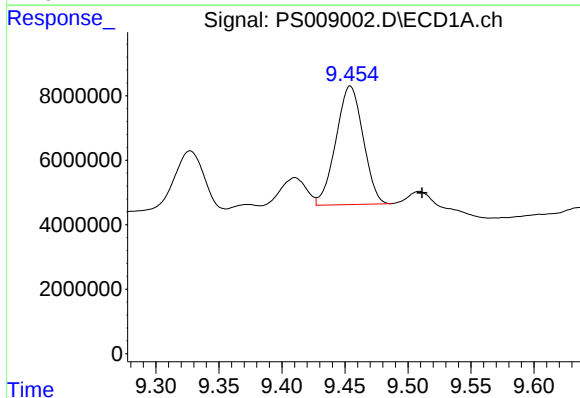


#12 2,4,5-T

R.T.: 9.454 min
Delta R.T.: -0.057 min
Response: 55153497
Conc: 5.16 ng/ml

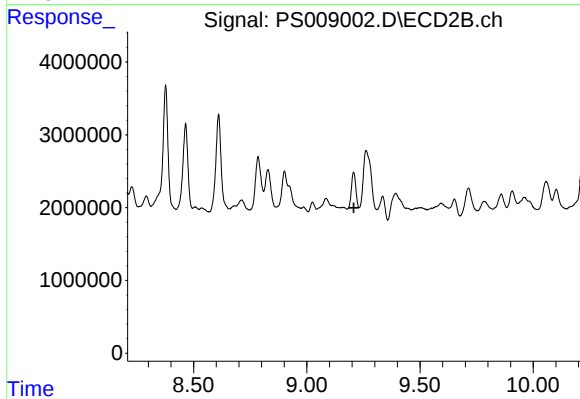

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

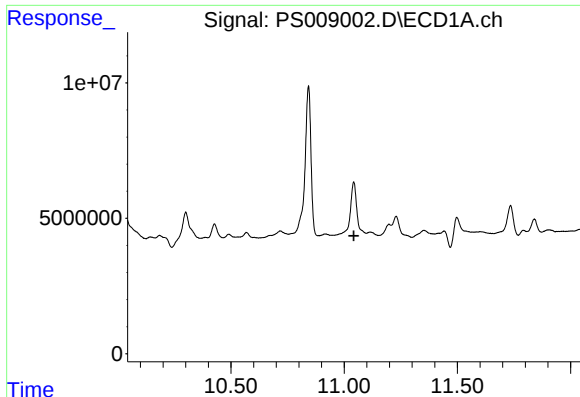

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127074TB

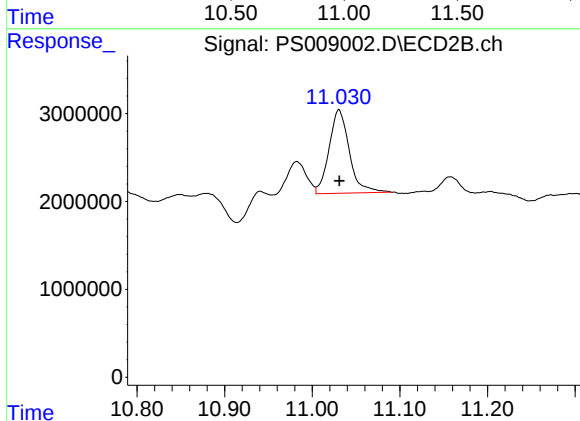


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 15251205
Conc: 2.10 ng/ml

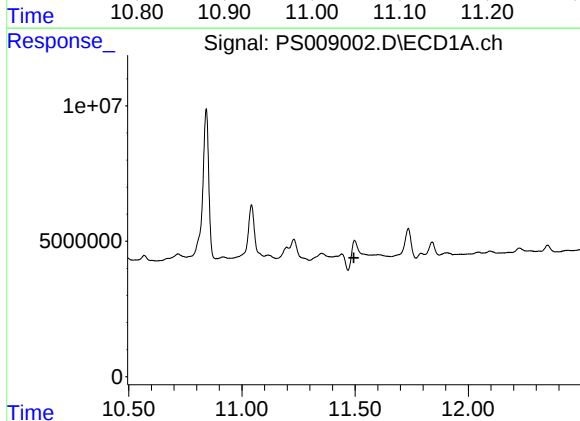

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

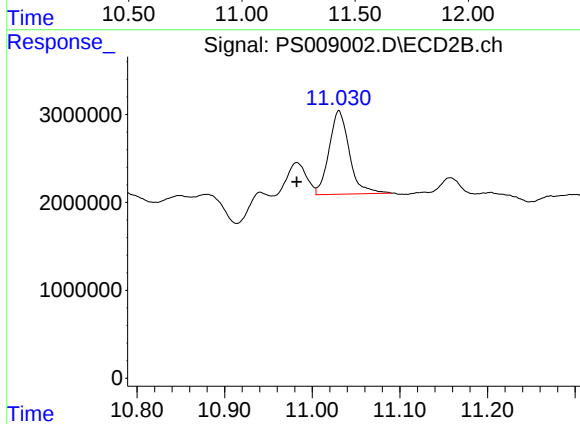

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.048 min
Response: 15251205
Conc: 2.20 ng/ml