

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
 Data File : PS009003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 18:19
 Operator : DD\AJ
 Sample : L1367-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-02-022420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:13:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	662.5E6	370.3E6	302.982	384.273 #
Target Compounds							
1) T	Dalapon	0.000	2.593	0	253.9E6	N.D.	173.656
2) T	3,5-DICHL...	0.000	6.115	0	159.6E6	N.D.	109.389
5) T	DICAMBA	0.000	7.075	0	49047675	N.D.	11.849
7) T	MCPA	0.000	7.415	0	18357610	N.D.	4.149
8) T	DICHLORPROP	0.000	7.760	0	96248835	N.D.	96.063
11) T	2,4,5-TP ...	0.000	8.784	0	31103597	N.D.	5.742
12) T	2,4,5-T	9.451	0.000	127.1E6	0	11.889	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
Data File : PS009003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 18:19
Operator : DD\AJ
Sample : L1367-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
OK-02-022420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:13:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

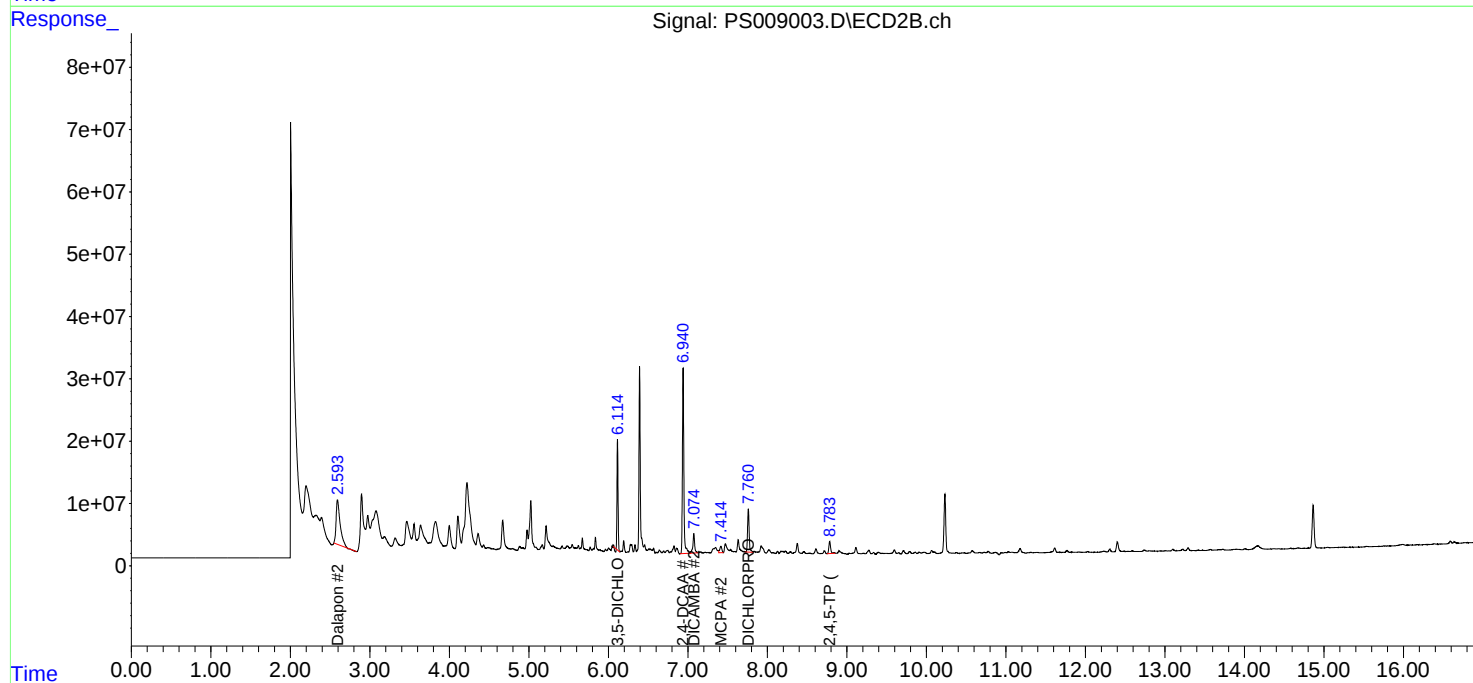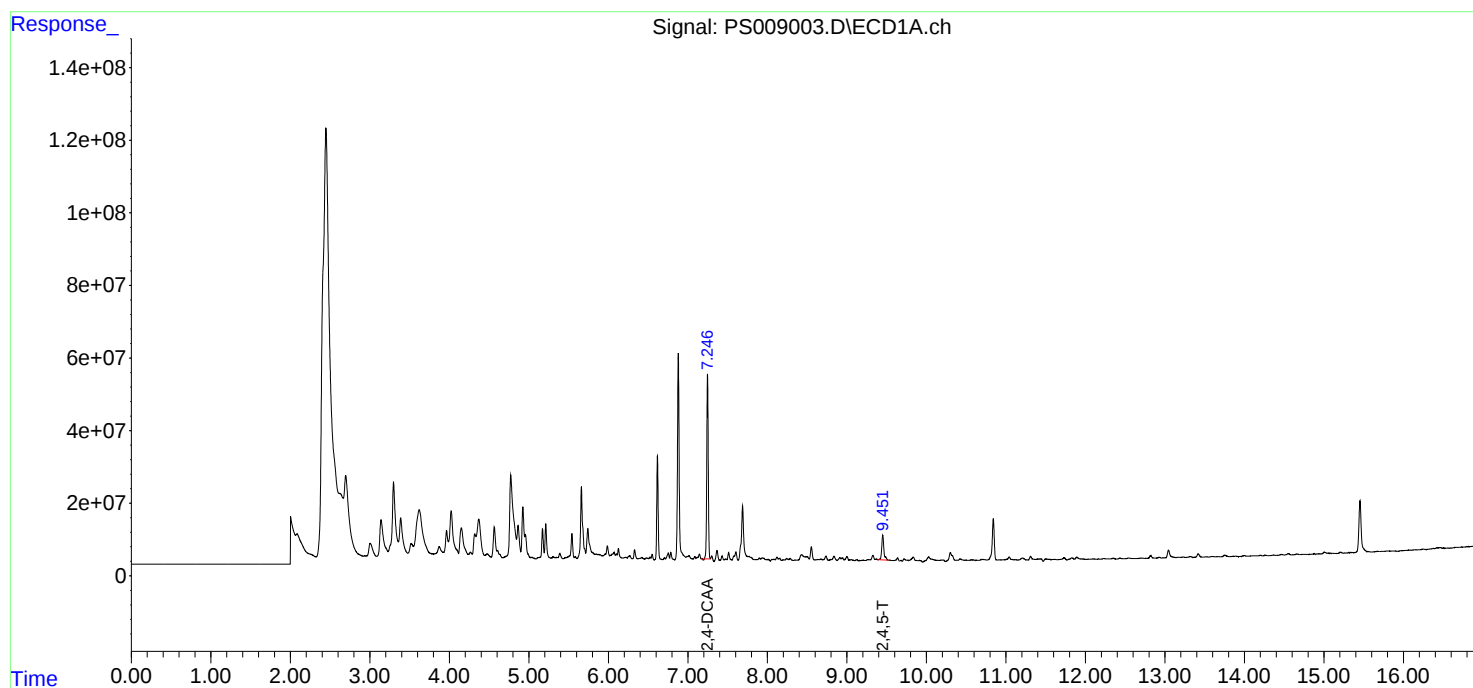


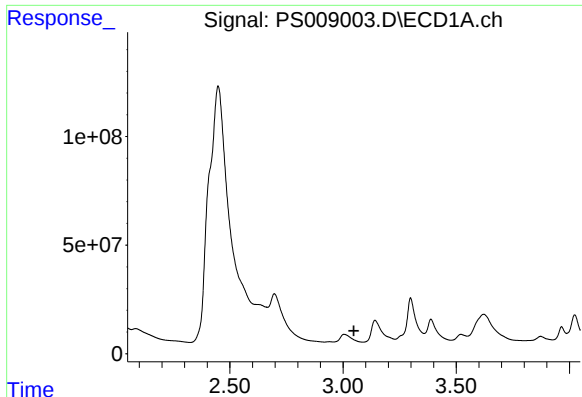

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-02-022420

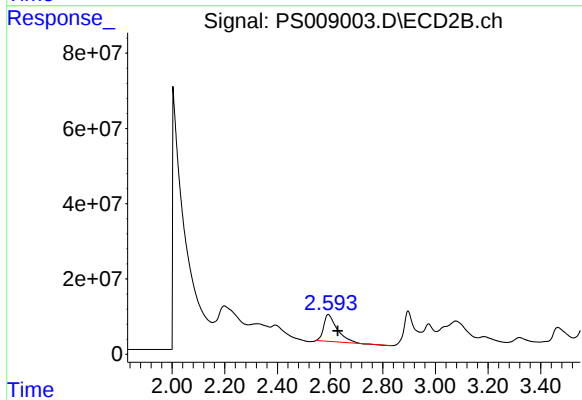


#1 Dalapon

R.T.: 2.593 min
Delta R.T.: -0.037 min
Response: 253923911
Conc: 173.66 ng/ml

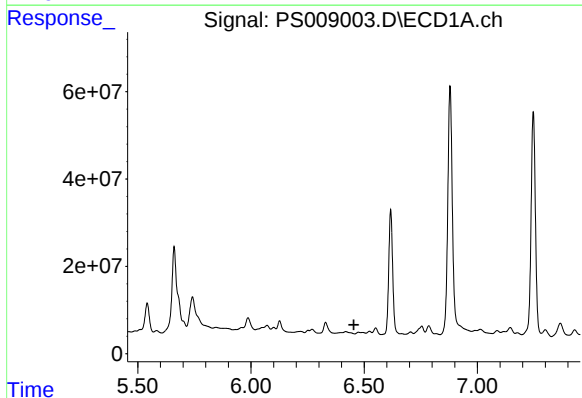


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

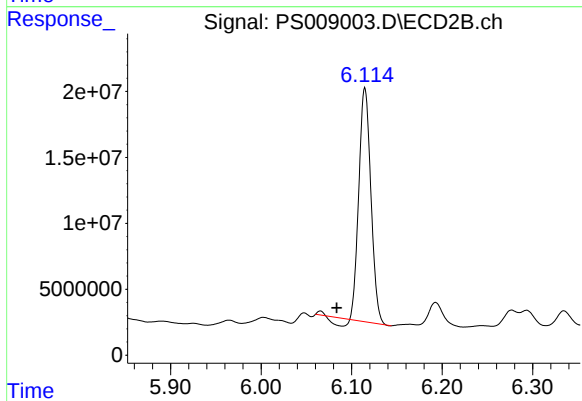

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 159627827
Conc: 109.39 ng/ml

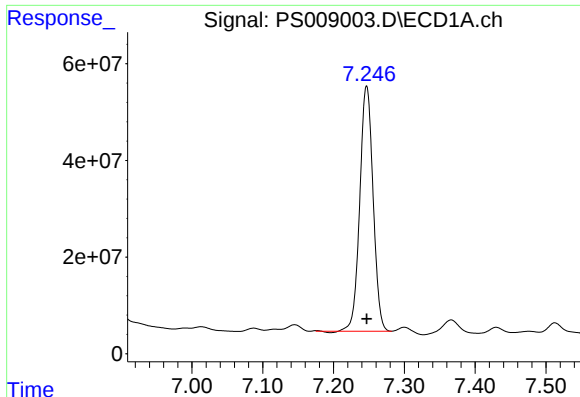

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 662498468
Conc: 302.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-02-022420

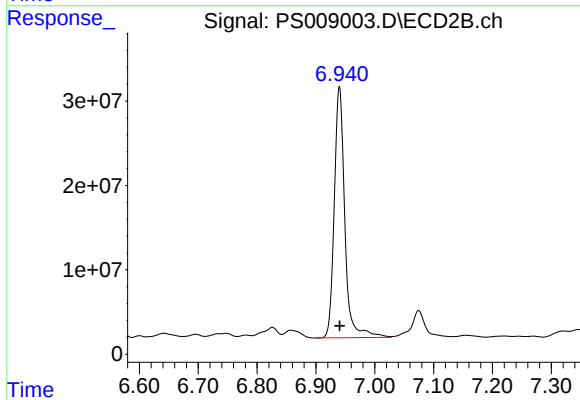


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 370268347
Conc: 384.27 ng/ml

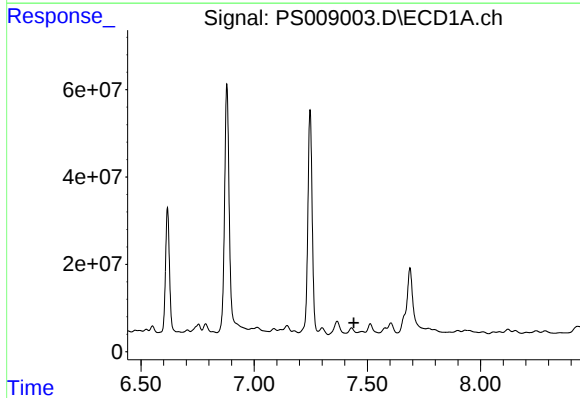


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

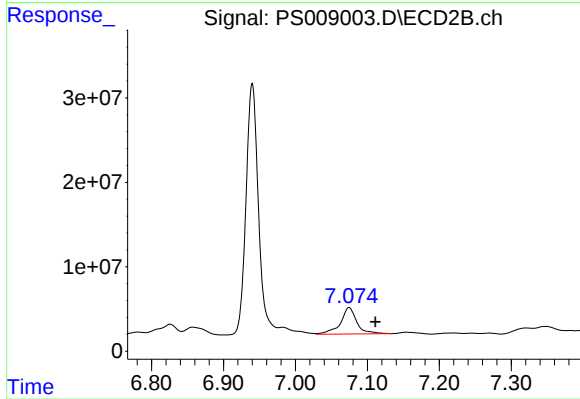

#5 DICAMBA


R.T.: 7.075 min
Delta R.T.: -0.037 min
Response: 49047675
Conc: 11.85 ng/ml

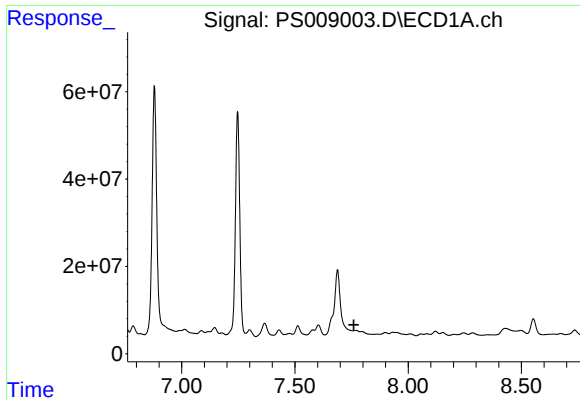

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.761 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-02-022420

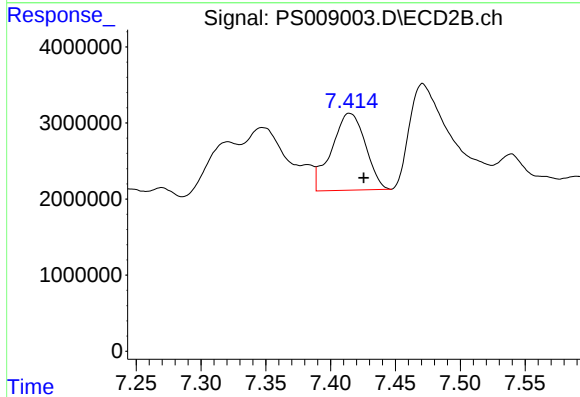


#7 MCPA

R.T.: 7.415 min
Delta R.T.: -0.011 min
Response: 18357610
Conc: 4.15 ug/ml

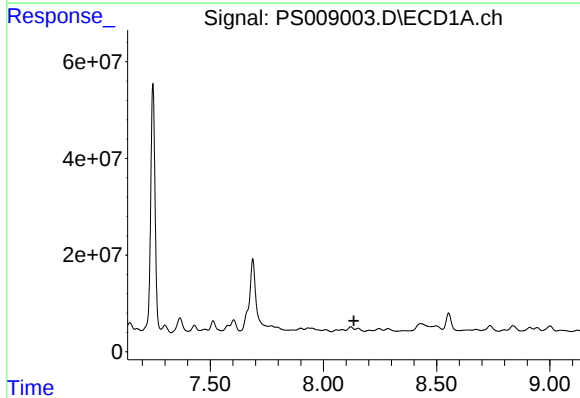


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

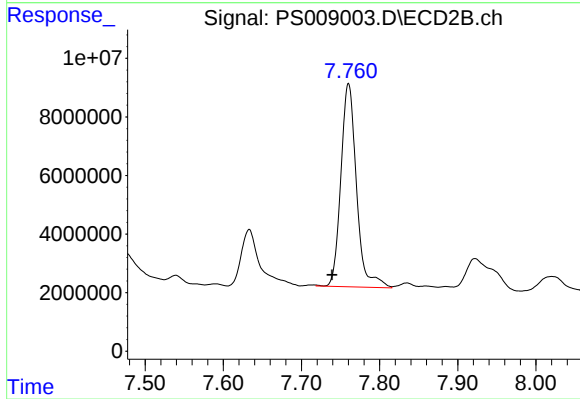

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 96248835
Conc: 96.06 ng/ml

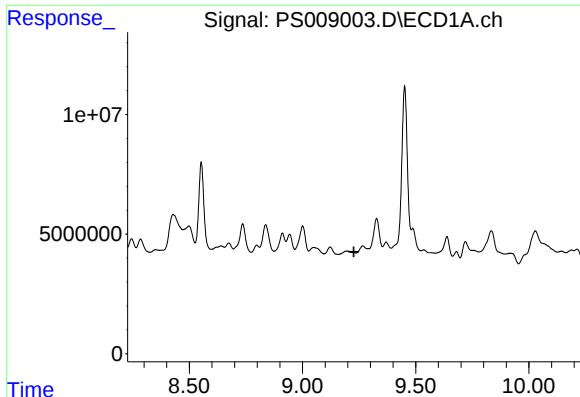

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-02-022420

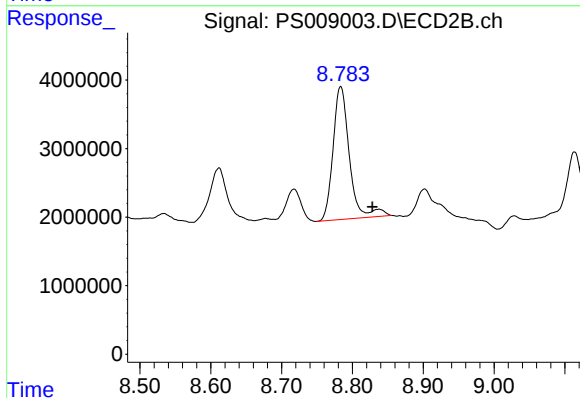


#11 2,4,5-TP (SILVEX)

R.T.: 8.784 min
Delta R.T.: -0.044 min
Response: 31103597
Conc: 5.74 ng/ml

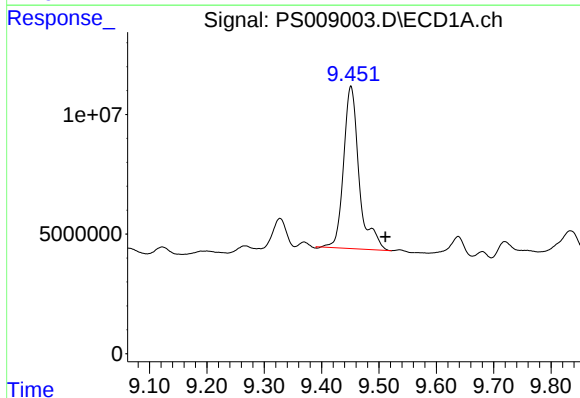

#12 2,4,5-T

R.T.: 9.451 min
Delta R.T.: -0.060 min
Response: 127113800
Conc: 11.89 ng/ml

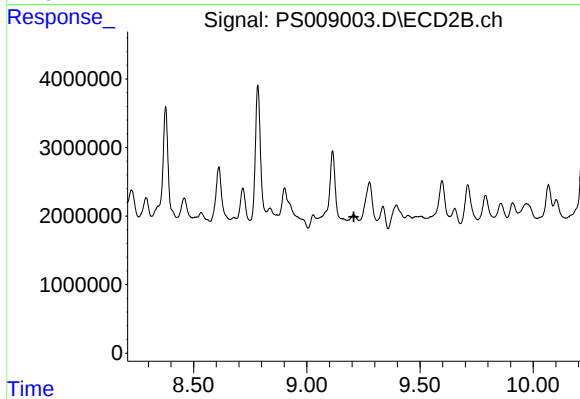

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.