

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
 Data File : PS009008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2020 20:13
 Operator : DD\AJ
 Sample : L1659-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WH-1-COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 01:14:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.250	6.940	646.7E6	321.6E6	295.756	333.801
Target Compounds							
1) T	Dalapon	0.000	2.592	0	242.7E6	N.D.	166.007
2) T	3,5-DICHL...	0.000	6.115	0	150.5E6	N.D.	103.108
7) T	MCPA	7.692	7.414	208.4E6	17921254	25.911	4.051 #
8) T	DICHLORPROP	0.000	7.760	0	86416729	N.D.	86.250
10) T	Pentachlo...	0.000	8.465	0	15345119	N.D.	1.080
11) T	2,4,5-TP ...	0.000	8.784	0	154.8E6	N.D.	28.578
12) T	2,4,5-T	9.456	0.000	175.9E6	0	16.449	N.D. #
15) T	Picloram	0.000	11.030	0	13508110	N.D.	1.859
16) T	DCPA	0.000	11.030	0	13508110	N.D.	1.952



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022520\
Data File : PS009008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2020 20:13
Operator : DD\AJ
Sample : L1659-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WH-1-COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 01:14:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

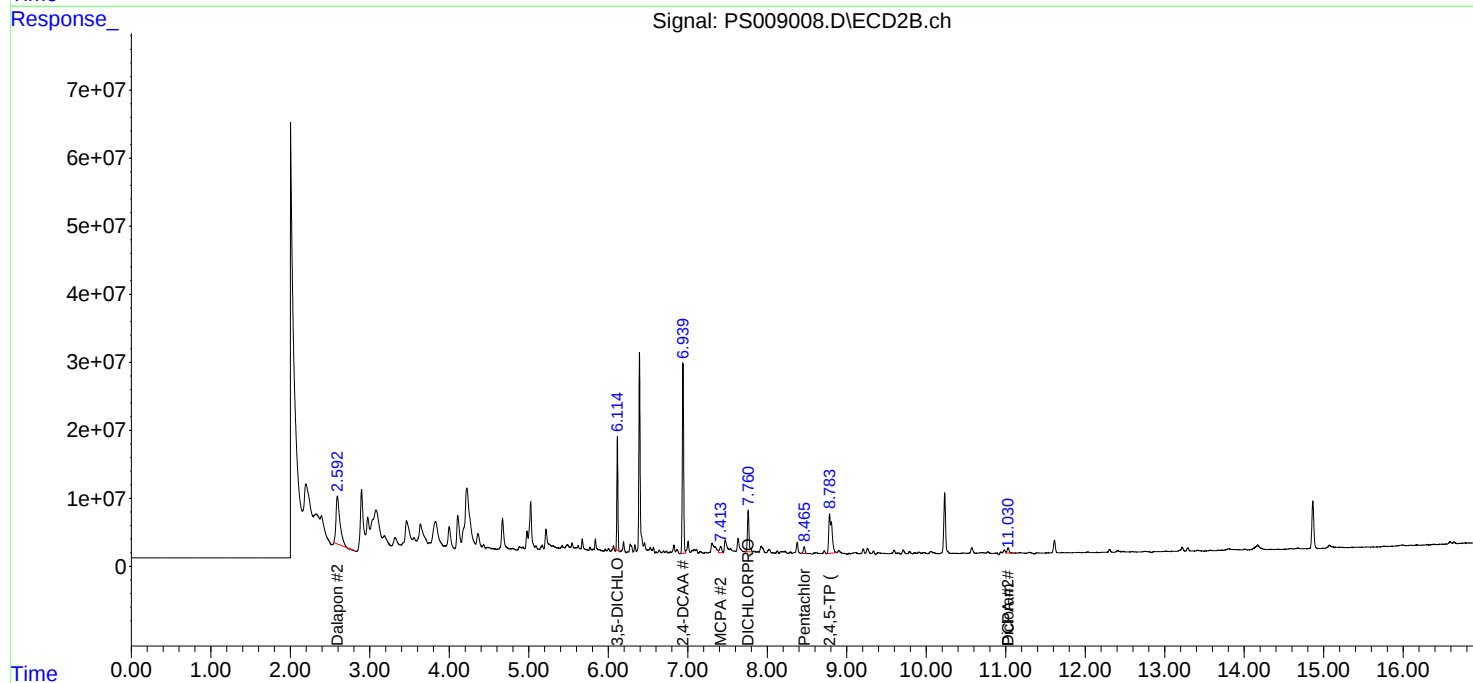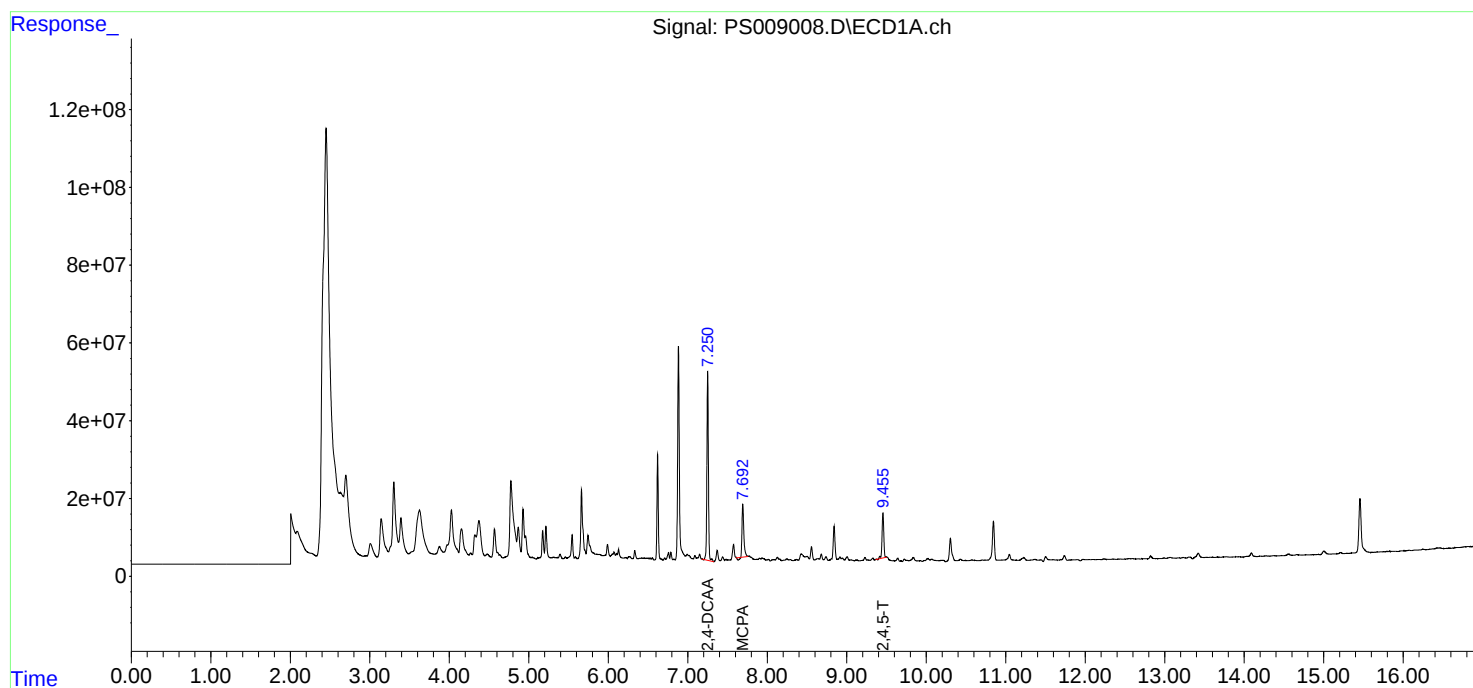


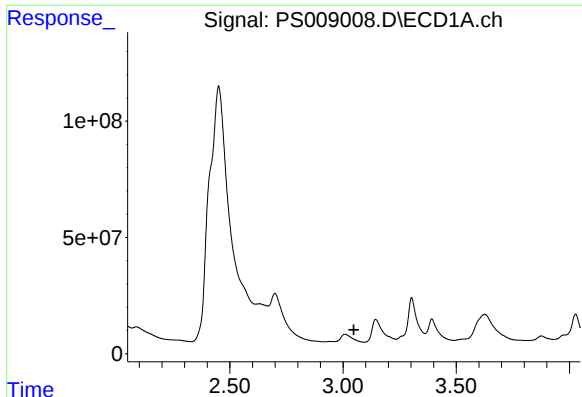

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WH-1-COMP-1

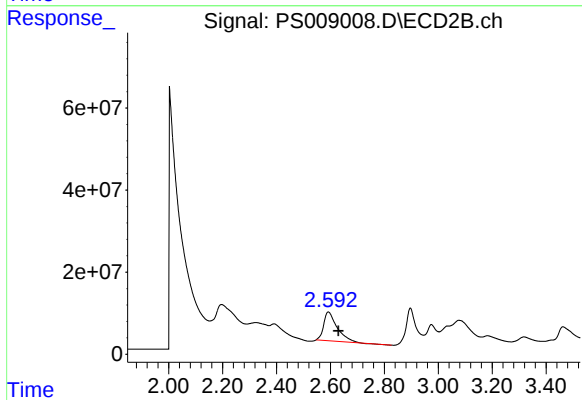


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 242738122
Conc: 166.01 ng/ml

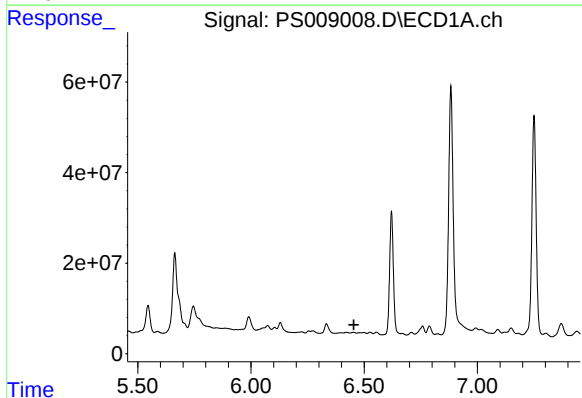


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

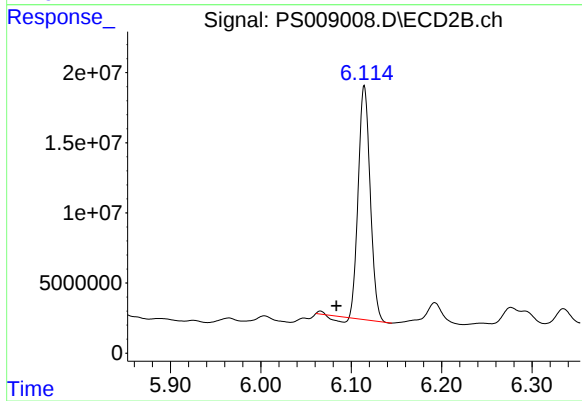

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.115 min
Delta R.T.: 0.031 min
Response: 150461906
Conc: 103.11 ng/ml

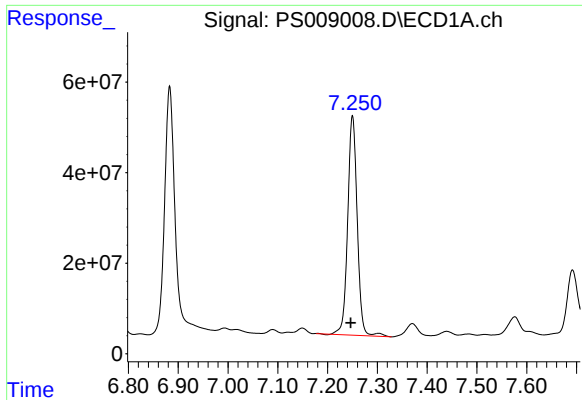

#4 2,4-DCAA


R.T.: 7.250 min
Delta R.T.: 0.003 min
Response: 646697040
Conc: 295.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
WH-1-COMP-1

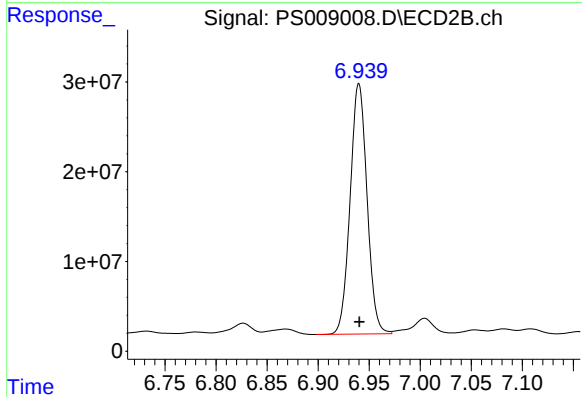


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 321636186
Conc: 333.80 ng/ml

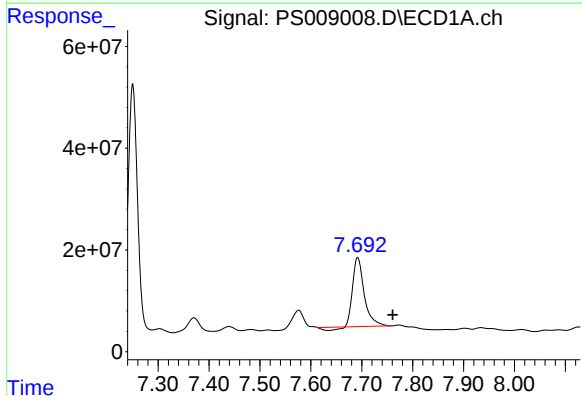


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.069 min
Response: 208426672
Conc: 25.91 ug/ml

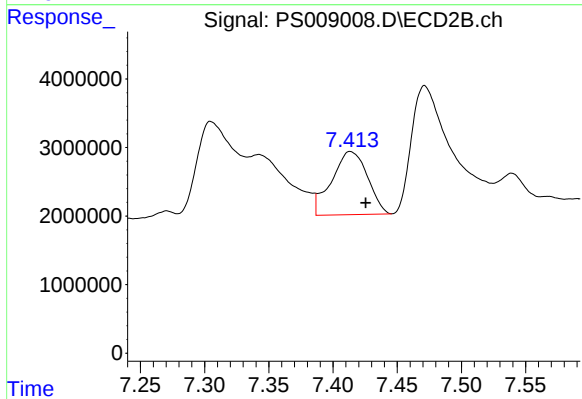

#7 MCPA


R.T.: 7.414 min
Delta R.T.: -0.012 min
Response: 17921254
Conc: 4.05 ug/ml

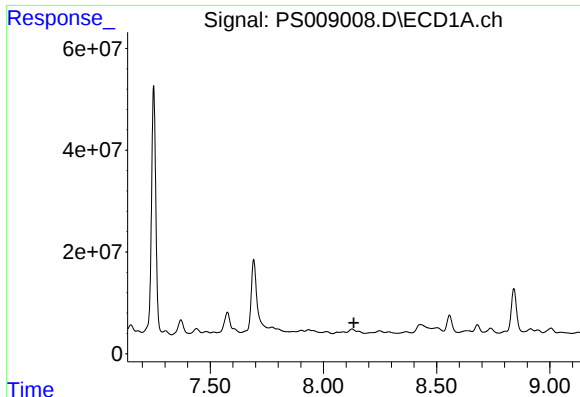

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WH-1-COMP-1

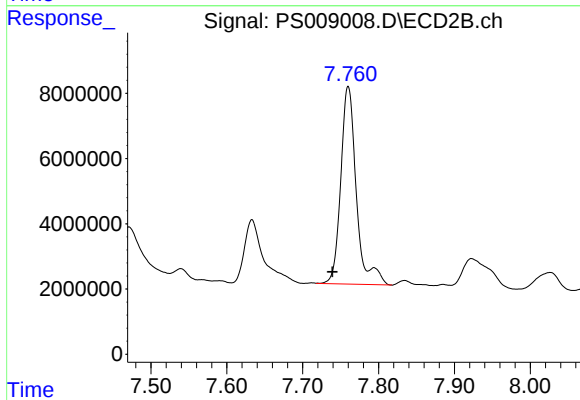


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 86416729
Conc: 86.25 ng/ml

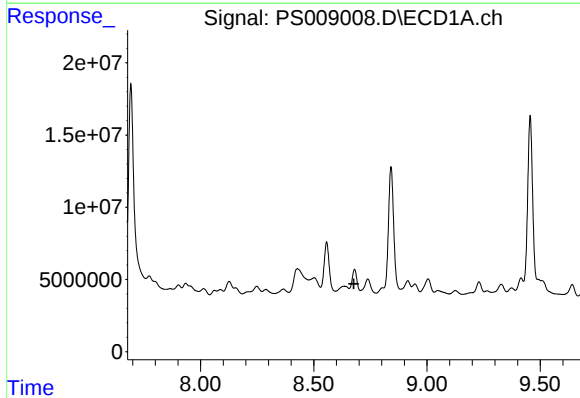


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

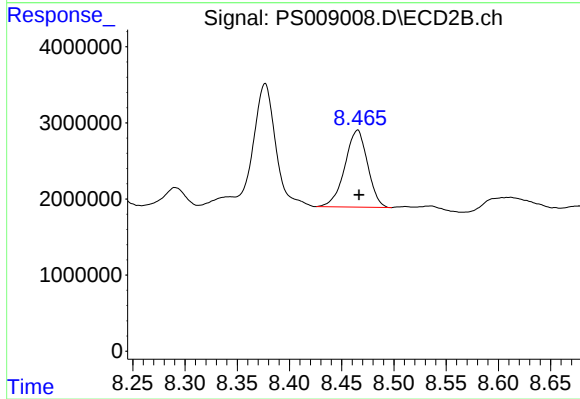

#10 Pentachlorophenol


R.T.: 8.465 min
Delta R.T.: -0.002 min
Response: 15345119
Conc: 1.08 ng/ml

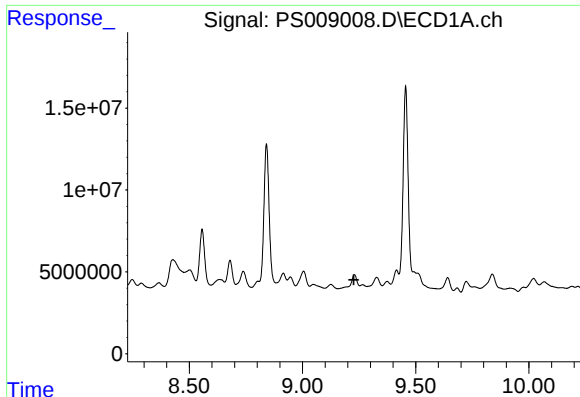

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WH-1-COMP-1

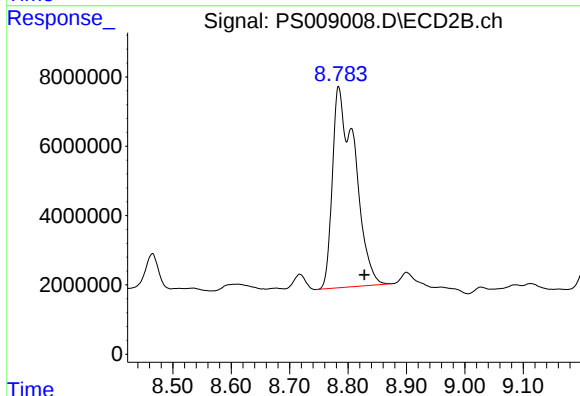


#11 2,4,5-TP (SILVEX)

R.T.: 8.784 min
Delta R.T.: -0.044 min
Response: 154803660
Conc: 28.58 ng/ml

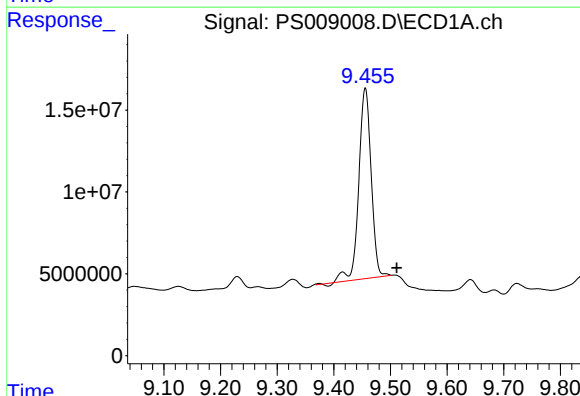


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.056 min
Response: 175876146
Conc: 16.45 ng/ml

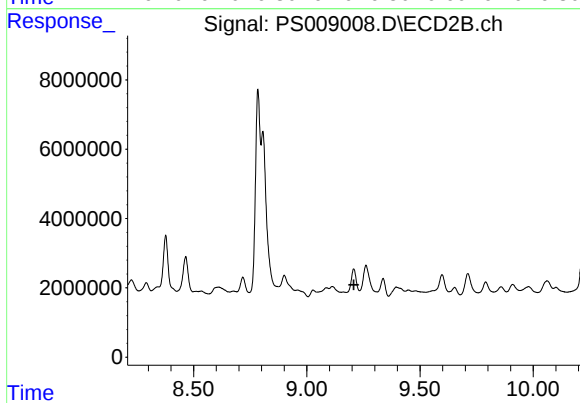

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

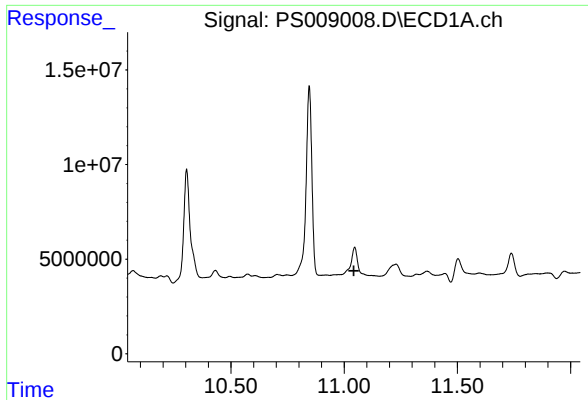

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WH-1-COMP-1

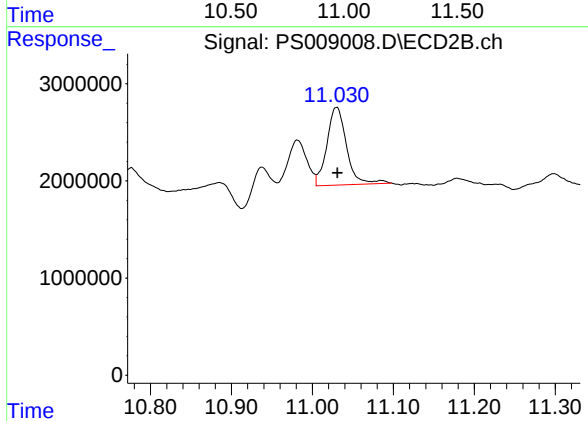


#15 Picloram

R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 13508110
Conc: 1.86 ng/ml

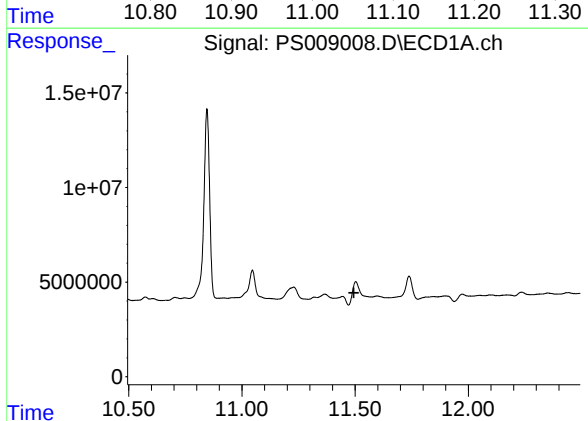

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

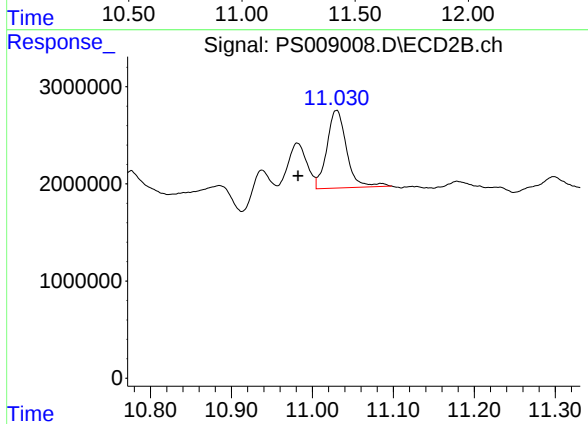

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.047 min
Response: 13508110
Conc: 1.95 ng/ml