

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022522\
 Data File : PS018428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2022 08:17
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 21:31:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	7.216	6.791	9999917	3896749	1.521 1.388
8) T	DICHLORPROP	7.904	7.405	4595840	2778522	2.717 3.774 #
9) T	2,4-D	8.151	7.706	15514723	3878663	7.605 4.143 #
10) T	Pentachlo...	8.423	8.098	24286636	9827534	1.026 1.031
11) T	2,4,5-TP ...	8.974	8.462	16903373	7425997	1.775 1.799
12) T	2,4,5-T	9.268	8.851	60486109	13247472	6.013 3.366 #
13) T	2,4-DB	9.828	0.000	16422332	0	9.450 N.D. #
14) T	DINOSEB	10.940	9.660	24997971	6250637	3.218 2.150 #
15) T	Picloram	10.797	10.656	389.0E6	196.8E6	30.614 34.026
16) T	DCPA	11.210	10.583	22446743	13648288	1.867 2.749 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022522\
Data File : PS018428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2022 08:17
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 21:31:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

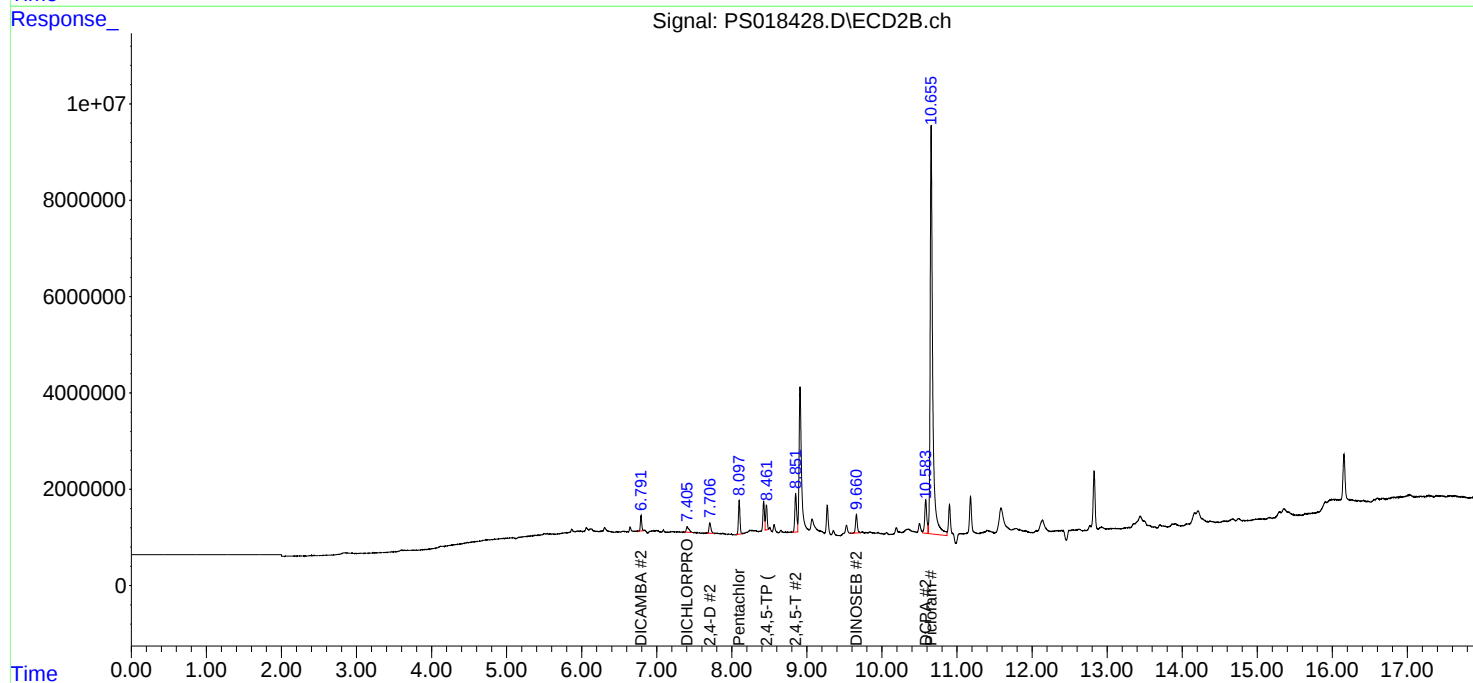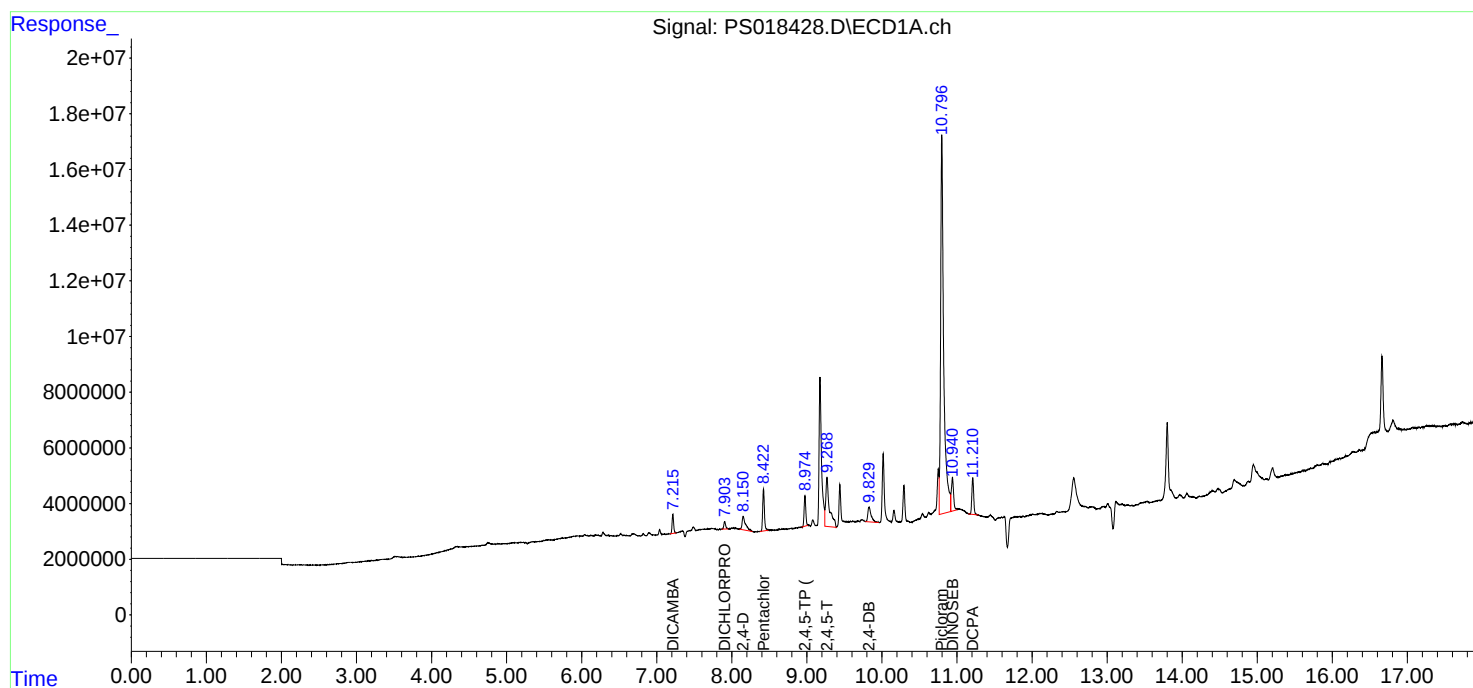


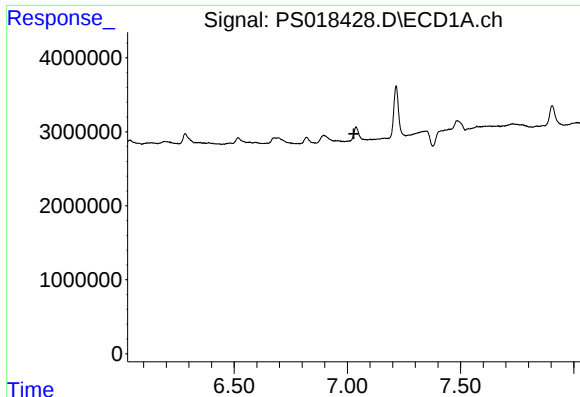

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

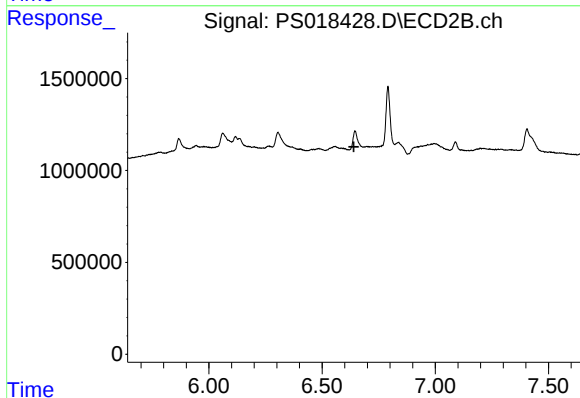


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

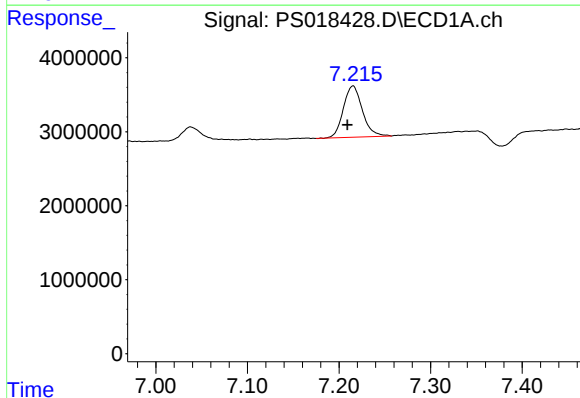


#5 DICAMBA

R.T.: 7.216 min
Delta R.T.: 0.006 min
Response: 9999917
Conc: 1.52 ng/ml

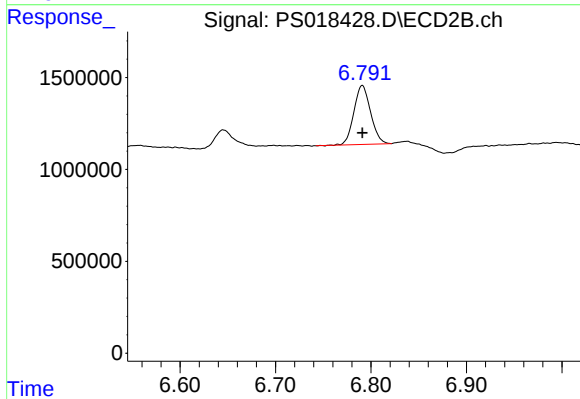

#5 DICAMBA


R.T.: 6.791 min
Delta R.T.: 0.000 min
Response: 3896749
Conc: 1.39 ng/ml

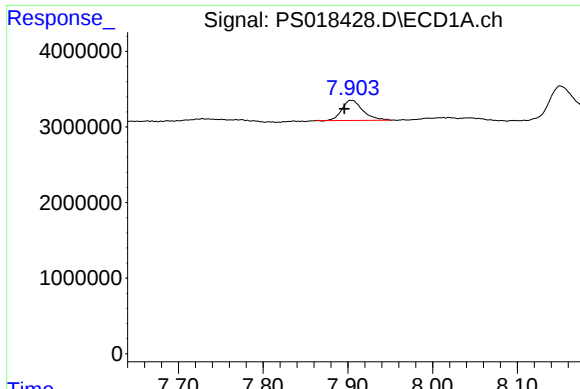

#8 DICHLORPROP


R.T.: 7.904 min
Delta R.T.: 0.008 min
Response: 4595840
Conc: 2.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

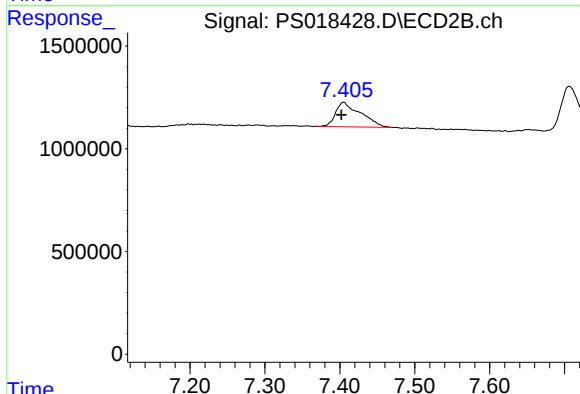


#8 DICHLORPROP

R.T.: 7.405 min
Delta R.T.: 0.003 min
Response: 2778522
Conc: 3.77 ng/ml

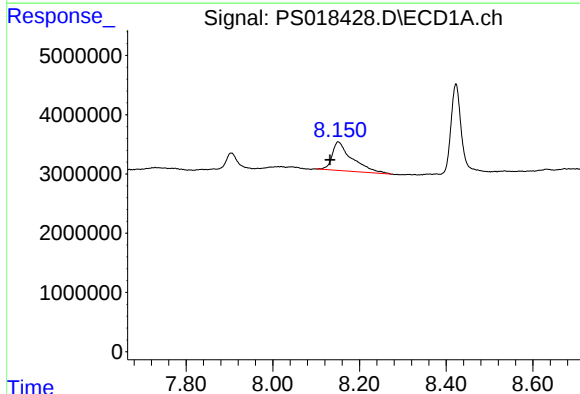


#9 2,4-D

R.T.: 8.151 min
Delta R.T.: 0.018 min
Response: 15514723
Conc: 7.61 ng/ml

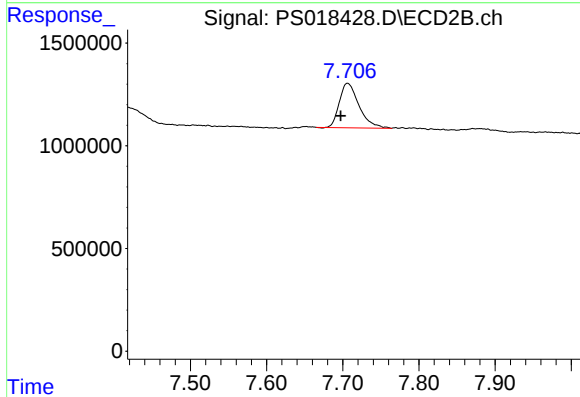

#9 2,4-D


R.T.: 7.706 min
Delta R.T.: 0.009 min
Response: 3878663
Conc: 4.14 ng/ml

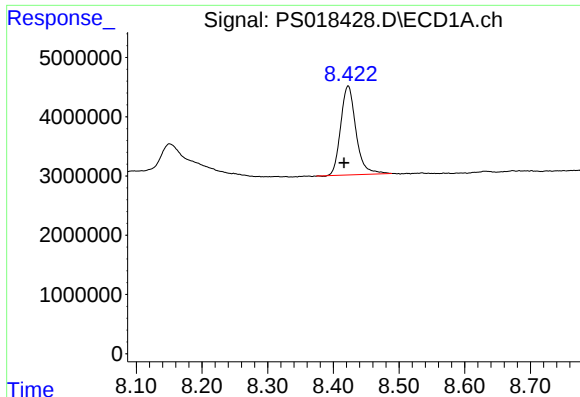

#10 Pentachlorophenol


R.T.: 8.423 min
Delta R.T.: 0.006 min
Response: 24286636
Conc: 1.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

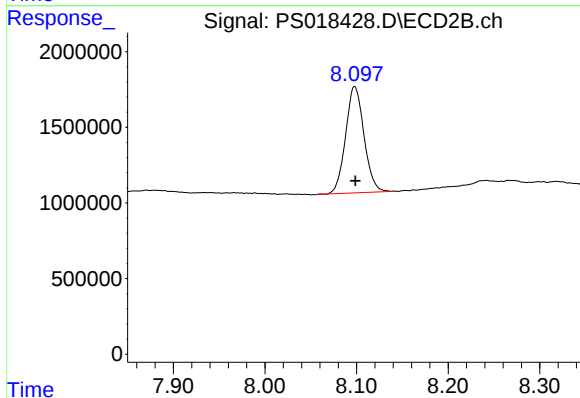


#10 Pentachlorophenol

R.T.: 8.098 min
Delta R.T.: 0.000 min
Response: 9827534
Conc: 1.03 ng/ml

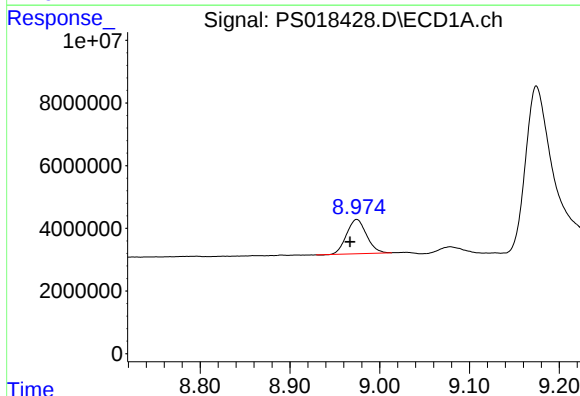


#11 2,4,5-TP (SILVEX)

R.T.: 8.974 min
Delta R.T.: 0.007 min
Response: 16903373
Conc: 1.78 ng/ml

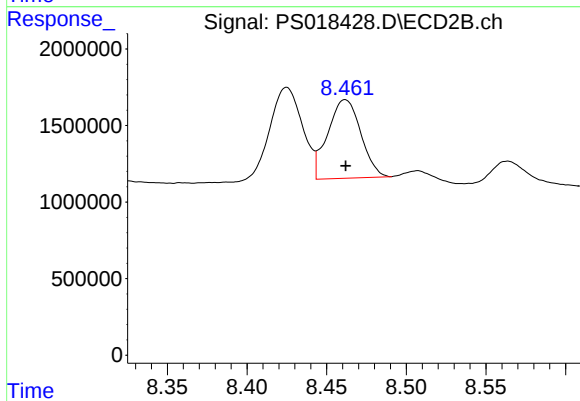

#11 2,4,5-TP (SILVEX)


R.T.: 8.462 min
Delta R.T.: 0.000 min
Response: 7425997
Conc: 1.80 ng/ml

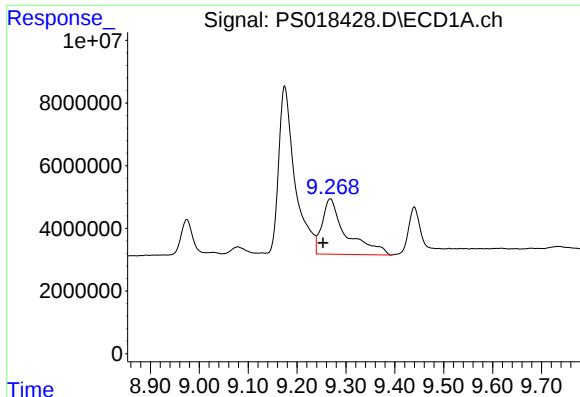

#12 2,4,5-T


R.T.: 9.268 min
Delta R.T.: 0.015 min
Response: 60486109
Conc: 6.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

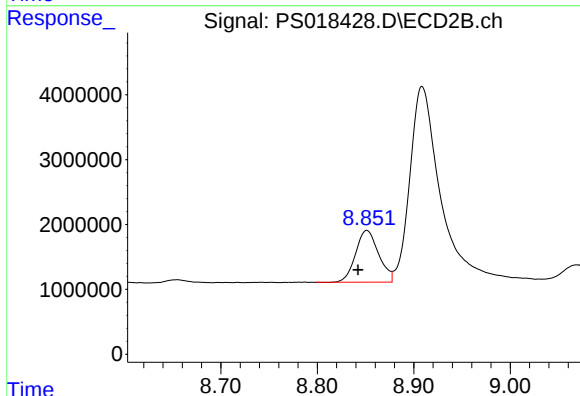


#12 2,4,5-T

R.T.: 8.851 min
Delta R.T.: 0.009 min
Response: 13247472
Conc: 3.37 ng/ml

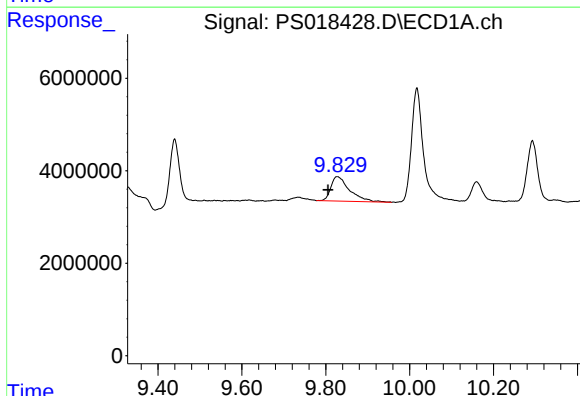


#13 2,4-DB

R.T.: 9.828 min
Delta R.T.: 0.022 min
Response: 16422332
Conc: 9.45 ng/ml

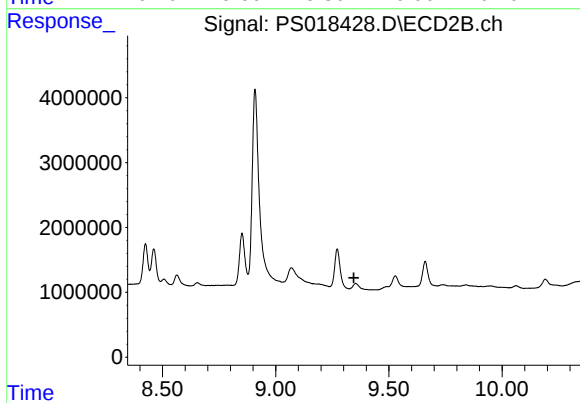

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.345 min
Response: 0
Conc: N.D.

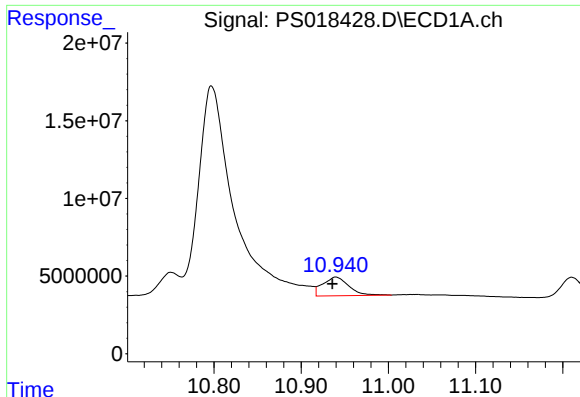

#14 DINOSEB


R.T.: 10.940 min
Delta R.T.: 0.004 min
Response: 24997971
Conc: 3.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

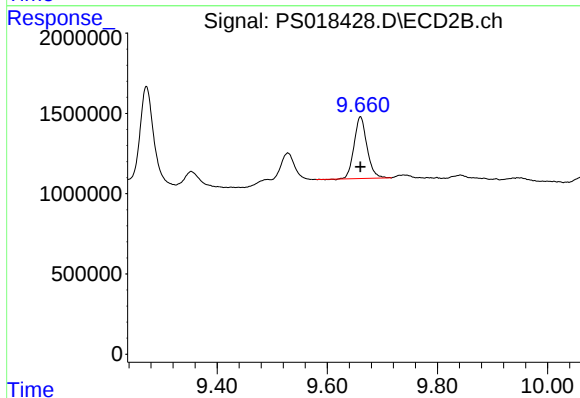


#14 DINOSEB

R.T.: 9.660 min
Delta R.T.: 0.000 min
Response: 6250637
Conc: 2.15 ng/ml

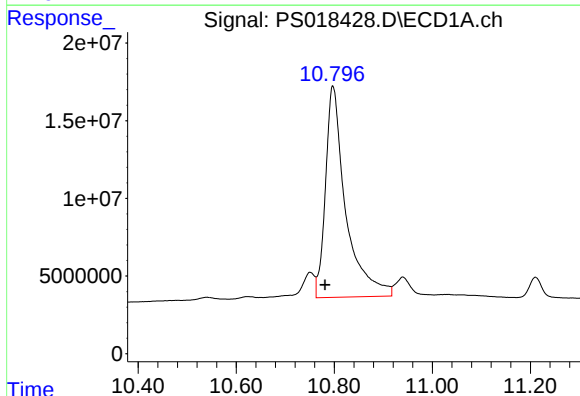


#15 Picloram

R.T.: 10.797 min
Delta R.T.: 0.016 min
Response: 388984010
Conc: 30.61 ng/ml

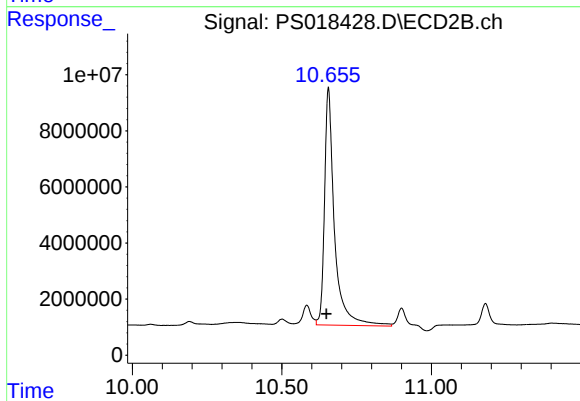

#15 Picloram


R.T.: 10.656 min
Delta R.T.: 0.007 min
Response: 196770977
Conc: 34.03 ng/ml

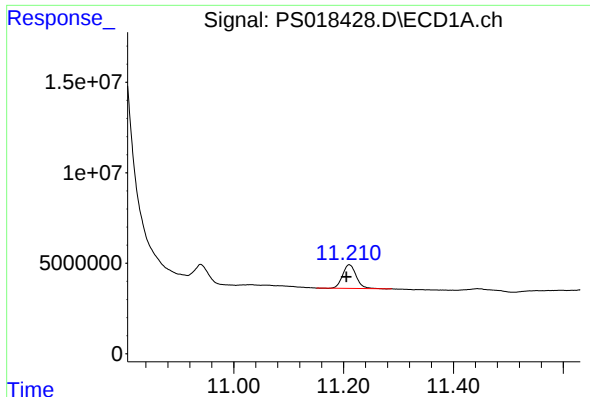

#16 DCPA

R.T.: 11.210 min
Delta R.T.: 0.005 min
Response: 22446743
Conc: 1.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

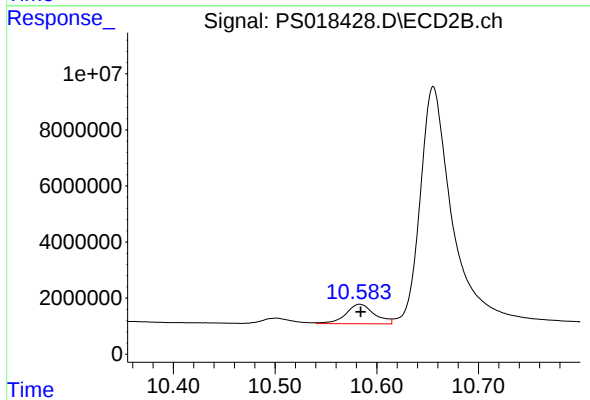

#16 DCPA

R.T.: 10.583 min
Delta R.T.: 0.000 min
Response: 13648288
Conc: 2.75 ng/ml