

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022522\
 Data File : PS018429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2022 08:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 21:32:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.029	6.641	604.9E6	387.2E6	363.506	581.046 #
Target Compounds							
10) T	Pentachlo...	0.000	8.111	0	1911918	N.D.	<MDL
11) T	2,4,5-TP ...	8.979	8.443	3245666	13206948	<MDL	3.199 #
12) T	2,4,5-T	9.225	8.896f	91688179	3266546	9.115	<MDL #
13) T	2,4-DB	0.000	9.289f	0	16281880	N.D.	30.137
15) T	Picloram	10.844f	10.698f	255.5E6	134.4E6	20.108	23.246
16) T	DCPA	11.210	10.589	4787687	4738331	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022522\
Data File : PS018429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2022 08:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 21:32:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

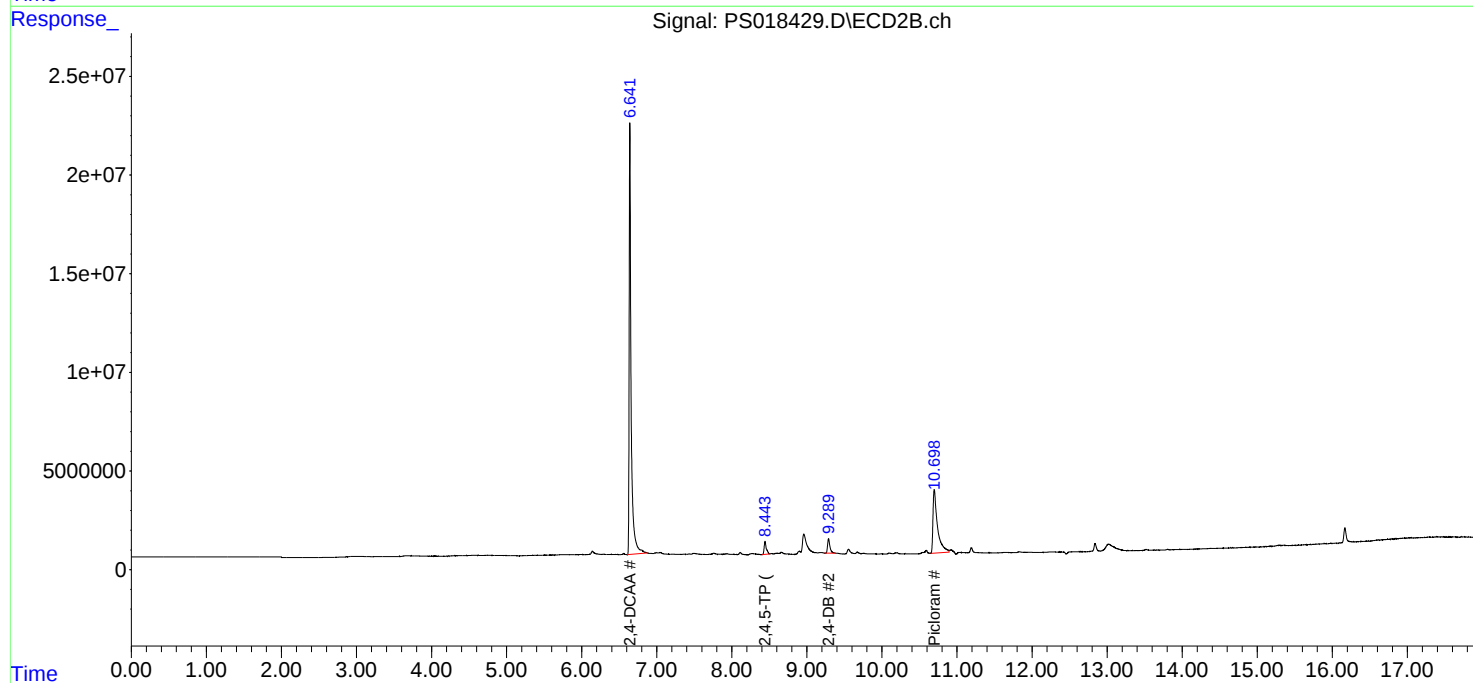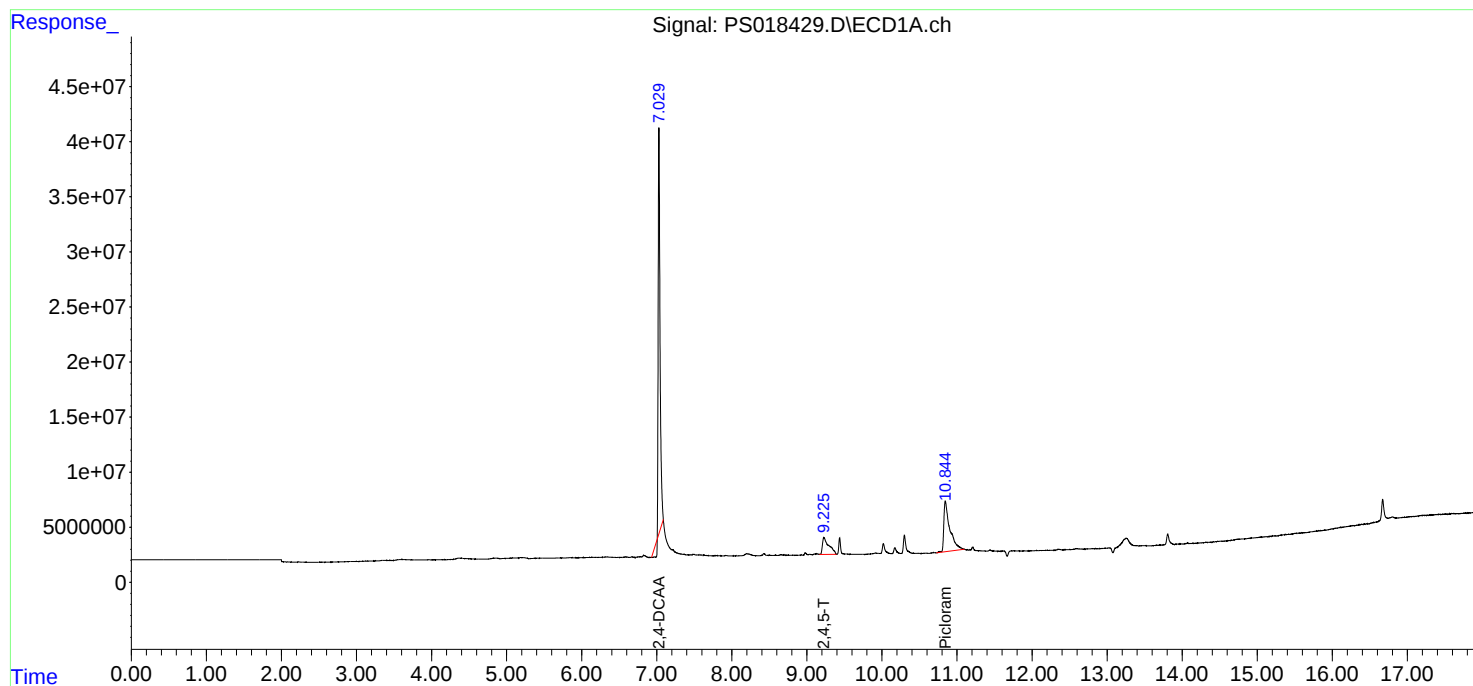


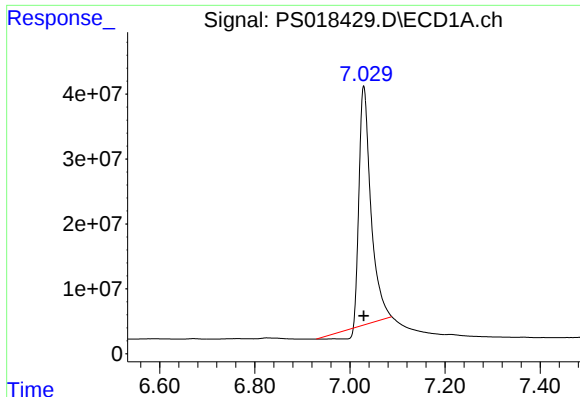

#4 2,4-DCAA


R.T.: 7.029 min
Delta R.T.: 0.000 min
Response: 604891444
Conc: 363.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

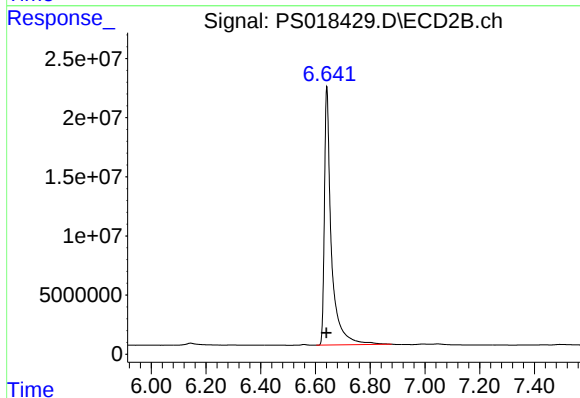


#4 2,4-DCAA

R.T.: 6.641 min
Delta R.T.: 0.001 min
Response: 387175453
Conc: 581.05 ng/ml

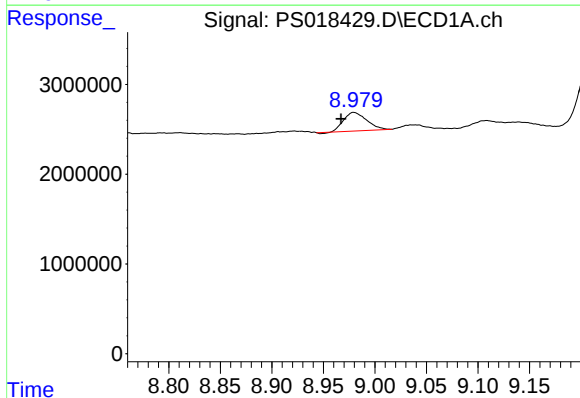


#11 2,4,5-TP (SILVEX)

R.T.: 8.979 min
Delta R.T.: 0.012 min
Response: 3245666
Conc: N.D.

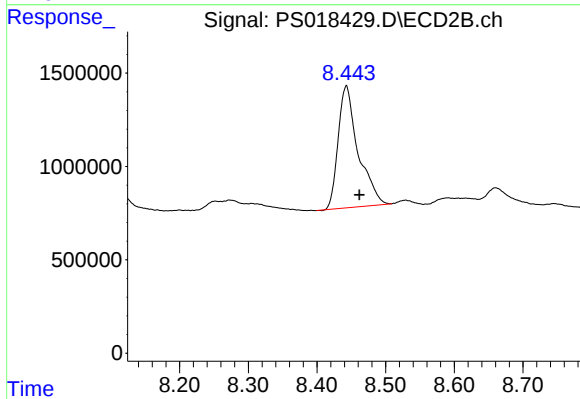

#11 2,4,5-TP (SILVEX)


R.T.: 8.443 min
Delta R.T.: -0.019 min
Response: 13206948
Conc: 3.20 ng/ml

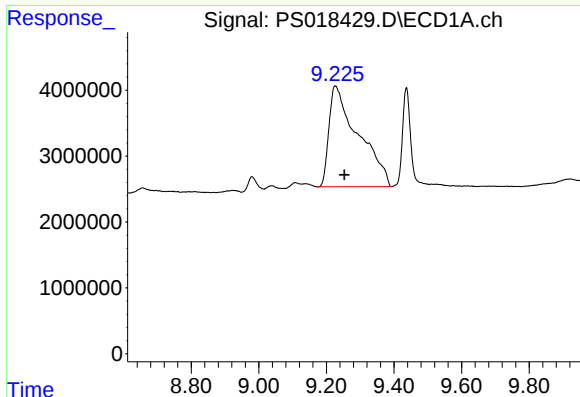

#12 2,4,5-T


R.T.: 9.225 min
Delta R.T.: -0.028 min
Response: 91688179
Conc: 9.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

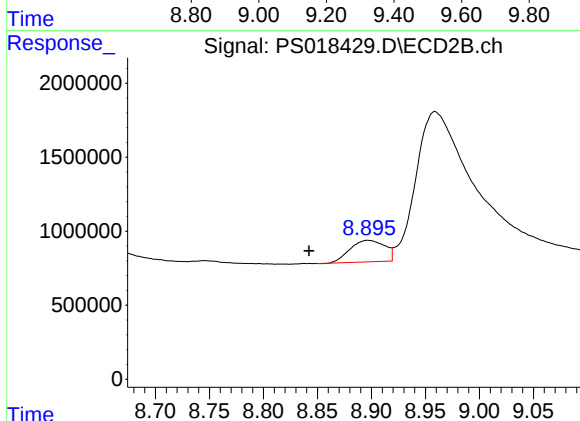


#12 2,4,5-T

R.T.: 8.896 min
Delta R.T.: 0.054 min
Response: 3266546
Conc: N.D.

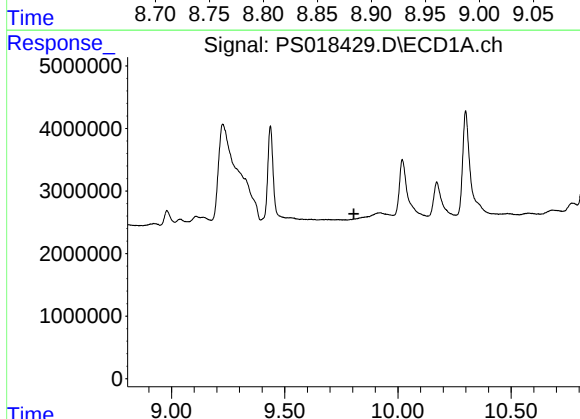


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.806 min
Response: 0
Conc: N.D.

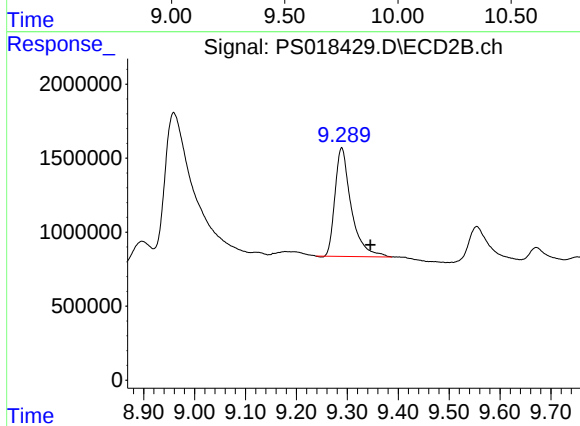

#13 2,4-DB


R.T.: 9.289 min
Delta R.T.: -0.056 min
Response: 16281880
Conc: 30.14 ng/ml

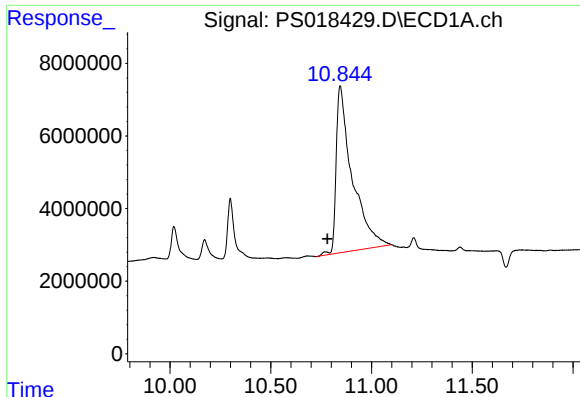

#15 Picloram

R.T.: 10.844 min
Delta R.T.: 0.063 min
Response: 255497730
Conc: 20.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

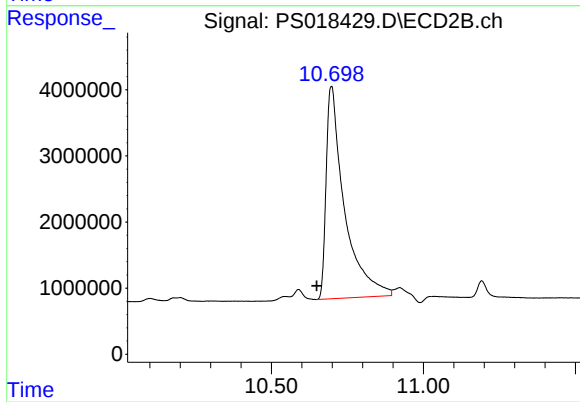

#15 Picloram

R.T.: 10.698 min
Delta R.T.: 0.049 min
Response: 134431198
Conc: 23.25 ng/ml