

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022522\
 Data File : PS018444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Feb 2022 22:22
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 25 23:04:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.026	6.639	764.8E6	394.3E6	459.589	591.710 #
Target Compounds							
5) T	DICAMBA	0.000	6.793	0	1433592	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.468f	0	2220132	N.D.	3.015
9) T	2,4-D	8.187f	0.000	4110281	0	2.015	N.D. #
11) T	2,4,5-TP ...	9.025f	8.434	7168993	22238348	<MDL	5.386 #
12) T	2,4,5-T	9.216	8.878	13671469	3021743	1.359	<MDL #
13) T	2,4-DB	0.000	9.358	0	3067752	N.D.	5.678
14) T	DINOSEB	10.913	9.677	27043171	6246380	3.481	2.149 #
15) T	Picloram	10.757	10.690f	14078982	36700628	1.108	6.346 #
16) T	DCPA	0.000	10.587	0	2384248	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022522\
Data File : PS018444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Feb 2022 22:22
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 25 23:04:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

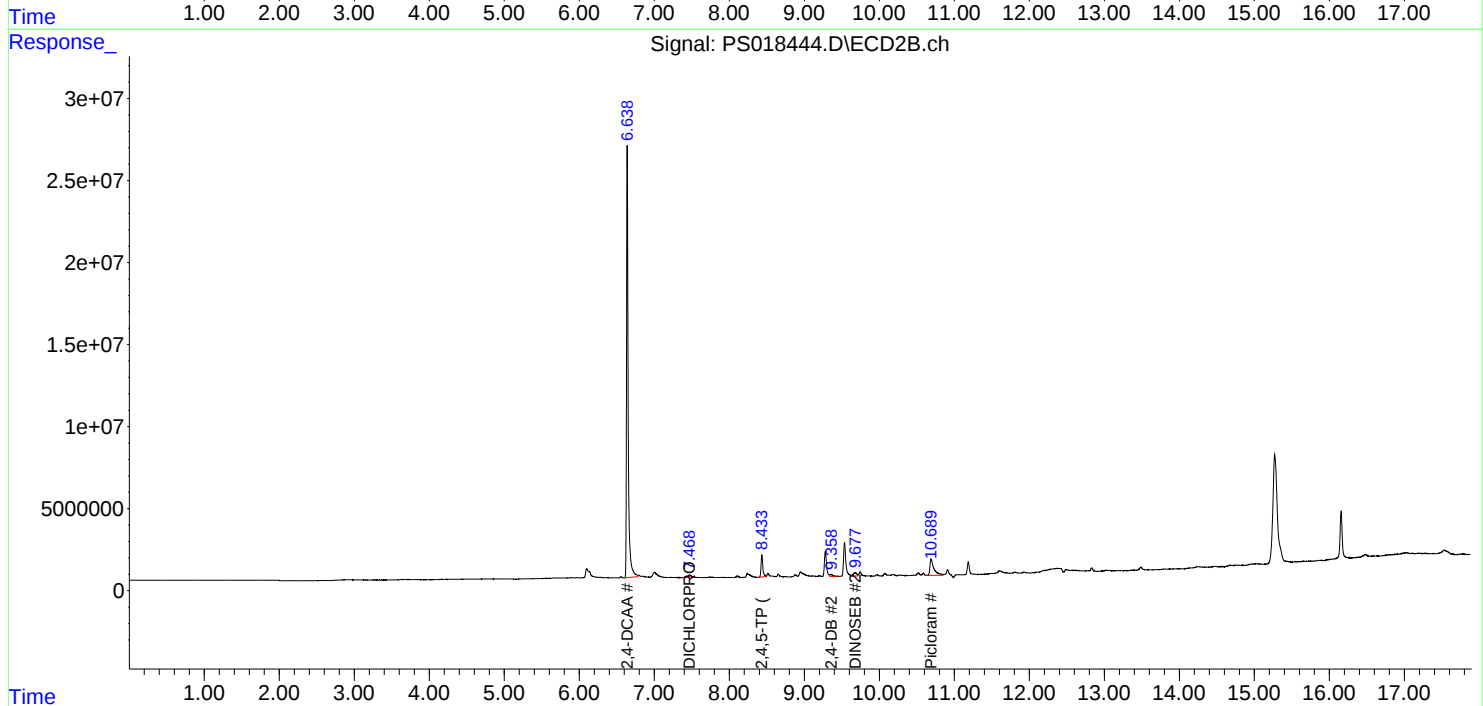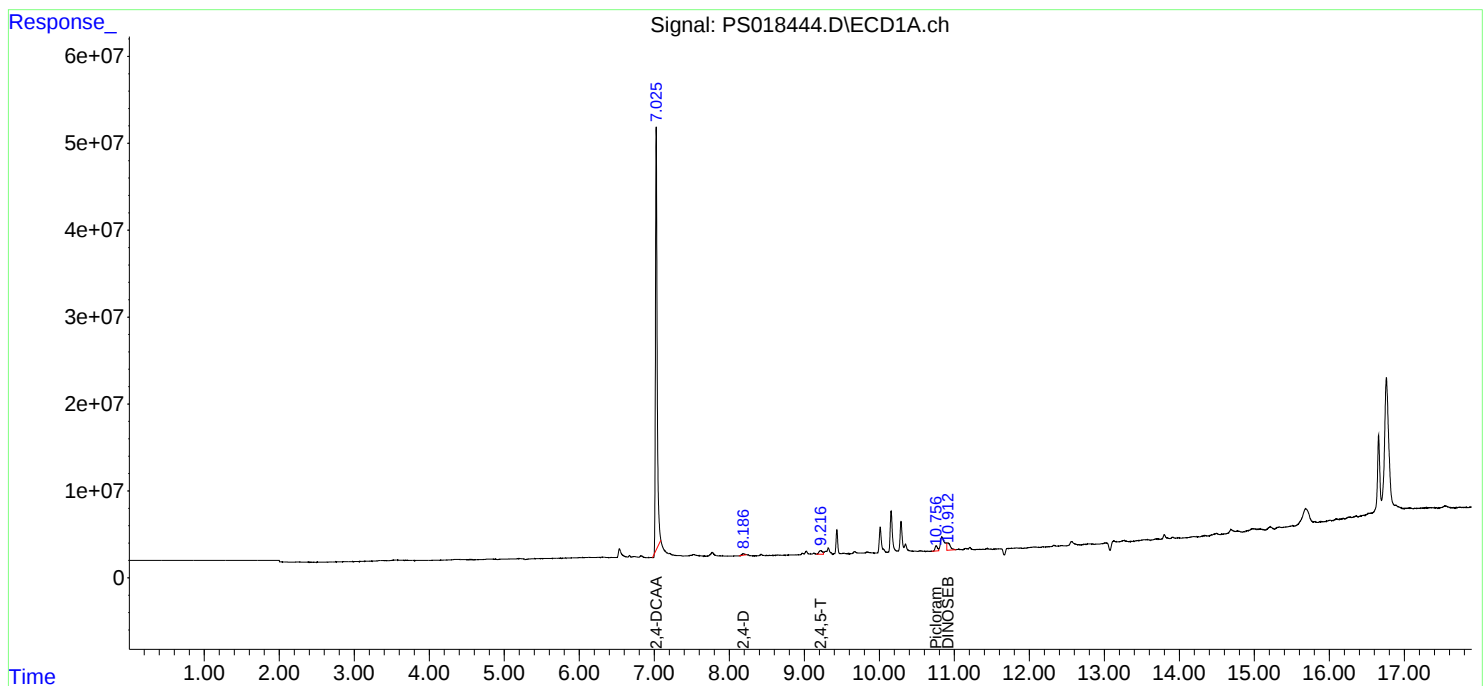


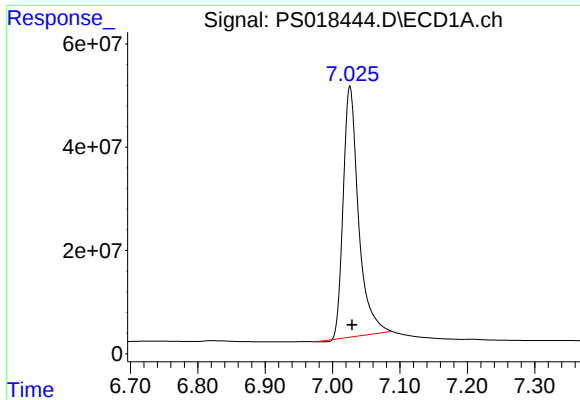

#4 2,4-DCAA


R.T.: 7.026 min
Delta R.T.: -0.003 min
Response: 764778998
Conc: 459.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

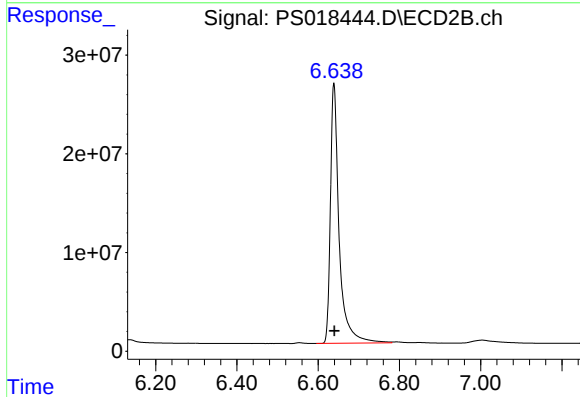


#4 2,4-DCAA

R.T.: 6.639 min
Delta R.T.: -0.001 min
Response: 394281693
Conc: 591.71 ng/ml

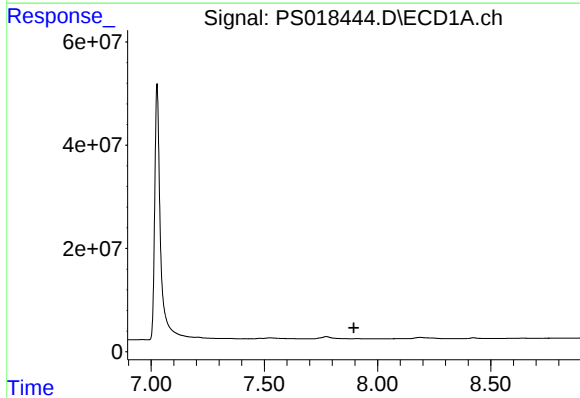


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.896 min
Response: 0
Conc: N.D.

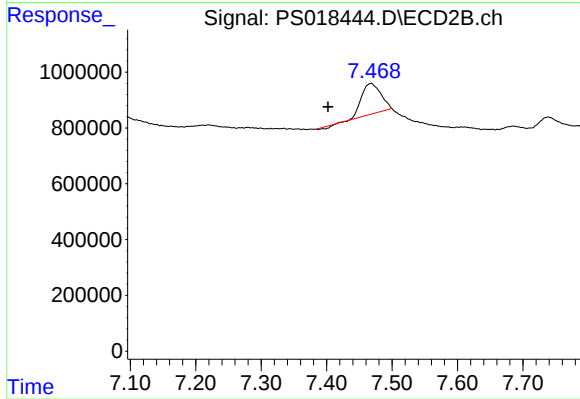

#8 DICHLORPROP


R.T.: 7.468 min
Delta R.T.: 0.066 min
Response: 2220132
Conc: 3.02 ng/ml

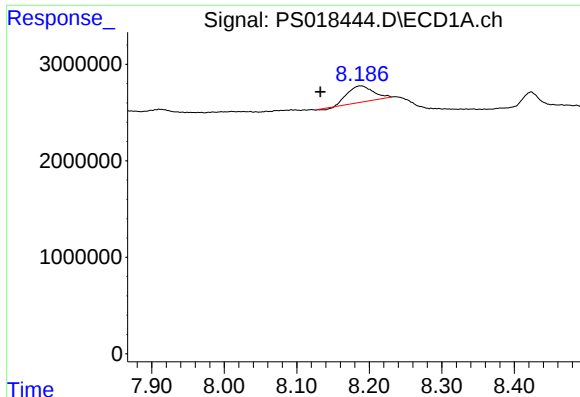

#9 2,4-D


R.T.: 8.187 min
Delta R.T.: 0.055 min
Response: 4110281
Conc: 2.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

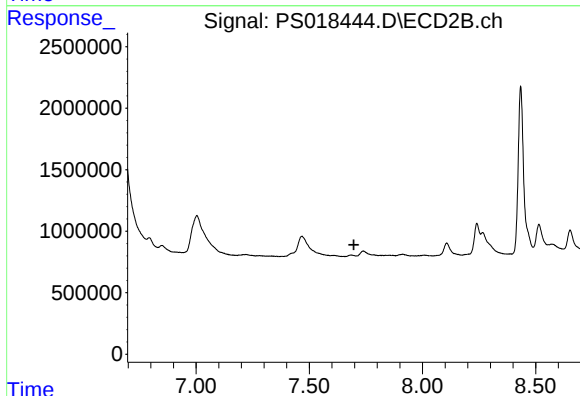


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.697 min
Response: 0
Conc: N.D.

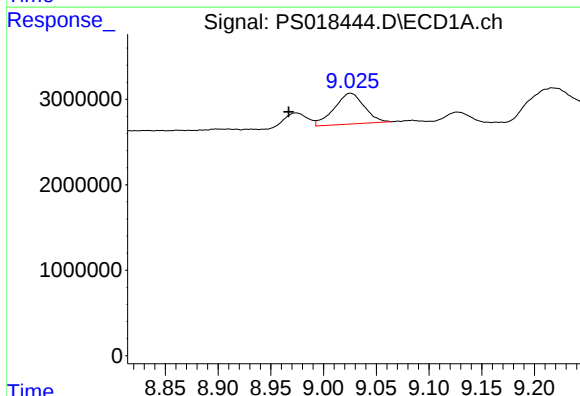


#11 2,4,5-TP (SILVEX)

R.T.: 9.025 min
Delta R.T.: 0.058 min
Response: 7168993
Conc: N.D.

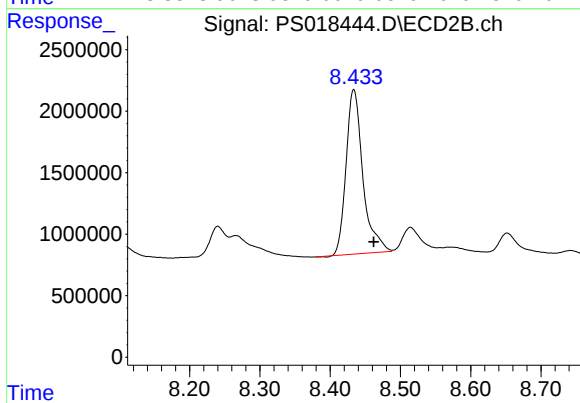

#11 2,4,5-TP (SILVEX)


R.T.: 8.434 min
Delta R.T.: -0.028 min
Response: 22238348
Conc: 5.39 ng/ml

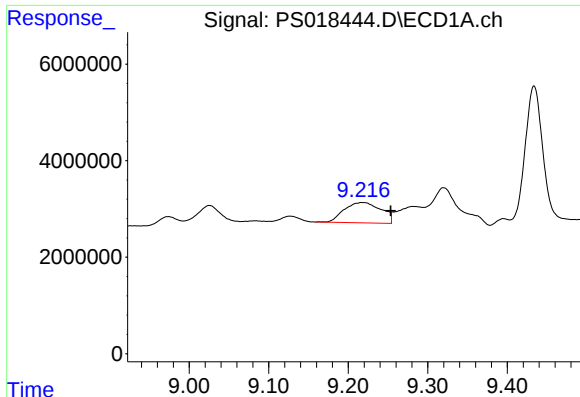

#12 2,4,5-T


R.T.: 9.216 min
Delta R.T.: -0.037 min
Response: 13671469
Conc: 1.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

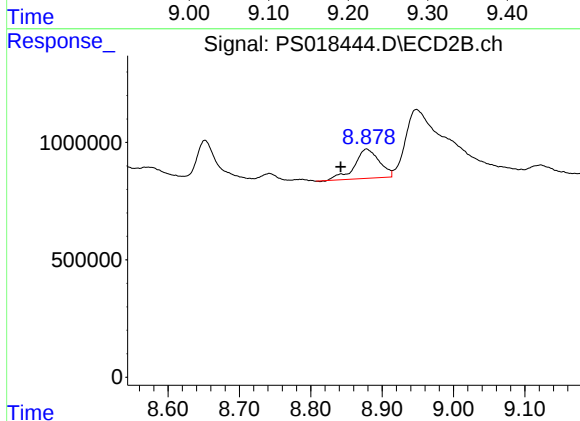


#12 2,4,5-T

R.T.: 8.878 min
Delta R.T.: 0.036 min
Response: 3021743
Conc: N.D.

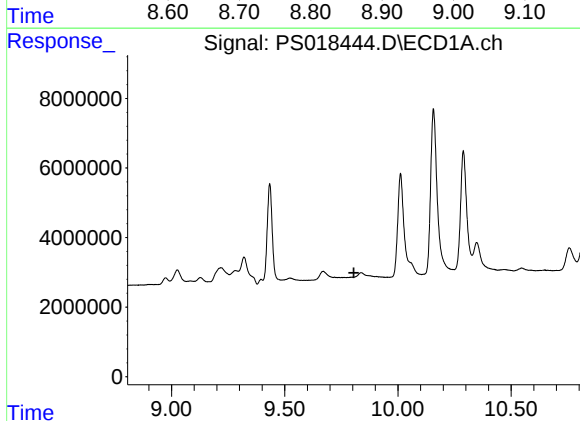


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.806 min
Response: 0
Conc: N.D.

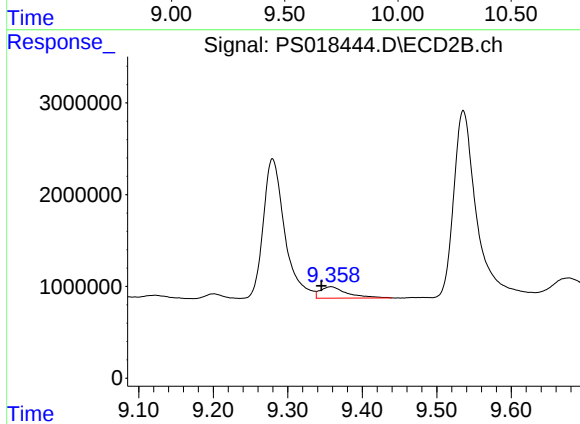

#13 2,4-DB


R.T.: 9.358 min
Delta R.T.: 0.013 min
Response: 3067752
Conc: 5.68 ng/ml

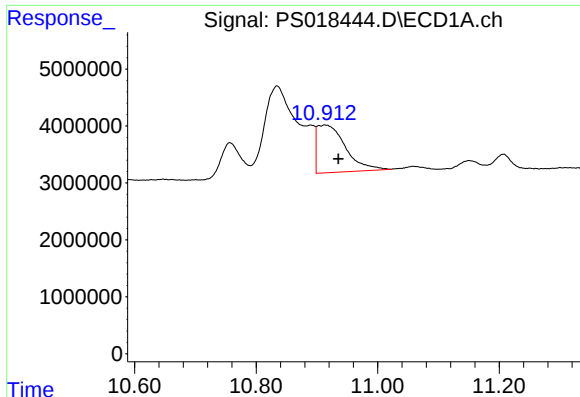

#14 DINoseb


R.T.: 10.913 min
Delta R.T.: -0.023 min
Response: 27043171
Conc: 3.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

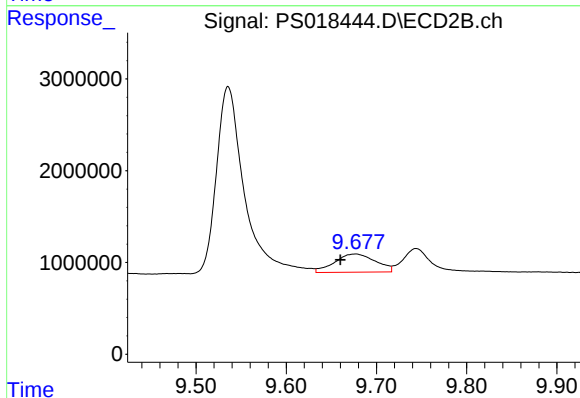


#14 DINoseb

R.T.: 9.677 min
Delta R.T.: 0.017 min
Response: 6246380
Conc: 2.15 ng/ml

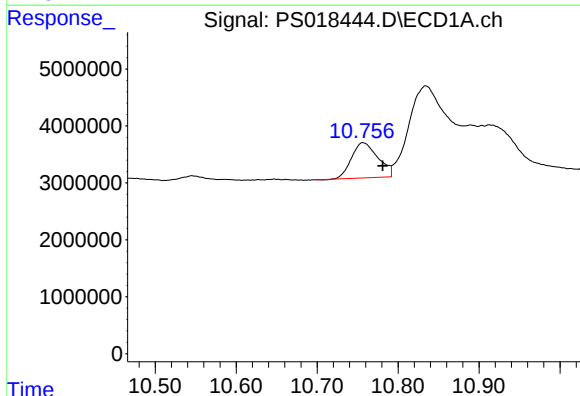

#15 Picloram

R.T.: 10.757 min
Delta R.T.: -0.025 min
Response: 14078982
Conc: 1.11 ng/ml

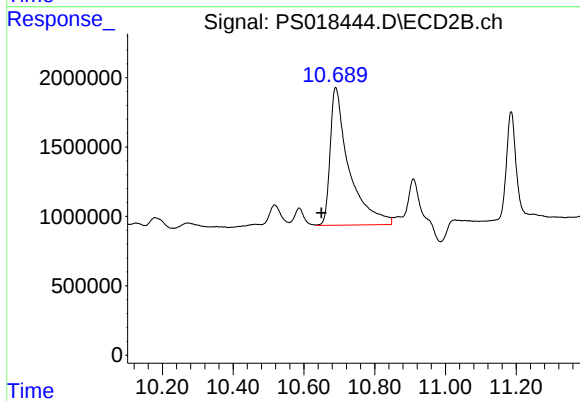

#15 Picloram

R.T.: 10.690 min
Delta R.T.: 0.041 min
Response: 36700628
Conc: 6.35 ng/ml