

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
 Data File : PS003337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2019 09:31
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:49:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.777	173.7E6	317.0E6	457.417	741.545 #
Target Compounds							
1) T	Dalapon	2.838	2.312	81071829	383.8E6	146.963	716.190 #
2) T	3,5-DICHL...	0.000	8.938	0	5217686	N.D.	9.258 #
3) T	4-Nitroph...	10.876	9.930	120.0E6	147.5E6	620.171	705.503
8) T	DICHLORPROP	0.000	12.182	0	276.7E6	N.D.	723.738 #
9) T	2,4-D	13.137	12.655	108.5E6	231.0E6	235.220	460.734 #
11) T	2,4,5-TP ...	14.374	13.814	1881.2E6	1790.7E6	746.986	721.965
12) T	2,4,5-T	14.777	14.378	1784.9E6	235.7E6	731.675	123.163 #
14) T	DINOSEB	16.985	0.000	1453.6E6	0	772.668	N.D. #
15) T	Picloram	16.769	16.687	1794.0E6	1672.4E6	567.061	556.288
16) T	DCPA	0.000	16.687	0	1672.4E6	N.D.	539.912 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
Data File : PS003337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2019 09:31
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:49:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

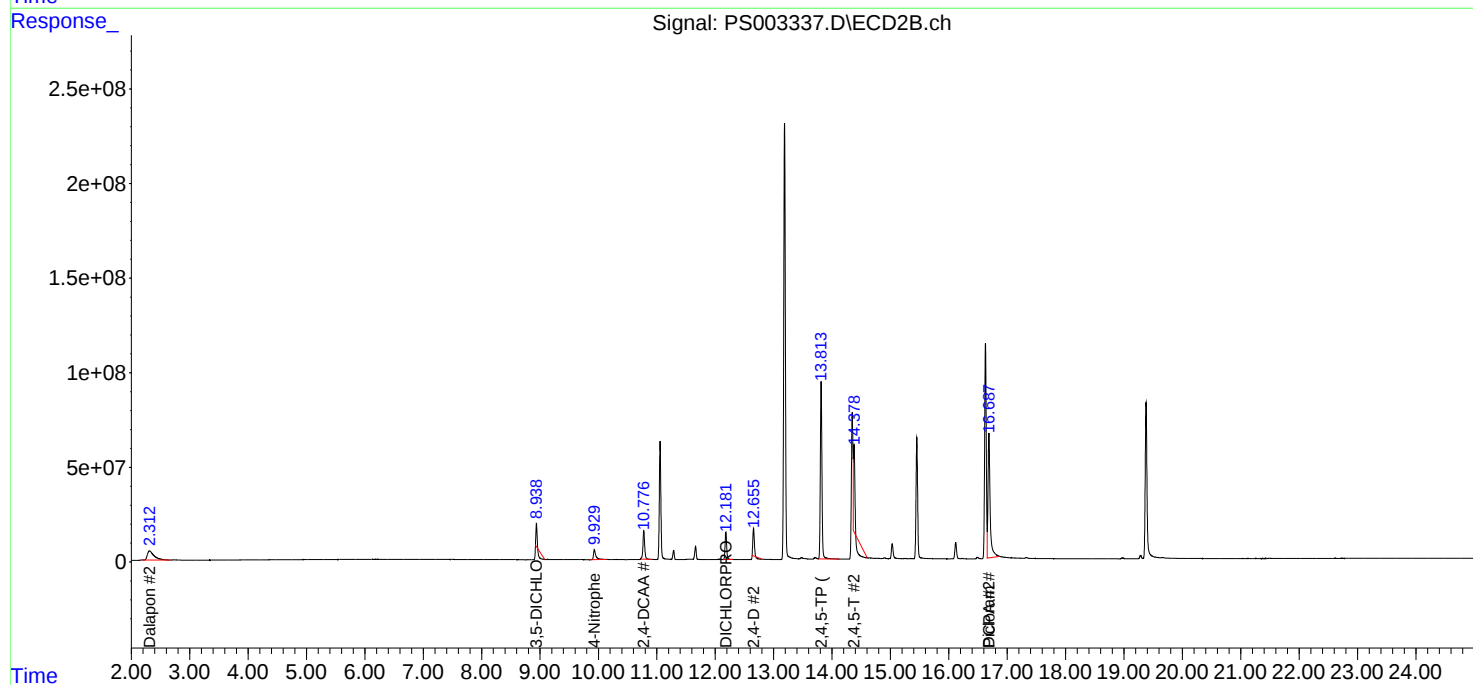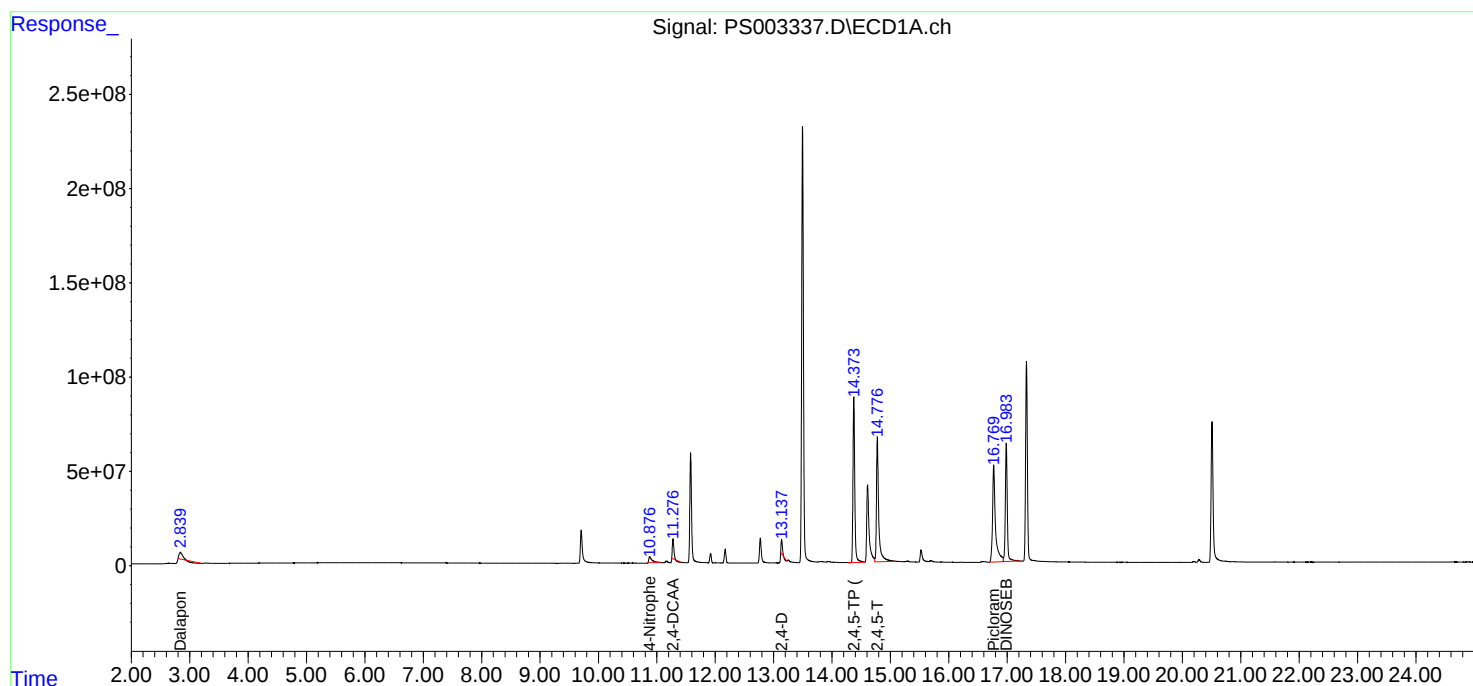


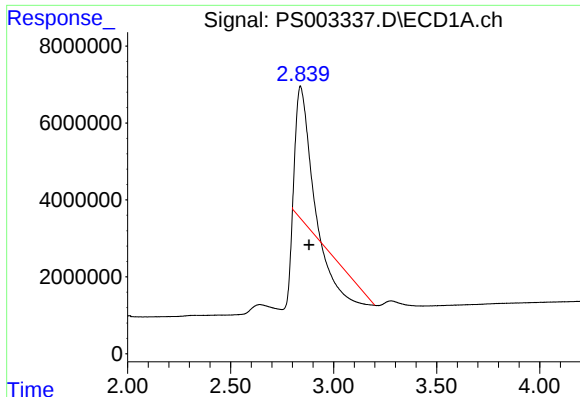

#1 Dalapon


R.T.: 2.838 min
Delta R.T.: -0.042 min
Response: 81071829
Conc: 146.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

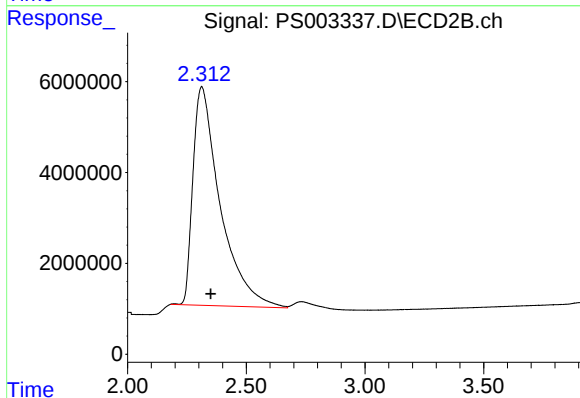


#1 Dalapon

R.T.: 2.312 min
Delta R.T.: -0.039 min
Response: 383821429
Conc: 716.19 ng/ml

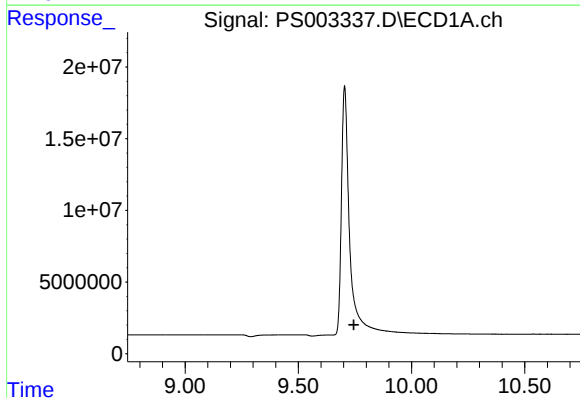


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

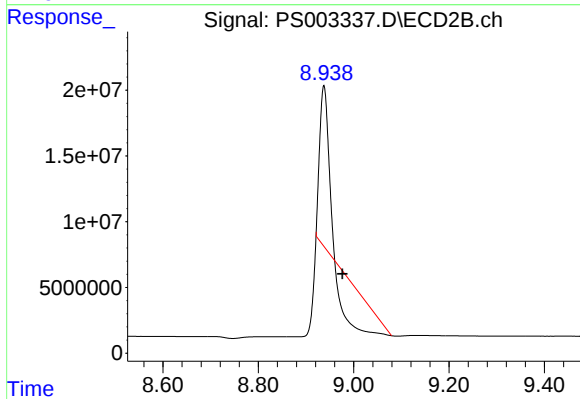

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.938 min
Delta R.T.: -0.039 min
Response: 5217686
Conc: 9.26 ng/ml

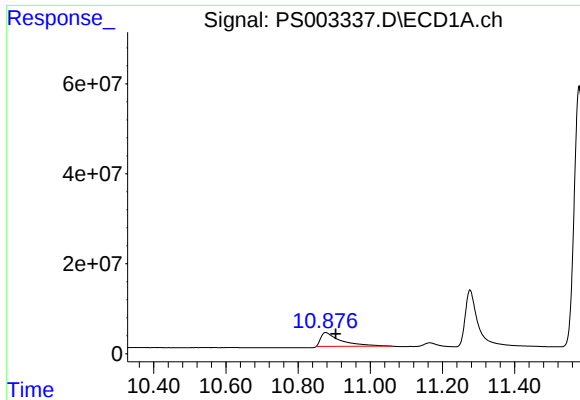

#3 4-Nitrophenol


R.T.: 10.876 min
Delta R.T.: -0.028 min
Response: 120027278
Conc: 620.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

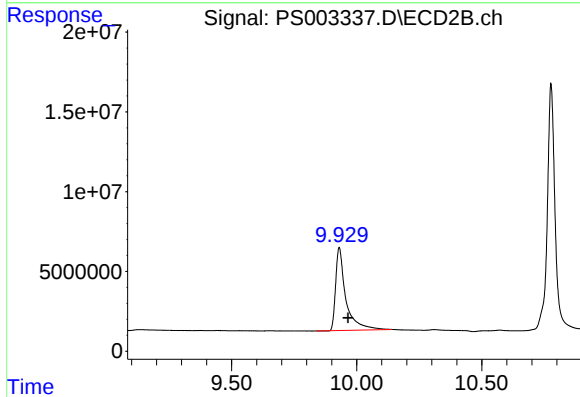


#3 4-Nitrophenol

R.T.: 9.930 min
Delta R.T.: -0.035 min
Response: 147465950
Conc: 705.50 ng/ml

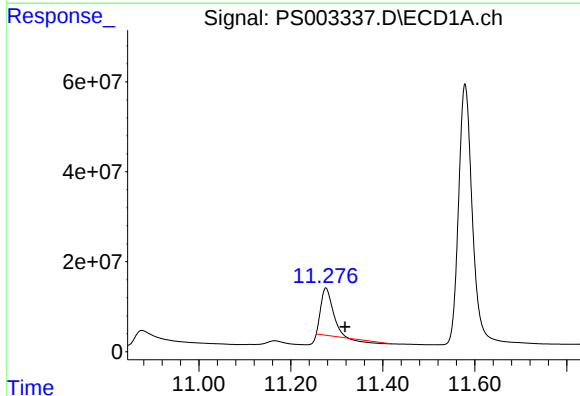


#4 2,4-DCAA

R.T.: 11.276 min
Delta R.T.: -0.042 min
Response: 173654139
Conc: 457.42 ng/ml

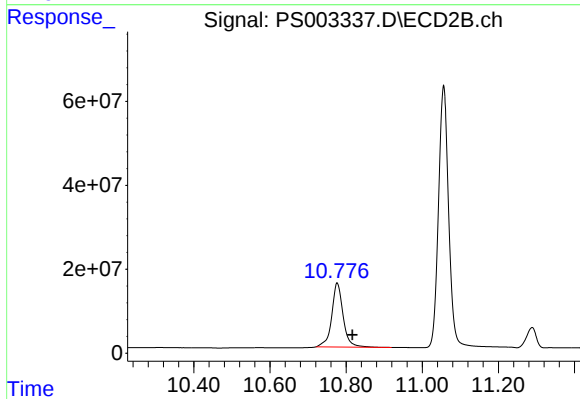

#4 2,4-DCAA


R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 317044349
Conc: 741.54 ng/ml

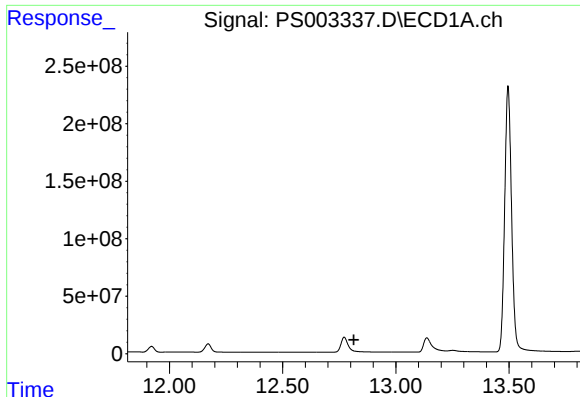

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

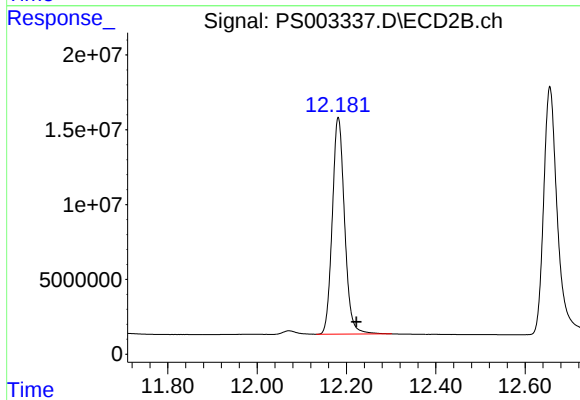


#8 DICHLORPROP

R.T.: 12.182 min
Delta R.T.: -0.040 min
Response: 276714851
Conc: 723.74 ng/ml

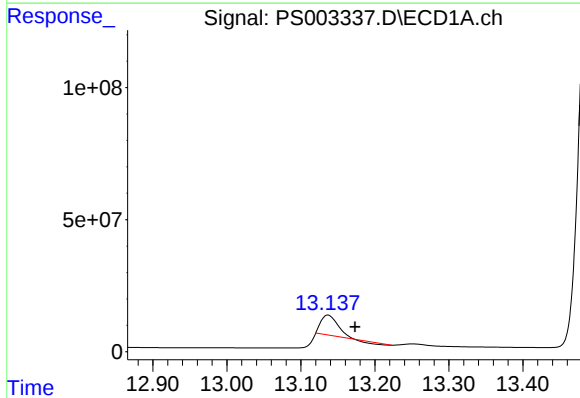


#9 2,4-D

R.T.: 13.137 min
Delta R.T.: -0.037 min
Response: 108450066
Conc: 235.22 ng/ml

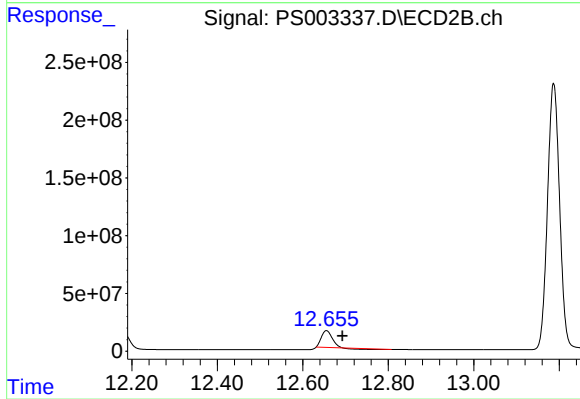

#9 2,4-D


R.T.: 12.655 min
Delta R.T.: -0.037 min
Response: 231005269
Conc: 460.73 ng/ml

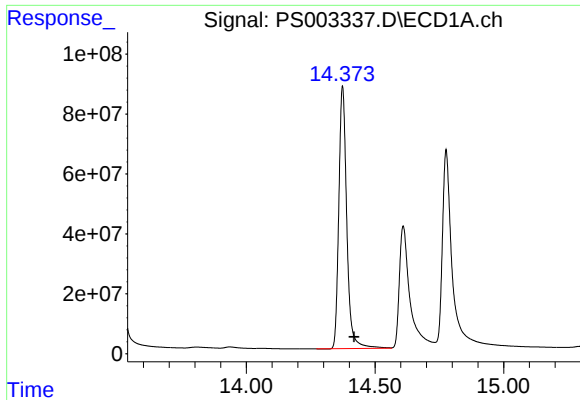

#11 2,4,5-TP (SILVEX)


R.T.: 14.374 min
Delta R.T.: -0.046 min
Response: 1881189879
Conc: 746.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

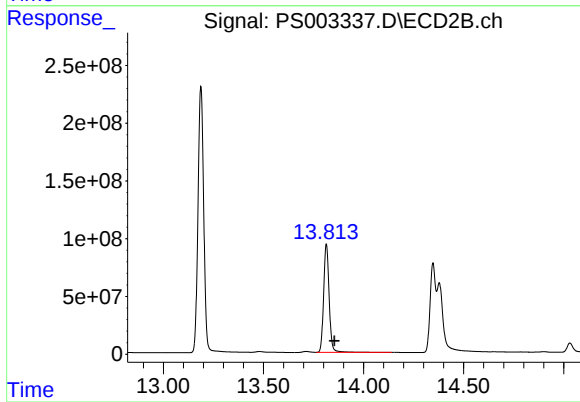


#11 2,4,5-TP (SILVEX)

R.T.: 13.814 min
Delta R.T.: -0.040 min
Response: 1790729570
Conc: 721.96 ng/ml

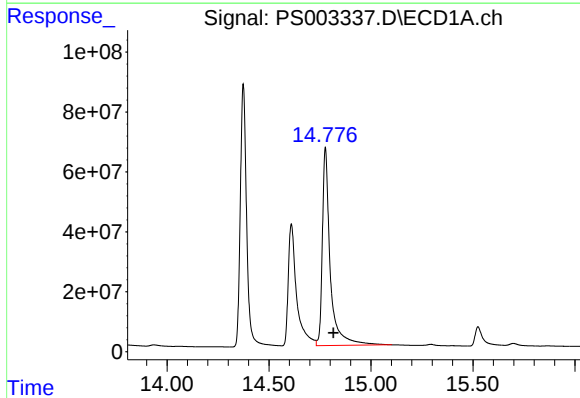


#12 2,4,5-T

R.T.: 14.777 min
Delta R.T.: -0.040 min
Response: 1784852412
Conc: 731.68 ng/ml

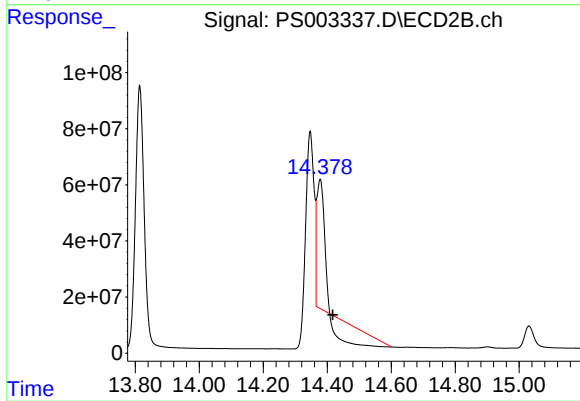

#12 2,4,5-T


R.T.: 14.378 min
Delta R.T.: -0.039 min
Response: 235671831
Conc: 123.16 ng/ml

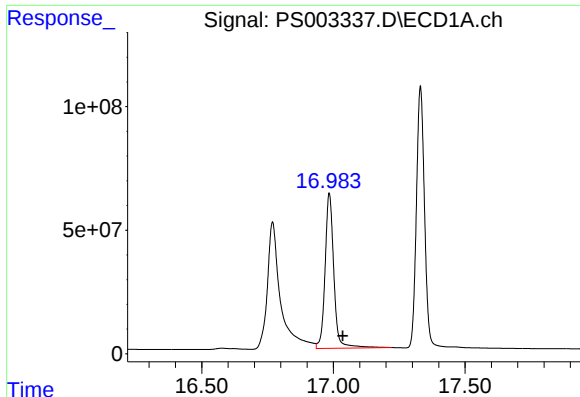

#14 DINOSEB


R.T.: 16.985 min
Delta R.T.: -0.051 min
Response: 1453641906
Conc: 772.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

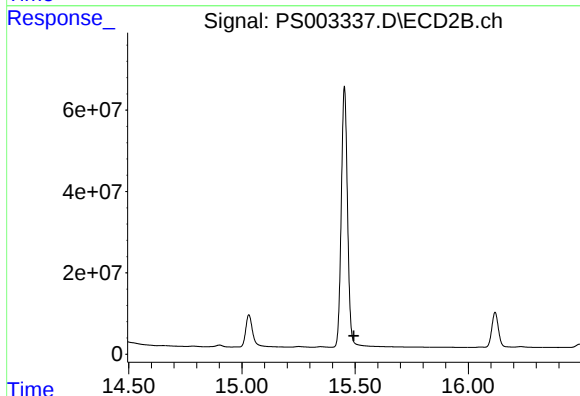


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 15.495 min
Response: 0
Conc: N.D.

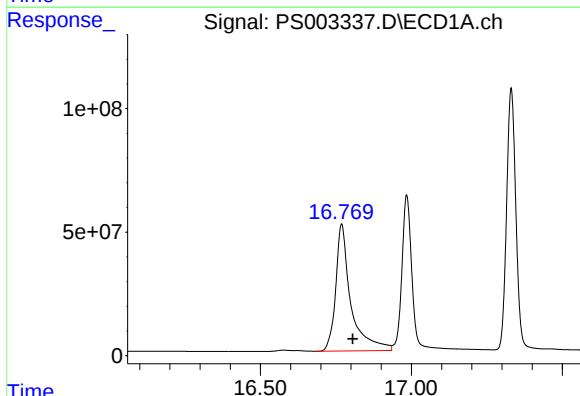


#15 Picloram

R.T.: 16.769 min
Delta R.T.: -0.037 min
Response: 1793973299
Conc: 567.06 ng/ml

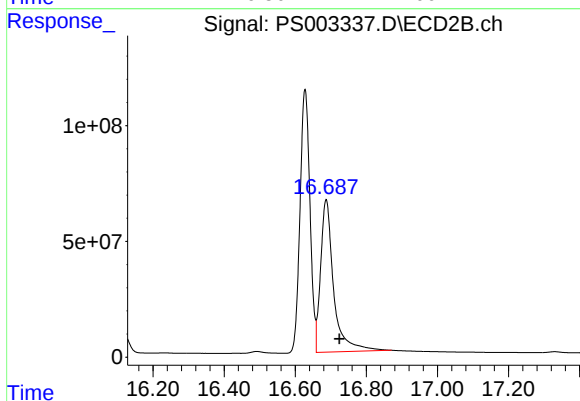

#15 Picloram


R.T.: 16.687 min
Delta R.T.: -0.037 min
Response: 1672426147
Conc: 556.29 ng/ml

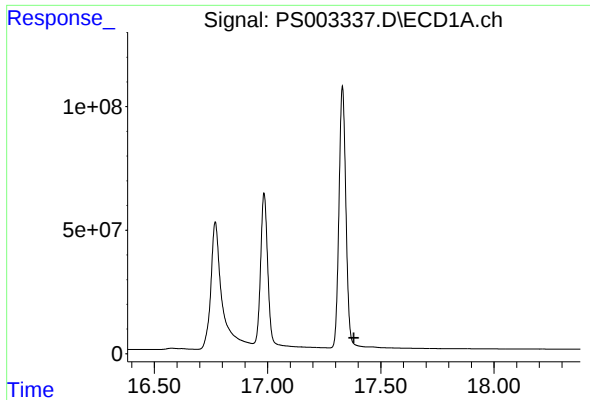

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

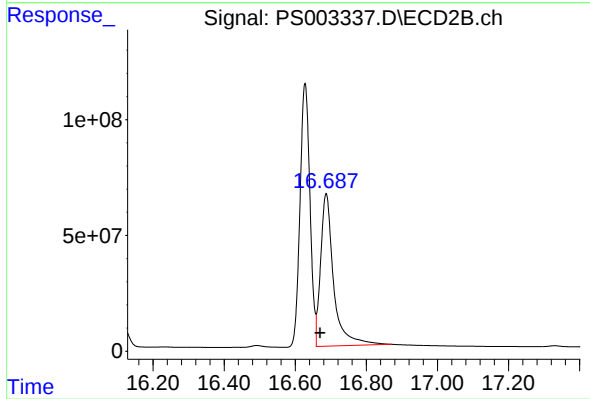

#16 DCPA

R.T.: 16.687 min
Delta R.T.: 0.017 min
Response: 1672426147
Conc: 539.91 ng/ml