

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
 Data File : PS003338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2019 10:29
 Operator : EI\SJ
 Sample : K1348-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-022219-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:50:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.282	10.773	100.4E6	154.0E6	264.446	360.177 #
Target Compounds							
6) T	MCP	11.988	0.000	3779099	0	3.154	N.D. #
7) T	MCPA	12.221	0.000	6133993	0	3.466	N.D. #
12) T	2,4,5-T	0.000	14.403	0	7789327	N.D.	4.071 #
15) T	Picloram	16.851	16.711	2116931	13623201	0.669	4.531 #
16) T	DCPA	0.000	16.633	0	2039009	N.D.	0.658 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
Data File : PS003338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2019 10:29
Operator : EI\SJ
Sample : K1348-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:50:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

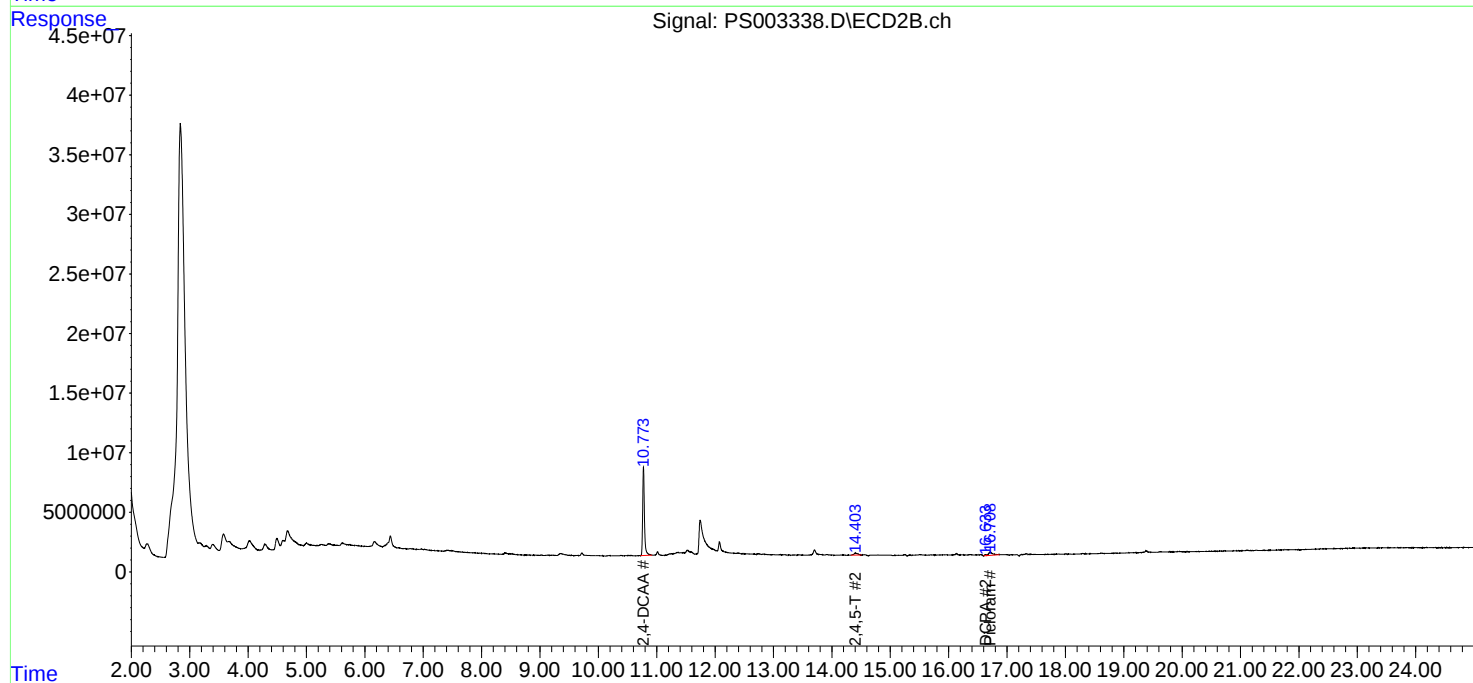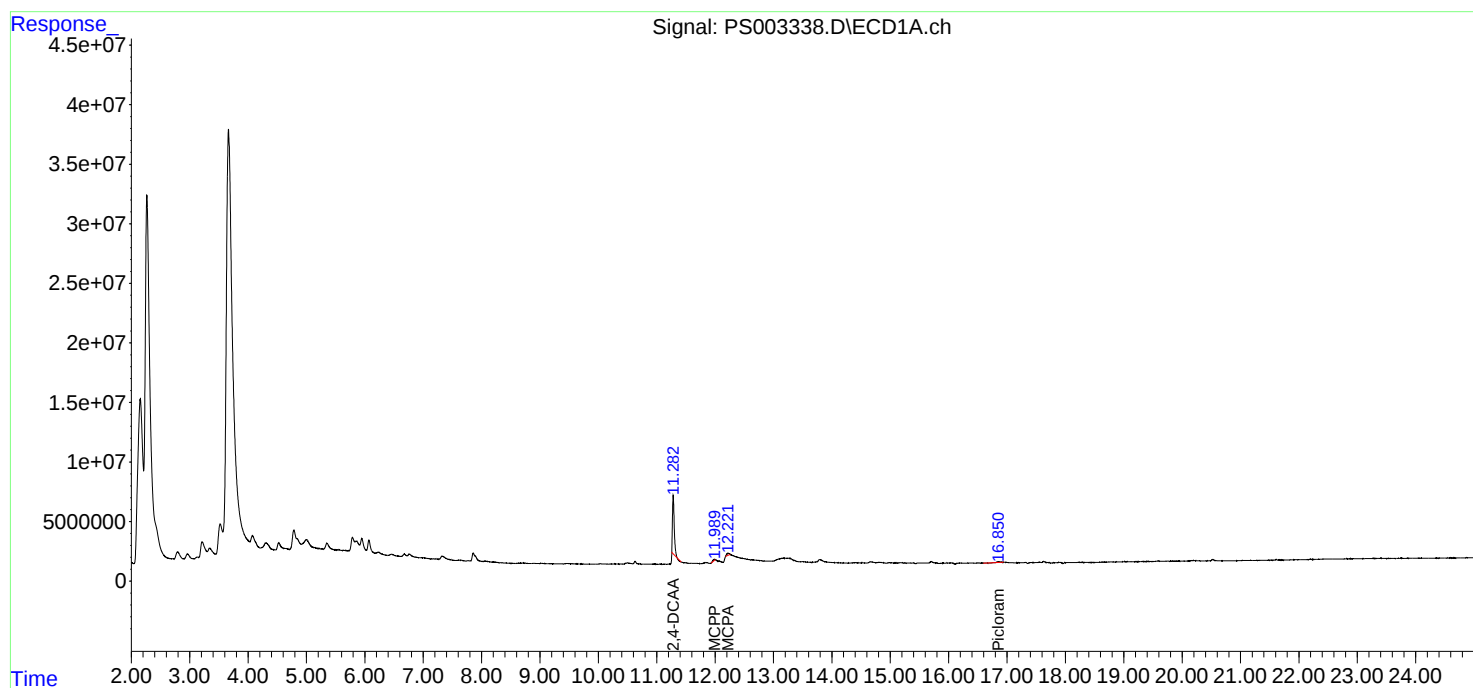


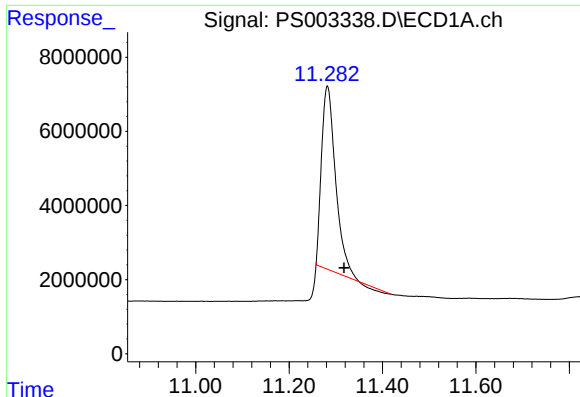

#4 2,4-DCAA


R.T.: 11.282 min
Delta R.T.: -0.036 min
Response: 100394454
Conc: 264.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-A

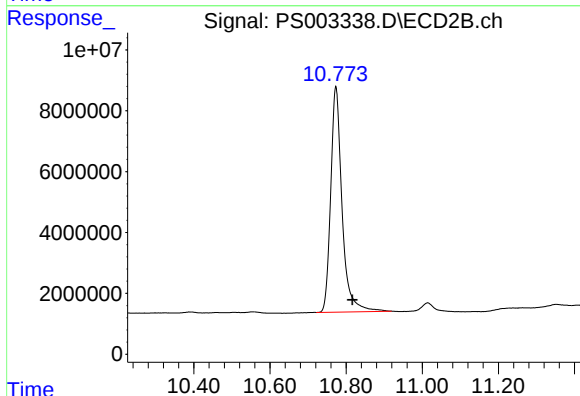


#4 2,4-DCAA

R.T.: 10.773 min
Delta R.T.: -0.044 min
Response: 153992231
Conc: 360.18 ng/ml

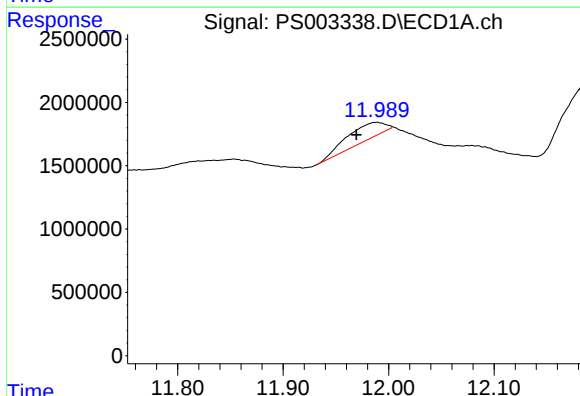


#6 MCPP

R.T.: 11.988 min
Delta R.T.: 0.019 min
Response: 3779099
Conc: 3.15 ug/ml

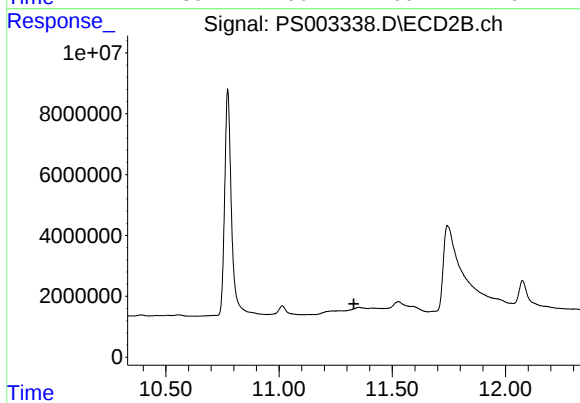

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

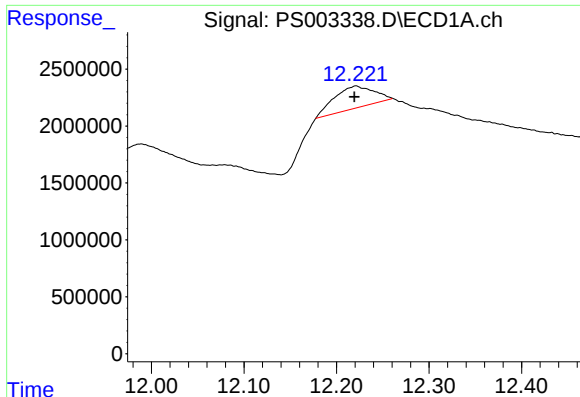

#7 MCPA


R.T.: 12.221 min
Delta R.T.: 0.002 min
Response: 6133993
Conc: 3.47 ug/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-A

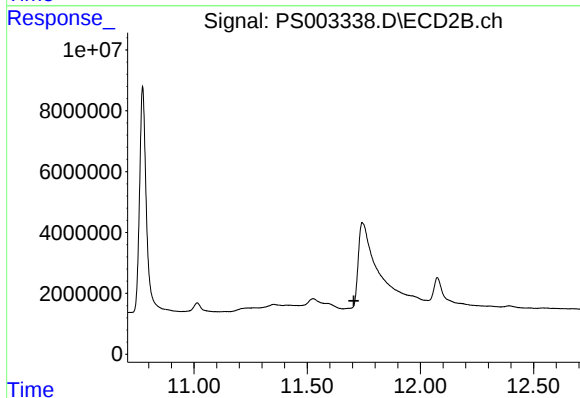


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

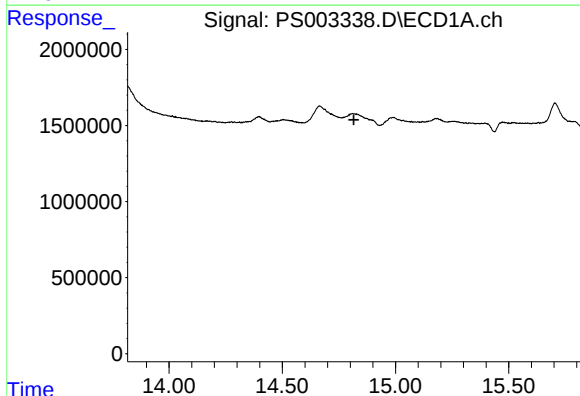


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

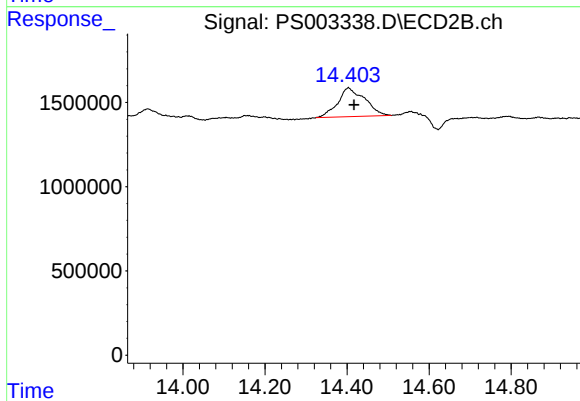

#12 2,4,5-T


R.T.: 14.403 min
Delta R.T.: -0.014 min
Response: 7789327
Conc: 4.07 ng/ml

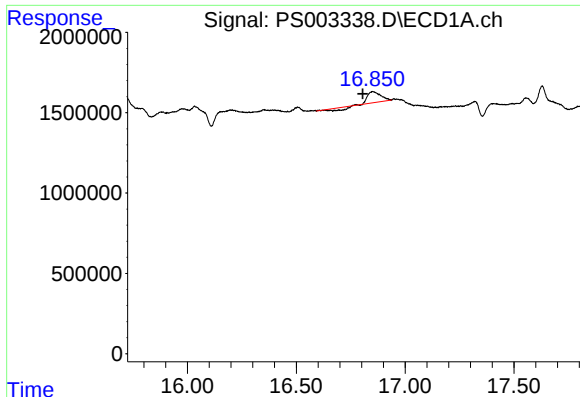

#15 Picloram


R.T.: 16.851 min
Delta R.T.: 0.045 min
Response: 2116931
Conc: 0.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-A

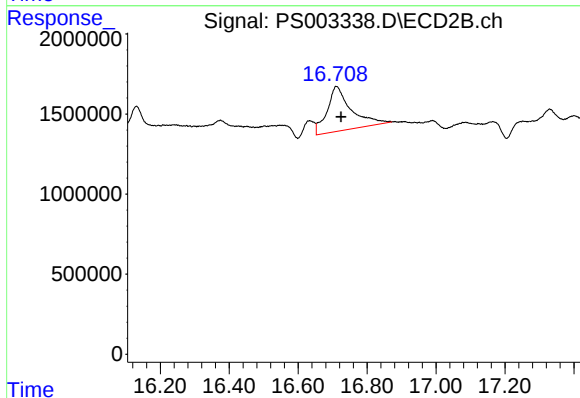


#15 Picloram

R.T.: 16.711 min
Delta R.T.: -0.013 min
Response: 13623201
Conc: 4.53 ng/ml

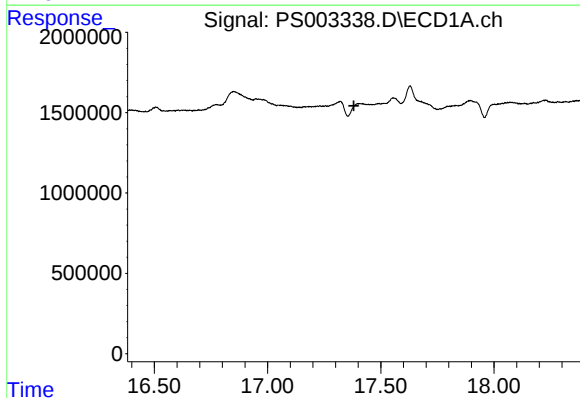

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

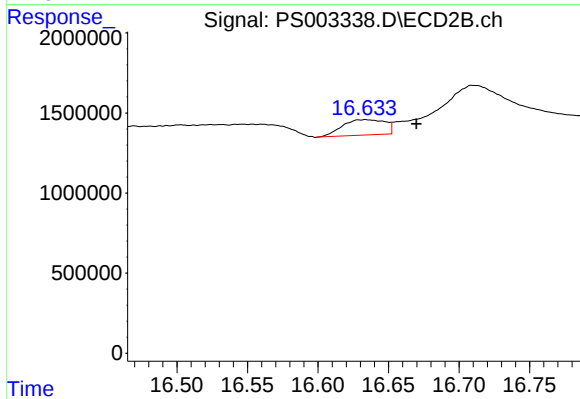

#16 DCPA

R.T.: 16.633 min
Delta R.T.: -0.037 min
Response: 2039009
Conc: 0.66 ng/ml