

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
 Data File : PS003339.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2019 11:00
 Operator : EI\SJ
 Sample : K1348-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OK-03-022219-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:50:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.297	10.795	171.9E6	185.8E6	452.781	434.498
Target Compounds							
1) T	Dalapon	0.000	2.296	0	8715415	N.D.	16.262 #
2) T	3,5-DICHL...	0.000	9.046	0	3840338	N.D.	6.814 #
3) T	4-Nitroph...	0.000	10.015	0	6206279	N.D.	29.692 #
7) T	MCPA	12.240	11.765	10788160	129.6E6	6.095	82.391 #
12) T	2,4,5-T	0.000	14.457	0	3427942	N.D.	1.791 #
15) T	Picloram	0.000	16.732	0	7957788	N.D.	2.647 #
16) T	DCPA	0.000	16.660	0	4421842	N.D.	1.428 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
Data File : PS003339.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2019 11:00
Operator : EI\SJ
Sample : K1348-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:50:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

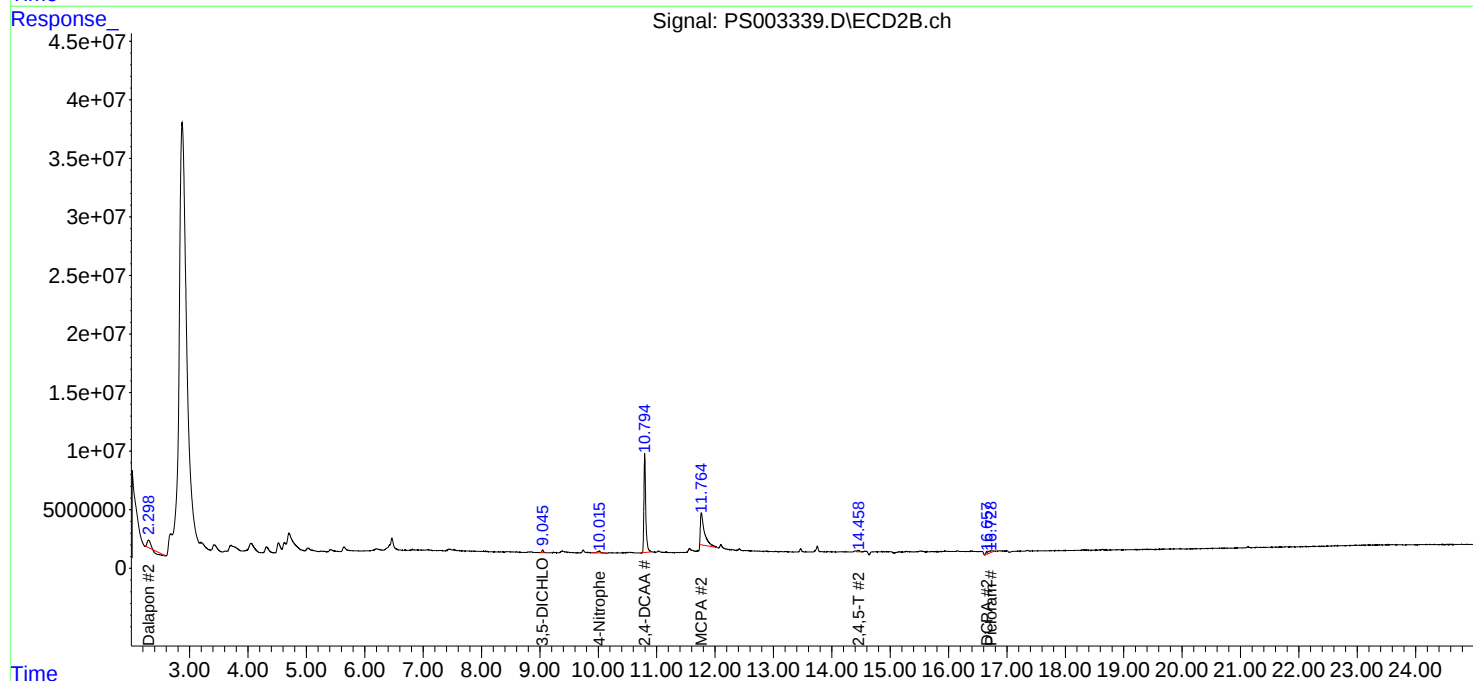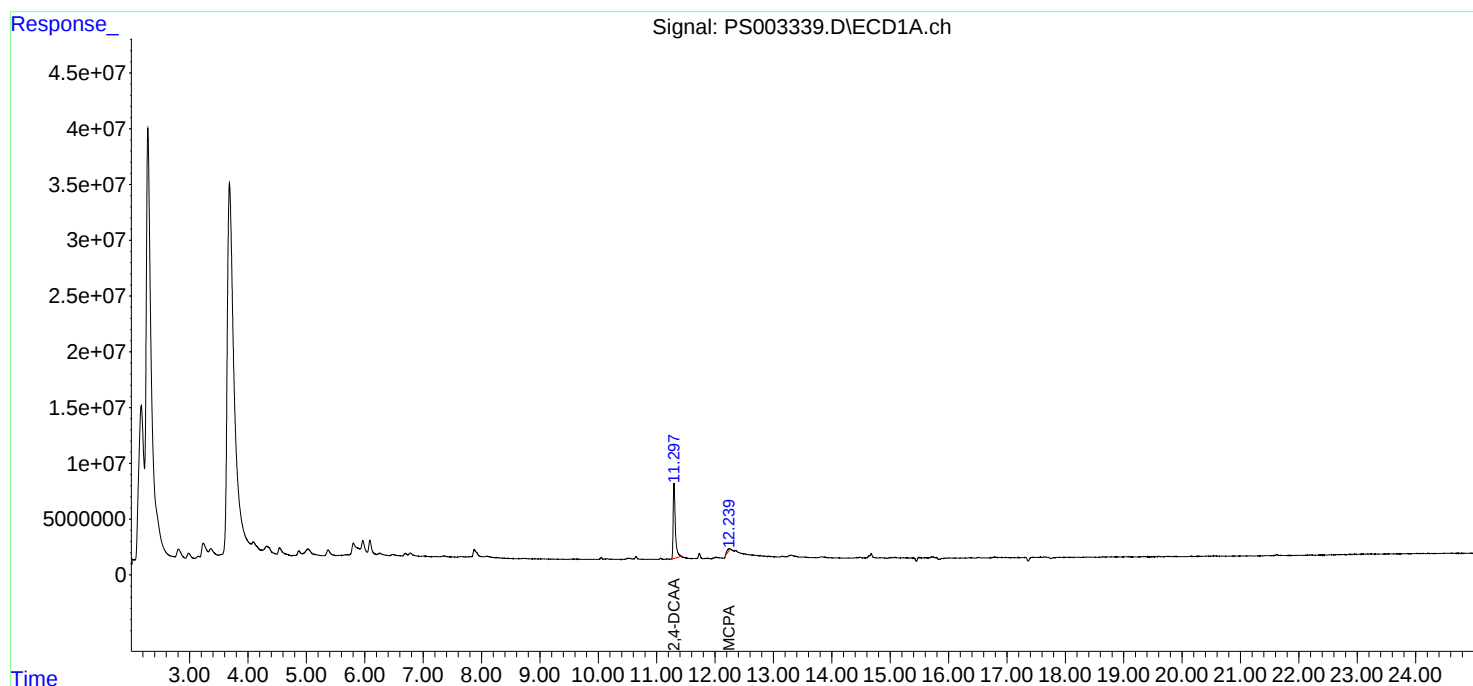


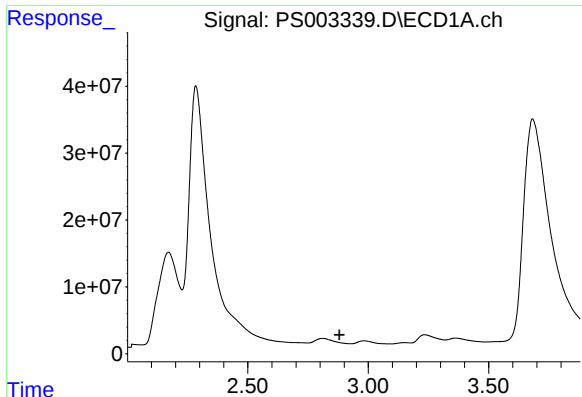

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-B

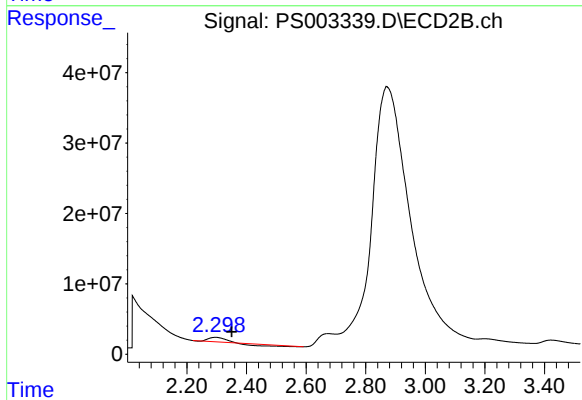


#1 Dalapon

R.T.: 2.296 min
Delta R.T.: -0.054 min
Response: 8715415
Conc: 16.26 ng/ml

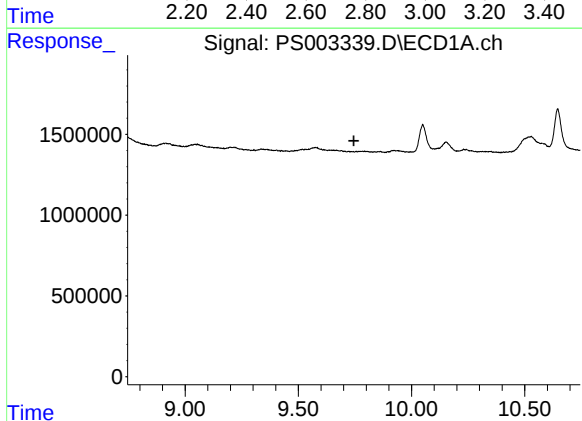


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

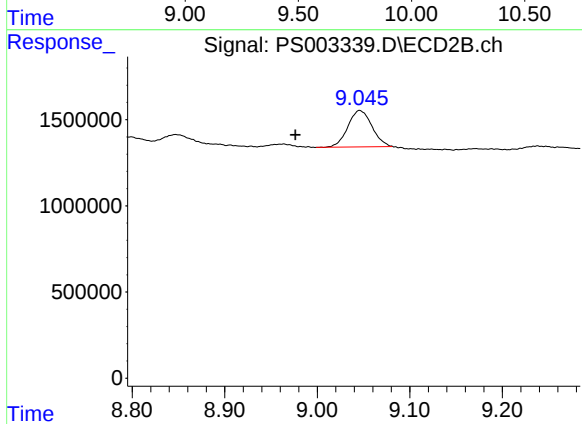

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.046 min
Delta R.T.: 0.070 min
Response: 3840338
Conc: 6.81 ng/ml

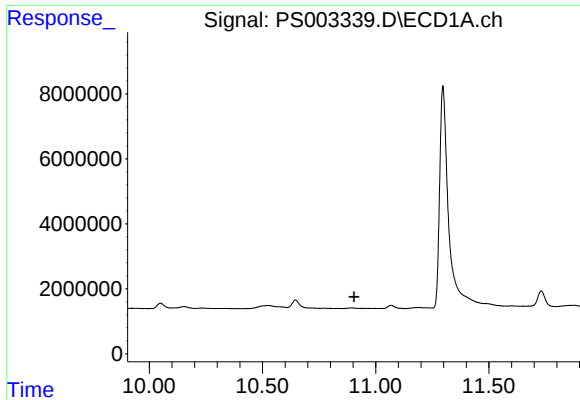

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-B

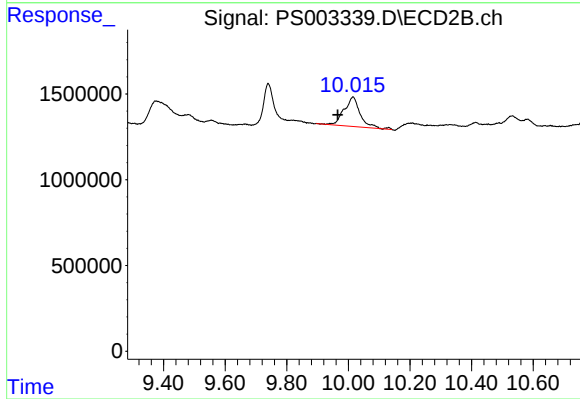


#3 4-Nitrophenol

R.T.: 10.015 min
Delta R.T.: 0.050 min
Response: 6206279
Conc: 29.69 ng/ml

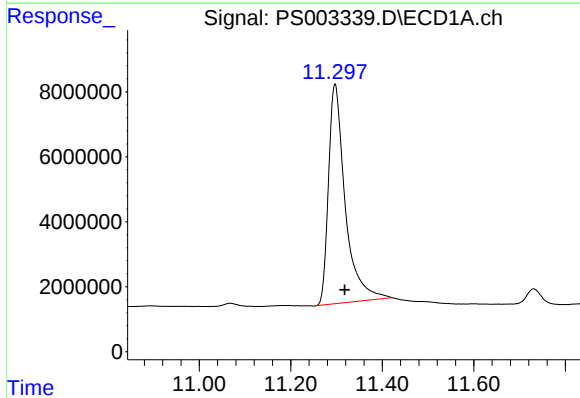


#4 2,4-DCAA

R.T.: 11.297 min
Delta R.T.: -0.021 min
Response: 171894181
Conc: 452.78 ng/ml

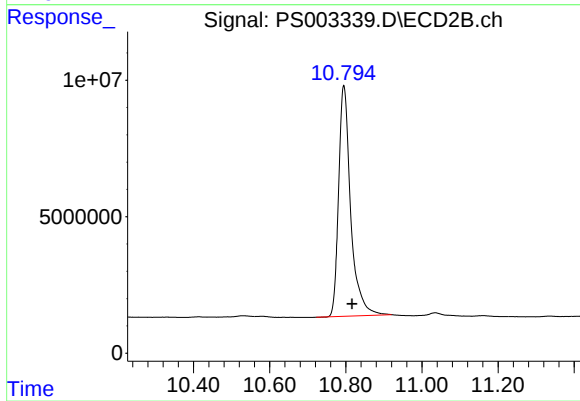

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: -0.022 min
Response: 185767937
Conc: 434.50 ng/ml

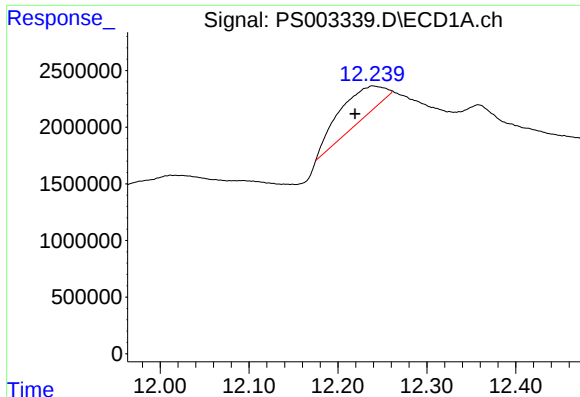

#7 MCPA


R.T.: 12.240 min
Delta R.T.: 0.021 min
Response: 10788160
Conc: 6.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-B

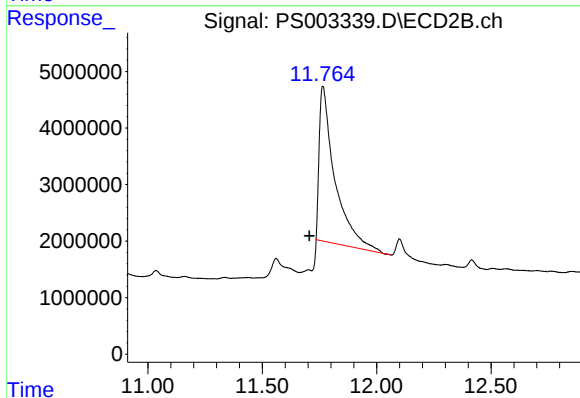


#7 MCPA

R.T.: 11.765 min
Delta R.T.: 0.059 min
Response: 129606348
Conc: 82.39 ug/ml

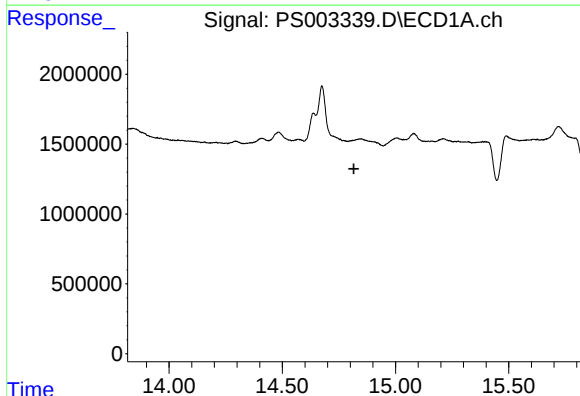


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

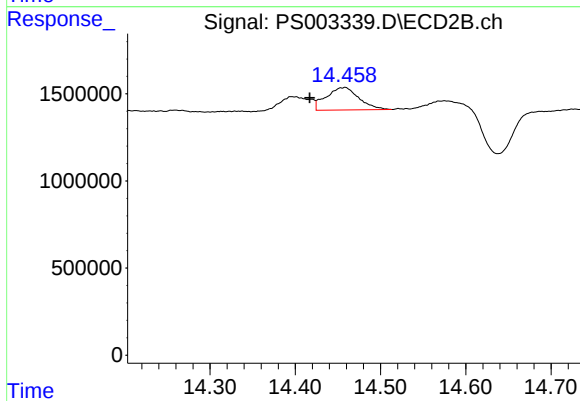

#12 2,4,5-T


R.T.: 14.457 min
Delta R.T.: 0.040 min
Response: 3427942
Conc: 1.79 ng/ml

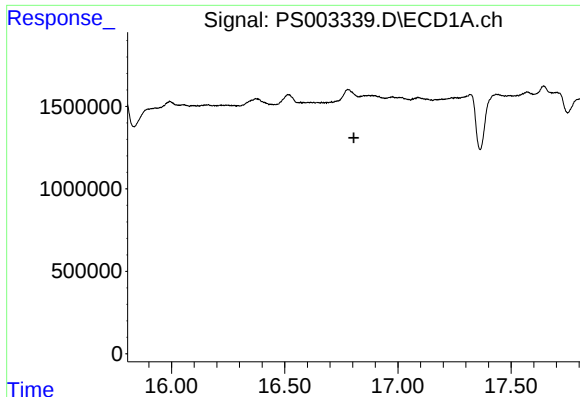

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OK-03-022219-B

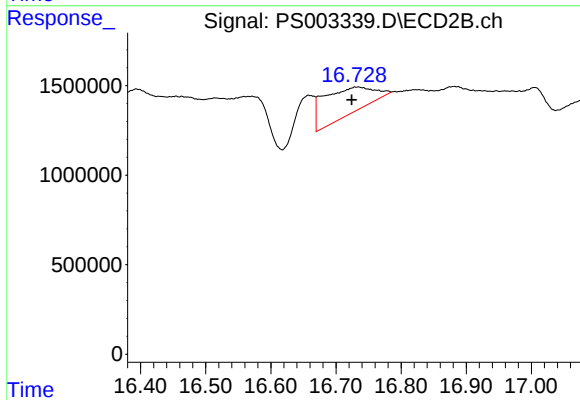


#15 Picloram

R.T.: 16.732 min
Delta R.T.: 0.008 min
Response: 7957788
Conc: 2.65 ng/ml

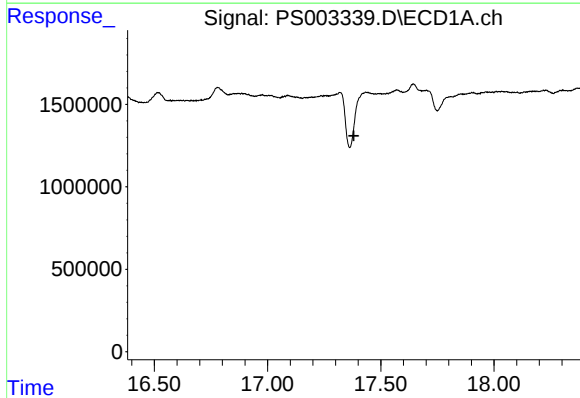

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

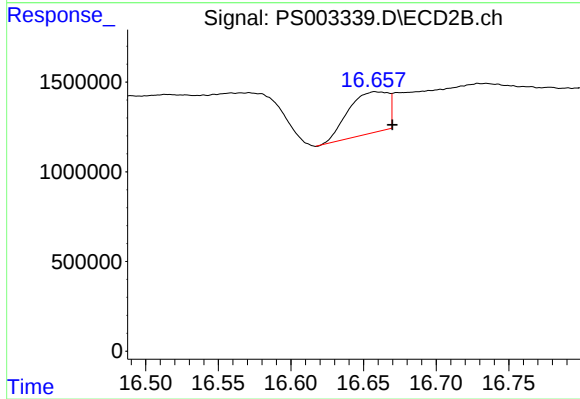

#16 DCPA

R.T.: 16.660 min
Delta R.T.: -0.010 min
Response: 4421842
Conc: 1.43 ng/ml