

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
 Data File : PS003341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2019 12:02
 Operator : EI\SJ
 Sample : K1356-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-02-022219-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:51:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.279	10.780	95082564	190.8E6	250.454	446.282 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.030	0	4758696	N.D.	8.444 #
3) T	4-Nitroph...	0.000	9.999	0	7466394	N.D.	35.721 #
6) T	MCP	11.983	0.000	1905401	0	1.590	N.D. #
12) T	2,4,5-T	0.000	14.439	0	3553186	N.D.	1.857 #
15) T	Picloram	16.763	0.000	3588635	0	1.134	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
Data File : PS003341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2019 12:02
Operator : EI\SJ
Sample : K1356-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-02-022219-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:51:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

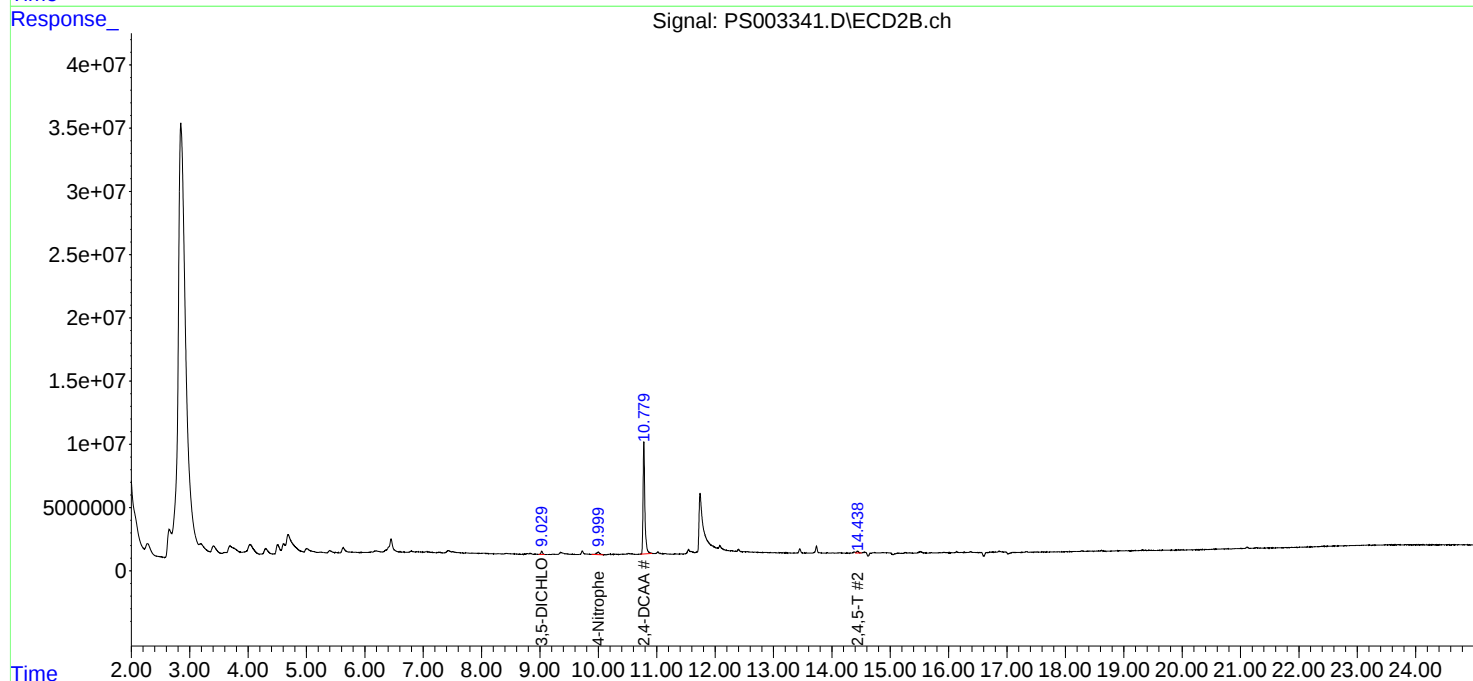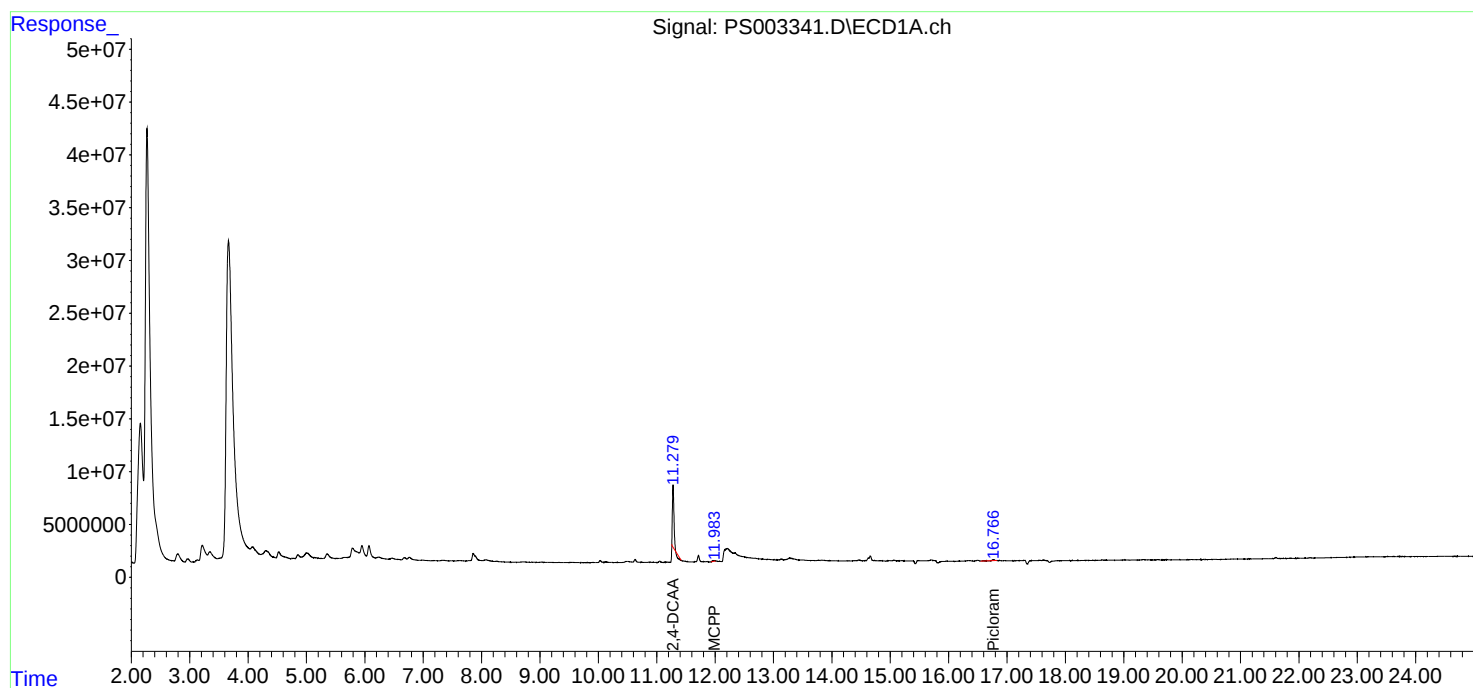


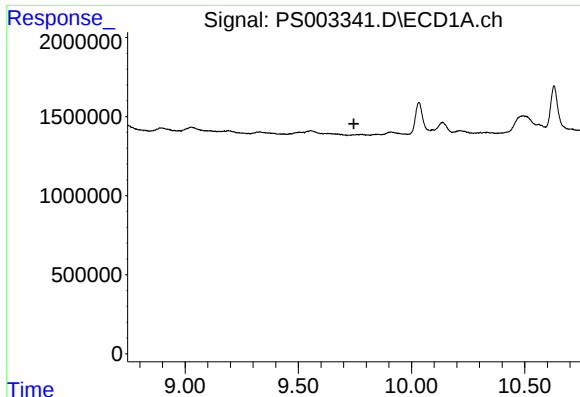

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-02-022219-B

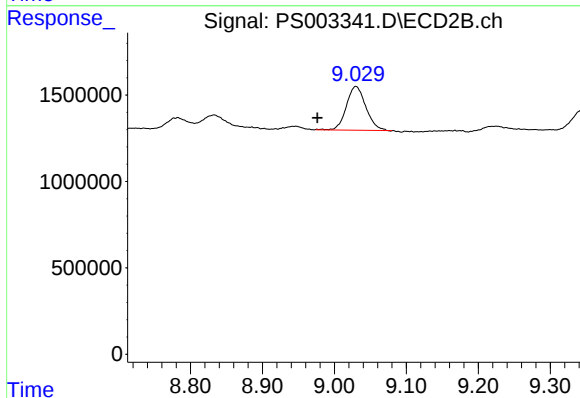


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.030 min
Delta R.T.: 0.054 min
Response: 4758696
Conc: 8.44 ng/ml

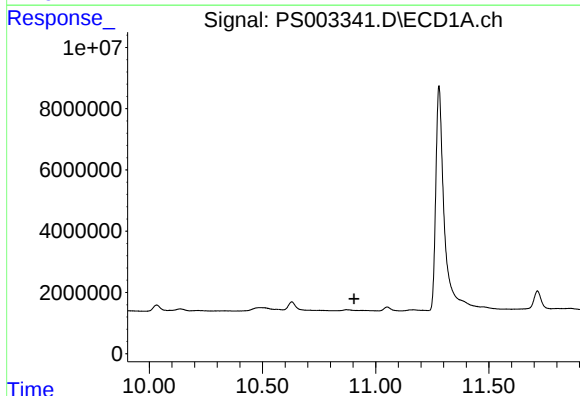


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

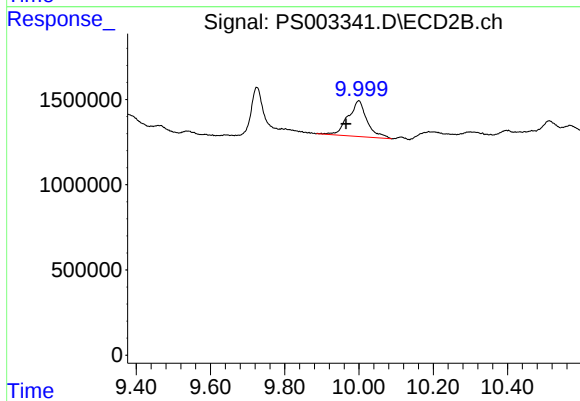

#3 4-Nitrophenol


R.T.: 9.999 min
Delta R.T.: 0.034 min
Response: 7466394
Conc: 35.72 ng/ml

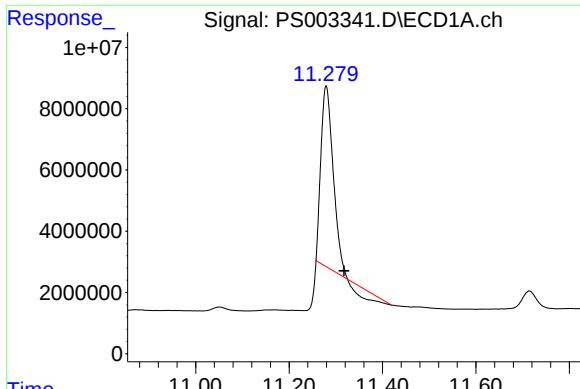

#4 2,4-DCAA


R.T.: 11.279 min
Delta R.T.: -0.038 min
Response: 95082564
Conc: 250.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-02-022219-B

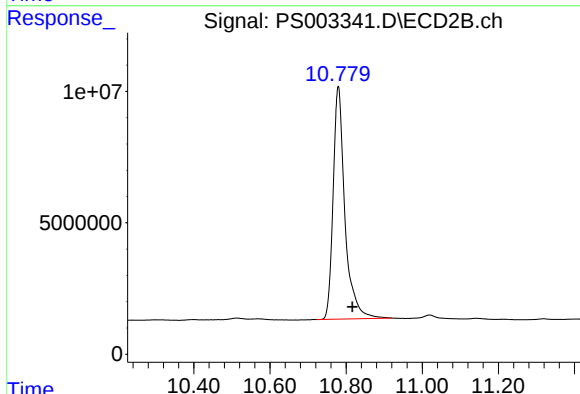


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 190805763
Conc: 446.28 ng/ml

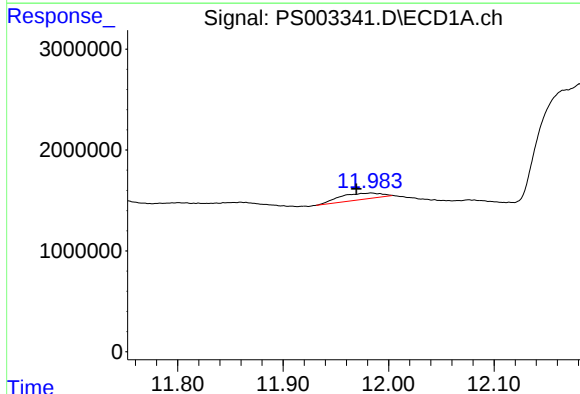


#6 MCP

R.T.: 11.983 min
Delta R.T.: 0.014 min
Response: 1905401
Conc: 1.59 ug/ml

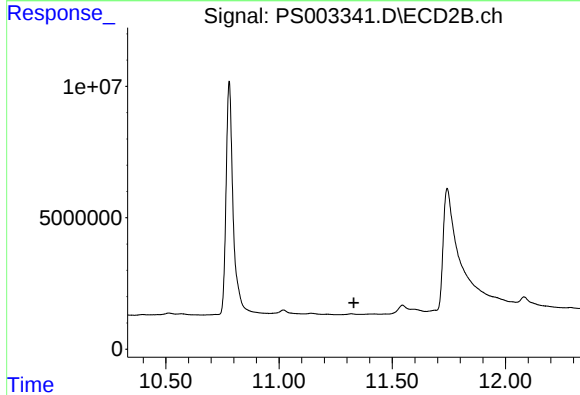

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

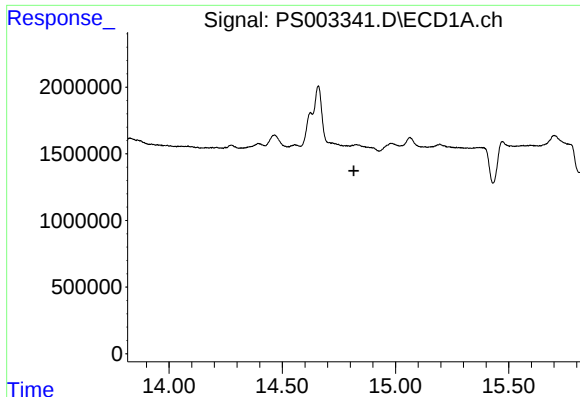

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-02-022219-B

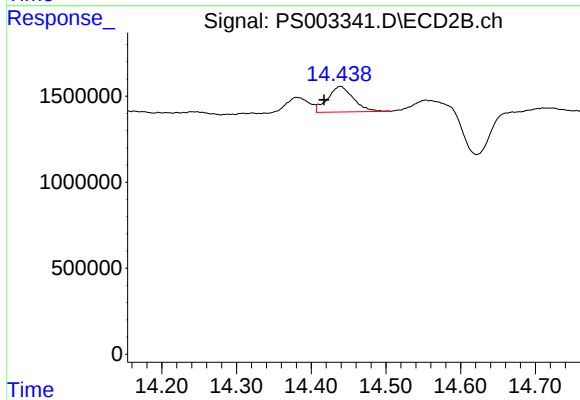


#12 2,4,5-T

R.T.: 14.439 min
Delta R.T.: 0.022 min
Response: 3553186
Conc: 1.86 ng/ml

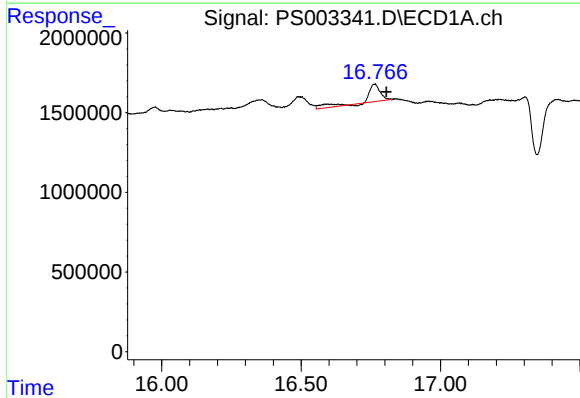

#15 Picloram

R.T.: 16.763 min
Delta R.T.: -0.043 min
Response: 3588635
Conc: 1.13 ng/ml

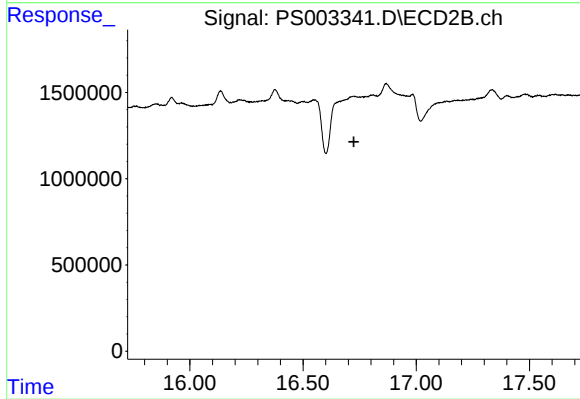

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.724 min
Response: 0
Conc: N.D.