

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
 Data File : PS003350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2019 16:41
 Operator : EI\SJ
 Sample : K1596-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:53:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.777	41639898	181.1E6	109.682	423.506 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.028	0	4486628	N.D.	7.961 #
3) T	4-Nitroph...	0.000	9.997	0	7130735	N.D.	34.115 #
6) T	MCP	11.984	0.000	1529366	0	1.276	N.D. #
7) T	MCPA	12.220	0.000	4103772	0	2.319	N.D. #
12) T	2,4,5-T	0.000	14.439	0	3637242	N.D.	1.901 #
14) T	DINOSEB	0.000	15.498	0	5721368	N.D.	3.264 #
15) T	Picloram	16.757	16.741	1949300	16511704	0.616	5.492 #
16) T	DCPA	17.413	0.000	2097379	0	0.697	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
Data File : PS003350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2019 16:41
Operator : EI\SJ
Sample : K1596-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:53:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

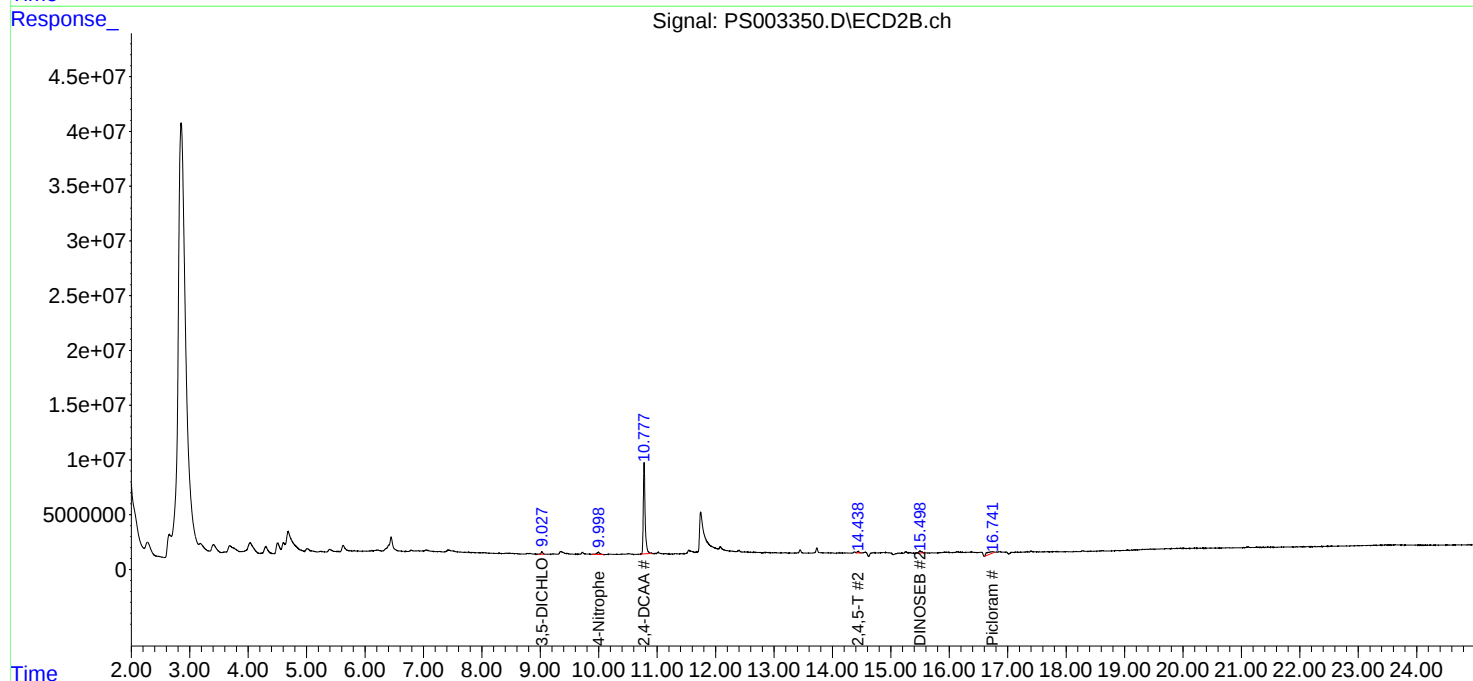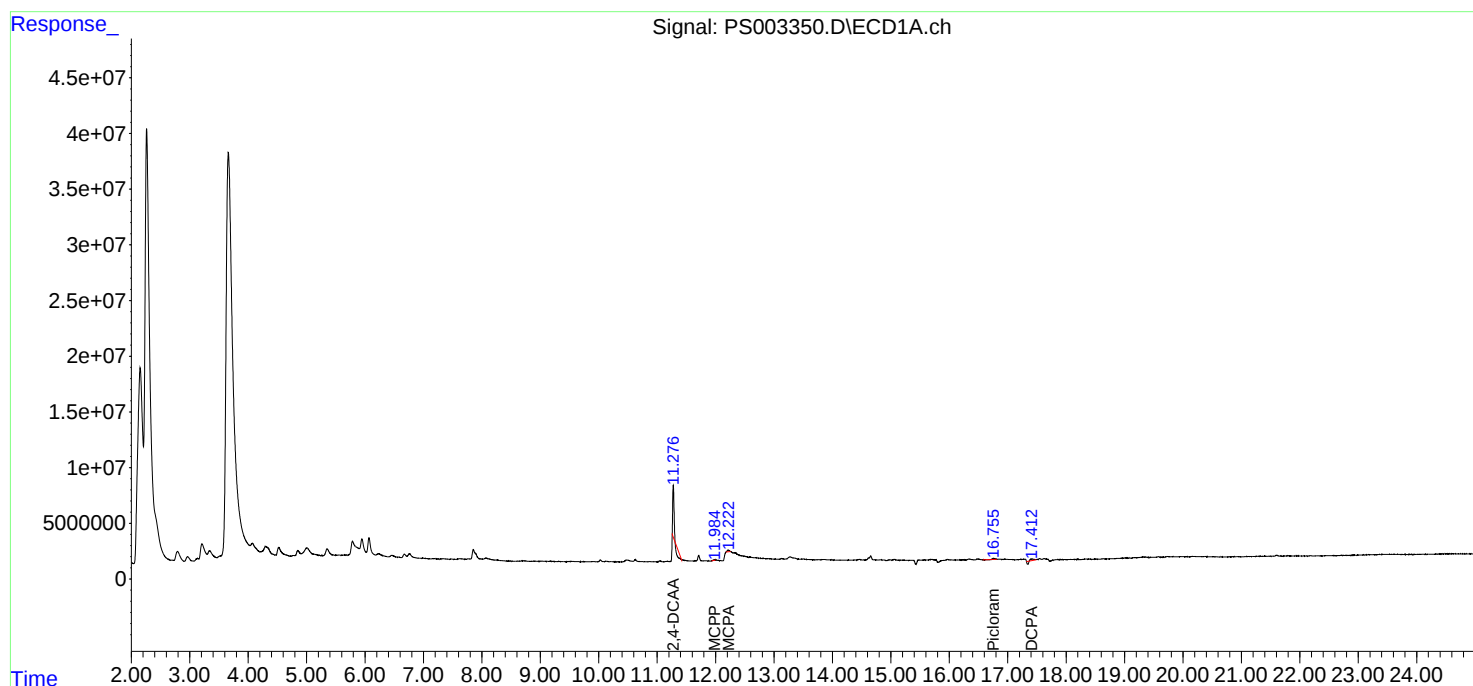


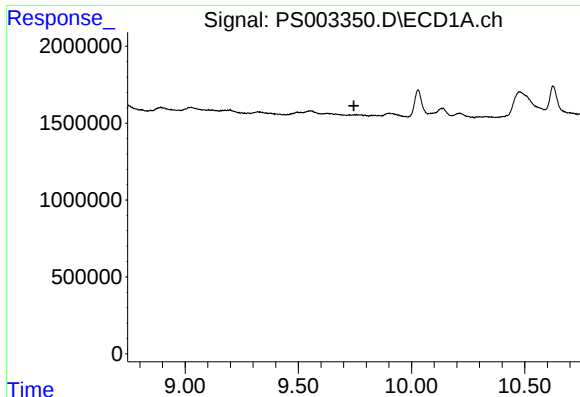

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.745 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-13

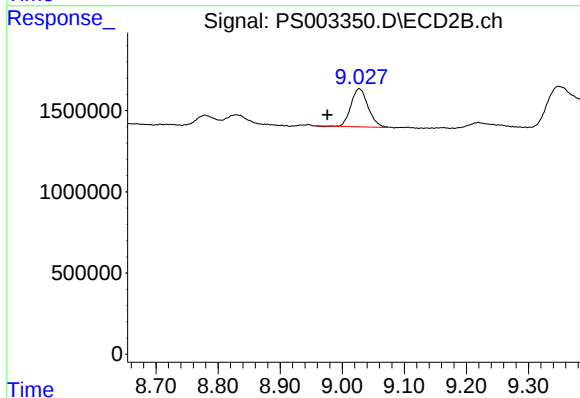


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.028 min
Delta R.T.: 0.051 min
Response: 4486628
Conc: 7.96 ng/ml

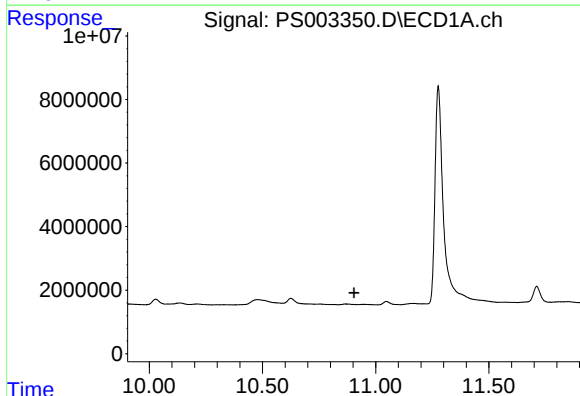


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

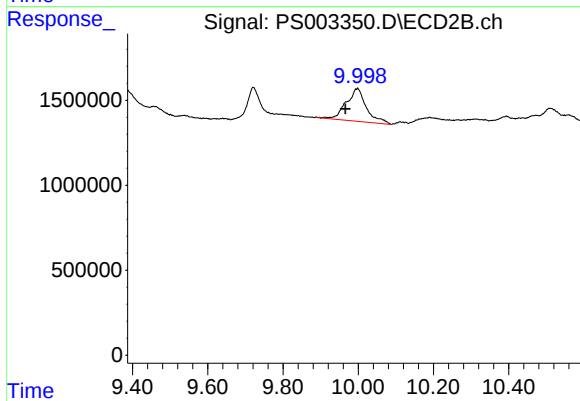

#3 4-Nitrophenol


R.T.: 9.997 min
Delta R.T.: 0.032 min
Response: 7130735
Conc: 34.11 ng/ml

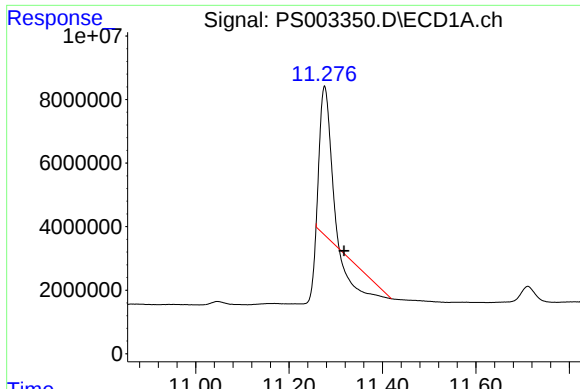

#4 2,4-DCAA


R.T.: 11.276 min
Delta R.T.: -0.042 min
Response: 41639898
Conc: 109.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-13

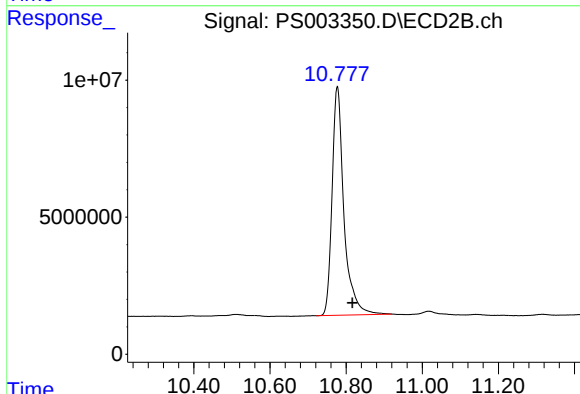


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.040 min
Response: 181068272
Conc: 423.51 ng/ml

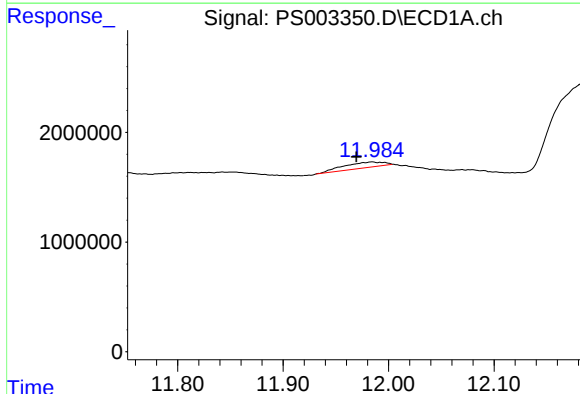


#6 MCP

R.T.: 11.984 min
Delta R.T.: 0.015 min
Response: 1529366
Conc: 1.28 ug/ml

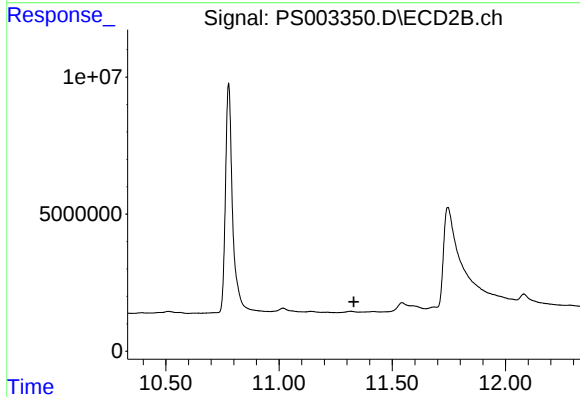

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.330 min
Response: 0
Conc: N.D.

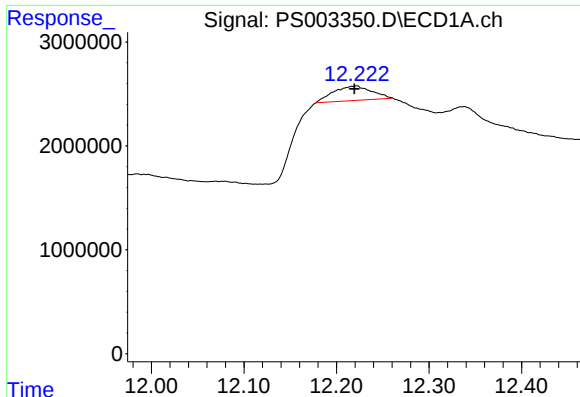

#7 MCPA


R.T.: 12.220 min
Delta R.T.: 0.000 min
Response: 4103772
Conc: 2.32 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-13

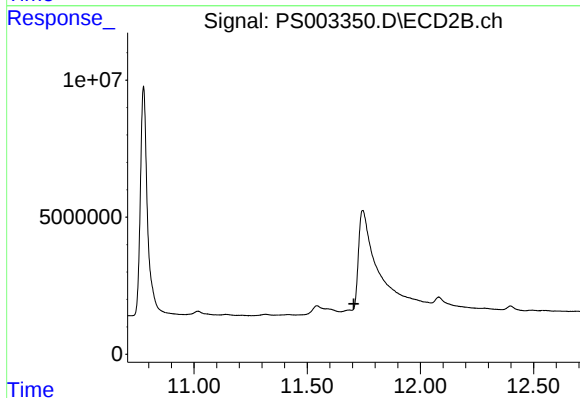


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

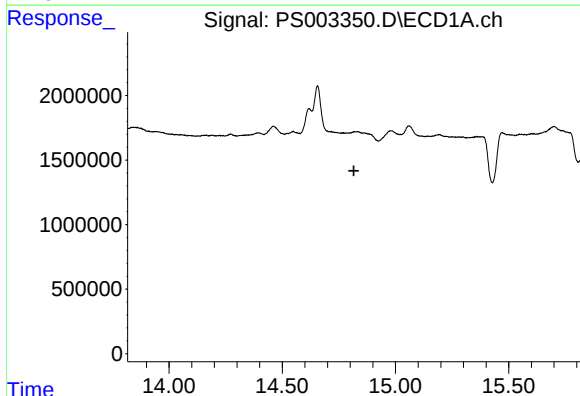


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

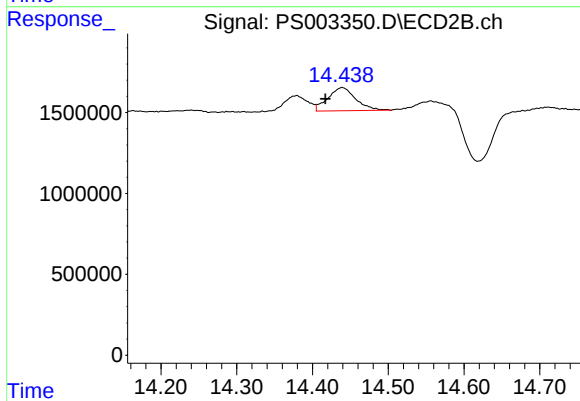

#12 2,4,5-T


R.T.: 14.439 min
Delta R.T.: 0.022 min
Response: 3637242
Conc: 1.90 ng/ml

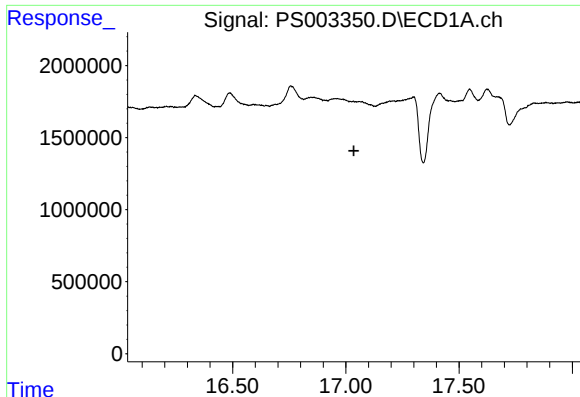

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-13

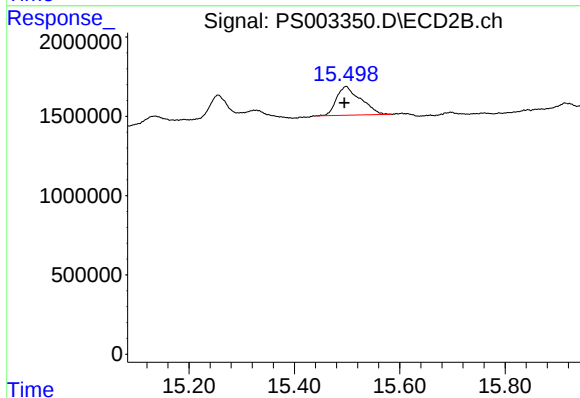


#14 DINOSEB

R.T.: 15.498 min
Delta R.T.: 0.003 min
Response: 5721368
Conc: 3.26 ng/ml

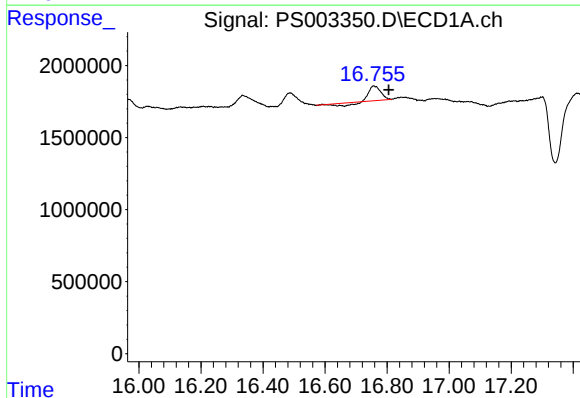


#15 Picloram

R.T.: 16.757 min
Delta R.T.: -0.049 min
Response: 1949300
Conc: 0.62 ng/ml

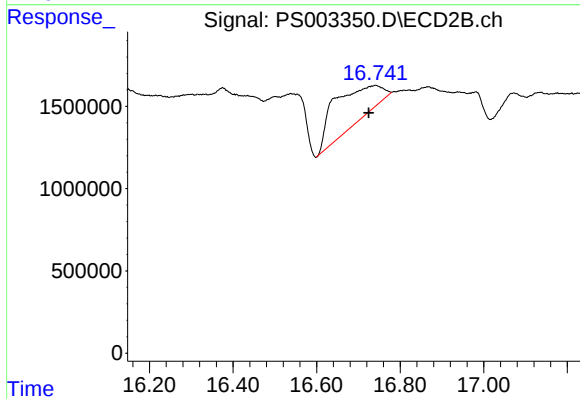

#15 Picloram


R.T.: 16.741 min
Delta R.T.: 0.017 min
Response: 16511704
Conc: 5.49 ng/ml

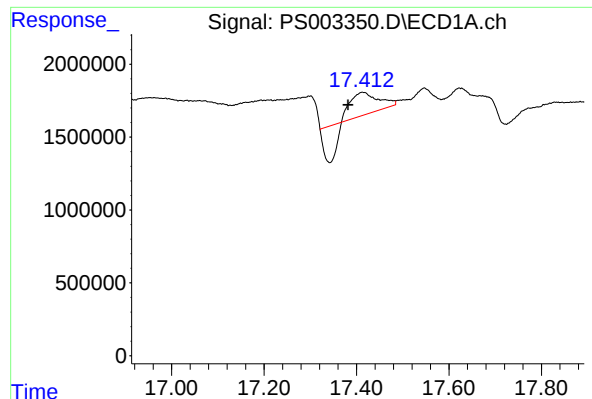

#16 DCPA

R.T.: 17.413 min
Delta R.T.: 0.032 min
Response: 2097379
Conc: 0.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-13

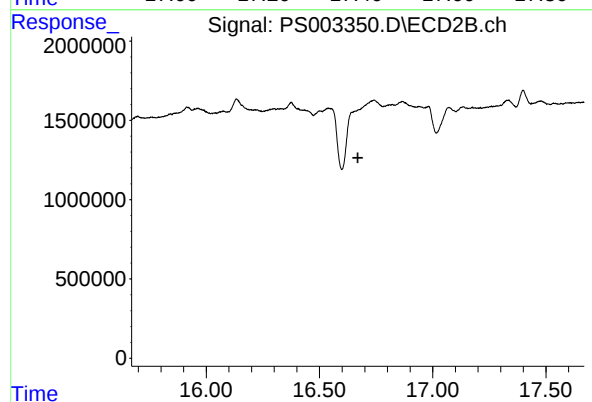

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.670 min
Response: 0
Conc: N.D.