

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
 Data File : PS003351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2019 17:13
 Operator : EI\SJ
 Sample : K1596-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:53:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.797	190.6E6	203.9E6	502.139	476.960
Target Compounds							
1) T	Dalapon	0.000	2.297	0	6893648	N.D.	12.863 #
3) T	4-Nitroph...	0.000	10.018	0	7622420	N.D.	36.467 #
7) T	MCPA	12.242	11.767	9290772	154.8E6	5.249	98.431 #
11) T	2,4,5-TP ...	14.481	0.000	3790302	0	1.505	N.D. #
12) T	2,4,5-T	0.000	14.399	0	1995882	N.D.	1.043 #
14) T	DINOSEB	0.000	15.516	0	5810860	N.D.	3.315 #
15) T	Picloram	16.777	16.764	2993164	16532902	0.946	5.499 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
Data File : PS003351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2019 17:13
Operator : EI\SJ
Sample : K1596-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
COMP-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:53:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

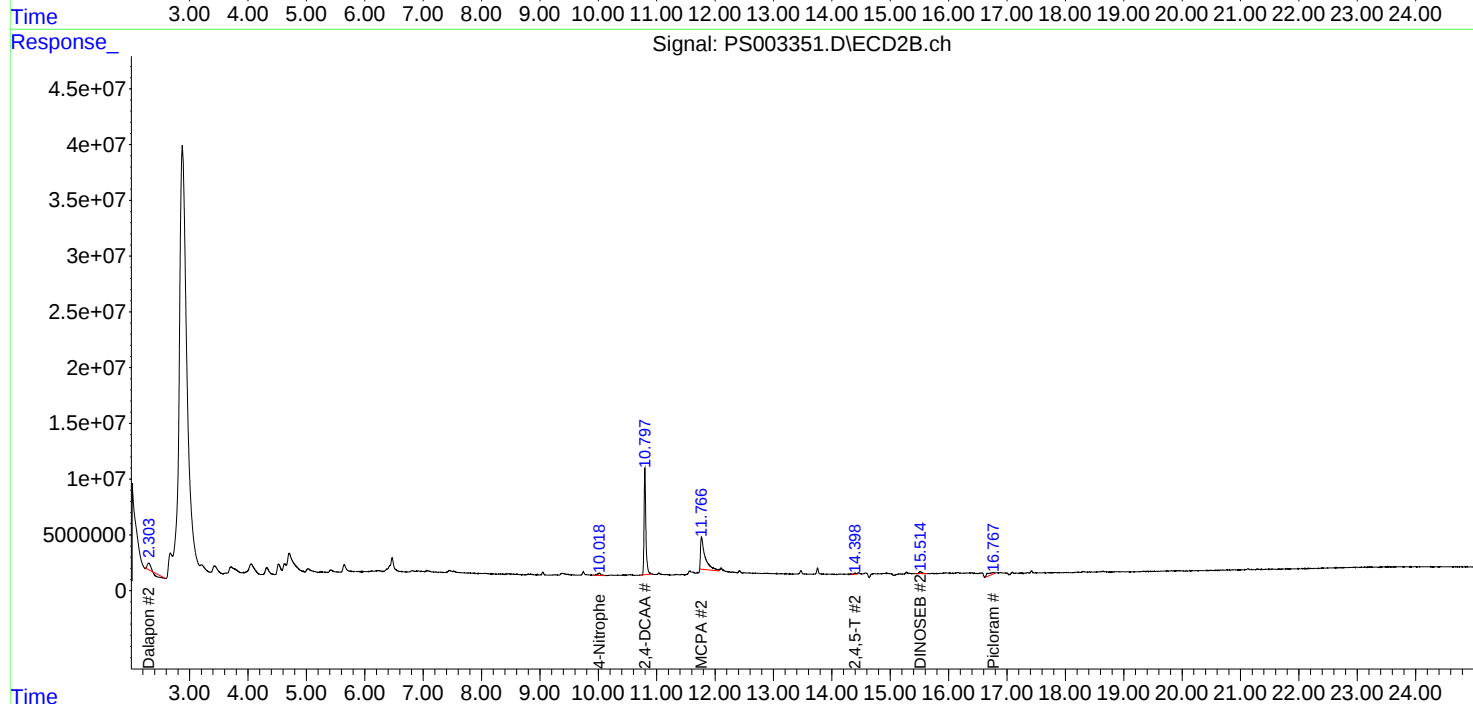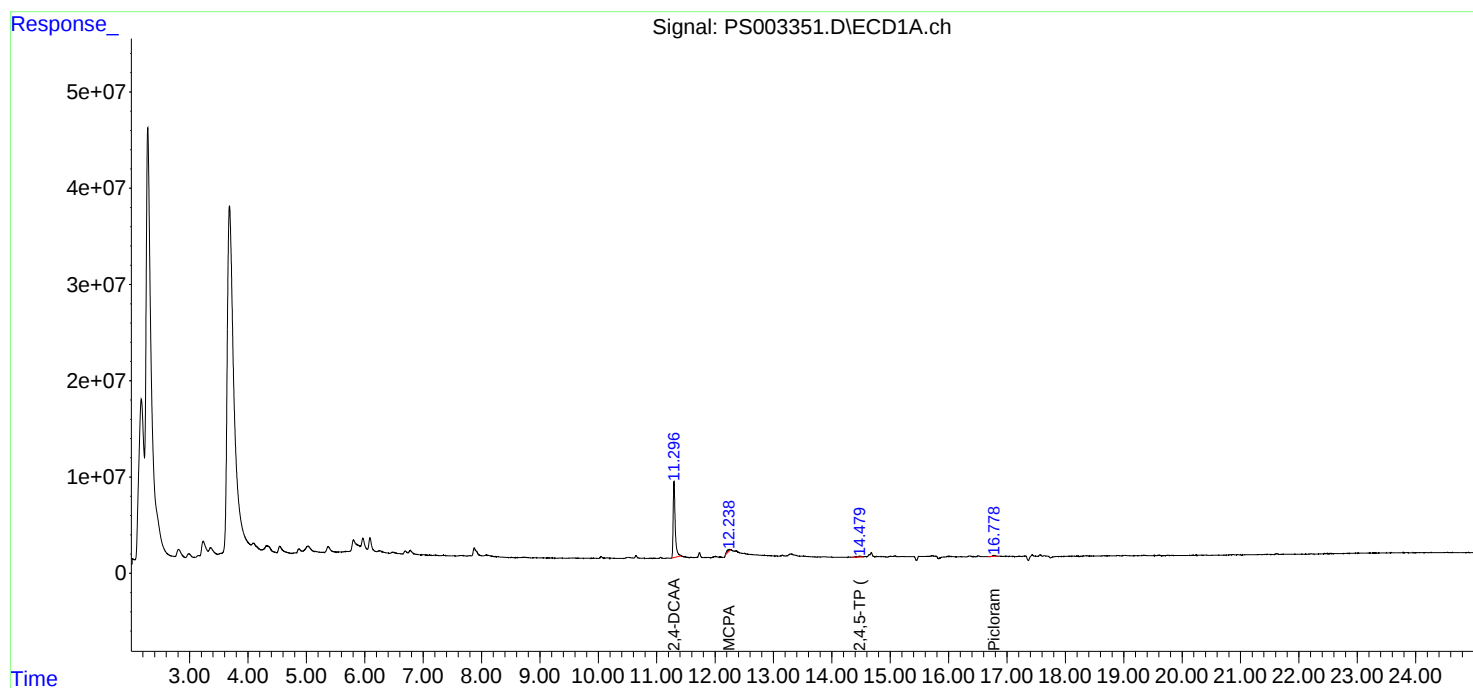


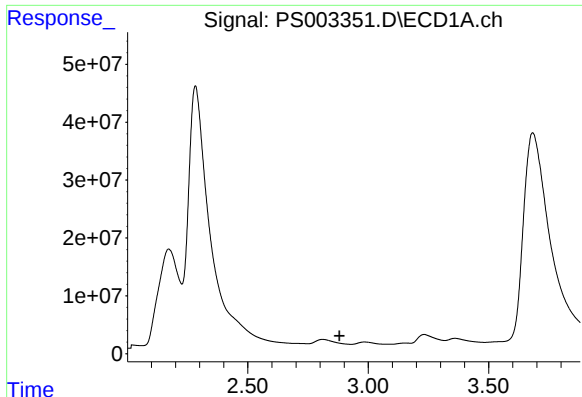

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.880 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-14

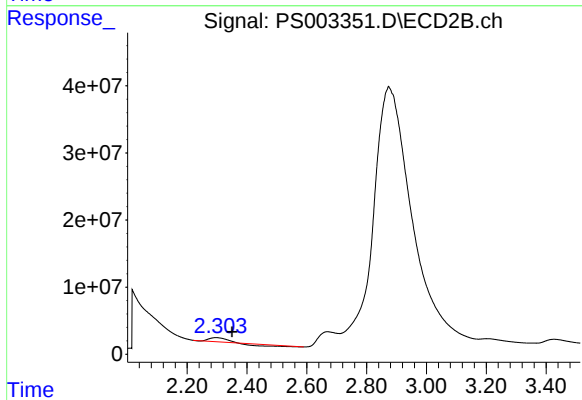


#1 Dalapon

R.T.: 2.297 min
Delta R.T.: -0.054 min
Response: 6893648
Conc: 12.86 ng/ml

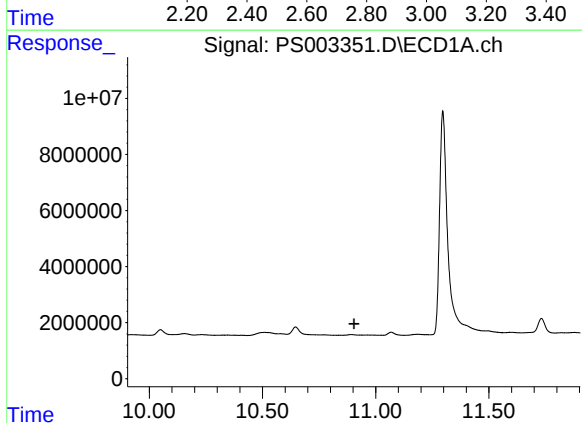


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

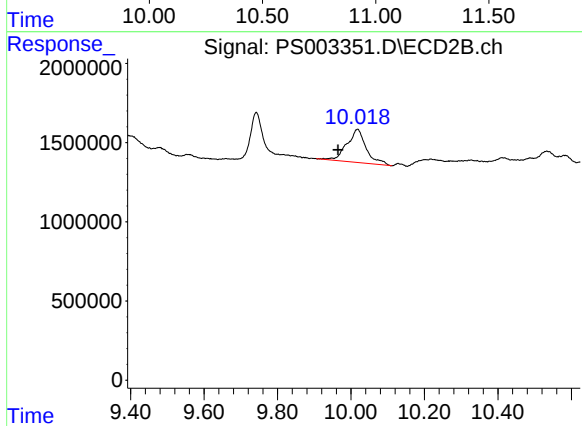

#3 4-Nitrophenol


R.T.: 10.018 min
Delta R.T.: 0.052 min
Response: 7622420
Conc: 36.47 ng/ml

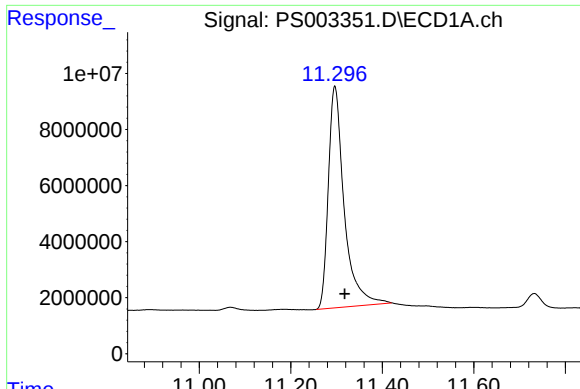

#4 2,4-DCAA


R.T.: 11.296 min
Delta R.T.: -0.021 min
Response: 190632447
Conc: 502.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-14

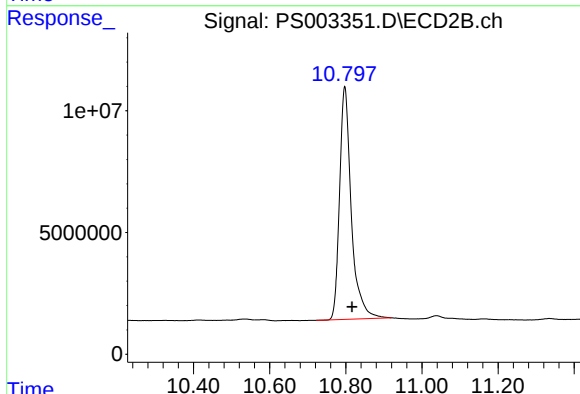


#4 2,4-DCAA

R.T.: 10.797 min
Delta R.T.: -0.019 min
Response: 203922268
Conc: 476.96 ng/ml

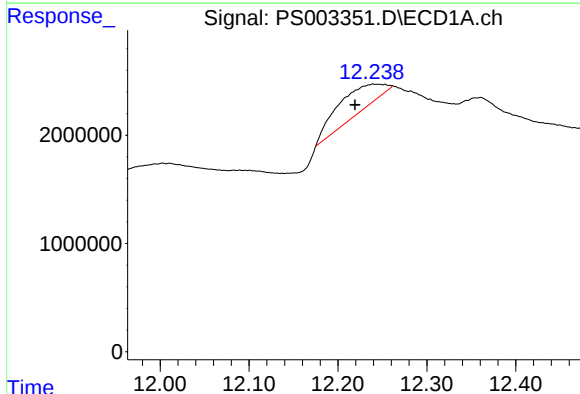


#7 MCPA

R.T.: 12.242 min
Delta R.T.: 0.023 min
Response: 9290772
Conc: 5.25 ug/ml

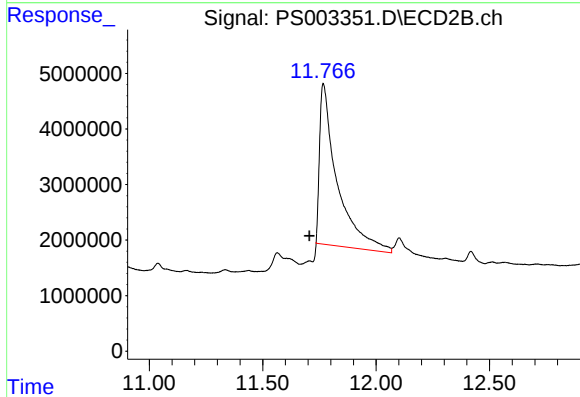

#7 MCPA


R.T.: 11.767 min
Delta R.T.: 0.061 min
Response: 154838322
Conc: 98.43 ug/ml

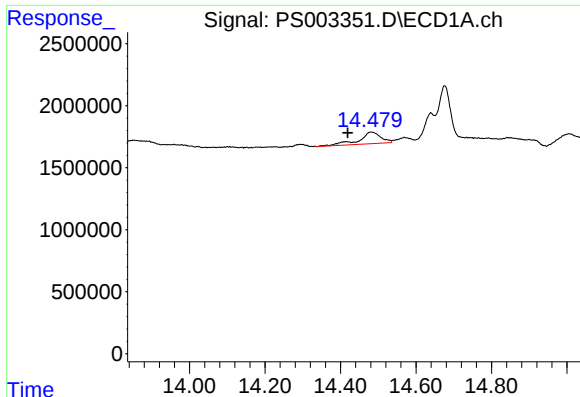

#11 2,4,5-TP (SILVEX)


R.T.: 14.481 min
Delta R.T.: 0.061 min
Response: 3790302
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-14

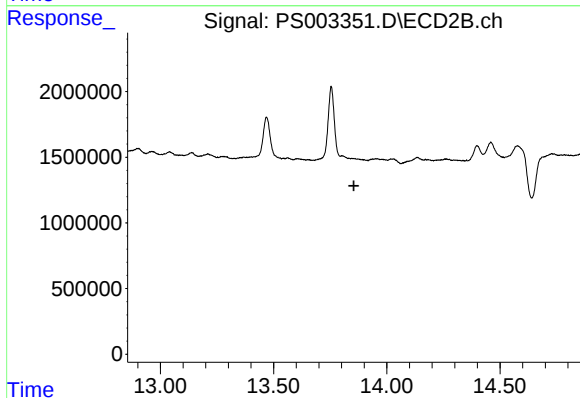


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 13.854 min
Response: 0
Conc: N.D.

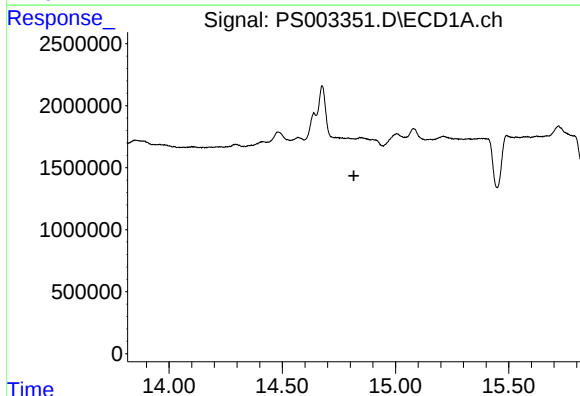


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.817 min
Response: 0
Conc: N.D.

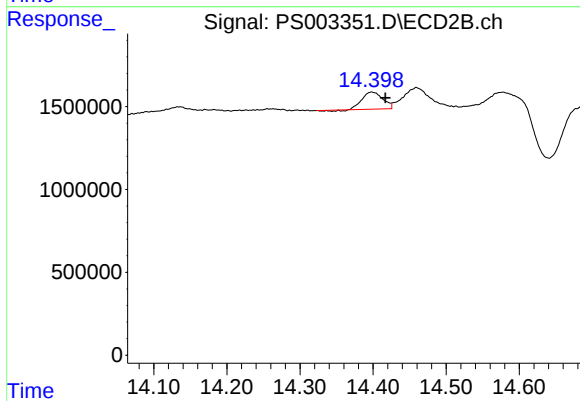

#12 2,4,5-T


R.T.: 14.399 min
Delta R.T.: -0.018 min
Response: 1995882
Conc: 1.04 ng/ml

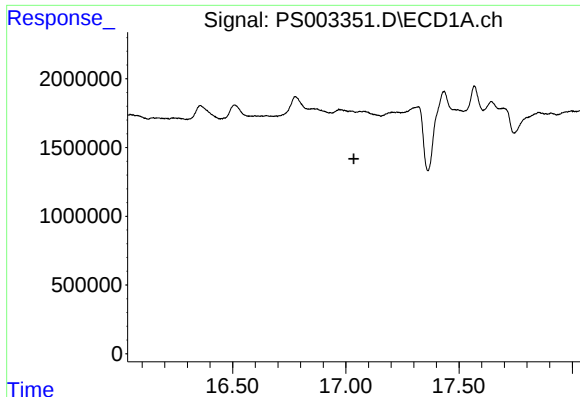

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-14

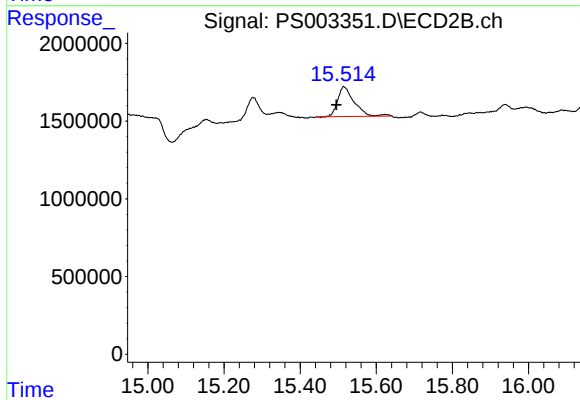


#14 DINOSEB

R.T.: 15.516 min
Delta R.T.: 0.021 min
Response: 5810860
Conc: 3.31 ng/ml

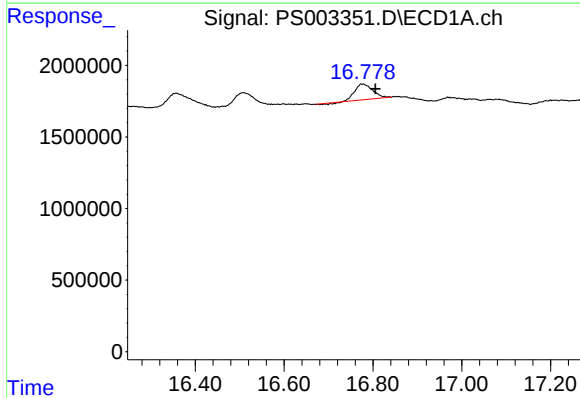

#15 Picloram

R.T.: 16.777 min
Delta R.T.: -0.029 min
Response: 2993164
Conc: 0.95 ng/ml

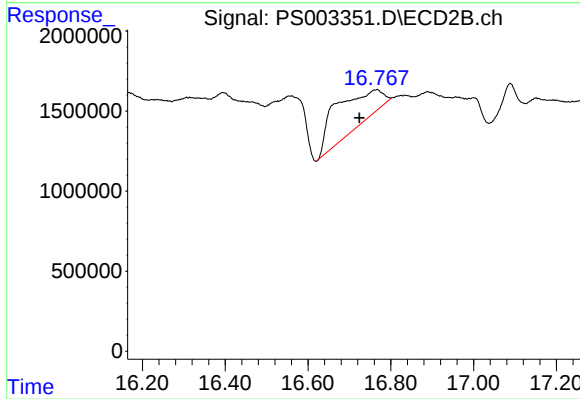

#15 Picloram

R.T.: 16.764 min
Delta R.T.: 0.040 min
Response: 16532902
Conc: 5.50 ng/ml