

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
 Data File : PS003358.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2019 20:50
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 27 02:55:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
 Quant Title : 8080.M
 QLast Update : Tue Jan 29 06:11:45 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.780	0	321.8E6	N.D.	752.729 #
Target Compounds							
1) T	Dalapon	2.841	2.313	98683160	373.7E6	178.888	697.215 #
2) T	3,5-DICHL...	0.000	8.940	0	152.3E6	N.D.	270.224 #
3) T	4-Nitroph...	0.000	9.932	0	147.2E6	N.D.	704.394 #
5) T	DICAMBA	0.000	11.059	0	263.9E6	N.D.	166.304 #
8) T	DICHLORPROP	0.000	12.184	0	276.9E6	N.D.	724.272 #
9) T	2,4-D	0.000	12.658	0	284.2E6	N.D.	566.890 #
11) T	2,4,5-TP ...	14.376	13.816	1898.1E6	1801.4E6	753.691	726.279
12) T	2,4,5-T	14.778	14.381	1812.8E6	924.3E6	743.127	483.041 #
14) T	DINOSEB	16.987	15.455	1457.5E6	-812885959	774.713	N.D. #
15) T	Picloram	16.769	16.689	1900.0E6	1761.6E6	600.577	585.950
16) T	DCPA	0.000	16.689	0	1761.6E6	N.D.	568.701 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022619\
Data File : PS003358.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2019 20:50
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 27 02:55:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS012819.M
Quant Title : 8080.M
QLast Update : Tue Jan 29 06:11:45 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

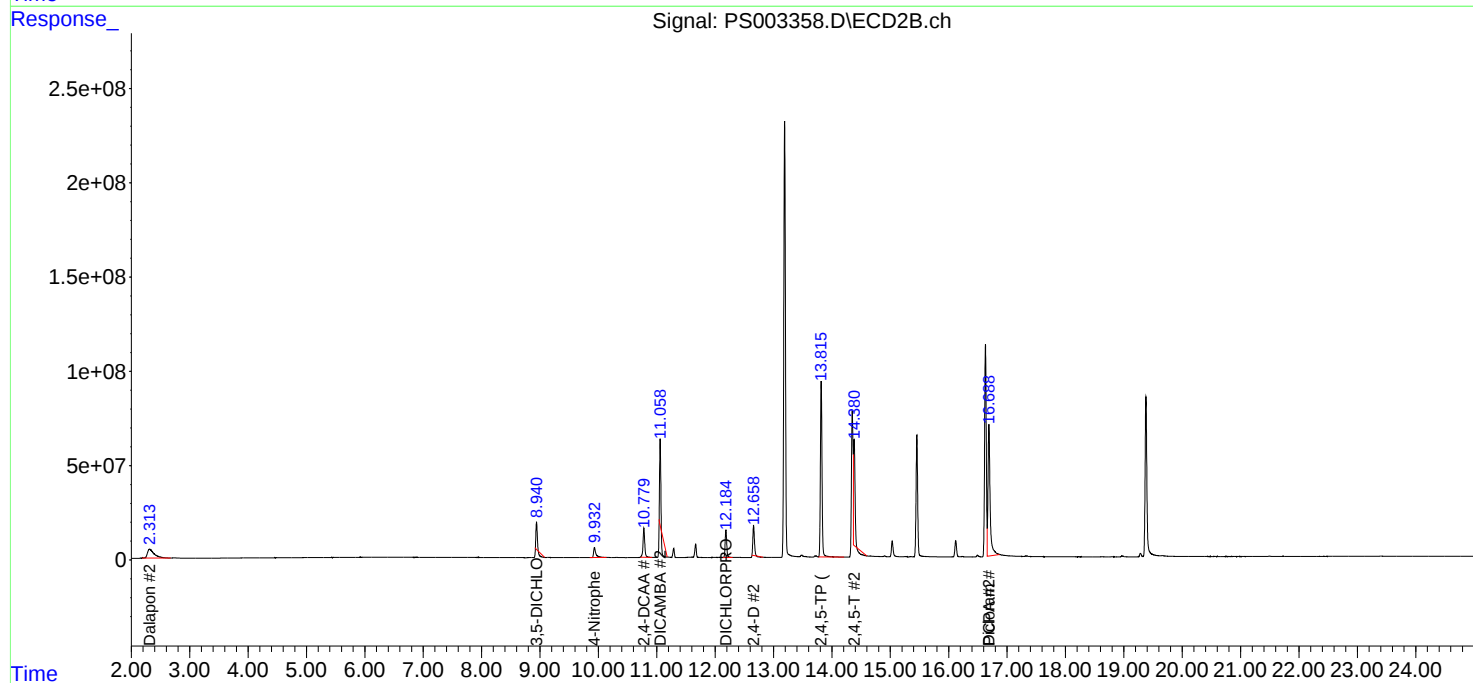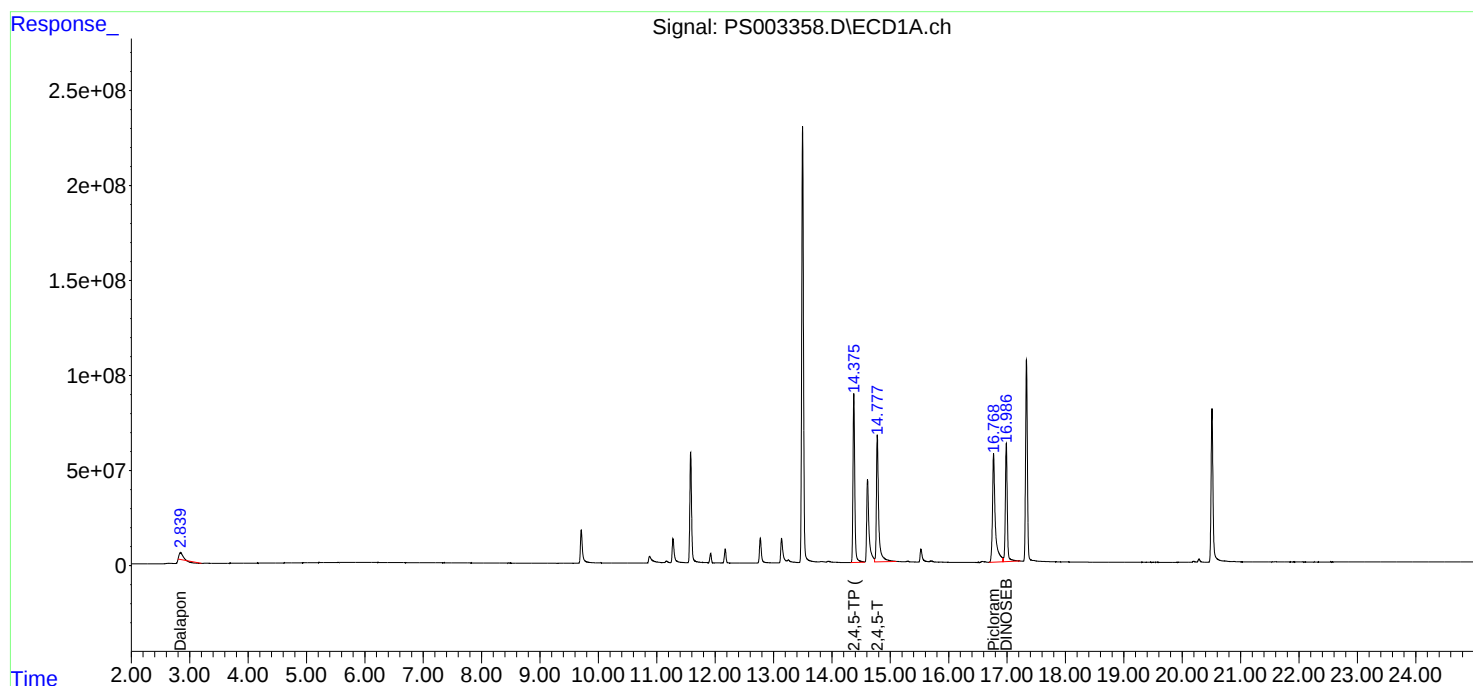


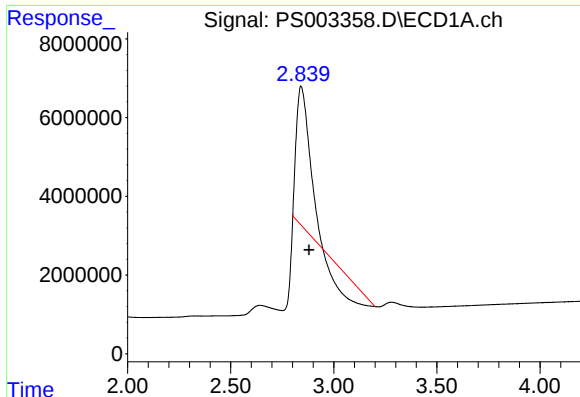

#1 Dalapon


R.T.: 2.841 min
Delta R.T.: -0.039 min
Response: 98683160
Conc: 178.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

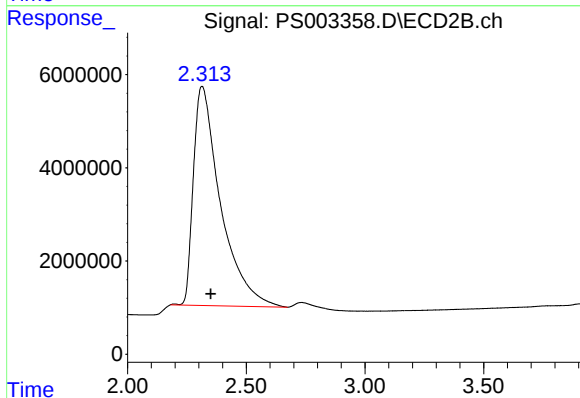


#1 Dalapon

R.T.: 2.313 min
Delta R.T.: -0.037 min
Response: 373652447
Conc: 697.22 ng/ml

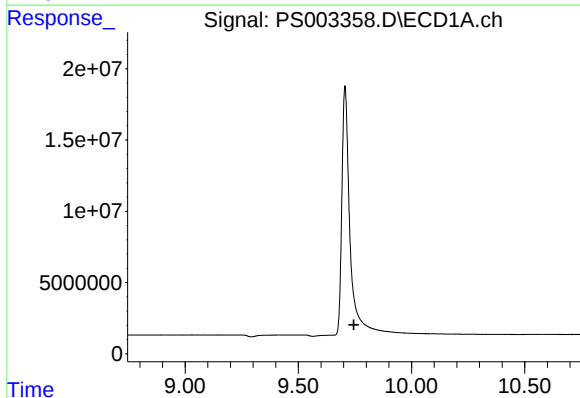


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.745 min
Response: 0
Conc: N.D.

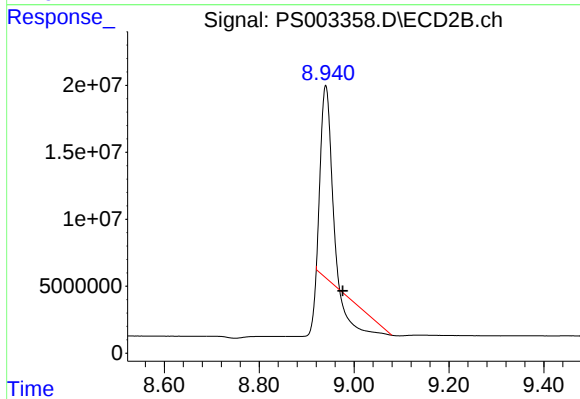

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.940 min
Delta R.T.: -0.036 min
Response: 152289509
Conc: 270.22 ng/ml

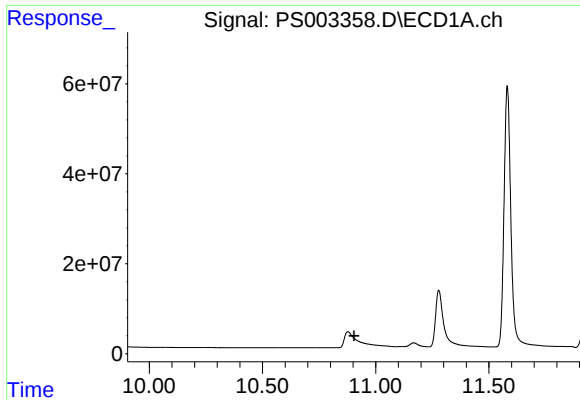

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

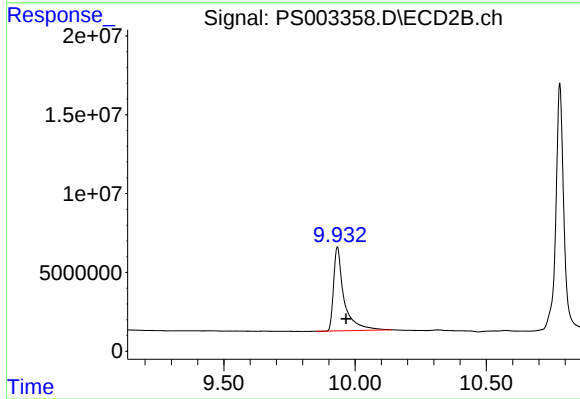


#3 4-Nitrophenol

R.T.: 9.932 min
Delta R.T.: -0.033 min
Response: 147234153
Conc: 704.39 ng/ml

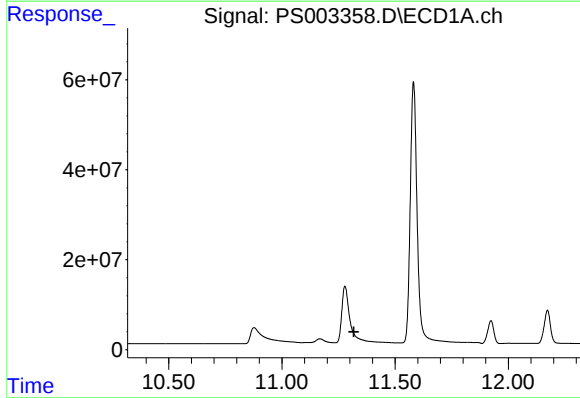


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.318 min
Response: 0
Conc: N.D.

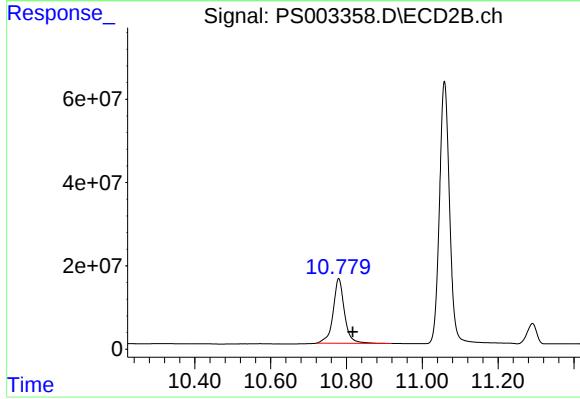

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: -0.037 min
Response: 321826278
Conc: 752.73 ng/ml

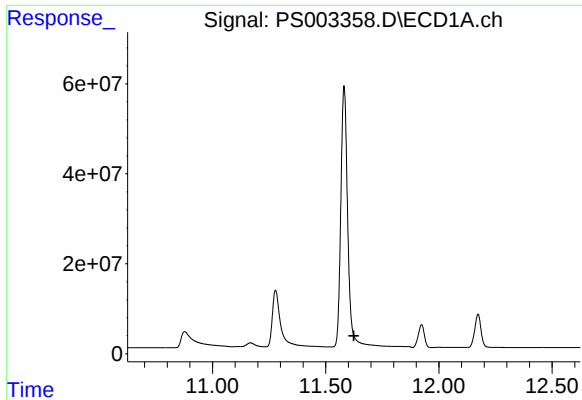

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.624 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

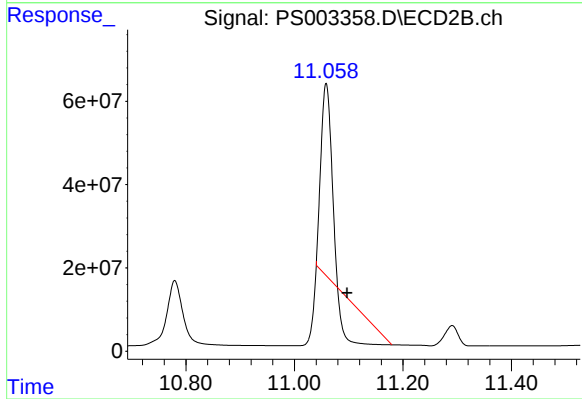


#5 DICAMBA

R.T.: 11.059 min
Delta R.T.: -0.038 min
Response: 263868605
Conc: 166.30 ng/ml

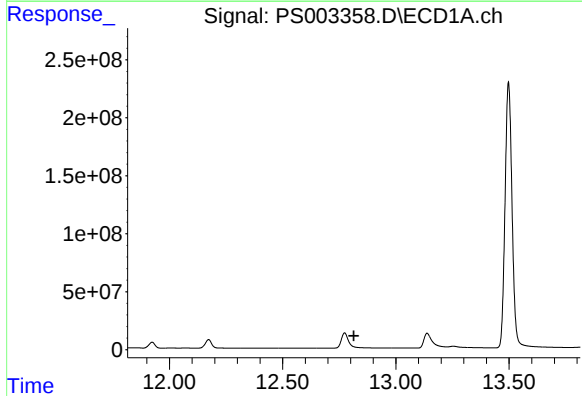


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.815 min
Response: 0
Conc: N.D.

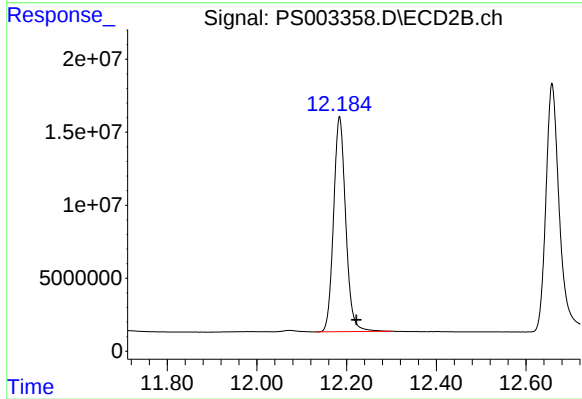

#8 DICHLORPROP


R.T.: 12.184 min
Delta R.T.: -0.038 min
Response: 276919011
Conc: 724.27 ng/ml

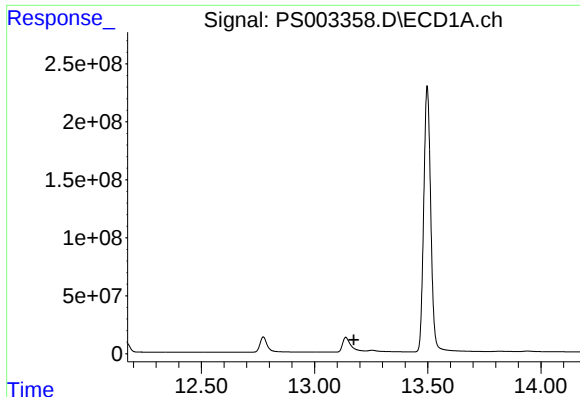

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.173 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

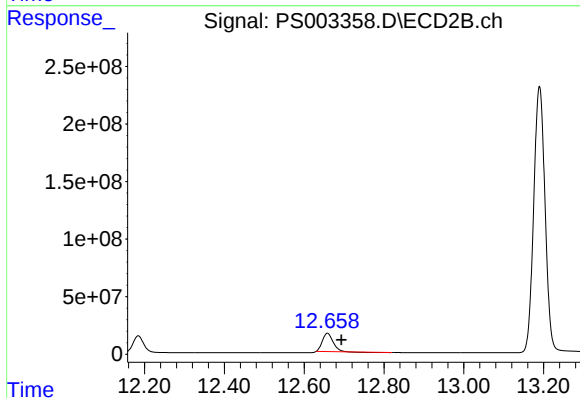


#9 2,4-D

R.T.: 12.658 min
Delta R.T.: -0.035 min
Response: 284230551
Conc: 566.89 ng/ml

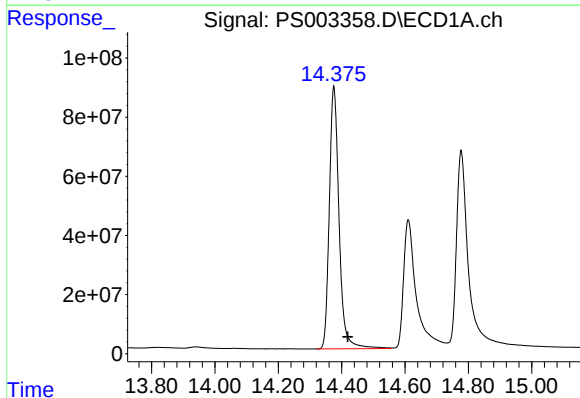


#11 2,4,5-TP (SILVEX)

R.T.: 14.376 min
Delta R.T.: -0.044 min
Response: 1898076443
Conc: 753.69 ng/ml

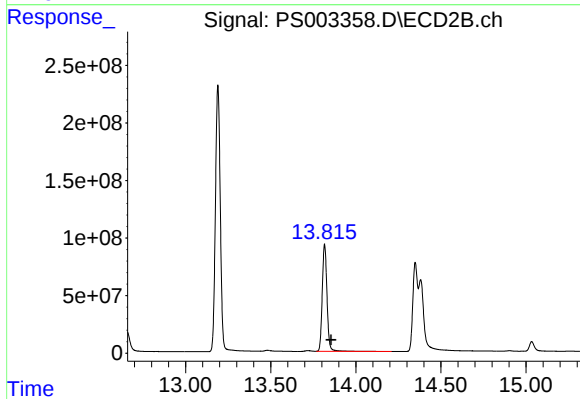

#11 2,4,5-TP (SILVEX)


R.T.: 13.816 min
Delta R.T.: -0.038 min
Response: 1801431109
Conc: 726.28 ng/ml

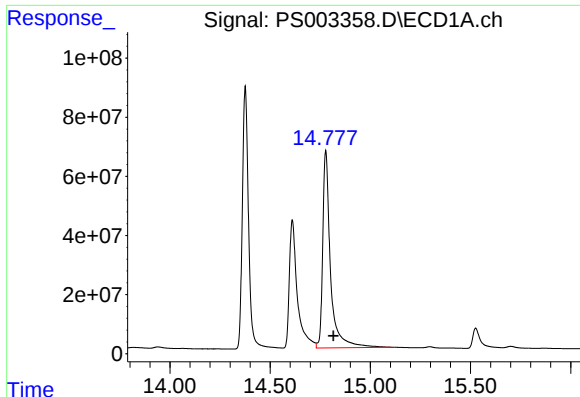

#12 2,4,5-T


R.T.: 14.778 min
Delta R.T.: -0.039 min
Response: 1812786652
Conc: 743.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

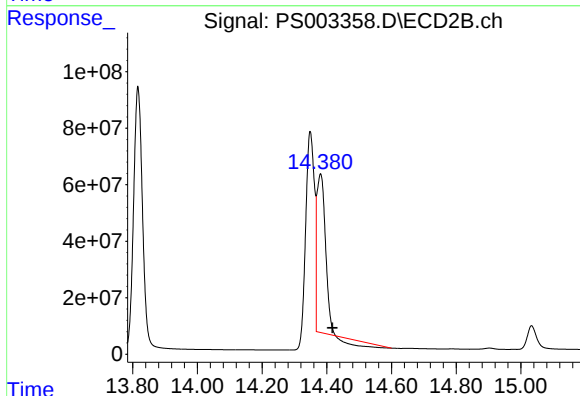


#12 2,4,5-T

R.T.: 14.381 min
Delta R.T.: -0.036 min
Response: 924293378
Conc: 483.04 ng/ml

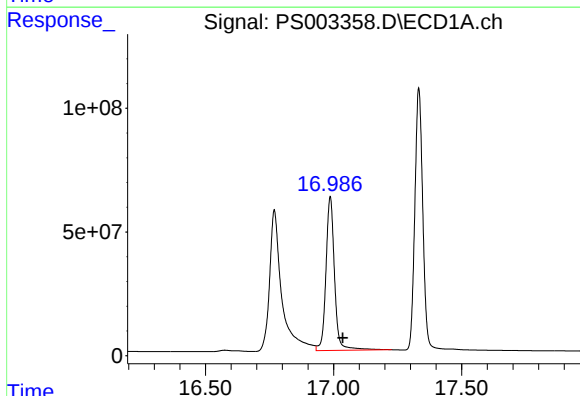


#14 DINOSEB

R.T.: 16.987 min
Delta R.T.: -0.049 min
Response: 1457488796
Conc: 774.71 ng/ml

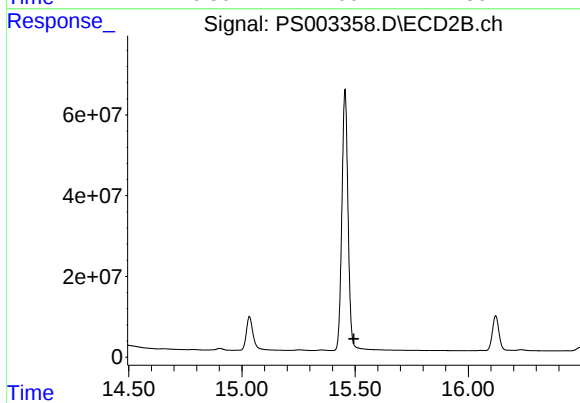

#14 DINOSEB


R.T.: 15.455 min
Delta R.T.: -0.040 min
Response: -812885959
Conc: N.D.

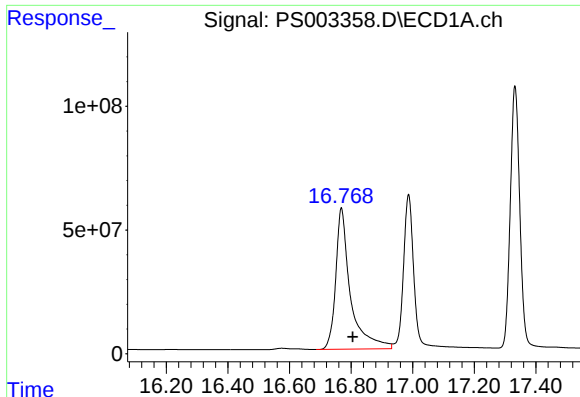

#15 Picloram


R.T.: 16.769 min
Delta R.T.: -0.037 min
Response: 1900006200
Conc: 600.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

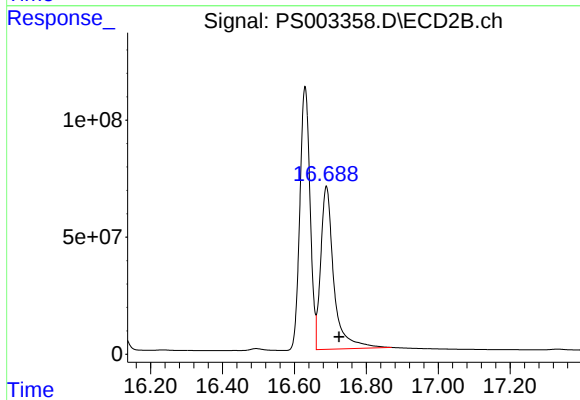


#15 Picloram

R.T.: 16.689 min
Delta R.T.: -0.035 min
Response: 1761601581
Conc: 585.95 ng/ml

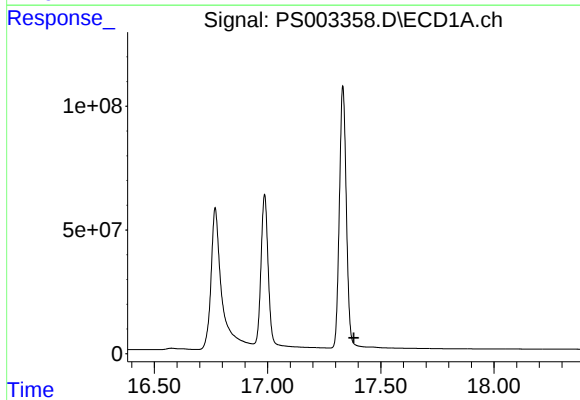

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.382 min
Response: 0
Conc: N.D.

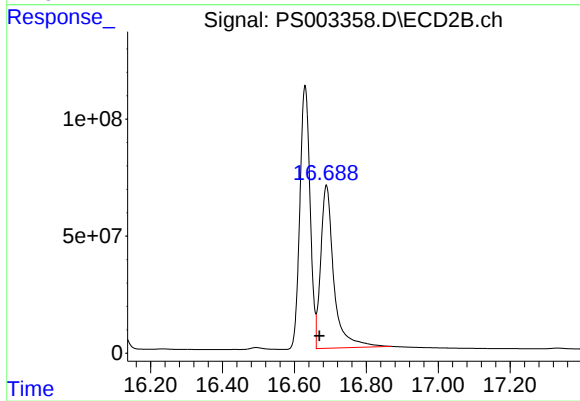

#16 DCPA

R.T.: 16.689 min
Delta R.T.: 0.019 min
Response: 1761601581
Conc: 568.70 ng/ml