

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
 Data File : PS003359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 15:51
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 03:01:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	0.000	9.925	0	56518	N.D. 0.251 #
5) T	DICAMBA	0.000	11.126	0	101570	N.D. 0.061 #
6) T	MCP	0.000	11.293	0	13737	N.D. 0.012 #
7) T	MCPA	0.000	11.676	0	369523	N.D. 0.214 #
10) T	Pentachlo...	0.000	13.202	0	26230	N.D. 0.004 #
11) T	2,4,5-TP ...	0.000	13.810	0	149268	N.D. 0.059 #
12) T	2,4,5-T	0.000	14.411	0	2155307	N.D. 1.069 #
13) T	2,4-DB	0.000	15.016	0	115127	N.D. 0.451 #
14) T	DINOSEB	0.000	15.439	0	125574	N.D. 0.070 #
15) T	Picloram	0.000	16.731	0	181453	N.D. 0.071 #
16) T	DCPA	0.000	16.645	0	271995	N.D. 0.087 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
Data File : PS003359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 15:51
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 03:01:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

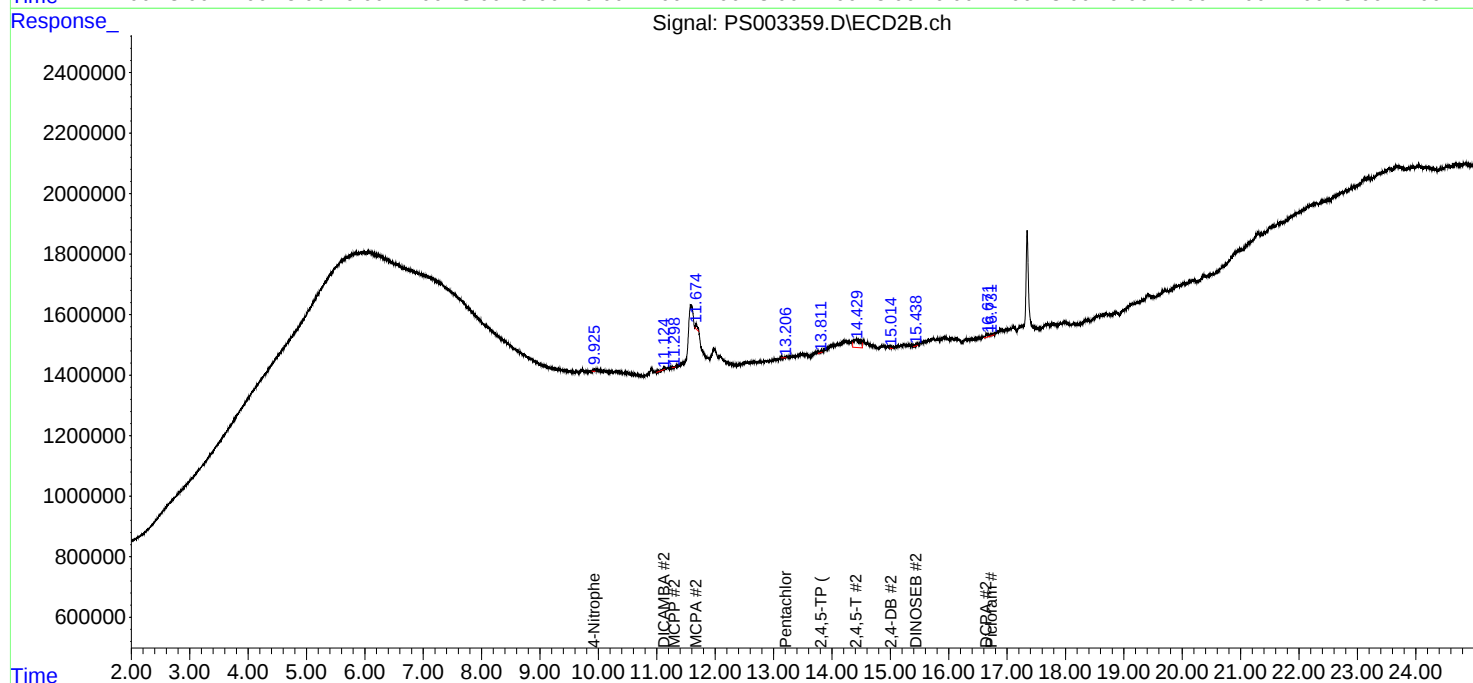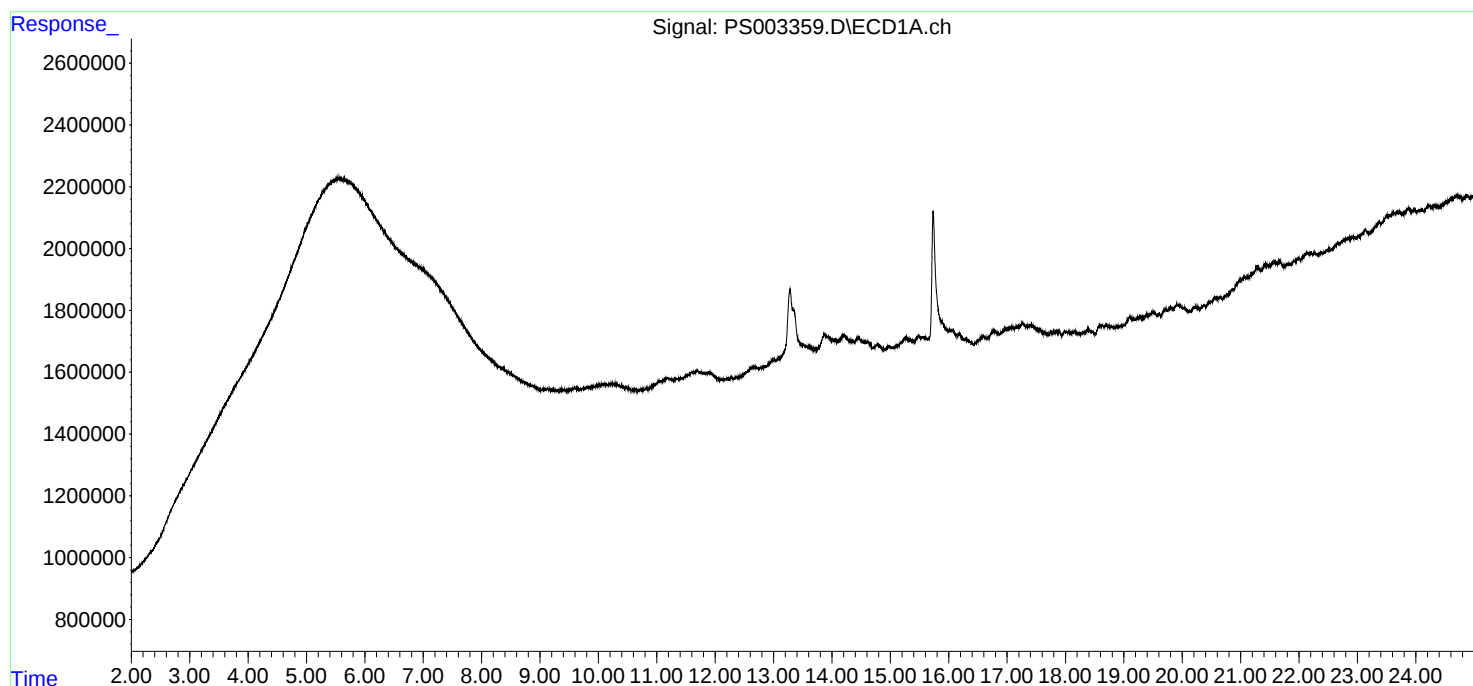


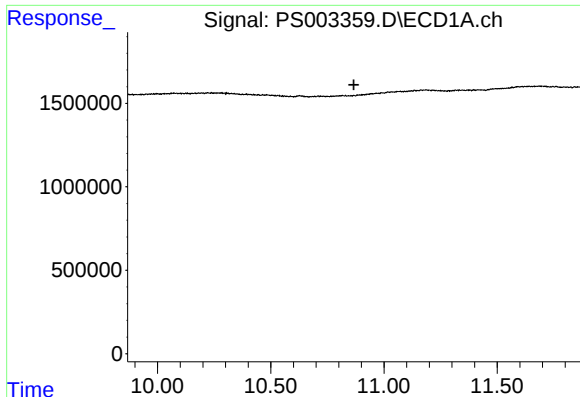

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

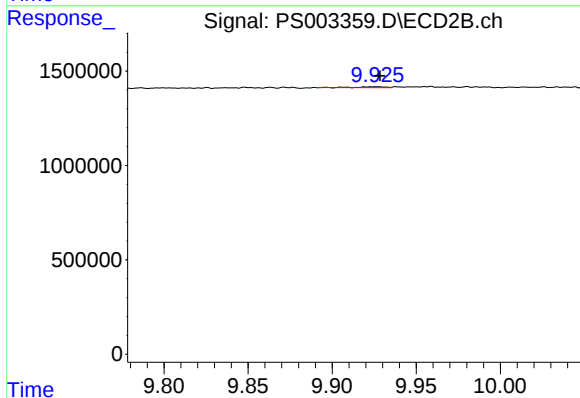


#3 4-Nitrophenol

R.T.: 9.925 min
Delta R.T.: -0.003 min
Response: 56518
Conc: 0.25 ng/ml

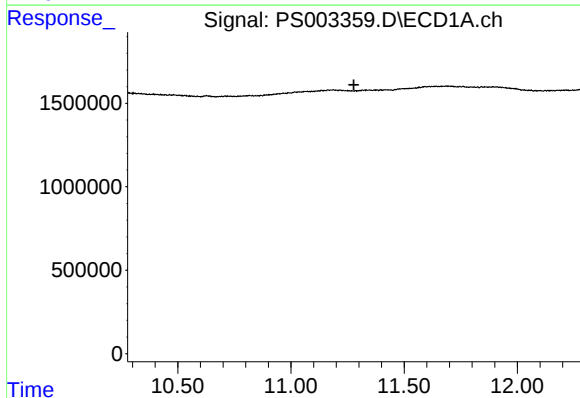


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

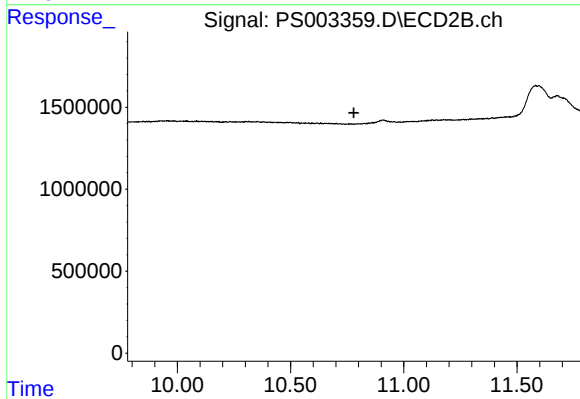

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.780 min
Response: 0
Conc: N.D.

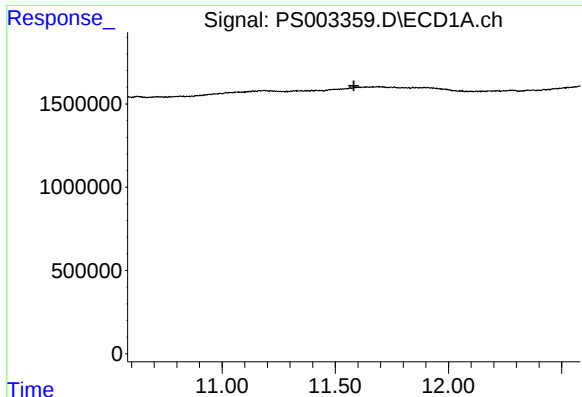

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

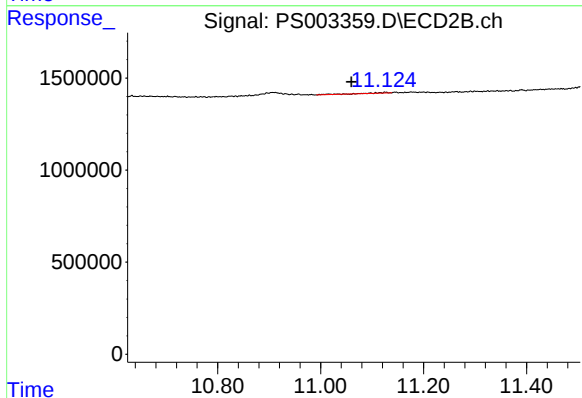


#5 DICAMBA

R.T.: 11.126 min
Delta R.T.: 0.067 min
Response: 101570
Conc: 0.06 ng/ml

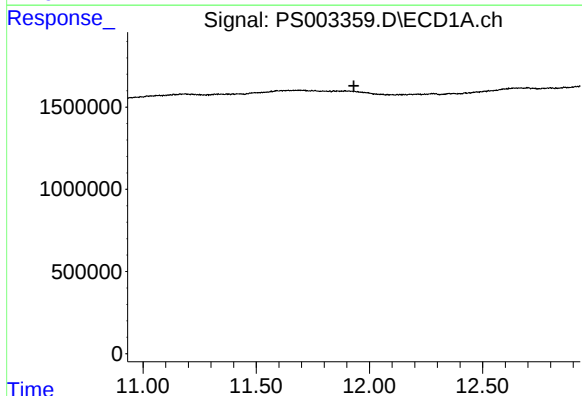


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.931 min
Response: 0
Conc: N.D.

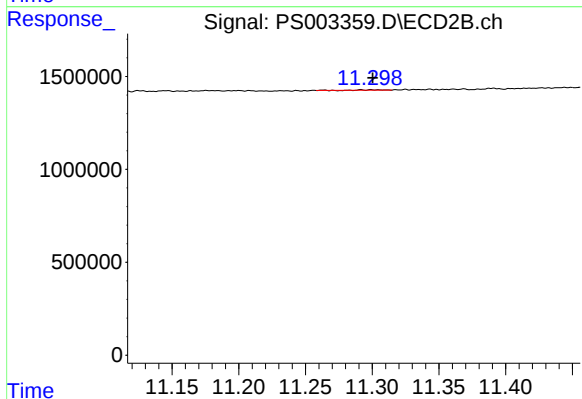

#6 MCP


R.T.: 11.293 min
Delta R.T.: -0.008 min
Response: 13737
Conc: 0.01 ug/ml

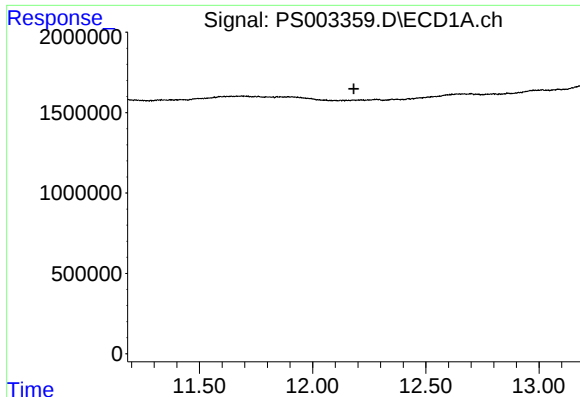

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

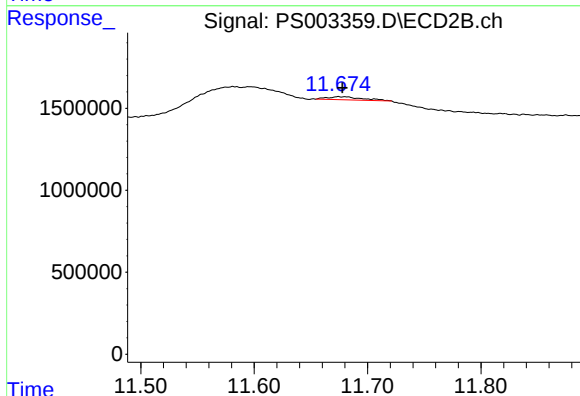


#7 MCPA

R.T.: 11.676 min
Delta R.T.: -0.002 min
Response: 369523
Conc: 0.21 ug/ml

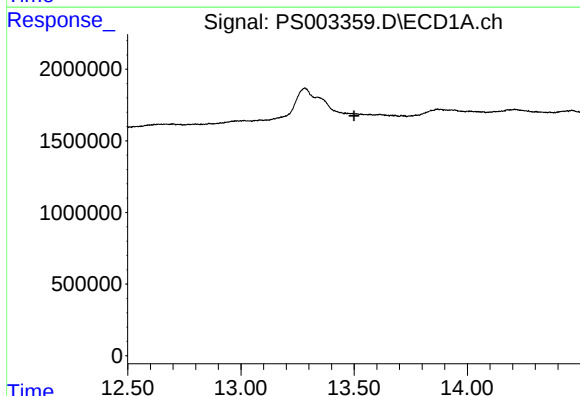


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

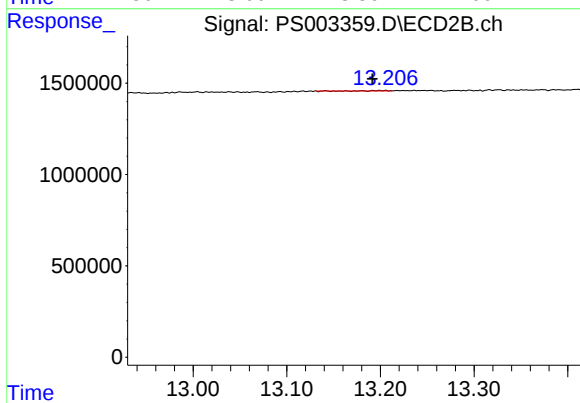

#10 Pentachlorophenol


R.T.: 13.202 min
Delta R.T.: 0.010 min
Response: 26230
Conc: 0.00 ng/ml

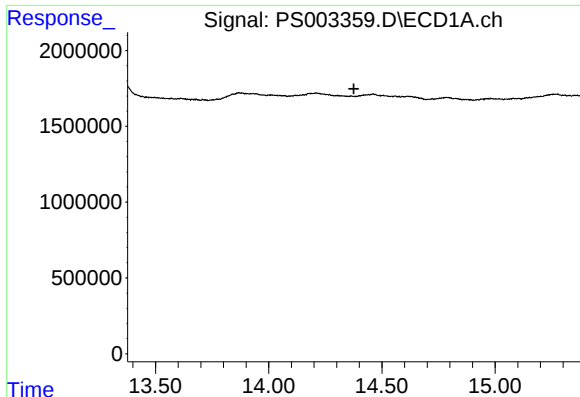

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

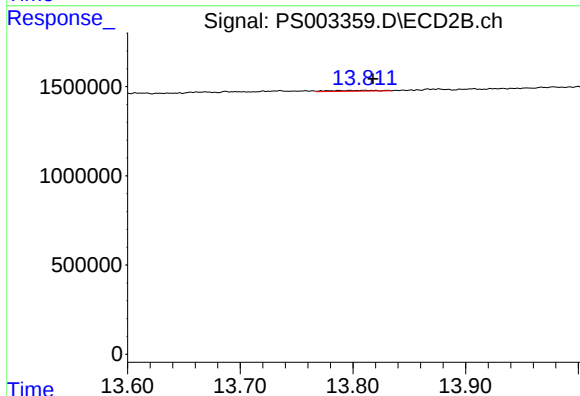


#11 2,4,5-TP (SILVEX)

R.T.: 13.810 min
Delta R.T.: -0.008 min
Response: 149268
Conc: 0.06 ng/ml

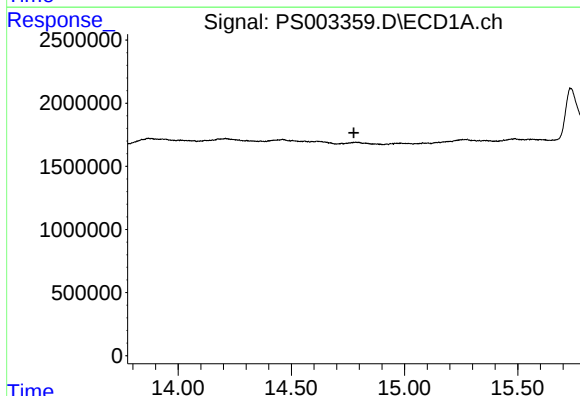


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

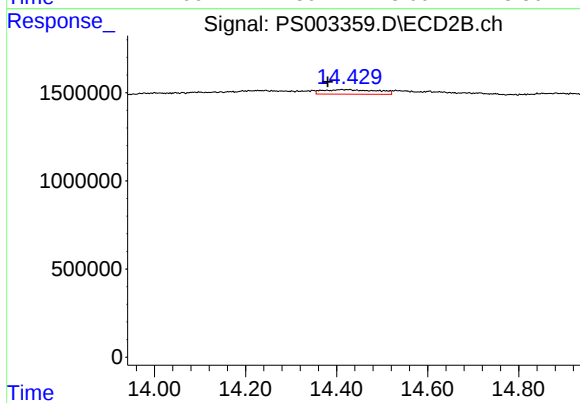

#12 2,4,5-T


R.T.: 14.411 min
Delta R.T.: 0.030 min
Response: 2155307
Conc: 1.07 ng/ml

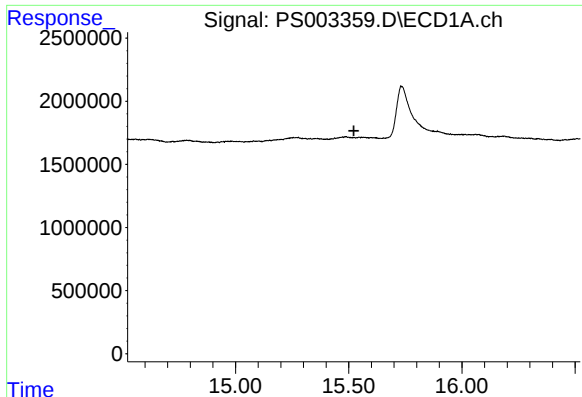

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

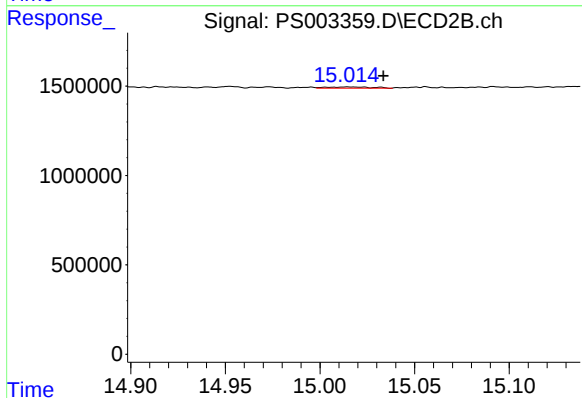


#13 2,4-DB

R.T.: 15.016 min
Delta R.T.: -0.018 min
Response: 115127
Conc: 0.45 ng/ml

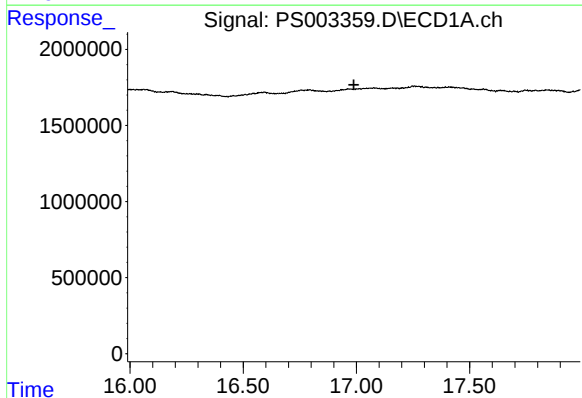


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

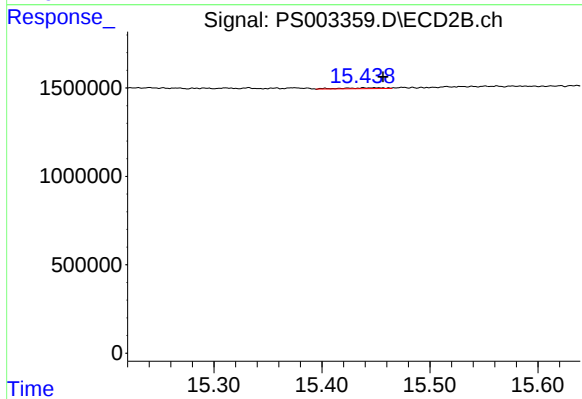

#14 DINOSEB


R.T.: 15.439 min
Delta R.T.: -0.018 min
Response: 125574
Conc: 0.07 ng/ml

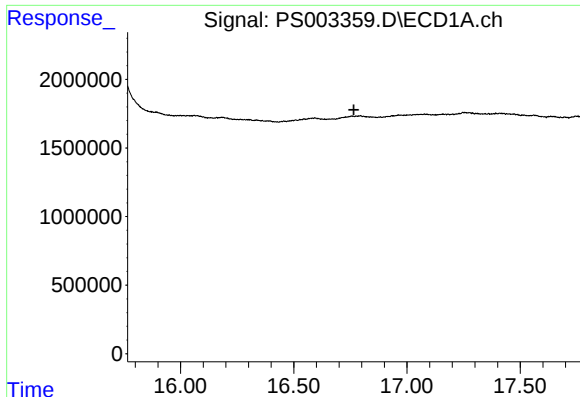

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

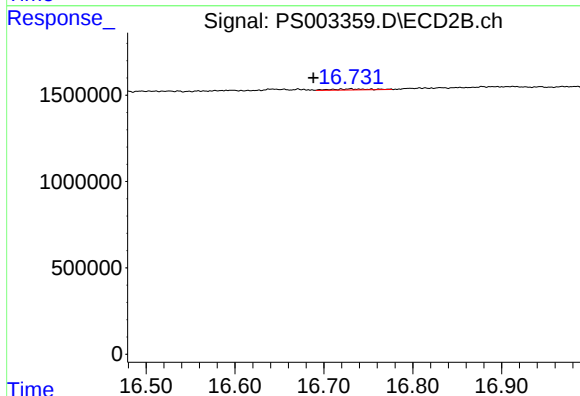


#15 Picloram

R.T.: 16.731 min
Delta R.T.: 0.042 min
Response: 181453
Conc: 0.07 ng/ml

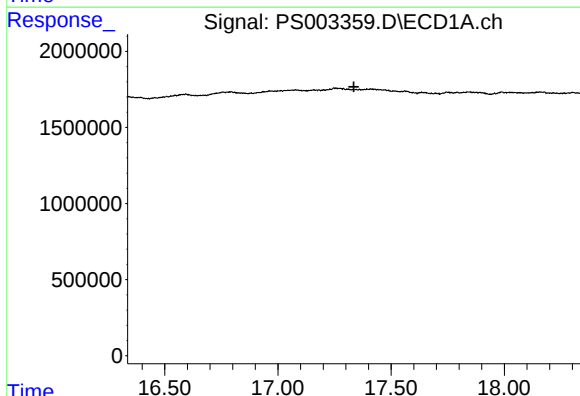

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

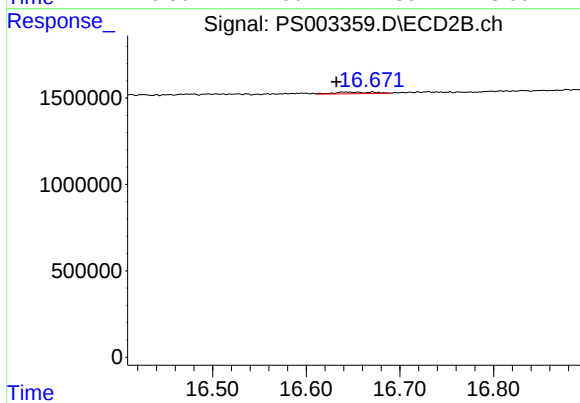

#16 DCPA

R.T.: 16.645 min
Delta R.T.: 0.013 min
Response: 271995
Conc: 0.09 ng/ml