

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
 Data File : PS003360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 16:22
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 03:02:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.289	10.786	215.5E6	207.4E6	490.974	441.698
Target Compounds							
2) T	3,5-DICHL...	0.000	8.946	0	44008	N.D.	0.071 #
7) T	MCPA	0.000	11.670	0	335919	N.D.	0.195 #
9) T	2,4-D	0.000	12.688	0	641207	N.D.	1.222 #
10) T	Pentachlo...	0.000	13.204	0	586459	N.D.	0.089 #
11) T	2,4,5-TP ...	0.000	13.783	0	315550	N.D.	0.124 #
12) T	2,4,5-T	0.000	14.402	0	301008	N.D.	0.149 #
14) T	DINOSEB	0.000	15.453	0	1086667	N.D.	0.609 #
15) T	Picloram	0.000	16.643	0	755881	N.D.	0.298 #
16) T	DCPA	0.000	16.643	0	755881	N.D.	0.243 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
Data File : PS003360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 16:22
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 03:02:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

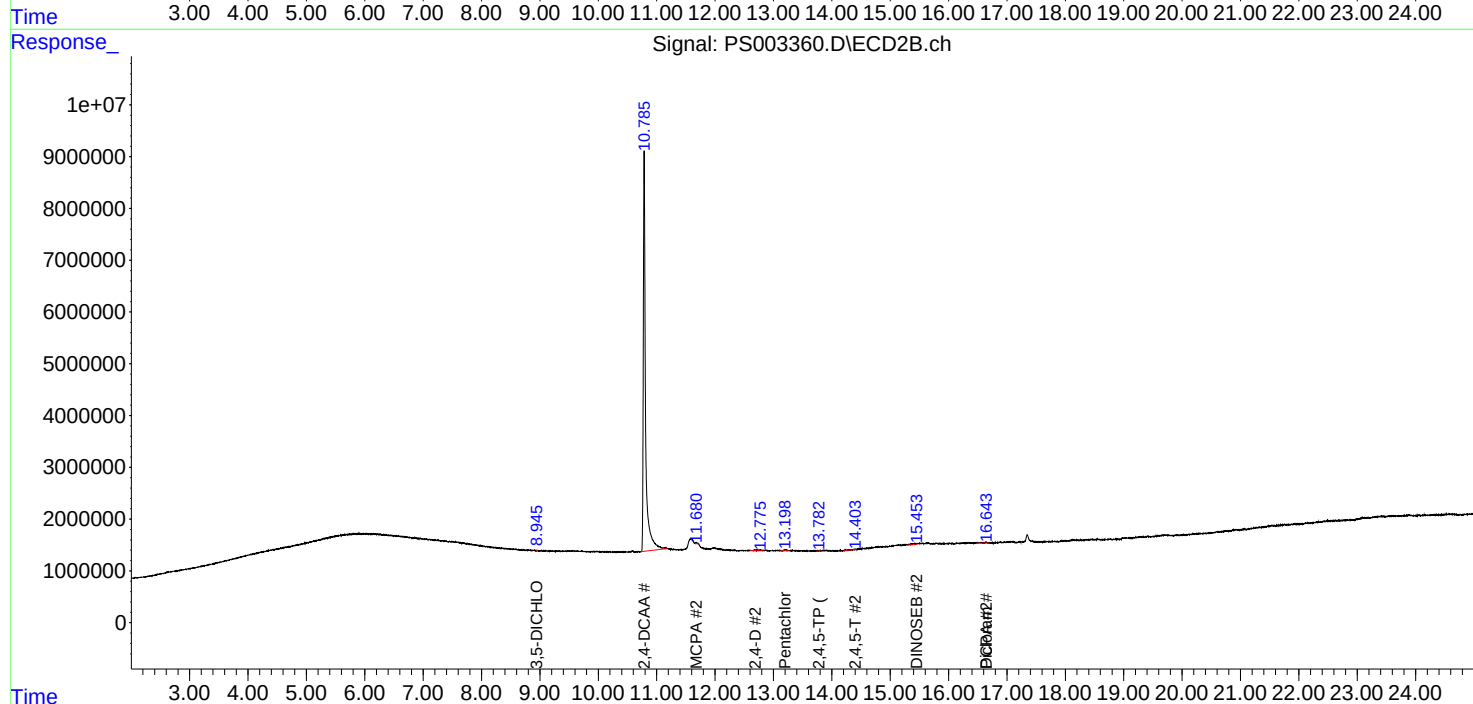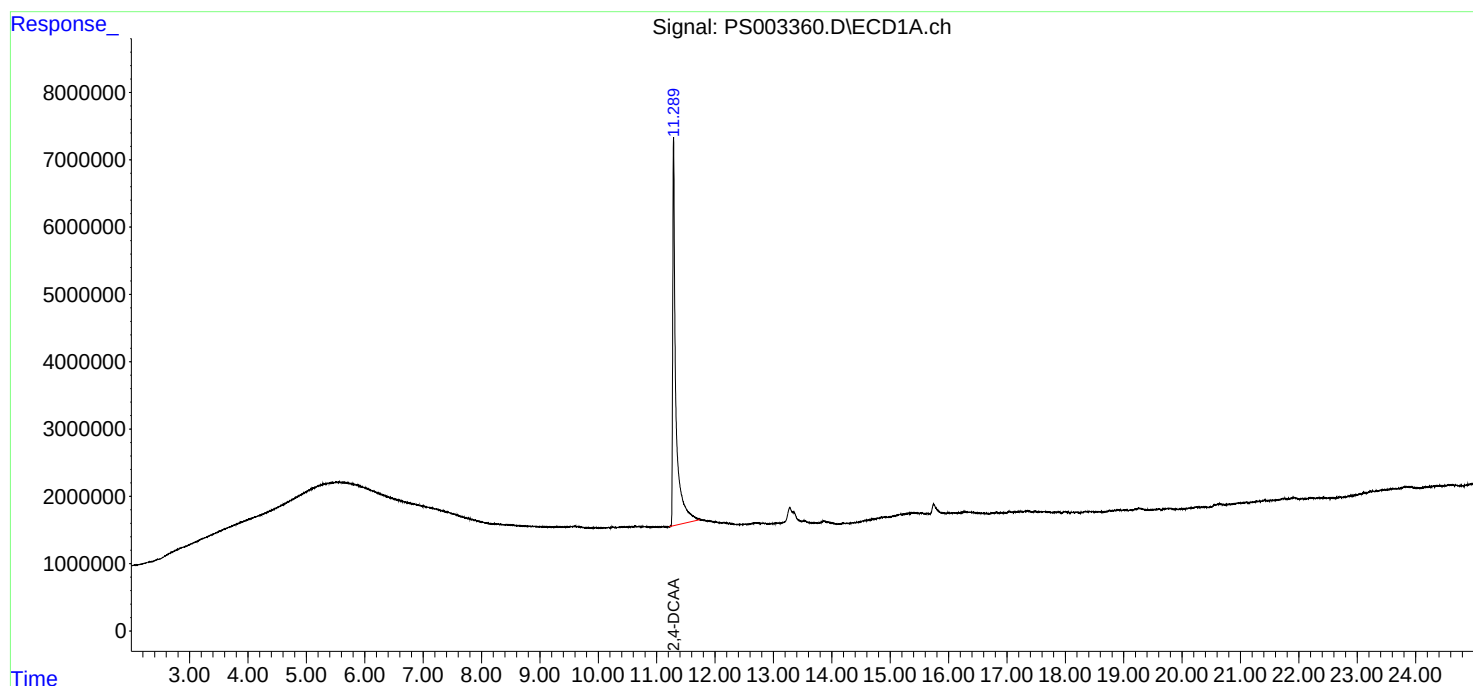


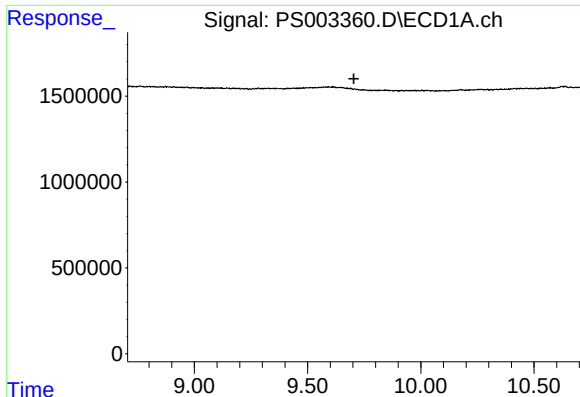

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

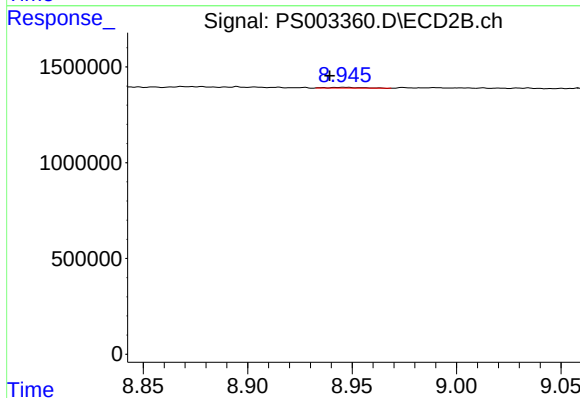


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.946 min
Delta R.T.: 0.006 min
Response: 44008
Conc: 0.07 ng/ml

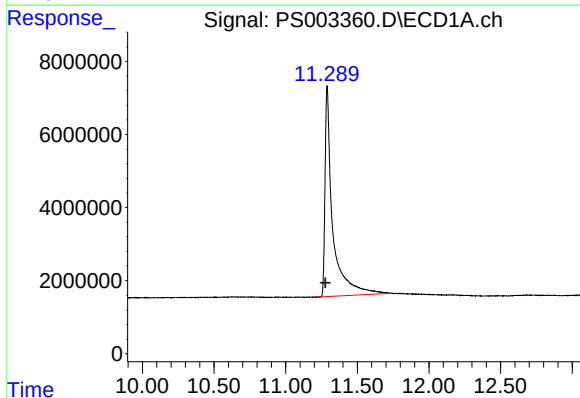


#4 2,4-DCAA

R.T.: 11.289 min
Delta R.T.: 0.011 min
Response: 215549545
Conc: 490.97 ng/ml

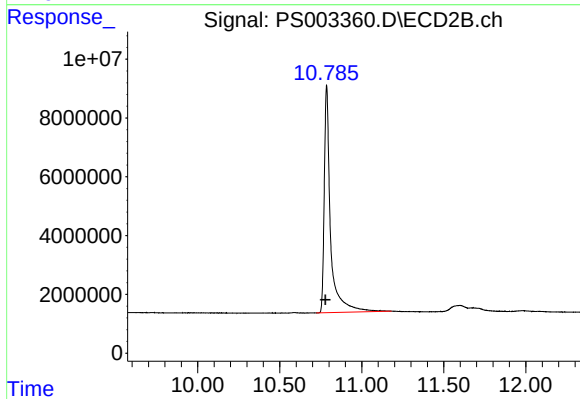

#4 2,4-DCAA


R.T.: 10.786 min
Delta R.T.: 0.006 min
Response: 207407928
Conc: 441.70 ng/ml

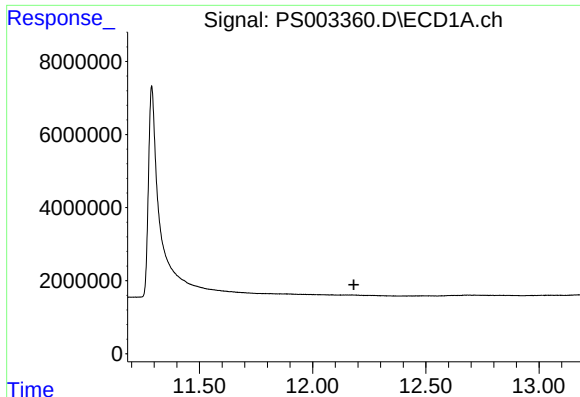

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

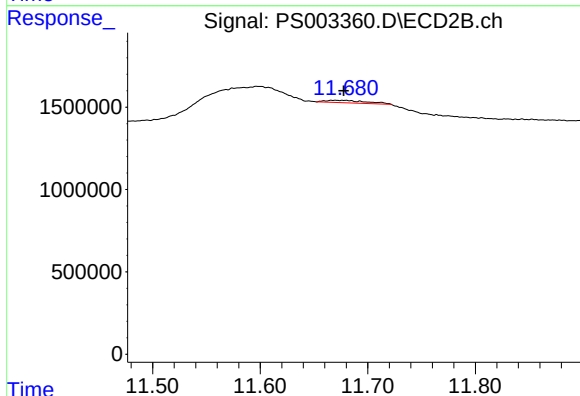


#7 MCPA

R.T.: 11.670 min
Delta R.T.: -0.008 min
Response: 335919
Conc: 0.19 ug/ml

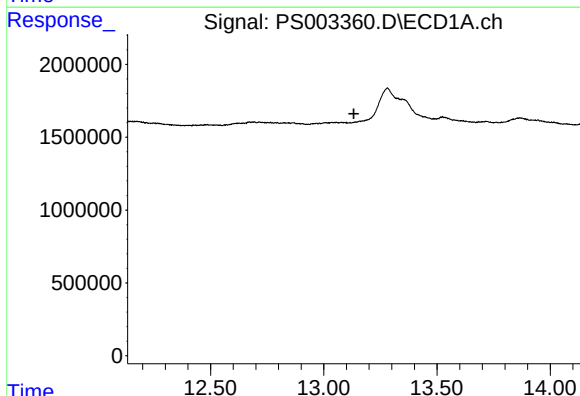


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

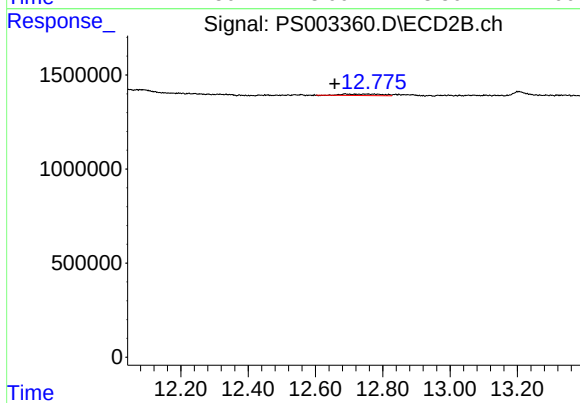

#9 2,4-D


R.T.: 12.688 min
Delta R.T.: 0.031 min
Response: 641207
Conc: 1.22 ng/ml

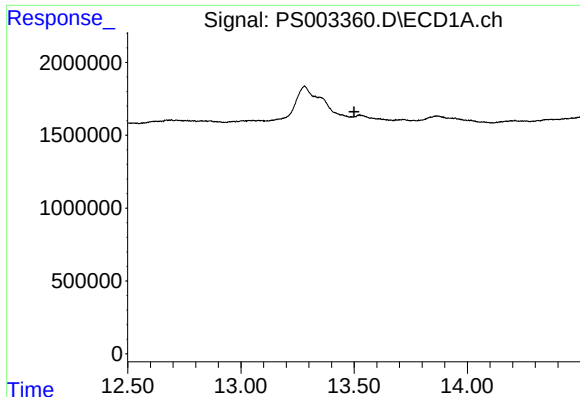

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

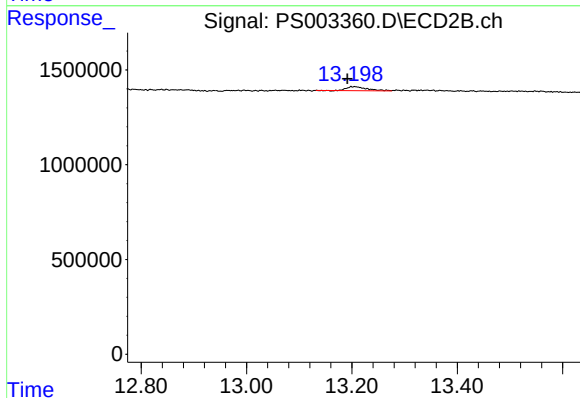


#10 Pentachlorophenol

R.T.: 13.204 min
Delta R.T.: 0.013 min
Response: 586459
Conc: 0.09 ng/ml

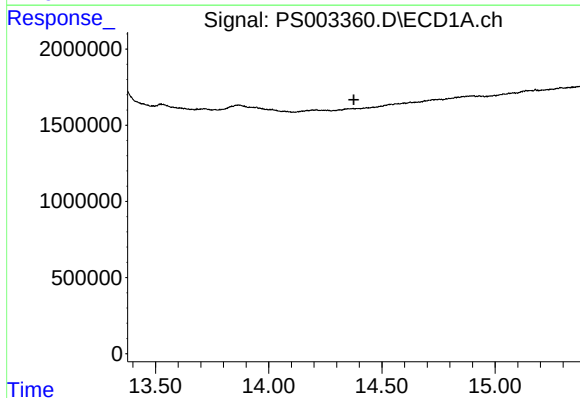


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

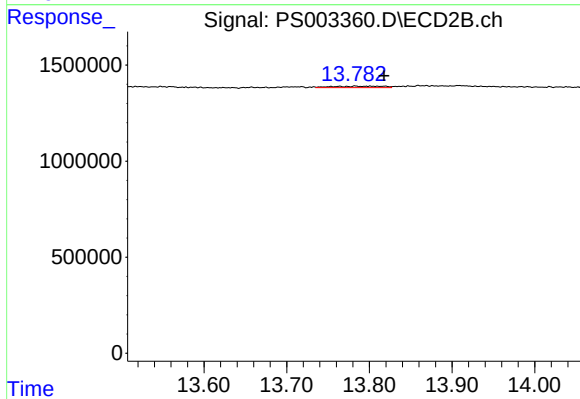

#11 2,4,5-TP (SILVEX)


R.T.: 13.783 min
Delta R.T.: -0.034 min
Response: 315550
Conc: 0.12 ng/ml

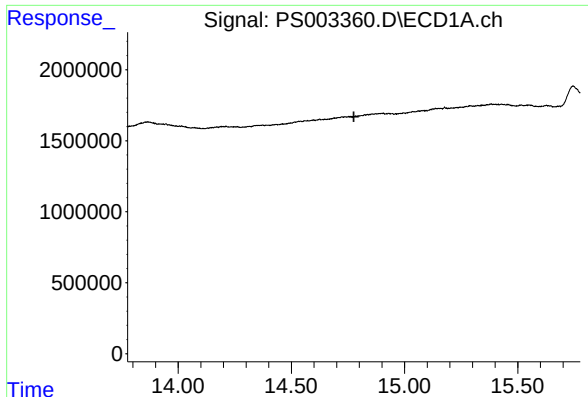

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

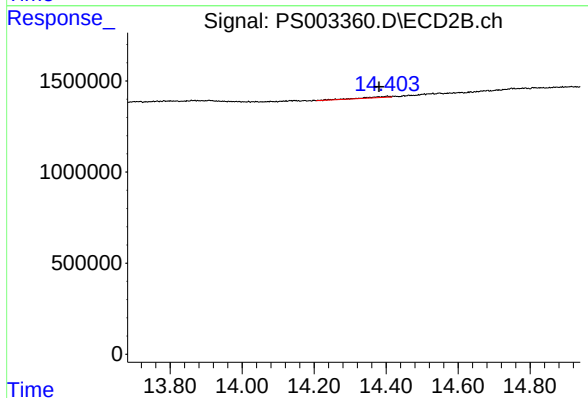


#12 2,4,5-T

R.T.: 14.402 min
Delta R.T.: 0.022 min
Response: 301008
Conc: 0.15 ng/ml

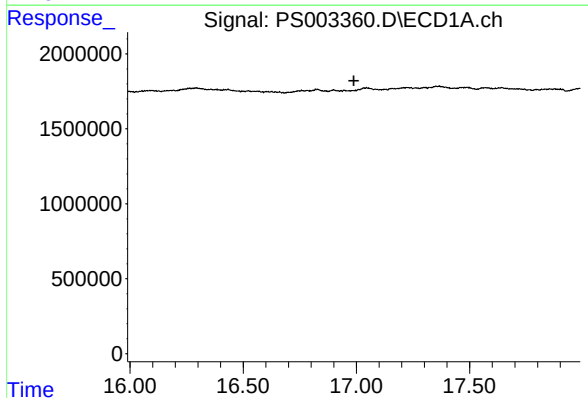


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

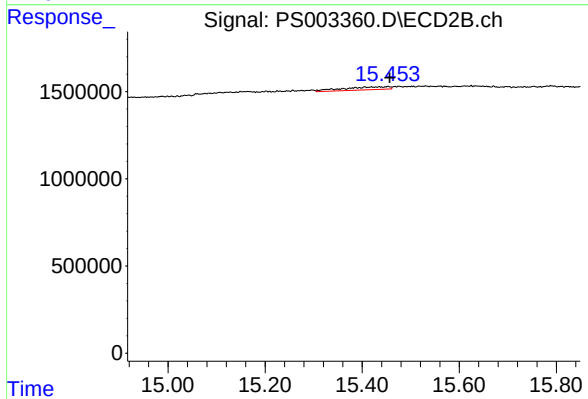

#14 DINOSEB


R.T.: 15.453 min
Delta R.T.: -0.004 min
Response: 1086667
Conc: 0.61 ng/ml

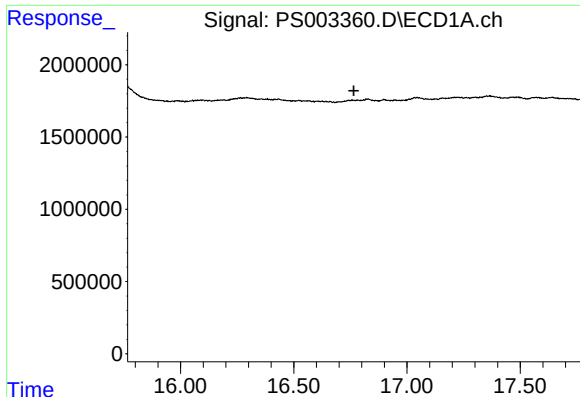

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

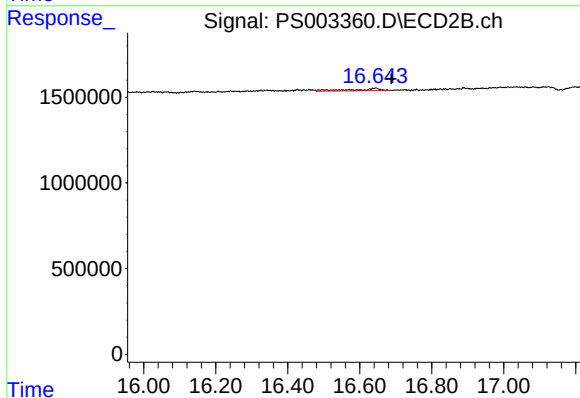


#15 Picloram

R.T.: 16.643 min
Delta R.T.: -0.046 min
Response: 755881
Conc: 0.30 ng/ml

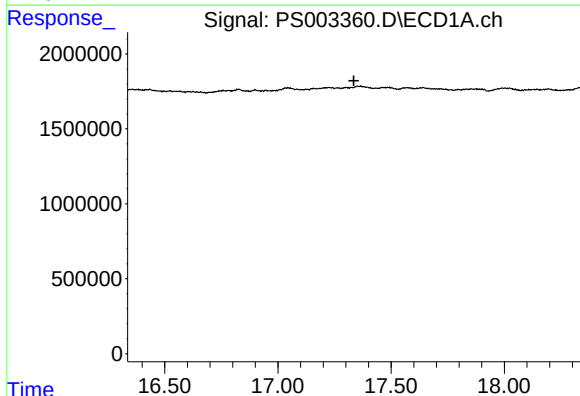

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

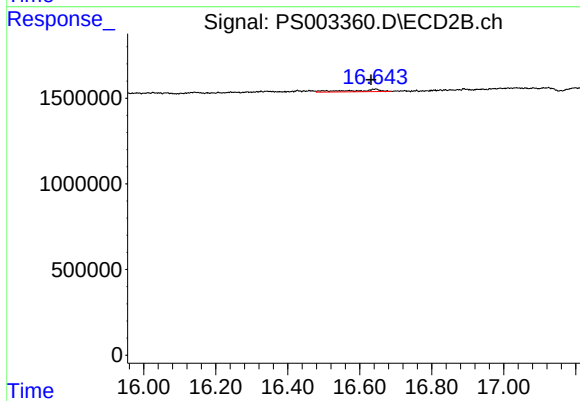

#16 DCPA

R.T.: 16.643 min
Delta R.T.: 0.011 min
Response: 755881
Conc: 0.24 ng/ml