

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
 Data File : PS003370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 21:33
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 03:03:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.288	10.783	214.7E6	211.3E6	489.131	450.092
Target Compounds							
2) T	3,5-DICHL...	0.000	9.008	0	88444	N.D.	0.143 #
3) T	4-Nitroph...	0.000	9.948	0	52089	N.D.	0.232 #
7) T	MCPA	0.000	11.663	0	520020	N.D.	0.301 #
8) T	DICHLORPROP	0.000	12.182	0	581043	N.D.	1.406 #
9) T	2,4-D	0.000	12.661	0	86964	N.D.	0.166 #
10) T	Pentachlo...	0.000	13.205	0	1717321	N.D.	0.261 #
11) T	2,4,5-TP ...	0.000	13.841	0	520960	N.D.	0.205 #
14) T	DINOSEB	0.000	15.469	0	818897	N.D.	0.459 #
15) T	Picloram	0.000	16.637	0	985736	N.D.	0.388 #
16) T	DCPA	0.000	16.637	0	985736	N.D.	0.317 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
Data File : PS003370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 21:33
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 03:03:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

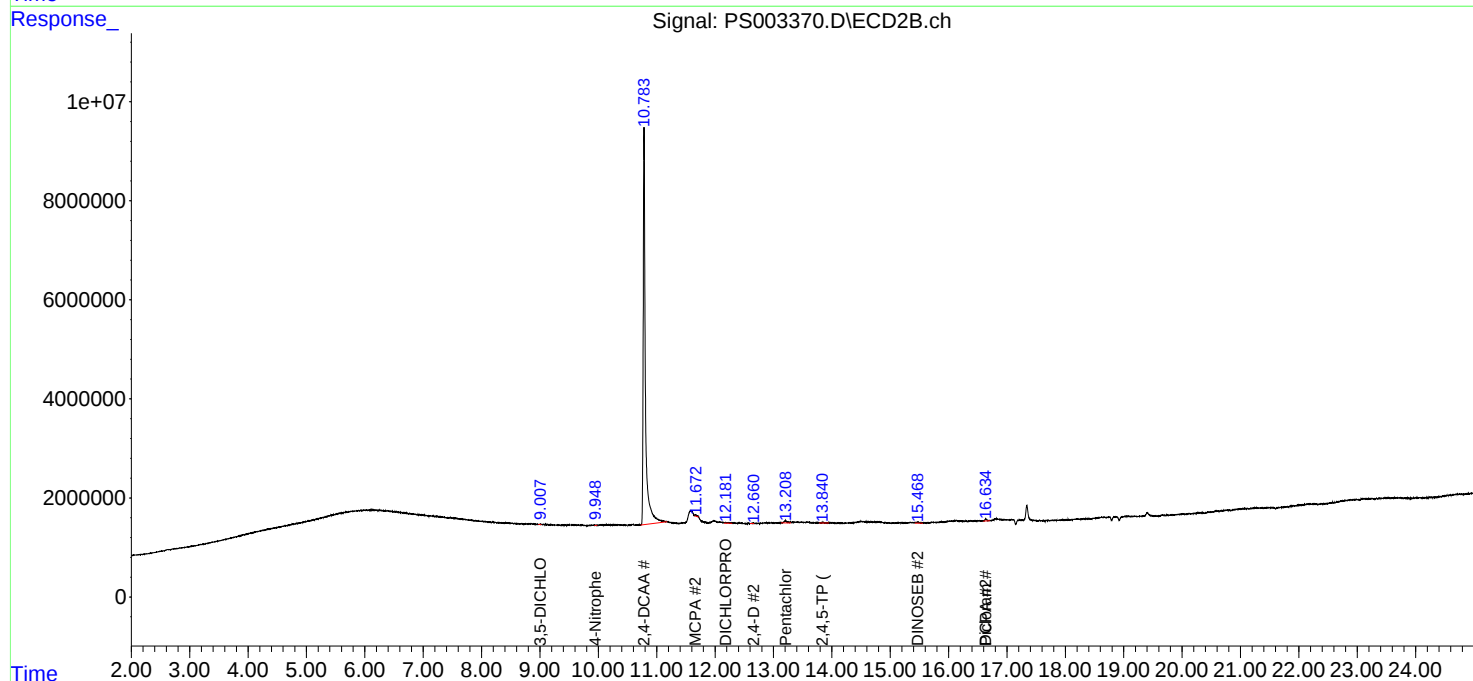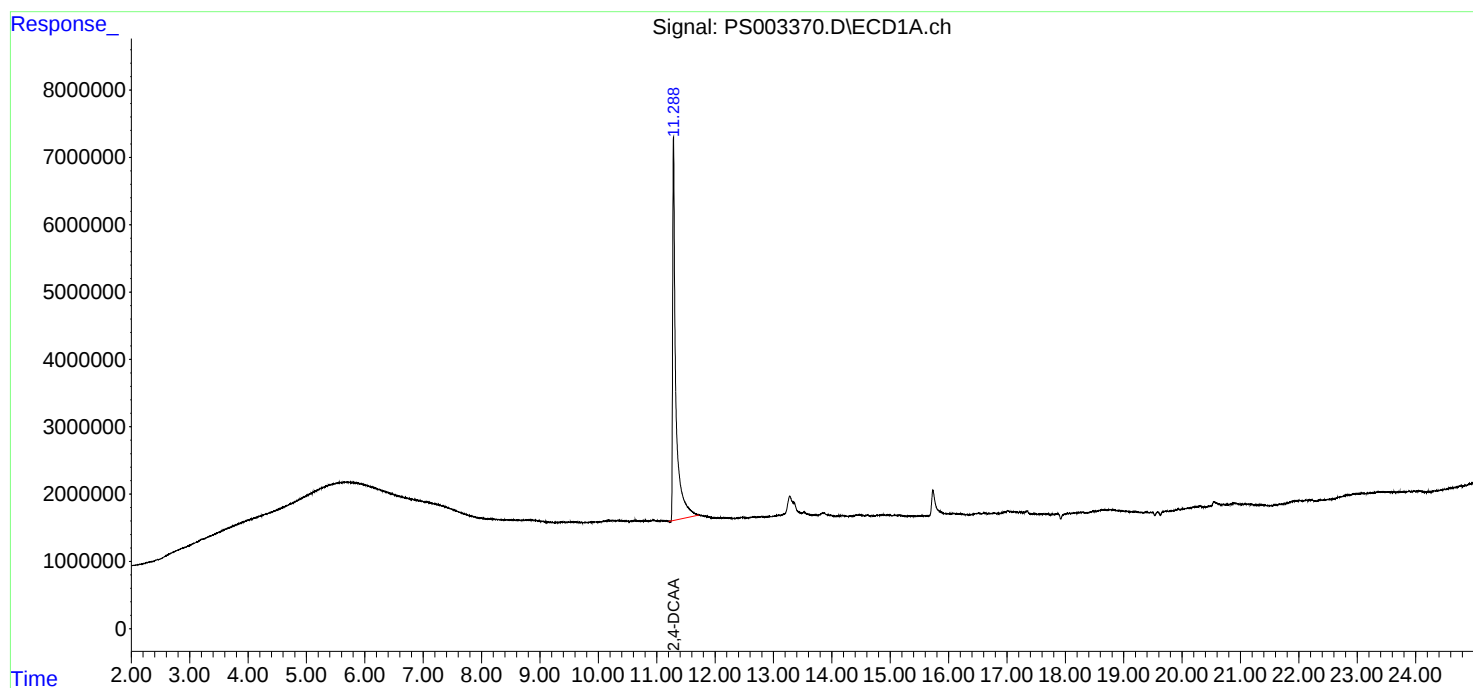


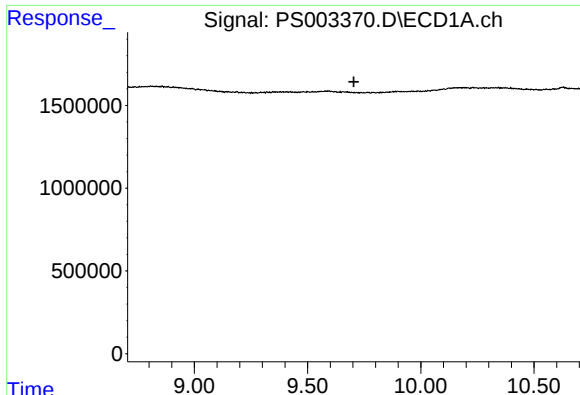

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

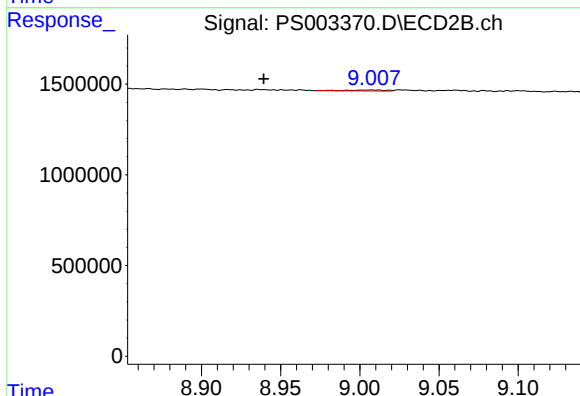


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.008 min
Delta R.T.: 0.069 min
Response: 88444
Conc: 0.14 ng/ml

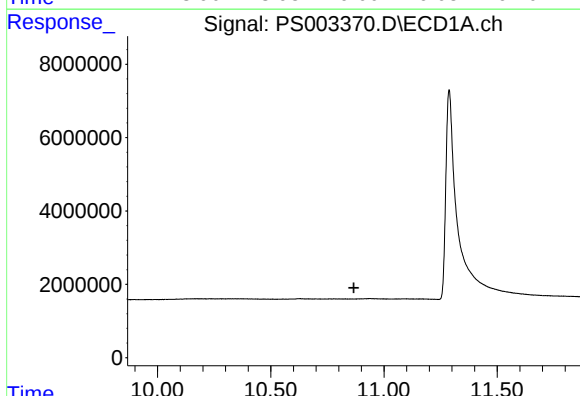


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

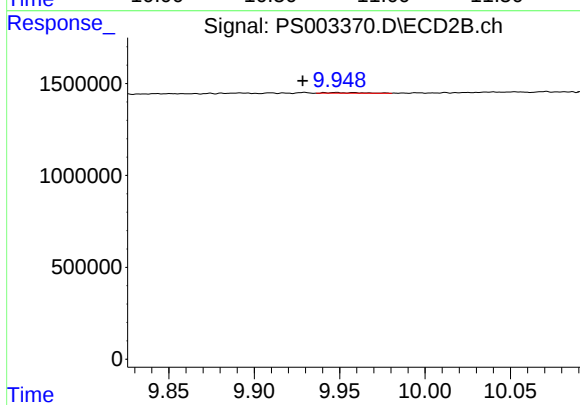

#3 4-Nitrophenol


R.T.: 9.948 min
Delta R.T.: 0.019 min
Response: 52089
Conc: 0.23 ng/ml

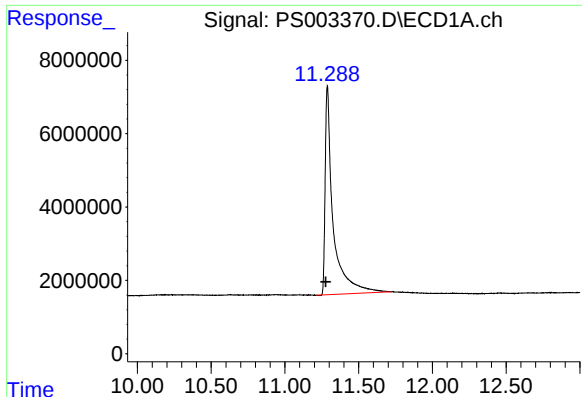

#4 2,4-DCAA


R.T.: 11.288 min
Delta R.T.: 0.010 min
Response: 214740301
Conc: 489.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

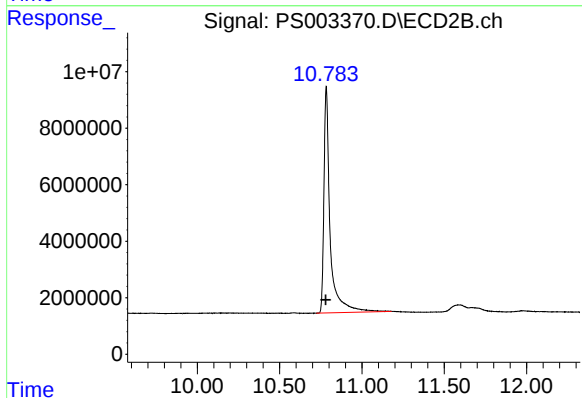


#4 2,4-DCAA

R.T.: 10.783 min
Delta R.T.: 0.003 min
Response: 211349406
Conc: 450.09 ng/ml

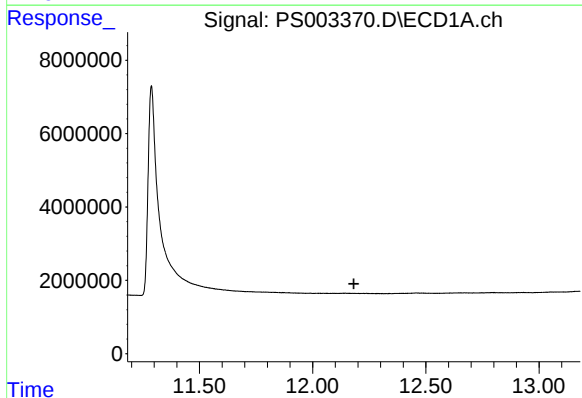


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

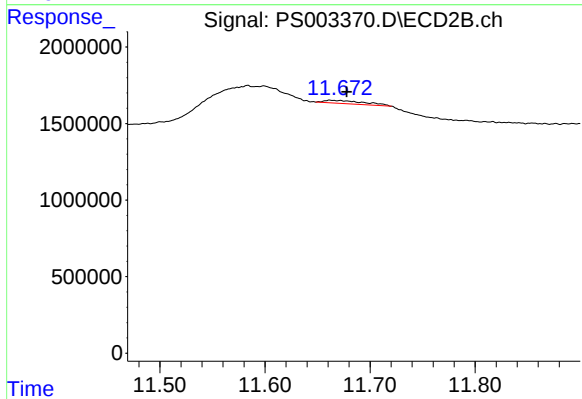

#7 MCPA


R.T.: 11.663 min
Delta R.T.: -0.015 min
Response: 520020
Conc: 0.30 ug/ml

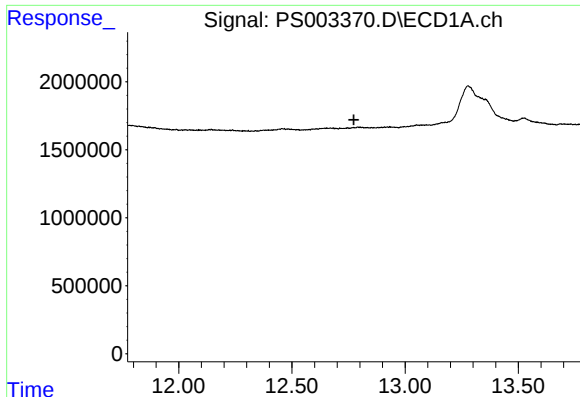

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

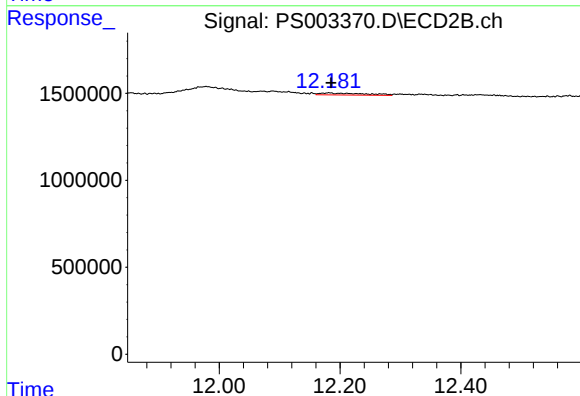


#8 DICHLORPROP

R.T.: 12.182 min
Delta R.T.: -0.003 min
Response: 581043
Conc: 1.41 ng/ml

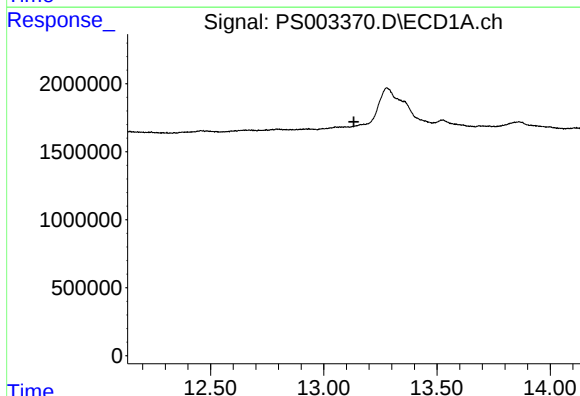


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

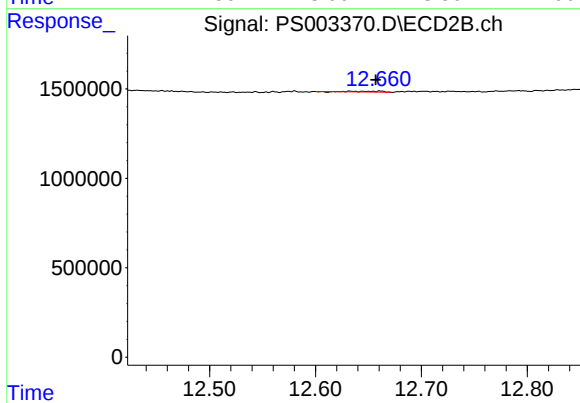

#9 2,4-D


R.T.: 12.661 min
Delta R.T.: 0.004 min
Response: 86964
Conc: 0.17 ng/ml

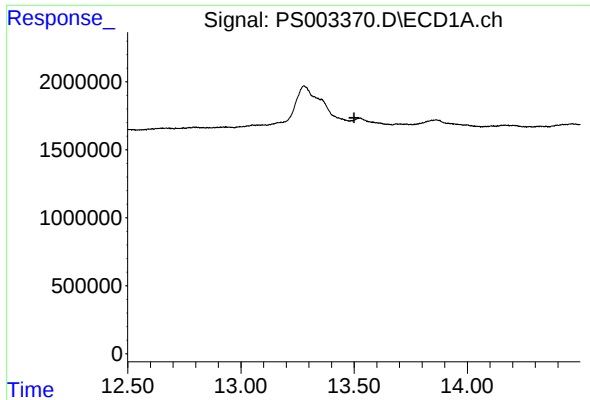

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

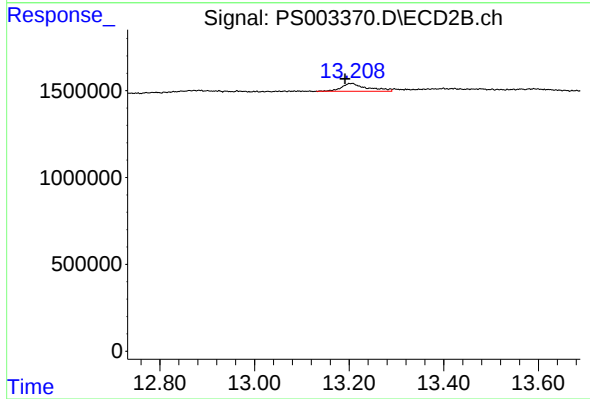


#10 Pentachlorophenol

R.T.: 13.205 min
Delta R.T.: 0.013 min
Response: 1717321
Conc: 0.26 ng/ml

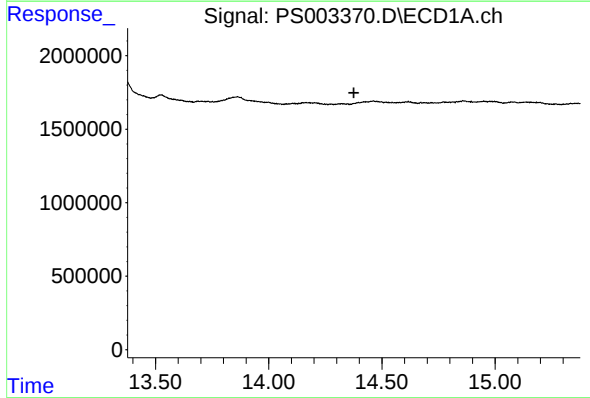


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

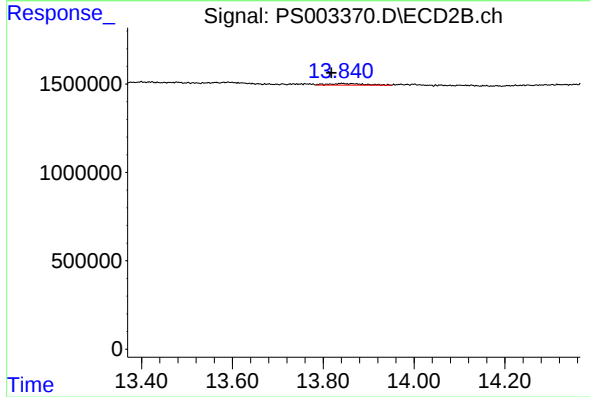

#11 2,4,5-TP (SILVEX)

R.T.: 13.841 min
Delta R.T.: 0.023 min
Response: 520960
Conc: 0.20 ng/ml

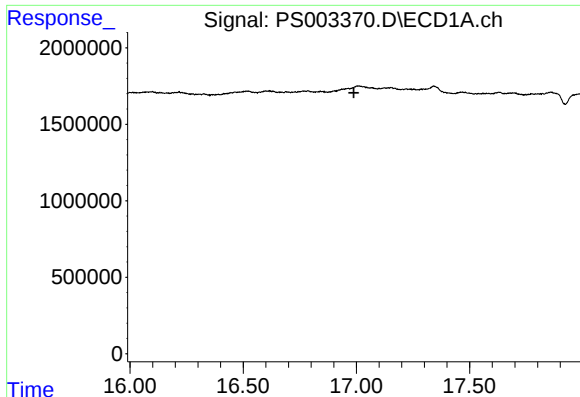

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

#14 DINOSEB


R.T.: 15.469 min
Delta R.T.: 0.012 min
Response: 818897
Conc: 0.46 ng/ml

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

#15 Picloram


R.T.: 16.637 min
Delta R.T.: -0.051 min
Response: 985736
Conc: 0.39 ng/ml

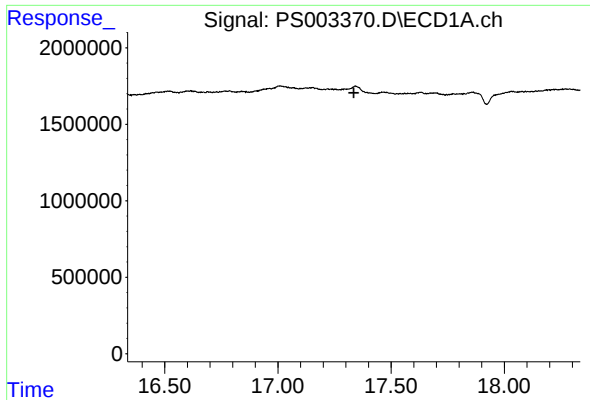

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

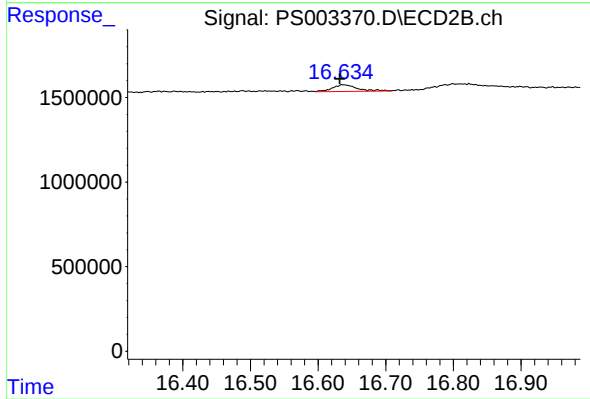

#16 DCPA

R.T.: 16.637 min
Delta R.T.: 0.005 min
Response: 985736
Conc: 0.32 ng/ml