

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
 Data File : PS003363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2019 17:55
 Operator : EI\SJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 02:45:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 02:44:14 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.285	10.785	318.2E6	335.5E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.847	2.318	426.2E6	413.8E6	682.500	682.500
2) T	3,5-DICHL...	9.712	8.945	441.0E6	411.6E6	697.500	697.500
3) T	4-Nitroph...	10.885	9.938	150.9E6	149.1E6	682.500	682.500
5) T	DICAMBA	11.586	11.064	1203.4E6	1139.4E6	705.000	705.000
6) T	MCPD	11.928	11.296	90953995	81908746	70.500	70.500
7) T	MCPA	12.178	11.671	135.5E6	118.4E6	69.750	69.750
8) T	DICHLORPROP	12.779	12.190	290.5E6	277.6E6	705.000	705.000
9) T	2,4-D	13.144	12.664	322.7E6	356.5E6	705.000	705.000
10) T	Pentachlo...	13.503	13.195	4903.1E6	4559.1E6	712.500	712.500
11) T	2,4,5-TP ...	14.381	13.822	1866.9E6	1759.8E6	712.500	712.500
12) T	2,4,5-T	14.785	14.387	1844.0E6	1377.2E6	712.500	712.500
13) T	2,4-DB	15.533	15.040	169.2E6	179.3E6	712.500	712.500
14) T	DINOSEB	16.992	15.461	1543.6E6	1213.3E6	705.000	705.000
15) T	Picloram	16.776	16.695	1801.0E6	1789.3E6	712.500	712.500
16) T	DCPA	17.338	16.636	2287.3E6	2171.7E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022719\
Data File : PS003363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2019 17:55
Operator : EI\SJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 02:45:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 02:44:14 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

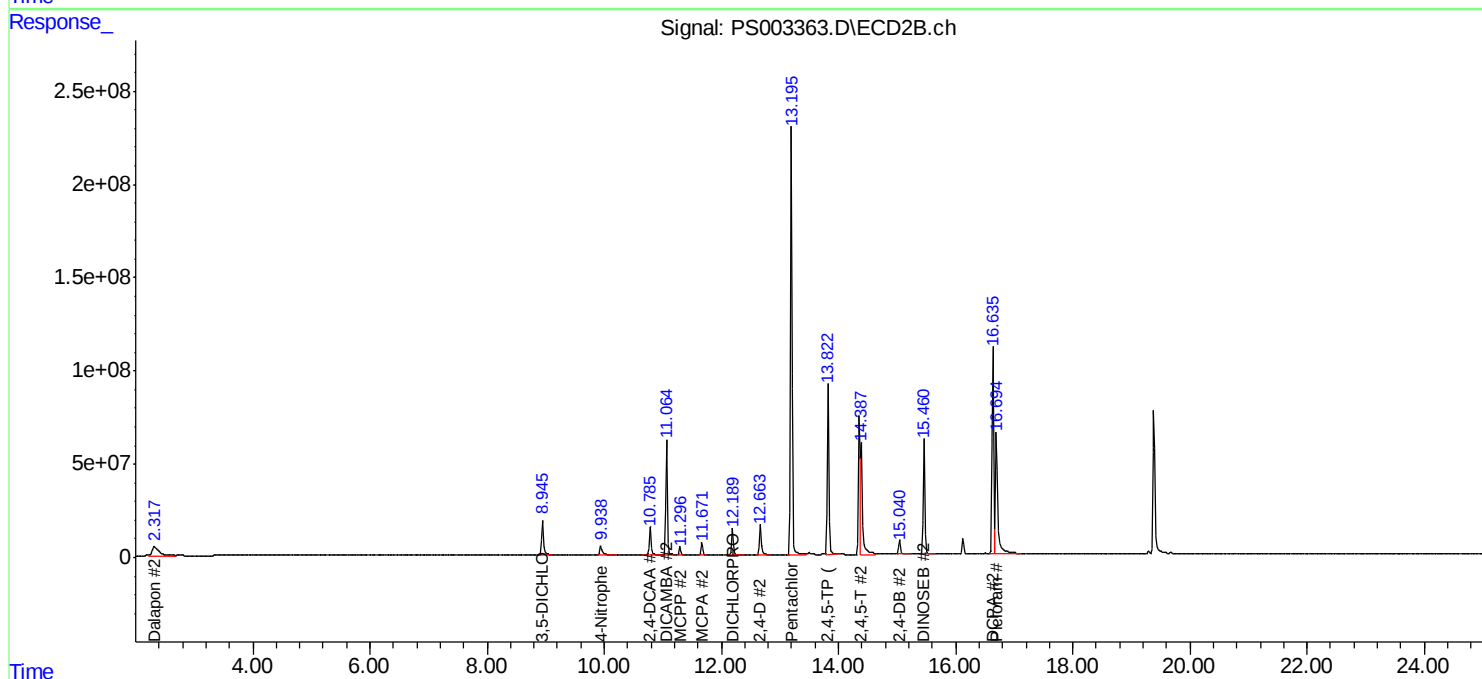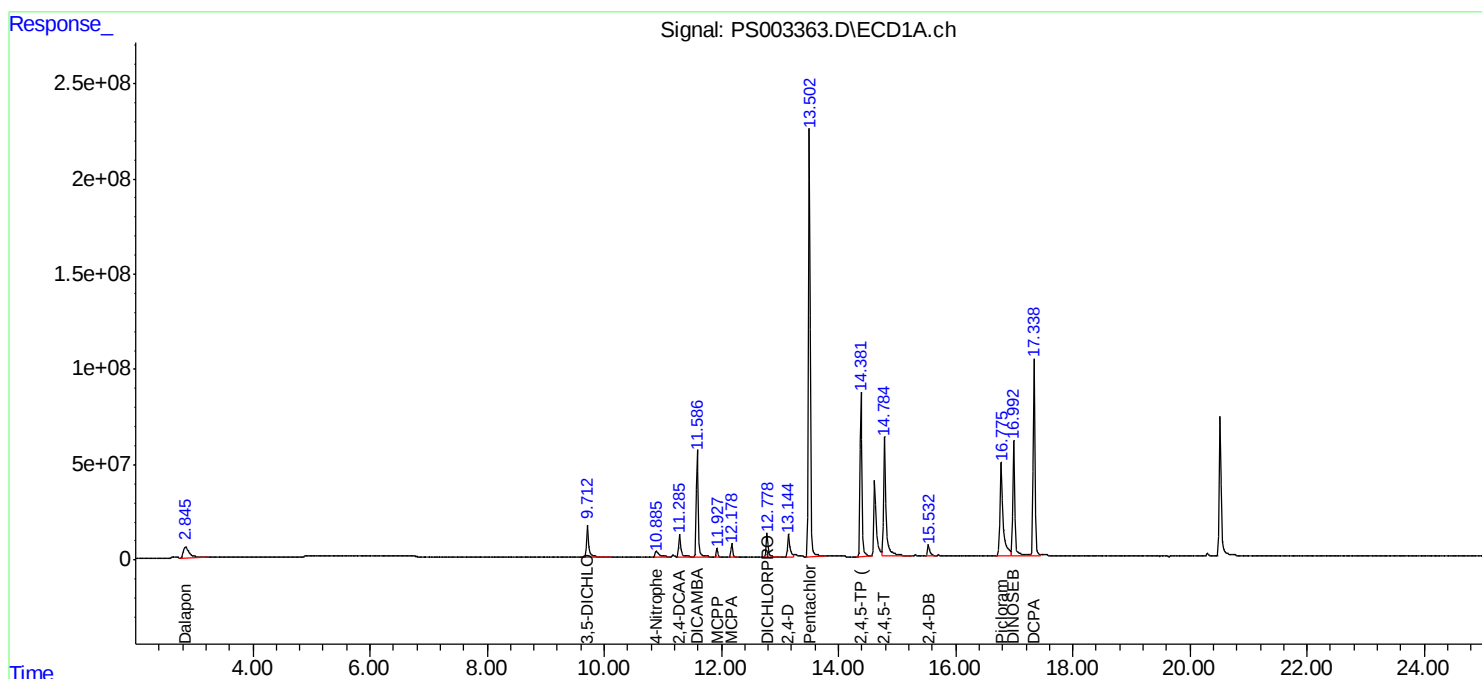


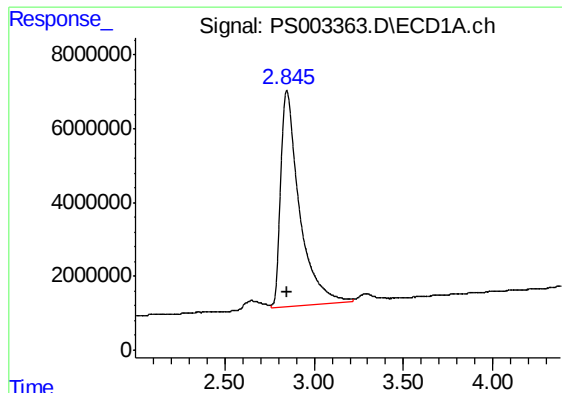

#1 Dalapon


R.T.: 2.847 min
Delta R.T.: 0.000 min
Response: 426169259
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

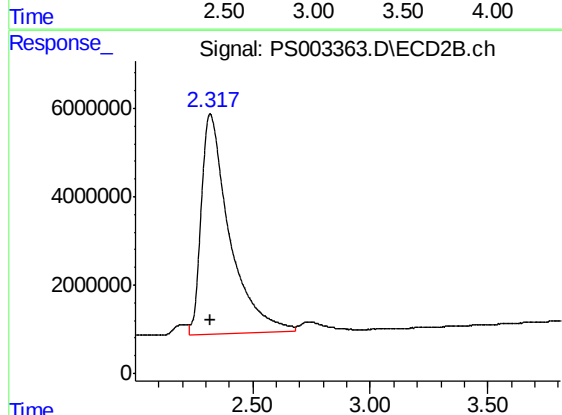


#1 Dalapon

R.T.: 2.318 min
Delta R.T.: 0.000 min
Response: 413842830
Conc: 682.50 ng/ml

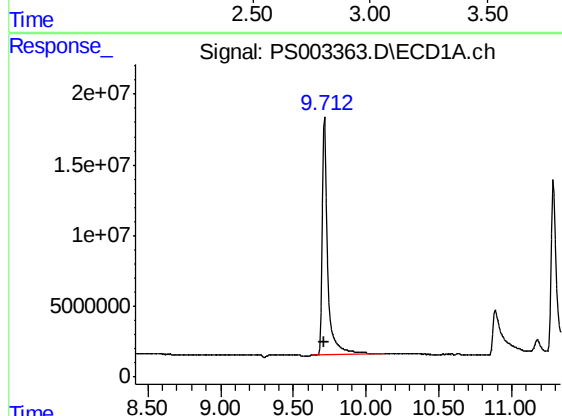


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.712 min
Delta R.T.: 0.000 min
Response: 441036964
Conc: 697.50 ng/ml

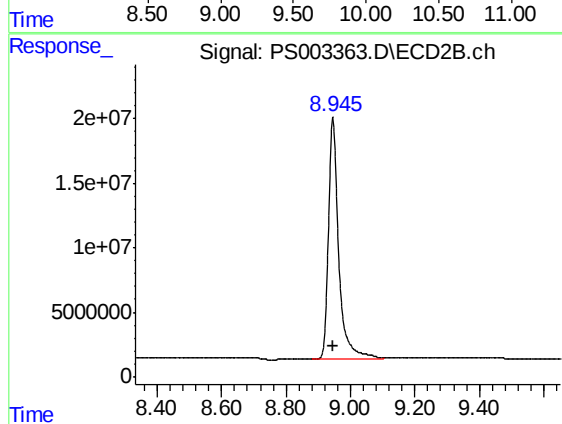

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.945 min
Delta R.T.: 0.000 min
Response: 411555463
Conc: 697.50 ng/ml

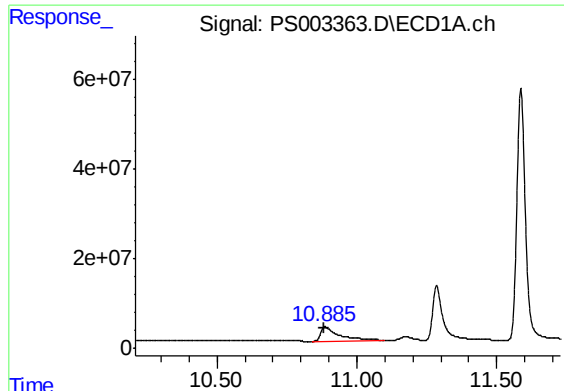

#3 4-Nitrophenol


R.T.: 10.885 min
Delta R.T.: 0.000 min
Response: 150949101
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

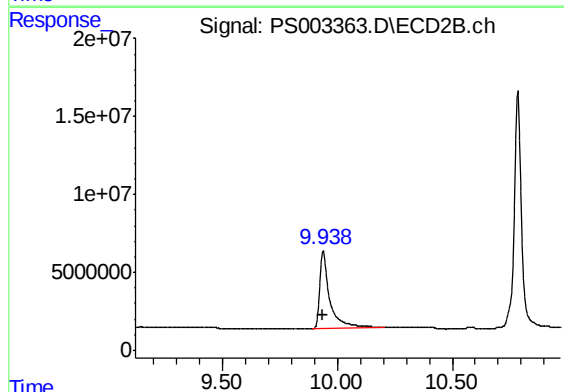


#3 4-Nitrophenol

R.T.: 9.938 min
Delta R.T.: 0.000 min
Response: 149067510
Conc: 682.50 ng/ml

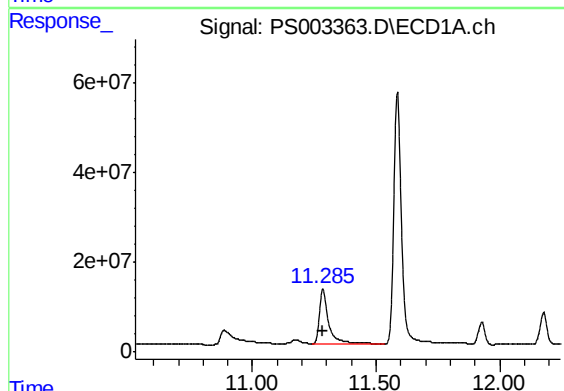


#4 2,4-DCAA

R.T.: 11.285 min
Delta R.T.: 0.000 min
Response: 318168641
Conc: 750.00 ng/ml

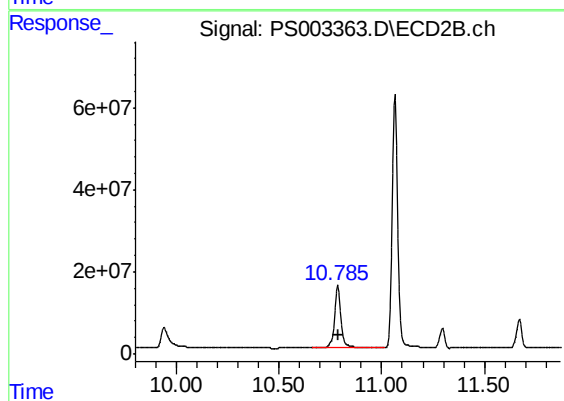

#4 2,4-DCAA


R.T.: 10.785 min
Delta R.T.: 0.000 min
Response: 335490309
Conc: 750.00 ng/ml

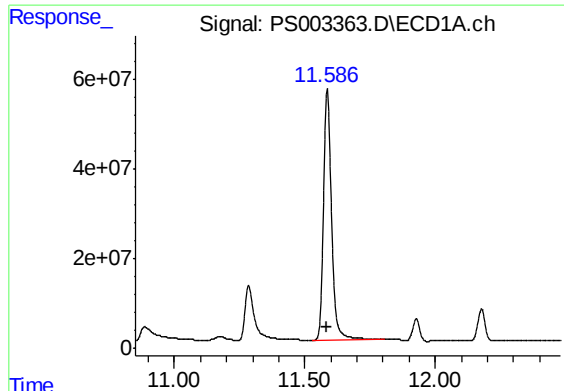

#5 DICAMBA


R.T.: 11.586 min
Delta R.T.: 0.000 min
Response: 1203410843
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

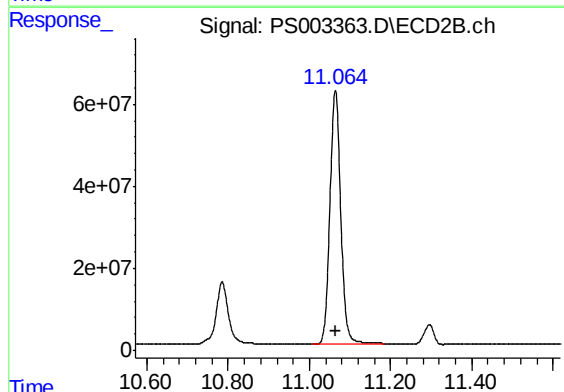


#5 DICAMBA

R.T.: 11.064 min
Delta R.T.: 0.000 min
Response: 1139352410
Conc: 705.00 ng/ml

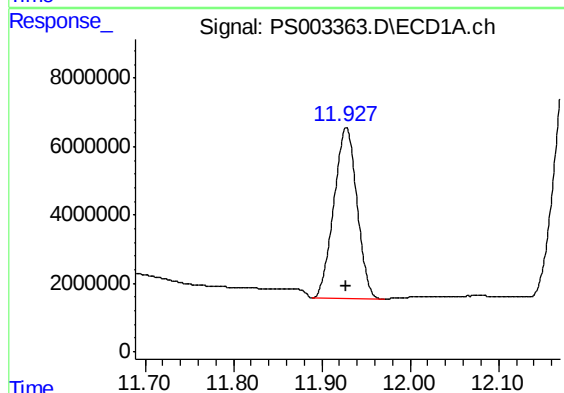


#6 MCPP

R.T.: 11.928 min
Delta R.T.: 0.000 min
Response: 90953995
Conc: 70.50 ug/ml

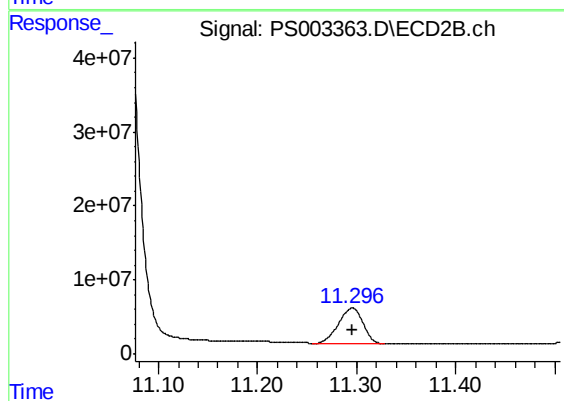

#6 MCPP


R.T.: 11.296 min
Delta R.T.: 0.000 min
Response: 81908746
Conc: 70.50 ug/ml

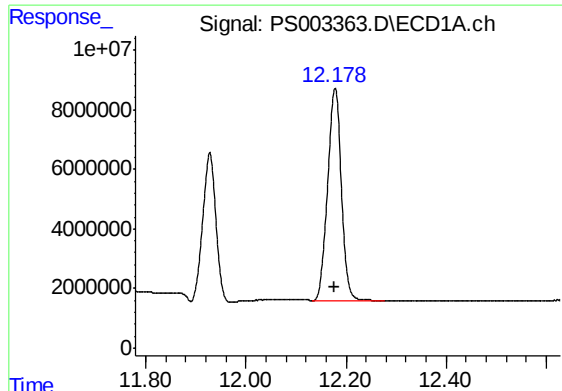

#7 MCPA


R.T.: 12.178 min
Delta R.T.: 0.000 min
Response: 135482826
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

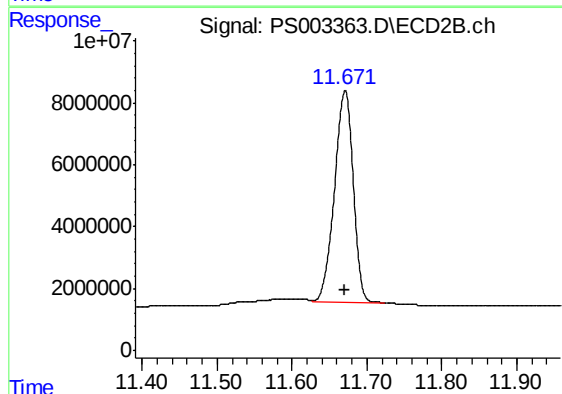


#7 MCPA

R.T.: 11.671 min
Delta R.T.: 0.000 min
Response: 118399832
Conc: 69.75 ug/ml

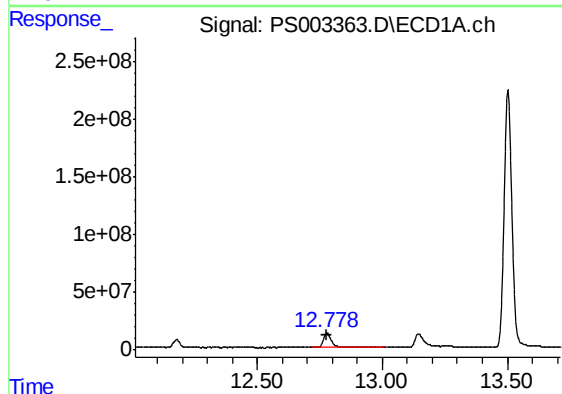


#8 DICHLORPROP

R.T.: 12.779 min
Delta R.T.: 0.000 min
Response: 290506151
Conc: 705.00 ng/ml

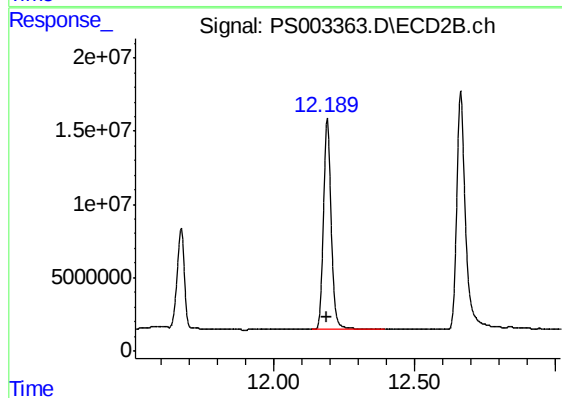

#8 DICHLORPROP


R.T.: 12.190 min
Delta R.T.: 0.000 min
Response: 277566982
Conc: 705.00 ng/ml

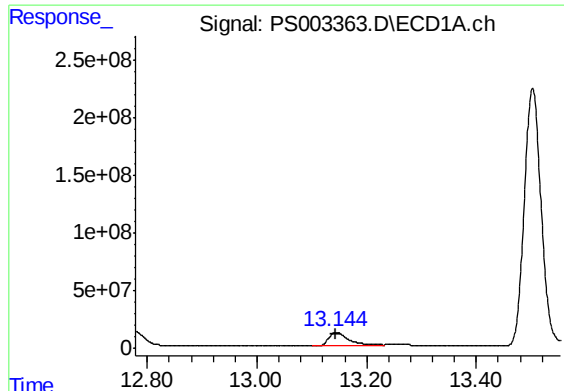

#9 2,4-D


R.T.: 13.144 min
Delta R.T.: 0.000 min
Response: 322660947
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

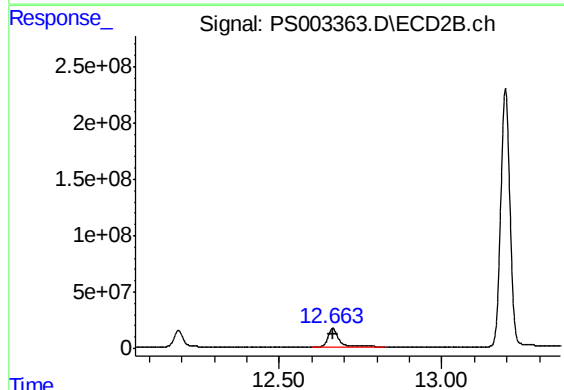


#9 2,4-D

R.T.: 12.664 min
Delta R.T.: 0.000 min
Response: 356546052
Conc: 705.00 ng/ml

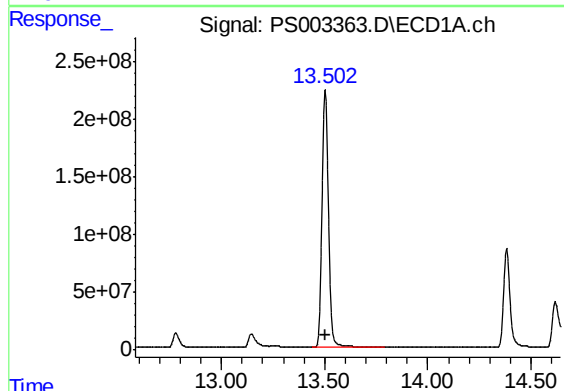


#10 Pentachlorophenol

R.T.: 13.503 min
Delta R.T.: 0.000 min
Response: 4903148144
Conc: 712.50 ng/ml

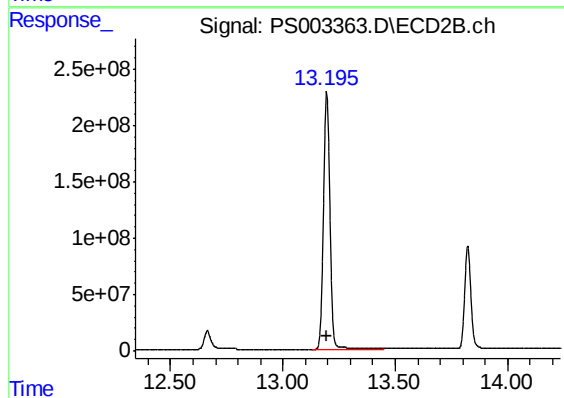

#10 Pentachlorophenol


R.T.: 13.195 min
Delta R.T.: 0.000 min
Response: 4559064849
Conc: 712.50 ng/ml

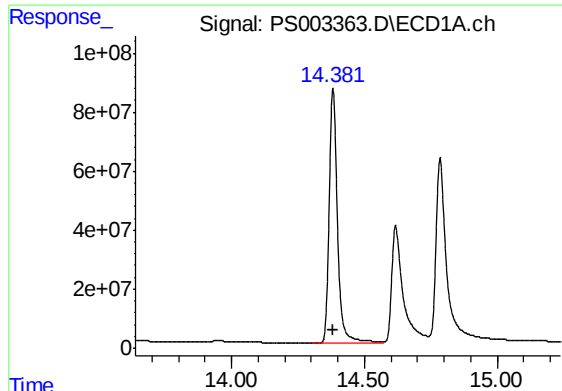

#11 2,4,5-TP (SILVEX)


R.T.: 14.381 min
Delta R.T.: 0.000 min
Response: 1866940185
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

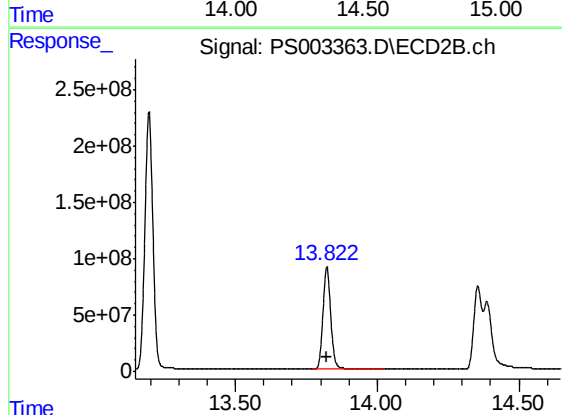


#11 2,4,5-TP (SILVEX)

R.T.: 13.822 min
Delta R.T.: 0.000 min
Response: 1759777964
Conc: 712.50 ng/ml

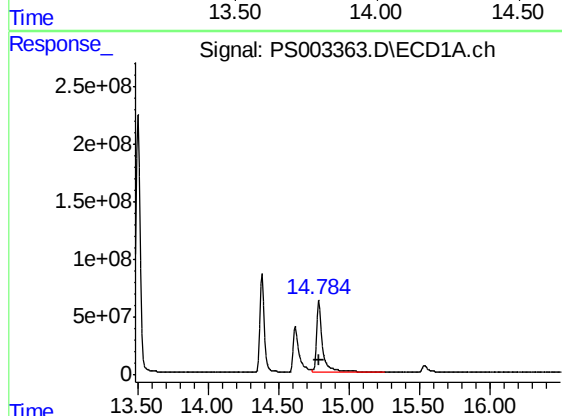


#12 2,4,5-T

R.T.: 14.785 min
Delta R.T.: 0.000 min
Response: 1843968492
Conc: 712.50 ng/ml

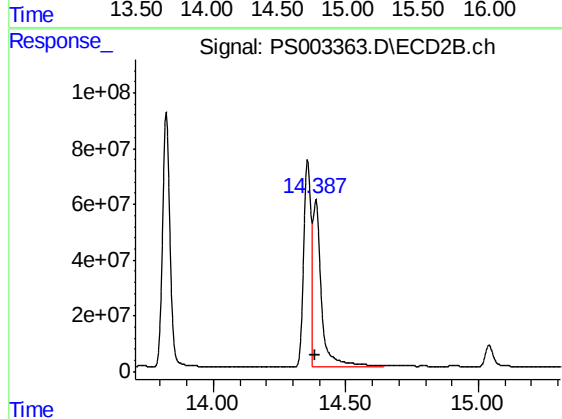

#12 2,4,5-T


R.T.: 14.387 min
Delta R.T.: 0.000 min
Response: 1377224591
Conc: 712.50 ng/ml

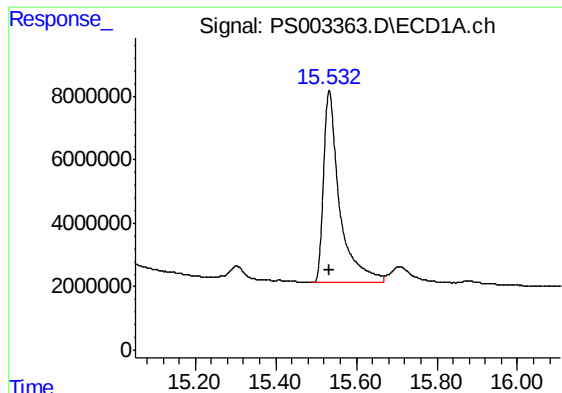

#13 2,4-DB


R.T.: 15.533 min
Delta R.T.: 0.000 min
Response: 169216621
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

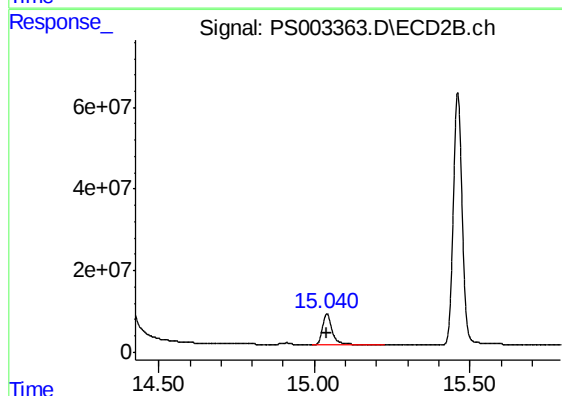


#13 2,4-DB

R.T.: 15.040 min
Delta R.T.: 0.000 min
Response: 179292975
Conc: 712.50 ng/ml

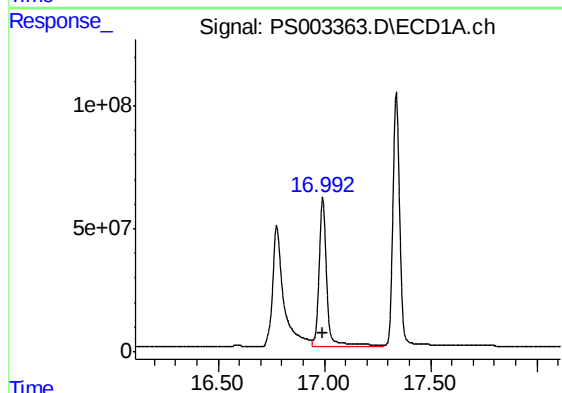


#14 DINOSEB

R.T.: 16.992 min
Delta R.T.: 0.000 min
Response: 1543587877
Conc: 705.00 ng/ml

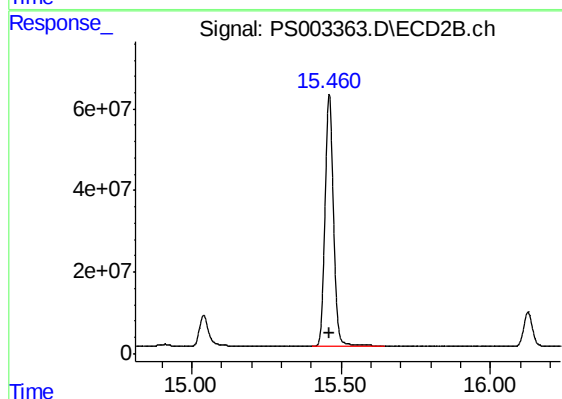

#14 DINOSEB


R.T.: 15.461 min
Delta R.T.: 0.000 min
Response: 1213321188
Conc: 705.00 ng/ml

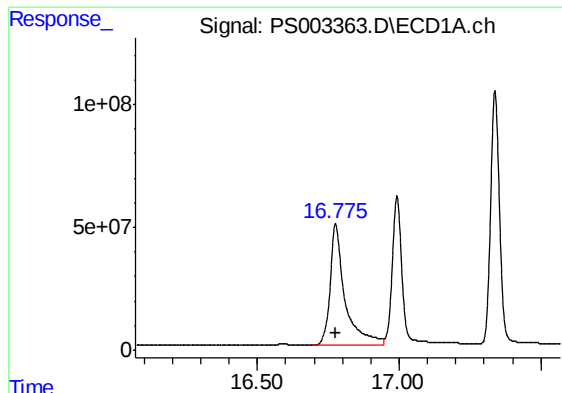

#15 Picloram


R.T.: 16.776 min
Delta R.T.: 0.000 min
Response: 1801034529
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

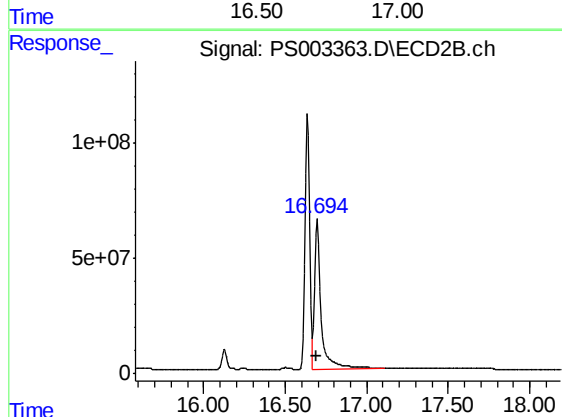


#15 Picloram

R.T.: 16.695 min
Delta R.T.: 0.000 min
Response: 1789346312
Conc: 712.50 ng/ml

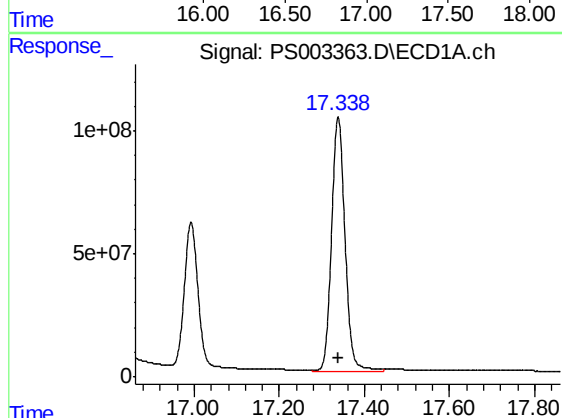

#16 DCPA

R.T.: 17.338 min
Delta R.T.: 0.000 min
Response: 2287332165
Conc: 720.00 ng/ml

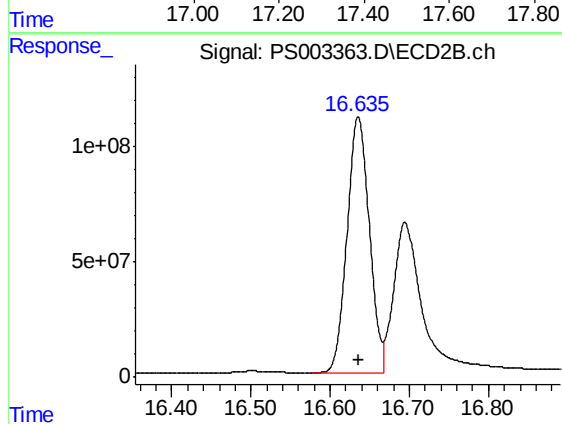

#16 DCPA

R.T.: 16.636 min
Delta R.T.: 0.000 min
Response: 2171734403
Conc: 720.00 ng/ml