

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 11:12
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:32:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.250	6.939	929.0E6	490.7E6	424.851	509.265
Target Compounds							
5) T	DICAMBA	0.000	7.109	0	8637527	N.D.	2.087
10) T	Pentachlo...	0.000	8.465	0	16372137	N.D.	1.152
11) T	2,4,5-TP ...	0.000	8.828	0	13503283	N.D.	2.493
12) T	2,4,5-T	0.000	9.208	0	24459822	N.D.	4.519
15) T	Picloram	11.048	11.032	325.6E6	198.7E6	23.779	27.342
16) T	DCPA	0.000	10.982	0	19020357	N.D.	2.749



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 11:12
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:32:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

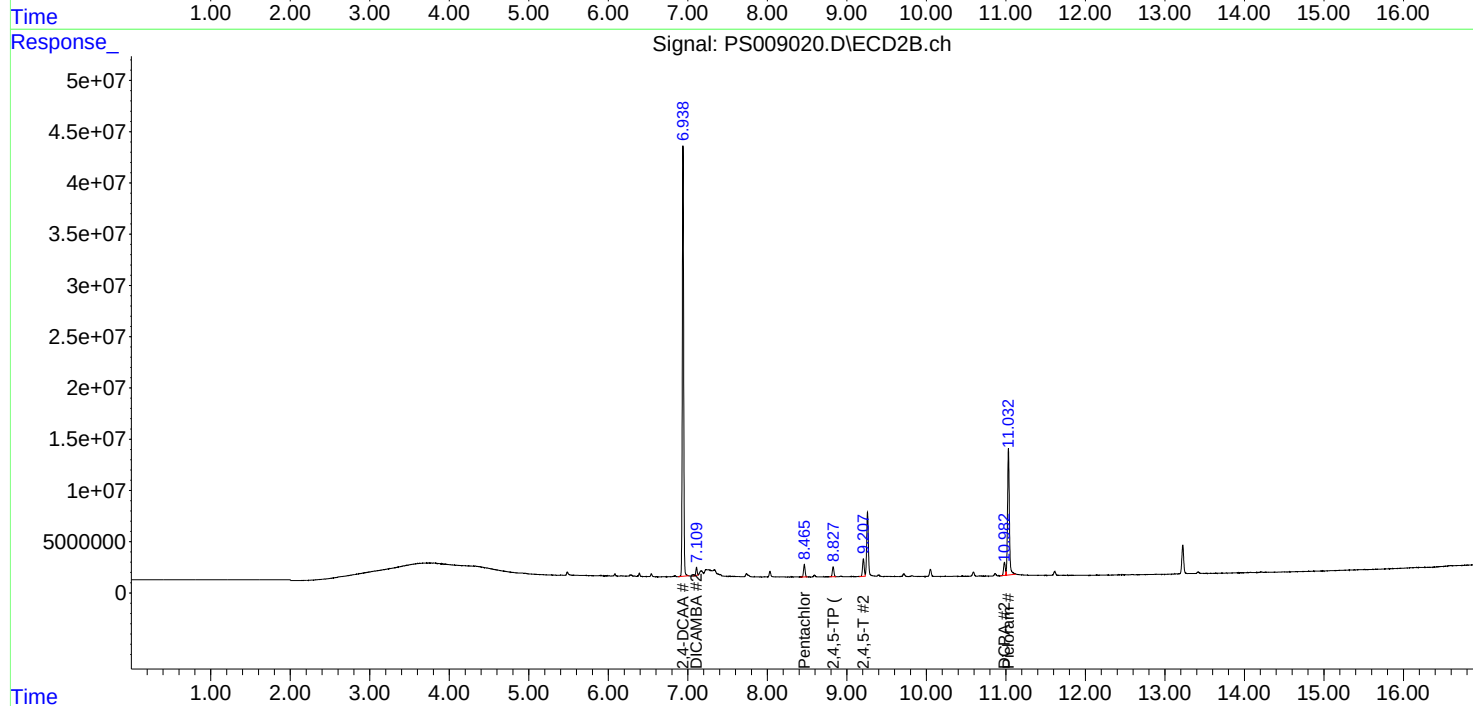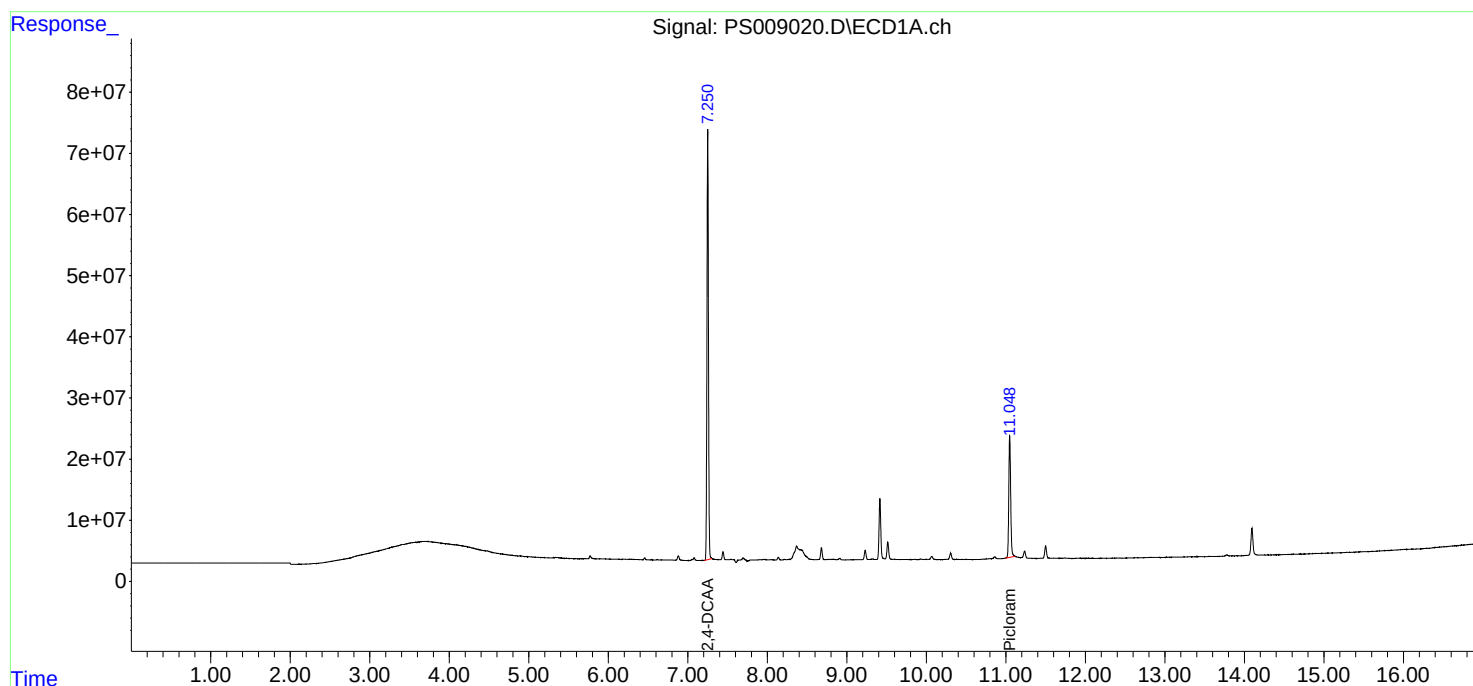


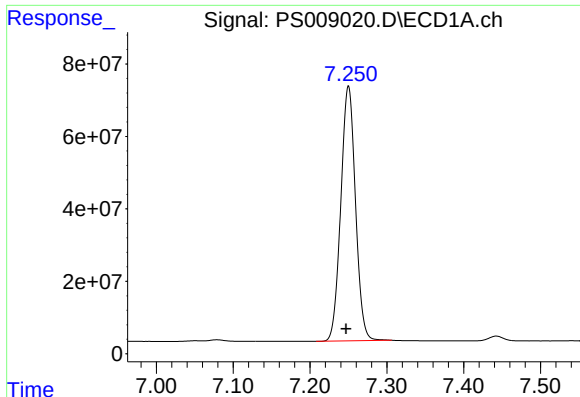

#4 2,4-DCAA


R.T.: 7.250 min
Delta R.T.: 0.003 min
Response: 928976883
Conc: 424.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

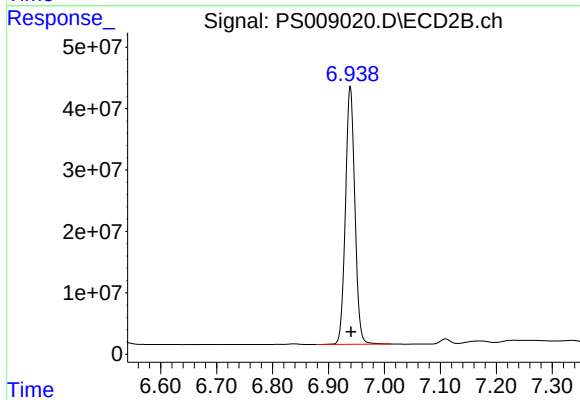


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 490704913
Conc: 509.26 ng/ml

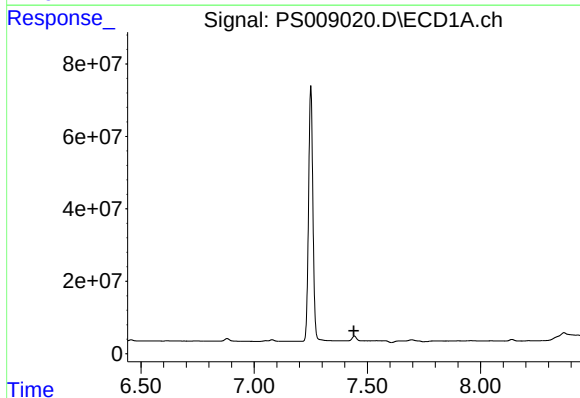


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

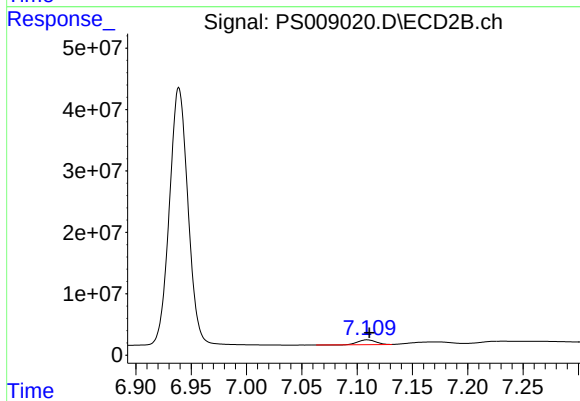

#5 DICAMBA


R.T.: 7.109 min
Delta R.T.: -0.002 min
Response: 8637527
Conc: 2.09 ng/ml

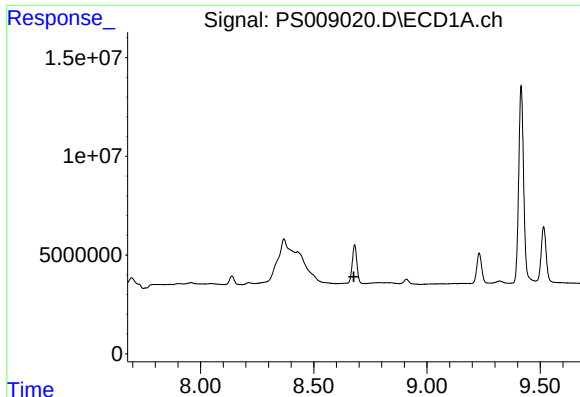

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

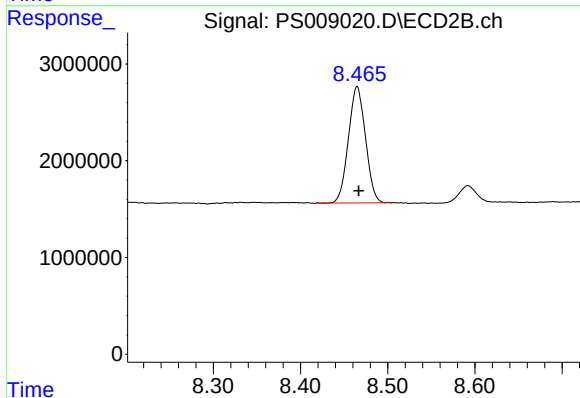


#10 Pentachlorophenol

R.T.: 8.465 min
Delta R.T.: -0.002 min
Response: 16372137
Conc: 1.15 ng/ml

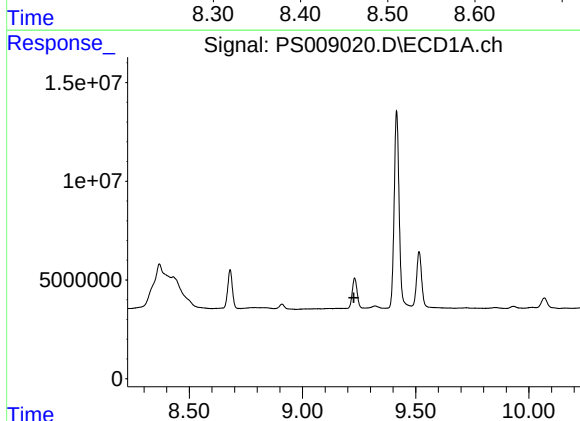


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

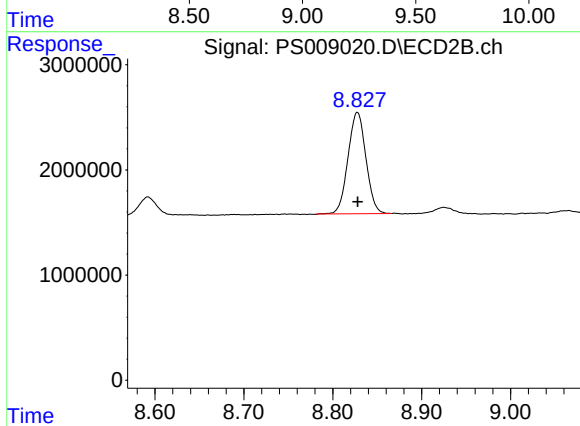

#11 2,4,5-TP (SILVEX)


R.T.: 8.828 min
Delta R.T.: 0.000 min
Response: 13503283
Conc: 2.49 ng/ml

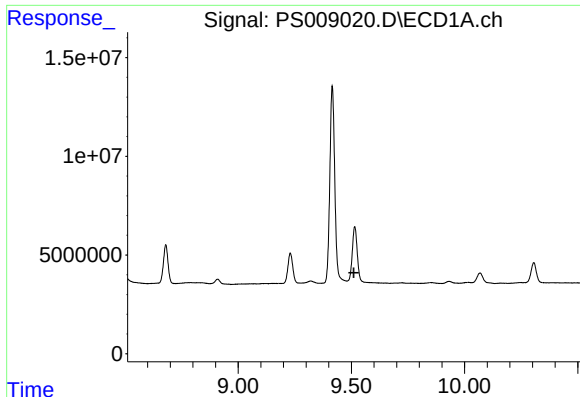

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

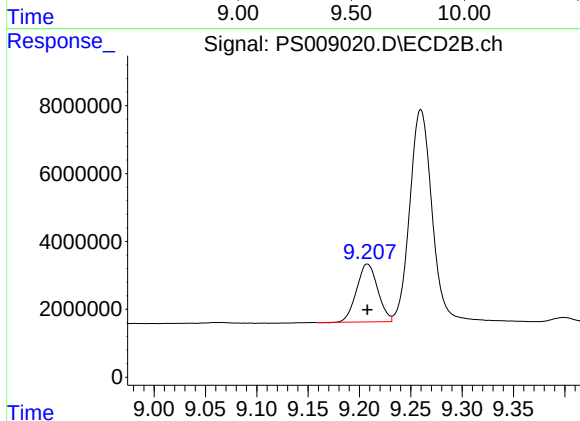


#12 2,4,5-T

R.T.: 9.208 min
Delta R.T.: 0.000 min
Response: 24459822
Conc: 4.52 ng/ml

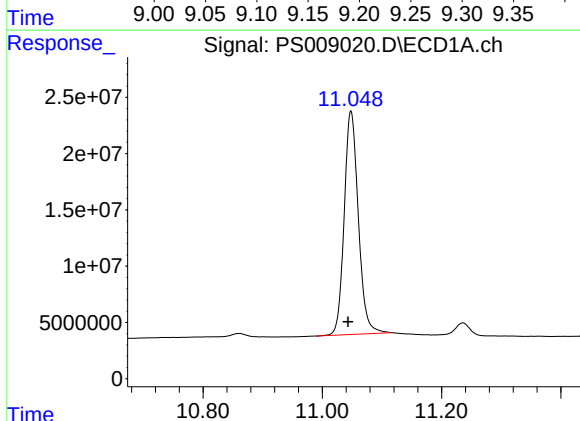


#15 Picloram

R.T.: 11.048 min
Delta R.T.: 0.005 min
Response: 325555605
Conc: 23.78 ng/ml

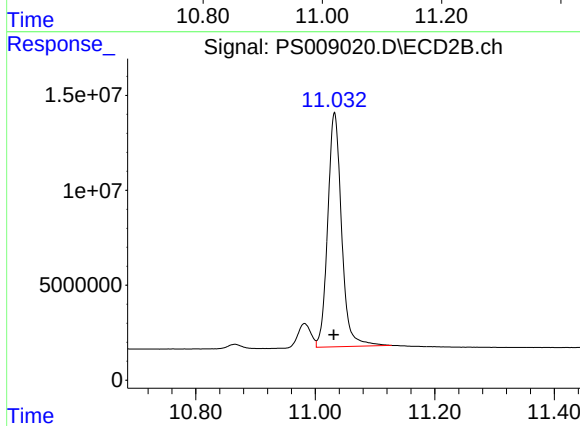

#15 Picloram


R.T.: 11.032 min
Delta R.T.: 0.001 min
Response: 198680135
Conc: 27.34 ng/ml

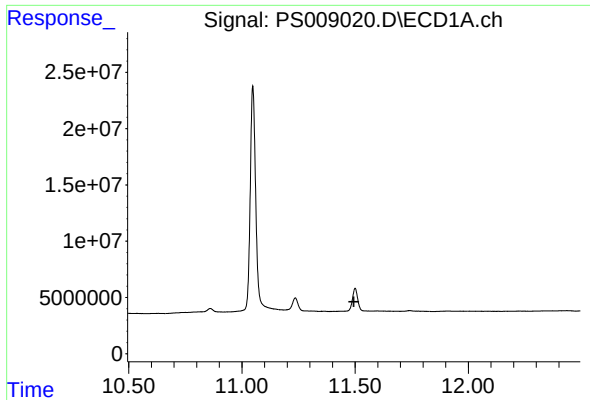

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

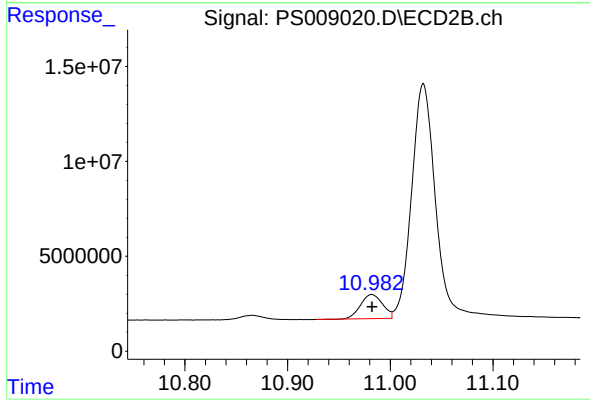

#16 DCPA

R.T.: 10.982 min
Delta R.T.: 0.000 min
Response: 19020357
Conc: 2.75 ng/ml