

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 15:28
 Operator : DD\AJ
 Sample : PB127126BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:33:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.940	1069.1E6	542.6E6	488.933	563.125
Target Compounds							
1) T	Dalapon	0.000	2.592	0 41869388		N.D.	28.634
2) T	3,5-DICHL...	0.000	6.114	0 96203143		N.D.	65.926
7) T	MCPA	7.800	7.408	277.5E6	161.0E6	34.500	36.387
8) T	DICHLORPROP	0.000	7.760	0 79098679		N.D.	78.946
11) T	2,4,5-TP ...	0.000	8.795	0 51427592		N.D.	9.494
12) T	2,4,5-T	9.455	9.259	67881333	75730275	6.349	13.990 #
14) T	DINOSEB	0.000	10.053	0 37400433		N.D.	9.459
15) T	Picloram	11.044	11.031	547.4E6	337.2E6	39.982	46.411
16) T	DCPA	0.000	10.982	0 20679728		N.D.	2.989



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 15:28
Operator : DD\AJ
Sample : PB127126BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:33:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

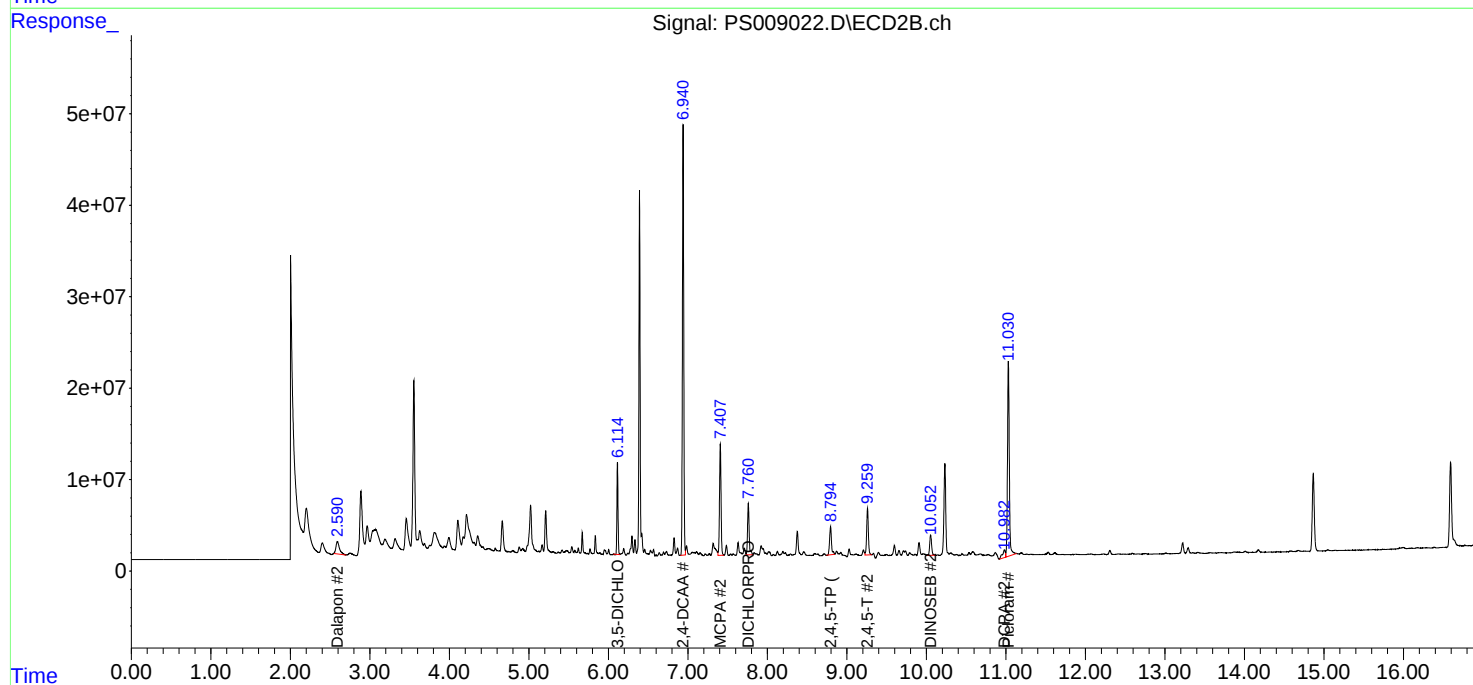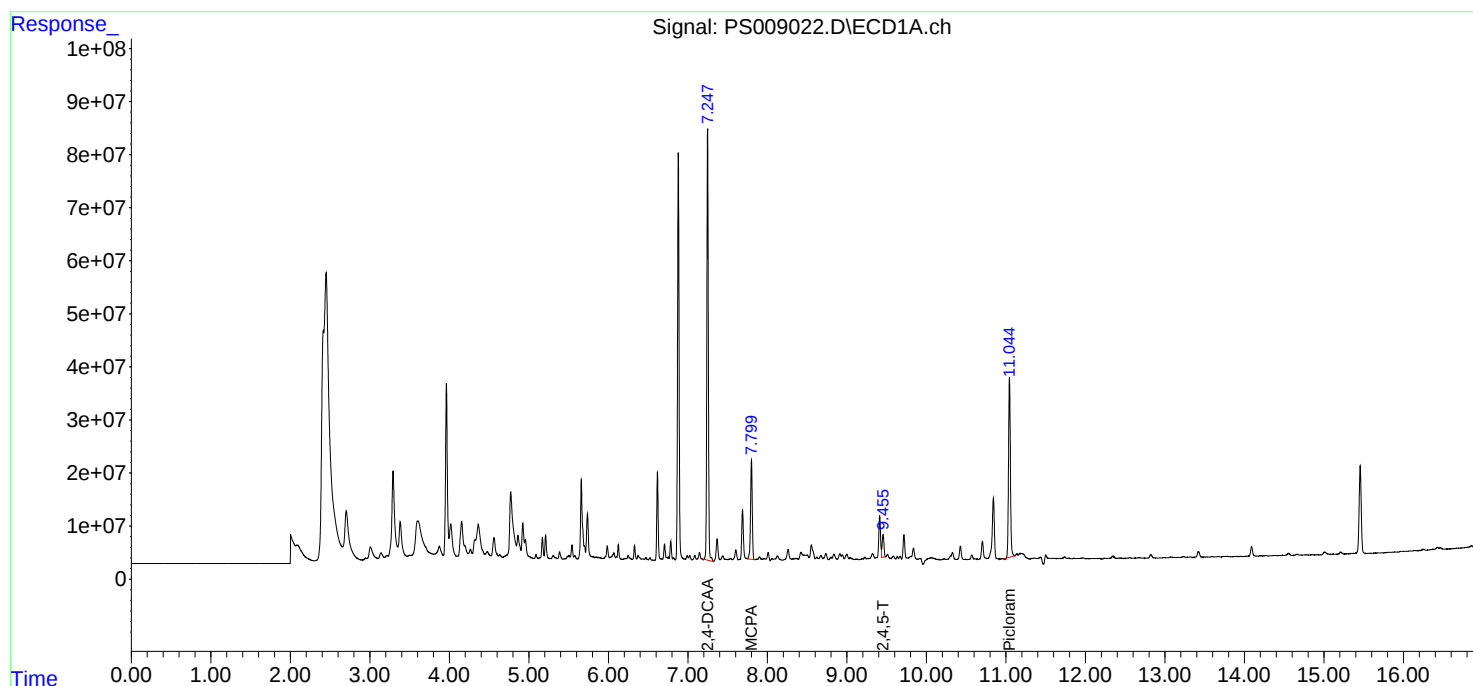


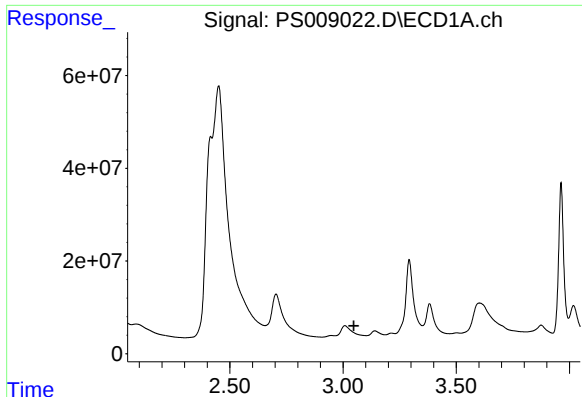

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

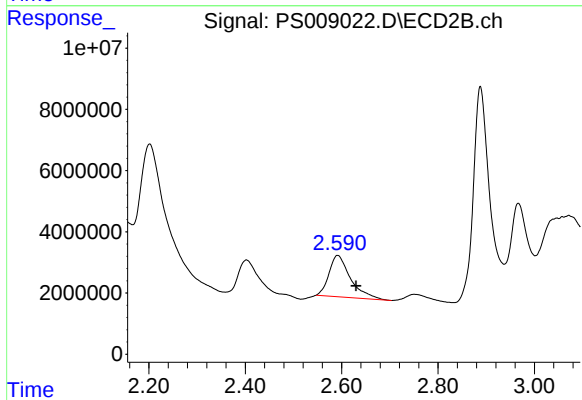


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 41869388
Conc: 28.63 ng/ml

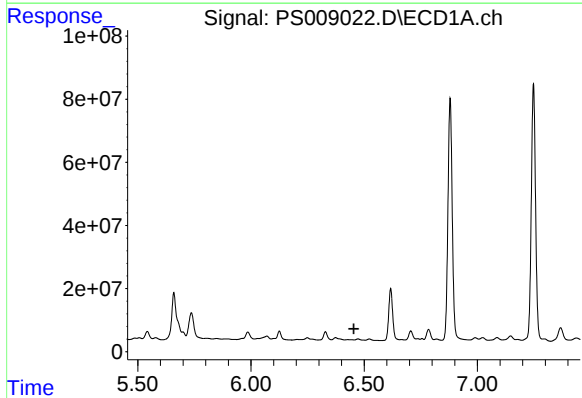


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

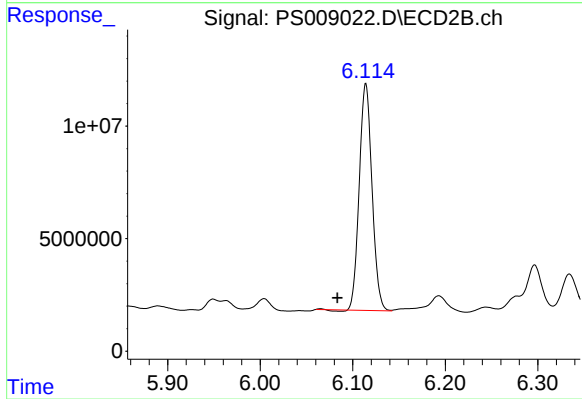

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 96203143
Conc: 65.93 ng/ml

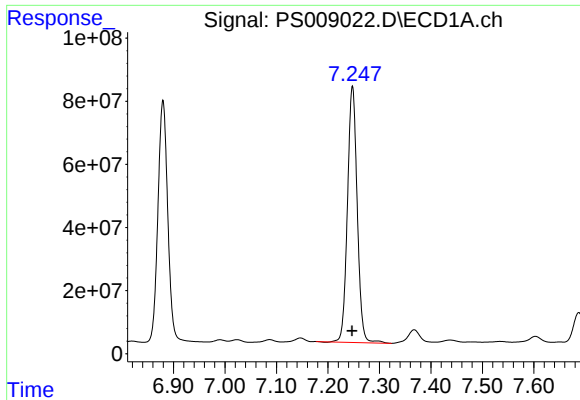

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: 0.000 min
Response: 1069097672
Conc: 488.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

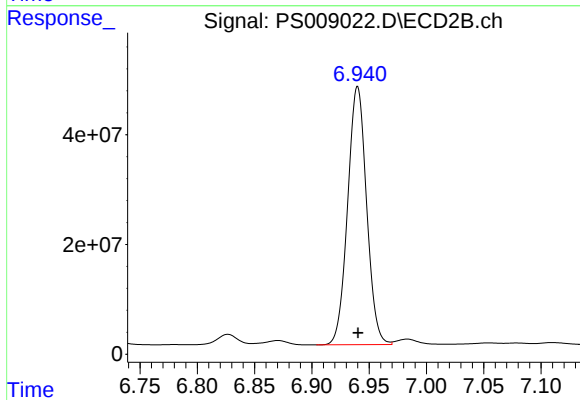


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 542602258
Conc: 563.13 ng/ml

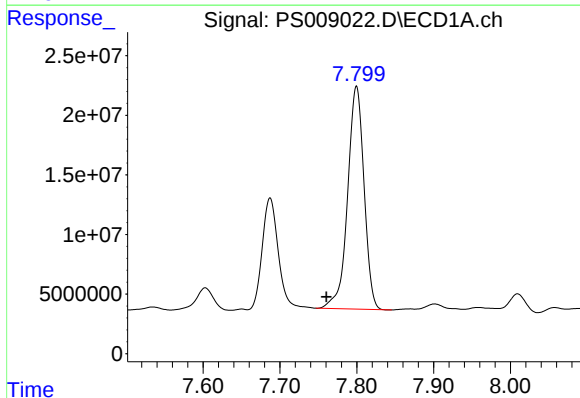


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 277520174
Conc: 34.50 ug/ml

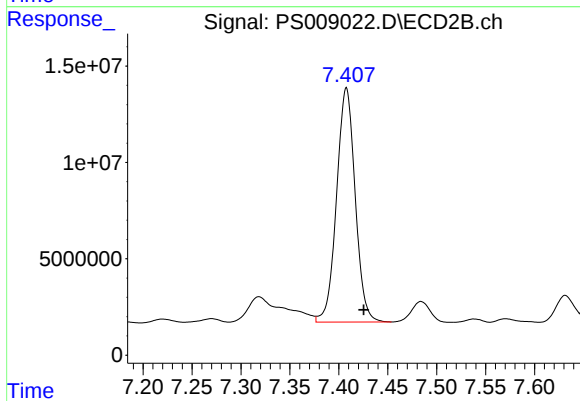

#7 MCPA


R.T.: 7.408 min
Delta R.T.: -0.018 min
Response: 160982734
Conc: 36.39 ug/ml

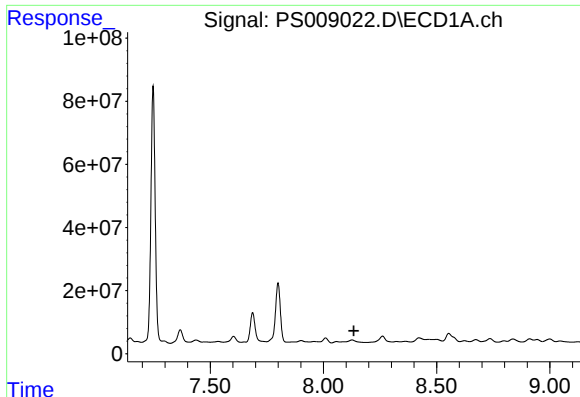

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

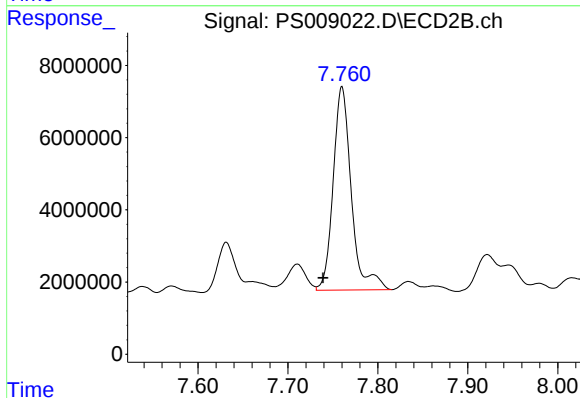


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 79098679
Conc: 78.95 ng/ml

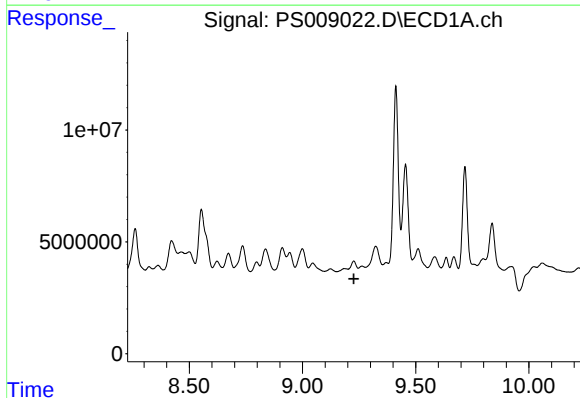


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

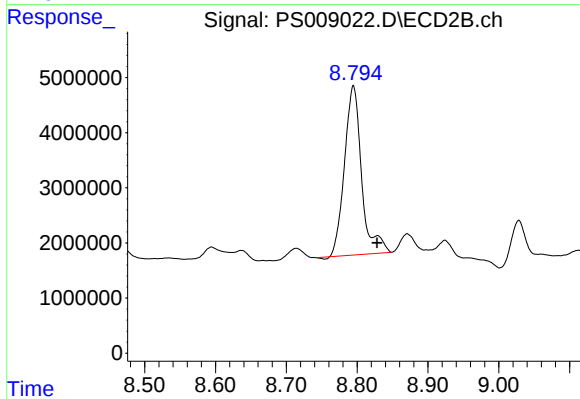

#11 2,4,5-TP (SILVEX)


R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 51427592
Conc: 9.49 ng/ml

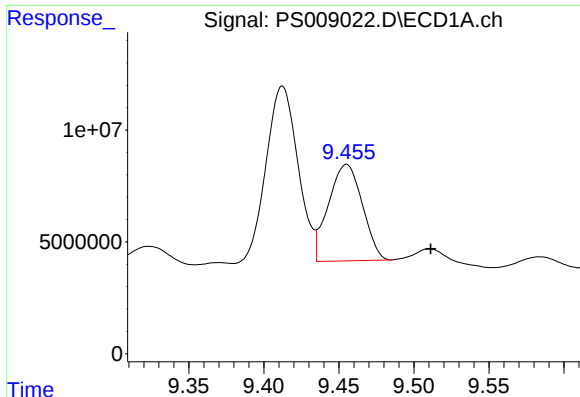

#12 2,4,5-T


R.T.: 9.455 min
Delta R.T.: -0.056 min
Response: 67881333
Conc: 6.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

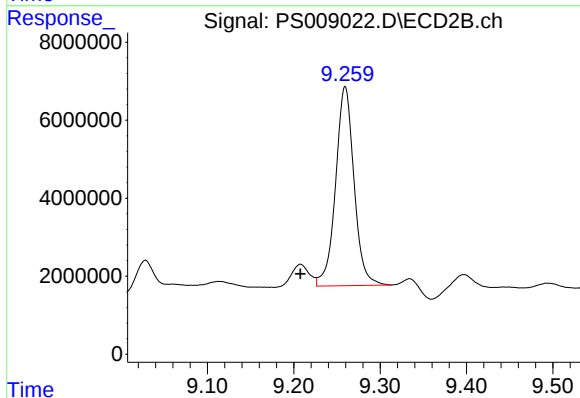


#12 2,4,5-T

R.T.: 9.259 min
Delta R.T.: 0.052 min
Response: 75730275
Conc: 13.99 ng/ml

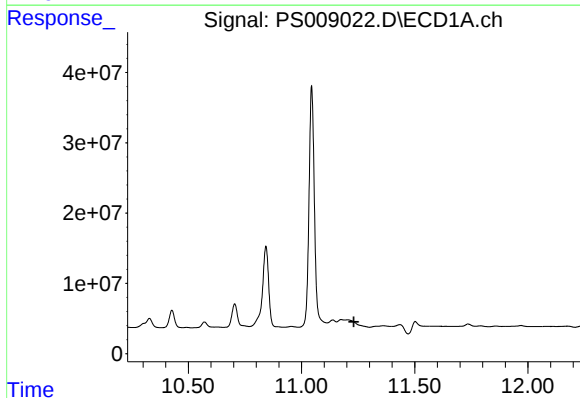


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

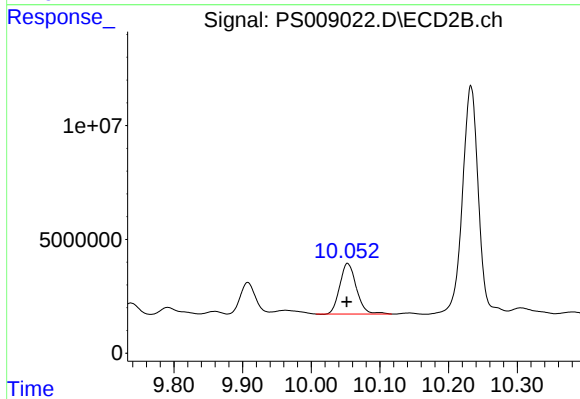

#14 DINOSEB


R.T.: 10.053 min
Delta R.T.: 0.002 min
Response: 37400433
Conc: 9.46 ng/ml

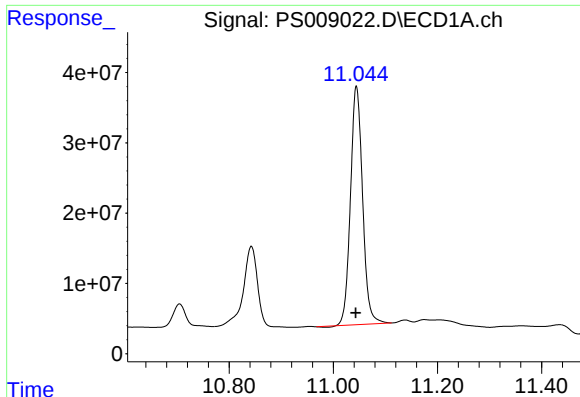

#15 Picloram


R.T.: 11.044 min
Delta R.T.: 0.001 min
Response: 547390268
Conc: 39.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

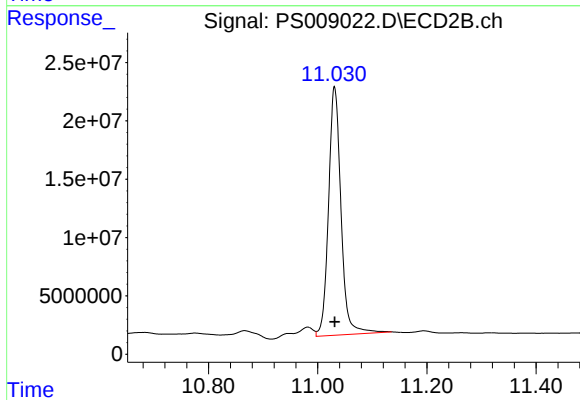


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 337246892
Conc: 46.41 ng/ml

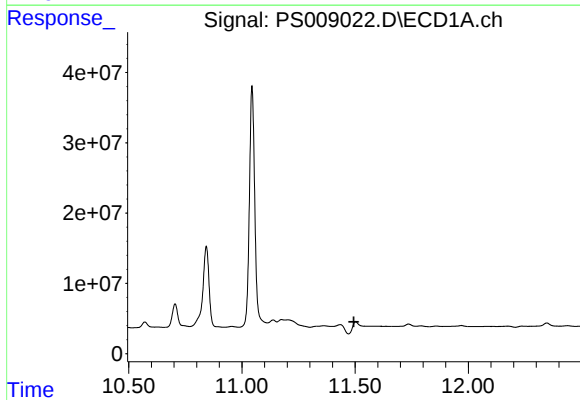

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

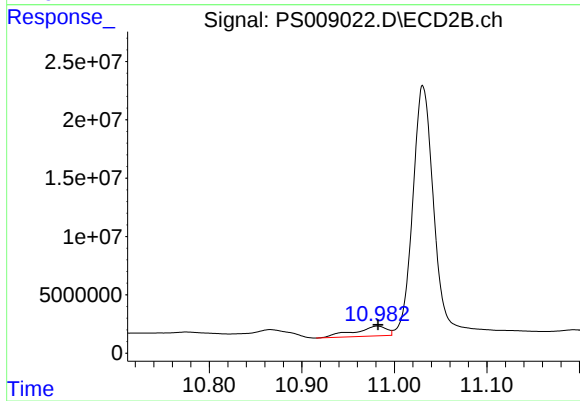

#16 DCPA

R.T.: 10.982 min
Delta R.T.: 0.000 min
Response: 20679728
Conc: 2.99 ng/ml