

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 16:13
 Operator : DD\AJ
 Sample : PB127126TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:33:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.940	646.4E6	320.1E6	295.641	332.226
Target Compounds							
1) T	Dalapon	0.000	2.592	0 48626323		N.D.	33.255
2) T	3,5-DICHL...	0.000	6.114	0 125.2E6		N.D.	85.817
8) T	DICHLORPROP	0.000	7.760	0 81347961		N.D.	81.191
10) T	Pentachlo...	0.000	8.465	0 18431335		N.D.	1.297
11) T	2,4,5-TP ...	0.000	8.784	0 85412000		N.D.	15.768
12) T	2,4,5-T	9.452	9.260	228.3E6	14561294	21.352	2.690 #
15) T	Picloram	0.000	11.031	0 27392576		N.D.	3.770
16) T	DCPA	0.000	11.031	0 27392576		N.D.	3.959



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 16:13
Operator : DD\AJ
Sample : PB127126TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:33:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

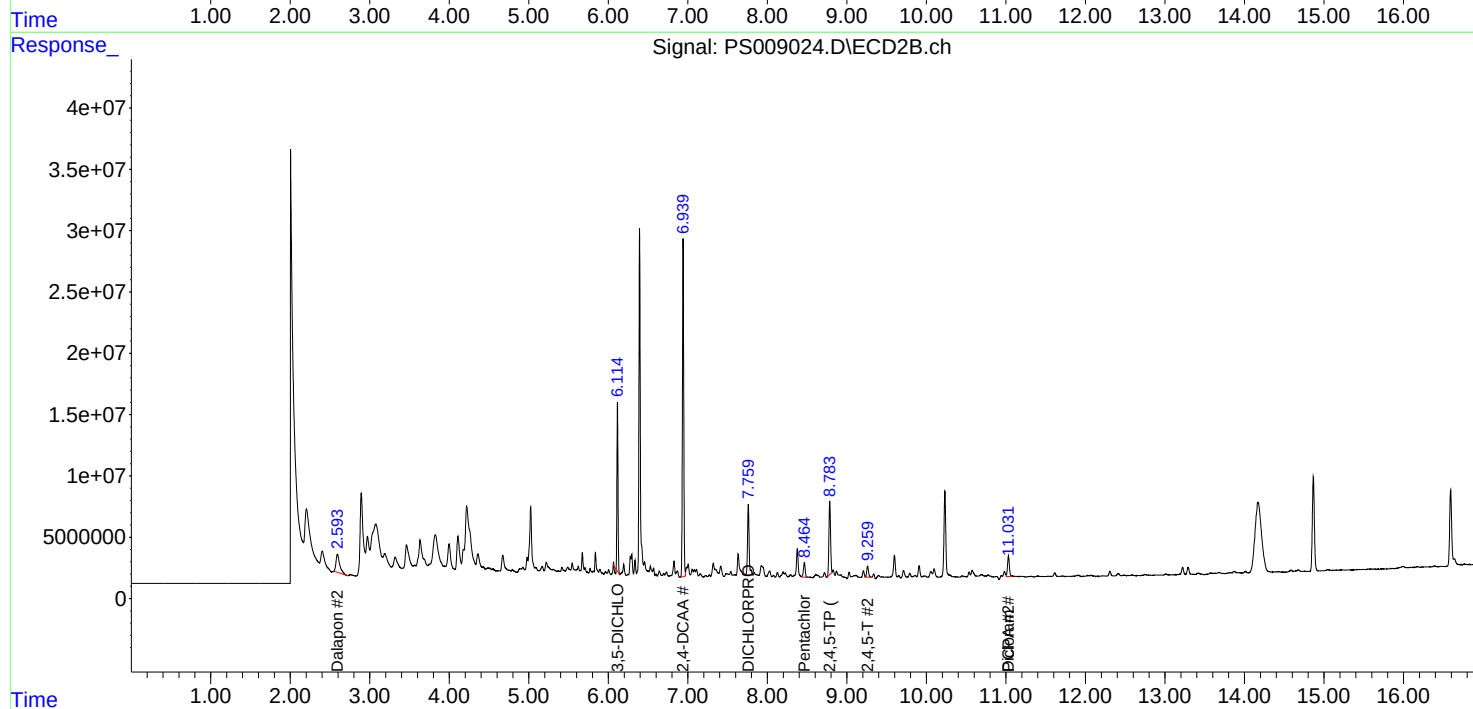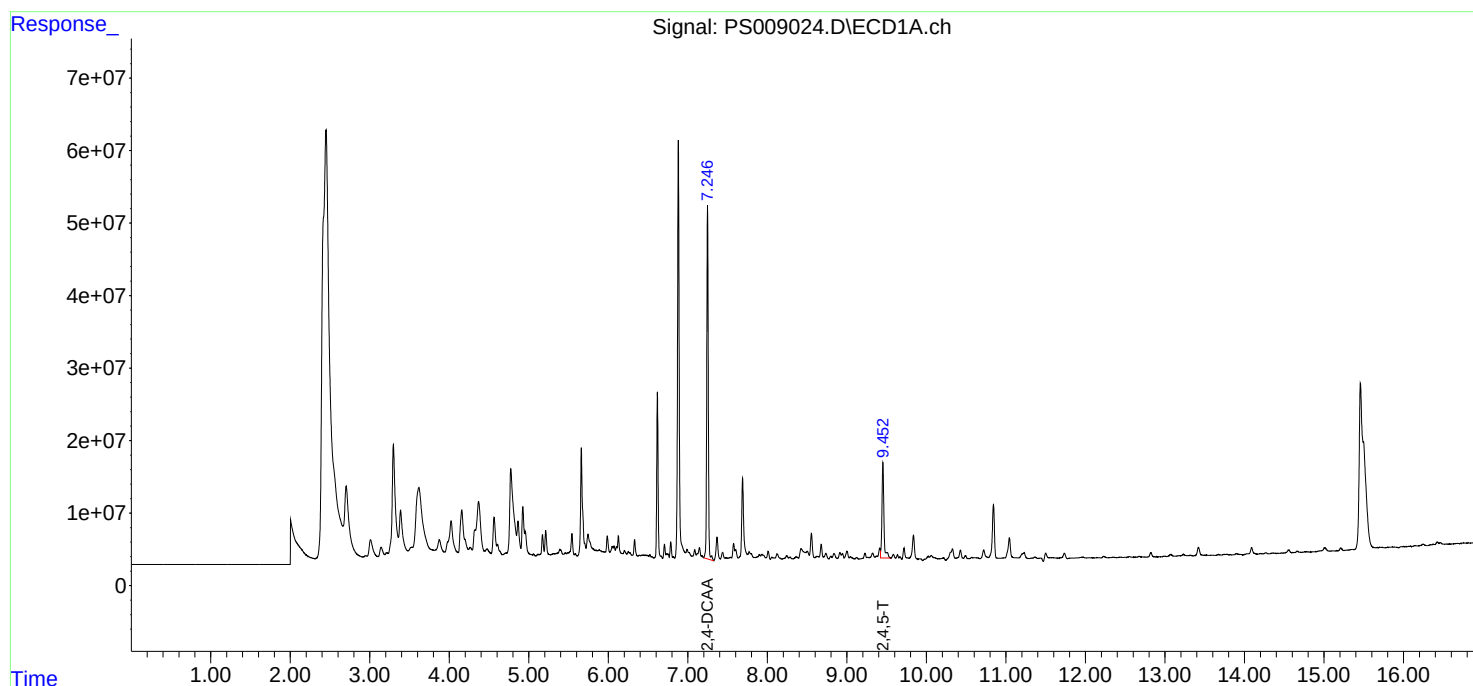


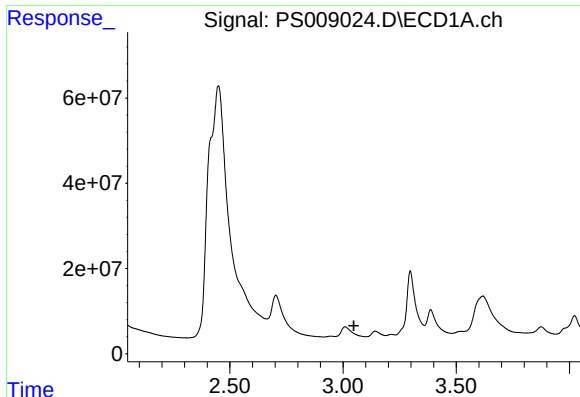

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

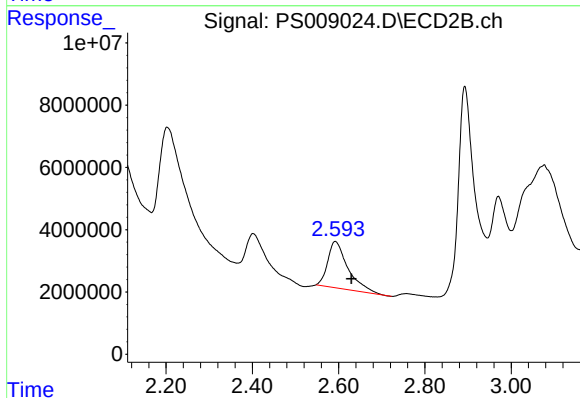


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 48626323
Conc: 33.26 ng/ml

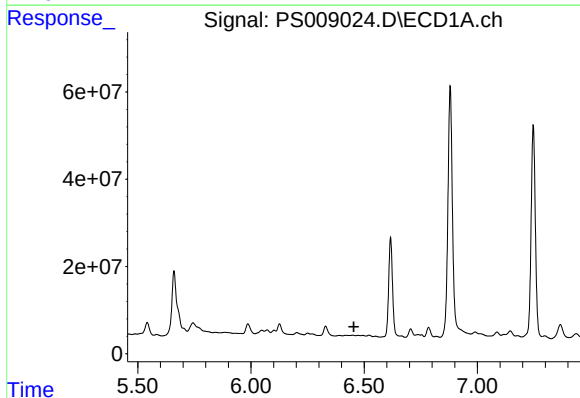


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

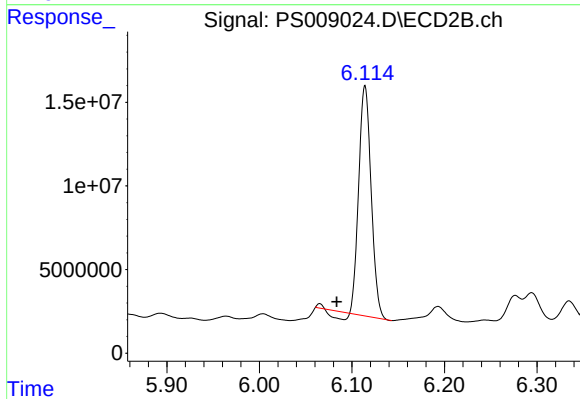

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 125230170
Conc: 85.82 ng/ml

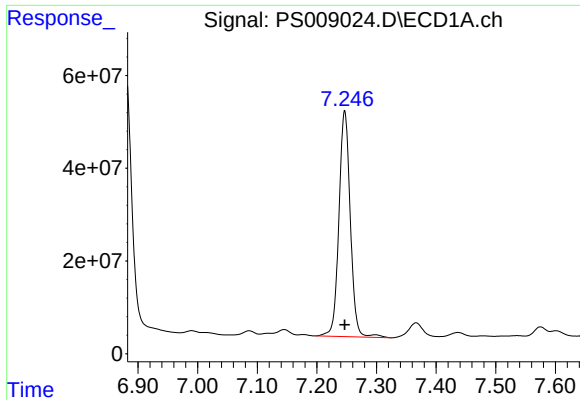

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 646446696
Conc: 295.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

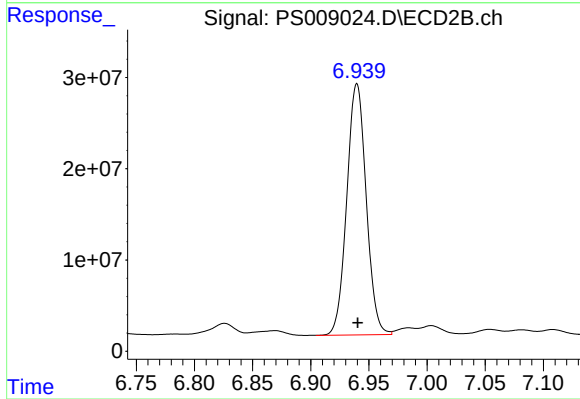


#4 2,4-DCAA

R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 320118119
Conc: 332.23 ng/ml

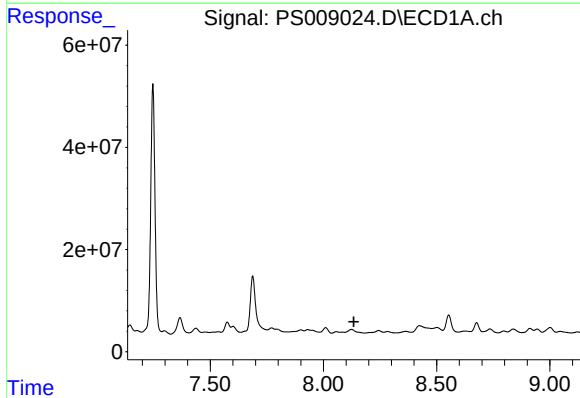


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

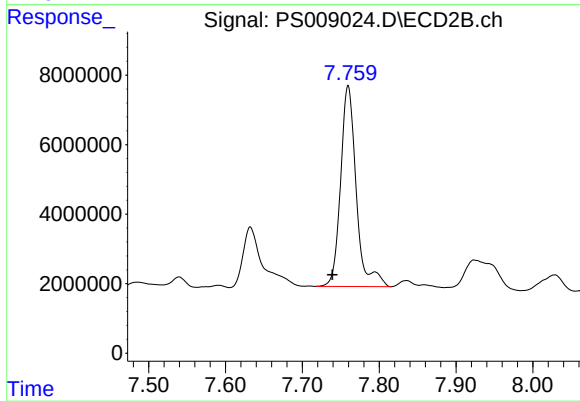

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.020 min
Response: 81347961
Conc: 81.19 ng/ml

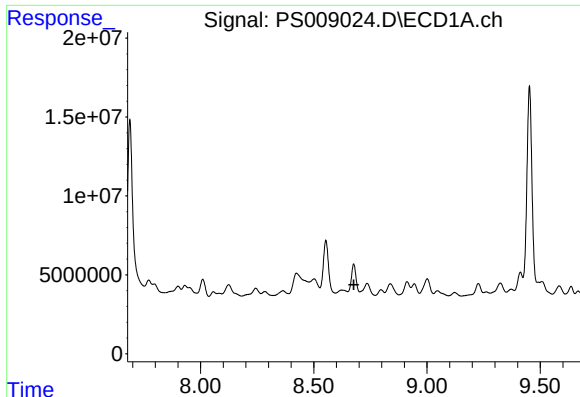

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

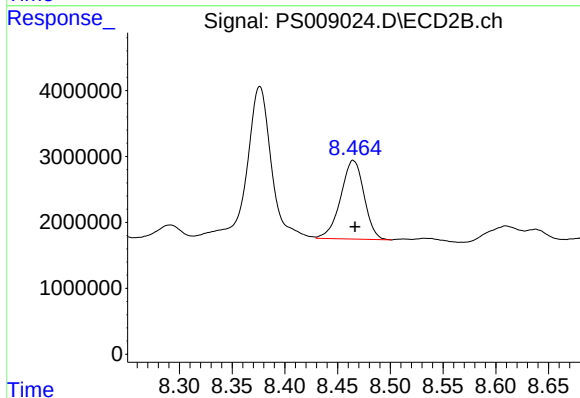


#10 Pentachlorophenol

R.T.: 8.465 min
Delta R.T.: -0.002 min
Response: 18431335
Conc: 1.30 ng/ml

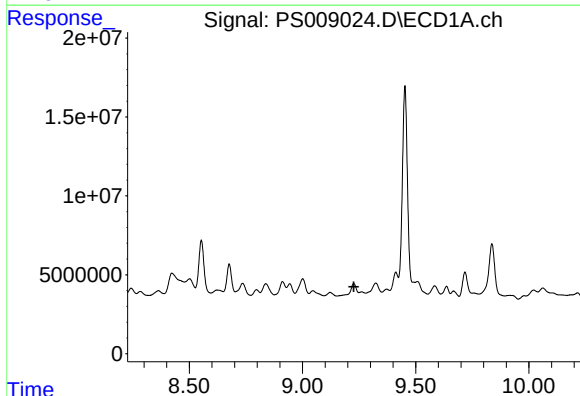


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

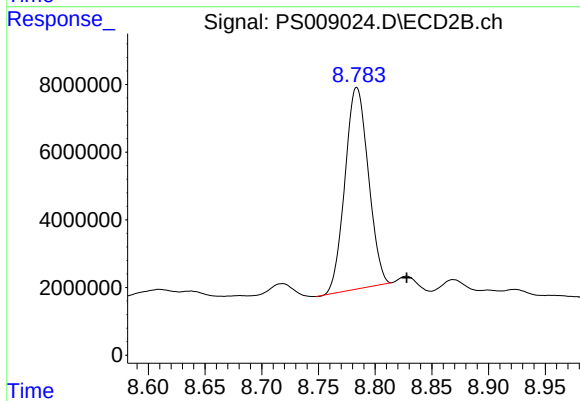

#11 2,4,5-TP (SILVEX)


R.T.: 8.784 min
Delta R.T.: -0.044 min
Response: 85412000
Conc: 15.77 ng/ml

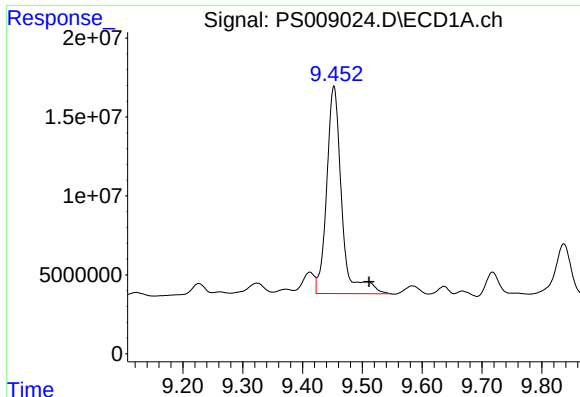

#12 2,4,5-T


R.T.: 9.452 min
Delta R.T.: -0.059 min
Response: 228297495
Conc: 21.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

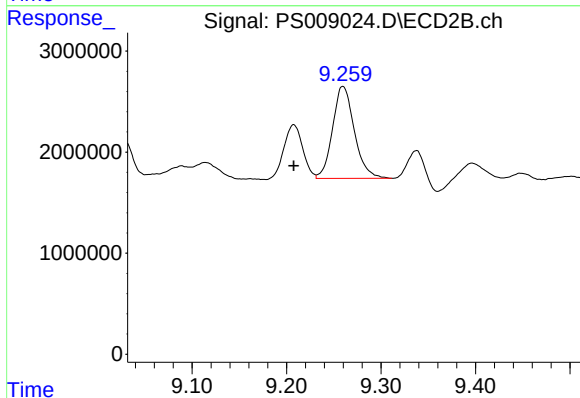


#12 2,4,5-T

R.T.: 9.260 min
Delta R.T.: 0.052 min
Response: 14561294
Conc: 2.69 ng/ml

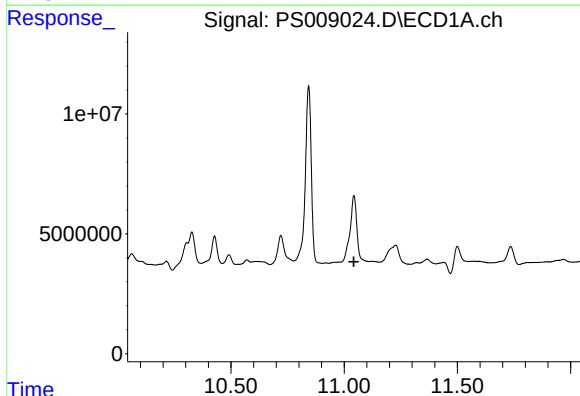


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

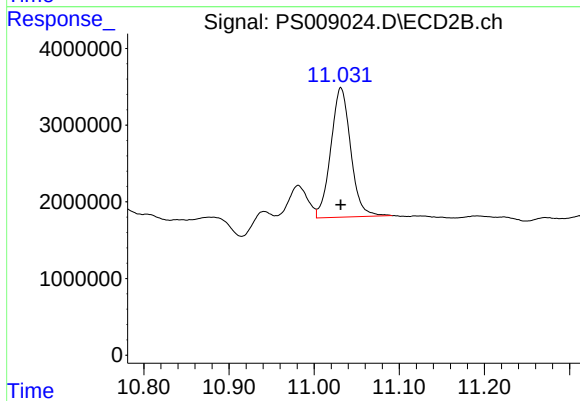

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 27392576
Conc: 3.77 ng/ml

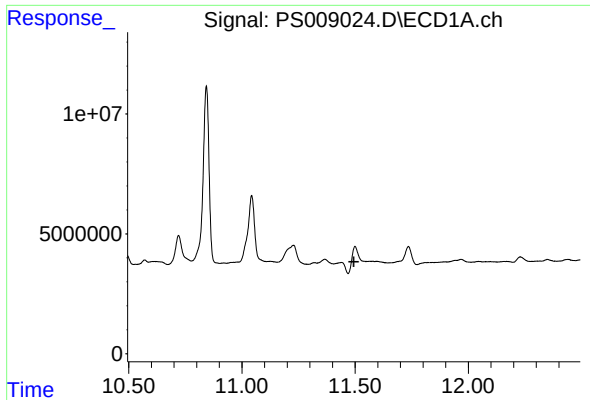

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

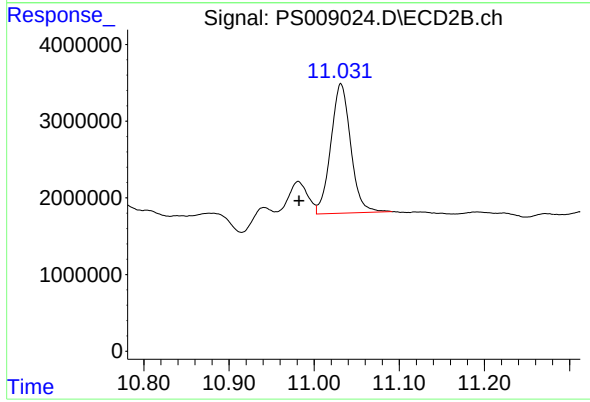

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.049 min
Response: 27392576
Conc: 3.96 ng/ml