

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 18:30
 Operator : DD\AJ
 Sample : PB127119BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:35:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.939	1003.5E6	519.6E6	458.948	539.261
Target Compounds							
1) T	Dalapon	0.000	2.592	0	34663175	N.D.	23.706
2) T	3,5-DICHL...	0.000	6.114	0	143.6E6	N.D.	98.432
5) T	DICAMBA	0.000	7.074	0	28938826	N.D.	6.991
7) T	MCPA	7.798	7.407	66798625	50545550	8.304	11.425 #
8) T	DICHLORPROP	0.000	7.760	0	13130260	N.D.	13.105
11) T	2,4,5-TP ...	0.000	8.795	0	195.7E6	N.D.	36.122
13) T	2,4-DB	0.000	9.655	0	21795666	N.D.	31.029
14) T	DINOSEB	0.000	10.060	0	17608213	N.D.	4.453
15) T	Picloram	0.000	11.032	0	29855058	N.D.	4.109
16) T	DCPA	0.000	11.032	0	29855058	N.D.	4.315



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 18:30
Operator : DD\AJ
Sample : PB127119BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:35:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

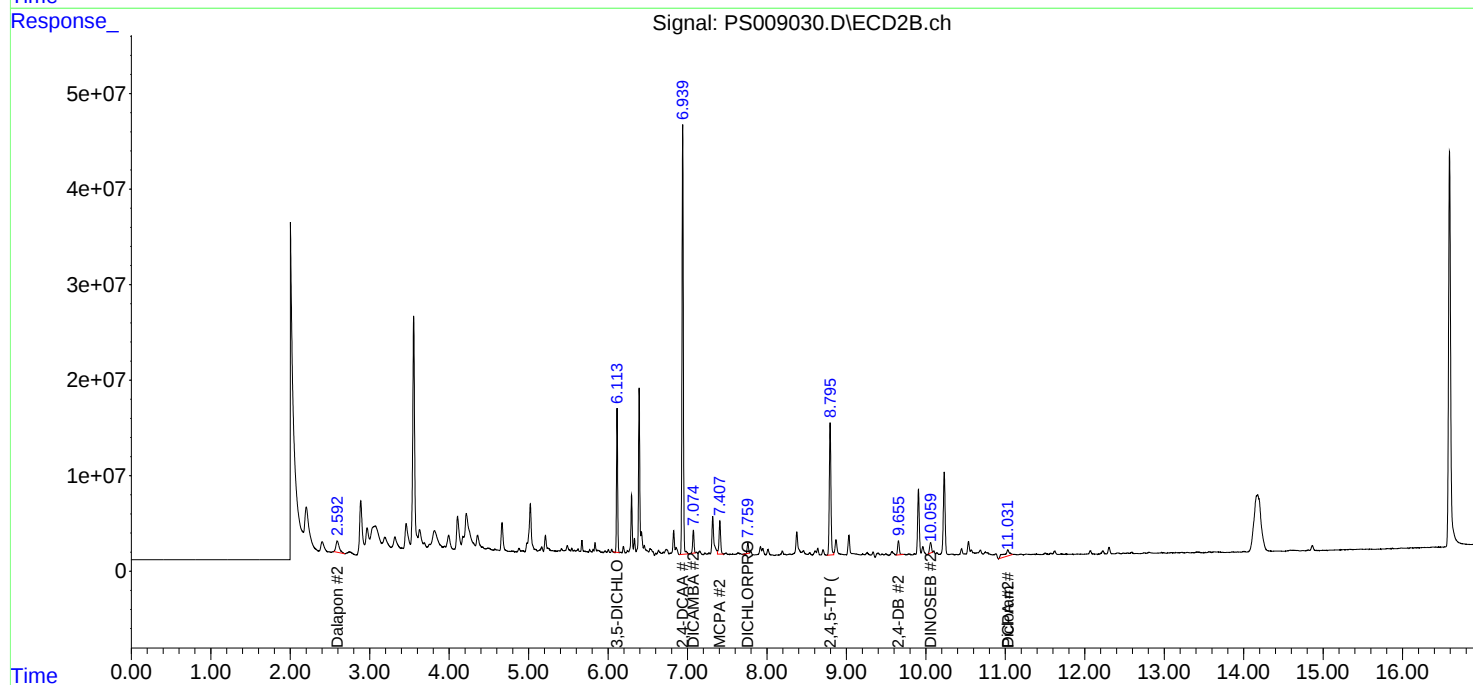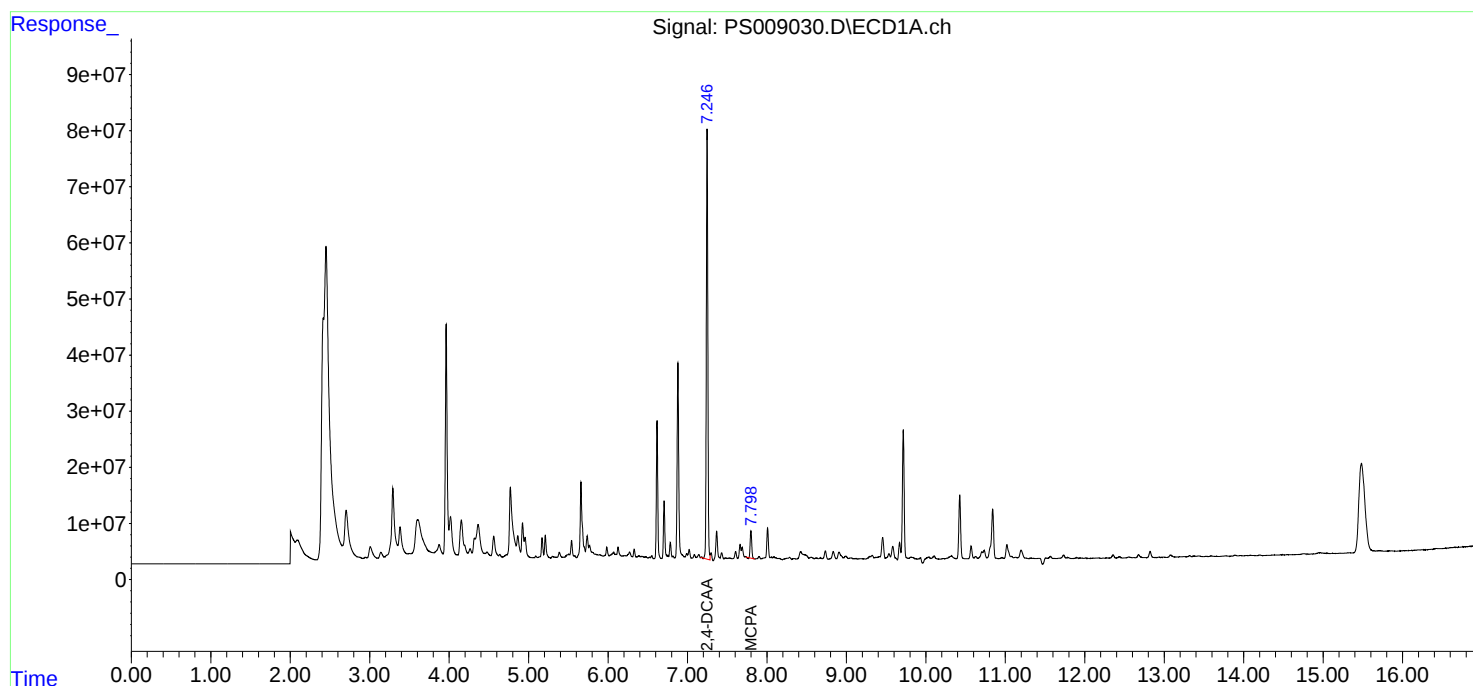


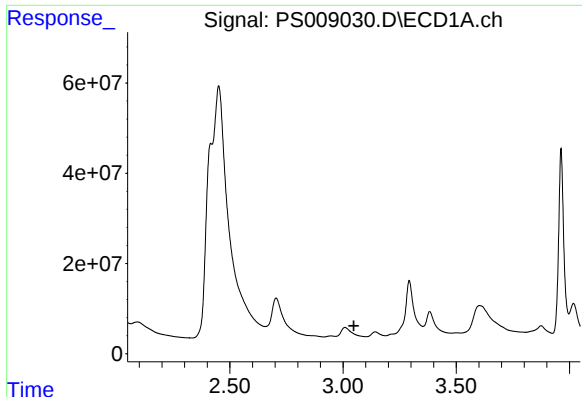

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

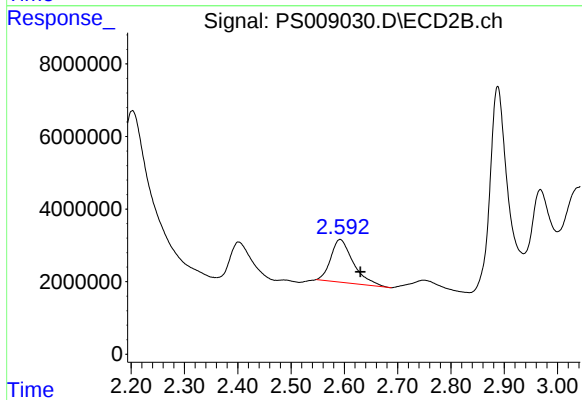


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 34663175
Conc: 23.71 ng/ml

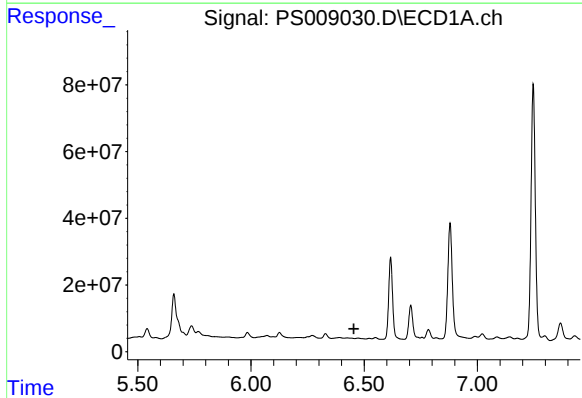


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

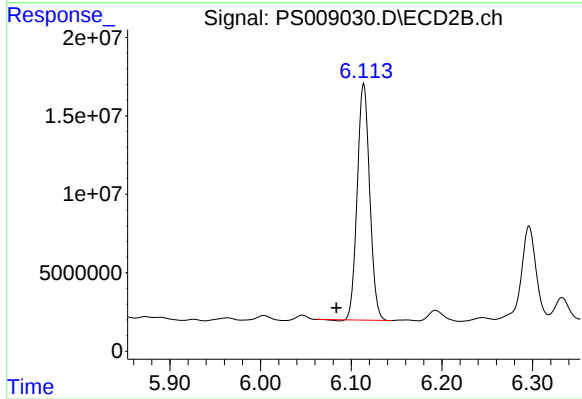

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 143639591
Conc: 98.43 ng/ml

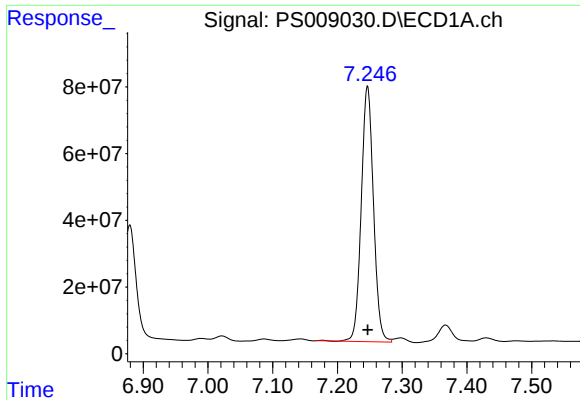

#4 2,4-DCAA


R.T.: 7.246 min
Delta R.T.: 0.000 min
Response: 1003531509
Conc: 458.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

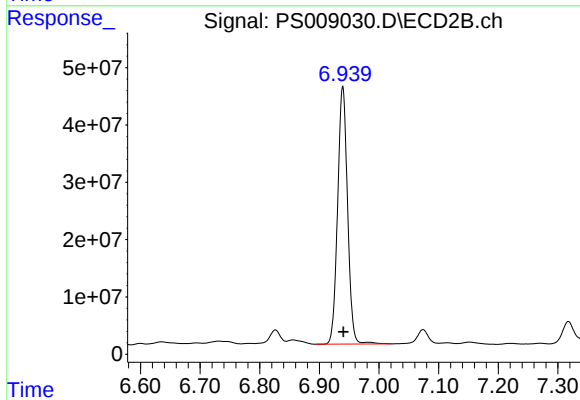


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 519607792
Conc: 539.26 ng/ml

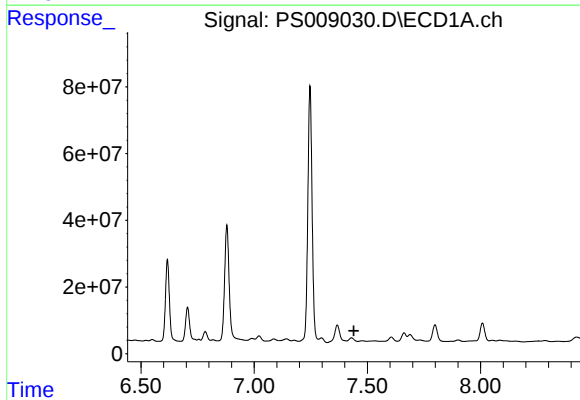


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

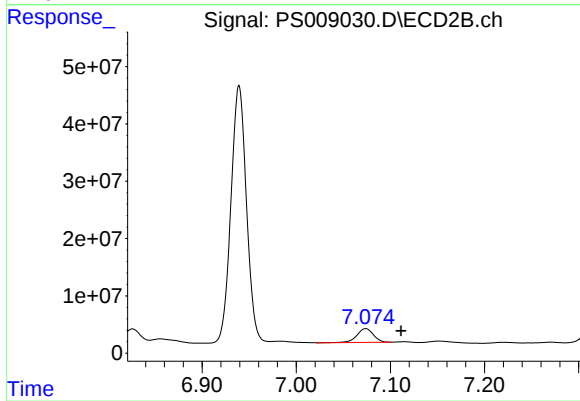

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 28938826
Conc: 6.99 ng/ml

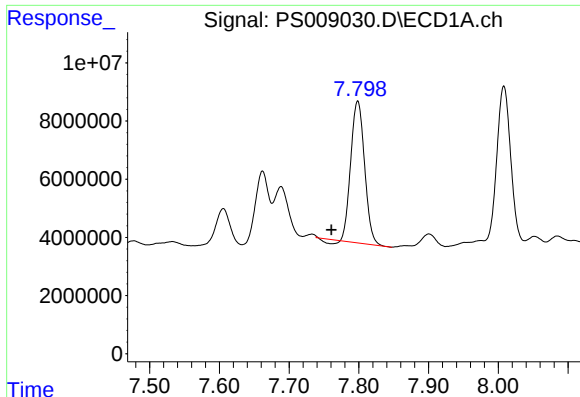

#7 MCPA


R.T.: 7.798 min
Delta R.T.: 0.038 min
Response: 66798625
Conc: 8.30 ug/ml

Instrument :
ECD_S
ClientSampleId :

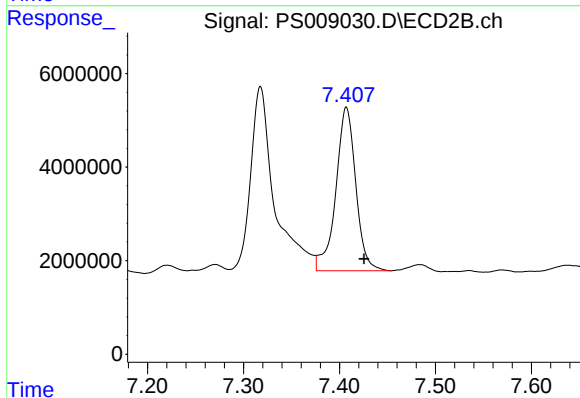


#7 MCPA

R.T.: 7.407 min
Delta R.T.: -0.018 min
Response: 50545550
Conc: 11.42 ug/ml

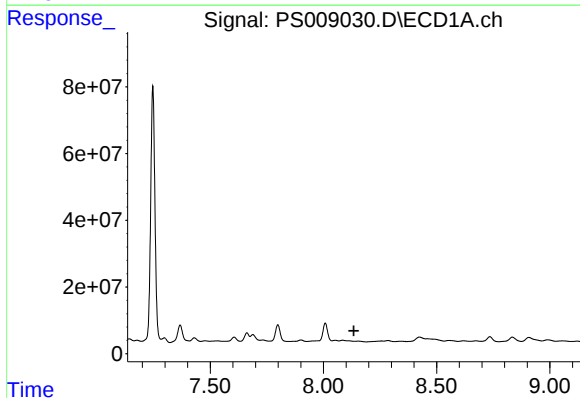


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

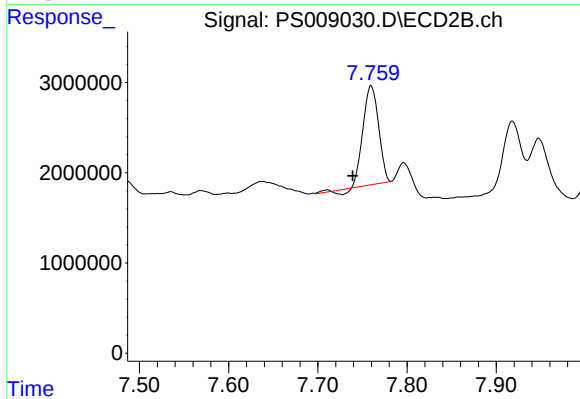

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 13130260
Conc: 13.10 ng/ml

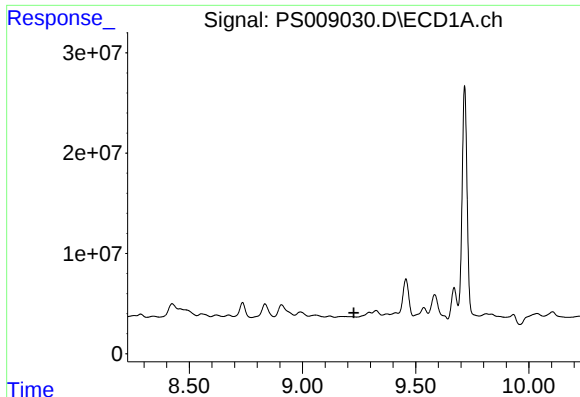

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

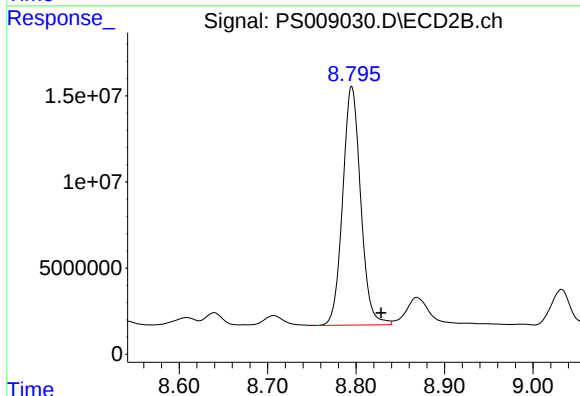


#11 2,4,5-TP (SILVEX)

R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 195668736
Conc: 36.12 ng/ml

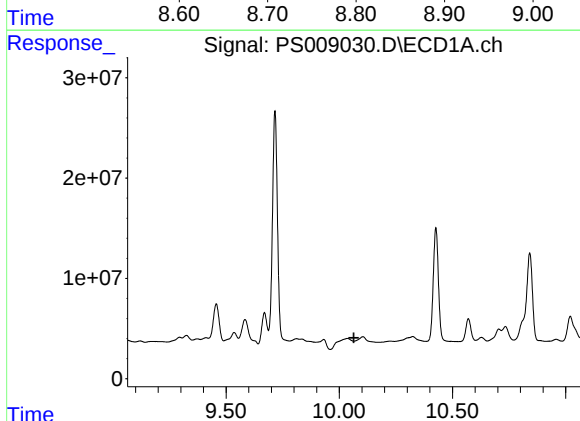


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

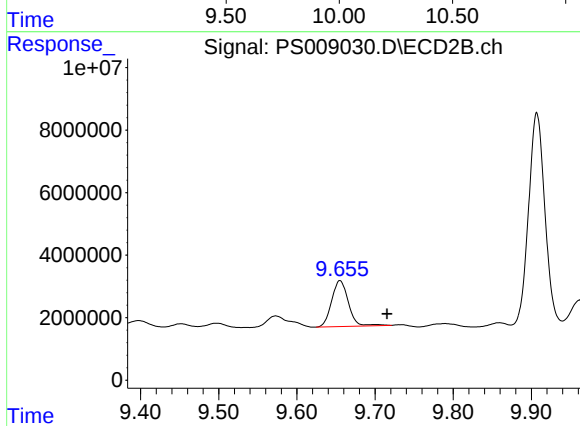

#13 2,4-DB


R.T.: 9.655 min
Delta R.T.: -0.060 min
Response: 21795666
Conc: 31.03 ng/ml

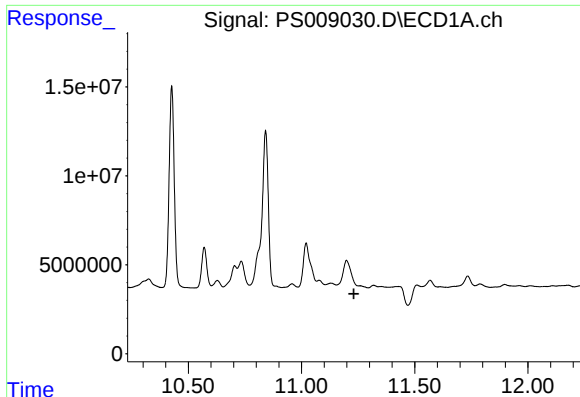

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

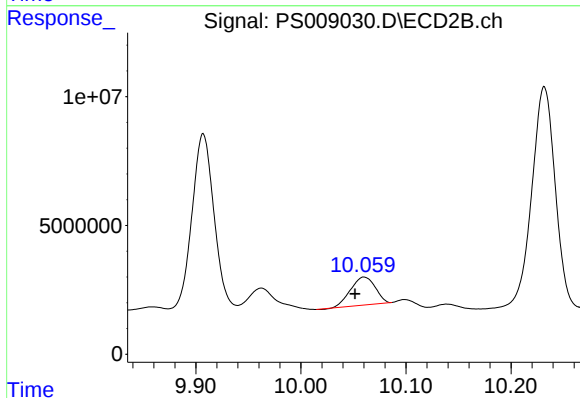


#14 DINOSEB

R.T.: 10.060 min
Delta R.T.: 0.009 min
Response: 17608213
Conc: 4.45 ng/ml

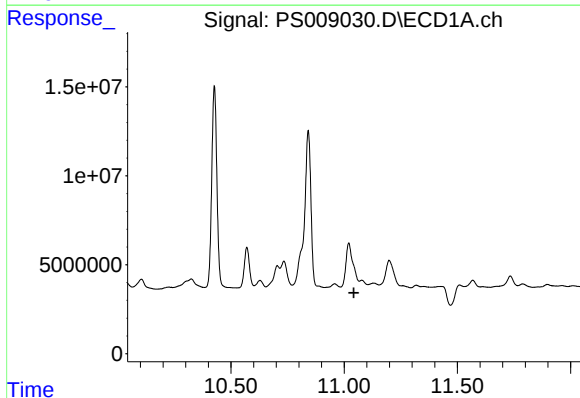


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.043 min
Response: 0
Conc: N.D.

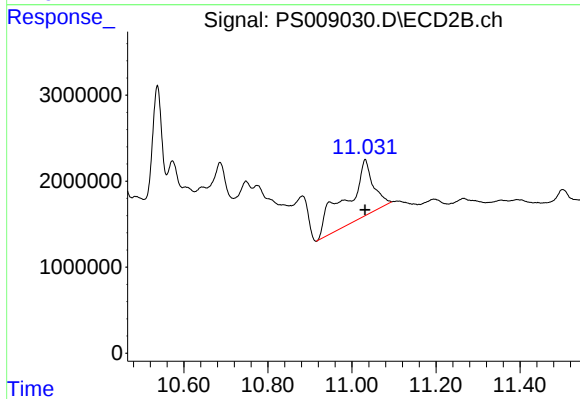

#15 Picloram


R.T.: 11.032 min
Delta R.T.: 0.000 min
Response: 29855058
Conc: 4.11 ng/ml

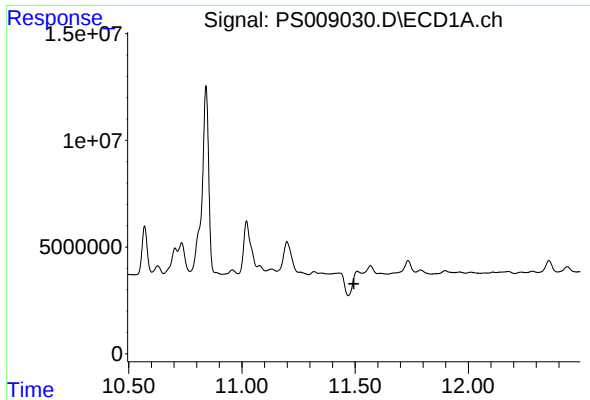

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

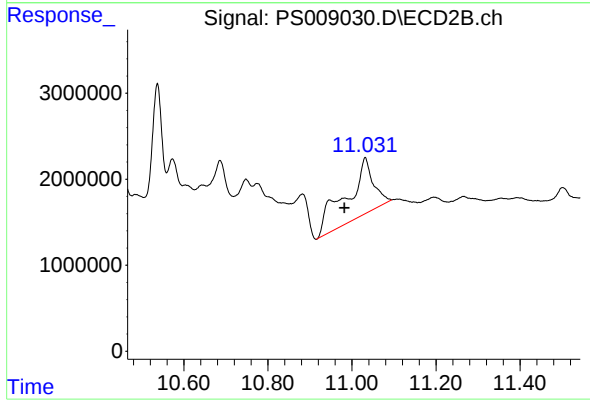

#16 DCPA

R.T.: 11.032 min
Delta R.T.: 0.049 min
Response: 29855058
Conc: 4.31 ng/ml