

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 20:48
 Operator : DD\AJ
 Sample : L1656-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:36:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.591	0	185.5E6	N.D. 126.883
2) T	3,5-DICHL...	0.000	6.114	0	80934378	N.D. 55.462
7) T	MCPA	7.798	7.406	225.1E6	120.9E6	27.987 27.330
8) T	DICHLORPROP	0.000	7.759	0	58215628	N.D. 58.103
10) T	Pentachlo...	0.000	8.465	0	26457516	N.D. 1.862
11) T	2,4,5-TP ...	0.000	8.826	0	15533146	N.D. 2.868
12) T	2,4,5-T	9.454	9.206	154.6E6	20325862	14.459 3.755 #
13) T	2,4-DB	0.000	9.708	0	17492646	N.D. 24.903
14) T	DINOSEB	0.000	10.052	0	28000193	N.D. 7.081
15) T	Picloram	11.043	11.030	352.0E6	212.9E6	25.710 29.304
16) T	DCPA	0.000	10.981	0	28525164	N.D. 4.123



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 20:48
Operator : DD\AJ
Sample : L1656-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:36:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

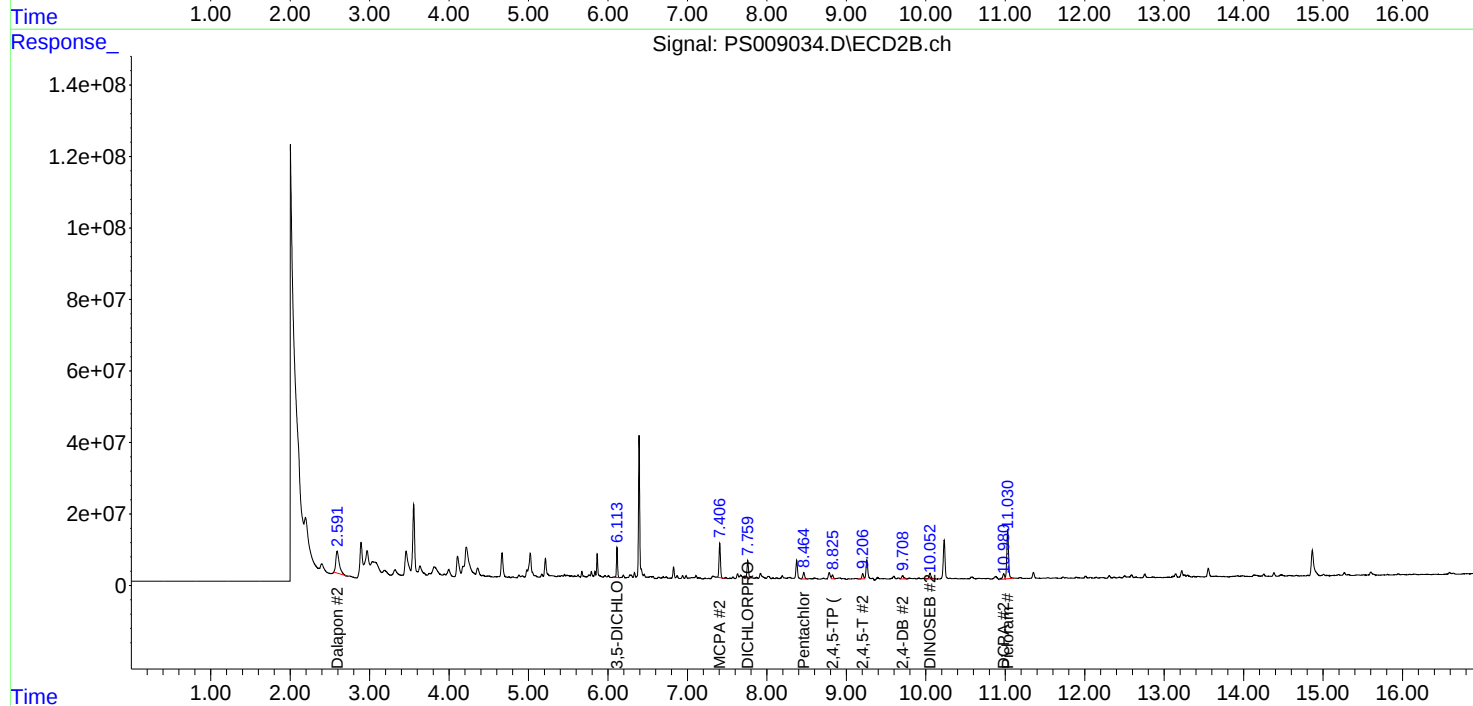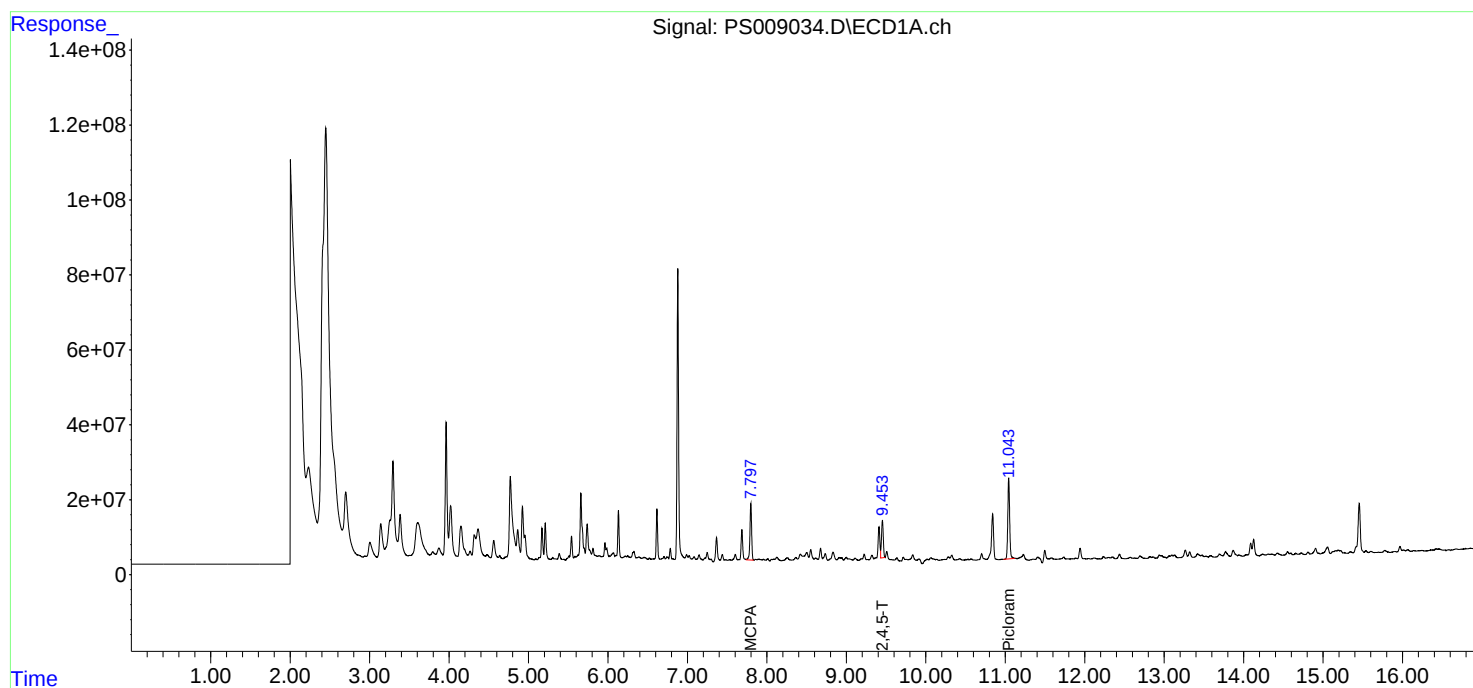


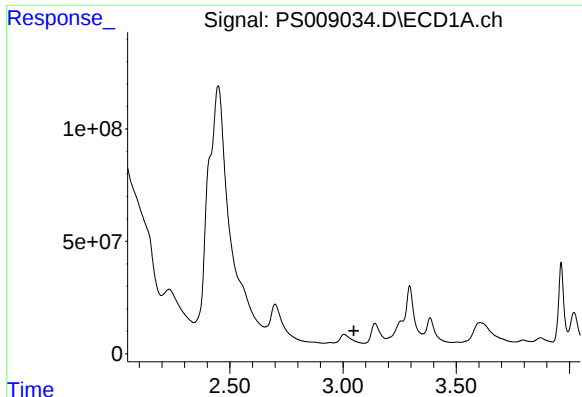

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

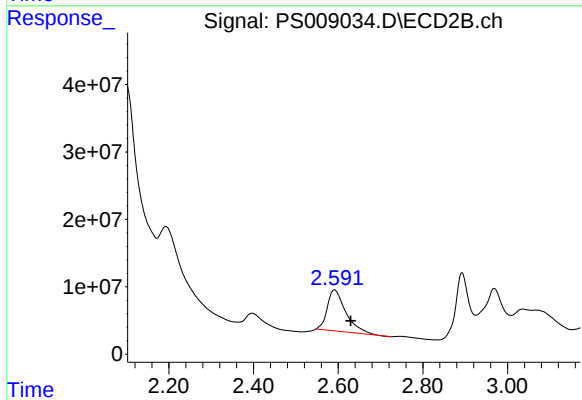


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 185531586
Conc: 126.88 ng/ml

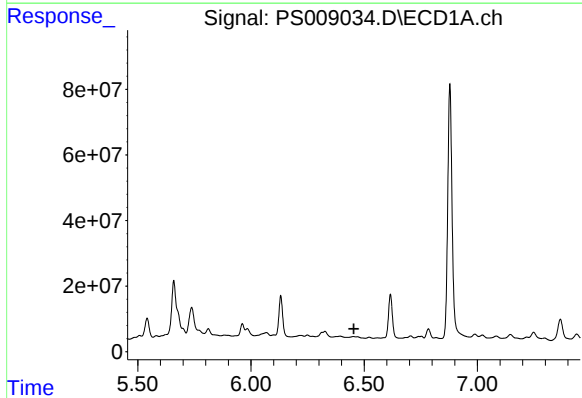


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

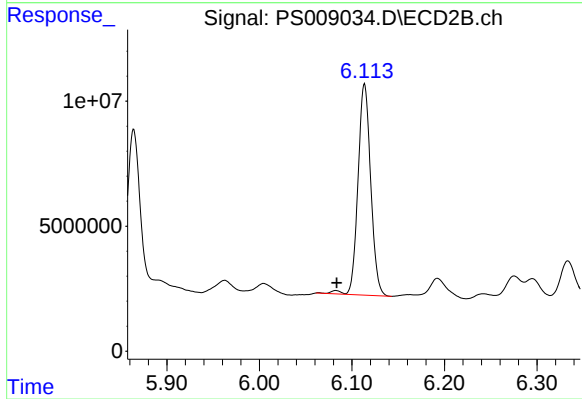

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 80934378
Conc: 55.46 ng/ml

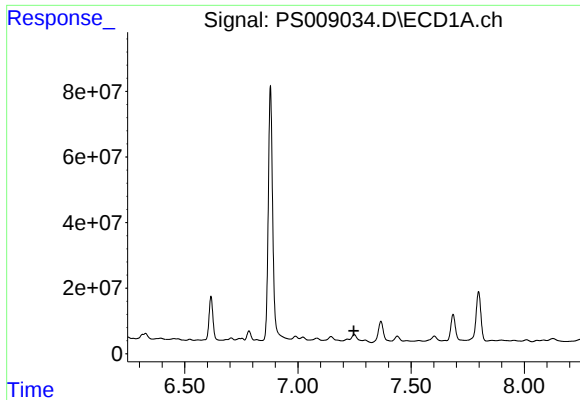

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.247 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

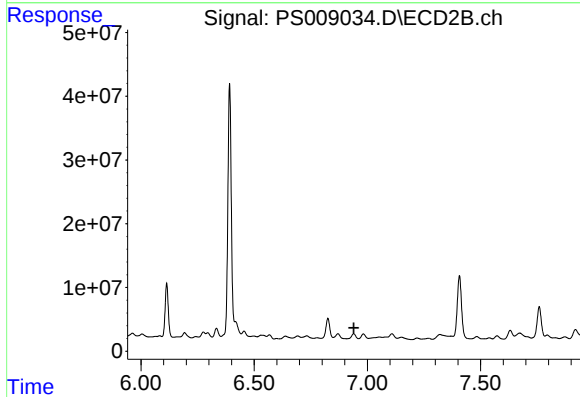


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.940 min
Response: 0
Conc: N.D.

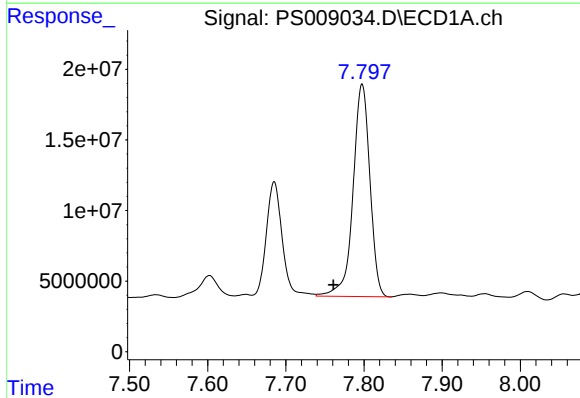


#7 MCPA

R.T.: 7.798 min
Delta R.T.: 0.037 min
Response: 225129376
Conc: 27.99 ug/ml

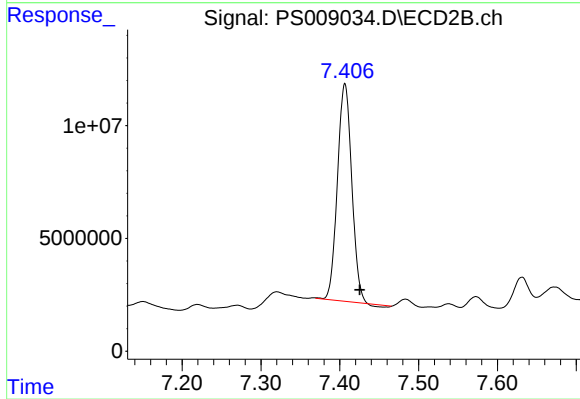

#7 MCPA


R.T.: 7.406 min
Delta R.T.: -0.019 min
Response: 120916280
Conc: 27.33 ug/ml

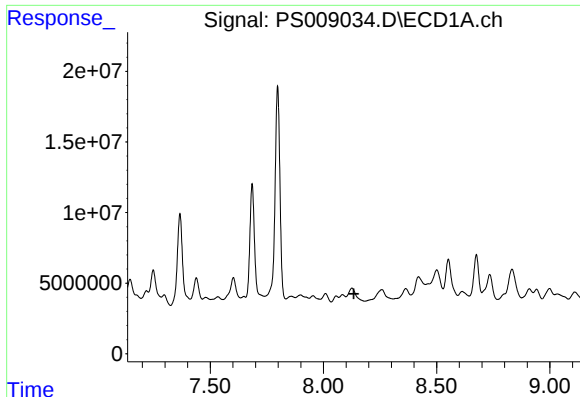

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

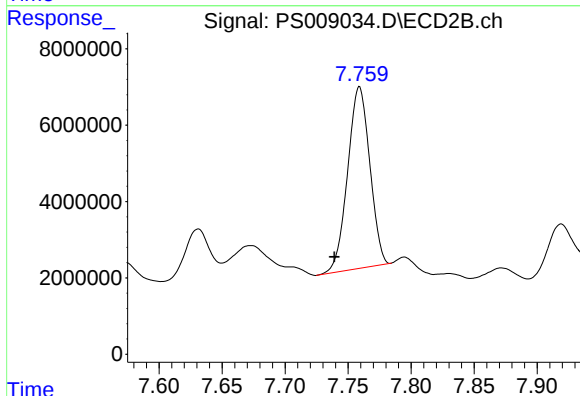


#8 DICHLORPROP

R.T.: 7.759 min
Delta R.T.: 0.020 min
Response: 58215628
Conc: 58.10 ng/ml

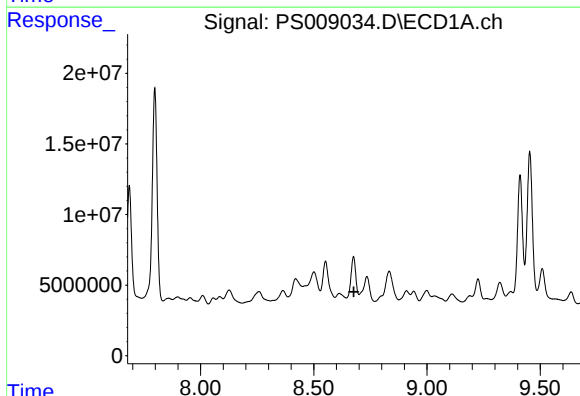


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

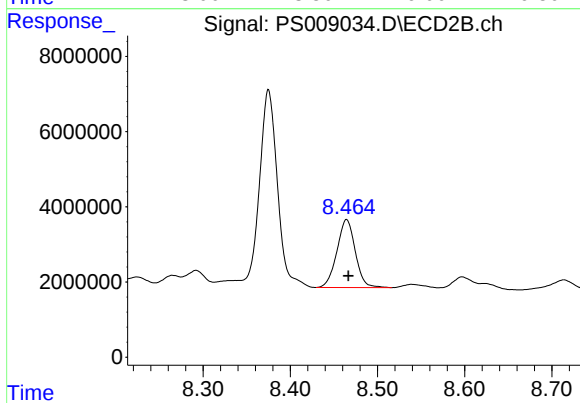

#10 Pentachlorophenol


R.T.: 8.465 min
Delta R.T.: -0.002 min
Response: 26457516
Conc: 1.86 ng/ml

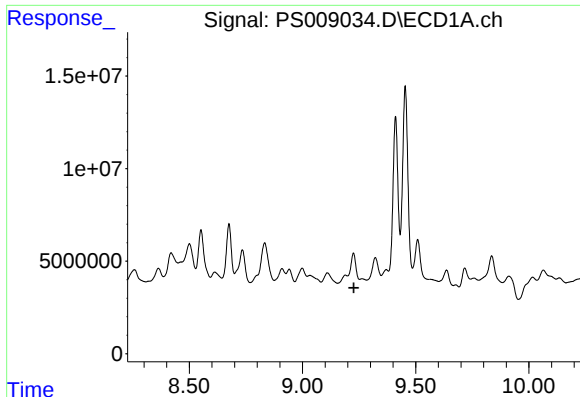

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

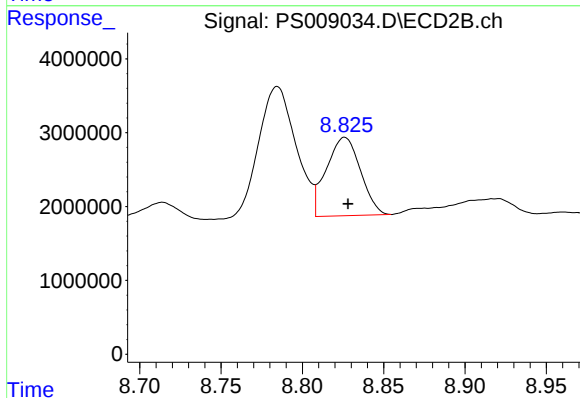


#11 2,4,5-TP (SILVEX)

R.T.: 8.826 min
Delta R.T.: -0.002 min
Response: 15533146
Conc: 2.87 ng/ml

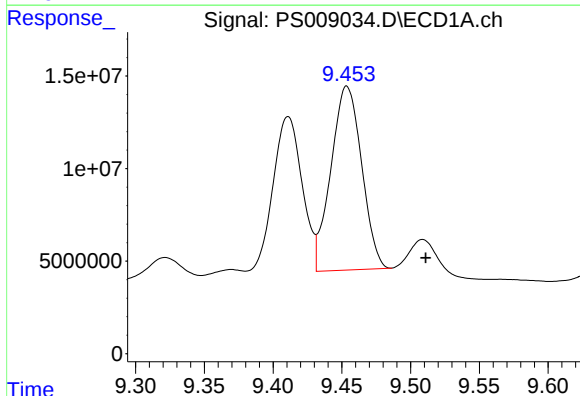


#12 2,4,5-T

R.T.: 9.454 min
Delta R.T.: -0.057 min
Response: 154601530
Conc: 14.46 ng/ml

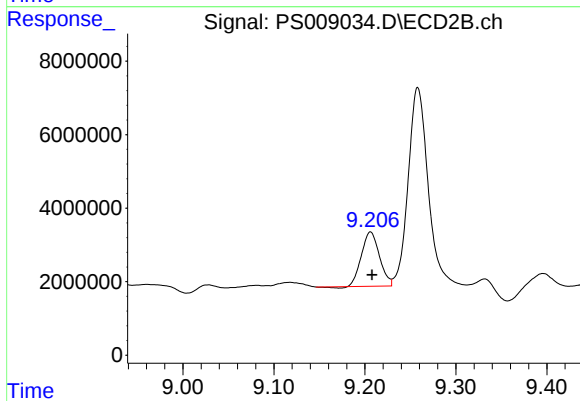

#12 2,4,5-T


R.T.: 9.206 min
Delta R.T.: -0.001 min
Response: 20325862
Conc: 3.75 ng/ml

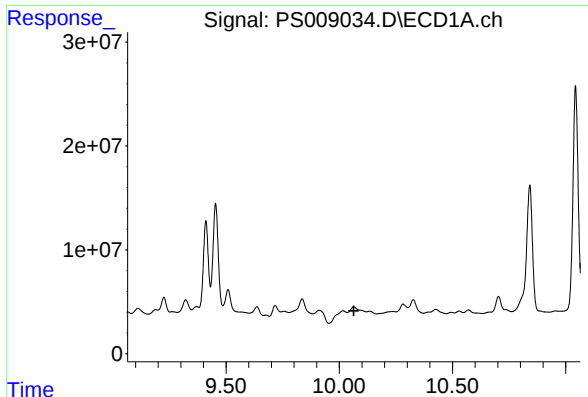

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

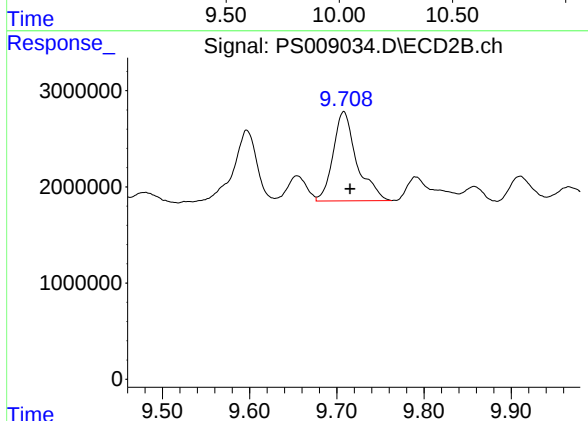


#13 2,4-DB

R.T.: 9.708 min
Delta R.T.: -0.007 min
Response: 17492646
Conc: 24.90 ng/ml

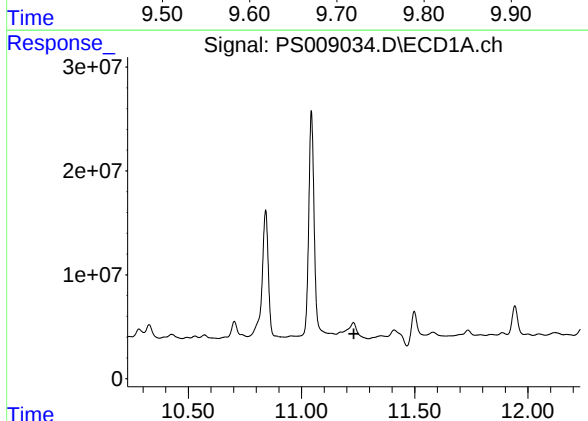


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

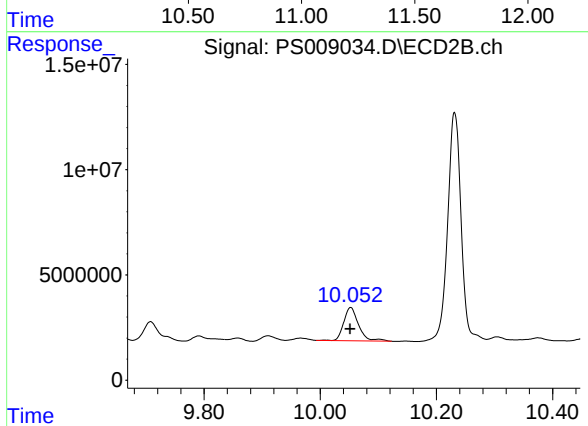

#14 DINOSEB


R.T.: 10.052 min
Delta R.T.: 0.000 min
Response: 28000193
Conc: 7.08 ng/ml

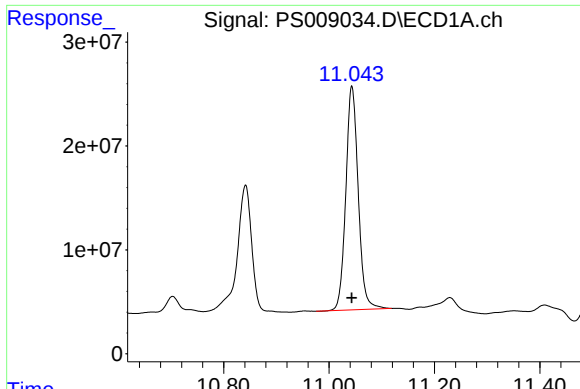

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 351988638
Conc: 25.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

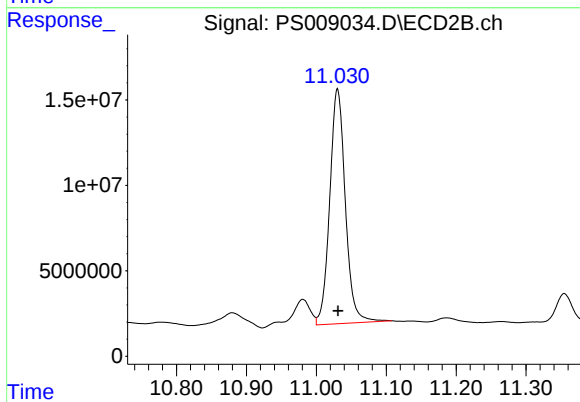


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.000 min
Response: 212939126
Conc: 29.30 ng/ml

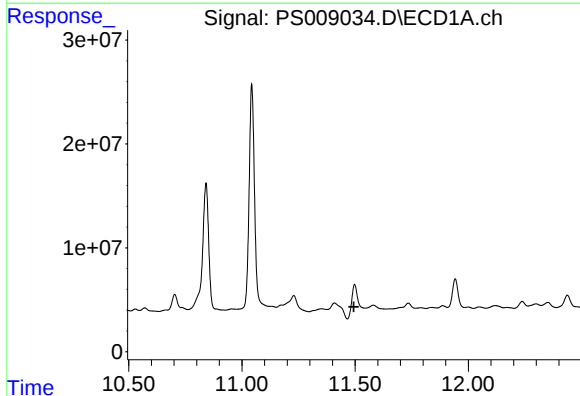

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

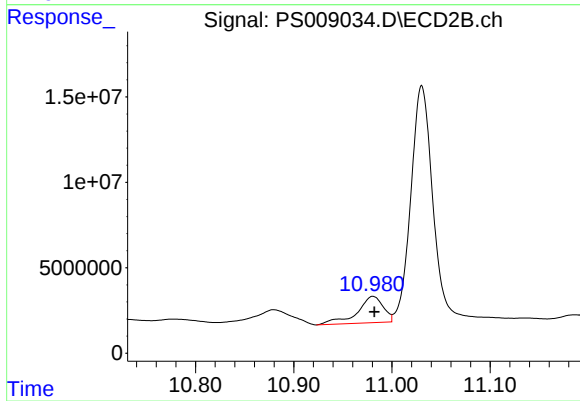

#16 DCPA

R.T.: 10.981 min
Delta R.T.: -0.002 min
Response: 28525164
Conc: 4.12 ng/ml