

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009035.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 21:11
 Operator : DD\AJ
 Sample : L1676-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:36:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	589.6E6	281.7E6	269.653	292.407
Target Compounds							
1) T	Dalapon	0.000	2.591	0	48907627	N.D.	33.448
2) T	3,5-DICHL...	0.000	6.114	0	172.6E6	N.D.	118.305
5) T	DICAMBA	0.000	7.076	0	54347563	N.D.	13.130
7) T	MCPA	7.798	7.407	57487035	39703483	7.147	8.974 #
8) T	DICHLORPROP	0.000	7.760	0	18795642	N.D.	18.759
10) T	Pentachlo...	0.000	8.481	0	30868372	N.D.	2.173
11) T	2,4,5-TP ...	0.000	8.795	0	204.4E6	N.D.	37.730
12) T	2,4,5-T	9.456	0.000	107.8E6	0	10.087	N.D. #
13) T	2,4-DB	0.000	9.656	0	31291610	N.D.	44.547
14) T	DINOSEB	0.000	10.061	0	35840437	N.D.	9.064
15) T	Picloram	11.020	11.030	100.7E6	22378510	7.358	3.080 #
16) T	DCPA	0.000	10.961	0	22145092	N.D.	3.200



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009035.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 21:11
Operator : DD\AJ
Sample : L1676-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:36:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

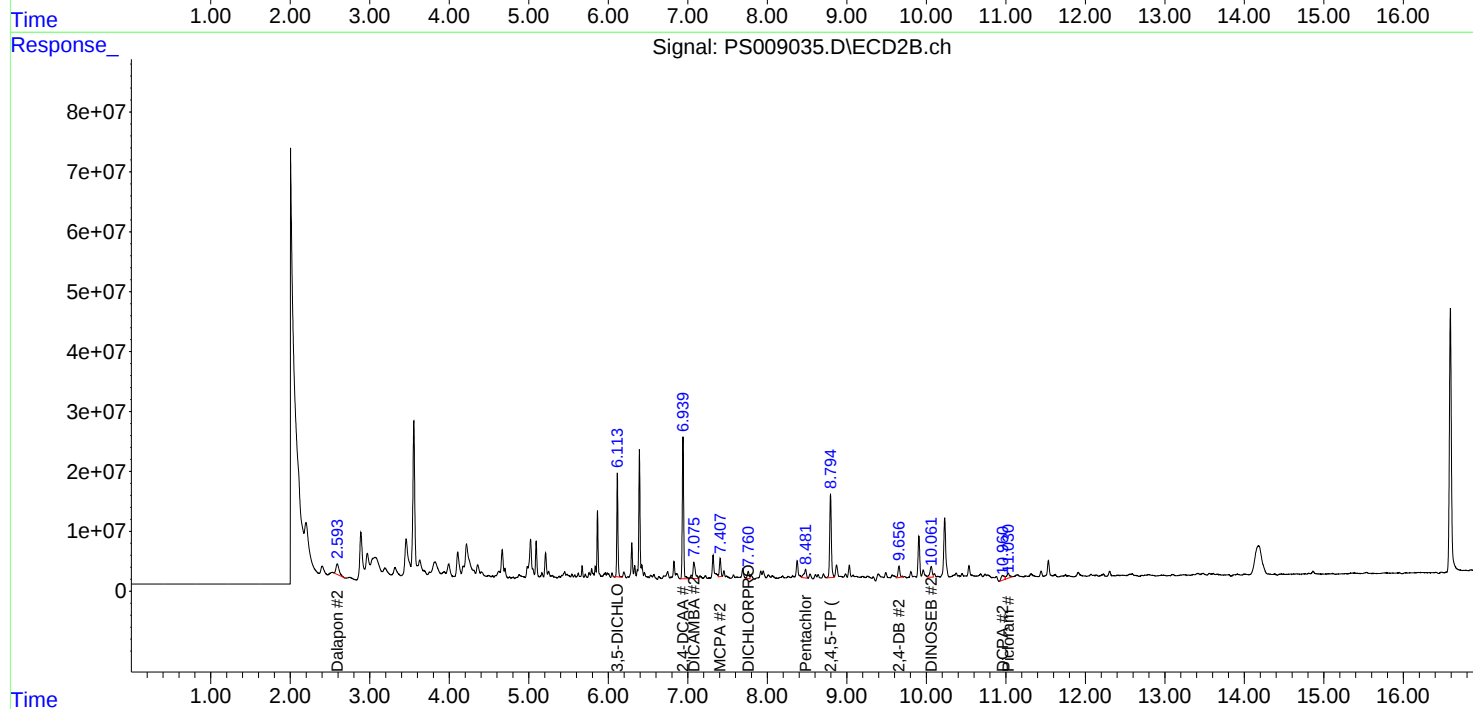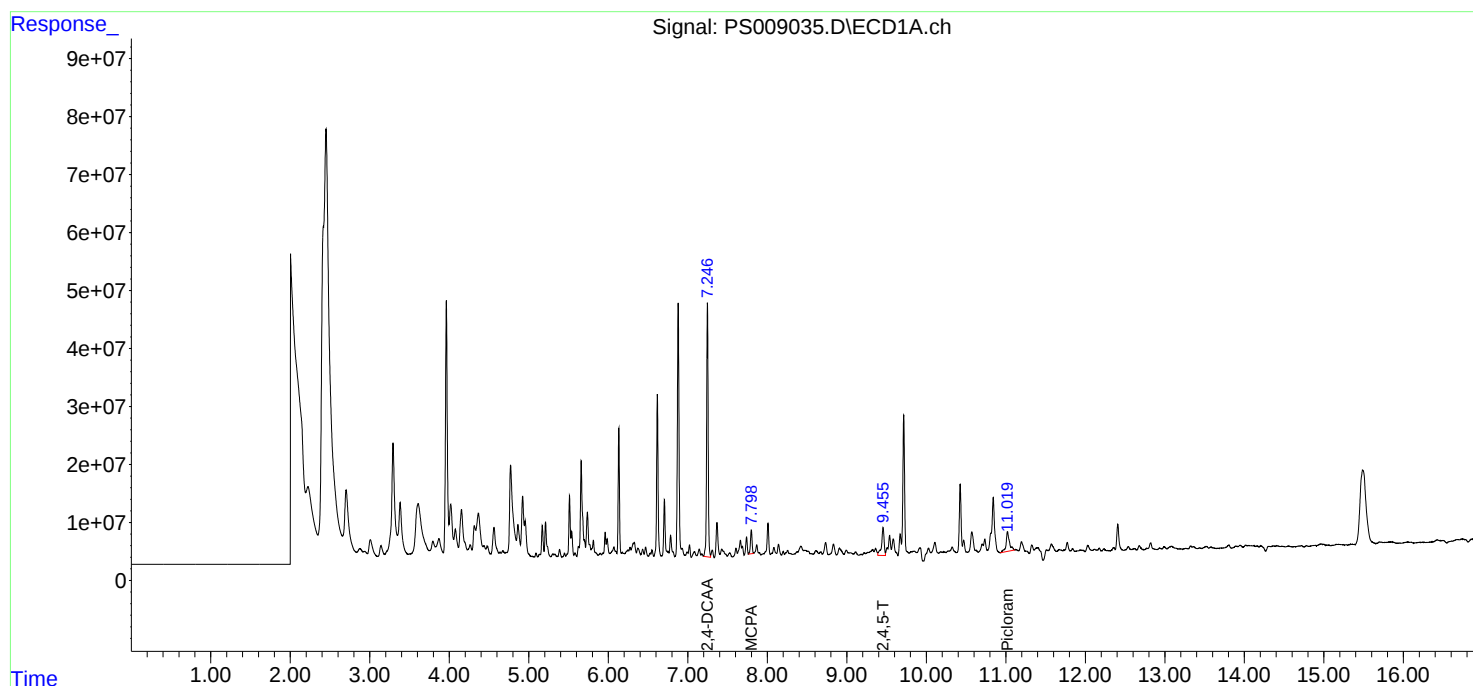


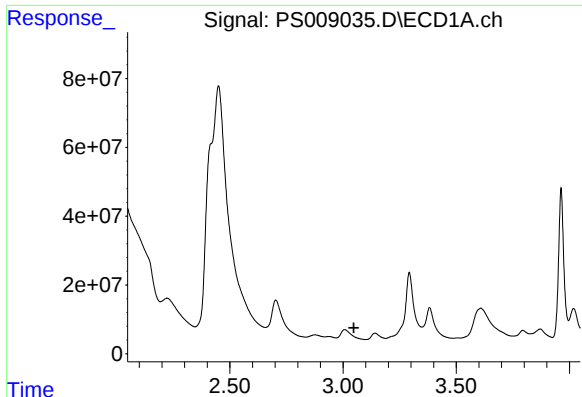

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

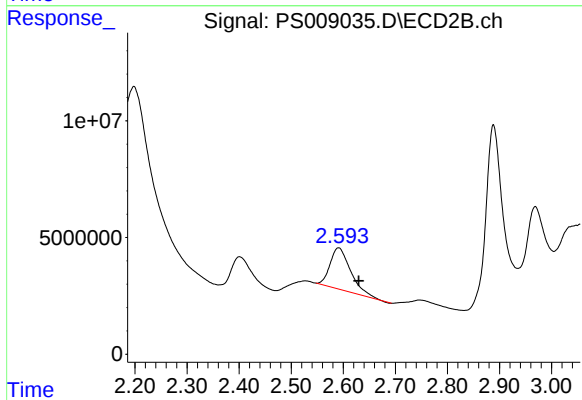


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 48907627
Conc: 33.45 ng/ml

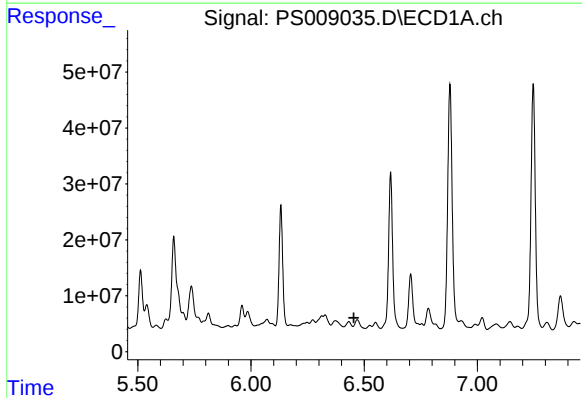


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

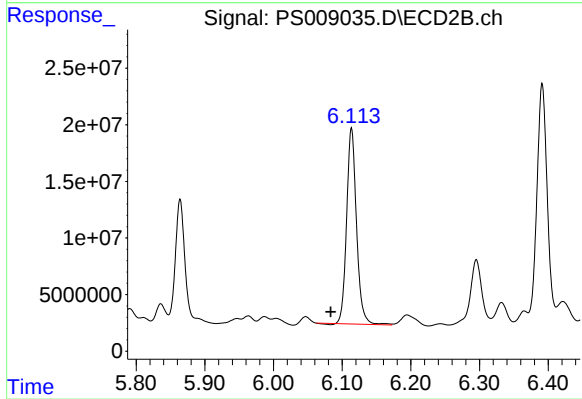

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 172638912
Conc: 118.30 ng/ml

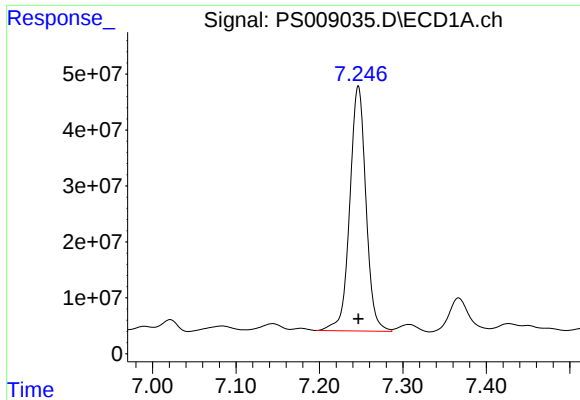

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 589621545
Conc: 269.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

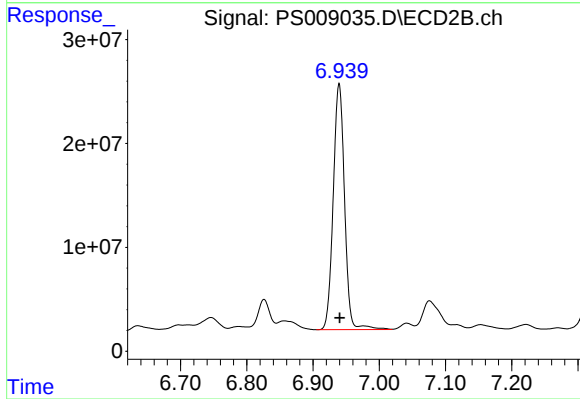


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 281749906
Conc: 292.41 ng/ml

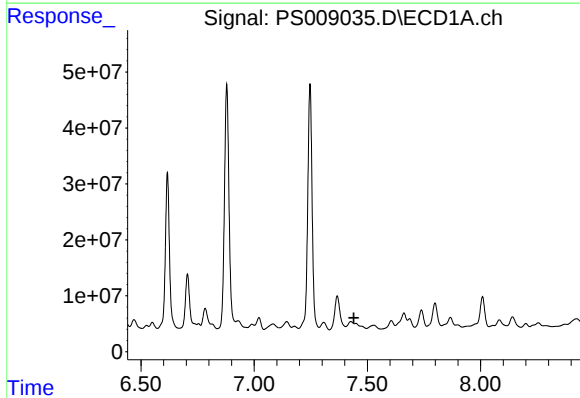


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

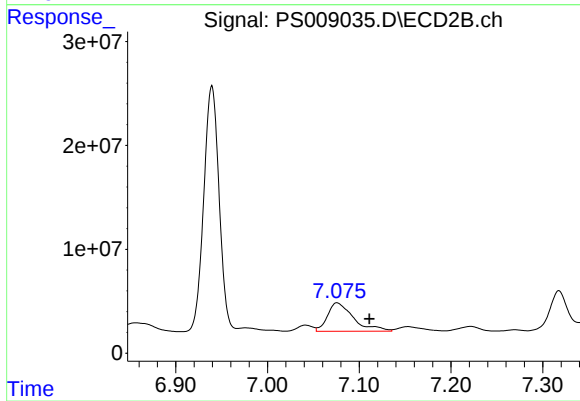

#5 DICAMBA


R.T.: 7.076 min
Delta R.T.: -0.035 min
Response: 54347563
Conc: 13.13 ng/ml

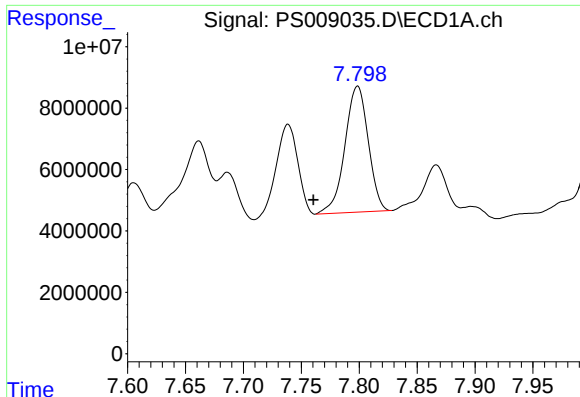

#7 MCPA


R.T.: 7.798 min
Delta R.T.: 0.038 min
Response: 57487035
Conc: 7.15 ug/ml

Instrument :
ECD_S
ClientSampleId :

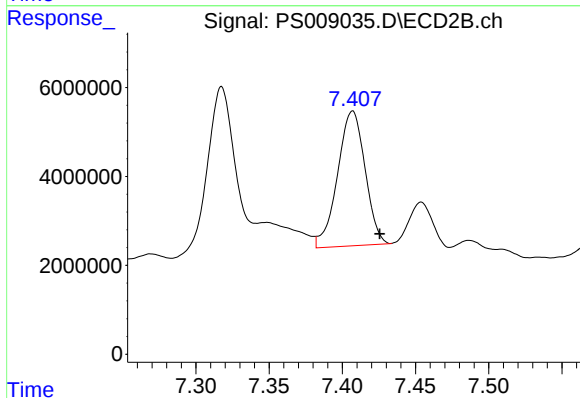


#7 MCPA

R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 39703483
Conc: 8.97 ug/ml

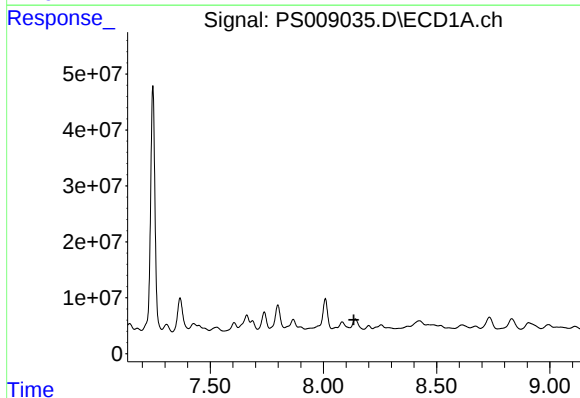


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

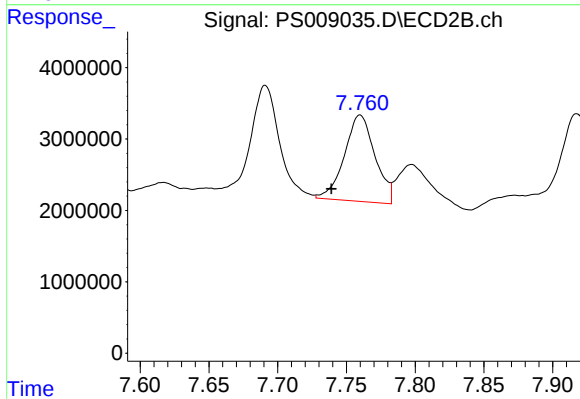

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 18795642
Conc: 18.76 ng/ml

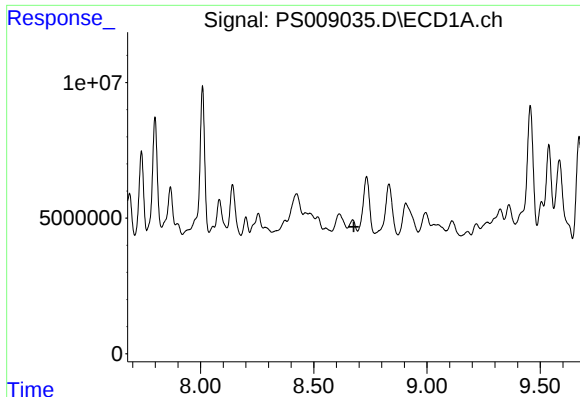

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

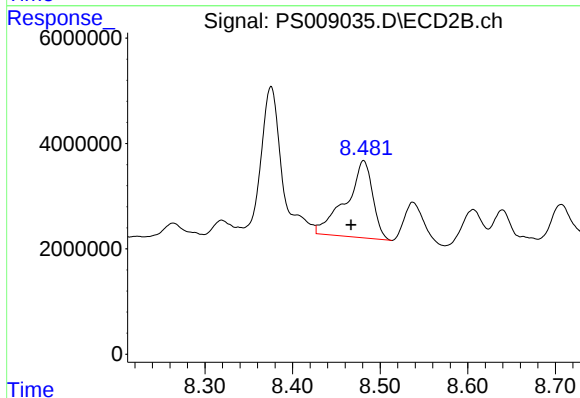


#10 Pentachlorophenol

R.T.: 8.481 min
Delta R.T.: 0.014 min
Response: 30868372
Conc: 2.17 ng/ml

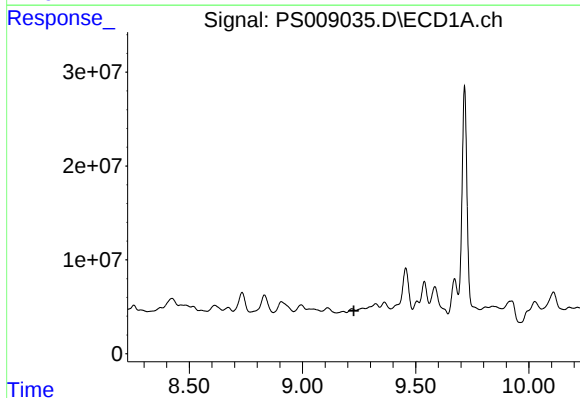


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

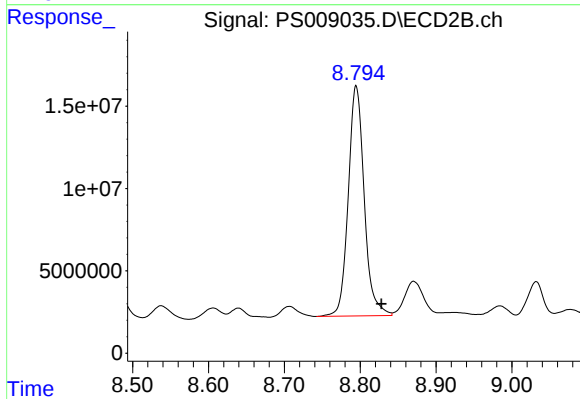

#11 2,4,5-TP (SILVEX)


R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 204382066
Conc: 37.73 ng/ml

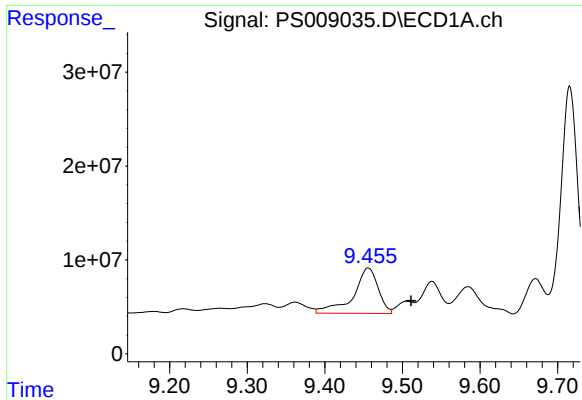

#12 2,4,5-T


R.T.: 9.456 min
Delta R.T.: -0.055 min
Response: 107847381
Conc: 10.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

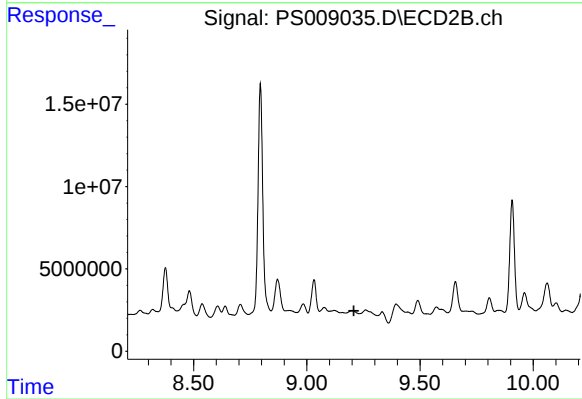


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

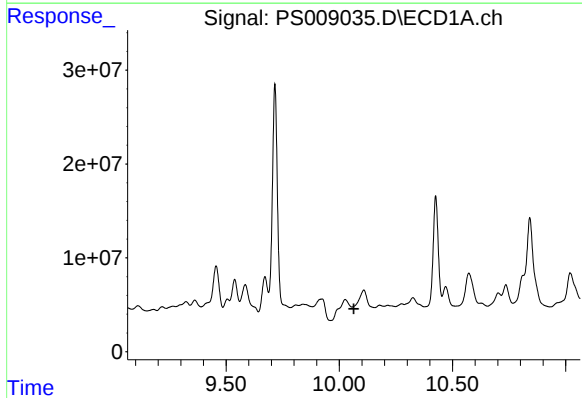


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

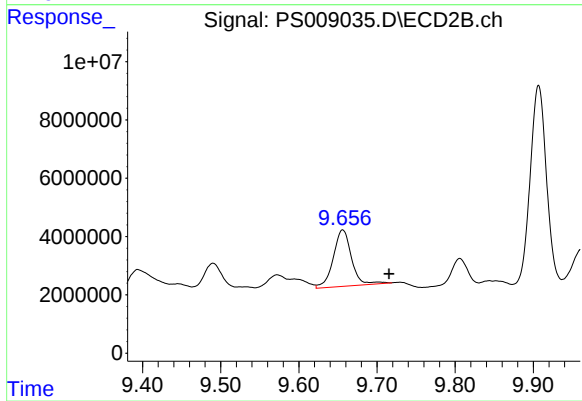

#13 2,4-DB


R.T.: 9.656 min
Delta R.T.: -0.059 min
Response: 31291610
Conc: 44.55 ng/ml

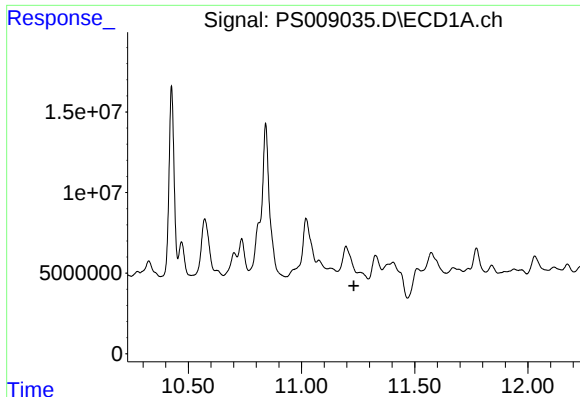

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

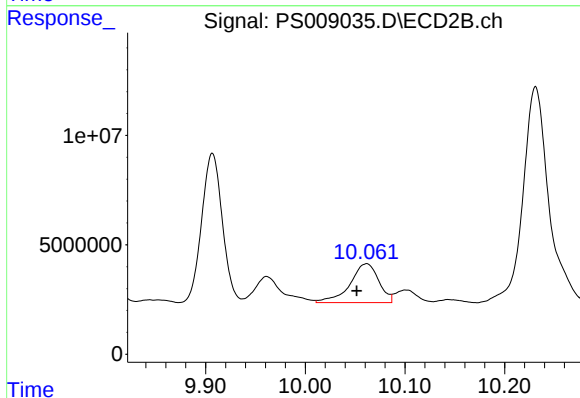


#14 DINOSEB

R.T.: 10.061 min
Delta R.T.: 0.010 min
Response: 35840437
Conc: 9.06 ng/ml

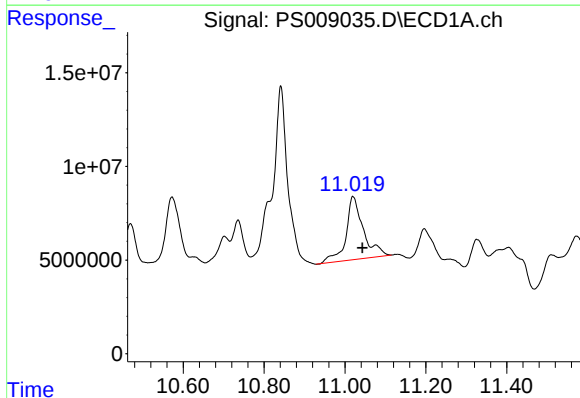


#15 Picloram

R.T.: 11.020 min
Delta R.T.: -0.023 min
Response: 100744903
Conc: 7.36 ng/ml

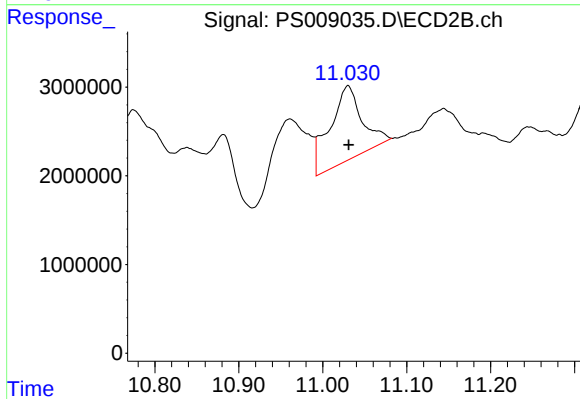

#15 Picloram


R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 22378510
Conc: 3.08 ng/ml

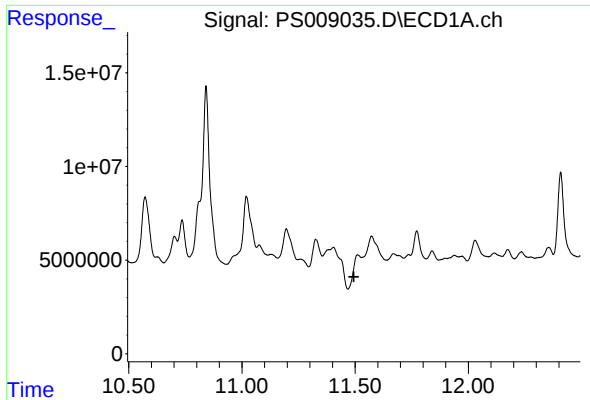

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

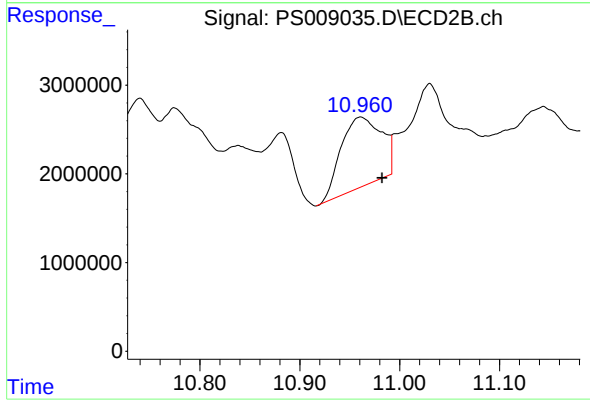

#16 DCPA

R.T.: 10.961 min
Delta R.T.: -0.021 min
Response: 22145092
Conc: 3.20 ng/ml