

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 21:33
 Operator : DD\AJ
 Sample : L1681-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:37:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	616.0E6	286.8E6	281.700	297.608
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	196.8E6	N.D.	134.878
5) T	DICAMBA	0.000	7.074	0	41434888	N.D.	10.010
7) T	MCPA	7.799	7.407	56307709	48093777	7.000	10.871 #
8) T	DICHLORPROP	0.000	7.760	0	20858584	N.D.	20.818
9) T	2,4-D	0.000	8.015	0	17051014	N.D.	14.391
11) T	2,4,5-TP ...	0.000	8.795	0	178.8E6	N.D.	33.010
12) T	2,4,5-T	9.455	0.000	134.8E6	0	12.603	N.D. #
13) T	2,4-DB	0.000	9.656	0	16198092	N.D.	23.060
14) T	DINOSEB	0.000	10.056	0	36550902	N.D.	9.244



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 21:33
Operator : DD\AJ
Sample : L1681-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:37:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

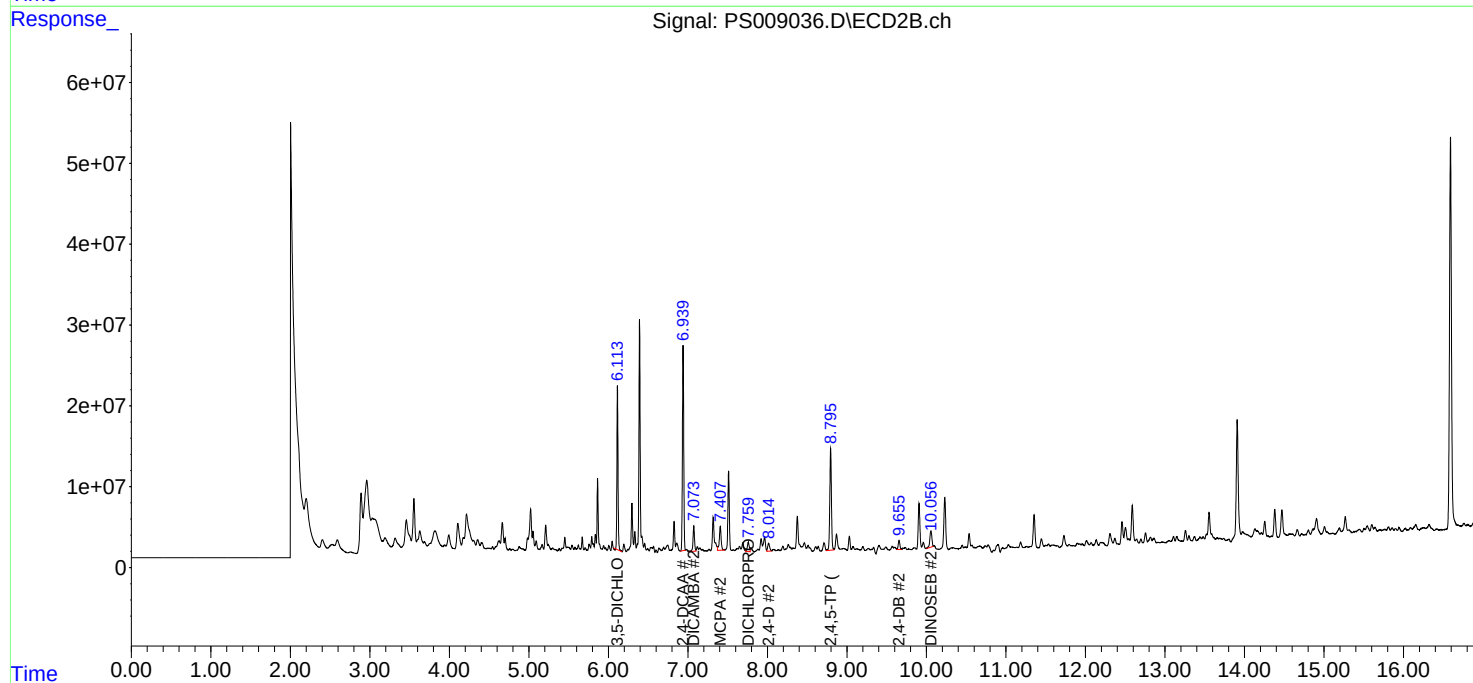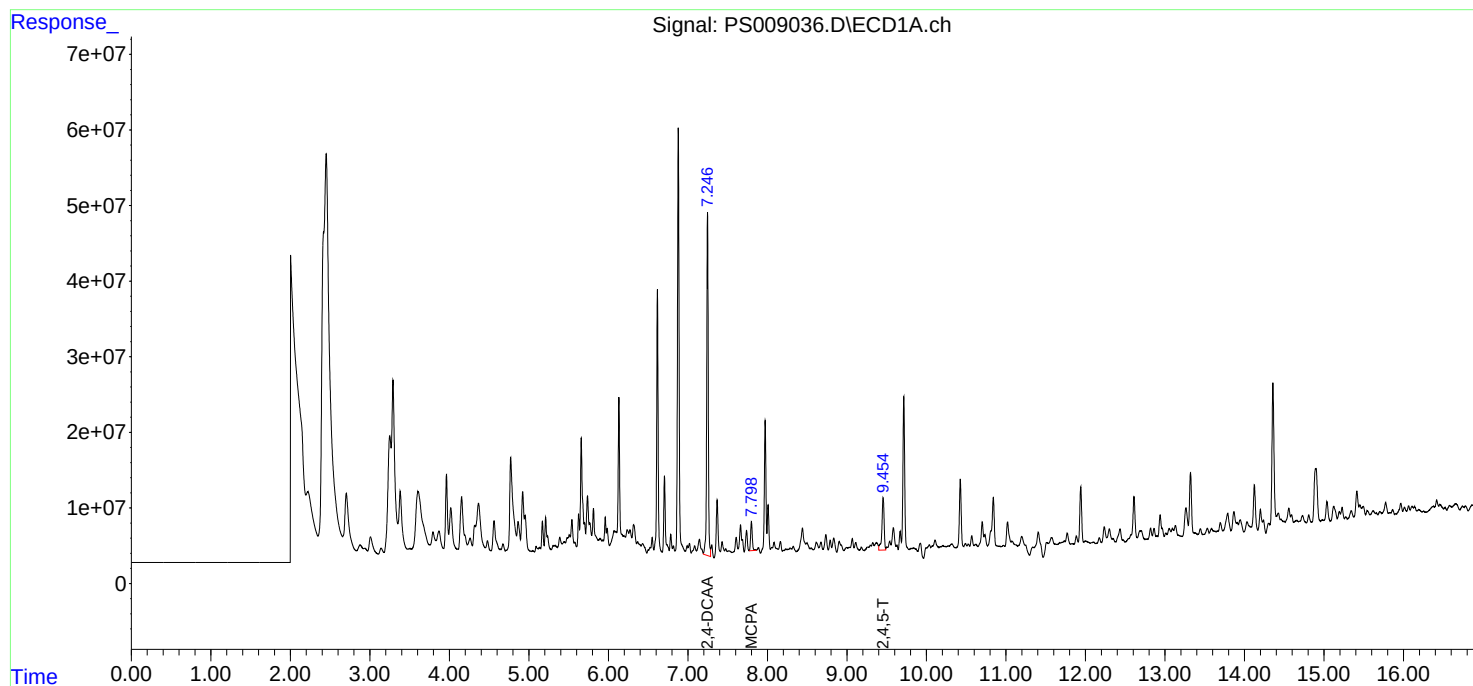


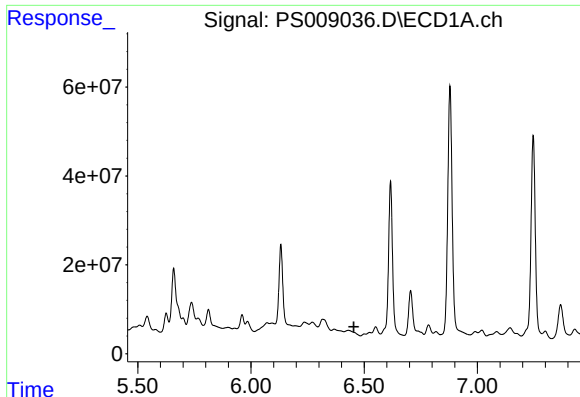

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

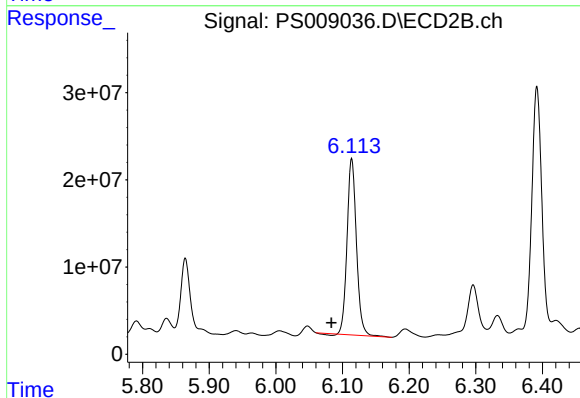


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 196822913
Conc: 134.88 ng/ml

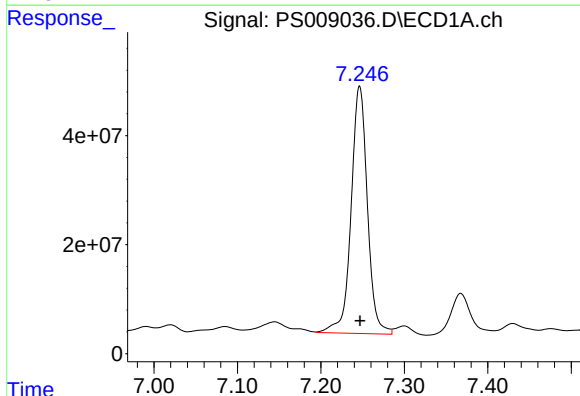


#4 2,4-DCAA

R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 615962404
Conc: 281.70 ng/ml

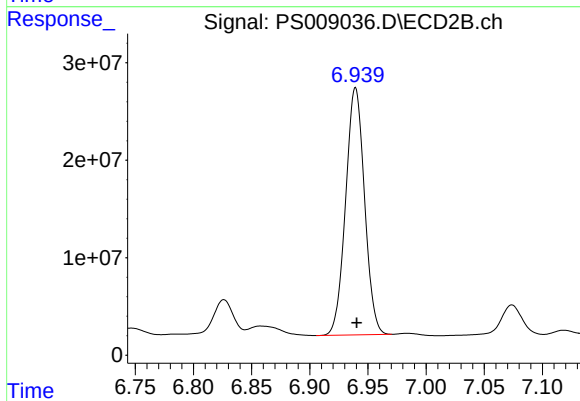

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 286761836
Conc: 297.61 ng/ml

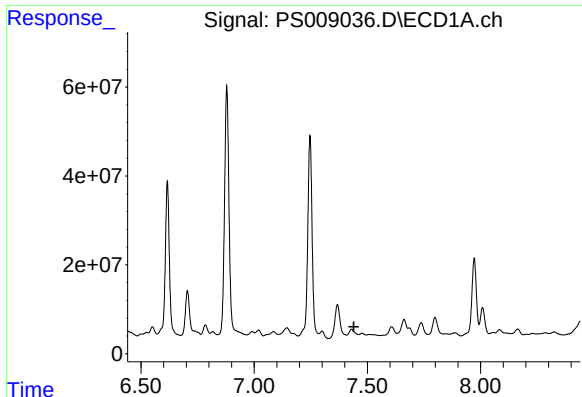

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

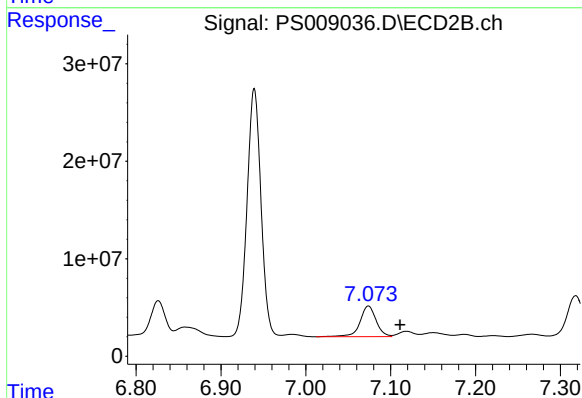


#5 DICAMBA

R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 41434888
Conc: 10.01 ng/ml

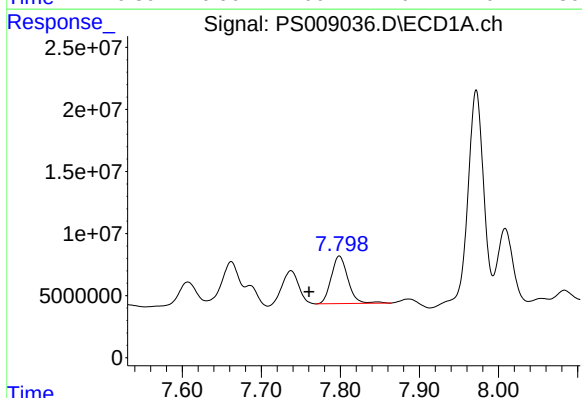


#7 MCPA

R.T.: 7.799 min
Delta R.T.: 0.038 min
Response: 56307709
Conc: 7.00 ug/ml

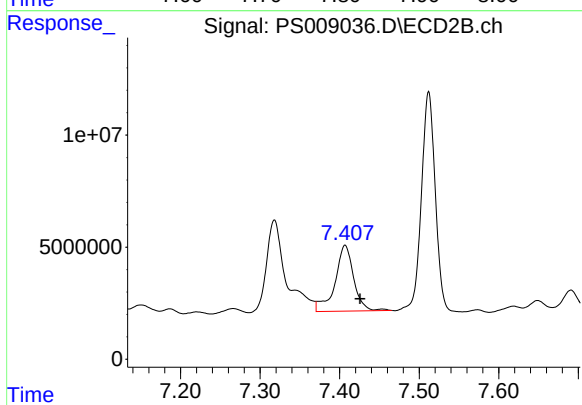

#7 MCPA


R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 48093777
Conc: 10.87 ug/ml

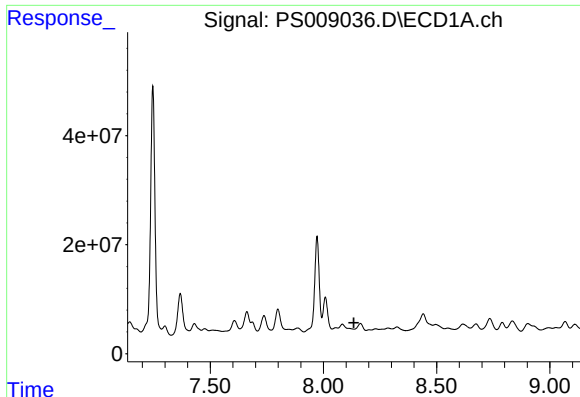

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

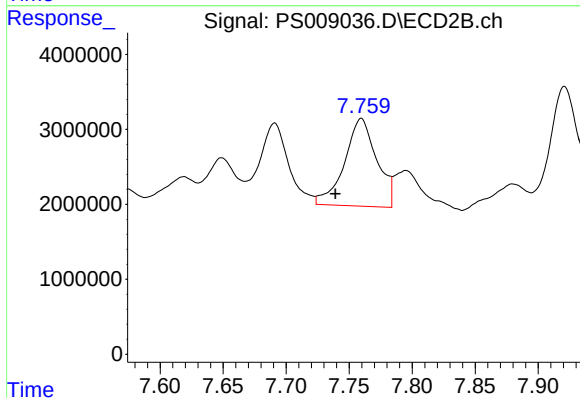


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.020 min
Response: 20858584
Conc: 20.82 ng/ml

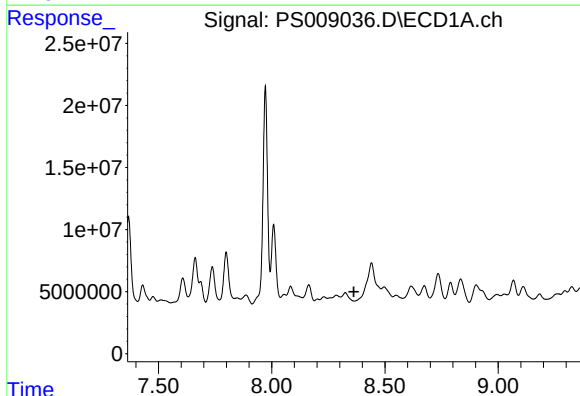


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.363 min
Response: 0
Conc: N.D.

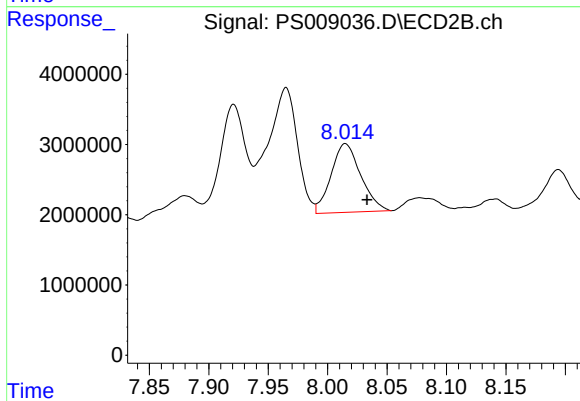

#9 2,4-D


R.T.: 8.015 min
Delta R.T.: -0.018 min
Response: 17051014
Conc: 14.39 ng/ml

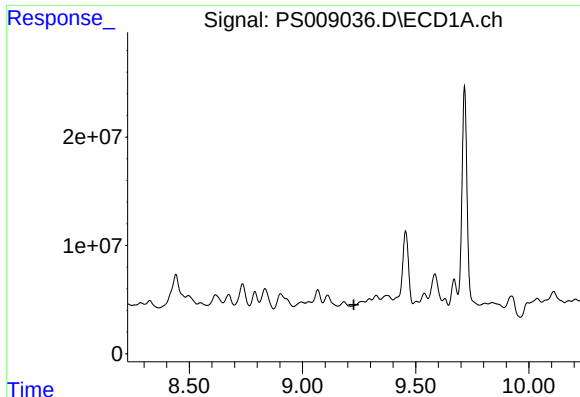

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

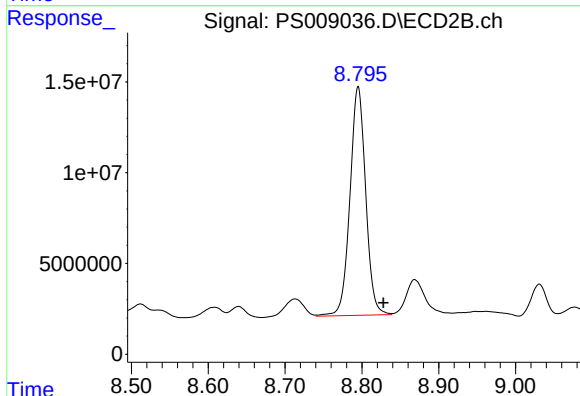


#11 2,4,5-TP (SILVEX)

R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 178814141
Conc: 33.01 ng/ml

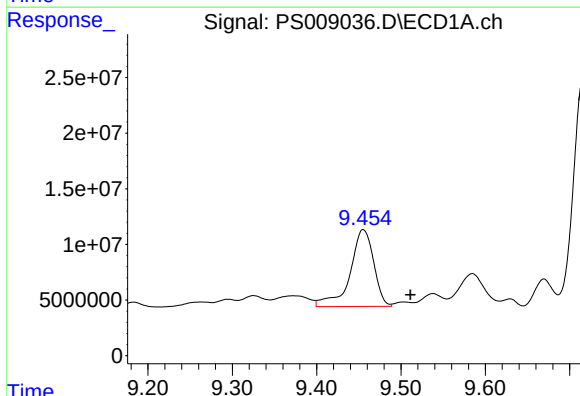


#12 2,4,5-T

R.T.: 9.455 min
Delta R.T.: -0.056 min
Response: 134755240
Conc: 12.60 ng/ml

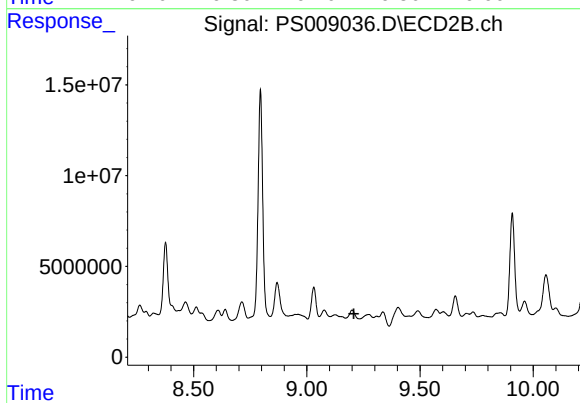

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

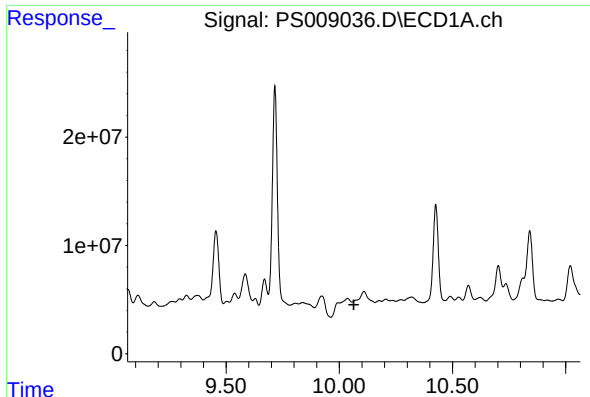

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

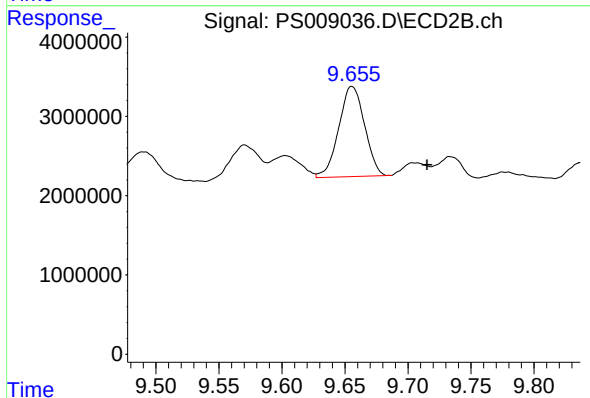


#13 2,4-DB

R.T.: 9.656 min
Delta R.T.: -0.059 min
Response: 16198092
Conc: 23.06 ng/ml

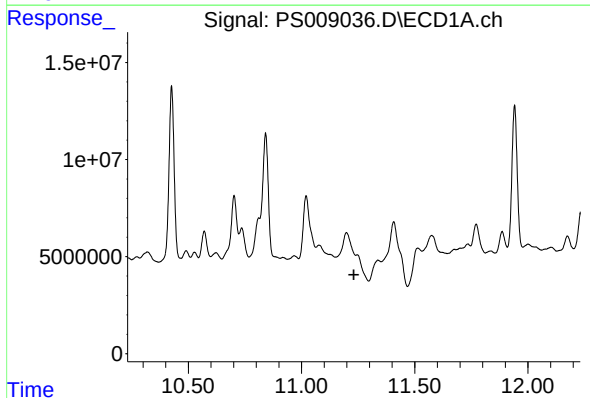

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

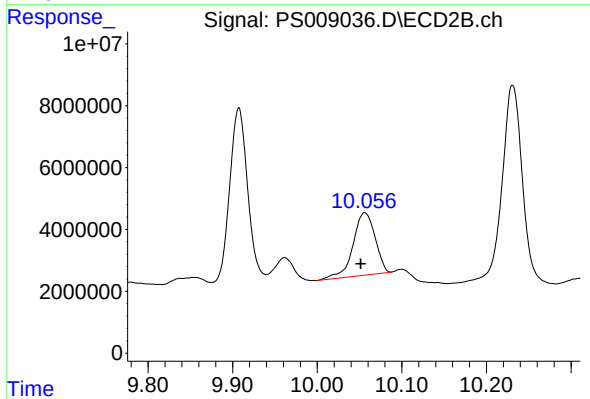

#14 DINOSEB

R.T.: 10.056 min
Delta R.T.: 0.005 min
Response: 36550902
Conc: 9.24 ng/ml