

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
 Data File : PS009039.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2020 22:42
 Operator : DD\AJ
 Sample : L1681-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 00:38:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.592	0	51544439	N.D. 35.251
2) T	3,5-DICHL...	0.000	6.114	0	76396985	N.D. 52.353
5) T	DICAMBA	0.000	7.074	0	15455035	N.D. 3.734
7) T	MCPA	7.799	7.407	61685637	44335057	7.669 10.021 #
11) T	2,4,5-TP ...	0.000	8.795	0	191.2E6	N.D. 35.294
12) T	2,4,5-T	9.456	0.000	71028608	0	6.643 N.D. #
13) T	2,4-DB	0.000	9.656	0	14840896	N.D. 21.128
14) T	DINOSEB	0.000	10.062	0	14952465	N.D. 3.782
15) T	Picloram	11.021	11.031	96526084	21698468	7.050 2.986 #
16) T	DCPA	0.000	11.031	0	21698468	N.D. 3.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022720\
Data File : PS009039.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2020 22:42
Operator : DD\AJ
Sample : L1681-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 00:38:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

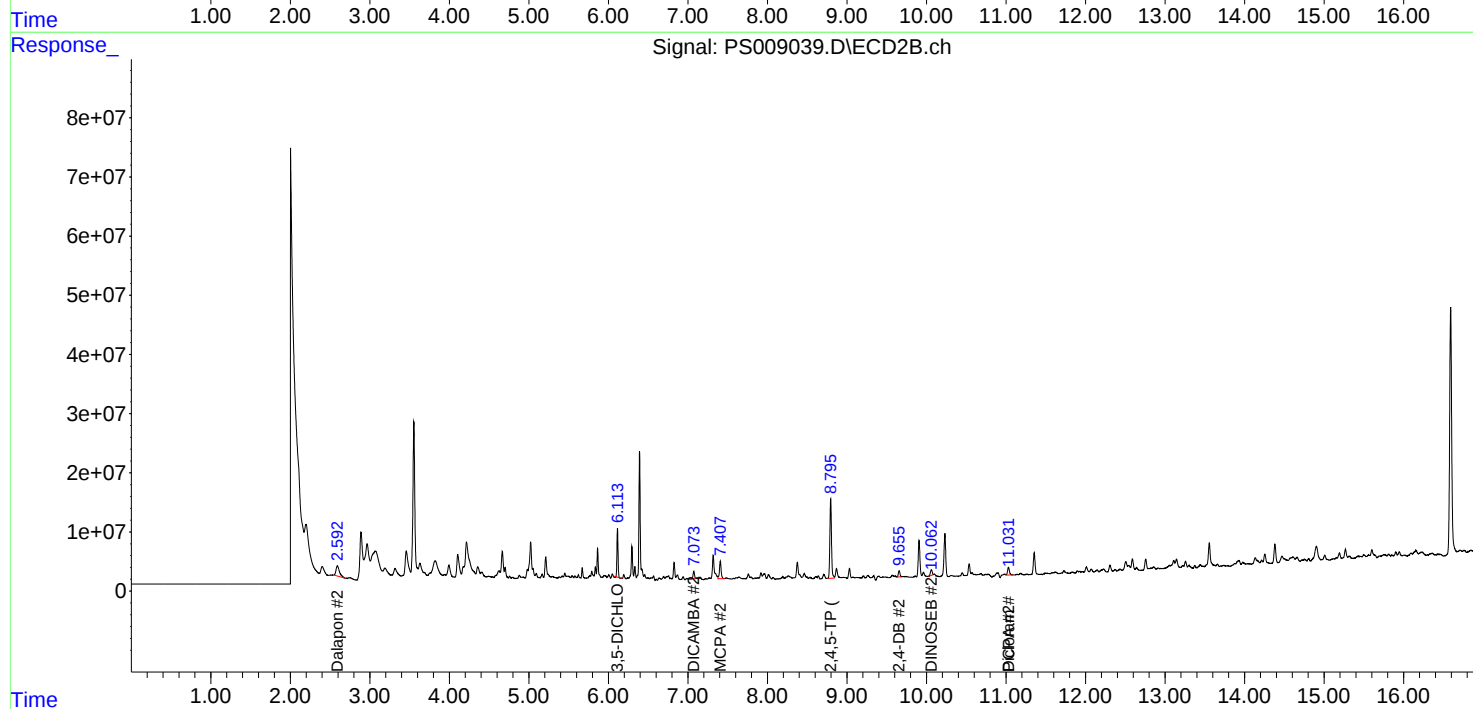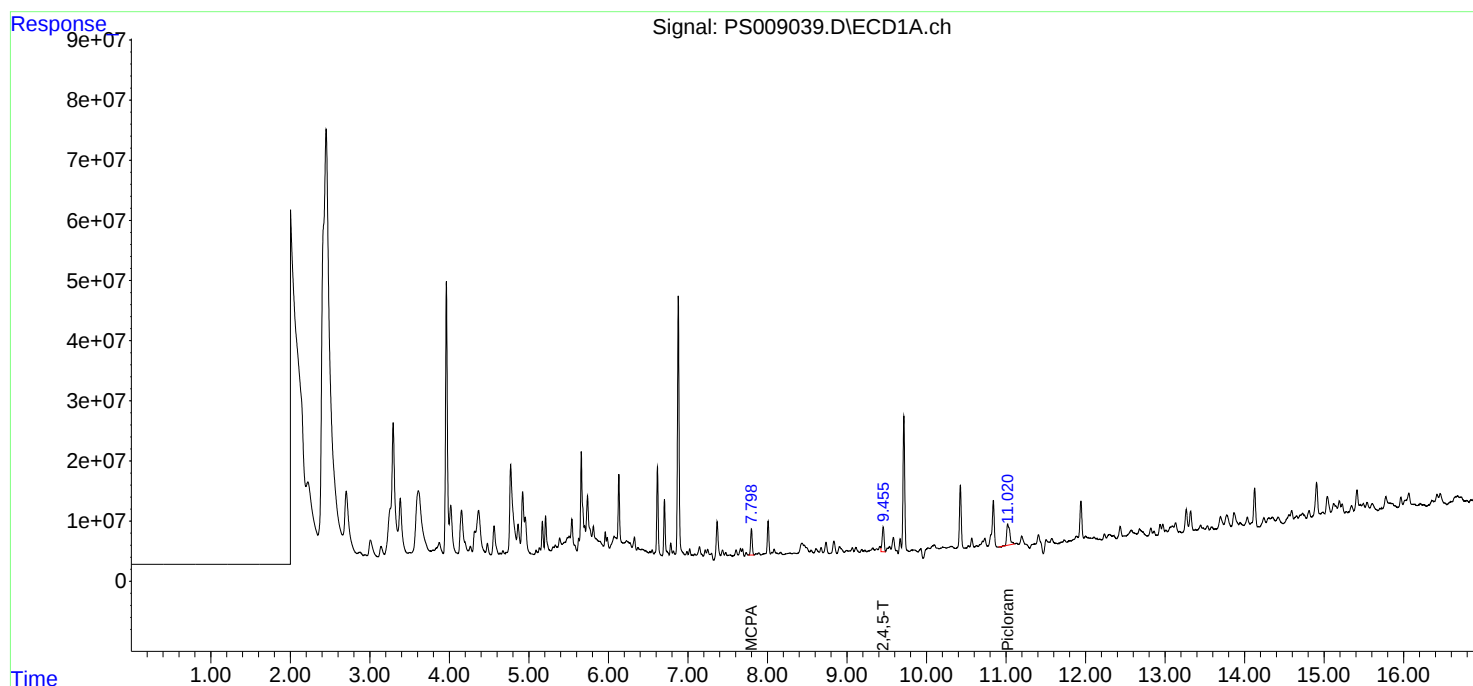


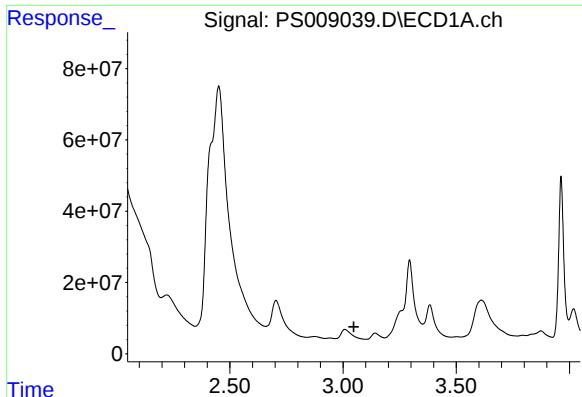

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

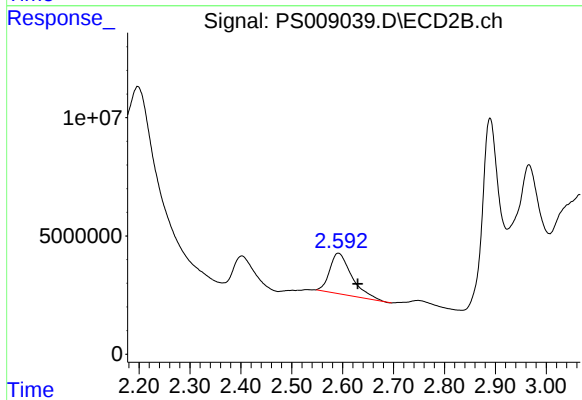


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.038 min
Response: 51544439
Conc: 35.25 ng/ml

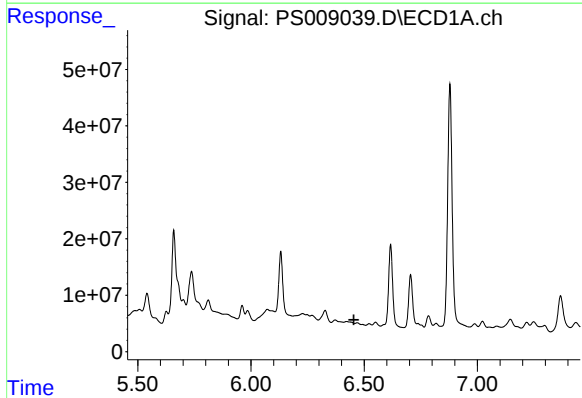


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

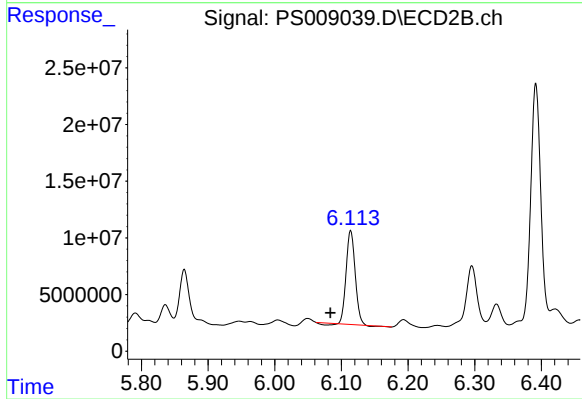

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 76396985
Conc: 52.35 ng/ml

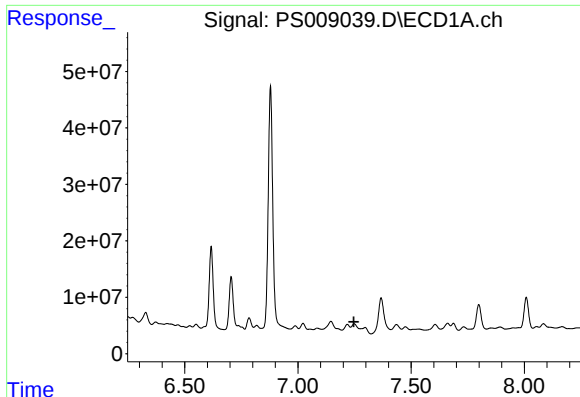

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.247 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

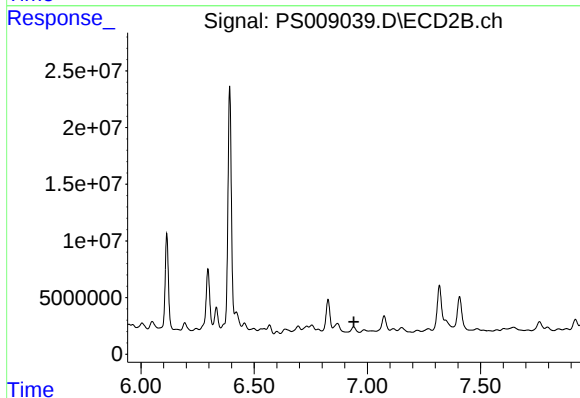


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.940 min
Response: 0
Conc: N.D.

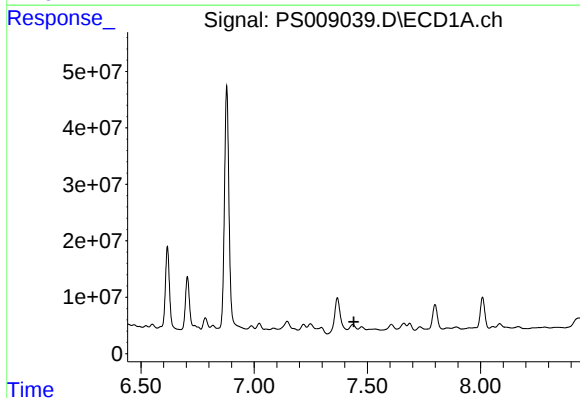


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

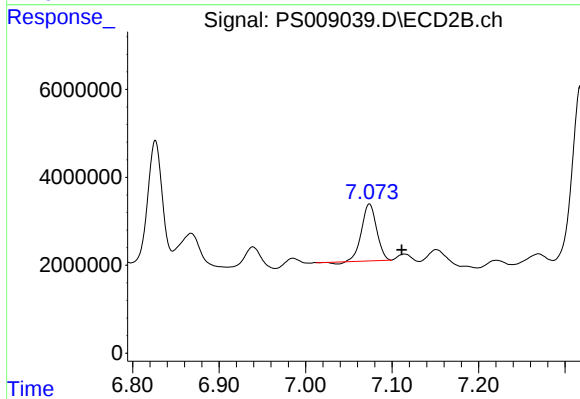

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 15455035
Conc: 3.73 ng/ml

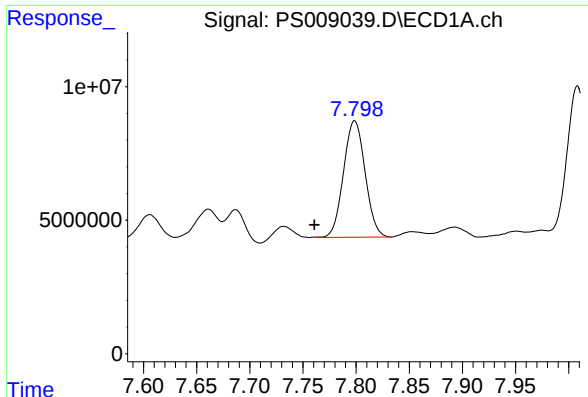

#7 MCPA


R.T.: 7.799 min
Delta R.T.: 0.038 min
Response: 61685637
Conc: 7.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

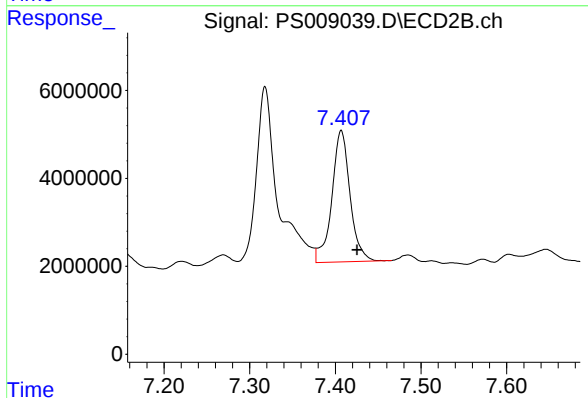


#7 MCPA

R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 44335057
Conc: 10.02 ug/ml

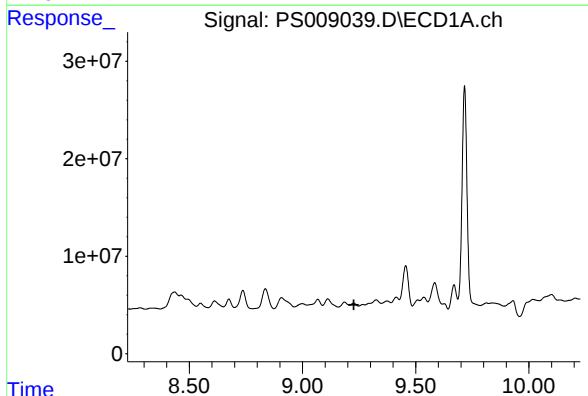


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

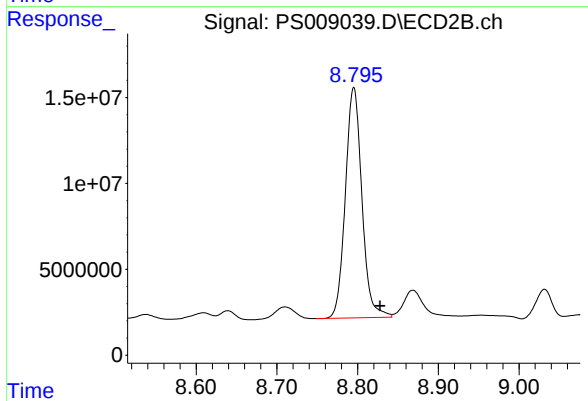

#11 2,4,5-TP (SILVEX)


R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 191184253
Conc: 35.29 ng/ml

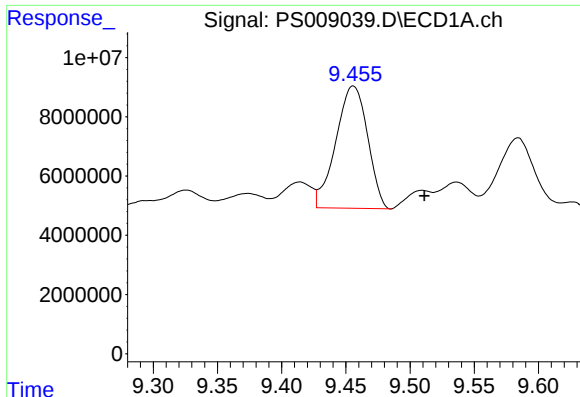

#12 2,4,5-T


R.T.: 9.456 min
Delta R.T.: -0.055 min
Response: 71028608
Conc: 6.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

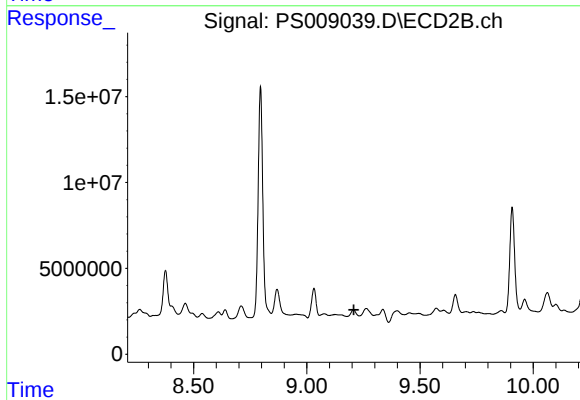


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

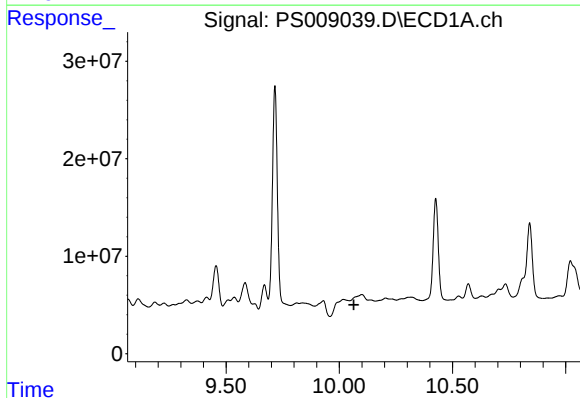


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

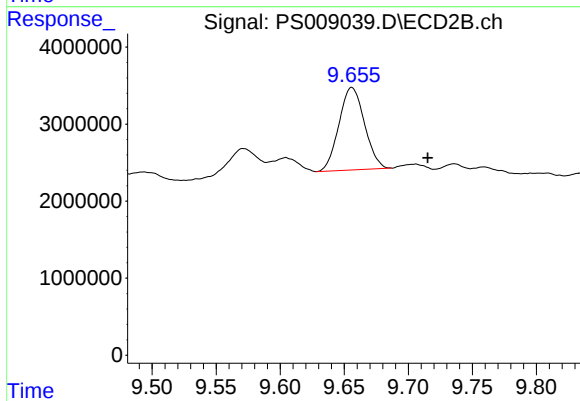

#13 2,4-DB


R.T.: 9.656 min
Delta R.T.: -0.059 min
Response: 14840896
Conc: 21.13 ng/ml

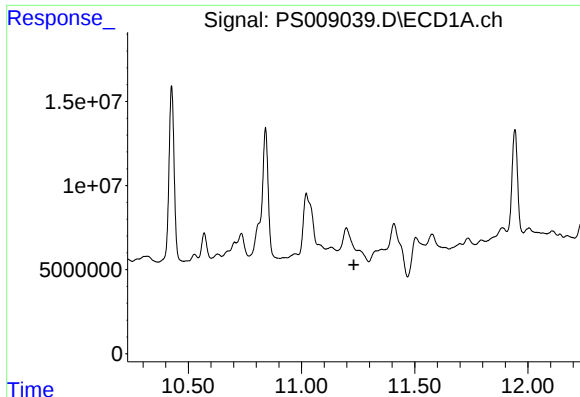

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

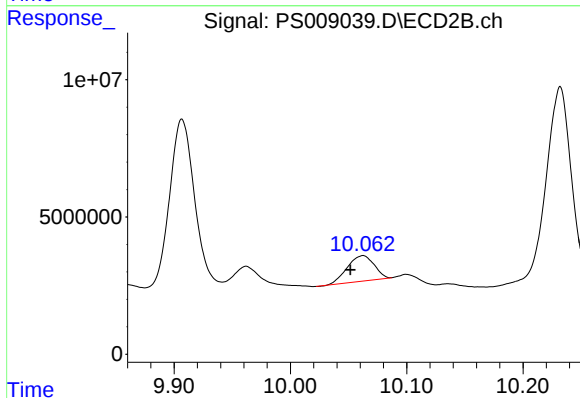


#14 DINOSEB

R.T.: 10.062 min
Delta R.T.: 0.010 min
Response: 14952465
Conc: 3.78 ng/ml

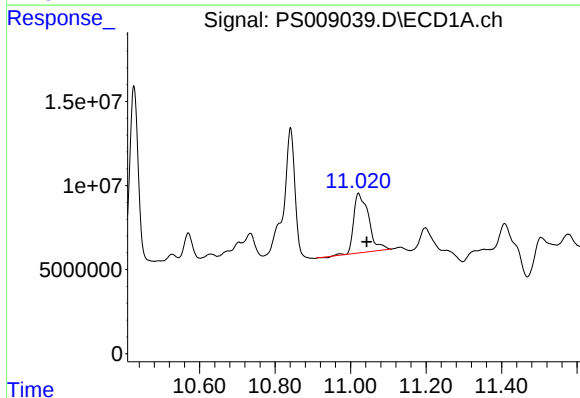


#15 Picloram

R.T.: 11.021 min
Delta R.T.: -0.022 min
Response: 96526084
Conc: 7.05 ng/ml

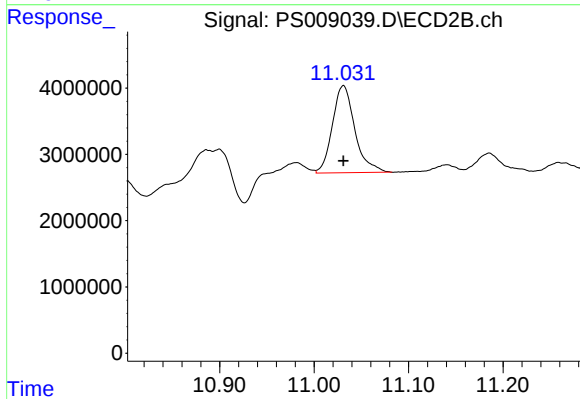

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 21698468
Conc: 2.99 ng/ml

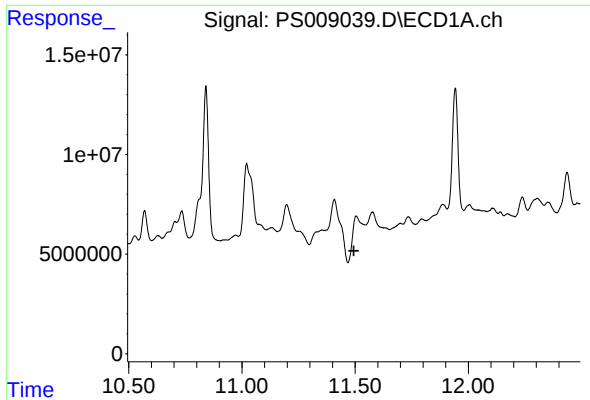

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

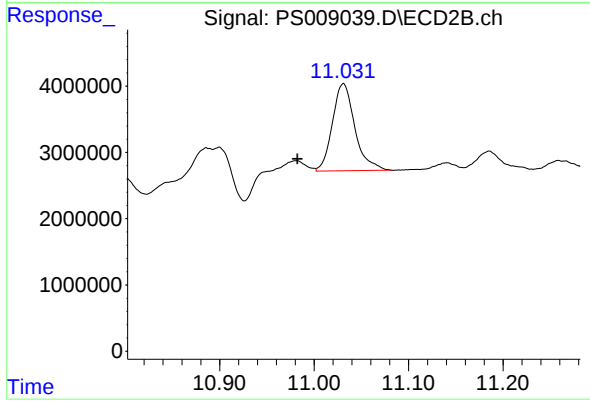

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.049 min
Response: 21698468
Conc: 3.14 ng/ml