

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022724\
 Data File : PS026048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Feb 2024 16:16
 Operator : AR\AJ
 Sample : P1564-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 LKWD-BACKFILL-16

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/28/2024
 Supervised By :Ankita Jodhani 02/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 03:17:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022224.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 22 12:24:27 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.238	7.773	1246.5E6	273.5E6	479.988m	359.736 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022724\
Data File : PS026048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Feb 2024 16:16
Operator : AR\AJ
Sample : P1564-15
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
LKWD-BACKFILL-16


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/28/2024
Supervised By : Ankita Jodhani 02/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 03:17:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022224.M
Quant Title : 8080.M
QLast Update : Thu Feb 22 12:24:27 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

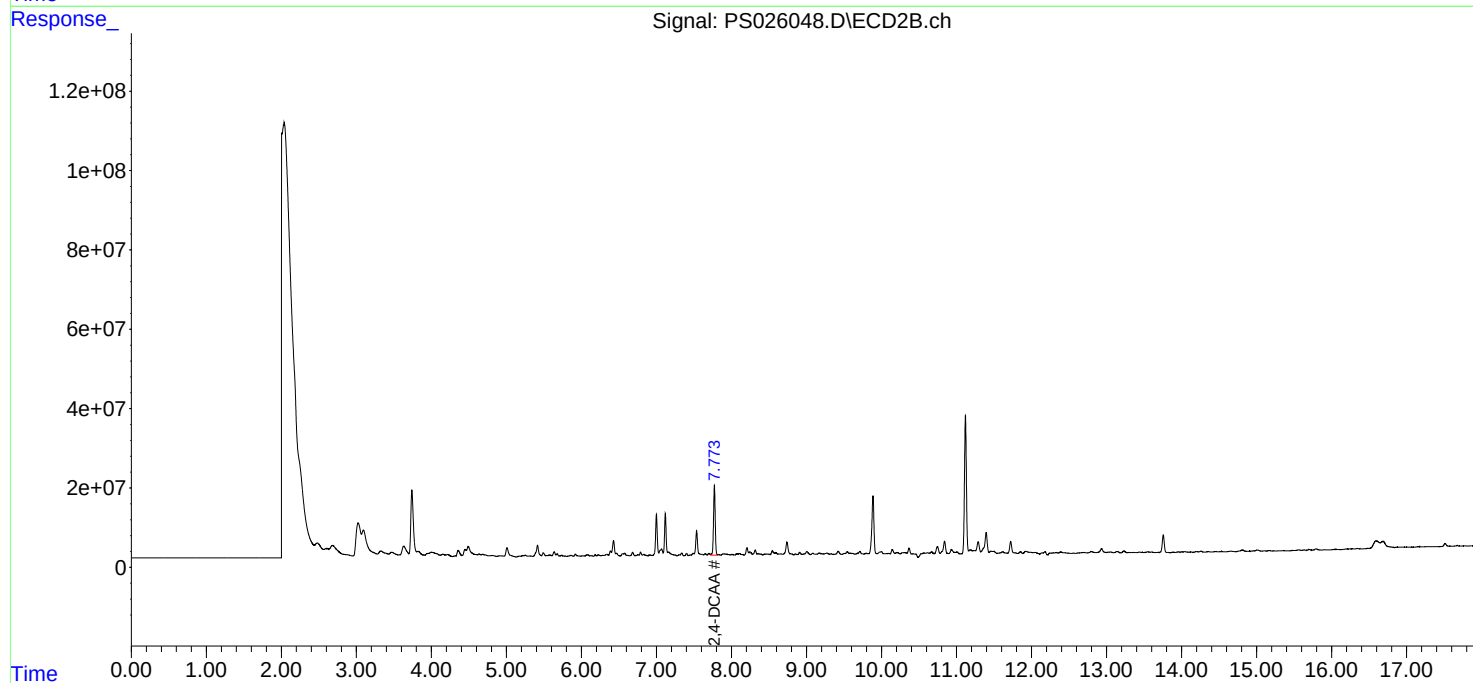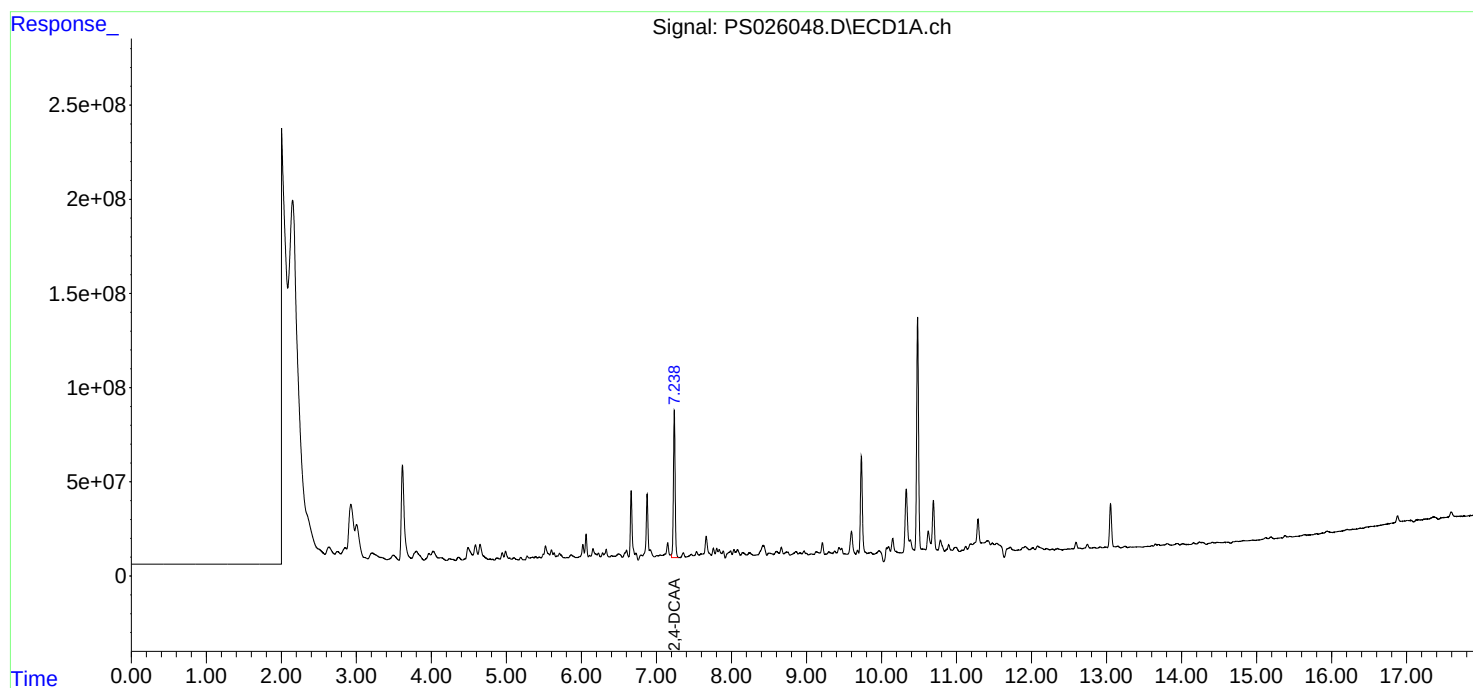

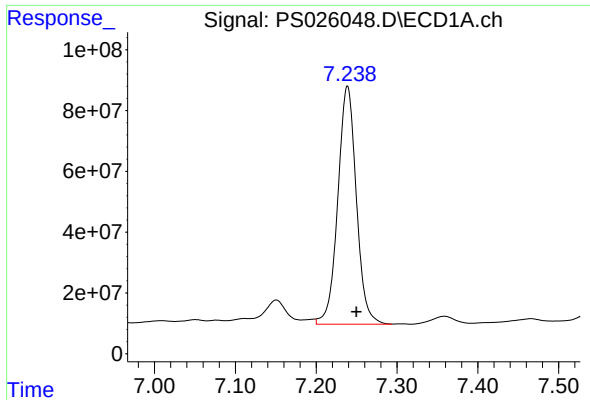


#4 2,4-DCAA

R.T.: 7.238 min
Delta R.T.: -0.011 min
Response: 1246467785
Conc: 479.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
LKWD-BACKFILL-16

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/28/2024
Supervised By :Ankita Jodhani 02/28/2024

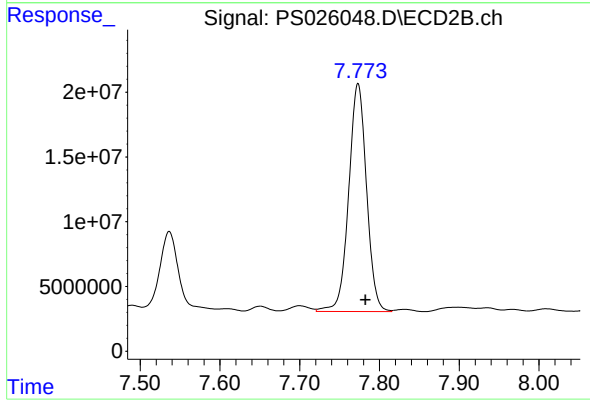

#4 2,4-DCAA

R.T.: 7.773 min
Delta R.T.: -0.009 min
Response: 273531659
Conc: 359.74 ng/ml