

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022725\
 Data File : PS029308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2025 01:03
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 04:34:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	7.627	2249.9E6	506.5E6	546.017	538.651
Target Compounds							
1) T	Dalapon	2.647f	2.686f	52626258	26075715	9.533	12.317 #
2) T	3,5-DICHL...	6.352	0.000	775743	0	<MDL	N.D. #
3) T	4-Nitroph...	6.955	0.000	12826689	0	5.481	N.D. #
8) T	DICHLORPROP	8.043	0.000	2621323	0	<MDL	N.D. #
10) T	Pentachlo...	8.566	0.000	15332192	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.113f	9.752	16422428	5335107	<MDL	<MDL #
12) T	2,4,5-T	9.454	0.000	10089633	0	<MDL	N.D. #
13) T	2,4-DB	9.975	0.000	2397034	0	<MDL	N.D. #
14) T	DINOSEB	11.189	0.000	1315760	0	<MDL	N.D. #
15) T	Picloram	10.997	12.200	2089665	8935156	<MDL	<MDL #
16) T	DCPA	11.488	0.000	3027059	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022725\
Data File : PS029308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2025 01:03
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 04:34:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

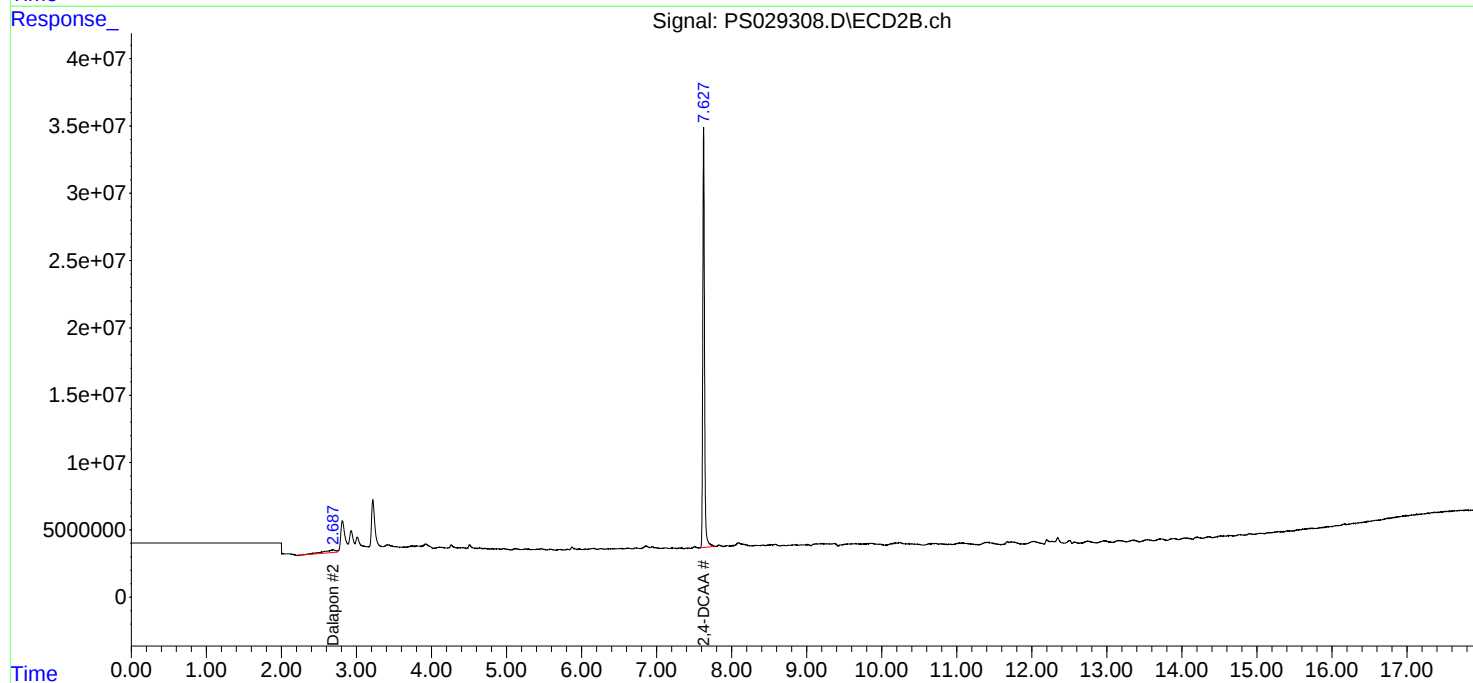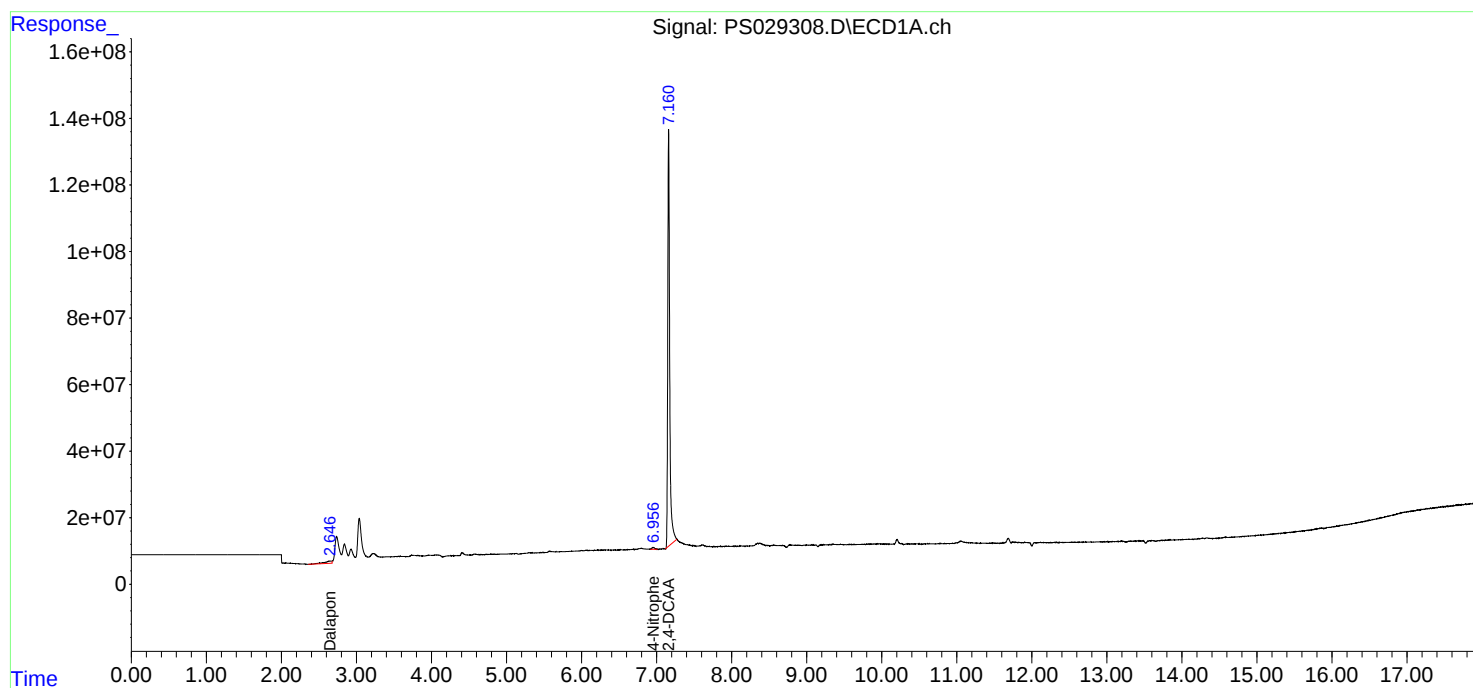


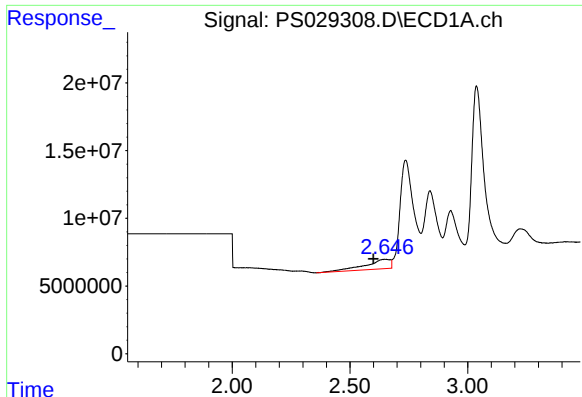

#1 Dalapon


R.T.: 2.647 min
Delta R.T.: 0.047 min
Response: 52626258
Conc: 9.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

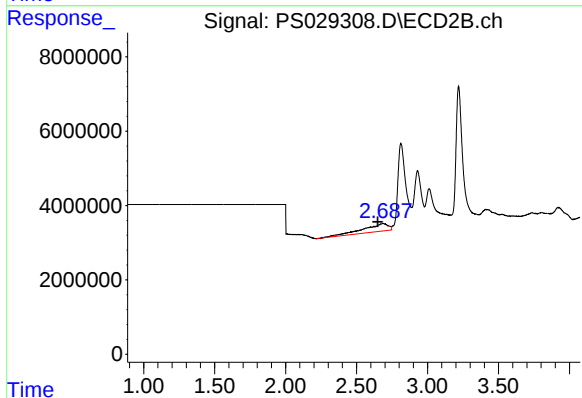


#1 Dalapon

R.T.: 2.686 min
Delta R.T.: 0.036 min
Response: 26075715
Conc: 12.32 ng/ml

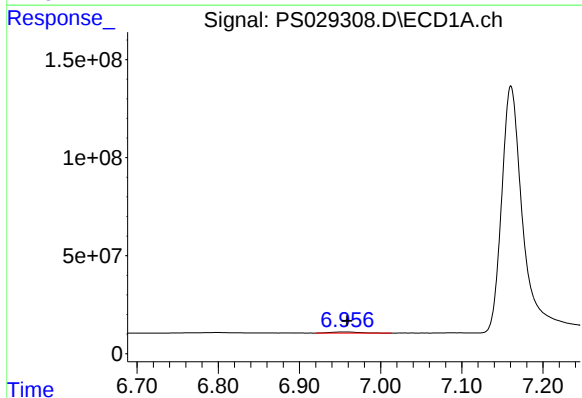


#3 4-Nitrophenol

R.T.: 6.955 min
Delta R.T.: -0.003 min
Response: 12826689
Conc: 5.48 ng/ml

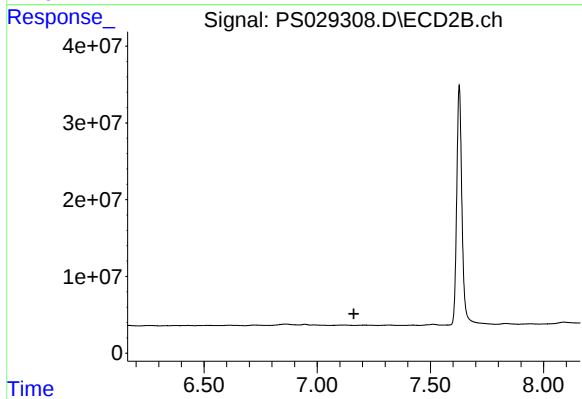

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.162 min
Response: 0
Conc: N.D.

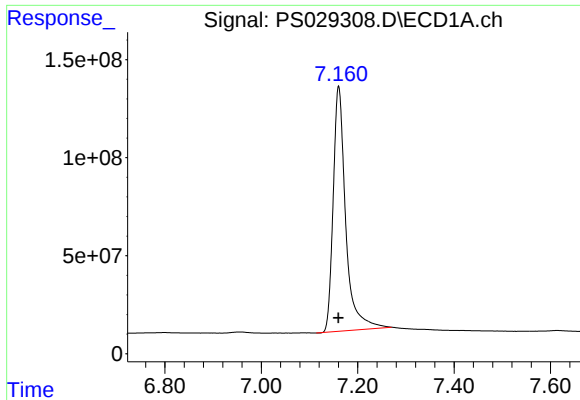

#4 2,4-DCAA

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 2249907053
Conc: 546.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

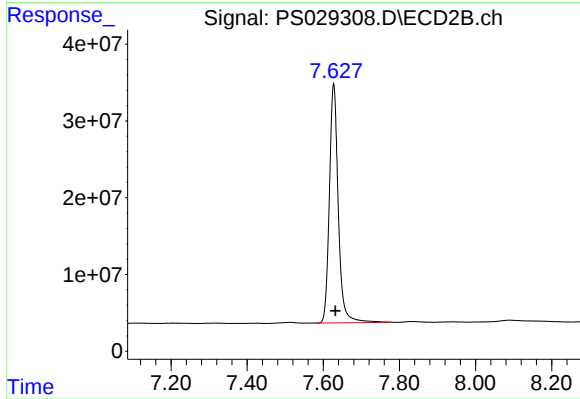

#4 2,4-DCAA

R.T.: 7.627 min
Delta R.T.: -0.005 min
Response: 506511394
Conc: 538.65 ng/ml