

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022725\
 Data File : PS029323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2025 09:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 10:21:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	7.626	2276.9E6	515.9E6	552.573	548.601
Target Compounds							
1) T	Dalapon	2.642f	2.682f	5820255	18927057	1.054	8.940 #
2) T	3,5-DICHL...	6.325	0.000	1890538	0	<MDL	N.D. #
3) T	4-Nitroph...	6.951	0.000	13939689	0	5.957	N.D. #
5) T	DICAMBA	0.000	7.831	0	3044915	N.D.	<MDL
8) T	DICHLORPROP	8.033	8.580f	3320109	9723213	<MDL	7.604 #
10) T	Pentachlo...	8.564	9.371	10197363	20841531	<MDL	<MDL #
11) T	2,4,5-TP ...	9.118	9.751	11060232	28804552	<MDL	3.188 #
12) T	2,4,5-T	9.449	10.182	6924163	5982937	<MDL	<MDL #
13) T	2,4-DB	9.962f	0.000	3183469	0	<MDL	N.D. #
14) T	DINOSEB	11.190	0.000	1333336	0	<MDL	N.D. #
15) T	Picloram	10.996	12.202	9590702	4728616	<MDL	<MDL #
16) T	DCPA	11.485	0.000	4252825	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022725\
Data File : PS029323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2025 09:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 10:21:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

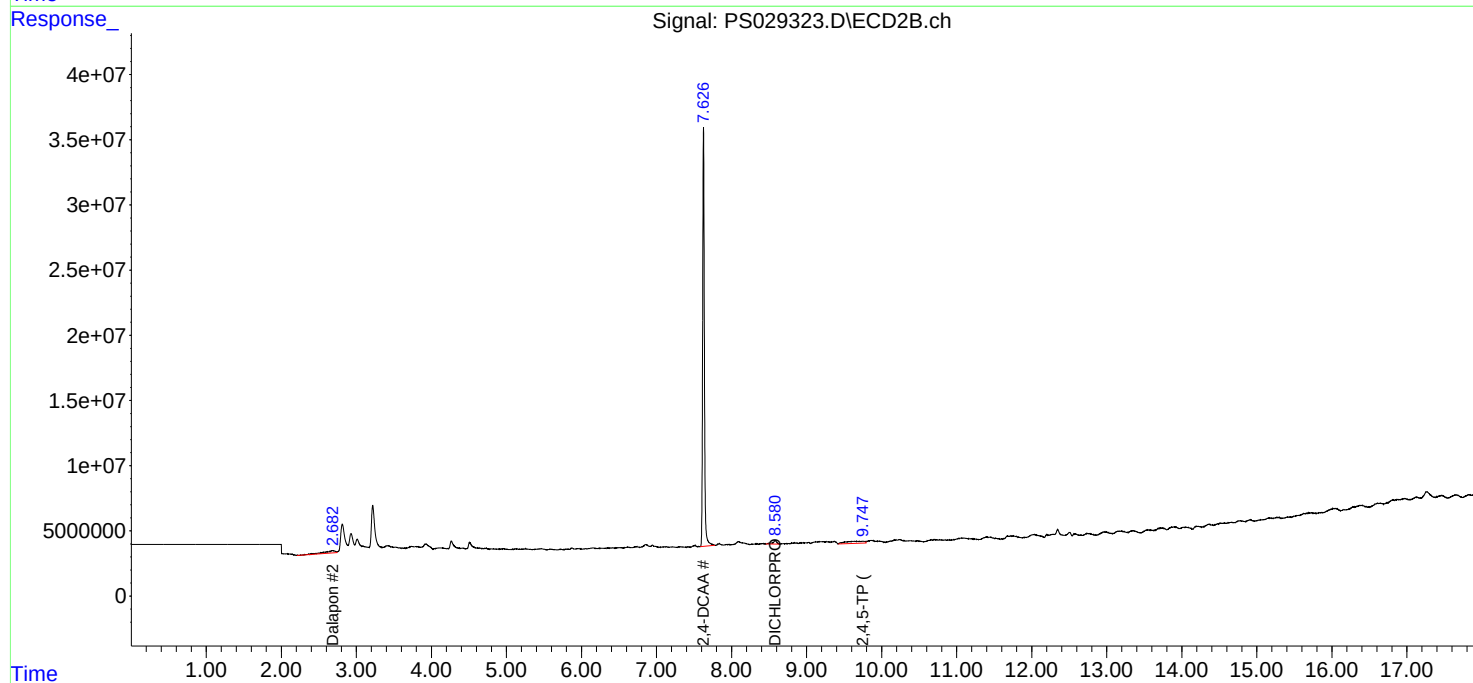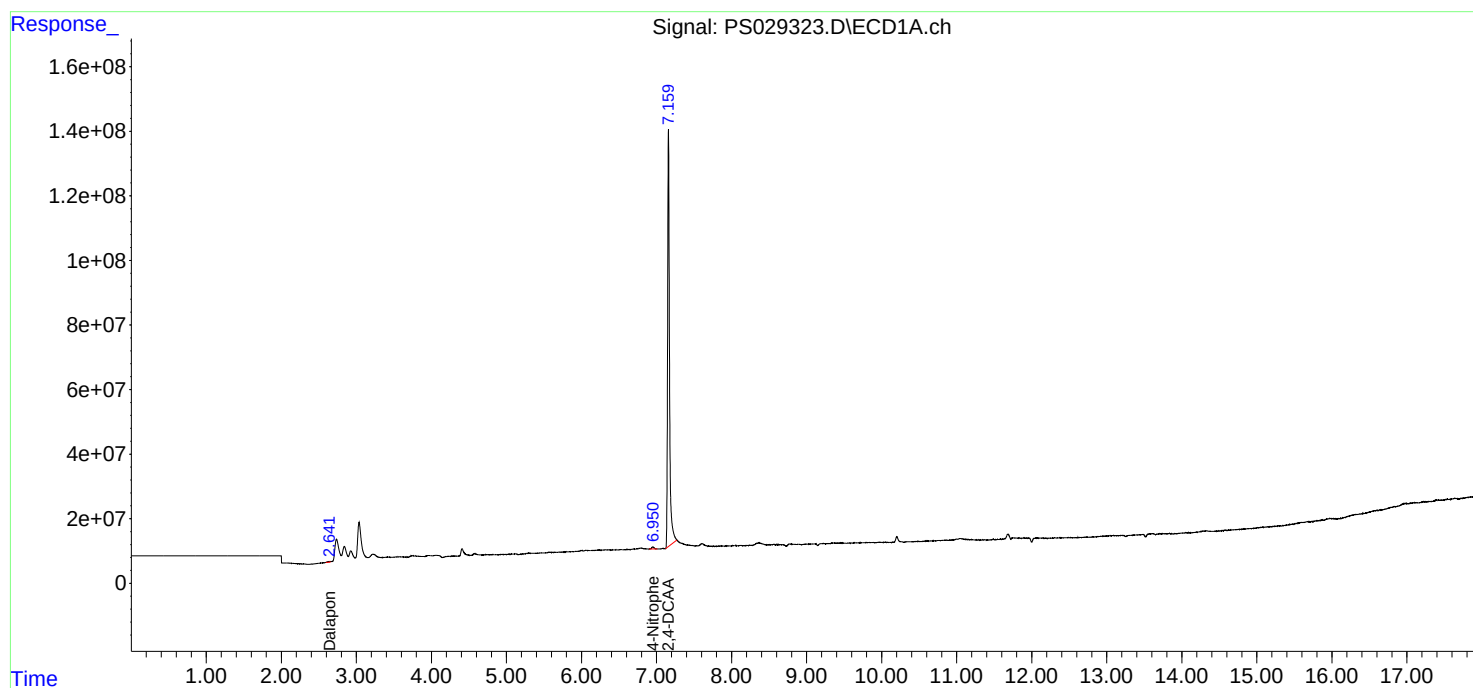


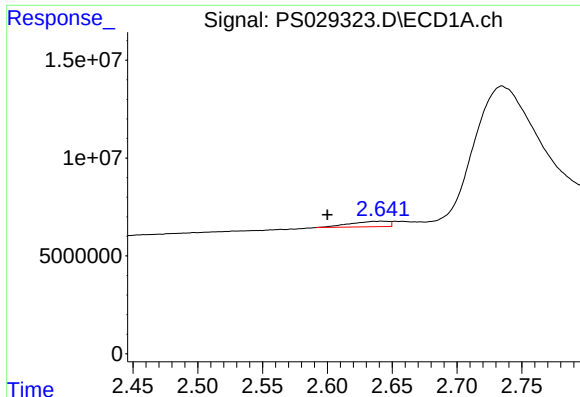

#1 Dalapon


R.T.: 2.642 min
Delta R.T.: 0.042 min
Response: 5820255
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

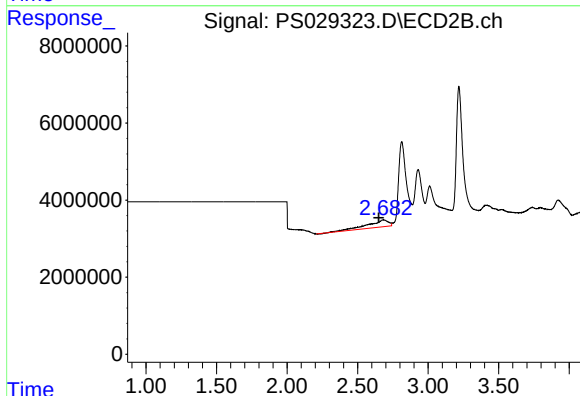


#1 Dalapon

R.T.: 2.682 min
Delta R.T.: 0.031 min
Response: 18927057
Conc: 8.94 ng/ml

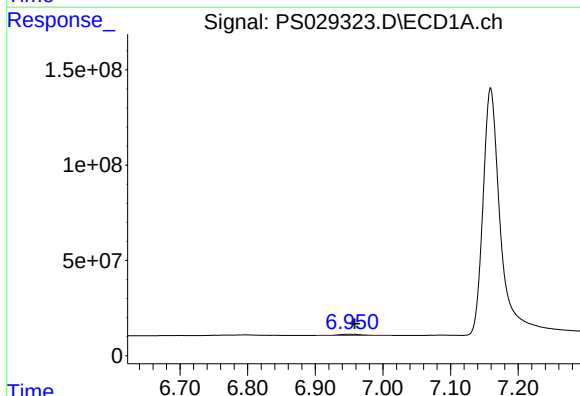


#3 4-Nitrophenol

R.T.: 6.951 min
Delta R.T.: -0.008 min
Response: 13939689
Conc: 5.96 ng/ml

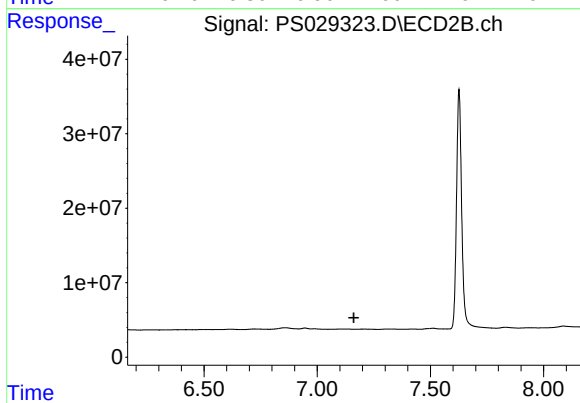

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.162 min
Response: 0
Conc: N.D.

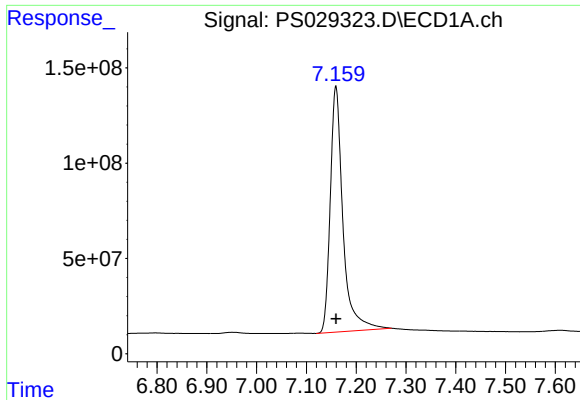

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.000 min
Response: 2276919096
Conc: 552.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

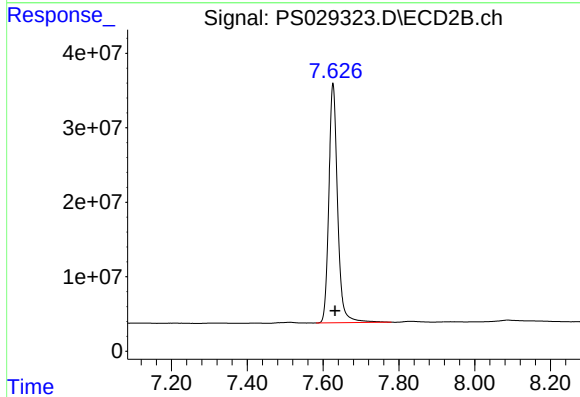


#4 2,4-DCAA

R.T.: 7.626 min
Delta R.T.: -0.006 min
Response: 515867108
Conc: 548.60 ng/ml

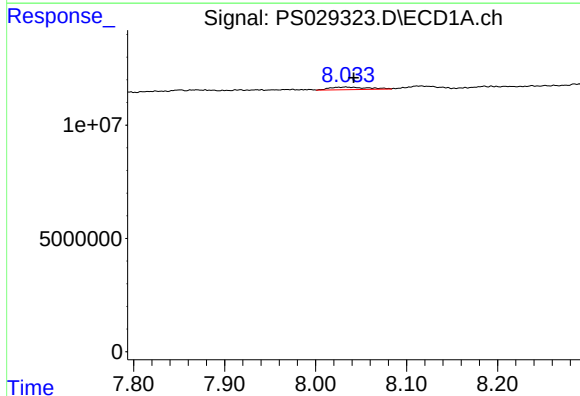


#8 DICHLORPROP

R.T.: 8.033 min
Delta R.T.: -0.009 min
Response: 3320109
Conc: N.D.

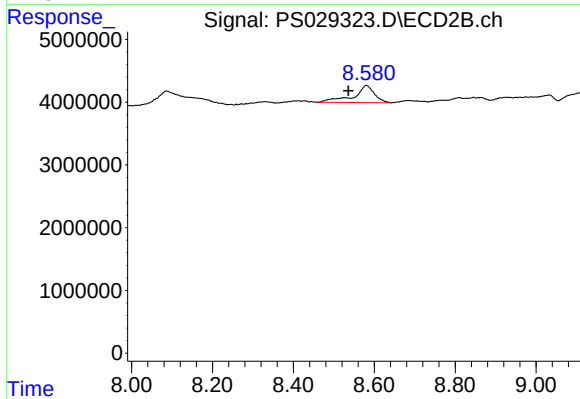

#8 DICHLORPROP


R.T.: 8.580 min
Delta R.T.: 0.044 min
Response: 9723213
Conc: 7.60 ng/ml

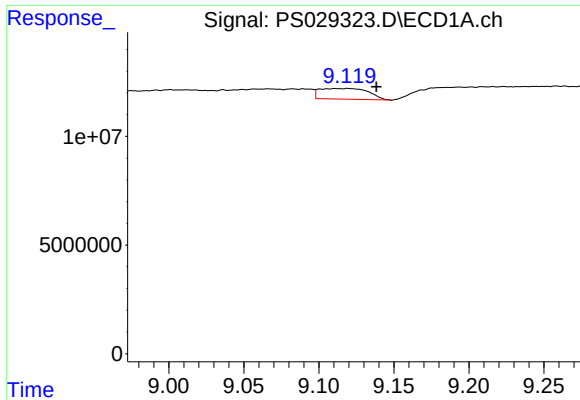

#11 2,4,5-TP (SILVEX)

R.T.: 9.118 min
Delta R.T.: -0.021 min
Response: 11060232
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

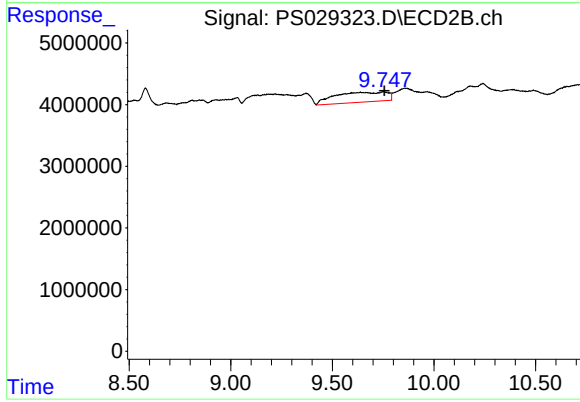

#11 2,4,5-TP (SILVEX)

R.T.: 9.751 min
Delta R.T.: -0.005 min
Response: 28804552
Conc: 3.19 ng/ml